

A11100 986094

NBS  
PUBLICATIONS


NATL INST. OF STAND & TECH R.I.C.



A11105 042895

# CONTAINER BOARD

report no. 121  
October 1979

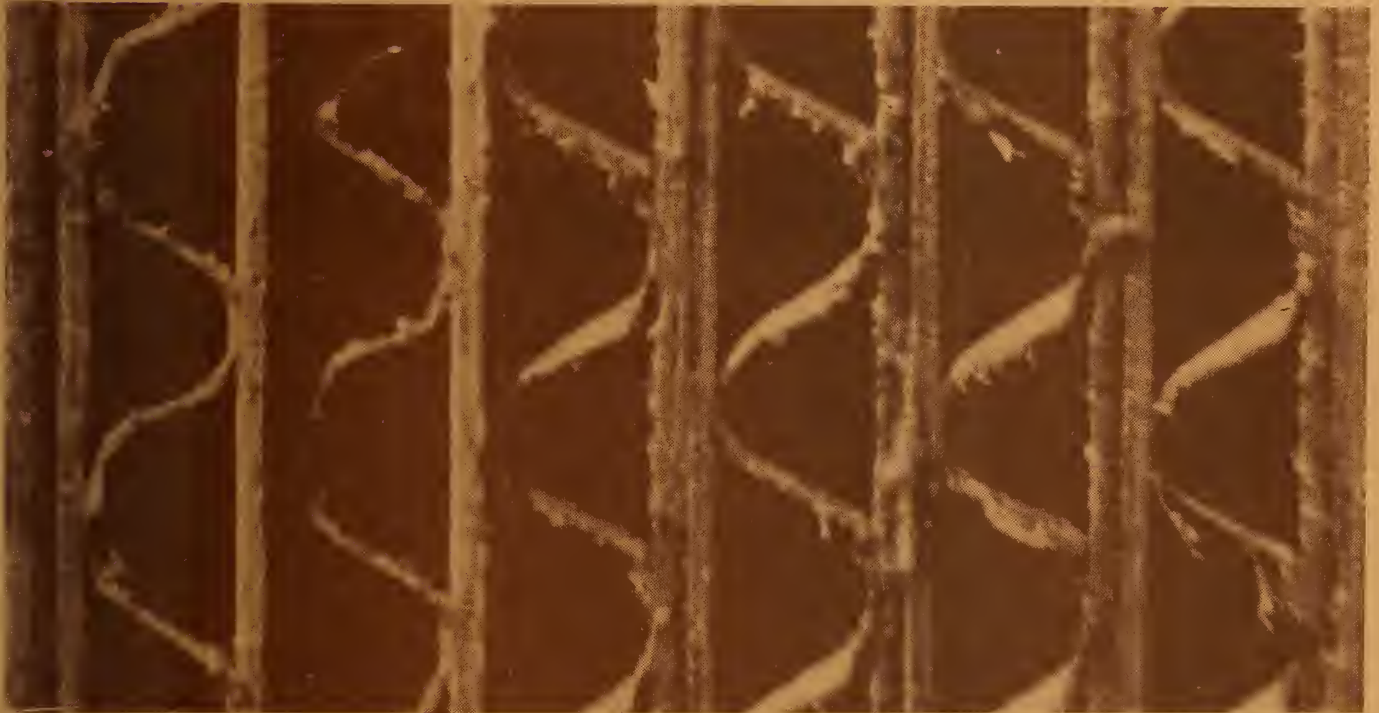

NBS Collaborative Reference  
Program for Containerboard

Fourdrinier Kraft Board Group  
American Paper Institute, Inc.  
and U.S. Department of  
Commerce, National Bureau  
of Standards

QC  
100  
U56  
79-1816  
1979  
C.2

NBS COLLABORATIVE REFERENCE PROGRAMS

TAPPI Paper and Board (6 times per year)

Bursting strength	Smoothness
Tearing strength	Surface pick strength
Tensile breaking strength	K & N ink absorption
Elongation to break	pH
Tensile energy absorption	Opacity
Folding endurance	Blue reflectance (brightness)
Stiffness	Specular gloss, 75°
Air resistance	Thickness
Grammage	Concora (flat crush)
	Ring crush

FKBG-API Containerboard (48 times per year)

Mullen burst of linerboard  
Concora test of medium

MCCA Color and Appearance (4 times per year)

Gloss at 60°  
Color and color difference

CTS Rubber (4 times per year)

Tensile strength, ultimate elongation and tensile stress  
Hardness  
Mooney viscosity  
Vulcanization properties

CTS Thermal Insulation Materials (2 times per year)

19 test methods for thermal insulation materials covering:  
thermal properties; strength properties; dimensions, stability,  
and density properties; fire properties; and properties of  
vapor barriers

ASTM Cement (2 times per year)

Chemical (11 chemical components)  
Physical (8 characteristics)

AASHTO Bituminous

Asphalt cement (2 times per year)  
Cutbacks (once a year)

NBS Collaborative Reference Programs  
A05 Technology Building  
National Bureau of Standards  
Washington, DC 20234

National Bureau of Standards  
FEB 27 1980  
not Acc. Cur  
QC100  
USG  
79-1816  
1979  
c ↓

# CONTAINER BOARD

Collaborative Reference  
Program for  
Containerboard

report no. 121  
October 1979

T.L. Cummings  
NBS Research Associate  
Collaborative Testing  
Services, Inc.

J. Horlick  
Office of Testing Laboratory  
Evaluation Technology,  
Office of Engineering Standards,  
National Engineering Laboratory

U.S. Department of Commerce,  
National Bureau of Standards

Fourdrinier Kraft Board Group  
American Paper Institute, Inc.




## INTRODUCTION

The Collaborative Reference Program (CRP) for Containerboard is cosponsored by the Fourdrinier Kraft Board Group (FKBG) of the American Paper Institute, Inc. and the National Bureau of Standards. The program is maintained and operated by Collaborative Testing Services, Inc. (CTS). CTS is a non-profit organization of associations that offers CRPs to a wide range of industries.

Samples of three weights of linerboard, nominally 26 lb, 42 lb, and 69 lb and of corrugating medium (26 lb) are separately randomized from uniform narrow rolls and packaged for distribution to the participants. Each month, sufficient test material for four weekly tests is mailed to participants for testing Mullen bursting strength according to TAPPI official testing method T807 os-75 or Concora flat crush strength according to TAPPI official testing method T809 os-71. The participants return their test results to NBS for analysis and receive two monthly reports from NBS. One report is a preliminary individualized report comparing a laboratory's results with the industrial mean. The other is a longer report (as illustrated by this report) showing the data from all participants.

If there are any questions on the notes, the analyses, or the reports in general, contact Thomas L. Cummings or Jeffrey Horlick on (301) 921-2946.

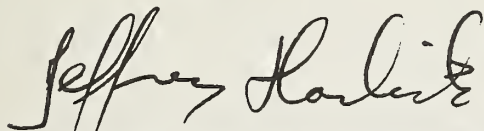

Jeffrey Horlick, Technical Administrator  
NBS Collaborative Reference Programs  
Office of Testing Laboratory Evaluation Technology

November 30, 1979



## TABLE OF CONTENTS

### Page

1	Explanation of Tables
4	Instrument Codes
5	Use of Average Mean as a Reference Standard
6	Bursting Strength, Linerboard 42L1, weeks 1 - 4
8	Bursting Strength, Linerboard 26K1, weeks 1 - 4
10	Concora Flat Crush, Corrugating Medium 26D2





## EXPLANATION OF TABLES

Each table shows laboratory test results for Mullen bursting strength of linerboard or Concora flat crush strength of corrugating medium. The data are divided into three time spans. On the left of each table is an analysis for each week of the month. In the center is cumulative data for the month and on the right is cumulative data for up to 16 weeks.

Conservative statistical tests have been used in excluding extreme data from the analyses. Thus, where the mean (average) for one laboratory is compared with the average for many laboratories, limits have been used that would exclude only one laboratory in a hundred if all laboratories followed exactly the same testing procedure. Consequently, laboratories receiving "X" flags should review their testing procedures, instrument calibration, and control processes. Similar conservative criteria were used in flagging within-laboratory standard deviations and other statistics.

<u>WEEKLY VALUES:</u>	LAB	MEANS THIS MONTH			
	CODE V	WK-1	WK-2	WK-3	WK-4

LAB CODE - Confidential laboratory identification number known only to the participant and the Collaborative Reference Program staff.

V - Code for indicating instrument type, units used, and any other variation in test procedure or conditions. A '+' in this column means a non-standard variation. Data marked '+' are not included in the combined averages for all laboratories. (see page 4).

MEANS THIS MONTH - For each laboratory each weekly mean is the average of individual test determinations, usually an average of 20 determinations.

FLAGS (following means and standard deviations) -

X - Data excluded from an AV MEAN or average standard deviation because value deviated from the AV MEAN or average standard deviation by more than 2.576 times the appropriate standard deviation. A laboratory following the prescribed test method could obtain such an extreme value by chance only one time in a hundred. Corrective action is almost certainly required.

\* - Data included in the CUMULATIVE AV MEAN but the value deviated from this mean by more than 1.960 and less than 2.576 times the SD CUM MEAN. A laboratory following the prescribed test method could obtain such an extreme value by chance only one time in twenty. Corrective action may be desired.

- S - This is a warning to the laboratory but does not affect inclusion or exclusion of the laboratory's results from the corresponding AV MEAN. This flag indicates an extremely high or low within-laboratory standard deviation (SDR, not shown) that could occur by chance only one time in a hundred if the laboratory is following the prescribed test method.
- AV MEAN - (at bottom of table) - The average for the indicated week of the means for all laboratories, except those laboratories marked '+' in column V and those means marked with an 'X'.
- SDR - (not shown) - The standard deviation of within-laboratory measurements; i.e., the Standard Deviation of the Replicate measurements made at one time in one laboratory on one package of test pieces.
- AV SDR - The average for the indicated week of the SDR's of all the laboratories, except those omitted from the AV MEAN. Also an extremely high or low SDR as compared with the AV SDR based on the remaining laboratories is omitted from the AV SDR and the letter 'S' is placed after the laboratory mean for that week. The AV SDR is an index of the within-laboratory precision for repeated measurements; i.e., a measure of the ability of an average laboratory to repeat its results over a short period of time. It includes measurement error and sample variation.
- SD LABS - For each week the standard deviation of the means about the AV MEAN for that week after omitting those means marked with an 'X' or noted '+' in column V. The SD LABS is an index of the among-laboratory precision of the test method as applied by the participating laboratories; i.e., a measure of the ability of laboratories to get comparable results.
- NO. INCL - The number of laboratory means included in the AV MEAN for that week.
- NO. OMIT - The number of laboratory means reported but omitted from AV MEAN because of non-standard equipment, environment or procedure ('+' in column V) or because of extreme results (X following mean).
- NOT RCD - The number of laboratories failing to report data on time or in usable form for this week (but who reported data for at least one of the other weeks of this month), or who received test pieces from a different sample of material and whose data therefore are shown in another table of this report.
- SD SHTS - (Concora only) The average for the indicated week of the among-sheet within-laboratory standard deviations. The SD SHTS is an index primarily of the variability among sheets.

VALUES THIS MONTH:

THIS MONTH  
MEAN      SDR    SDWKS

- MEAN -      The average for the indicated laboratory of the reported weekly MEANS THIS MONTH.
- SDR -      The average for the indicated laboratory of the weekly SDRs for the current month.
- SDWKS -     For the indicated laboratory, the standard deviation among the laboratory's weekly MEANS THIS MONTH (including those means marked with an 'X').

CUMULATIVE VALUES:

CUMULATIVE  
MEAN      SDR    SDWKS    WKS

- MEAN -      The average for the indicated laboratory of all its weekly means for the number of weeks indicated, including those for the current month. An '\*' or 'X' following this CUMULATIVE MEAN indicates the laboratory is running consistently low or high. (See above for explanation of these flags).
- SDR -      The average for the indicated laboratory of the weekly SDRs for the indicated number of weeks.
- SDWKS -     For the indicated laboratory, the standard deviation among the laboratory's weekly means (including those means marked with an 'X'). SDWKS is an index of the week to week precision; i.e., a measure of the ability of a laboratory to repeat its results from week to week.
- WKS -      Number of weeks for which usable results have been reported by that laboratory. At most, 16 weeks of data are included.

GRAND AVERAGES

GRAND AVERAGES:      THIS MONTH      CUMULATIVE 12 WEEKS

- THIS MONTH - Averages for the four weeks of the quantities shown to the left.
- CUMULATIVE - Averages for the indicated number of weeks, including the four weeks of the current month.

AV SDWKS - The average of the SDWKS for all laboratories excluding those marked '+' in column V or with an 'X' following the corresponding THIS MONTH or CUMULATIVE MEAN or SDWKS.

SD CUM MEAN - The larger of either (1) the standard deviation of the CUMULATIVE MEANS about the average CUMULATIVE MEAN after omitting those CUMULATIVE MEANS marked with an 'X' or with a '+' in column V, or (2) the CUMULATIVE SD LABS divided by the square root of the number of weeks cumulated. The former will be appreciably larger than the latter only when there are persistent systematic differences among the laboratories.

INSTRUMENT CODES  
FOR  
MULLEN BURST OF LINERBOARD  
(Column V)

<u>Code</u>	<u>Description</u>
A	Model A, Manual Clamp
H	Model AH, Hydraulic Clamp
I	Model A, Hydraulic Clamp added
J	Jumbo, Hand Clamp, Hand Driven
L	Lhomargy, Hydraulic Clamp, in kPa
M	Model AH, Hydraulic Clamp, Transducer
R	Model A, Air Clamp added
X	Other Model, Please Describe Instrument Make and Model
Y	Nonstandard Instrument or Method
Z	Data received too late to be included in statistical analysis

INSTRUMENT CODES  
FOR  
CONCORA TEST OF MEDIUM  
(Column V)

<u>Code</u>	<u>Description</u>
Z	Data received too late to be included in statistical analysis

## Use of Average Mean as a Reference Standard

A large supply of linerboard in three weights was randomized and placed in sealed packages ready for shipment. The supply for each weight of board was divided into several narrow "rolls" or cross-machine "positions" of a larger roll, and each position was separately randomized. Each package contains test pieces from one position only. The position is designated by the number following the letter in the code marked on the package. Thus 42H 1 indicates that this package contains 42 lb board from position 1 of lot H. Samples from the first position are distributed until exhausted, then from the second position, and so forth for each weight of board. Thus for short periods of time (several weeks to months), the samples that the participants test are from the same position of a lot, and for a longer period from the same lot.

The three weights of linerboard distributed in this program may be used as reference standards. The best reference values are the cumulative grand AV MEANS in the latest reports. These values are given at the bottom right of each table. For each weight of board, comparisons should be made first for measurements made on the same position, i.e., for checking your current measurement, use grand AV MEANS that have the same position code as on the packages being tested. The position is shown in the upper left corner of the table. If no report is yet available on the current position, grand AV MEANS from previously tested positions of the same lot may be used as approximate reference values.

Similarly a large supply of a 26 lb corrugating medium was randomized, after dividing into several narrow rolls or positions. The above discussion for linerboard also applies to the corrugating medium.

We are currently using the fourth lot of linerboard and the fourth lot of corrugating medium:

<u>Lot</u>	<u>Material</u>	<u>Codes</u>	<u>Used</u>
1	linerboard	A,B,C	October 1969 - April 1973
2	linerboard	D,E,F	September 1972 - September 1976
3	linerboard	G,H,I,J	October 1976 - September 1979
4	linerboard	K,L,M	September 1979 -
1	corrugating medium	(A)	May 1973 - March 1976
2	corrugating medium	B	April 1976 - February 1977
3	corrugating medium	C	March 1977 - August 1978
4	corrugating medium	D	Septemher 1978 -

LAB CODE	V	MEANS THIS MONTH				THIS MONTH			CUMULATIVE			
		WK-1	WK-2	WK-3	WK-4	MEAN	SDR	SDWKS	MEAN	SDR	SDWKS	WKS
100	H	114.9	115.0	114.5	114.2	114.7	5.0	.4	115.4	6.0	1.2	6
101	H	119.3	120.3	120.3	121.0	120.2	4.7	.7	120.2	4.7	.7	4
102	H	116.1	116.9	116.5	111.9	115.4	5.1	2.3	115.8	5.9	2.4	6
103	I	113.7	114.7	114.4	116.8	114.9	5.0	1.3	115.2	5.1	1.6	6
105	M	121.3	118.9	119.2	120.3S	119.9	8.4	1.1	119.5	8.3	1.4	6
106	H	114.5	120.9	122.1	118.7	119.1	7.8	3.4	117.9	7.6	3.7	6
108	M	117.1	113.7	116.4	115.1	115.6	6.8	1.5	115.6	6.8	1.5	4
109	H	110.6	117.8	114.1	118.2	115.2	8.7	3.6	112.5	8.5	5.0X	6
110	M	115.2	115.8	113.4	114.8	114.8	6.9	1.0	114.4	7.5	1.0	6
111	M	113.5	112.9	116.6	113.7	114.2	8.7	1.7	114.6	8.6	2.4	6
112	H	115.6	108.1	109.8	110.9	111.1	4.4	3.2	110.2	4.6	3.0	6
113	R	118.7	117.1	119.3	119.9	118.8	6.3	1.2	117.9	6.7	1.7	6
114	M	114.6	112.2	121.2	116.9	116.2	6.7	3.8	116.6	7.5	3.0	6
115	R	116.8	123.0	116.1	121.2	119.3	4.6	3.4	117.3	5.4	4.1	6
117	H	112.4	108.9	110.5	111.6	110.9	6.5	1.5	109.7*	7.5	4.1	6
119	H	114.4	117.7	113.1	117.4	115.6	6.4	2.3	115.4	7.2	1.9	6
120	R	104.8X	107.3	109.3	107.9	107.3X	5.9	1.9	111.6	6.0	6.8X	6
121	M	119.6	118.4	115.5	115.7	117.3	7.6	2.0	117.7	7.1	1.8	6
123	R	109.4	103.5X	111.8	113.8	109.6	7.3	4.5	108.5*	7.3	4.1	6
125	I	119.3	122.1	119.0	116.2	119.2	6.0	2.4	118.1	6.4	2.5	6
127	H	110.6	111.0	110.2	112.2	111.0	6.2	.9	111.1	6.3	1.0	6
128	R	115.4	112.3	110.9	113.1	112.9	7.8	1.9	113.0	7.5	1.6	6
129	R	106.5X	104.9	108.7	118.7S	109.7	5.6	6.2	108.6*	5.0	5.1X	6
130	H	113.0	116.8	114.6	117.5	115.5	8.1	2.1	115.5	8.1	1.6	6
131	R	113.0	116.9	114.9	113.9	114.7	7.2	1.7	114.7	7.1	1.3	6
133	A	115.6	115.5	114.3	122.1	116.9	6.3	3.5	117.1	6.3	2.8	6
134	H	118.1	121.3	119.4	122.2	120.3	6.2	1.8	120.1	6.0	1.5	6
135	I	121.7	120.4	112.1	111.8	116.5	7.1	5.3	117.8	6.9	4.6X	6
136	H	114.0	113.8	113.4	109.5	112.7	7.0	2.1	112.7	7.0	2.1	4
137	H	119.1	119.5	126.6X	121.0	121.6	7.9	3.5	121.4	8.4	3.5	6
138	H	116.6S	116.3	118.2	118.6	117.4	9.0	1.1	117.7	8.8	2.2	6
139	R	126.9X	124.8	124.8	122.2	124.7X	6.8	1.9	124.4X	7.1	1.6	6
140	H	111.4	112.4	112.2	112.9	112.3	6.5	.6	113.2	6.0	1.6	6
141	M	115.4	112.4	115.3	113.8	114.2	6.3	1.4	114.0	6.3	1.5	6
142	A	114.8	109.7	113.2	108.1	111.5	7.2	3.1	111.1	7.0	2.7	6
143	H			121.9		121.9	6.9		122.2*	8.0	.5	2
145	H	116.1	112.6	108.1	117.2	113.5	6.3	4.1	113.5	6.2	3.6	6
147	H	111.4	113.7	112.2	115.2	113.2	6.8	1.7	112.5	6.9	1.9	6
149	H	124.0X	121.5	120.0	119.0	121.1	7.4	2.2	120.7	7.1	2.1	6
151	H	116.7	117.1	118.7	115.2	116.9	6.6	1.4	116.8	7.2	1.2	6
153	H	128.8X	130.6X	126.3X	127.1X	128.2X	9.2	1.9	127.8X	9.3	2.1	6
155	H	115.3	116.7	118.4	115.3	116.5	8.5	1.5	116.8	8.0	1.4	6
157	+X	117.5	114.6	113.4	120.1	116.4	7.1	3.0	116.7	6.7	2.6	6
161	+X	118.7	116.7	115.0	114.0	116.1	7.8	2.0	117.1	7.6	2.2	6
163	H	112.2	109.9	112.2	113.1	111.9	6.2	1.4	111.7	6.2	1.2	5
165	R	113.3	115.8	115.4	113.0	114.4	7.9	1.4	114.8	7.5	1.5	6
166	H	118.9	119.6	122.1		120.2	7.9	1.7	119.6	8.0	1.4	5
167	H	117.0	115.4	111.0	113.9	114.4	7.4	2.6	114.1	7.3	2.1	6
169	I	115.1	119.3	118.4	114.2	116.8	6.6	2.5	115.7	6.2	2.5	6
171	H	116.3	111.8	114.5	116.6	114.8	6.8	2.2	115.1	7.4	1.8	6
172	H	117.0	115.6	113.2	110.7	114.1	6.5	2.8	114.6	7.0	2.5	6
173	H	117.2S	115.1	115.6	115.8	115.9	4.0	.9	115.9	4.0X	.9	4
174	H	115.4	116.9	113.3	113.0	114.7	6.5	1.8	114.8	7.4	1.4	6
175	H	116.9	115.2	116.7	114.6	115.9	7.5	1.1	115.3	7.4	1.9	6
176	H	116.0	115.4	119.7	113.6	116.2	8.4	2.6	116.0	8.4	2.1	6

LAB CODE	V	MEANS THIS MONTH				THIS MONTH			CUMULATIVE			WKS
		WK-1	WK-2	WK-3	WK-4	MEAN	SDR	SDWKS	MEAN	SDR	SDWKS	
177	H	108.0X	106.8	107.8	109.5S	108.1	9.2	1.1	107.1X	8.8	2.0	6
182	H	115.4	123.8	117.6	119.1	119.0	6.4	3.6	118.5	6.8	3.0	6
184	H	122.1	117.7	121.9	117.2	119.8	8.4	2.6	119.2	7.5	2.2	6
186	I	113.1	107.8	111.8	114.9	111.9	6.0	3.0	113.4	6.2	3.9	6
188	I	115.2	112.3	117.4	117.4	115.6	7.4	2.4	116.8	7.3	2.7	6
198	R	118.4	114.7S	112.2	111.8	114.3	8.1	3.0	114.3	8.1	3.0	4
250	*L	103.1X	101.1X			102.1X	8.4	1.4	102.6X	9.1	1.0	4
274	H	114.8	114.9	115.3	115.0	115.0	6.5	.2	116.1	6.4	1.6	6
283	H	117.2	119.0	118.3	120.4	118.7	6.5	1.3	118.2	6.2	1.6	6
287	A	122.4	122.1	116.7	125.6X	121.7	6.7	3.7	120.7	7.2	3.3	6
350	H	113.8	112.3	115.1	107.2	112.1	9.4	3.5	112.1	9.4	3.5	4
553	M	115.1	113.7	116.9	113.0	114.7	8.3	1.7	115.4	7.9	1.8	6
562	A	125.6X	123.9	131.0X	130.8X	127.8X	8.6	3.6	127.9X	9.0	3.0	6
568	I	116.9	110.6	108.3	113.7	112.4	7.9	3.7	115.6	8.9	7.0X	6
569	A	131.3X	127.5X	121.8	125.0	126.4X	8.6	4.0	125.4X	7.8	3.5	6
658	H	117.7	118.2	117.3	118.1	117.9	7.0	.4	118.3	6.9	.8	6
682	*X	118.5	118.2	107.5	110.5	113.7	6.5	5.6	114.5	6.3	4.5	6
701	H	116.9	116.7	115.9	118.0	116.9	7.1	.8	116.8	7.6	1.1	6

	WK-1	WK-2	WK-3	WK-4	GRAND AVERAGES		
					THIS MONTH	CUMULATIVE	6 WEEKS
AV MEAN	115.8	115.7	115.5	115.6	AV MEAN	115.6	115.8
AV SDR	7.1	6.9	6.8	6.8	AV SDR	6.9	7.0
SD LABS	2.8	4.4	3.9	3.8	SD LABS	3.7	3.8
NO. INCL	60	65	66	64	NO. INCL	63.7	62.3
NO. OMIT	12	7	6	6	AV SDWKS	2.3	2.1
NET RCD	1	1	1	3	SD CUM MEAN		3.1

LAB CODE	V	MEANS THIS MONTH				THIS MONTH			CUMULATIVE			WKS
		WK-1	WK-2	WK-3	WK-4	MEAN	SDR	SDWKS	MEAN	SDR	SDWKS	
100	H	79.9	80.3	78.5	77.8	79.1	6.5	1.2	79.1	6.5	1.2	4
101	H	72.7	72.9	73.3	75.4	73.6	5.8	1.2	73.6*	5.8	1.2	4
102	H	78.4	80.2	78.0	77.2	78.5	5.6	1.2	78.5	5.6	1.2	4
103	I	77.7	79.1	78.3	78.0	78.3	4.8	.6	78.3	4.8	.6	4
105	M	87.3	82.3	83.7	84.8	84.6	6.6	2.1	84.6	6.6	2.1	4
106	H	79.3	84.2	85.4	83.5	83.1	7.7	2.7	83.1	7.7	2.7	4
108	M	78.6	78.5	80.8	79.3	79.3	6.4	1.0	79.3	6.4	1.0	4
109	H	73.2S	80.1	76.5	82.4	78.0	6.8	4.0	78.0	6.8	4.0X	4
110	M	83.8	83.1	84.4	83.7	83.7	6.3	.5	83.7	6.3	.5	4
111	M	78.2	81.3	79.9	79.5	79.7	6.3	1.3	79.7	6.3	1.3	4
112	H	71.6	73.4	71.9	75.8	73.2	5.9	1.9	73.2*	5.9	1.9	4
113	R	78.7	79.4	81.4	81.6	80.3	5.4	1.4	80.3	5.4	1.4	4
114	M	81.5	84.5	79.3	79.3	81.2	6.5	2.4	81.2	6.5	2.4	4
115	R	77.8	80.8	76.2	80.8	78.9	5.5	2.3	78.9	5.5	2.3	4
117	H	81.5	76.7	77.4	77.6	78.3	6.4	2.2	78.3	6.4	2.2	4
119	H	79.9	82.4	81.0	79.3	80.7	6.2	1.4	80.7	6.2	1.4	4
120	R	75.7	78.6S	78.8	78.9	78.0	7.1	1.5	78.0	7.1	1.5	4
121	M	84.4	85.5	81.5	85.4	84.2	6.1	1.9	84.2	6.1	1.9	4
123	R	73.7	76.0	75.1	79.4	76.1	6.9	2.4	76.1	6.9	2.4	4
125	I	84.9	83.1	84.5	87.9	85.1	5.6	2.0	85.1	5.6	2.0	4
127	H	76.1	78.7	78.4	80.1	78.3	5.9	1.7	78.3	5.9	1.7	4
128	H	82.3	79.9	77.1	79.7	79.7	6.5	2.1	79.7	6.5	2.1	4
129	R	74.8	74.8S	76.0	75.8	75.4	7.3	.7	75.4	7.3	.7	4
130	H	81.3S	80.8	79.2	83.8	81.3	8.6	1.9	81.3	8.6X	1.9	4
131	R	79.2	79.7	82.7	80.7	80.6	6.7	1.5	80.6	6.7	1.5	4
133	A	80.3	81.6	76.8	85.4	81.0	6.8	3.5	81.0	6.8	3.5	4
134	H	80.7	88.7	86.2	79.3	83.7	6.5	4.5	83.7	6.5	4.5X	4
135	I	77.9	87.2	76.6	78.8	80.1	6.2	4.8	80.1	6.2	4.8X	4
136	H	81.4	81.0	79.9	82.4	81.2	5.5	1.0	81.2	5.5	1.0	4
137	H	73.1	73.3	86.0	76.3	77.2	6.8	6.1	77.2	6.8	6.1X	4
138	H	86.8S	81.0	83.2	82.6	83.4	8.5	2.4	83.4	8.5X	2.4	4
139	R	88.6	88.8	90.3X	87.9	88.9X	6.9	1.0	88.9X	6.9	1.0	4
140	H	72.9	70.8X	73.2	73.1	72.5	5.0	1.1	72.5*	5.0	1.1	4
141	M	77.8	75.8	77.2	77.9	77.2	6.3	1.0	77.2	6.3	1.0	4
142	A	73.4	74.3	72.8	72.3	73.2	6.6	.9	73.2*	6.6	.9	4
143	H			79.6		79.6	6.8		79.6	6.8		1
145	H	80.8	83.1	78.0	76.7	79.7	5.4	2.9	79.7	5.4	2.9	4
147	H	80.0	79.1	83.4	79.6	80.5	7.9	2.0	80.5	7.9	2.0	4
149	H	88.5	85.2	83.5	84.2	85.4	6.8	2.2	85.4	6.8	2.2	4
151	H	78.0	75.7	77.0		76.8	5.0	1.0	76.8	5.0	1.0	4
153	H	82.7S	84.4	84.5	82.3	83.5	9.3	1.2	83.5	9.3X	1.2	4
155	H	79.4	79.3	80.8	79.8	79.9	6.1	.7	79.9	6.1	.7	4
157	*X	83.2	82.2	81.8	80.5	81.9	6.2	1.1	81.9	6.2	1.1	4
161	*X	78.5	79.2	83.1	83.3	81.0	7.0	2.5	81.0	7.0	2.5	4
163	H	79.0	79.8	77.8	77.3	78.5	6.7	1.1	78.5	6.7	1.1	4
165	R	78.7	82.1	80.4	83.3	81.2	6.1	2.0	81.2	6.1	2.0	4
166	H	78.6	76.9	78.3		77.9	5.6	.9	77.9	5.6	.9	3
167	H	75.8	78.0	77.5	76.4	77.9	5.8	1.4	77.9	5.8	1.4	4
169	I	81.1	81.6	83.1	80.7	81.6	5.5	1.1	81.6	5.5	1.1	4
171	H	76.0	81.0	82.5	81.9	80.3	7.7	3.0	80.3	7.7	3.0	4
172	H	81.9	74.9	78.0	76.0	77.7	6.6	3.1	77.7	6.6	3.1	4
173	H	82.2	79.4	81.2	82.5	81.3	4.8	1.4	81.3	4.8	1.4	4
174	H	83.4	81.7	81.4	81.9	82.1	6.1	.9	82.1	6.1	.9	4
175	H	83.4	81.7	84.4	79.1	82.2	6.4	2.3	82.2	6.4	2.3	4
176	H	78.9	78.5	81.9	79.8	79.8	6.4	1.5	79.8	6.4	1.5	4



LAB CODE	V	MEANS THIS MONTH				THIS MONTH			CUMULATIVE			WKS
		WK-1	WK-2	WK-3	WK-4	MEAN	SDR	SDWKS	MEAN	SDR	SDWKS	
177	H	73.4	74.0	72.6	74.5	73.6	5.6	.8	73.6*	5.6	.8	4
182	H	80.1	81.2	86.4	84.9	83.2	6.4	3.0	83.2	6.4	3.0	4
184	H	83.6	80.0	81.9	80.7	81.6	6.5	1.6	81.6	6.5	1.6	4
186	I	78.9	83.2	78.2	76.9	79.3	5.3	2.7	79.3	5.3	2.7	4
188	I	80.9	79.6	79.3	80.1	80.0	5.4	.7	80.0	5.4	.7	4
198	R	81.3	81.1	82.4	83.3	82.0	6.6	1.0	82.0	6.6	1.0	4
250	*L	71.4	70.3X			70.9X	5.5	.8	70.9X	5.5	.8	2
274	H	74.3	74.0	73.5	73.6	73.9	6.2	.4	73.9*	6.2	.4	4
283	H	80.0	82.3	83.5	81.4	81.8	6.7	1.5	81.8	6.7	1.5	4
287	A	88.7	85.7	86.7S	90.7X	88.0X	6.7	2.2	88.0*	6.7	2.2	4
350	H	78.7	79.3	77.8	81.8	79.4	5.6	1.7	79.4	5.6	1.7	4
553	M	79.38	83.1	83.8	86.4	83.2	7.8	2.9	83.2	7.8	2.9	4
562	A	82.0	86.4	86.2	85.0	84.9	7.5	2.0	84.9	7.5	2.0	4
568	I	79.6	77.8	77.0	78.2	78.2	7.1	1.1	78.2	7.1	1.1	4
569	A	79.5	85.5	84.9	81.6	82.9	5.9	2.8	82.9	5.9	2.8	4
658	H	84.3	83.8	81.2	78.2	81.9	5.6	2.8	81.9	5.6	2.8	4
682	*X	75.1	77.8	76.2	76.0	76.3	5.7	1.1	76.3	5.7	1.1	4
701	H	78.8	84.3	83.1	80.7	81.7	7.9	2.5	81.7	7.9	2.5	4

	WK-1	WK-2	WK-3	WK-4	GRAND AVERAGES		
					THIS MONTH	CUMULATIVE	4 WEEKS
AV MEAN	79.7	80.5	80.1	80.2	AV MEAN	80.1	80.1
AV SDR	6.1	6.2	6.4	6.5	AV SDR	6.3	6.3
SD LABS	3.9	3.7	3.8	3.5	SD LABS	3.7	3.7
NO. INCL	68	67	68	66	NO. INCL	67.2	67.2
NO. OMIT	4	5	4	4	AV SDWKS	1.9	1.7
NOT RCD	1	1	1	3	SD CUM MEAN		3.1

LAB CODE	V	MEANS THIS MONTH				THIS MONTH			CUMULATIVE			
		WK-1	WK-2	WK-3	WK-4	MEAN	SDR	SDWKS	MEAN	SDR	SDWKS	WKS
100		77.7	72.9	72.6	72.6	74.0	4.3	2.5	73.6	4.4	1.4	16
102		72.4	73.2	71.5	72.5	72.4	2.8	.7	72.0	2.9	.9	14
105		72.3	73.3S	72.6	71.8	72.5	4.4	.6	75.0	4.2	3.0	16
106		74.3	73.2	72.9	72.0	73.1	3.8	1.0	73.3	3.7	.7	16
110		73.9	73.4	75.5	75.8	74.7	4.1	1.2	73.3	3.9	1.3	15
113		71.4	71.6	70.9	71.7	71.4	2.4	.4	71.4	2.7	.4	16
114		69.2	72.0	71.0	69.8	70.5	2.1	1.3	70.6	2.6	.9	16
115		76.2	72.1	72.6	73.1	73.5	4.3	1.9	74.2	4.0	1.7	16
119		69.1	71.7	68.3	75.0	71.0	4.0	3.0	69.9	3.8	2.1	14
120		69.2	69.9	68.3	70.1	69.4	3.3	.8	69.8	3.3	1.2	15
125		80.3X	80.0X	82.0X	84.2X	81.6X	4.2	1.9	80.2X	4.7	2.4	16
128		72.5	72.4	72.0	71.4	72.1	3.3	.5	72.6	3.2	.9	16
136				71.6	74.0	72.8	4.0	1.7	73.4	4.2	2.1	6
138		77.9	76.3	77.2	76.9	77.1	3.9	.7	75.7	4.2	1.5	16
140		72.6	72.6	73.7	73.8	73.2	4.3	.7	75.5	4.2	2.2	16
143		74.0	72.5			73.3	3.9	1.0	72.8	3.1	.7	9
151		71.3	73.3	71.9	73.4	72.5	3.5	1.0	70.5	3.9	2.9	11
161		86.0XS	79.8X	79.5X	71.4	79.2X	5.0	6.0	73.9	4.7	4.5X	16
164		67.3	70.1	69.4	71.6	69.6	2.8	1.8	68.6*	3.4	2.7	12
167		72.3	76.0	74.1	74.3	74.2	3.0	1.5	73.2	3.8	1.4	16
177		71.2	71.8	73.2	70.3	71.6	3.3	1.2	70.7	3.5	1.4	14
182		73.7	71.2	72.9	72.6	72.6	4.0	1.0	77.2*	4.1	3.5	16
188		72.8	70.5	70.7	69.9	71.0	3.4	1.3	71.5	3.2	1.1	16
198		75.2	74.3	74.3	72.0	74.0	4.0	1.4	71.8	4.1	3.5	6
237		72.6	74.5S	72.1	73.2	73.1	5.2	1.0	72.7	4.3	1.3	12
250		69.7	69.8			69.8	2.9	.1	71.0	2.5	1.2	12
269		74.4	73.8	72.5	74.6	73.8	3.7	.9	72.8	3.7	1.3	16
274		72.2	72.5	73.3	72.9	72.7	3.3	.5	72.9	3.0	.4	16
283		72.3	73.2	72.9	74.7	73.3	2.6	1.0	73.0	3.0	1.9	16
284		71.7	71.5	69.6	68.6	70.4	4.0	1.5	69.3	3.7	2.8	15
287		72.6	73.0	74.3	76.2S	74.1	4.3	1.6	74.3	4.1	1.7	16
289		56.3X	67.2X	52.9X	59.2X	58.9X	2.3	6.1	59.6X	3.1	7.0X	15
292		71.7	69.6	70.4	71.0	70.7	2.8	.9	68.4*	3.1	2.7	16
350		87.4X	87.7X	84.3X	86.3X	86.4X	4.7	1.5	85.2X	4.8	1.9	14
351		68.5	70.5	72.0	72.4	70.9	2.2	1.8	71.8	2.4	1.2	16
353		74.3		76.3	79.5X	76.7	3.6	2.6	73.4	3.8	2.7	15
355		71.7	73.5	71.9	73.1	72.6	3.5	.9	73.1	3.3	2.1	16
357		73.9	74.7	74.6		74.4	3.8	.4	74.4	4.0	1.4	13
361		70.7	69.9	71.8		70.8	3.1	1.0	70.9	3.4	1.6	14
363		66.4	68.8	69.4	71.2	69.0	3.5	2.0	69.0	3.7	1.9	16
365		68.1	70.0	69.3	70.6	69.5	3.4	1.1	69.7	3.3	2.0	16
367			74.8	75.4	73.5	74.6	3.7	1.0	74.3	4.1	2.0	13
369		73.1	70.6	73.1	72.4	72.3	3.2	1.2	72.6	3.3	.8	16
377		75.3	75.3S	74.1	75.9	75.2	4.7	.8	75.5	4.2	1.3	16
379		74.9	73.4	74.0	73.9	74.1	3.9	.6	73.9	4.0	1.2	15
381		71.9	74.8	72.0	73.7	73.1	3.2	1.4	71.9	3.4	1.4	15
383		72.9	74.5	75.5	78.5X	75.4	3.0	2.4	75.0	3.5	3.7	16
385		74.0	71.9	74.7	68.8	72.4	4.4	2.7	73.1	4.8	3.1	16
387		72.5	71.8	73.1	72.1	72.4	4.0	.6	73.5	3.7	1.7	16
391		70.1	68.8	75.0	74.6S	72.1	3.8	3.1	70.1	3.4	3.0	16
393		72.4	74.2	73.6	74.7	73.8	4.2	1.0	73.8	3.9	2.4	16
395		72.9	73.9	75.2	74.2	74.1	3.6	.9	73.5	3.7	1.1	16
397		72.8	74.0	70.5	71.3	72.2	4.3	1.6	73.6	4.1	1.7	16
399		69.1	73.3	69.7	72.2	71.1	4.0	2.0	73.7	4.0	2.8	14
553		69.4	75.2	72.2	71.1	72.0	3.0	2.5	71.7	3.0	2.2	16

LAB CODE V	MEANS THIS MONTH				THIS MONTH			CUMULATIVE			WKS
	WK-1	WK-2	WK-3	WK-4	MEAN	SDR	SDWKS	MEAN	SDR	SDWKS	
555	74.2	74.8	74.8	73.7	74.4	2.1	0.5	74.2	2.4	1.5	16
562	72.4	71.6	73.6	71.3	72.3	3.5	1.0	71.8	3.9	1.6	16
568	70.0	65.1X	70.7	76.6	70.6	3.4	4.7	69.5	3.3	3.5	16
572	72.4	74.5	73.9	72.2	73.3	3.9	1.1	73.7	3.9	2.4	15
578	77.9	74.7	72.0	74.5S	74.8	4.4	2.4	70.6	4.2	8.5X	16
609	78.2	75.8	76.4	76.2	76.6	3.5	1.1	75.9	3.6	2.0	16
617	77.0	76.6S	75.6S	67.9S	74.3	6.6	4.3	77.2*	6.2X	4.1X	16

	WK-1	WK-2	WK-3	WK-4	GRAND AVERAGES		
					THIS MONTH	CUMULATIVE 16 WEEKS	
AV MEAN	72.5	72.8	72.7	72.8	AV MEAN	72.7	72.6
AV SDR	3.6	3.5	3.6	3.4	AV SDR	3.5	3.6
SD LABS	2.6	2.0	2.1	2.1	SD LABS	2.2	2.4
NO. INCL	56	55	50	53	NO. INCL	55.0	53.0
NO. OMIT	4	5	4	5	AV SDWKS	1.6	1.8
NOT RCD	2	2	2	4	SD CUM MEAN		2.1
SD SHTS	2.0	2.2	2.0	2.3			

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO.  FKBG CRP 121	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE CONTAINERBOARD Collaborative Reference Program for Containerboard Report No. 121		5. Publication Date November 30, 1979	
7. AUTHOR(S) T.L. Cummings, J. Horlick		6. Performing Organization Code	
9. PERFORMING ORGANIZATION NAME AND ADDRESS  NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, DC 20234		8. Performing Organ. Report No. NBSIR 79-1816	
12. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS (Street, City, State, ZIP) Collaborative Testing Services, Inc. 9241 Wood Glade Drive, Great Falls, VA 22066 and American Paper Institute/Fourdrinier Kraft Board Group		10. Project/Task/Work Unit No.	
15. SUPPLEMENTARY NOTES  <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.		11. Contract/Grant No.	
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.)  Collaborative Reference Programs provide participating laboratories with the means for checking periodically the level and uniformity of their testing in comparison with that of other participating laboratories. An important by-product of the programs is the provision of realistic pictures of the state of the testing art. This is one of the periodic reports showing averages for each participant, within and between laboratory variability, and other information for participants and standards committees.		13. Type of Report & Period Covered  FINAL	
17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons)  Collaborative reference program; Containerboard; Laboratory evaluation; Precision; Reference samples; Testing calibration		14. Sponsoring Agency Code	
18. AVAILABILITY <input type="checkbox"/> Unlimited  <input checked="" type="checkbox"/> For Official Distribution. Do Not Release to NTIS  <input type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office, Washington, DC 20402, SD Stock No. SN003-003-  <input type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA, 22161	19. SECURITY CLASS (THIS REPORT)  UNCLASSIFIED	21. NO. OF PRINTED PAGES  15	
	20. SECURITY CLASS (THIS PAGE)  UNCLASSIFIED	22. Price	



