


Reference

NBS  
Publi-  
cations

NAT'L INST. OF STAND & TECH



A11107 386203



TECHNICAL ASSOCIATION OF THE  
PULP AND PAPER INDUSTRY

NBSIR 80-1833

COLLABORATIVE REFERENCE PROGRAM  
FOR PAPER

REPORT NO. 63G



U.S. DEPARTMENT OF COMMERCE  
National Bureau of Standards

QC

100

.U56

80-1833

1980

NBS COLLABORATIVE REFERENCE PROGRAMS

TAPPI Paper and Board (6 times per year)

Bursting strength	Smoothness
Tearing strength	Surface pick strength
Tensile breaking strength	K & N ink absorption
Elongation to break	Moisture content
Tensile energy absorption	Opacity
Folding endurance	Blue reflectance (brightness)
Stiffness	Specular gloss, 75°
Air resistance	Thickness
Grammage	Concora (flat crush)
	Ring crush

FKBG-API Containerboard (48 times per year)

Mullen burst of linerboard  
Concora test of medium

MCCA Color and Appearance (4 times per year)

Gloss at 60°  
Color and color difference

CTS Rubber (4 times per year)

Tensile strength, ultimate elongation and tensile stress  
Hardness  
Mooney viscosity  
Vulcanization properties

ASTM Cement (2 times per year)

Chemical (11 chemical components)  
Physical (15 characteristics)

AASHTO Bituminous

Asphalt cement (2 times per year)  
Cutbacks (once a year)

NBS Collaborative Reference Programs  
A05 Technology Building  
National Bureau of Standards  
Washington, DC 20234

SEP 19 1980

100-10-1-100  
50-100  
1156  
70-1833  
1485

**TECHNICAL ASSOCIATION OF THE  
PULP AND PAPER INDUSTRY**

**COLLABORATIVE REFERENCE PROGRAM  
FOR PAPER**

Report No. 63G

**R. G. Powell  
CTS-NBS Research Associate  
Collaborative Testing Services, Inc.**

**J. Horlick  
Office of Testing Laboratory Evaluation Technology  
Office of Engineering Standards  
National Engineering Laboratory**

**NBSIR 80-1833**

**U.S. DEPARTMENT OF COMMERCE  
National Bureau of Standards**



## INTRODUCTION

Reports 63S and 63G comprise the third set of reports for the 79-80 program year. Participants in tests which involve strength properties of paper will receive only the S report; those in tests which measure other properties will receive only the G report.

Notes and comments to individual laboratories and "Best Values" applicable to a particular method are given following Table 1 for each method. See page 1 of this report for an explanation of "Best Values". Please do not confuse these Best Values with provisional values included with the samples to detect serious discrepancies at the time of test.

If there are any questions on the notes, the analyses, or the reports in general, contact Robert G. Powell or Jeffrey Horlick on 301/921-2946.



Jeffrey Horlick, Administrator  
NBS-TAPPI Collaborative Reference Program  
Office of Testing Laboratory Evaluation Technology

June 13, 1980



## TAPPI-NBS COLLABORATIVE REFERENCE PROGRAM

### BACKGROUND AND PURPOSE

In 1969, the National Bureau of Standards and the Technical Association of the Pulp and Paper Industry established a collaborative reference program to provide a participating laboratory with a means to check periodically the level and uniformity of its testing in comparison with that of other laboratories.

The interchange of paper and board products and of the raw materials for these products requires agreement among raw material suppliers, paper and board producers, converters, distributors, retailers, commercial testing laboratories, user organizations and the ultimate consumer as to the meaning of test results, an agreement that cannot be achieved without accurate and precise testing. This program is designed to help assure agreement.

### HOW THE PROGRAM WORKS

Participants Select the Tests in which they wish to participate. This choice is made on joining the program, but additional tests may be added at any time. Also new participants may enter the program at any time.

Test Samples are Distributed Bimonthly; i.e. every 2 months.

Provisional Values are Provided with the Samples for one or both of the test levels, depending on method. The provisional values permit serious discrepancies to be detected without delay. (It is left to the discretion of the laboratory supervisor as to whether these values should be known to the operator.)

Each Participant Tests the Samples, following instructions provided for each test method. The full check on a single instrument should normally take no more than 30 minutes. The test results are then sent to NBS for analysis. The participant is also asked to report other information relevant to an accurate analysis, such as test conditions and the instruments used.

Industry Means, Best Values and Other Statistics are developed from the data by NBS. The best values are estimates based on a careful examination of all data, both current and past, with special attention to results obtained by the National Bureau of Standards and other recognized reference laboratories in this and other countries.

A Quick Report is Prepared for each participating laboratory reporting data on time. This report shows the industry mean values, and the deviations of the laboratory's results from these values for each test method.

A Longer Summary Report, Showing the Data from all Participants, is also prepared. In the summary report, of which this report is an example, each laboratory is identified by a code number so that the information is maintained on a confidential basis. However, instruments are identified by type so participants can compare their results with those obtained on similar instruments of different manufacture. This report includes test averages, best values and standard deviations for individual participants and for the group as a whole. A participant should be able to readily determine the level and variability of his results in comparison with those of the other laboratories.

Repeatability and Reproducibility Statements such as Contained in ASTM, TAPPI and ISO Standards are included at the end of the report. Participants can check their performance level against the precision statement given in the test method or specification.

TABLE OF CONTENTS

Analyses In This Report

PAGE  
-----

1	Introduction
ii	Description of Program
iv	Metric Conversion Table
1	Key to Tables and Graphs
3	40-1 Air Resistance, Gurley Oil type
6	40-2 Air Resistance, Sheffield type
9	41-1 Air Resistance, Gurley Mercury type
11	44-1 Smoothness, Parker Printsurf
12	45-1 Smoothness, Sheffield type
17	45-2 Smoothness, Bekk type
19	47-1 Smoothness, Bendtsen type
21	53-1 Moisture
23	56-1 K & N Ink Absorption
25	60-1 Opacity, White (89%) Backing, Fine papers
30	60-2 Opacity, Paper Backing, Elrepho type, Fine papers
32	61-1 Opacity, White (89%) Backing, News Paper
35	65-1 Blue Reflectance (Brightness), Directional
38	65-2 Blue Reflectance, Diffuse, Elrepho (Gloss Trap)
40	65-3 Blue Reflectance, Diffuse, Elrepho (No Gloss Trap)
42	75-1 Specular Gloss, 75 degree, High Range
45	76-1 Specular Gloss, 75 degree, Low range
47	90-1 Thickness (Caliper)
52	95-1 Grammage (Basis Weight)
55	Summary

Analyses In The S Report

10-1	Bursting Strength - Up to 45 psi
10-2	Bursting Strength - Up to 45 psi, Air Clamps
11-1	Bursting Strength - Up to 100 psi
15-1	Tearing Strength - Printing Papers
16-1	Tearing Strength - Packaging Papers
19-1	Tensile Breaking Strength - Packaging Papers
20-1	Tensile Breaking Strength - Printing Papers, CRE
20-2	Tensile Breaking Strength - Printing Papers, Pendulum
25-1	Tensile Energy Absorption - Packaging Papers
26-1	Tensile Energy Absorption - Printing Papers
28-1	Elongation to Break - Packaging Papers
29-1	Elongation to Break - Printing Papers
30-1	Folding Endurance, MIT type
30-2	Folding Endurance, MIT type, log (base 10)
35-1	Stiffness, Gurley
36-1	Stiffness, Taber
49-1	Surface Pick Strength, IGT
50-1	Surface Pick Strength, Wax
91-1	Concora (Flat Crush)
96-1	Ring Crush

TABLE OF CONVERSION FACTORS TO METRIC (SI) UNITS

<u>Physical Quantity</u>	<u>To Convert From</u>	<u>To</u>	<u>Multiply by</u>
Bursting strength	psi	kPa	6.895
	kg/cm <sup>2</sup>	kPa	98.07
	bar	kPa	100.00
Tearing strength	g	mN	9.807
Tensile strength	lb/in.	kN/m	.1751
	lb/0.5 in.	kN/m	.3502
	lb/15 mm	kN/m	.2965
	kg/15 mm	kN/m	.6538
	kg/25 mm	kN/m	.3923
	kg/mm	kN/m	9.807
	Tensile energy absorption	ft-lb/ft <sup>2</sup>	J/m <sup>2</sup>
in.-lb/in. <sup>2</sup>		J/m <sup>2</sup>	175.1
kg-m/m <sup>2</sup>		J/m <sup>2</sup>	9.807
Bending stiffness	g·cm	μN·m	98.07
Flat-crush strength (Concora)	lb	N	4.448
Ring-crush (TAPPI)	lb	N	4.448
	(ISO)	lb/6.00 in.	kN/m
Thickness	mil	μm	25.40



KEY TO TABLES AND GRAPHS

- MEAN - The average of individual TEST DETERMINATIONS. The number of TEST DETERMINATIONS in the mean is given in the upper right corner of the first table (TEST D.) and again at the bottom of this table.
- GRAND MEAN - (GR. MEAN) The average of the individual laboratory MEANS, excluding laboratories flagged (see column F) with an X, #, or +. The GRAND MEAN is given in US customary units and, where applicable, in SI metric units.
- SD OF MEANS - (SD MEANS) The standard deviation of the laboratory MEANS about the GRAND MEAN; an index of the among-laboratory precision.
- DEV - The deviation or difference of the laboratory MEAN from the GRAND MEAN.
- N. DEV - The normal deviate or ratio of the DEV to the SD OF MEANS; an indication of the degree of divergence of the laboratory MEAN from the GRAND MEAN. A N. DEV of more than 2 or less than -2 may indicate that the participant is not following the procedure considered standard for this analysis.
- SDR - The standard deviation of repeated measurements; that is, of individual test determinations about their MEAN.
- AVERAGE SDR - The average of the individual laboratory SDR's; an index of the within-laboratory precision of repeated measurements.
- R. SDR - The relative standard deviation of repeated measurements; that is, the ratio of the SDR to the AVERAGE SDR; an indication of the ability of a participant to repeat his or her measurements relative to the average ability. The greater the number of TEST DETERMINATIONS the closer the R. SDR should be to unity. If R. SDR is outside the limits given below, the participant may not be following the procedure considered standard for this analysis:
- | No. of test Determinations | Lower limit for R. SDR | Upper limit for R. SDR |
|----------------------------|------------------------|------------------------|
| 3                          | 0.09                   | 2.58                   |
| 4                          | 0.12                   | 2.25                   |
| 5                          | 0.26                   | 2.06                   |
| 8                          | 0.40                   | 1.77                   |
| 10                         | 0.46                   | 1.67                   |
| 15                         | 0.56                   | 1.53                   |
| 20                         | 0.61                   | 1.45                   |
| 25                         | 0.65                   | 1.39                   |
- VAR - Code for instrument type or variation in condition, see second table.
- F - Flag, with following meaning:
- Ø - Included in grand mean and inside 95% error ellipse.
  - \* - Included in grand means but plotted point falls outside of the 95% error ellipse. The participant should take this as a warning to reexamine his or her testing procedure.
  - X - Excluded because plotted point would fall outside of the 99% error ellipse, (see page 2 for explanation of Graph).
  - # - Excluded because data were not understood or because of a non-coded variation reported by the laboratory. (See the notes following Table 1 for each method).
  - + - Excluded from grand means because VAR was non-standard for the analysis.
  - M - Excluded because data for one sample are missing.
  - S - Included in grand mean but only after omission of one or more 'wild' values; that is test determinations more than 3 times AVERAGE SDR from the laboratory's MEAN. Not more than 20% of the test determination may be excluded in this manner without rejecting the laboratory.
- Best values - Given at the end of Table 1 for each method for which sufficient information is available. These best values are estimates based on a careful examination of all data, both current and past, with special attention to results obtained by the National Bureau of Standards and other recognized reference laboratories in this and other countries. All participants using equipment that is standard for the analysis should be able to achieve results within the plus-minus (+/-) limits, when these are shown along with the best values.
- COORDINATES - Distances along major and minor axes of error ellipse. If special additive or concurrent model of the measuring process applies to this method, the distance along the minor axis represents the random error within a laboratory while that along the major axis also includes a systematic laboratory component of error.
- 95% ELLIPSE - Lengths of the major and minor axes of the ellipse and the angle that the major axis makes with the horizontal axis.
- AVG P. SDR - Average of the R. SDR for the two samples; an indication of the laboratory's precision of repeated measurements.

Graph -

For each laboratory the MEAN for the second sample is plotted against the MEAN for the first sample, with each point representing a laboratory. The horizontal and vertical lines are the GRAND MEANS. The dashed line is drawn at 45 degrees. The solid sloping line, which may or may not lie close to the 45 degree line, is along the major axis of the error ellipse. The ellipse is drawn so that, on the average, it will include 95% of the points representing the laboratories.

Plotted symbols are as explained above (under F), except that an 'S' is plotted as an 'G'. A participant whose plotted point falls outside of the ellipse should carefully reexamine the testing procedure he or she is following.

The graph is plotted with an ellipse when there are 20 or more laboratories in the analysis. When there are 10 through 19 laboratories in the analysis, the graph is plotted but the ellipse is omitted. When there are fewer than 10 laboratories retained in the analysis, the graph is not plotted.

The International System of Units (SI) is used on the plots wherever possible to aid participants in familiarizing themselves with SI. Grand means in SI units are given at the top of the plot, and supplementary scales in SI units are drawn along the axes allowing the reader to compare means and variability in common units and SI units for the same data.

SUMMARY -  
(At end of report)

In addition to several quantities already defined above, the summary shows the following values for each test method:

REPL CRP -

The number of replicate test determinations used in this Collaborative Reference Program.

REPL TAPPI -

The number of replicate test determinations in a test result required by the applicable TAPPI Official Test Method or assumed here if there is no TAPPI Official Test Method. This quantity is needed in the computation of TAPPI repeatability and reproducibility from the SD OF MEANS and the AVERAGE SDR. See TAPPI Official Test Method T1206 for definitions and computations.

REPEAT -

TAPPI repeatability; a measure of the within-laboratory precision of a test result.

REPROD -

TAPPI reproducibility; a measure of the between-laboratory precision of a test result.

ANALYSIS 140-1 TABLE 1  
 AIR RESISTANCE, GURLEY UNITS (SECONDS/100 CC)  
 TAPPI OFFICIAL TEST METHOD T460 68-75, AIR RESISTANCE OF PAPER

LAB CODE	SAMPLE B68 MEAN	HEAT-SET OFFSET BOOK 93 GRAMS PER SQUARE METER				SAMPLE Z08 MEAN	M.F. SULPHITE 36 GRAMS PER SQUARE METER				TEST D. = 10		
		DEV	N. DEV	SDR	R. SDR		DEV	N. DEV	SDR	R. SDR	VAR	F	LAB
L100	44.6	-4.6	-1.44	3.5	.75	89.8	-6.0	-7.7	7.0	.78	40D	6	L100
L106	46.5	-2.7	-0.85	5.6	1.19	93.6	-2.2	-2.8	10.8	1.21	40D	6	L106
L107	46.9	-2.3	-0.72	4.8	1.02	92.5	-3.3	-4.2	10.6	1.19	40D	6	L107
L121	50.5	1.3	.40	5.1	1.05	85.0	-10.8	-1.37	9.5	1.07	40D	6	L121
L122	51.5	2.2	.70	3.8	.81	98.3	2.5	.31	6.1	.68	40D	6	L122
L123	50.2	.9	.29	4.4	.94	95.7	-0.1	-0.01	9.9	1.11	40D	6	L123
L124G	48.5	-0.7	-0.23	6.3	1.33	106.0	10.2	1.29	9.9	1.12	40D	6	L124G
L125	48.9	-0.3	-0.10	4.4	.94	97.7	1.9	.24	8.9	1.00	40D	6	L125
L128	52.3	3.1	.56	5.7	1.22	100.2	4.4	.55	10.9	1.22	40D	6	L128
L141	49.2	.0	.01	5.1	1.05	99.4	3.6	.45	10.8	1.21	40D	6	L141
L148	48.7	-0.5	-0.16	3.8	.81	102.5	6.7	.85	4.8	.54	40D	6	L148
L153	49.1	-1.1	-0.35	4.4	.94	94.1	-1.7	-2.2	7.6	.85	40D	6	L153
L158	47.5	-1.7	-0.54	4.7	.99	90.0	-5.8	-0.74	4.8	.54	40D	6	L158
L159	44.1	-5.1	-1.58	2.9	.61	82.7	-7.1	-0.90	12.7	1.43	40D	6	L159
L163	45.8	-3.4	-1.07	2.0	.43	95.2	-0.6	-0.02	5.6	.63	40D	6	L163
L166	51.4	2.2	.67	4.6	.97	103.8	8.0	1.02	10.7	1.20	40D	6	L166
L174	48.1	-1.1	-0.34	4.7	.99	98.5	2.6	.33	7.9	.89	40D	6	L174
L176	50.0	.8	.23	4.7	1.00	93.7	-2.1	-0.27	5.0	.56	40D	6	L176
L182G	50.5	1.3	.40	8.2	1.74	92.1	-3.7	-0.47	11.7	1.31	40D	6	L182G
L183	49.7	.5	.15	8.5	1.81	96.4	.6	.07	13.1	1.47	40D	6	L183
L190C	53.2	4.0	1.24	5.3	1.13	95.3	-0.5	-0.07	9.1	1.02	40D	6	L190C
L190R	39.2	-10.0	-3.12	3.5	.74	82.6	-13.2	-1.68	10.9	1.23	40D	6	L190R
L212	46.7	-2.5	-0.79	5.4	1.14	95.1	-0.7	-0.09	13.8	1.55	40D	6	L212
L219	47.1	-2.1	-0.66	2.8	.60	80.5	-15.3	-1.95	6.7	.75	40D	6	L219
L223	51.8	2.6	.80	4.6	.97	101.7	5.9	.75	4.9	.56	40D	6	L223
L230G	49.9	.7	.21	4.5	.95	104.1	8.3	1.05	8.6	.96	40D	6	L230G
L238A	47.2	-2.0	-0.63	6.1	1.28	84.8	-11.0	-1.40	10.7	1.21	40D	6	L238A
L241	45.4	-3.8	-1.19	3.6	.76	81.0	-14.8	-1.88	8.4	.94	40D	6	L241
L242	35.1	-14.1	-4.39	3.1	.67	51.8	-44.0	-5.55	4.7	.53	40D	6	L242
L243G	51.3	2.1	.64	3.6	.76	88.1	-7.7	-0.98	8.4	.94	40D	6	L243G
L254	52.2	3.0	.92	4.4	.94	97.8	2.0	.25	9.0	1.01	40D	6	L254
L259	47.3	-1.5	-0.59	5.6	1.10	92.9	-2.9	-0.37	10.3	1.16	40D	6	L259
L261	48.4	-0.8	-0.26	3.0	.63	47.8	-48.0	-6.05	2.8	.31	40D	6	L261
L262G	43.0	-6.2	-1.94	4.2	.89	58.1	-37.7	-4.72	3.2	.36	40D	6	L262G
L278	47.4	-1.9	-0.58	3.9	.82	79.4	-16.5	-2.05	9.0	1.02	40D	6	L278
L285	50.7	1.5	.46	2.9	.62	103.4	7.6	.96	10.0	1.12	40D	6	L285
L308	53.7	4.5	1.39	2.5	.53	95.4	-0.4	-0.05	8.9	1.00	40D	6	L308
L313	48.0	-1.2	-0.37	5.4	1.14	98.0	2.1	.27	10.0	1.12	40D	6	L313
L320	43.2	-6.0	-1.87	2.5	.54	80.8	-15.0	-1.51	2.5	.28	40D	6	L320
L321	49.4	.2	.05	3.0	.63	106.4	10.6	1.34	9.8	1.10	40D	6	L321
L324	51.1	1.9	.60	7.1	1.51	95.1	-0.7	-0.09	6.7	.75	40D	6	L324
L326	53.5	4.3	1.33	5.0	1.06	102.0	6.2	.78	9.0	1.01	40D	6	L326
L328	54.4	5.2	1.60	6.7	1.41	100.1	4.2	.54	12.8	1.44	40D	6	L328
L337	46.0	-3.2	-0.99	6.0	1.27	94.7	-1.1	-0.14	7.5	.85	40D	6	L337
L339	41.7	-7.5	-2.33	5.1	1.05	64.8	-31.0	-3.94	8.9	1.00	40D	6	L339
L348	54.1	4.9	1.52	4.9	1.05	107.6	11.8	1.49	8.0	.90	40D	6	L348
L376	53.6	4.3	1.35	7.4	1.56	109.1	13.3	1.65	28.0	3.15	40D	6	L376
L380	50.8	1.6	.49	4.9	1.04	92.3	-3.5	-0.45	6.2	.70	40D	6	L380
L388	51.7	2.4	.76	5.2	1.10	106.6	10.7	1.36	9.8	1.11	40D	6	L388
L396M	51.1	1.5	.58	5.8	1.24	98.8	3.0	.38	4.6	.52	40D	6	L396M
L484	45.8	-3.4	-1.07	4.1	.87	90.7	-5.1	-0.65	8.0	.90	40H	6	L484
L554	55.2	6.0	1.86	6.7	1.43	117.2	21.4	2.71	10.7	1.20	40D	6	L554
L567	51.4	2.2	.68	4.2	.90	95.3	3.4	.44	11.4	1.28	40D	6	L567
L576	49.6	.4	.12	4.8	1.02	82.7	-7.1	-0.90	5.7	.64	40D	6	L576
L585	51.6	2.4	.74	7.5	1.58	105.4	9.6	1.21	11.2	1.26	40D	6	L585
L616	45.3	-3.9	-1.22	1.8	.35	93.9	-1.9	-0.25	3.7	.42	40D	6	L616
L636	44.5	-4.7	-1.47	4.7	1.00	85.1	-10.7	-1.36	6.7	.75	40D	6	L636
L651	35.6	-13.6	-4.24	4.9	1.04	70.6	-25.2	-3.20	8.7	.98	40D	6	L651
L676	51.6	2.3	.73	3.9	.82	105.2	9.4	1.19	7.7	.86	40D	6	L676
L697	47.1	-2.1	-0.66	3.4	.72	93.1	-2.7	-0.35	9.4	1.06	40D	6	L697
L702	50.5	1.3	.40	5.8	1.22	96.0	.2	.02	7.9	.89	40D	6	L702
L715	53.8	4.6	1.43	4.0	.85	102.2	6.4	.81	6.4	.72	40D	6	L715
L737	45.7	-3.5	-1.09	3.4	.72	94.5	-1.3	-0.17	8.9	1.00	40D	6	L737

GR. MEAN = 49.2 GURLEY UNITS      GRAND MEAN = 95.8 GURLEY UNITS      TEST DETERMINATIONS = 10  
 SD MEANS = 3.2 GURLEY UNITS      SD OF MEANS = 7.9 GURLEY UNITS      58 LABS IN GRAND MEANS  
 AVERAGE SDR = 4.7 GURLEY UNITS      AVERAGE SDR = 8.9 GURLEY UNITS

L115 45.2 -4.0 -1.25 1.7 .36      NO DATA REPORTED FOR SAMPLE Z08      40U \* L115  
 L291 46.4 -2.8 -.88 5.4 1.14      112.8 17.0 2.15 6.8 .76      40U \* L291

TOTAL NUMBER OF LABORATORIES REPORTING = 65

Best values: B68 49.3 ± 4.7 Gurley units  
 Z08 96 ± 12 Gurley units

The following laboratories were omitted from the grand means because of extreme test results: 242, 261, 262G, 339, 651




AIR RESISTANCE, GURLEY UNITS (SECONDS/100 CC)  
TAPPI OFFICIAL TEST METHOD T460 GS-75, AIR RESISTANCE OF PAPER

LAB CODE	F	MEANS		COORDINATES		AVG R <sub>0</sub> SDR VAR	PROPERTY---TEST INSTRUMENT---CONDITIONS		
		B68	Z08	MAJOR	MINOR				
L242	#	35.1	51.8	-46.2	.9	.60	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L651	#	35.6	70.6	-28.1	5.8	1.01	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L190R	*	39.2	82.6	-15.5	5.2	.98	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L339	#	41.7	64.8	-31.9	-1.7	1.04	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L262G	#	43.0	58.1	-37.9	-4.2	.62	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L320	Ø	43.2	80.8	-16.1	1.5	.41	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L159	Ø	44.1	88.7	-8.3	2.8	1.02	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L636	Ø	44.5	85.1	-11.6	1.5	.87	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L100	Ø	44.6	89.8	-7.1	2.7	.77	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L115	*	45.2				.36	40U	AIR RESISTANCE,	SHEFFIELD IN GURLEY UNITS
L616	Ø	45.3	93.9	-3.0	3.2	.40	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L241	Ø	45.4	81.0	-15.3	-.6	.85	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L737	Ø	45.7	94.5	-2.3	3.0	.86	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L484	Ø	45.8	90.7	-5.9	1.8	.88	40H	AIR RESISTANCE,	REGMED-TYPE GURLEY DENSOMETER - GIL FLOTATION
L163	Ø	45.8	95.2	-1.6	3.1	.63	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L337	Ø	46.0	94.7	-2.0	2.7	1.06	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L291	*	46.4	112.2	15.4	7.6	.95	40U	AIR RESISTANCE,	SHEFFIELD IN GURLEY UNITS
L106	Ø	46.5	93.6	-2.9	2.0	1.20	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L212	Ø	46.7	95.1	-1.4	2.2	1.35	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L107	Ø	46.9	92.5	-3.9	1.3	1.11	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L697	Ø	47.1	93.1	-3.2	1.3	.89	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L219	Ø	47.1	80.5	-15.3	-2.4	.68	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L238A	Ø	47.2	84.2	-11.1	-1.2	1.24	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L259	Ø	47.3	92.9	-3.3	1.0	1.17	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L278	Ø	47.4	79.4	-16.3	-2.9	.92	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L158	Ø	47.5	90.0	-6.1	-.0	.77	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L313	Ø	48.0	98.0	1.7	1.7	1.13	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L153	Ø	48.1	94.1	-2.0	.6	.90	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L174	Ø	48.1	98.5	2.2	1.8	.94	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L261	#	48.4	47.8	-46.2	-12.9	.47	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L124G	Ø	48.5	106.0	9.5	3.6	1.22	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L148	Ø	48.7	102.5	6.3	2.4	.67	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L125	Ø	48.9	97.7	1.7	.8	.97	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L141	Ø	49.2	99.4	3.4	1.0	1.15	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L321	Ø	49.4	106.4	10.2	2.9	.66	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L576	Ø	49.6	88.7	-6.7	-2.4	.83	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L183	Ø	49.7	96.4	.7	-.3	1.64	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L230G	Ø	49.9	104.1	8.1	1.7	.96	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L176	Ø	50.0	93.7	-1.8	-1.3	.78	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L123	Ø	50.2	95.7	.2	-.9	1.03	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L182G	Ø	50.5	92.1	-3.2	-2.3	1.53	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L702	Ø	50.5	96.0	.5	-1.2	1.06	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L121	Ø	50.5	85.0	-10.0	-4.3	1.08	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L285	Ø	50.7	103.4	7.7	.8	.87	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L380	Ø	50.8	92.3	-2.9	-2.5	.87	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L396M	Ø	51.1	98.2	3.4	-.9	.88	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L324	Ø	51.1	95.1	-.2	-2.1	1.13	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L243G	Ø	51.3	88.1	-6.8	-4.2	.85	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L166	Ø	51.4	103.8	8.3	.2	1.08	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L567	Ø	51.4	99.3	3.9	-1.1	1.09	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L122	Ø	51.5	98.3	3.0	-1.4	.75	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L676	Ø	51.6	105.2	9.6	.5	.84	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L585	Ø	51.6	105.4	9.8	.5	1.42	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L388	Ø	51.7	106.6	11.0	.7	1.10	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L223	Ø	51.8	101.7	6.4	-.8	.76	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L254	Ø	52.2	97.8	2.7	-2.3	.58	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L128	Ø	52.3	100.2	5.1	-1.7	1.22	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L190C	Ø	53.2	95.3	.6	-4.0	1.07	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L326	Ø	53.5	102.0	7.1	-2.3	1.04	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L376	Ø	53.6	109.1	14.0	-.3	2.35	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L308	Ø	53.7	95.4	.9	-4.4	.77	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L715	Ø	53.8	102.2	7.5	-2.5	.79	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L348	Ø	54.1	107.6	12.7	-1.3	.97	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L328	Ø	54.4	100.1	5.5	-3.7	1.43	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
L554	*	55.2	117.2	22.2	.4	1.32	40D	AIR RESISTANCE,	GURLEY DENSOMETER - GIL FLOTATION
GMEANS:		46.2	95.2	20.2	5.2	1.00			
		95% ELLIPSE				WITH GAMMA = 73 DEGREES			

# AIR RESISTANCE, GURLEY

SAMPLE B68 = 49. GURLEY UNITS    SAMPLe Z08 = 96. GURLEY UNITS

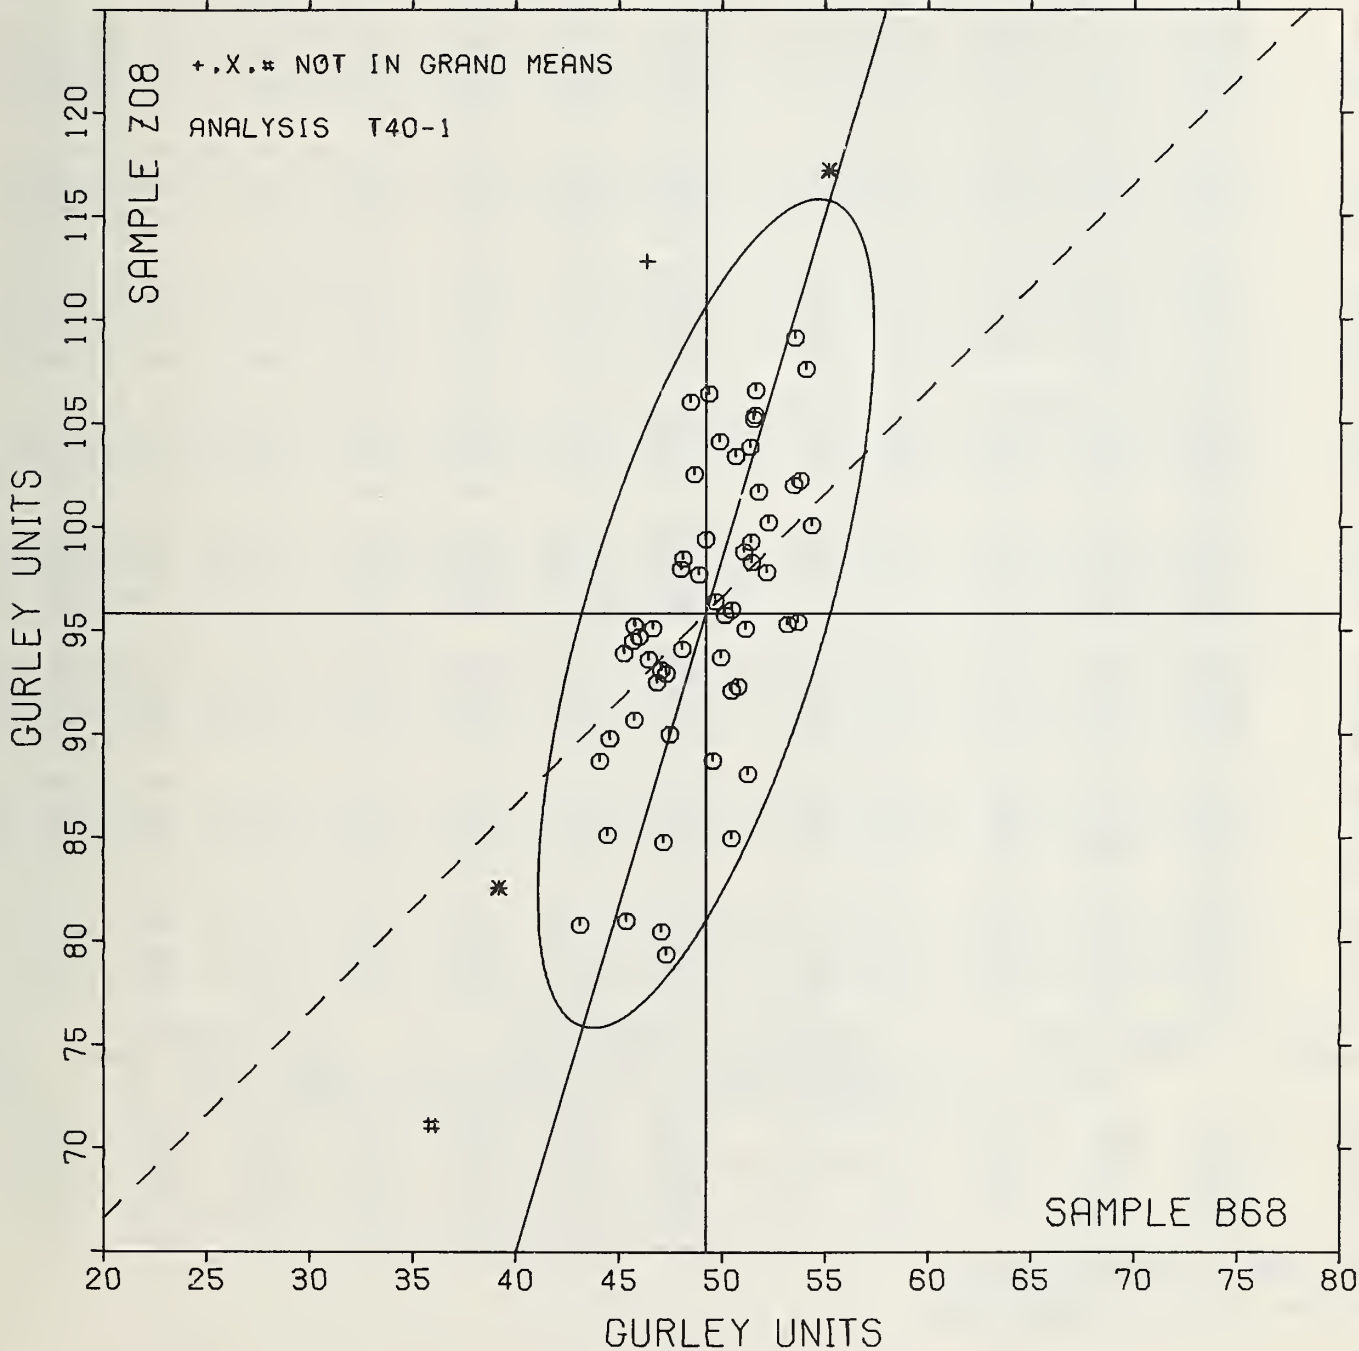



AIR RESISTANCE, SHEFFIELD UNITS (CC/MIN) FOR 0.442 SQ. IN (3/4 IN. DIA) ORIFICE  
TAPPI USEFUL TEST METHOD UM 524, POROSITY BY RESISTANCE TO AIRFLOW

LAB CODE	SAMPLE B68 MEAN	HEAT-SET OFFSET BOOK 93 GRAMS PER SQUARE METER			SAMPLE Z08 MEAN	M.F. SULPHITE 36 GRAMS PER SQUARE METER				TEST D <sub>0</sub> = 10			
		DEV	N <sub>0</sub> DEV	SDR		R <sub>0</sub> SDR	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L114	79.5	8.3	1.68	5.6	.86	35.5	-0.7	-0.23	4.5	1.50	40S	0	L114
L121	80.5	9.3	1.89	6.4	.98	41.5	5.3	1.74	4.7	1.58	40S	0	L121
L122S	71.5	.3	.07	8.1	1.24	37.3	1.1	.36	4.4	1.47	40S	0	L122S
L124S	72.1	.9	.19	7.0	1.07	35.2	-1.0	-0.33	3.0	1.00	40S	0	L124S
L132	66.2	-5.0	-1.01	7.7	1.17	39.1	2.9	.95	4.9	1.62	40S	0	L132
L148	64.3	-6.9	-1.39	8.1	1.24	28.3	-7.9	-2.59	1.6	.55	40S	*	L148
L150	72.3	1.1	.23	9.1	1.39	37.5	1.3	.42	3.5	1.16	40S	0	L150
L157	71.4	.2	.05	7.5	1.15	35.0	-1.2	-.40	2.6	.86	40S	0	L157
L158	77.5	6.3	1.28	5.9	.90	41.2	5.0	1.64	2.2	.73	40S	0	L158
L173B	65.0	-6.2	-1.25	6.2	.95	32.6	-3.6	-1.18	2.0	.67	40S	0	L173B
L190C	79.3	8.1	1.64	5.5	.84	37.7	1.5	.49	4.8	1.59	40S	0	L190C
L213	72.0	.8	.17	5.8	.89	36.3	.1	.03	2.5	.83	40S	0	L213
L223	70.5	-0.7	-.14	4.5	.68	37.0	.8	.26	2.4	.82	40S	0	L223
L228	71.9	.7	.15	2.5	.38	36.8	.6	.19	2.7	.89	40S	0	L228
L230S	75.1	3.9	.79	6.2	.94	34.4	-1.8	-.59	2.5	.82	40S	0	L230S
L233	64.1	-7.1	-1.43	8.5	1.30	36.9	.7	.23	3.3	1.12	40S	0	L233
L241	83.0	11.8	2.39	3.6	.54	48.3	12.1	3.96	3.4	1.13	40S	X	L241
L249	70.2	-1.0	-.20	4.6	.70	34.3	-1.9	-.62	2.4	.80	40S	0	L249
L255	63.7	-7.5	-1.51	7.5	1.15	34.5	-1.7	-.56	2.8	.95	40S	0	L255
L260	71.7	.5	.11	6.1	.94	34.9	-1.3	-.43	2.4	.79	40S	0	L260
L262S	72.1	.9	.19	4.4	.66	36.2	-0.0	-.00	3.1	1.03	40S	0	L262S
L288	77.1	5.9	1.20	5.7	.86	32.3	-3.9	-1.28	3.6	1.20	40S	0	L288
L305	60.7	-10.5	-2.12	7.1	1.08	34.3	-1.9	-.62	3.4	1.12	40S	0	L305
L315	63.5	-7.7	-1.55	5.0	.77	31.2	-5.0	-1.64	2.3	.78	40S	0	L315
L318	72.4	1.2	.25	10.2	1.56	37.8	1.6	.52	4.0	1.34	40S	0	L318
L352	72.2	1.0	.21	6.3	.96	35.4	-0.8	-.26	2.2	.72	40S	0	L352
L354	69.1	-2.1	-.42	7.3	1.12	35.6	-0.6	-.20	2.4	.80	40S	0	L354
L360	73.8	2.6	.53	7.6	1.15	37.6	1.4	.46	2.4	.79	40S	0	L360
L562	84.0	12.8	2.59	10.5	1.61	54.6	18.4	6.03	5.5	1.83	40S	X	L562
L575	67.8	-3.4	-.68	8.2	1.24	35.3	-0.9	-.30	2.9	.98	40S	0	L575
L585	68.5	-2.7	-.54	8.5	1.30	33.4	-2.8	-.92	2.9	.96	40S	0	L585
L600	73.1	1.9	.39	3.1	.47	36.9	.7	.23	3.3	1.09	40S	0	L600
L626	67.8	-3.4	-.68	6.3	.96	33.6	-2.6	-.85	1.6	.55	40S	0	L626
L684	76.2	5.0	1.02	1.8	.27	37.5	1.3	.42	2.3	.77	40S	0	L684
L687	72.7	1.8	.31	8.6	1.31	39.9	3.7	1.21	2.2	.73	40S	0	L687
L698	64.2	-7.0	-1.41	8.9	1.36	38.3	2.1	.69	3.1	1.02	40S	0	L698
L704	75.5	4.3	.87	5.5	.84	36.5	.3	.10	2.5	.84	40S	0	L704
L729	52.9	-18.3	-3.70	5.7	.86	23.9	-12.3	-4.03	3.1	1.05	40S	X	L729
L738	77.0	5.8	1.18	9.8	1.49	45.8	9.6	3.14	5.5	1.82	40S	*	L738
L740	71.0	-0.2	-.04	10.2	1.56	36.0	-0.2	-.07	3.2	1.08	40S	0	L740

GR. MEAN = 71.2 SHEFF. UNITS      GRAND MEAN = 36.2 SHEFF. UNITS      TEST DETERMINATIONS = 10  
SD MEANS = 4.9 SHEFF. UNITS      SD OF MEANS = 3.1 SHEFF. UNITS      37 LABS IN GRAND MEANS  
AVERAGE SDR = 6.6 SHEFF. UNITS      AVERAGE SDR = 3.0 SHEFF. UNITS

L182B	138.0	66.8	13.52	14.2	2.16	251.5	215.3	70.56	33.7	11.22	40E	*	L182E
L243E	204.4	133.2	26.95	17.3	2.64	107.5	71.3	23.36	4.5	1.50	40E	*	L243B
L280	118.0	46.8	9.47	21.0	3.21	66.6	30.4	9.96	4.6	1.55	40E	*	L280
L312	78.4	7.2	1.46	4.8	.73	37.7	1.5	.49	4.2	1.41	40E	*	L312
L333	222.0	150.8	30.51	20.4	3.12	140.0	103.8	34.02	10.5	3.51	40E	*	L333
L484	289.0	217.8	44.06	28.8	4.40	259.0	222.8	73.01	13.7	4.57	40E	*	L484

TOTAL NUMBER OF LABORATORIES REPORTING = 46


Best values: B68 71 ± 8 Sheffield units  
Z08 36 ± 5 Sheffield units

AIR RESISTANCE, SHEFFIELD UNITS (CC/MIN) FOR 0.442 SQ. IN (3/4 IN. DIA) ORIFICE  
TAPPI USEFUL TEST METHOD UM 524, POROSITY BY RESISTANCE TO AIRFLOW

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		B68	Z08	MAJØF	MINØR	R. SDR	VAR			
L729	X	52.9	23.9	-21.6	-4.4	.56	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L305	Ø	60.7	34.3	-10.4	2.2	1.10	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L315	Ø	63.5	31.2	-9.0	-1.7	.77	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L255	Ø	63.7	34.5	-7.6	1.3	1.05	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L233	Ø	64.1	36.9	-6.3	3.3	1.21	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L698	Ø	64.2	38.3	-5.7	4.6	1.19	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L148	*	64.3	28.3	-9.4	-4.7	.89	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L173H	Ø	65.0	32.6	-7.1	-1.0	.81	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L132	Ø	66.2	39.1	-3.5	4.6	1.39	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L626	Ø	67.8	33.6	-4.1	-1.1	.75	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L575	Ø	67.8	35.3	-3.5	.4	1.11	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L585	Ø	68.5	33.4	-3.5	-1.6	1.13	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L354	Ø	69.1	35.6	-2.2	.2	.96	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L249	Ø	70.2	34.3	-1.6	-1.4	.75	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L223	Ø	70.5	37.0	-.3	1.0	.75	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L740	Ø	71.0	36.0	-.2	-.1	1.32	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L157	Ø	71.4	35.0	-.2	-1.2	1.00	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L122S	Ø	71.5	37.3	.7	.9	1.35	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L260	Ø	71.7	34.5	-.0	-1.4	.87	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L228	Ø	71.9	36.8	.9	.3	.63	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L213	Ø	72.0	36.3	.8	-.2	.86	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L262S	Ø	72.1	36.2	.5	-.4	.85	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L124S	Ø	72.1	35.2	.5	-1.3	1.04	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L352	Ø	72.2	35.4	.6	-1.1	.64	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L150	Ø	72.3	37.5	1.5	.8	1.27	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L318	Ø	72.4	37.8	1.7	1.0	1.45	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L687	Ø	72.7	39.5	2.8	2.8	1.02	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L600	Ø	73.1	36.5	2.0	-.1	.78	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L360	Ø	73.8	37.6	3.0	.3	.97	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L230S	Ø	75.1	34.4	2.9	-3.2	.88	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L704	Ø	75.5	36.5	4.1	-1.4	.84	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L684	Ø	76.2	37.5	5.1	-.7	.52	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L738	*	77.0	45.8	9.0	6.7	1.65	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L288	Ø	77.1	32.3	4.0	-5.9	1.03	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L158	Ø	77.5	41.2	7.7	2.2	.82	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L312	*	78.4	37.7	7.3	-1.4	1.07	40T	AIR RESISTANCE,	SHEFFIELD (3	INCH DIAMETER ORIFICE)
L190C	Ø	79.3	37.7	8.1	-1.7	1.21	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L114	Ø	79.5	35.5	7.4	-3.8	1.18	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L121	Ø	80.5	41.5	10.6	1.4	1.28	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L241	X	83.0	48.3	15.5	6.7	.84	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L562	X	84.0	54.6	18.8	12.2	1.72	40S	AIR RESISTANCE,	SHEFFIELD (3/4	INCH DIAMETER ORIFICE)
L280	*	118.0	66.6	54.9	10.3	2.38	40H	AIR RESISTANCE,	HENDTSEN, WG	150
L182H	*	138.0	251.5	143.5	173.8	6.69	40H	AIR RESISTANCE,	HENDTSEN, WG	150
L243H	*	204.4	107.5	150.3	15.4	2.07	40H	AIR RESISTANCE,	HENDTSEN, WG	150
L333	*	222.0	140.0	178.9	38.8	3.32	40H	AIR RESISTANCE,	HENDTSEN, WG	150
L484	*	289.0	259.0	286.1	123.4	4.48	40H	AIR RESISTANCE,	HENDTSEN, WG	150
GMEANS:		71.2	36.2			1.00				
		95% ELLIPSE:	13.6	6.5				WITH GAMMA = 22 DEGREES		

# AIR RESISTANCE, SHEFFIELD

SAMPLE B68 = 71.2 SHEFF. UNITS    SAMPLe Z08 = 36.2 SHEFF. UNITS

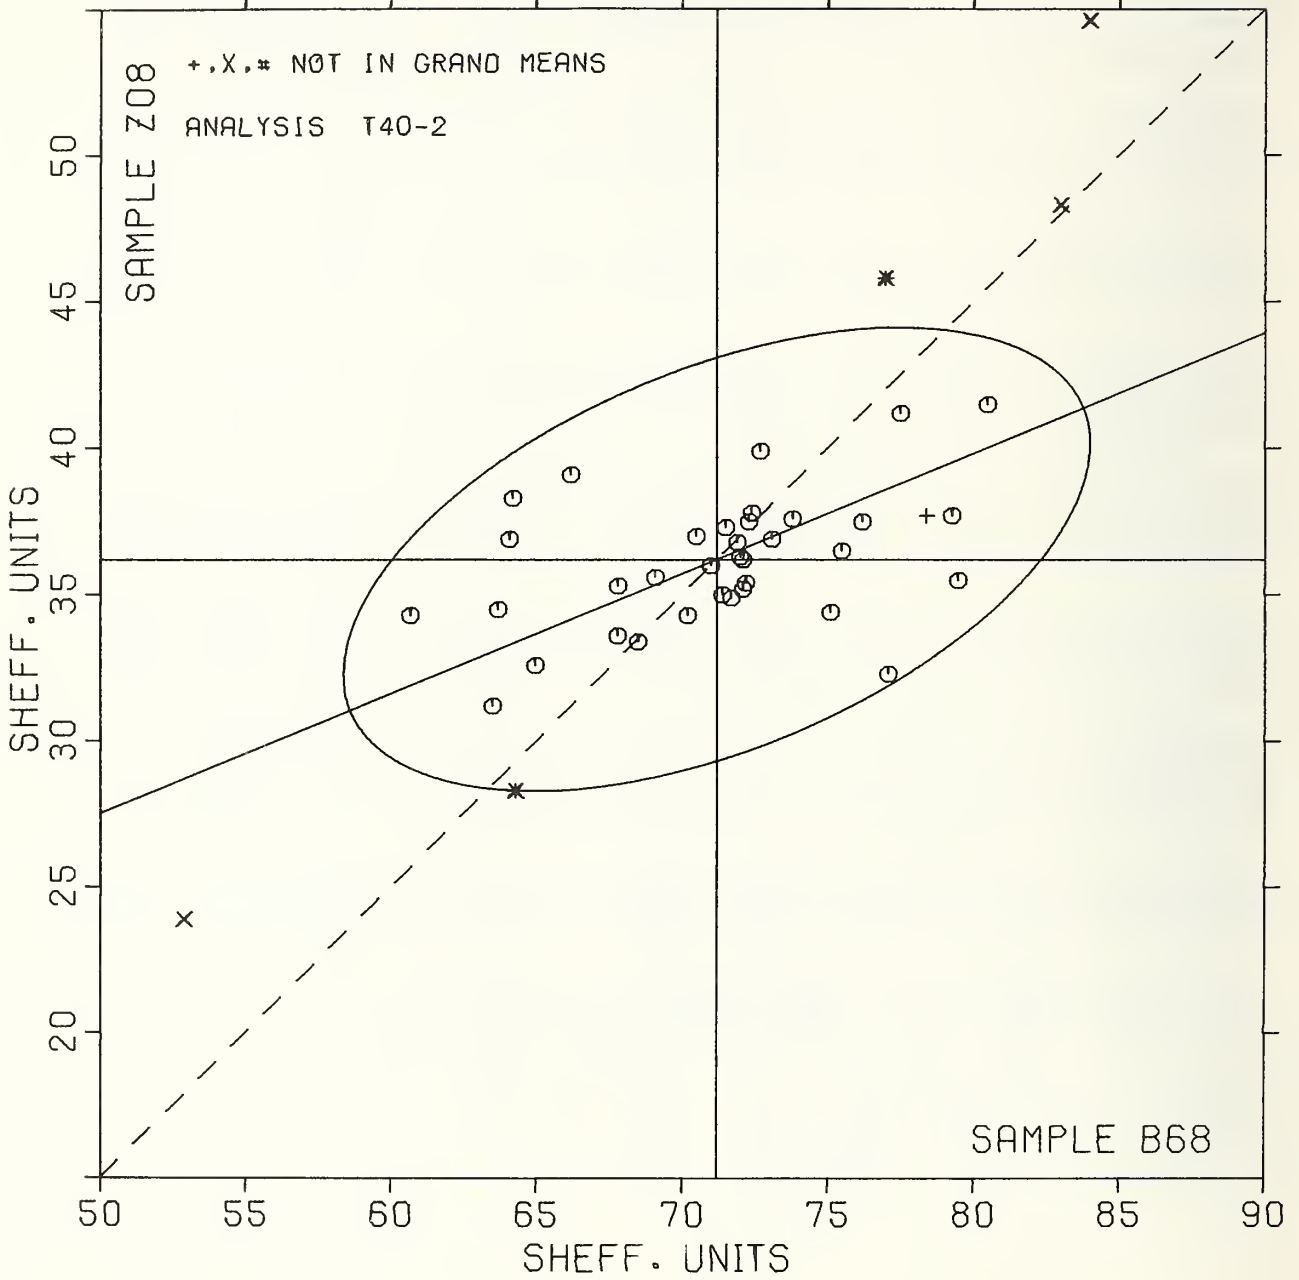






# AIR RESISTANCE, GURLEY HG FLOTATION

SAMPLE E37 = 764. SEC/10 CC

SAMPLE B73 = 1284. SEC/10 CC

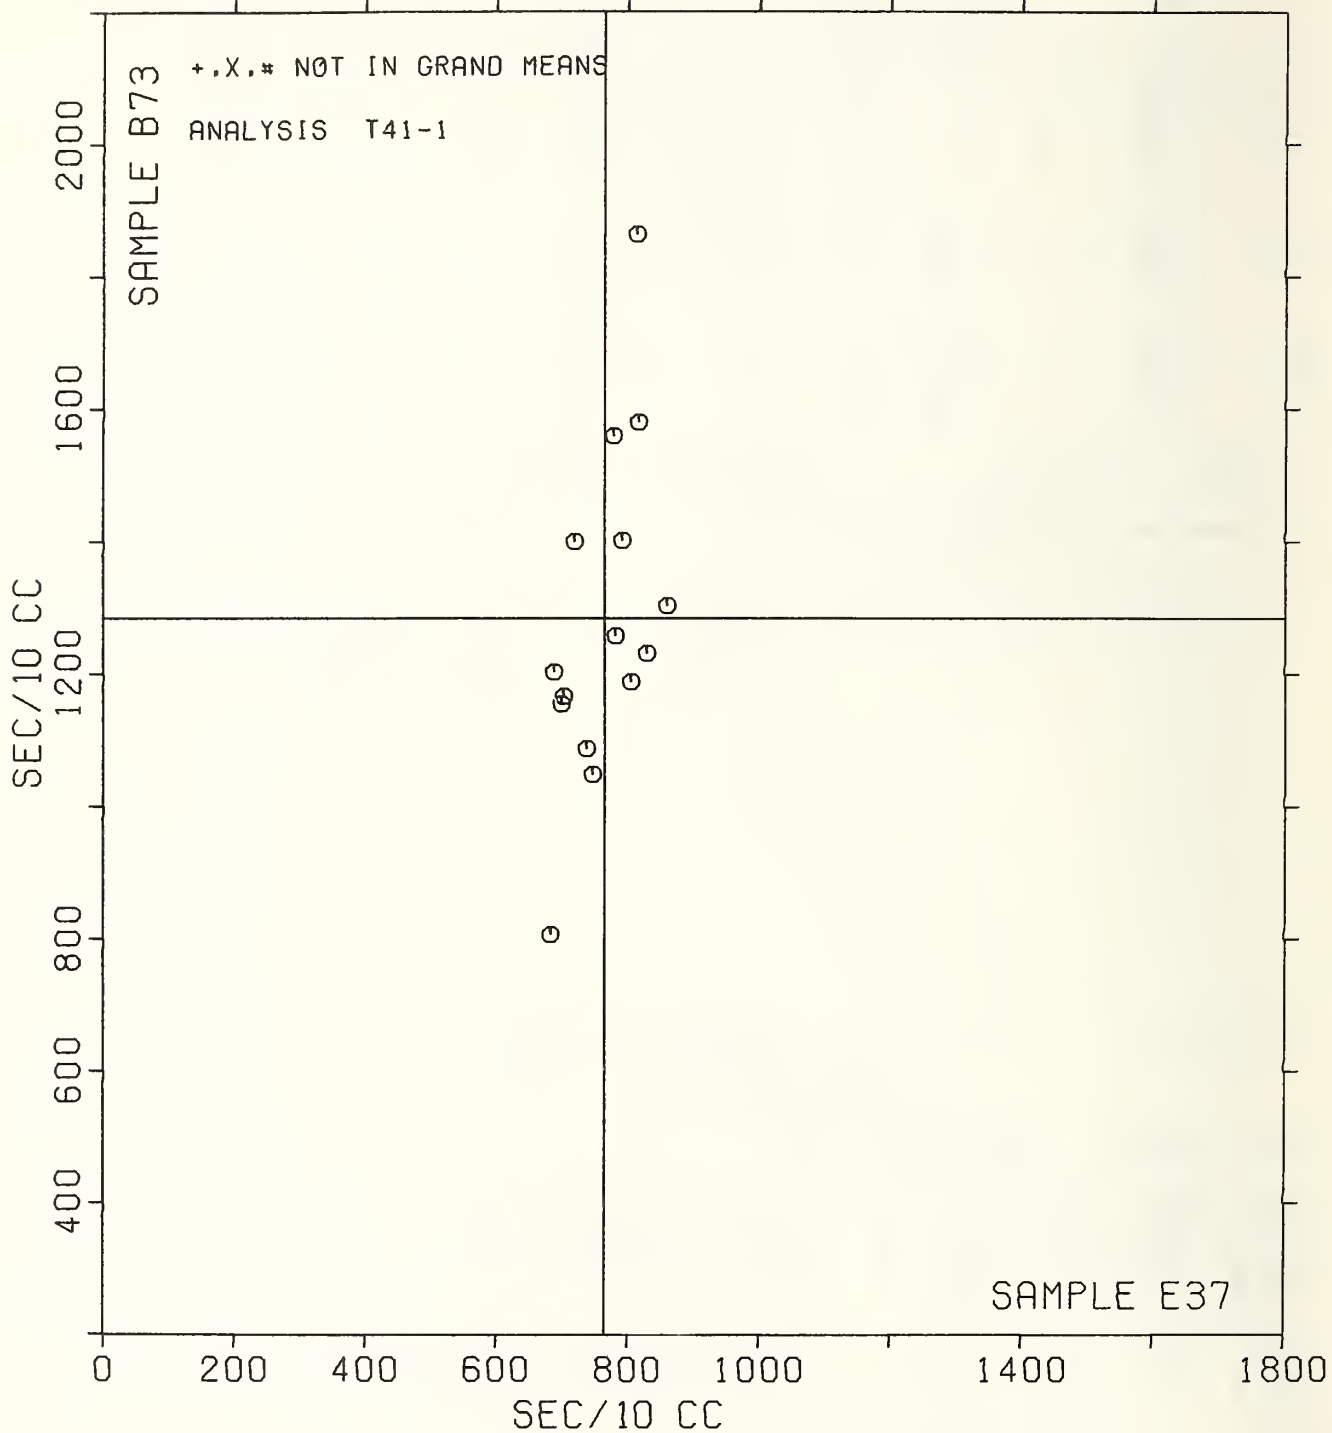



TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T44-1 TABLE 1  
SMOOTHNESS, PARKER PRINTSURF

LAB CODE	VELLUM ENVELOPE					OFFSET PRINTING					TEST D <sub>o</sub> - 10		
	SAMPLE A84 MEAN	91 GRAMS PER SQUARE METER				SAMPLE A83 MEAN	54 GRAMS PER SQUARE METER				VAR	F	LAE
		DEV	N <sub>o</sub> DEV	SDR	R <sub>o</sub> SDR		DEV	N <sub>o</sub> DEV	SDR	R <sub>o</sub> SDR			
L122	6.668	.925	3.97	.107	1.26	5.424	.858	4.38	.340	1.96	44P	#	L122
L182	6.090	.407	1.64	.061	.73	4.850	.284	1.45	.151	.87	44P	Ø	L182
L288	5.700	.017	.07	.047	.56	4.630	.064	.33	.241	1.39	44P	Ø	L288
L317	5.690	.007	.03	.088	1.03	4.290	-.276	-1.41	.120	.69	44P	Ø	L317
L484	5.540	-.143	-.58	.081	.96	4.570	.004	.02	.169	.97	44P	Ø	L484
L588	5.340	-.343	-1.39	.097	1.14	4.410	-.156	-.80	.228	1.32	44P	Ø	L588
L669	5.741	.058	.23	.134	1.59	4.646	.080	.41	.133	.77	44P	Ø	L669

GR<sub>o</sub> MEAN = 5.683 MICRONS  
SD MEANS = .248 MICRONS

GRAND MEAN = 4.566 MICRONS  
SD OF MEANS = .196 MICRONS

TEST DETERMINATIONS = 10  
6 LABS IN GRAND MEANS

AVERAGE SDR = .085 MICRONS  
AVERAGE SDR = .174 MICRONS

TOTAL NUMBER OF LABORATORIES REPORTING = 7

Best values: A84 5.7 microns  
A83 4.6 microns

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T44-1 TABLE 2  
SMOOTHNESS, PARKER PRINTSURF

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY--TEST INSTRUMENT--CONDITIONS
		A84	A83	MAJOR	MINOR	R <sub>o</sub> SDR	VAR	
L588	Ø	5.340	4.410	-.370	.074	1.23	44P	SMOOTHNESS, PARKER PRINTSURF
L484	Ø	5.540	4.570	-.114	.087	.96	44P	SMOOTHNESS, PARKER PRINTSURF
L317	Ø	5.690	4.290	-.156	-.228	.86	44P	SMOOTHNESS, PARKER PRINTSURF
L288	Ø	5.700	4.630	.051	.042	.97	44P	SMOOTHNESS, PARKER PRINTSURF
L669	Ø	5.741	4.646	.093	.031	1.18	44P	SMOOTHNESS, PARKER PRINTSURF
L182	Ø	6.090	4.850	.496	-.007	.80	44P	SMOOTHNESS, PARKER PRINTSURF
L122	#	6.668	5.424	1.300	.122	1.61	44P	SMOOTHNESS, PARKER PRINTSURF

GMEANS: 5.683 4.566  
95% ELLIPSE: 1.224 .485  
WITH GAMMA = 35 DEGREES

SMOOTHNESS, SHEFFIELD UNITS  
TAPPI USEFUL TEST METHOD UM 510, SMOOTHNESS OF PAPER (SHEFFIELD)

LAB CODE	SAMPLE A84 MEAN	VELLUM ENVELOPE				SAMPLE A83 MEAN	OFFSET PRINTING				TEST D <sub>0</sub> - 15		
		91 GRAMS PER SQUARE METER DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR		54 GRAMS PER SQUARE METER DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L100	232.7	4.9	.48	7.3	.89	117.2	9.7	1.02	13.2	1.16	45S	0	L100
L107	223.0	-4.8	-.46	5.6	.68	127.3	19.8	2.09	8.2	.72	45S	#	L107
L108	218.6	-9.2	-.89	4.5	.55	107.5	.0	.01	6.6	.58	45S	0	L108
L114	233.2	5.4	.53	8.7	1.06	123.4	15.9	1.67	15.3	1.35	45S	0	L114
L115	223.3	-4.4	-.43	7.2	.88	102.3	-5.2	-.54	8.2	.72	45S	0	L115
L121	210.0	-17.8	-1.73	7.6	.92	90.3	-17.2	-1.80	7.9	.69	45S	0	L121
L122	234.7	7.0	.68	7.2	.88	110.9	3.4	.36	13.1	1.15	45S	0	L122
L123	231.0	3.2	.31	13.5	1.65	99.4	-8.1	-.85	11.5	1.01	45S	0	L123
L124	212.3	-15.4	-1.50	6.4	.78	92.9	-14.6	-1.53	8.4	.74	45S	0	L124
L125	228.0	.2	.02	9.8	1.19	109.0	1.5	.16	17.6	1.55	45S	0	L125
L126	242.5	14.8	1.44	6.9	.85	116.9	9.4	.99	5.8	.51	45S	0	L126
L128	228.0	.2	.02	10.1	1.24	101.0	-6.5	-.68	7.4	.65	45S	0	L128
L132	236.0	8.2	.80	8.3	1.01	110.5	3.0	.32	11.1	.98	45S	0	L132
L134	232.7	4.9	.48	11.2	1.36	97.7	-9.8	-1.03	9.8	.86	45S	0	L134
L139S	230.3	2.6	.25	5.8	.71	124.2	16.7	1.76	9.9	.87	45S	0	L139S
L148	234.0	6.2	.61	7.7	.94	114.0	6.5	.69	11.3	.99	45S	0	L148
L150	236.8	9.0	.88	8.4	1.02	104.7	-2.8	-.29	7.7	.68	45S	0	L150
L152	230.7	2.9	.28	5.6	.69	114.7	7.2	.76	6.4	.56	45S	0	L152
L153	265.7	37.5	3.69	8.4	1.03	130.5	23.0	2.42	12.4	1.09	45S	X	L153
L157	215.1	-12.7	-1.23	13.2	1.62	102.9	-4.6	-.48	12.4	1.09	45S	0	L157
L158	215.3	-12.4	-1.21	10.6	1.25	91.3	-16.2	-1.70	6.9	.61	45S	0	L158
L159	228.9	1.2	.11	7.9	.97	116.7	9.2	.97	10.1	.89	45S	0	L159
L162	231.3	3.6	.35	8.8	1.07	101.0	-6.5	-.68	13.1	1.15	45S	0	L162
L166	213.1	-14.7	-1.43	6.4	.78	100.1	-7.4	-.78	14.4	1.27	45S	0	L166
L167	234.7	6.5	.67	4.8	.59	117.7	10.2	1.07	10.8	.95	45S	0	L167
L173B	234.7	6.5	.67	6.4	.78	119.0	11.5	1.21	19.6	1.72	45S	0	L173B
L183S	241.7	13.5	1.35	9.6	1.17	115.7	8.2	.86	17.3	1.52	45S	0	L183S
L190C	214.7	-13.1	-1.27	7.9	.97	113.7	6.2	.66	10.0	.88	45S	0	L190C
L190R	205.9	-21.5	-2.13	6.2	.75	91.9	-15.6	-1.64	11.3	.99	45S	0	L190R
L195	222.7	-5.1	-.50	8.0	.98	104.3	-3.2	-.33	9.0	.79	45S	0	L195
L206	217.5	-10.3	-1.00	28.1	3.43	103.5	-4.0	-.42	8.0	.71	45S	0	L206
L211	223.9	-3.5	-.38	11.4	1.35	98.4	-9.1	-.96	6.9	.61	45S	0	L211
L213	203.7	-24.0	-2.34	6.0	.73	92.3	-15.2	-1.60	12.3	1.08	45S	0	L213
L219	233.7	5.5	.57	5.5	.67	114.7	7.2	.76	8.8	.77	45S	0	L219
L223	235.5	8.2	.75	8.6	1.05	101.1	-6.4	-.67	21.2	1.87	45S	0	L223
L224	239.0	11.2	1.05	7.1	.87	113.5	6.0	.64	9.7	.85	45S	0	L224
L226B	220.7	-7.1	-.69	10.2	1.24	111.9	4.4	.47	10.6	.93	45S	0	L226B
L228	239.9	12.1	1.18	9.0	1.10	106.9	-6	-.06	15.2	1.34	45S	0	L228
L230S	227.0	-.8	-.07	7.5	.92	115.7	8.2	.86	9.6	.84	45S	0	L230S
L231	240.5	12.8	1.24	8.8	1.07	108.7	1.2	.12	18.2	1.60	45S	0	L231
L233	231.0	3.2	.31	7.1	.87	111.4	3.9	.41	11.2	.99	45S	0	L233
L237	235.7	7.9	.77	3.2	.39	104.7	-2.8	-.30	9.0	.79	45S	0	L237
L241	204.9	-22.8	-2.22	9.4	1.15	98.0	-9.5	-1.00	5.4	.47	45S	0	L241
L249	225.7	-2.1	-.20	8.0	.98	100.7	-6.8	-.71	13.5	1.18	45S	0	L249
L254	238.3	10.5	1.02	7.1	.87	99.2	-8.3	-.87	6.4	.56	45S	0	L254
L255	218.7	-9.0	-.88	6.5	.75	106.8	-7.7	-.07	9.2	.81	45S	0	L255
L259	256.0	28.2	2.75	5.1	.62	119.3	11.8	1.25	13.1	1.15	45S	#	L259
L260	218.7	-9.0	-.88	6.7	.82	117.1	9.6	1.01	12.9	1.13	45S	0	L260
L261	227.8	.0	.00	7.6	.93	113.6	6.1	.64	13.0	1.14	45S	0	L261
L262	226.7	-1.1	-.11	6.2	.75	103.3	-4.2	-.44	6.7	.59	45S	0	L262
L275	232.0	4.2	.41	7.7	.95	102.7	-4.8	-.51	14.5	1.27	45S	0	L275
L277	249.3	21.6	2.10	7.4	.91	97.9	-9.6	-1.00	5.8	.51	45S	#	L277
L278	243.7	15.5	1.55	7.2	.88	128.3	20.8	2.19	10.3	.90	45S	0	L278
L281	228.5	.7	.07	6.7	.82	103.5	-4.0	-.42	16.9	1.48	45S	0	L281
L285	224.5	-3.3	-.32	8.1	1.00	118.5	11.0	1.15	13.5	1.18	45S	0	L285
L288	227.2	-.6	-.05	8.1	.98	120.7	13.2	1.35	16.7	1.47	45S	0	L288
L290	203.3	-24.4	-2.38	6.8	.83	102.9	-4.6	-.48	15.3	1.34	45S	0	L290
L291S	237.2	9.4	.92	5.1	.63	112.2	4.7	.50	13.7	1.20	45S	0	L291S
L305	221.1	-6.7	-.65	6.3	.77	95.5	-12.0	-1.26	9.0	.79	45S	0	L305
L308	224.4	-3.4	-.33	6.7	.82	97.7	-9.8	-1.03	16.8	1.48	45S	0	L308
L312	266.3	38.5	3.74	5.8	.70	176.3	68.8	7.24	12.7	1.12	45S	#	L312
L317	225.3	-2.4	-.24	8.3	1.02	103.7	-3.8	-.40	12.9	1.13	45S	0	L317
L318	232.4	4.6	.45	7.1	.87	120.3	12.8	1.35	15.5	1.36	45S	0	L318
L321	217.3	-10.4	-1.01	8.0	.98	89.0	-18.5	-1.94	6.3	.56	45S	0	L321
L323	240.7	12.9	1.25	8.2	1.00	123.0	15.5	1.63	11.6	1.02	45S	0	L323

TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS 145-1 TABLE 1  
 SMOOTHNESS, SHEFFIELD UNITS  
 TAPPI USEFUL TEST METHOD UM 518, SMOOTHNESS OF PAPER (SHEFFIELD)

LAB CODE	VELLUM ENVELOPE 91 GRAMS PER SQUARE METER					GFFSET PRINTING 54 GRAMS PER SQUARE METER					TEST D <sub>0</sub> = 15		
	SAMPLE A84 MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	SAMPLE A83 MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L326	215.8	-12.0	-1.16	6.7	.82	107.0	-.5	-.05	9.3	.82	455	0	L326
L328	234.9	7.2	.70	10.8	1.32	55.6	-11.9	-1.25	7.3	.64	455	0	L328
L348	230.1	2.3	.22	10.0	1.22	102.4	-5.1	-.53	7.6	.67	455	0	L348
L349	219.6	-8.2	-.79	10.1	1.23	111.1	3.6	.38	13.1	1.15	455	0	L349
L352	233.7	5.9	.57	6.1	.75	108.3	.8	.09	10.5	.92	455	0	L352
L360	227.0	-.8	-.07	6.2	.76	107.8	.3	.03	13.1	1.15	455	0	L360
L366	235.5	7.8	.76	8.5	1.04	103.7	-3.8	-.40	12.1	1.06	455	0	L366
L376	231.3	3.6	.35	8.3	1.02	113.3	5.8	.62	9.9	.87	455	0	L376
L380	218.0	-9.8	-.95	5.3	.64	101.3	-6.2	-.65	3.5	.31	455	0	L380
L382	239.0	11.2	1.09	7.2	.88	112.7	5.2	.55	14.4	1.27	455	0	L382
L554	219.3	-8.5	-.83	8.4	1.02	87.7	-19.8	-2.08	10.9	.96	455	0	L554
L562	234.9	7.2	.70	6.1	.75	101.1	-6.4	-.67	15.0	1.32	455	0	L562
L567	215.6	-12.2	-1.18	9.0	1.10	124.5	17.0	1.75	27.3	2.40	455	*	L567
L571	230.0	2.2	.22	10.0	1.22	116.0	8.5	.90	18.4	1.62	455	0	L571
L575	241.1	13.3	1.29	6.7	.82	120.6	13.1	1.38	17.0	1.49	455	0	L575
L585	230.3	2.6	.25	9.9	1.21	99.7	-7.8	-.82	9.0	.79	455	0	L585
L600	234.3	6.6	.64	8.6	1.05	111.5	4.0	.42	7.5	.66	455	0	L600
L604	222.7	-5.1	-.50	7.0	.86	89.3	-18.2	-1.91	8.2	.72	455	0	L604
L626	232.0	4.2	.41	5.9	.72	103.2	-4.3	-.45	10.7	.94	455	0	L626
L636	224.9	-2.8	-.28	6.8	.84	114.5	7.0	.73	11.2	.98	455	0	L636
L651	228.8	1.0	.10	12.1	1.48	107.5	.0	.01	15.3	1.34	455	0	L651
L670	243.7	15.9	1.55	9.2	1.12	112.9	5.4	.57	11.2	.98	455	0	L670
L698	230.5	2.8	.27	9.7	1.18	103.8	-3.7	-.35	14.1	1.24	455	0	L698
L702	208.7	-19.1	-1.86	9.3	1.14	100.7	-6.8	-.72	13.3	1.17	455	0	L702
L704	224.3	-3.4	-.33	8.6	1.05	111.3	3.8	.40	14.9	1.31	455	0	L704
L729	228.0	.2	.02	5.9	.72	115.7	8.2	.86	9.3	.82	455	0	L729
L738	216.7	-11.1	-1.08	16.3	1.99	95.3	-12.2	-1.28	5.2	.45	455	0	L738

GR. MEAN = 227.8 SHEFF. UNITS      GRAND MEAN = 107.5 SHEFF. UNITS      TEST DETERMINATIONS = 15  
 SD MEANS = 10.3 SHEFF. UNITS      SD OF MEANS = 9.5 SHEFF. UNITS      90 LABS IN GRAND MEANS  
 AVERAGE SDR = 8.2 SHEFF. UNITS      AVERAGE SDR = 11.4 SHEFF. UNITS  
 TOTAL NUMBER OF LABORATORIES REPORTING = 92

Best values: A84 230 ± 16 Sheffield units  
 A83 107 ± 15 Sheffield units

The following laboratories were omitted from the grand means because of extreme test results: 312



## TAPPI USEFUL TEST METHOD UM 518, SMOOTHNESS OF PAPER (SHEFFIELD)

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---	CONDITIONS
		A84	A83	MAJOR	MINOR	R <sub>0</sub> SDR	VAR		
L290	Ø	203.3	102.9	-21.7	12.2	1.08	45S	SMOOTHNESS, SHEFFIELD	
L213	Ø	203.7	92.3	-28.2	3.8	.91	45S	SMOOTHNESS, SHEFFIELD	
L241	Ø	204.9	98.0	-23.6	7.4	.81	45S	SMOOTHNESS, SHEFFIELD	
L190R	Ø	205.9	91.9	-26.8	2.1	.87	45S	SMOOTHNESS, SHEFFIELD	
L702	Ø	208.7	100.7	-19.0	7.0	1.16	45S	SMOOTHNESS, SHEFFIELD	
L121	Ø	210.0	90.3	-24.6	-1.7	.81	45S	SMOOTHNESS, SHEFFIELD	
L124	Ø	212.3	92.9	-21.2	-1.3	.76	45S	SMOOTHNESS, SHEFFIELD	
L166	Ø	213.1	100.1	-16.0	3.7	1.02	45S	SMOOTHNESS, SHEFFIELD	
L190C	Ø	214.7	113.7	-6.0	13.2	.92	45S	SMOOTHNESS, SHEFFIELD	
L157	Ø	215.1	102.9	-12.7	4.7	1.36	45S	SMOOTHNESS, SHEFFIELD	
L158	Ø	215.3	91.3	-19.9	-4.4	.95	45S	SMOOTHNESS, SHEFFIELD	
L567	*	215.6	124.5	1.6	20.8	1.75	45S	SMOOTHNESS, SHEFFIELD	
L326	Ø	215.8	107.0	-9.5	7.3	.82	45S	SMOOTHNESS, SHEFFIELD	
L738	Ø	216.7	95.3	-16.3	-2.2	1.22	45S	SMOOTHNESS, SHEFFIELD	
L321	Ø	217.3	89.0	-19.9	-7.5	.77	45S	SMOOTHNESS, SHEFFIELD	
L206	Ø	217.5	103.5	-10.4	3.6	2.07	45S	SMOOTHNESS, SHEFFIELD	
L380	Ø	218.0	101.3	-11.4	1.6	.48	45S	SMOOTHNESS, SHEFFIELD	
L108	Ø	218.6	107.5	-7.0	5.9	.56	45S	SMOOTHNESS, SHEFFIELD	
L260	Ø	218.7	117.1	-0.7	13.2	.97	45S	SMOOTHNESS, SHEFFIELD	
L255	Ø	218.7	106.8	-7.4	5.3	.80	45S	SMOOTHNESS, SHEFFIELD	
L554	Ø	219.3	87.7	-19.2	-6.7	.59	45S	SMOOTHNESS, SHEFFIELD	
L349	Ø	219.6	111.1	-3.9	8.0	1.19	45S	SMOOTHNESS, SHEFFIELD	
L226B	Ø	220.7	111.9	-2.6	8.0	1.08	45S	SMOOTHNESS, SHEFFIELD	
L305	Ø	221.1	95.5	-12.8	-4.9	.78	45S	SMOOTHNESS, SHEFFIELD	
L604	Ø	222.7	89.3	-15.6	-10.6	.79	45S	SMOOTHNESS, SHEFFIELD	
L195	Ø	222.7	104.3	-5.9	.9	.88	45S	SMOOTHNESS, SHEFFIELD	
L107	*	223.0	127.3	9.1	18.3	.70	45S	SMOOTHNESS, SHEFFIELD	
L115	Ø	223.3	102.3	-6.7	-1.1	.80	45S	SMOOTHNESS, SHEFFIELD	
L211	Ø	223.9	98.4	-8.8	-4.5	1.00	45S	SMOOTHNESS, SHEFFIELD	
L704	Ø	224.3	111.3	-0.2	5.2	1.18	45S	SMOOTHNESS, SHEFFIELD	
L308	Ø	224.4	97.7	-8.8	-5.3	1.15	45S	SMOOTHNESS, SHEFFIELD	
L285	Ø	224.5	118.5	4.5	10.5	1.09	45S	SMOOTHNESS, SHEFFIELD	
L636	Ø	224.9	114.5	2.3	7.2	.91	45S	SMOOTHNESS, SHEFFIELD	
L317	Ø	225.3	103.7	-4.3	-1.4	1.08	45S	SMOOTHNESS, SHEFFIELD	
L249	Ø	225.7	100.7	-5.9	-3.8	1.08	45S	SMOOTHNESS, SHEFFIELD	
L262	Ø	226.7	103.3	-3.5	-2.5	.67	45S	SMOOTHNESS, SHEFFIELD	
L360	Ø	227.0	107.8	-0.4	.7	.95	45S	SMOOTHNESS, SHEFFIELD	
L230S	Ø	227.0	115.7	4.7	6.8	.88	45S	SMOOTHNESS, SHEFFIELD	
L288	Ø	227.2	120.7	8.0	10.5	1.23	45S	SMOOTHNESS, SHEFFIELD	
L261	Ø	227.8	113.6	4.0	4.7	1.03	45S	SMOOTHNESS, SHEFFIELD	
L729	Ø	228.0	115.7	5.4	6.1	.77	45S	SMOOTHNESS, SHEFFIELD	
L128	Ø	228.0	101.0	-4.0	-5.1	.94	45S	SMOOTHNESS, SHEFFIELD	
L125	Ø	228.0	109.0	1.2	1.0	1.37	45S	SMOOTHNESS, SHEFFIELD	
L281	Ø	228.5	103.5	-2.0	-3.5	1.15	45S	SMOOTHNESS, SHEFFIELD	
L651	Ø	228.8	107.5	.8	-0.6	1.41	45S	SMOOTHNESS, SHEFFIELD	
L159	Ø	228.9	116.7	6.8	6.3	.93	45S	SMOOTHNESS, SHEFFIELD	
L571	Ø	230.0	116.0	7.2	5.1	1.42	45S	SMOOTHNESS, SHEFFIELD	
L348	Ø	230.1	102.4	-1.5	-5.4	.95	45S	SMOOTHNESS, SHEFFIELD	
L585	Ø	230.3	99.7	-3.0	-7.6	1.00	45S	SMOOTHNESS, SHEFFIELD	
L139S	Ø	230.3	124.2	12.7	11.2	.79	45S	SMOOTHNESS, SHEFFIELD	
L698	Ø	230.5	103.8	-0.2	-4.6	1.21	45S	SMOOTHNESS, SHEFFIELD	
L152	Ø	230.7	114.7	6.9	3.7	.62	45S	SMOOTHNESS, SHEFFIELD	
L233	Ø	231.0	111.4	5.0	.9	.93	45S	SMOOTHNESS, SHEFFIELD	
L123	Ø	231.0	99.4	-2.7	-8.3	1.33	45S	SMOOTHNESS, SHEFFIELD	
L376	Ø	231.3	113.3	6.5	2.2	.94	45S	SMOOTHNESS, SHEFFIELD	
L162	Ø	231.3	101.0	-1.4	-7.3	1.11	45S	SMOOTHNESS, SHEFFIELD	
L275	Ø	232.0	102.7	.2	-6.4	1.11	45S	SMOOTHNESS, SHEFFIELD	
L626	Ø	232.0	103.2	.5	-6.0	.83	45S	SMOOTHNESS, SHEFFIELD	
L318	Ø	232.4	120.3	11.8	6.9	1.11	45S	SMOOTHNESS, SHEFFIELD	
L134	Ø	232.7	97.7	-2.5	-10.7	1.11	45S	SMOOTHNESS, SHEFFIELD	
L100	Ø	232.7	117.2	10.0	4.3	1.03	45S	SMOOTHNESS, SHEFFIELD	
L114	Ø	233.2	123.4	14.4	8.7	1.20	45S	SMOOTHNESS, SHEFFIELD	
L219	Ø	233.7	114.7	9.1	1.7	.72	45S	SMOOTHNESS, SHEFFIELD	
L352	Ø	233.7	108.3	5.1	-3.1	.83	45S	SMOOTHNESS, SHEFFIELD	
L148	Ø	234.0	114.0	9.0	1.0	.97	45S	SMOOTHNESS, SHEFFIELD	


TAPPI COLLABORATIVE REFERENCE PROGRAM  
 ANALYSIS 145-1 TABLE 2  
 SMCOTNESS, SHEFFIELD UNITS  
 TAPPI USEFUL TEST METHODS UM 512, SMCOTNESS OF PAPER (SHEFFIELD)

TAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		A64	A03	MAJOR	MINOR	R.	SDR VAR			
L600	Ø	234.3	111.5	7.6	-1.2	.86	458	SMCOTNESS,	SHEFFIELD	
L173B	Ø	234.7	119.0	12.7	4.4	1.25	458	SMCOTNESS,	SHEFFIELD	
L167	Ø	234.7	117.7	11.8	3.4	.77	458	SMCOTNESS,	SHEFFIELD	
L122	Ø	234.7	110.9	7.5	-1.9	1.02	458	SMCOTNESS,	SHEFFIELD	
L328	Ø	234.9	95.6	-2.1	-13.7	.96	458	SMCOTNESS,	SHEFFIELD	
L562	Ø	234.9	101.1	1.4	-9.5	1.03	458	SMCOTNESS,	SHEFFIELD	
L366	Ø	235.5	103.7	3.5	-7.9	1.05	458	SMCOTNESS,	SHEFFIELD	
L237	Ø	235.7	104.7	4.3	-7.2	.59	458	SMCOTNESS,	SHEFFIELD	
L223	Ø	235.9	101.1	2.1	-10.2	1.46	458	SMCOTNESS,	SHEFFIELD	
L132	Ø	236.0	110.5	8.3	-2.9	.99	458	SMCOTNESS,	SHEFFIELD	
L150	Ø	236.8	104.7	5.2	-7.5	.85	458	SMCOTNESS,	SHEFFIELD	
L2918	Ø	237.2	112.2	10.3	-2.4	.92	458	SMCOTNESS,	SHEFFIELD	
L254	Ø	238.3	99.2	2.7	-13.1	.71	458	SMCOTNESS,	SHEFFIELD	
L224	Ø	239.0	113.5	12.5	-2.6	.66	458	SMCOTNESS,	SHEFFIELD	
L382	Ø	239.0	112.7	11.9	-3.2	1.07	458	SMCOTNESS,	SHEFFIELD	
L228	Ø	239.9	106.9	8.9	-8.2	1.22	458	SMCOTNESS,	SHEFFIELD	
L231	Ø	240.5	108.7	10.6	-7.3	1.34	458	SMCOTNESS,	SHEFFIELD	
L323	Ø	240.7	123.0	19.9	3.6	1.01	458	SMCOTNESS,	SHEFFIELD	
L575	Ø	241.1	120.6	18.6	1.5	1.16	458	SMCOTNESS,	SHEFFIELD	
L1838	Ø	241.7	115.7	15.9	-2.7	1.34	458	SMCOTNESS,	SHEFFIELD	
L126	Ø	242.5	116.5	17.3	-2.3	.68	458	SMCOTNESS,	SHEFFIELD	
L278	Ø	243.7	120.3	25.6	5.8	.89	458	SMCOTNESS,	SHEFFIELD	
L670	Ø	243.7	112.9	15.7	-6.1	1.05	458	SMCOTNESS,	SHEFFIELD	
L277	*	245.3	97.9	10.4	-21.2	.71	458	SMCOTNESS,	SHEFFIELD	
L259	*	256.0	119.3	29.3	-9.0	.88	458	SMCOTNESS,	SHEFFIELD	
L153	X	265.7	130.5	43.8	-6.7	1.06	458	SMCOTNESS,	SHEFFIELD	
L312	#	266.3	176.3	73.7	28.1	.91	458	SMCOTNESS,	SHEFFIELD	
GMEANS:		227.8	107.5			1.00				
		95% ELLIPSE:		29.8	18.5			WITH GAMMA = 39 DEGREE		



# SMOOTHNESS, SHEFFIELD

SAMPLE A84 = 228. SHEFF. UNITS    SAMPLE A83 = 107. SHEFF. UNITS

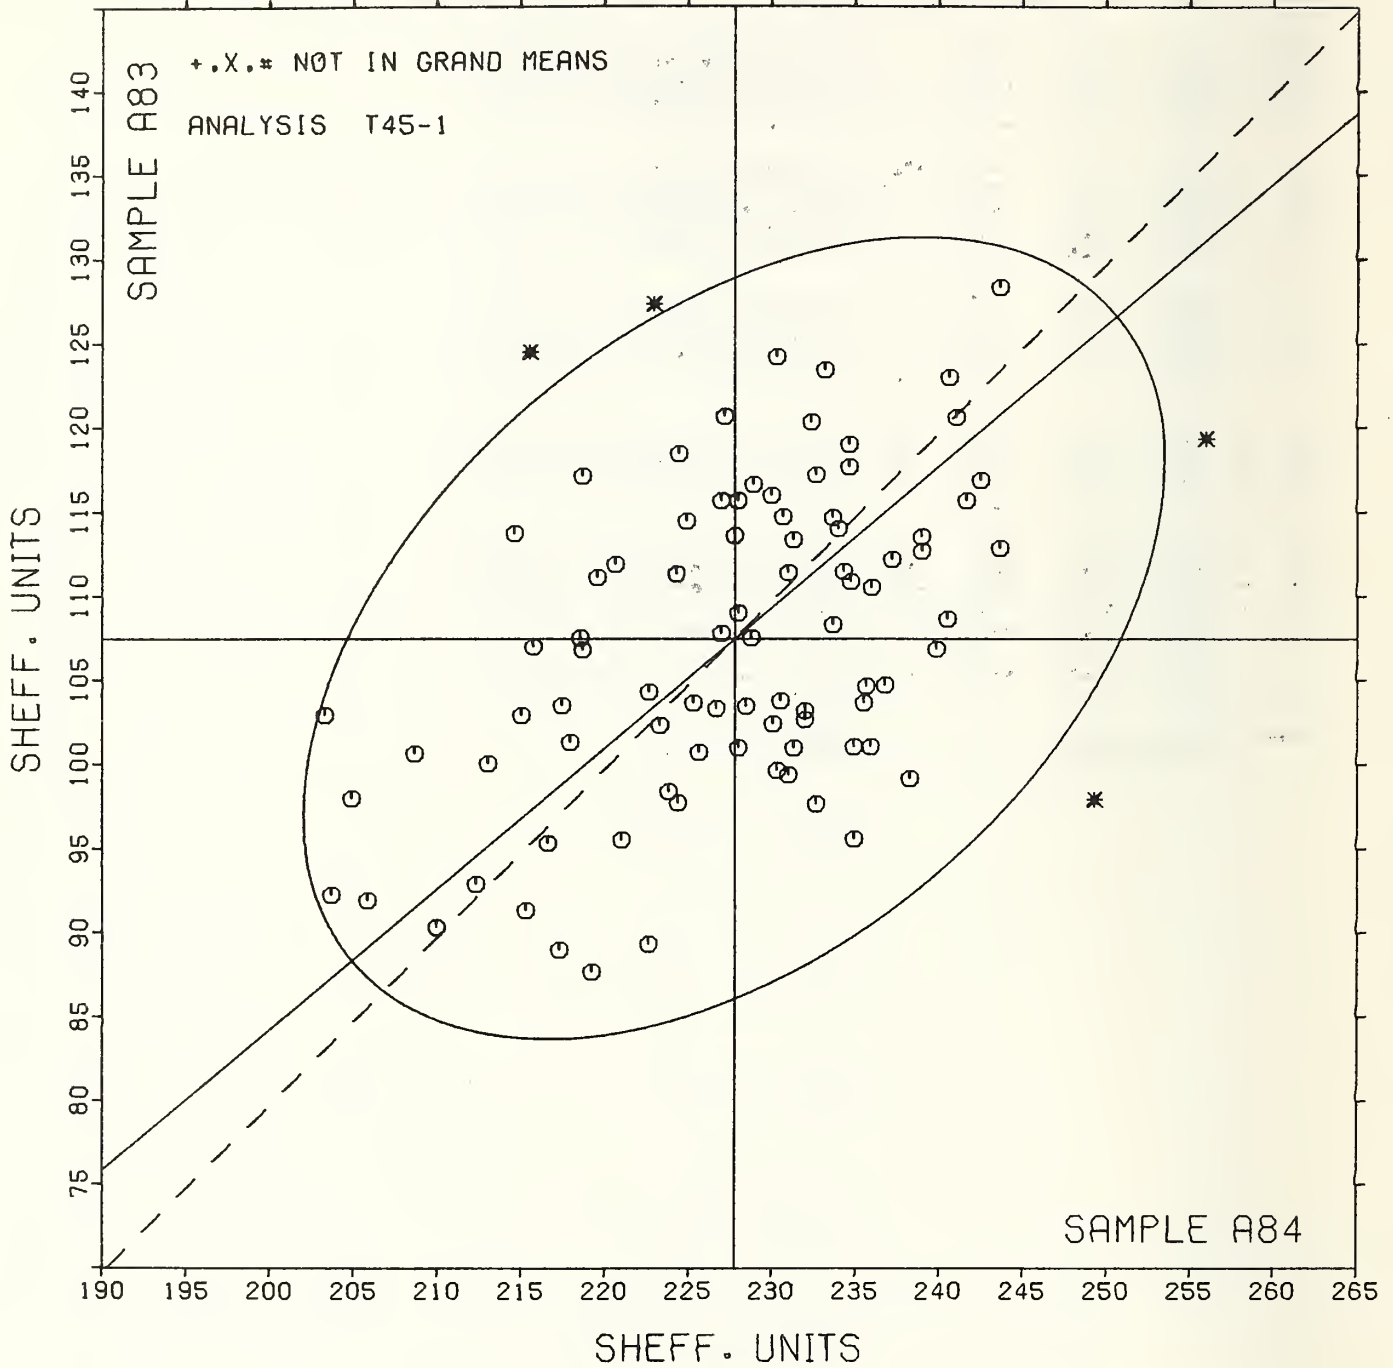

ANALYSIS T45-2 TABLE 1  
SMOOTHNESS, BEKK SECONDS  
TAPPI SUGGESTED METHOD T479 SU-71, SMOOTHNESS OF PAPER (BEKK METHOD)

LAB CODE	SAMPLE A84 MEAN	VELLUM ENVELOPE 91 GRAMS PER SQUARE METER				SAMPLE A83 MEAN	OFFSET PRINTING 94 GRAMS PER SQUARE METER				TEST D <sub>0</sub> = 15		
		DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR		DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L139H	14.52	1.47	1.60	1.02	1.22	53.87	-1.07	-0.15	7.75	0.84	45K	Ø	L139H
L162	13.09	0.04	0.05	0.88	1.05	42.87	-12.07	-1.64	4.82	0.52	45K	Ø	L162
L182K	12.35	-0.70	-0.76	0.50	0.59	50.80	-4.13	-0.56	8.06	0.87	45K	Ø	L182K
L190C	13.76	0.71	0.77	1.44	1.72	70.20	15.27	2.07	13.14	1.42	45K	Ø	L190C
L230H	11.47	-1.55	-1.73	0.52	0.62	51.73	-3.20	-0.43	11.07	1.20	45K	Ø	L230H
L243K	12.98	-0.07	-0.08	0.54	0.64	59.00	4.07	0.55	6.43	0.69	45K	Ø	L243K
L291K	12.59	-0.46	-0.50	0.69	0.83	56.20	1.27	0.17	10.81	1.17	45K	Ø	L291K
L564	12.80	-0.25	-0.28	0.68	0.81	50.39	-4.55	-0.62	9.67	1.05	45K	Ø	L564
L581	14.27	1.21	1.33	1.49	1.78	61.13	6.20	0.84	8.85	0.96	45K	Ø	L581
L697	12.69	-0.37	-0.40	0.63	0.76	53.15	-1.78	-0.24	11.86	1.28	45K	Ø	L697

GR. MEAN = 13.05 BEKK SECONDS      GRAND MEAN = 54.93 BEKK SECONDS      TEST DETERMINATIONS = 15  
SD MEANS = 0.92 BEKK SECONDS      SD OF MEANS = 7.36 BEKK SECONDS      10 LABS IN GRAND MEANS  
AVERAGE SDR = 0.84 BEKK SECONDS      AVERAGE SDR = 9.25 BEKK SECONDS

L250M	12.80	-0.25	-0.28	0.86	1.03	42.80	-12.13	-1.65	11.79	1.28	45L	+	L250M
L251	13.28	0.23	0.25	0.65	0.78	48.07	-6.87	-0.93	13.70	1.48	45L	+	L251

TOTAL NUMBER OF LABORATORIES REPORTING = 12

Best values: A84 13 Bekk seconds  
A83 55 Bekk seconds


ANALYSIS T45-2 TABLE 2  
SMOOTHNESS, BEKK SECONDS  
TAPPI SUGGESTED METHOD T479 SU-71, SMOOTHNESS OF PAPER (BEKK METHOD)

LAB CODE	F	MEANS		COORDINATES		AVG R <sub>0</sub> SDR	VAR	PROPERTY	TEST INSTRUMENT	CONDITIONS
		A84	A83	MAJOR	MINOR					
L230B	Ø	11.47	51.73	-3.28	1.42	0.91	45K	SMOOTHNESS, BEKK		
L182K	Ø	12.35	50.80	-4.16	0.48	0.73	45K	SMOOTHNESS, BEKK		
L291K	Ø	12.59	56.20	1.24	0.52	1.00	45K	SMOOTHNESS, BEKK		
L697	Ø	12.69	53.15	-1.80	0.27	1.02	45K	SMOOTHNESS, BEKK		
L250M	+	12.80	42.80	-12.13	-0.38	1.15	45L	SMOOTHNESS, BEKK, 20 C, 65% RH		
L564	Ø	12.80	50.39	-4.55	0.01	0.93	45K	SMOOTHNESS, BEKK		
L243K	Ø	12.98	59.00	4.06	0.28	0.67	45K	SMOOTHNESS, BEKK		
L162	Ø	13.09	42.87	-12.05	-0.67	0.78	45K	SMOOTHNESS, BEKK		
L251	+	13.28	48.07	-6.85	-0.59	1.13	45L	SMOOTHNESS, BEKK, 20 C, 65% RH		
L190C	Ø	13.76	70.20	15.28	0.05	1.57	45K	SMOOTHNESS, BEKK		
L581	Ø	14.27	61.13	6.25	-0.85	1.37	45K	SMOOTHNESS, BEKK		
L139H	Ø	14.52	53.87	-0.99	-1.52	1.03	45K	SMOOTHNESS, BEKK		

GMEANS: 13.05 54.93 1.00  
95% ELLIPSE: 23.35 2.64 WITH GAMMA = 87 DEGREES

# SMOOTHNESS, BEKK

SAMPLE A84 = 13.1 BEKK SECONDS    SAMPLE A83 = 54.9 BEKK SECONDS

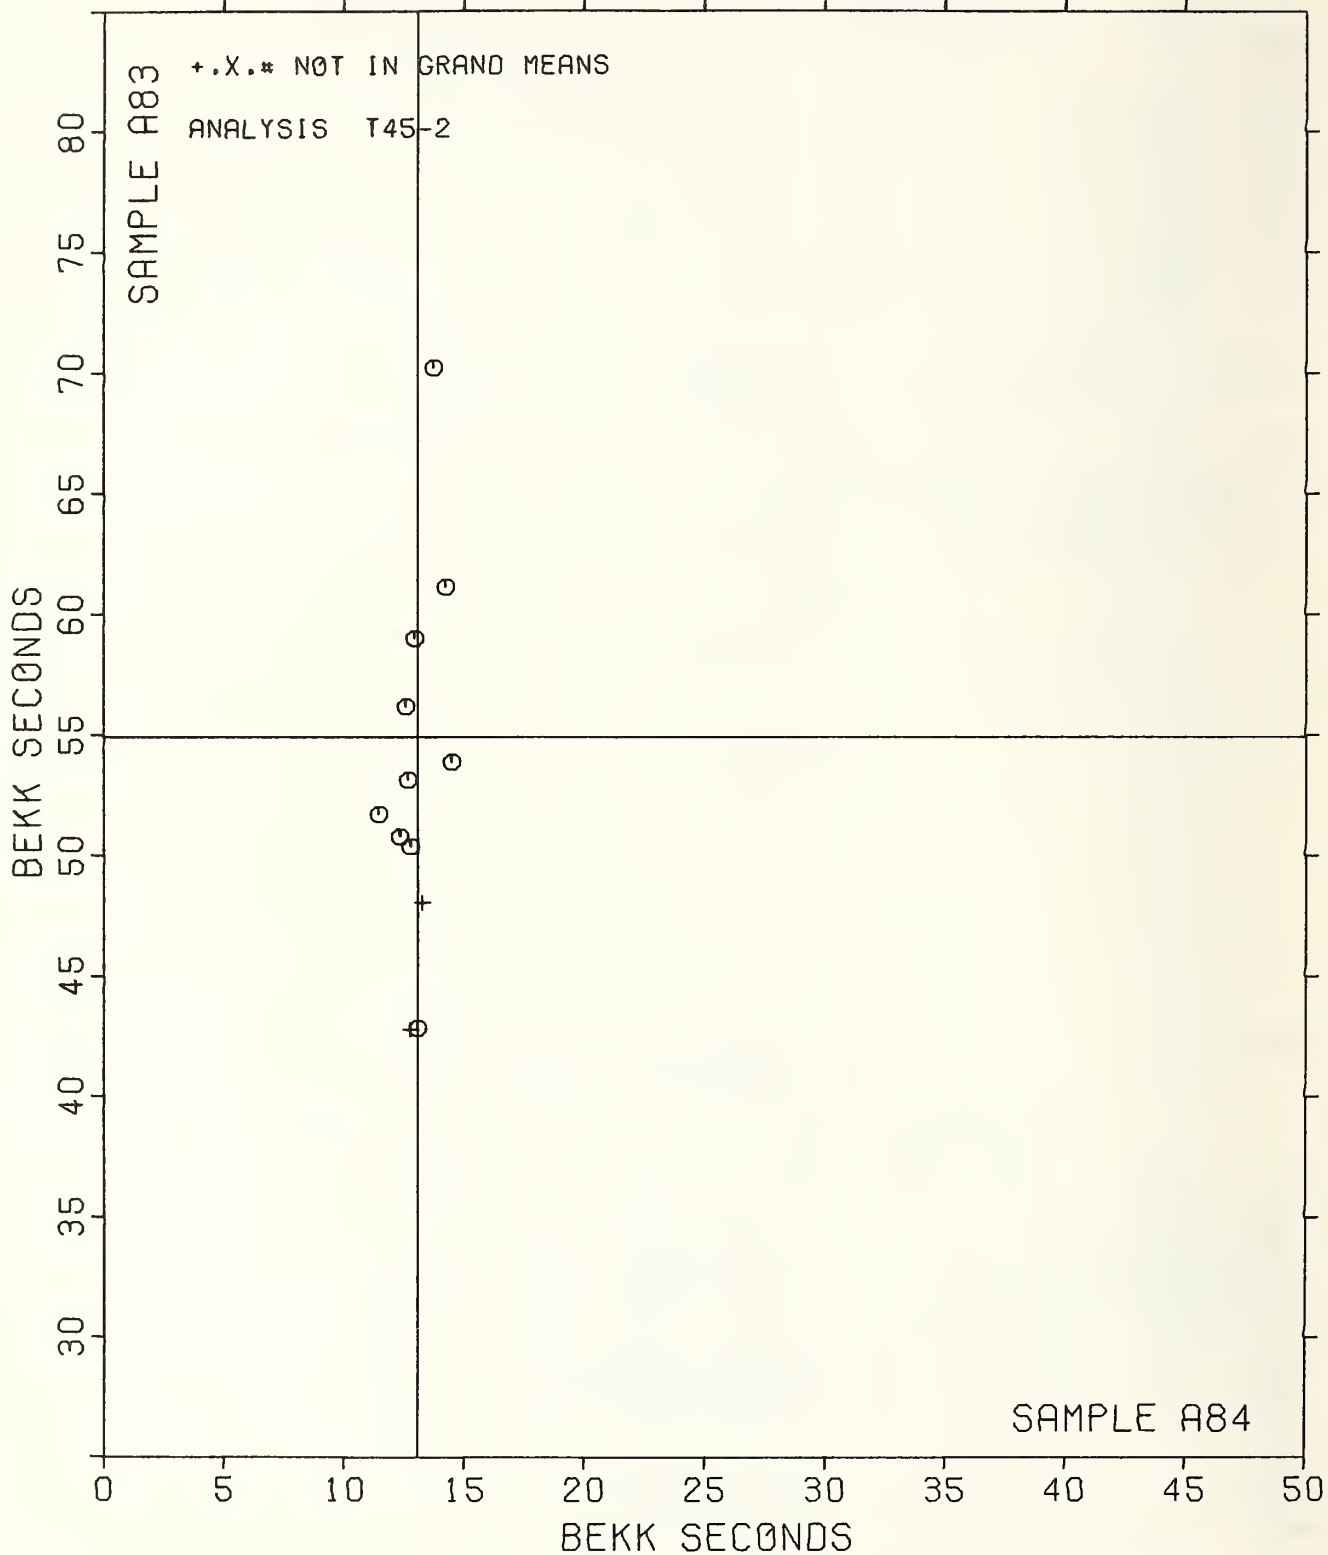

TAPPI USEFUL TEST METHOD UM 535, SMOOTHNESS OF PAPER AND PAPERBOARD (BENDTSEN TESTER)

LAB CODE	VELLUM ENVELOPE 91 GRAMS PER SQUARE METER					SAMPLE A83 94 GRAMS PER SQUARE METER					OFFSET PRINTING			TEST D <sub>0</sub> = 10			
	SAMPLE A84 MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAF	F	LAE
L100	336.	-3.	-.13	25.	1.00	116.	5.	.22	12.	.81					47B	Ø	L100
L182B	377.	37.	1.36	40.	1.59	150.	38.	1.81	18.	1.20					47B	Ø	L182B
L242	321.	-19.	-.70	18.	.70	106.	-5.	-.26	22.	1.41					47B	Ø	L242
L243B	364.	24.	.88	35.	1.39	110.	-2.	-.09	20.	1.33					47B	Ø	L243B
L244	353.	13.	.48	28.	1.12	110.	-2.	-.08	17.	1.09					47B	Ø	L244
L280	364.	24.	.68	29.	1.13	89.	-22.	-1.06	15.	1.00					47E	Ø	L280
L313	331.	-9.	-.33	38.	1.52	100.	-11.	-.53	14.	.89					47B	Ø	L313
L333	311.	-28.	-1.04	15.	.60	137.	25.	1.19	22.	1.46					47E	Ø	L333
L484	357.	17.	.63	13.	.49	130.	18.	.86	9.	.59					47B	Ø	L484
L685	340.	1.	.02	13.	.50	104.	-8.	-.37	12.	.78					47B	Ø	L685
L739	283.	-56.	-2.07	24.	.96	76.	-36.	-1.69	7.	.46					47E	Ø	L739

GP. MEAN =	340. ML/MIN	GRAND MEAN =	112. ML/MIN	TEST DETERMINATIONS =	10
SD MEANS =	27. ML/MIN	SD OF MEANS =	21. ML/MIN		11 LABS IN GRAND MEANS
	AVERAGE SDR = 25. ML/MIN		AVERAGE SDR = 15. ML/MIN		

TOTAL NUMBER OF LABORATORIES REPORTING = 11

Best values: A84  $340 \pm 55$  milliliter per minute  
A83  $115 \pm 35$  milliliter per minute


TAPPI USEFUL TEST METHOD UM 535, SMOOTHNESS OF PAPER AND PAPERBOARD (BENDTSEN TESTER)

LAB CODE	F	MEANS		COORDINATES		AVG R <sub>0</sub> SDR VAR	PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		A84	A83	MAJOR	MINOR				
L739	Ø	283.	76.	-67.	-3.	.71	47B	SMOOTHNESS,	BENDTSEN, WG 150
L333	Ø	311.	137.	-12.	36.	1.03	47B	SMOOTHNESS,	BENDTSEN, WG 150
L242	Ø	321.	106.	-19.	5.	1.06	47B	SMOOTHNESS,	BENDTSEN, WG 150
L313	Ø	331.	100.	-13.	-5.	1.20	47B	SMOOTHNESS,	BENDTSEN, WG 150
L100	Ø	336.	116.	-1.	6.	.91	47B	SMOOTHNESS,	BENDTSEN, WG 150
L685	Ø	340.	104.	-3.	-7.	.64	47B	SMOOTHNESS,	BENDTSEN, WG 150
L244	Ø	353.	110.	10.	-8.	1.10	47B	SMOOTHNESS,	BENDTSEN, WG 150
L484	Ø	357.	130.	24.	7.	.54	47B	SMOOTHNESS,	BENDTSEN, WG 150
L243B	Ø	364.	110.	20.	-14.	1.36	47B	SMOOTHNESS,	BENDTSEN, WG 150
L280	Ø	364.	89.	10.	-32.	1.06	47B	SMOOTHNESS,	BENDTSEN, WG 150
L182B	Ø	377.	150.	51.	14.	1.39	47B	SMOOTHNESS,	BENDTSEN, WG 150
GMEANS:		340.	112.			1.00			
95% ELLIPSE:				92.	53.			WIDE GAMMA = 30 DEGREE	

# SMOOTHNESS, BENDTSEN

SAMPLE A84 = 340. ML/MIN

SAMPLE A83 = 112. ML/MIN

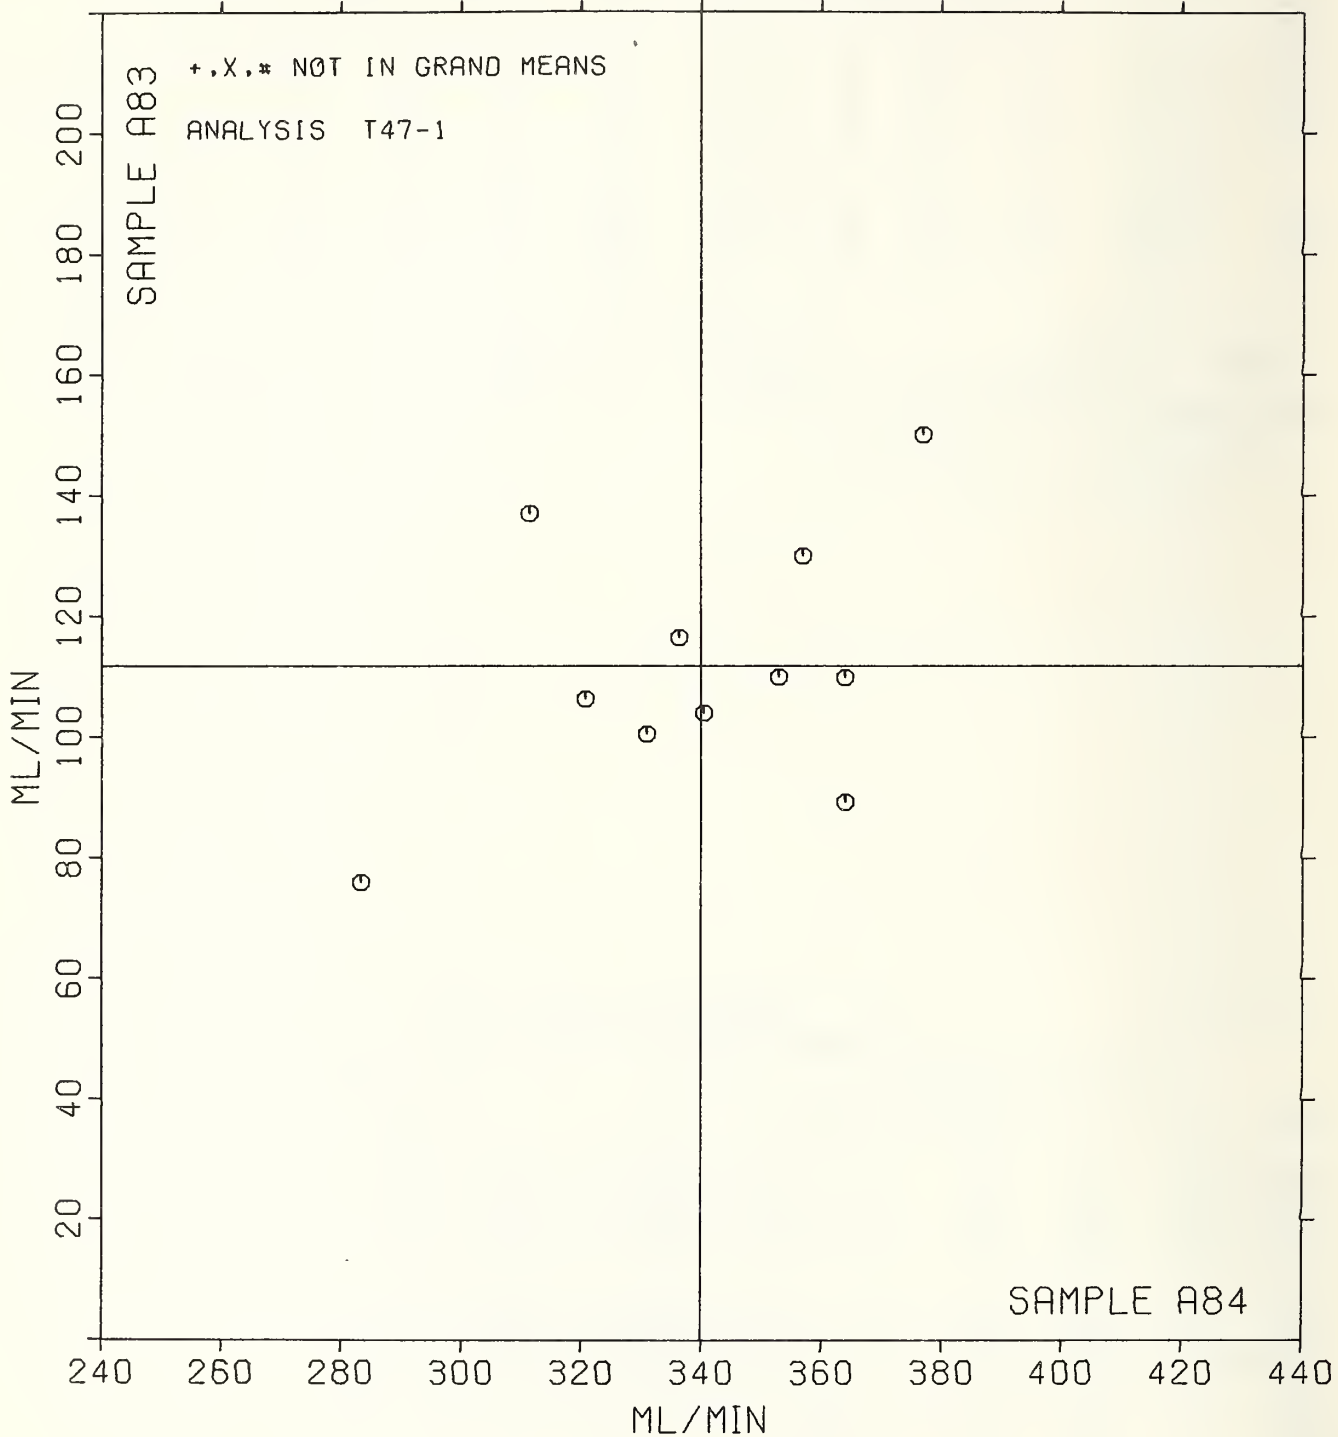



TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T53-1 TABLE 1  
MOISTURE IN PAPER, PERCENT  
TAPPI SUGGESTED METHOD T412 SU-69

LAB CODE	KRAFT WRAPPING E66 83 GRAMS PER SQUARE METER					BLEACHED KRAFT ENVELOPE G32 106 GRAMS PER SQUARE METER					TEST D <sub>0</sub> = 10		
	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAE
L134	5.98	-.10	-.17	.10	.73	5.73	.17	.39	.07	.38	53M	Ø	L134
L141	6.68	.60	1.07	.07	.47	5.99	.43	.99	.09	.53	53D	Ø	L141
L162	5.40	-.68	-1.21	.16	1.16	NO DATA REPORTED FOR SAMPLE G32					53M	M	L162
L213	6.48	.40	.72	.22	1.56	5.94	.38	.87	.05	.29	53M	Ø	L213
L244	6.26	.18	.33	.07	.52	5.73	.17	.40	.19	1.07	53D	Ø	L244
L291	6.10	.02	.04	.10	.71	5.87	.31	.71	.29	1.62	53D	Ø	L291
L376	5.78	-.30	-.53	.33	2.30	4.95	-.61	-1.40	.40	2.26	53D	Ø	L376
L442	6.06	-.02	-.03	.14	1.01	5.30	-.26	-.60	.27	1.50	53D	Ø	L442
L570	5.11	-.96	-1.72	.25	1.75	5.19	-.37	-.85	.21	1.16	53D	Ø	L570
L571	6.16	.08	.15	.22	1.54	6.76	1.20	2.76	.10	.54	53M	#	L571
L592	5.35	-.73	-1.30	.11	.76	5.01	-.55	-1.27	.10	.56	53M	Ø	L592
L729	7.08	1.00	1.79	.06	.45	6.21	.65	1.50	.15	.86	53D	Ø	L729
L739	5.96	-.12	-.21	.10	.74	5.24	-.32	-.74	.14	.77	53P	Ø	L739
GR <sub>C</sub> MEAN =		6.08 PERCENT			GRAND MEAN =		5.56 PERCENT			TEST DETERMINATIONS = 10			
SD MEANS =		.56 PERCENT			SD OF MEANS =		.43 PERCENT			11 LABS IN GRAND MEANS			
		AVERAGE SDR =			.14 PERCENT				AVERAGE SDR =		.18 PERCENT		
L100	6.39	.31	.56	.09	.62	5.83	.27	.62	.05	.27	53X	*	L100

TOTAL NUMBER OF LABORATORIES REPORTING = 14  
Best values: E66 6.1 ± 0.9 percent  
G32 5.6 ± 0.6 percent

The following laboratories were omitted from the grand means because of extreme test results: 571


TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T53-1 TABLE 2  
MOISTURE IN PAPER, PERCENT  
TAPPI SUGGESTED METHOD T412 SU-69

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---CONDITIONS				
		E66	G32	MAJOR	MINOR	R <sub>0</sub> SDR	VAR					
L570	Ø	5.11	5.16	-.99	.28	1.45	53D	MOISTURE CONTENT,	ØVEN DRYING METHOD			
L592	Ø	5.35	5.01	-.91	-.01	.66	53M	MOISTURE CONTENT,	MOISTIFEX			
L162	M	5.40				1.16	53M	MOISTURE CONTENT,	MOISTIFEX			
L376	Ø	5.78	4.95	-.60	-.31	2.28	53D	MOISTURE CONTENT,	ØVEN DRYING METHOD			
L739	Ø	5.96	5.24	-.29	-.19	.76	53P	MOISTURE CONTENT,	HØT PLATE/DESICCATOR			
L134	Ø	5.98	5.73	.02	.19	.56	53M	MOISTURE CONTENT,	MOISTIFEX			
L442	Ø	6.06	5.30	-.17	-.20	1.25	53D	MOISTURE CONTENT,	ØVEN DRYING METHOD			
L291	Ø	6.10	5.87	.20	.23	1.16	53D	MOISTURE CONTENT,	ØVEN DRYING METHOD			
L571	#	6.16	6.76	.78	.91	1.04	53M	MOISTURE CONTENT,	MOISTIFEX			
L244	Ø	6.26	5.73	.25	.03	.79	53D	MOISTURE CONTENT,	ØVEN DRYING METHOD			
L100	*	6.39	5.83	.41	.03	.45	53X	MOISTURE CONTENT:	DESCRIBE METHOD			
L213	Ø	6.48	5.94	.55	.06	.92	53M	MOISTURE CONTENT,	MOISTIFEX			
L141	Ø	6.68	5.99	.74	-.01	.50	53D	MOISTURE CONTENT,	ØVEN DRYING METHOD			
L729	Ø	7.08	6.21	1.19	-.08	.65	53D	MOISTURE CONTENT,	ØVEN DRYING METHOD			
GMEANS:		6.08	5.56			1.00						
		95% ELLIPSE:		2.10	.57	WITH GAMMA = 36 DEGREES						

# MOISTURE

SAMPLE E66 = 6.1 PERCENT

SAMPLE G32 = 5.6 PERCENT

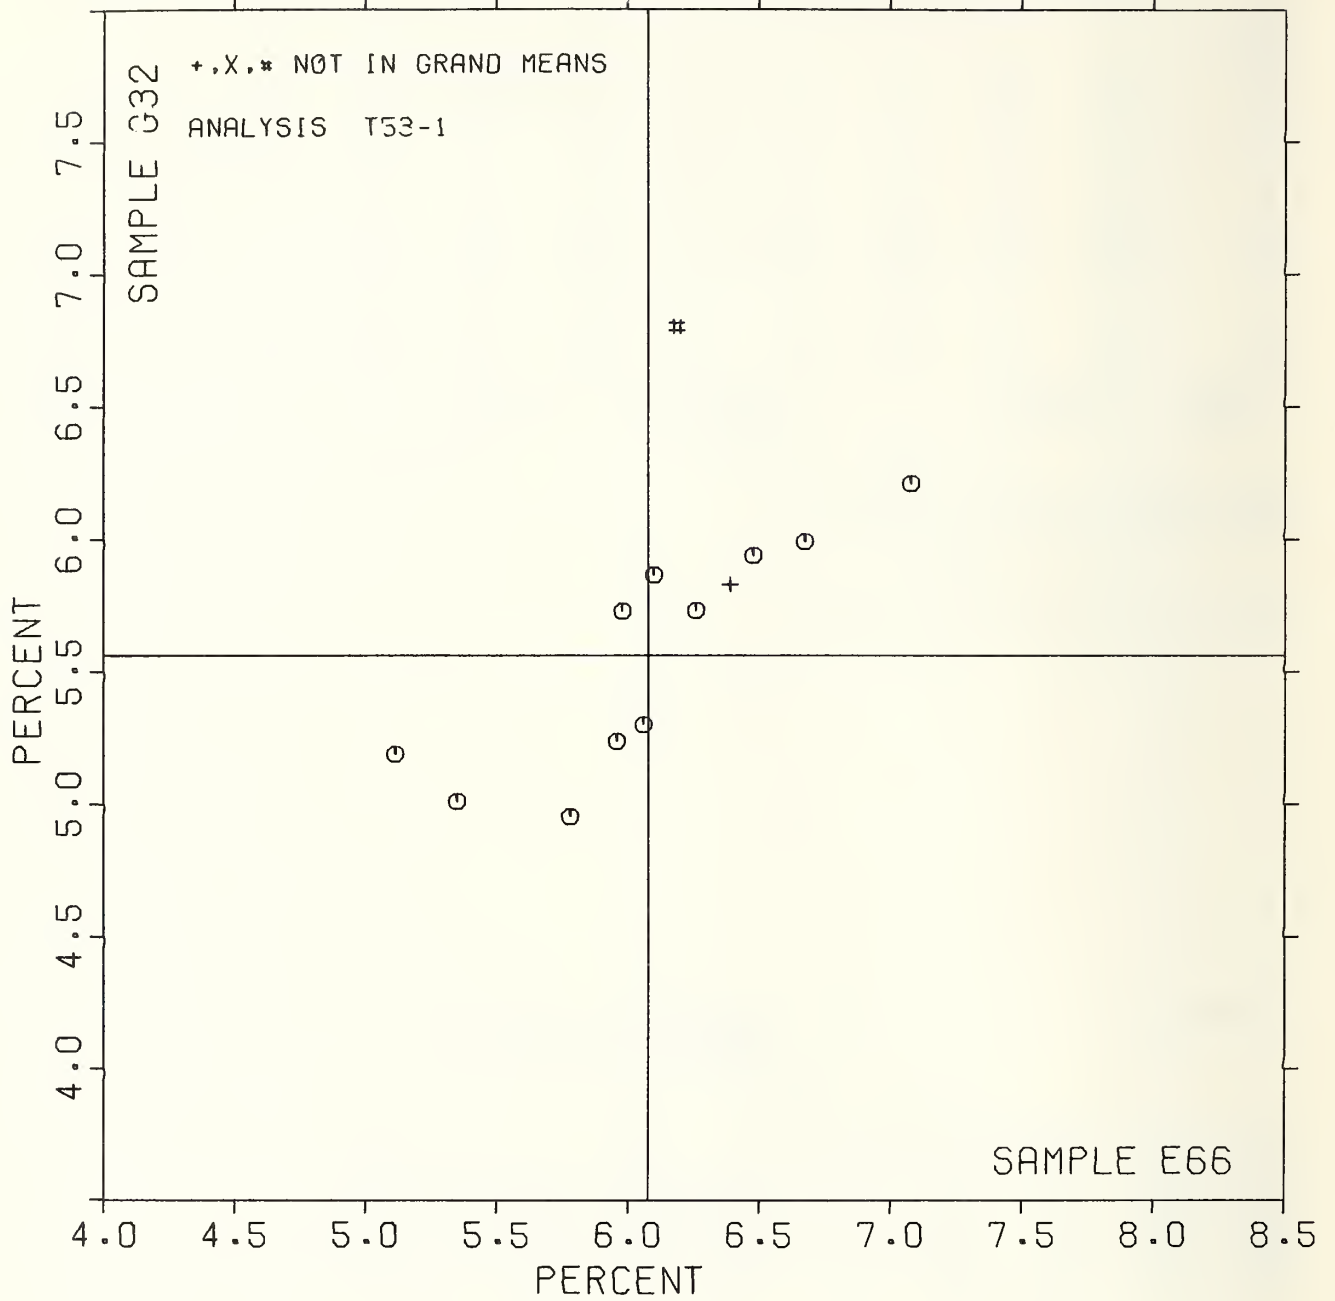

## TAPPI USEFUL TEST METHOD UM 553, PRINTING INK METHOD AND BRITISH STANDARD 4574-70

LAB CODE	SAMPLE E44		COATED GLASS 150 GRAMS PER SQUARE METER				SAMPLE G03		HEAT SET OFFSET BOOK 76 GRAMS PER SQUARE METER				TEST D <sub>0</sub> = 4	
	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB	
L126	29.5	-.1	-.02	.3	.46	58.0	.5	.08	.3	.57	56K	0	L126	
L149	31.0	1.4	.35	.8	1.28	55.0	-2.5	-.40	.0	.00	56K	0	L149	
L182	35.3	5.8	1.40	.1	.09	62.6	5.1	.82	.2	.27	56K	0	L182	
L277	29.1	-.4	-.11	.9	1.34	64.9	7.4	1.19	1.0	1.72	56K	0	L277	
L291	24.8	-4.7	-1.15	1.7	2.70	62.1	4.6	.74	.6	1.03	56K	0	L291	
L333	28.2	-1.4	-.34	.5	.73	51.0	-6.5	-1.05	1.2	1.92	56K	0	L333	
L337	24.1	-5.4	-1.32	.4	.67	47.1	-10.3	-1.67	.6	1.00	56K	0	L337	
L339	33.2	3.7	.89	.5	.78	65.7	8.3	1.33	1.0	1.60	56K	0	L339	
L616	25.2	-4.3	-1.05	.5	.78	54.5	-3.0	-.48	.6	.96	56K	0	L616	
L643	35.1	5.6	1.35	.7	1.17	54.1	-3.4	-.55	.6	.93	56K	0	L643	

GR<sub>0</sub> MEAN = 29.6 K & N UNITS

GRAND MEAN = 57.5 K &amp; N UNITS

TEST DETERMINATIONS = 4

SD MEANS = 4.1 K &amp; N UNITS

SD OF MEANS = 6.2 K &amp; N UNITS

10 LABS IN GRAND MEANS

AVERAGE SDR = .6 K &amp; N UNITS

AVERAGE SDR =

.6 K &amp; N UNITS

TOTAL NUMBER OF LABORATORIES REPORTING = 10

Best values: E44 30 K&N units  
G03 57 K&N units

## TAPPI USEFUL TEST METHOD UM 553, PRINTING INK METHOD AND BRITISH STANDARD 4574-70

LAB CODE	F	MEANS		COORDINATES		AVG R <sub>0</sub> SDR	VAR	PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		E44	G03	MAJOR	MINOR					
L337	0	24.1	47.1	-11.6	1.3	.83	56K	INK	ABSORPTION,	K&N INK TEST
L291	0	24.8	62.1	2.5	6.1	1.87	56K	INK	ABSORPTION,	K&N INK TEST
L616	0	25.2	54.5	-4.4	2.9	.87	56K	INK	ABSORPTION,	K&N INK TEST
L333	0	28.2	51.0	-6.6	-1.1	1.33	56K	INK	ABSORPTION,	K&N INK TEST
L277	0	29.1	64.9	6.7	3.1	1.53	56K	INK	ABSORPTION,	K&N INK TEST
L126	0	29.5	58.0	.4	.2	.51	56K	INK	ABSORPTION,	K&N INK TEST
L149	0	31.0	55.0	-1.8	-2.2	.64	56K	INK	ABSORPTION,	K&N INK TEST
L339	0	33.2	65.7	9.0	-.4	1.19	56K	INK	ABSORPTION,	K&N INK TEST
L643	0	35.1	54.1	-1.1	-6.4	1.05	56K	INK	ABSORPTION,	K&N INK TEST
L182	0	35.3	62.6	6.9	-3.5	.18	56K	INK	ABSORPTION,	K&N INK TEST
GMEANS:		29.6	57.5			1.00				
		95% ELLIPSE:		20.6	11.4	WITH GAMMA = 68 DEGREES				


# K & N INK ABSORPTION

SAMPLE E44 = 30.

K & N UNITS

SAMPLE G03 = 57.

K & N UNITS

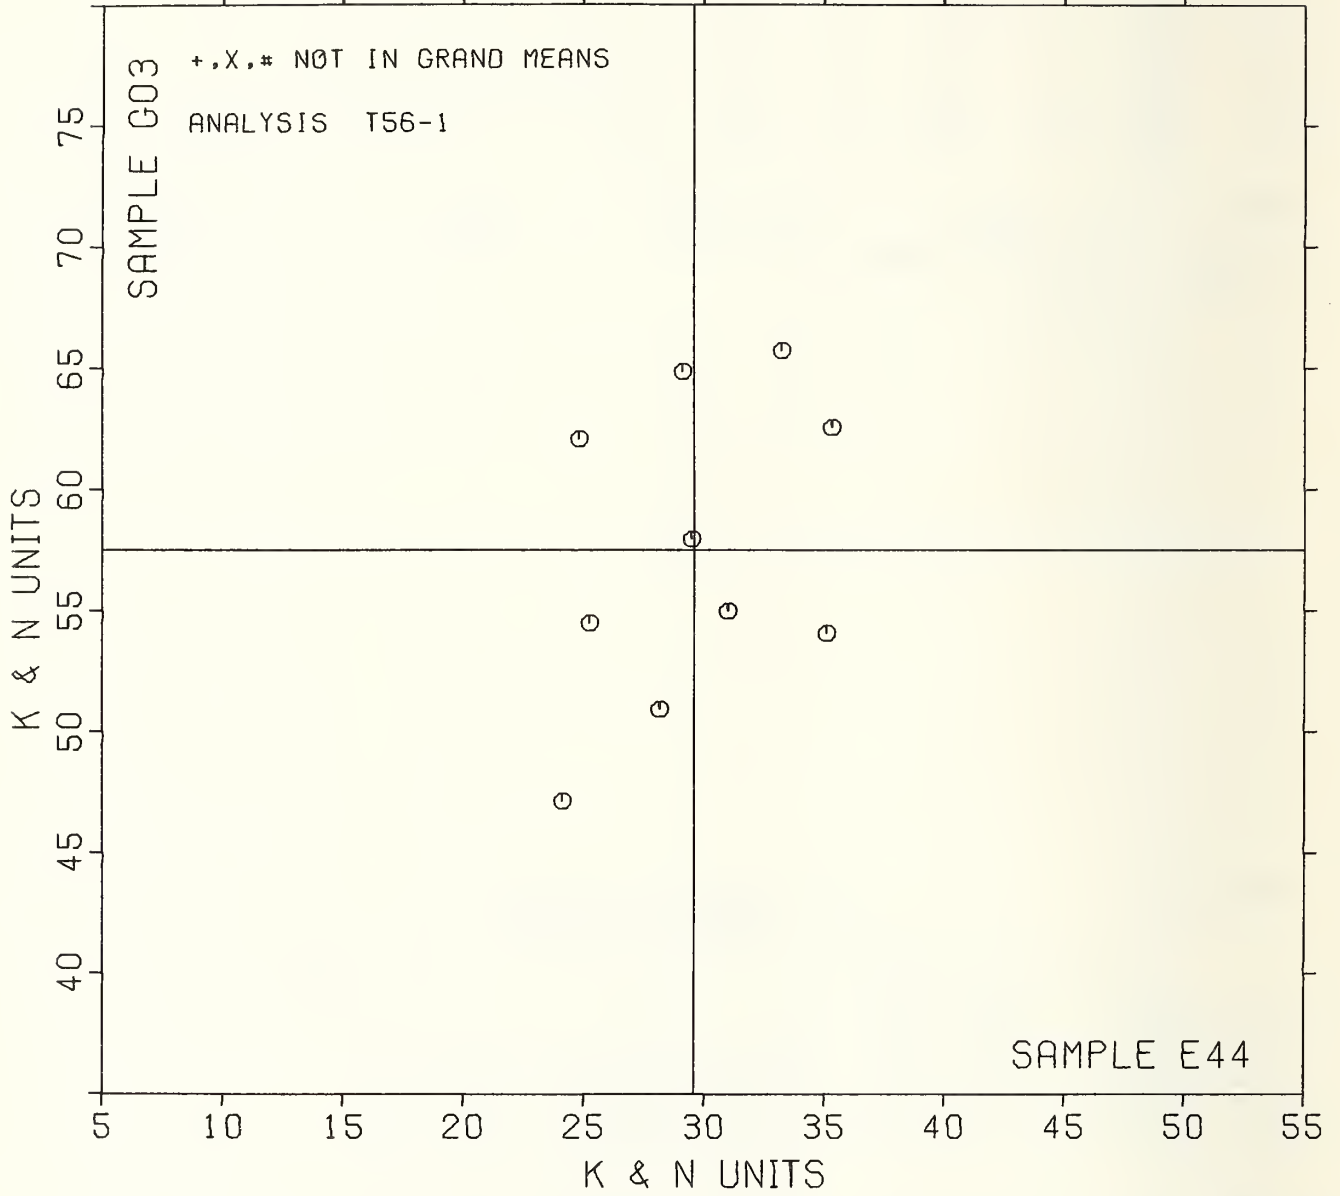



OPACITY (89% REFLECTANCE BACKING) IN PERCENT - PRIMARILY FINE PAPERS  
TAPPI OFFICIAL TEST METHOD 1425 GS-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) - B&I TYPE

LAB CODE	M.F. RELEASE PAPER 73 GRAMS PER SQUARE METER					OFFSET WHITE BOOK 72 GRAMS PER SQUARE METER					TEST D <sub>0</sub> = 10		
	G22 MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	G26 MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L105	87.22	1.52	2.08	.55	.57	88.24	-.01	-.02	.49	.51	60H	*	L105
L108	86.62	.92	1.26	.71	.74	87.54	-.71	-.98	.47	.49	60E	0	L108
L115	86.50	.80	1.10	1.02	1.06	88.93	.68	.93	.44	.46	60E	0	L115
L118	84.91	-.75	-1.07	1.33	1.37	88.64	.35	.53	.70	.72	60E	0	L118
L122	85.37	-.33	-.44	1.69	1.74	88.67	.42	.57	1.10	1.14	60D	0	L122
L123	86.20	.50	.65	1.40	1.45	88.17	-.08	-.12	1.07	1.11	60W	0	L123
L124	86.96	1.26	1.73	.67	.69	89.27	1.02	1.35	1.28	1.34	60E	0	L124
L125	86.40	.70	.76	.82	.85	88.31	.06	.08	1.59	1.66	60E	0	L125
L132	84.83	-.87	-1.18	1.36	1.40	88.30	.05	.06	1.10	1.14	60E	0	L132
L139	85.33	-.37	-.50	.44	.46	88.02	-.23	-.32	1.40	1.45	60E	0	L139
L148H	84.42	-1.28	-1.74	.54	.56	87.14	-1.11	-1.53	1.18	1.22	60E	0	L148H
L152	86.01	.31	.43	.60	.62	89.06	.81	1.10	.86	.90	60E	0	L152
L157	86.20	.50	.69	1.48	1.53	89.65	1.40	1.91	1.13	1.18	60E	0	L157
L158	85.54	-.16	-.21	1.87	1.94	88.58	.32	.45	.74	.77	60D	0	L158
L162	86.39	.65	.55	.96	1.00	88.93	.68	.93	.59	.62	60W	0	L162
L166	84.87	-.83	-1.13	.79	.82	87.89	-.36	-.50	1.04	1.08	60E	0	L166
L173A	85.34	-.36	-.48	.64	.66	88.02	-.23	-.32	.86	.90	60E	0	L173A
L190C	85.06	-.64	-.87	1.23	1.27	86.86	-1.39	-1.91	1.09	1.13	60E	0	L190C
L190R	85.92	.22	.21	.95	.95	87.13	-1.12	-1.54	1.79	1.14	60E	0	L190R
L206	85.28	-.42	-.57	1.15	1.15	88.07	-.18	-.25	.59	1.03	60E	0	L206
L210E	86.69	.95	1.36	1.10	1.13	88.68	.43	.58	1.17	1.22	60E	0	L210E
L210D	86.14	.44	.61	1.04	1.08	87.54	-.71	-.98	.82	.85	60E	0	L210D
L211S	84.98	-.72	-.98	.68	.71	88.44	.19	.25	1.27	1.32	60E	0	L211S
L212	85.66	-.04	-.05	.98	1.02	88.71	.46	.62	1.41	1.46	60H	0	L212
L213	85.67	-.03	-.03	.52	.53	89.09	.84	1.15	.77	.80	60E	0	L213
L223B	86.69	.95	1.36	.63	.65	89.06	.81	1.10	.84	.87	60E	0	L223B
L225	86.62	.92	1.26	.42	.44	88.72	.47	.64	1.10	1.14	60E	0	L225
L226B	85.30	-.40	-.54	1.24	1.28	87.87	-.38	-.53	.69	.72	60E	0	L226B
L228	84.47	-1.23	-1.67	1.13	1.16	87.44	-.81	-1.12	1.25	1.30	60E	0	L228
L230	85.78	.08	.12	.98	1.01	88.37	.12	.16	.79	.83	60E	0	L230
L238A	84.76	-.94	-1.28	.58	.60	87.13	-1.12	-1.54	.56	.58	60F	0	L238A
L241	85.88	.18	.25	.78	.81	87.52	-.73	-1.01	1.35	1.41	60E	0	L241
L243	85.27	-.43	-.58	1.23	1.27	87.80	-.45	-.62	1.10	1.14	60E	0	L243
L254	85.50	-.20	-.27	1.24	1.28	87.33	-.92	-1.27	.88	.91	60F	0	L254
L259	85.70	.00	.01	.79	.82	88.30	.05	.06	1.11	1.16	60E	0	L259
L262	85.67	-.03	-.03	.48	.50	89.95	1.70	2.33	.49	.51	60F	*	L262
L275	85.69	-.01	-.01	1.08	1.12	88.62	.37	.50	.27	.28	60F	0	L275
L278	85.58	-.12	-.16	1.14	1.18	87.77	-.48	-.67	1.06	1.10	60E	0	L278
L285D	84.86	-.84	-1.14	1.76	1.81	87.42	-.83	-1.15	1.64	1.71	60D	0	L285D
L285R	85.46	-.24	-.32	.80	.83	88.20	-.05	-.08	1.10	1.14	60E	0	L285R
L288	85.50	-.20	-.27	.66	.68	87.56	-.69	-.95	1.10	1.14	60D	0	L288
L308	86.54	.84	1.15	.77	.75	88.66	.41	.56	1.03	1.07	60E	0	L308
L317	85.61	-.05	-.12	.49	.51	87.74	-.51	-.71	.72	.75	60E	0	L317
L323	86.75	1.05	1.44	.88	.91	89.09	.84	1.15	.61	.64	60W	0	L323
L339	85.30	-.40	-.54	1.34	1.38	88.60	.35	.47	1.07	1.12	60E	0	L339
L341	84.79	-.91	-1.23	.58	.60	87.96	-.29	-.40	.64	.67	60F	0	L341
L348	84.80	-.90	-1.22	1.51	1.56	88.19	-.06	-.05	1.01	1.05	60D	0	L348
L349	85.45	-.25	-.33	1.05	1.05	88.05	-.20	-.28	.94	.98	60D	0	L349
L354	84.47	-1.23	-1.67	1.24	1.28	87.66	-.59	-.82	1.25	1.30	60E	0	L354
L366	85.60	-.10	-.13	1.24	1.28	89.18	.93	1.27	.80	.83	60E	0	L366
L554	85.75	.05	.13	.83	.86	87.57	-.68	-.94	1.14	1.18	60E	0	L554
L567	85.22	-.48	-.65	1.10	1.14	87.63	-.62	-.86	.71	.74	60D	0	L567
L571	86.53	.83	1.14	.51	.52	88.95	.70	.95	1.04	1.08	60E	0	L571
L573	86.12	.42	.58	1.25	1.25	88.70	.45	.61	.83	.86	60E	0	L573
L581	85.90	.20	.28	.98	1.01	88.66	.41	.56	.85	.88	60E	0	L581
L592	82.55	-3.15	-4.29	1.69	1.75	86.46	-1.79	-2.46	1.27	1.32	50W	*	L592
L608	88.12	2.42	3.31	1.22	1.26	90.87	2.62	3.55	1.16	1.21	60D	X	L608
L636	85.98	.28	.39	.80	.83	88.59	.34	.46	1.01	1.05	60F	0	L636
L654	86.59	.89	1.22	1.00	1.04	89.43	1.18	1.61	.75	.78	60D	0	L654
L673R	85.61	-.05	-.12	.62	.64	87.55	-.70	-.97	.48	.50	60E	0	L673R
L673T	85.49	-.21	-.28	.43	.45	87.49	-.76	-1.05	.92	.96	60E	0	L673T
L692	85.66	-.04	-.05	.73	.76	88.67	.42	.57	.92	.96	60D	0	L692
L698	84.01	-1.65	-2.30	1.32	1.36	86.74	-1.51	-2.08	1.00	1.05	60D	0	L698
L712	87.65	1.95	2.67	.94	.98	89.75	1.50	2.05	1.38	1.44	60E	*	L712

GR. MEAN = 85.70 PERCENT  
SD MEANS = .73 PERCENT

GRAND MEAN = 88.25 PERCENT  
SD OF MEANS = .73 PERCENT

TEST DETERMINATIONS = 10  
62 LABS IN GRAND MEANS

AVERAGE SDR = .97 PERCENT

AVERAGE SDR = .96 PERCENT

OPACITY (89% REFLECTANCE BACKING) IN PERCENT - PRIMARILY FINE PAPERS  
TAPPI OFFICIAL TEST METHOD T425 GS-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) - B&L TYPE

LAB CODE	SAMPLE G22		M.F. RELEASE PAPER 73 GRAMS PER SQUARE METER				SAMPLE G26		OFFSET WHITE BOOK 72 GRAMS PER SQUARE METER				TEST D <sub>0</sub> = 10		
	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB		
L100	86.05	.35	.48	1.30	1.34	88.22	-.03	-.05	.57	.59	60E	*	L100		
L219	88.91	3.21	4.35	.95	.98	90.98	2.73	3.74	.30	.31	60E	*	L219		
L224	85.53	-.17	-.23	.96	.99	88.13	-.12	-.17	.93	.96	60P	*	L224		
L249	81.57	-4.13	-5.63	1.21	1.25	85.55	-2.70	-3.71	.82	.85	60F	*	L249		
L256	86.46	.77	1.05	1.02	1.05	88.45	.19	.26	.96	1.00	60N	*	L256		
L277	85.50	-.20	-.27	.91	.94	87.65	-.60	-.83	1.20	1.25	60P	*	L277		
L312	82.60	-3.10	-4.22	.52	.53	86.20	-2.05	-2.82	.63	.66	60P	*	L312		
L380	84.80	-.90	-1.22	.79	.82	87.60	-.65	-.90	.52	.54	60P	*	L380		
L564	84.50	-1.20	-1.63	.85	.88	87.80	-.45	-.62	.92	.96	60P	*	L564		
L685B	84.69	-1.01	-1.37	.90	.94	87.57	-.68	-.94	.59	.61	60P	*	L685B		
L702	85.15	-.55	-.74	.82	.85	86.05	-2.20	-3.03	.83	.87	60P	*	L702		
L704	84.80	-.90	-1.22	.35	.36	88.00	.25	-.35	.35	.37	60P	*	L704		
L706	86.28	.58	.60	.96	1.00	89.24	.99	1.35	.63	.65	60X	*	L706		
L738	90.03	4.33	5.51	.94	.97	85.12	-3.13	-4.30	.42	.43	60X	*	L738		

TOTAL NUMBER OF LABORATORIES REPORTING = 78

Best values: G22 85.6 ± 1.1 percent  
G26 88.2 ± 1.1 percent

The following laboratories were omitted from the grand means because of extreme test results: 592



OPACITY (89% REFLECTANCE BACKING) IN PERCENT - PRIMARILY FINE PAPERS  
TAPPI OFFICIAL TEST METHOD T425 CS-75, OPACITY OF PAPER (15 DEG./DIPPOSE, ILLUMINANT A) - B&L TYPE

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---	CONDITIONS
		G22	G26	MAJOR	MINOR	R <sub>0</sub> SDR	VAR		
L249	*	81.57	85.55	-4.83	.92	1.05	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L592	#	82.55	86.46	-3.50	.94	1.53	60W	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN,DIGITAL
L312	*	82.60	86.20	-3.65	.72	.60	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L698	Ø	84.01	86.74	-2.26	.11	1.20	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L148B	Ø	84.42	87.14	-1.65	.11	.89	60B	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN
L354	Ø	84.47	87.66	-1.25	.44	1.29	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L228	Ø	84.47	87.44	-1.44	.28	1.23	60B	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN
L564	*	84.50	87.80	-1.17	.52	.92	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L685B	*	84.69	87.57	-1.20	.22	.77	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L238A	Ø	84.76	87.13	-1.46	-.14	.59	60R	OPACITY (WHITE BACKING)	82 T 95%, THWING-ALBERT (WAS SRL)
L341	Ø	84.79	87.96	-.85	.43	.63	60R	OPACITY (WHITE BACKING)	82 T 95%, THWING-ALBERT (WAS SRL)
L704	*	84.80	88.00	-.82	.45	.36	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L380	*	84.80	87.60	-1.10	.16	.68	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L348	Ø	84.80	88.19	-.68	.58	1.30	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L132	Ø	84.83	88.30	-.58	.64	1.27	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L285D	Ø	84.86	87.42	-1.18	-.01	1.76	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L166	Ø	84.87	87.89	-.84	.32	.95	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L118	Ø	84.91	88.64	-.29	.83	1.05	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L211S	Ø	84.98	88.44	-.38	.63	1.01	60R	OPACITY (WHITE BACKING)	82 T 95%, THWING-ALBERT (WAS SRL)
L190C	Ø	85.06	86.86	-1.43	-.54	1.20	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L702	*	85.15	86.05	-1.94	-1.18	.86	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L567	Ø	85.22	87.63	-.78	-.11	.94	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L243	Ø	85.27	87.80	-.62	-.02	1.21	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L206	Ø	85.28	88.07	-.43	.16	1.11	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L339	Ø	85.30	88.60	-.04	.52	1.25	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L226B	Ø	85.30	87.87	-.55	.00	1.00	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L139	Ø	85.33	88.02	-.42	.09	.56	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L173A	Ø	85.34	88.02	-.42	.08	.78	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L122	Ø	85.37	88.67	.06	.52	1.44	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L349	Ø	85.45	88.05	-.32	.03	1.03	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L285R	Ø	85.46	88.20	-.21	.13	.99	60R	OPACITY (WHITE BACKING)	82 T 95%, THWING-ALBERT (WAS SRL)
L673I	Ø	85.49	87.49	-.68	-.40	.70	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L277	*	85.50	87.65	-.56	-.29	1.10	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L288	Ø	85.50	87.56	-.63	-.36	.51	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L254	Ø	85.50	87.33	-.79	-.52	1.10	60R	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN
L224	*	85.53	88.13	-.21	.03	.98	60P	OPACITY (WHITE BACKING)	82 T 95%, PHOTOVELT
L158	Ø	85.54	88.58	.12	.34	1.35	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L278	Ø	85.58	87.77	-.42	-.26	1.14	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L366	Ø	85.60	89.18	.58	.72	1.06	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L673R	Ø	85.61	87.55	-.56	-.44	.57	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L317	Ø	85.61	87.74	-.42	-.31	.63	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L212	Ø	85.66	88.71	.30	.35	1.24	60B	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN
L692	Ø	85.66	88.67	.27	.32	.86	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L262	*	85.67	89.95	1.17	1.22	.50	60R	OPACITY (WHITE BACKING)	82 T 95%, THWING-ALBERT (WAS SRL)
L213	Ø	85.67	89.09	.57	.61	.67	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L275	Ø	85.69	88.62	.25	.26	.70	60R	OPACITY (WHITE BACKING)	82 T 95%, THWING-ALBERT (WAS SRL)
L259	Ø	85.70	88.30	.04	.03	.59	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L230	Ø	85.78	88.37	.14	.02	.52	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L554	Ø	85.79	87.57	-.41	-.55	1.02	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L241	Ø	85.88	87.52	-.39	-.65	1.11	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L581	Ø	85.90	88.66	.43	.14	.95	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L190R	Ø	85.92	87.13	-.63	-.96	1.06	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L636	Ø	85.98	88.59	.44	.04	.94	60R	OPACITY (WHITE BACKING)	82 T 95%, THWING-ALBERT (WAS SRL)
L152	Ø	86.01	89.06	.79	.35	.76	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L100	*	86.05	88.22	.23	-.27	.97	60E	OPACITY (WHITE BACKING)	82 T 95%, Z <sub>0</sub> ELREPBØ,FMY-C(10) FILTER
L573	Ø	86.12	88.70	.62	.02	1.08	60H	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN
L210D	Ø	86.14	87.54	-.19	-.82	.56	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2
L157	Ø	86.20	89.65	1.34	.64	1.35	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L123	Ø	86.20	88.17	.30	-.42	1.28	60W	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN,DIGITAL
L706	*	86.28	89.24	1.11	.29	.83	60X	OPACITY, 82 T 95%: GIVE INSTRUMENT MAKE, MODEL, BACKING	
L162	Ø	86.39	88.93	.57	-.01	.81	60W	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN,DIGITAL
L125	Ø	86.40	88.31	.54	-.46	1.25	60B	OPACITY (WHITE BACKING)	82 T 95%, HUYGEN
L256	*	86.46	88.45	.68	-.41	1.02	60N	OPACITY (WHITE BACKING)	82 T 95%, HUNTER
L115	Ø	86.50	88.93	1.05	-.09	.76	60B	OPACITY (WHITE BACKING)	82 T 95%, BAUSCH * LOMB
L571	Ø	86.53	88.95	1.08	-.09	.80	60D	OPACITY (WHITE BACKING)	82 T 95%, BNL-2

OPACITY (89% REFLECTANCE BACKING) IN PERCENT - PRIMARILY FINE PAPERS  
TAPPI OFFICIAL TEST METHOD T425 68-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) - B&I TYPE


LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		G22	G26	MAJOR	MINOR	R <sub>0</sub> SDR	VAR			
I308	Ø	86.54	88.66	.89	-0.31	.93	60H	OPACITY (WHITE BACKING)	82 TØ	95%, HUYGEN
I654	Ø	86.59	89.43	1.46	.21	.91	60D	OPACITY (WHITE BACKING)	82 TØ	95%, BNL-2
L225	Ø	86.62	88.72	.98	-0.32	.79	60B	OPACITY (WHITE BACKING)	82 TØ	95%, BAUSCH * LØMB
L108	Ø	86.62	87.54	.15	-1.16	.61	60E	OPACITY (WHITE BACKING)	82 TØ	95%, BAUSCH * LØMB
L223D	Ø	86.69	89.06	1.27	-0.13	.76	60B	OPACITY (WHITE BACKING)	82 TØ	95%, BAUSCH * LØMB
L210B	Ø	86.69	88.68	1.01	-0.40	1.18	60E	OPACITY (WHITE BACKING)	82 TØ	95%, BAUSCH * LØMB
L323	Ø	86.75	89.09	1.34	-0.15	.77	60W	OPACITY (WHITE BACKING)	82 TØ	95%, HUYGEN, DIGITAL
L124	Ø	86.96	89.27	1.61	-0.17	1.01	60B	OPACITY (WHITE BACKING)	82 TØ	95%, BAUSCH * LØMB
L105	*	87.22	88.24	1.07	-1.08	.54	60B	OPACITY (WHITE BACKING)	82 TØ	95%, HUYGEN
L712	*	87.65	89.75	2.44	-0.31	1.21	60B	OPACITY (WHITE BACKING)	82 TØ	95%, BAUSCH * LØMB
L698	X	88.12	90.87	3.56	.15	1.23	60D	OPACITY (WHITE BACKING)	82 TØ	95%, BNL-2
L219	*	88.91	90.98	4.20	-0.33	.65	60E	OPACITY (WHITE BACKING)	82 TØ	95%, ZØ ELREPHØ, FMY-C(10) FILTER
L738	*	90.03	85.12	.87	-5.28	.70	60X	OPACITY, 82 TØ	95%: GIVE INSTRUMENT MAKE, MODEL, BACKING	
GMEANS:		85.70	88.25			1.00				
		95% ELLIPSE:		2.33	1.19	WITH GAMMA = 44 DEGREES				



OPACITY, B&L, 89% BACKING, FINE P.

SAMPLE G22 = 85.7 PERCENT

SAMPLE G26 = 88.3 PERCENT

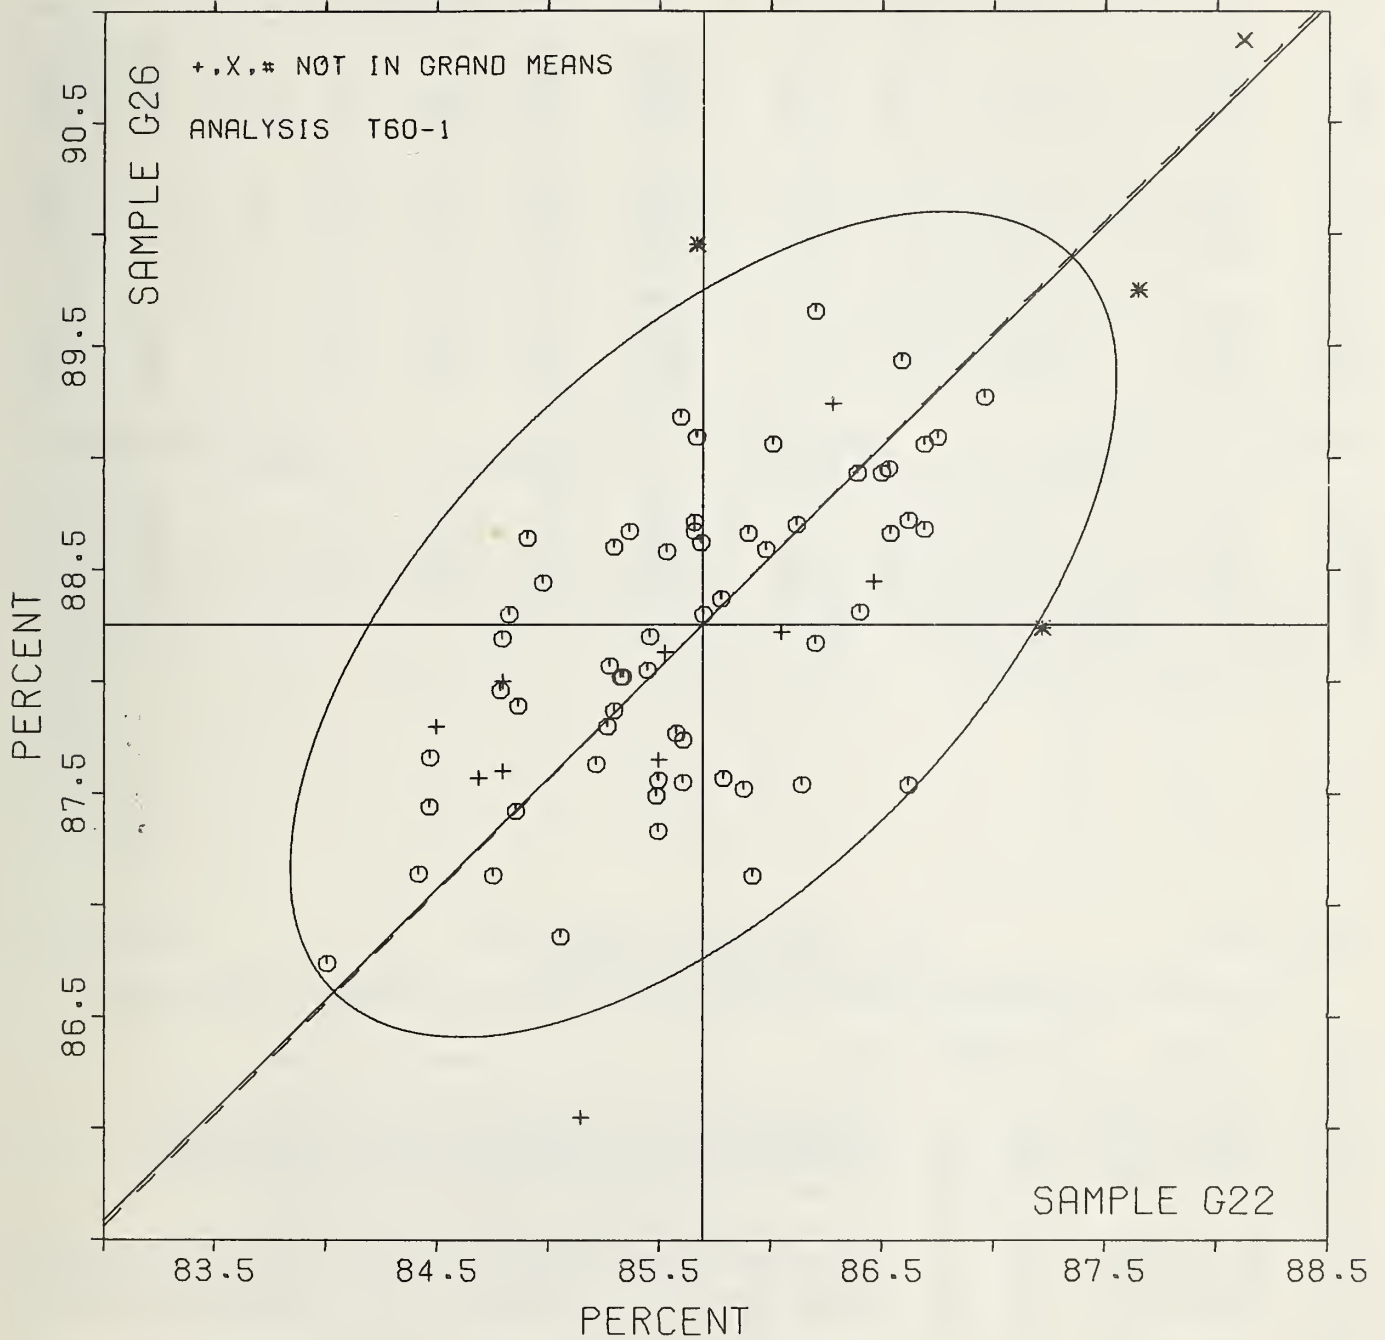

OPACITY (PAPER BACKING) IN PERCENT - PRIMARILY FINE PAPERS  
TAPPI OFFICIAL TEST METHOD T519 GS-78, DIFFUSE OPACITY OF PAPER - ILLUMINANT C, ELREPHO TYPE

LAB CODE	SAMPLE G22 MEAN	M.F. RELEASE PAPER 73 GRAMS PER SQUARE METER				SAMPLE G26 MEAN	OFFSET WHITE BOOK 72 GRAMS PER SQUARE METER				TEST D <sub>0</sub> = 10		
		DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR		DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAE
L100	87.10	.17	.39	1.28	1.41	90.13	-.10	-.24	.53	.72	60J	0	L100
L182E	86.69	-.24	-.56	1.08	1.19	89.90	-.33	-.76	.96	1.29	60J	0	L182E
L219	86.99	.06	.13	.99	1.10	90.73	.50	1.13	.93	1.24	60F	0	L219
L233	86.23	-.70	-1.62	.78	.86	90.20	-.03	-.08	.62	.83	60J	0	L233
L242	87.22	.29	.66	.71	.78	90.66	.43	.57	.61	.82	60J	0	L242
L250T	86.68	-.25	-.58	1.05	1.16	90.07	-.16	-.37	.75	1.01	60J	0	L250T
L251	86.68	-.25	-.57	.84	.93	90.43	.20	.45	.40	.53	60F	0	L251
L309	86.61	-.32	-.74	.70	.77	89.81	-.42	-.96	1.13	1.52	60J	0	L309
L313	87.63	.70	1.61	.71	.79	90.95	.72	1.63	.53	.71	60J	0	L313
L360	86.67	-.26	-.60	1.00	1.10	89.53	-.70	-1.60	1.04	1.39	60F	0	L360
L446	86.55	-.38	-.88	1.06	1.17	90.09	-.14	-.32	.69	.92	60J	0	L446
L575	86.63	-.30	-.70	.85	.93	89.55	-.68	-1.56	.79	1.06	60J	0	L575
L598	87.08	.15	.34	.82	.91	90.23	-.00	-.01	.69	.93	60J	0	L598
L678	87.69	.76	1.74	.93	1.03	90.86	.63	1.43	.76	1.03	60J	0	L678
L685A	87.53	.60	1.38	.81	.89	90.36	.13	.29	.75	1.01	60F	0	L685A

GP<sub>0</sub> MEAN = 86.93 PERCENT      GRAND MEAN = 90.23 PERCENT      TEST DETERMINATIONS = 10  
SD MEANS = .43 PERCENT      SD OF MEANS = .44 PERCENT      15 LABS IN GRAND MEANS  
AVERAGE SDR = .91 PERCENT      AVERAGE SDR = .74 PERCENT

L118	85.34	-1.59	-3.67	1.11	1.23	89.98	-.25	-.58	.91	1.22	60C	+	L118
L190C	85.42	-1.51	-3.48	1.44	1.59	90.01	-.22	-.51	.71	.96	60C	+	L190C
L190R	86.11	-.82	-1.89	1.15	1.26	89.57	-.66	-1.51	.77	1.04	60C	+	L190R
L243	86.30	-.63	-1.46	.76	.84	90.44	.21	.47	.85	1.15	60C	+	L243
L626	86.25	-.68	-1.57	.82	.91	88.90	-1.33	-3.04	.74	.99	60Q	+	L626

TOTAL NUMBER OF LABORATORIES REPORTING = 20

Best values: G22 86.8 ± 0.8 percent  
G26 90.2 ± 0.7 percent

OPACITY (PAPER BACKING) IN PERCENT - PRIMARILY FINE PAPERS  
TAPPI OFFICIAL TEST METHOD T519 GS-78, DIFFUSE OPACITY OF PAPER - ILLUMINANT C, ELREPHO TYPE


LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---CONDITIONS					
		G22	G26	MAJOR	MINOR	R <sub>0</sub> SDR	VAR						
L118	+	85.34	89.98	-1.30	.96	1.22	60C	OPACITY (PAPER BACKING)82 T0	95%	BAUSCH	+	L0MB	
L190C	+	85.42	90.01	-1.22	.92	1.28	60C	OPACITY (PAPER BACKING)82 T0	95%	BAUSCH	+	L0MB	
L190R	+	86.11	89.57	-1.05	.12	1.15	60C	OPACITY (PAPER BACKING)82 T0	95%	BAUSCH	+	L0MB	
L233	0	86.23	90.20	-.52	.48	.85	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L626	+	86.25	88.90	-1.43	-.45	.95	60Q	OPACITY (PAPER BACKING)82 T0	95%	PHOTOVOLT			
L243	+	86.30	90.44	-.30	.60	1.00	60C	OPACITY (PAPER BACKING)82 T0	95%	BAUSCH	+	L0MB	
L446	0	86.55	90.09	-.37	.17	1.04	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L309	0	86.61	89.81	-.53	-.07	1.14	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L575	0	86.63	89.55	-.70	-.26	1.00	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L360	0	86.67	89.53	-.69	-.31	1.25	60F	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)N0	TRAP	
L250T	0	86.68	90.07	-.29	.07	1.08	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L251	0	86.68	90.43	-.03	.32	.73	60F	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)N0	TRAP	
L182E	0	86.69	89.90	-.41	-.06	1.24	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L219	0	86.99	90.73	.39	.31	1.17	60F	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)N0	TRAP	
L598	0	87.08	90.23	.10	-.11	.92	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L100	0	87.10	90.13	.04	-.19	1.06	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L242	0	87.22	90.66	.51	.09	.80	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L685A	0	87.53	90.36	.51	-.34	.95	60F	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)N0	TRAP	
L313	0	87.63	90.95	1.00	.01	.75	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	
L678	0	87.69	90.86	.98	-.10	1.03	60J	OPACITY (PAPER BACKING)82 T0	95%	Z <sub>0</sub> ELREPHO	,FMY-C(10)	FILTER	

GMEANS: 86.93 90.23 1.00  
95% ELLIPSE: 1.63 .69 WITE GAMMA = 45 DEGREES

OPACITY, ELREPHO, PAPER BACKING, FINE P

SAMPLE G22 = 86.9 PERCENT

SAMPLE G26 = 90.2 PERCENT

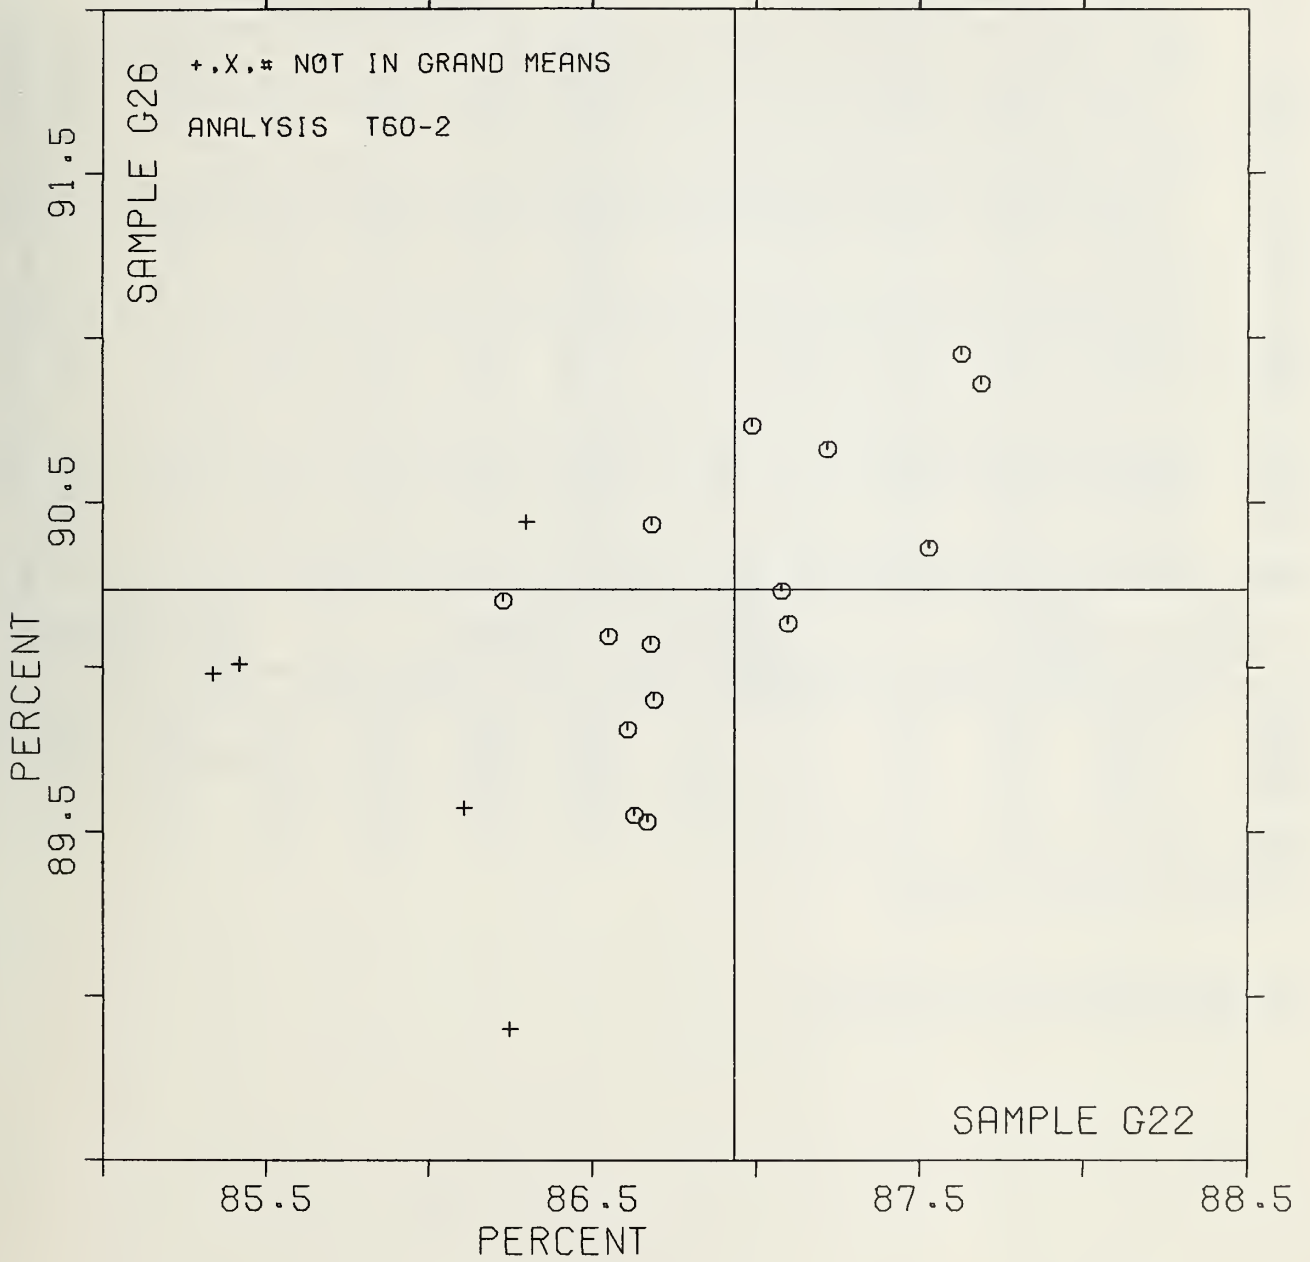

OPACITY (89% REFLECTANCE BACKING) IN PERCENT - PRIMARILY NEWS, DIRECTORY, AND CATALOG  
TAPPI OFFICIAL TEST METHOD T425 OS-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) - B&I TYPE

IAB CODE	RAG BOND 75 GRAMS PER SQUARE METER					AIR MAIL ENVELOPE 49 GRAMS PER SQUARE METER					TEST D <sub>0</sub> = 10		
	B01 MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	A56 MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L121	75.76	.61	.68	.76	1.09	78.85	.01	.01	.48	.52	61B	0	L121
L122	74.36	-.79	-.88	.73	1.04	77.81	-1.03	-.94	1.34	1.46	61D	0	L122
L131	74.40	-.75	-.83	.52	.74	77.60	-1.24	-1.13	.97	1.05	61R	e	L131
L134	79.10	3.95	4.40	.74	1.06	80.80	1.96	1.79	1.14	1.23	61F	#	L134
L150B	75.00	-.15	-.17	.88	1.26	77.65	-1.19	-1.08	1.03	1.12	61B	e	L150B
L159	74.34	-.81	-.90	.46	.66	78.66	-.18	-.16	.59	.65	61R	0	L159
L210B	75.93	.78	.87	.88	1.26	80.13	1.29	1.18	1.07	1.16	61B	0	L210B
L210D	75.42	.27	.30	.80	1.14	79.59	.75	.69	1.18	1.28	61D	e	L210D
L255	73.29	-1.86	-2.07	.57	.82	76.40	-2.44	-2.22	1.07	1.17	61E	0	L255
L261	75.73	.58	.65	.84	1.21	80.65	1.81	1.65	.65	.71	61B	0	L261
L281	76.19	1.04	1.16	.48	.69	79.61	.77	.70	.84	.92	61D	0	L281
L305	74.12	-1.03	-1.15	.70	1.01	78.19	-.65	-.59	.77	.83	61B	0	L305
L315	74.78	-.37	-.41	.83	1.19	79.53	.69	.63	1.16	1.26	61D	0	L315
L317	74.71	-.44	-.49	.58	.84	78.48	-.36	-.33	.79	.86	61B	e	L317
L318	75.60	.45	.50	.70	1.00	79.75	.91	.83	1.14	1.23	61E	0	L318
L326	73.87	-1.28	-1.42	.93	1.33	77.52	-1.32	-1.20	1.09	1.18	61B	0	L326
L328	76.70	1.55	1.73	.47	.68	80.78	1.94	1.77	.67	.73	61B	0	L328
L333	74.80	-.35	-.39	.60	.85	78.98	.14	.13	.81	.88	61B	e	L333
L352	75.43	.28	.31	.78	1.12	78.78	-.06	-.05	.71	.78	61R	0	L352
L581	75.74	.59	.66	.60	.86	78.96	.12	.11	.67	.73	61B	0	L581
L599	76.60	1.45	1.62	.74	1.06	79.35	.51	.47	1.76	1.91	61B	e	L599
L713	75.35	.20	.22	.80	1.15	78.32	-.52	-.47	.54	.59	61R	0	L713
GR <sub>0</sub> MEAN = 75.15 PERCENT			GRAND MEAN = 78.84 PERCENT			TEST DETERMINATIONS = 10							
SD MEANS = .90 PERCENT			SD OF MEANS = 1.10 PERCENT			21 LABS IN GRAND MEANS							
AVERAGE SDR = .70 PERCENT			AVERAGE SDR = .92 PERCENT										
L150J	76.80	1.66	1.84	.92	1.31	75.67	-3.17	-2.89	.23	.24	61J	+	L150J
L153	75.15	.00	.00	.41	.59	79.40	.56	.51	.97	1.05	61C	+	L153
L244	74.88	-.27	-.30	.30	.43	81.69	2.85	2.60	.95	1.03	61J	+	L244
L260	75.15	.00	.00	.47	.68	78.39	-.45	-.41	.41	.44	61F	+	L260
L687	74.80	-.35	-.39	.67	.97	78.35	-.49	-.44	.41	.45	61F	+	L687
L738	76.16	1.01	1.13	.37	.54	81.09	2.25	2.05	.74	.80	61X	+	L738
TOTAL NUMBER OF LABORATORIES REPORTING = 28													
Best values: B01 75.2 ± 1.4 percent													
A56 78.8 ± 1.9 percent													

The following laboratories were omitted from the grand means because of extreme test results: 134




OPACITY (89% REFLECTANCE BACKING) IN PERCENT - PRIMARILY NEWS, DIRECTORY, AND CATALOG  
TAPPI OFFICIAL TEST METHOD T425 6S-75, OPACITY OF PAPER (15 DEG./DIFFUSE, ILLUMINANT A) - B&L TYPE

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		B01	A56	MAJOR	MINOR	R <sub>s</sub>	SDR VAR			
L255	Ø	73.29	76.40	-3.07	-0.04	.99	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L326	Ø	73.87	77.52	-1.83	.19	1.26	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L305	Ø	74.12	78.19	-1.14	.41	.92	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L159	Ø	74.34	78.66	-0.64	.53	.65	61R	OPACITY (WHITE BACKING)	70	10 90%, TBWING-ALBERT (WAS SRI)
L172	Ø	74.36	77.81	-1.30	-0.01	1.25	61D	OPACITY (WHITE BACKING)	70	10 90%, BNL-2
L131	Ø	74.40	77.60	-1.44	-0.17	.89	61R	OPACITY (WHITE BACKING)	70	10 90%, TBWING-ALBERT (WAS SRI)
L317	Ø	74.71	78.48	-0.55	.12	.85	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L315	Ø	74.78	79.53	.32	.72	1.22	61D	OPACITY (WHITE BACKING)	70	10 90%, BNL-2
L687	+	74.80	78.35	-0.60	-0.03	.71	61F	OPACITY (WHITE BACKING)	70	10 90%, PHOTOVELT
L333	Ø	74.80	78.98	-0.10	.36	.87	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L244	+	74.88	81.69	2.08	1.97	.73	61J	OPACITY (PAPER BACKING)	70	10 90%, Z.ELREPHO,FMY-C(10) FILTER
L150B	Ø	75.00	77.65	-1.03	-0.62	1.19	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L260	+	75.15	78.39	-0.35	-0.28	.56	61P	OPACITY (WHITE BACKING)	70	10 90%, PHOTOVELT
L153	+	75.15	79.40	.44	.35	.82	61C	OPACITY (PAPER BACKING)	70	10 90%, BAUSCH + LOMB
L713	Ø	75.35	78.32	-0.28	-0.48	.87	61R	OPACITY (WHITE BACKING)	70	10 90%, TBWING-ALBERT (WAS SRI)
L210D	Ø	75.42	79.59	.76	.25	1.21	61D	OPACITY (WHITE BACKING)	70	10 90%, BNL-2
L352	Ø	75.43	78.78	.13	-0.26	.95	61R	OPACITY (WHITE BACKING)	70	10 90%, TBWING-ALBERT (WAS SRI)
L318	Ø	75.60	79.75	1.00	.21	1.12	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L261	Ø	75.73	80.65	1.79	.66	.96	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L581	Ø	75.74	78.96	.46	-0.39	.79	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L121	Ø	75.76	78.85	.39	-0.47	.80	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L210B	Ø	75.93	80.13	1.50	.18	1.21	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L738	+	76.16	81.09	2.40	.59	.67	61X	OPACITY, 70 TO 90%: GIVE INSTRUMENT MAKE, MODEL, BACKING		
L281	Ø	76.19	79.61	1.25	-0.34	.80	61D	OPACITY (WHITE BACKING)	70	10 90%, BNL-2
L599	Ø	76.60	79.35	1.30	-0.83	1.49	61B	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L328	Ø	76.70	80.78	2.49	-0.02	.70	61E	OPACITY (WHITE BACKING)	70	10 90%, BAUSCH + LOMB
L150J	+	76.80	75.67	-1.48	-3.26	.78	61J	OPACITY (PAPER BACKING)	70	10 90%, Z.ELREPHO,FMY-C(10) FILTER
L134	#	76.10	80.80	3.98	-1.90	1.14	61R	OPACITY (WHITE BACKING)	70	10 90%, TBWING-ALBERT (WAS SRI)
GMEANS:		75.15	78.84			1.00				
		95% ELLIPSE:		3.68	1.16			WITH GAMMA = 51 DEGREES		

OPACITY, B&L, 89% BACKING, NEWS

SAMPLE B01 = 75.1 PERCENT

SAMPLE A56 = 78.8 PERCENT

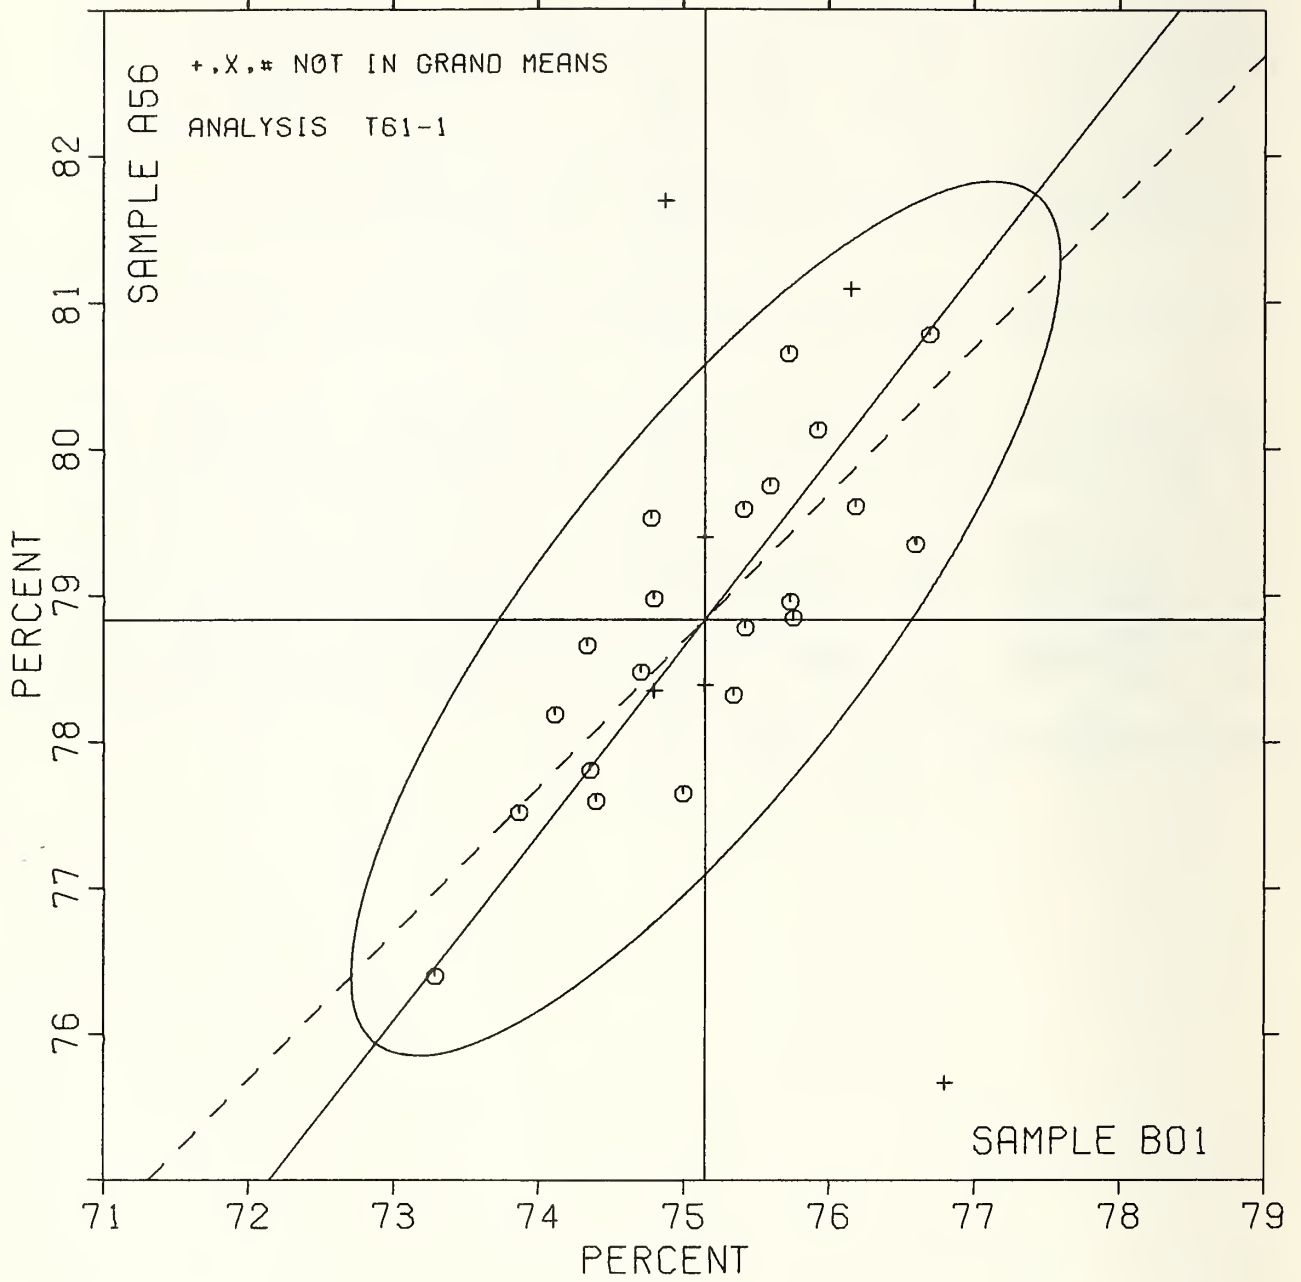

DIRECTIONAL BLUE REFLECTANCE IN PERCENT

TAPPI STANDARD T452 69-77, 'BRIGHTNESS'; MARTIN SWEETS (ACBT & GE) IS STANDARD FOR THIS ANALYSIS

LAB CODE	SAMPLE J34		PRINTING 73 GRAMS PER SQUARE METER				SAMPLE J38		PRINTING 69 GRAMS PER SQUARE METER				TEST D. = e		
	MEAN	DEV	No. DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	No. DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAE		
L109	67.15	-.05	-.11	.19	.94	75.79	-.15	-.32	.11	.68	65N	Ø	L109		
L115	67.31	.11	.24	.10	.50	75.57	-.37	-.77	.13	.78	65N	Ø	L115		
L122	67.14	-.06	-.14	.22	1.12	75.59	-.35	-.74	.11	.68	65N	Ø	L122		
L132	67.36	.16	.34	.19	.98	75.61	-.33	-.69	.14	.82	65N	Ø	L132		
L158	67.41	.21	.45	.16	.79	76.42	.48	1.01	.23	1.36	65N	Ø	L158		
L176A	66.31	-.29	-1.91	.32	1.62	74.80	-1.14	-2.39	.05	.32	65A	Ø	L176A		
L190C	67.11	-.09	-.19	.26	1.32	76.11	.17	.36	.14	.82	65A	Ø	L190C		
L210M	67.32	.12	.26	.28	1.43	76.22	.28	.59	.10	.63	65M	Ø	L210M		
L210N	67.35	.15	.32	.21	1.09	76.51	.57	1.19	.15	.88	65N	Ø	L210N		
L211	68.24	1.04	2.22	.13	.66	76.75	.81	1.69	.16	.97	65N	Ø	L211		
L225	67.52	.32	.69	.16	.80	76.27	.33	.70	.15	.90	65N	Ø	L225		
L243	66.97	-.23	-.49	.19	.97	76.25	.31	.64	.19	1.17	65A	Ø	L243		
L275	67.25	.05	.10	.38	1.92	75.65	-.29	-.61	.08	.46	65N	Ø	L275		
L285	67.91	.71	1.53	.12	.63	76.62	.68	1.43	.28	1.71	65N	Ø	L285		
L288	67.05	-.15	-.33	.18	.90	75.94	-.00	-.01	.63	3.84	65N	Ø	L288		
L308	67.42	.22	.48	.17	.85	76.14	.20	.41	.19	1.16	65N	Ø	L308		
L315	67.49	.29	.61	.24	1.20	76.34	.40	.83	.13	.79	65N	Ø	L315		
L317	66.95	-.25	-.54	.16	.81	75.14	-.80	-1.69	.20	1.21	65M	Ø	L317		
L565	67.71	.51	1.10	.12	.63	75.71	-.23	-.48	.11	.68	65A	Ø	L565		
L636A	66.72	-.48	-1.02	.21	1.04	75.72	-.22	-.45	.14	.84	65M	Ø	L636A		
L636B	66.85	-.35	-.76	.18	.90	75.94	-.00	-.01	.18	1.07	65M	Ø	L636B		
L636C	66.01	-1.15	-2.55	.47	2.41	75.86	-.08	-.17	.23	1.37	65M	*	L636C		
L673R	66.94	-.26	-.57	.14	.72	75.32	-.62	-1.29	.12	.71	65N	Ø	L673R		
L692	67.32	.12	.26	.23	1.18	76.31	.37	.78	.08	.51	65N	Ø	L692		

GR. MEAN = 67.20 PERCENT      GRAND MEAN = 75.94 PERCENT      TEST DETERMINATIONS = 6  
SD MEANS = .47 PERCENT      SD OF MEANS = .48 PERCENT      24 LABS IN GRAND MEANS

AVERAGE SDR = .20 PERCENT      AVERAGE SDR = .17 PERCENT

L105	66.64	-.56	-1.21	.14	.72	76.14	.20	.41	.16	.97	65I	+	L105
L213	67.07	-.13	-.27	.07	.36	76.10	.16	.33	.09	.56	65I	+	L213
L219	68.25	1.05	2.25	.27	1.36	78.12	2.18	4.57	.23	1.40	65F	+	L219
L223	67.45	.25	.53	.13	.67	76.89	.95	1.98	.14	.82	65G	+	L223
L224	67.56	.36	.77	.15	.77	76.57	.63	1.33	.18	1.11	65H	+	L224
L241	67.32	.12	.26	.21	1.08	76.06	.12	.25	.11	.64	65I	+	L241
L249	67.97	.77	1.66	.24	1.24	76.95	1.01	2.11	.09	.56	65F	+	L249
L256	66.54	-.66	-1.43	.18	.94	75.69	-.25	-.53	.18	1.10	65H	+	L256
L259	66.86	-.34	-.73	.22	1.12	75.77	-.17	-.35	.15	.90	65H	+	L259
L260	67.07	-.13	-.27	.07	.36	77.06	1.12	2.35	.09	.56	65F	+	L260
L277	68.12	.92	1.98	.64	3.26	74.69	-1.25	-2.63	1.69	10.23	65P	+	L277
L278	72.31	5.11	10.97	.59	3.02	81.00	5.06	10.60	.00	.00	65P	+	L278
L312	69.00	1.80	3.86	.00	.00	78.00	2.06	4.31	.00	.00	65F	+	L312
L321	69.00	1.80	3.86	.00	.00	79.00	3.06	6.41	.00	.00	65P	+	L321
L328	70.16	2.96	6.36	.22	1.12	77.45	1.51	3.16	.48	2.93	65F	+	L328
L339	69.62	2.42	5.20	.35	1.80	78.94	3.00	6.27	.18	1.07	65P	+	L339
L380	71.00	3.80	8.15	.00	.00	79.00	3.06	6.41	.00	.00	65P	+	L380
L442	66.75	-.45	-.97	.26	1.30	75.35	-.59	-1.24	.15	.92	65I	+	L442
L456	65.50	-1.70	-3.65	.19	.94	74.65	-1.29	-2.71	.19	1.12	65P	+	L456
L562	73.50	6.30	13.52	.00	.00	81.00	5.06	10.60	.00	.00	65P	+	L562
L564	70.12	2.92	6.27	.35	1.80	78.37	2.43	5.10	.52	3.14	65P	+	L564
L591	66.56	-.64	-1.38	.11	.58	75.22	-.72	-1.51	.12	.74	65H	+	L591
L617	68.14	.94	2.01	.51	2.58	77.66	1.72	3.60	.18	1.12	65G	+	L617
L626	69.44	2.24	4.80	.18	.90	77.56	1.62	3.39	.18	1.07	65P	+	L626
L643	67.17	-.03	-.06	.14	.71	75.77	-.17	-.35	.09	.54	65F	+	L643
L684	67.09	-.11	-.25	.49	2.47	67.69	-8.25	-17.29	.15	.88	65H	+	L684
L698	67.71	.51	1.10	.14	.69	76.60	.66	1.38	.13	.79	65I	+	L698
L702	70.00	2.80	6.01	.00	.00	78.44	2.50	5.23	.18	1.07	65X	+	L702
L704	68.87	1.67	3.59	.44	2.25	76.12	.18	.38	.23	1.40	65F	+	L704
L706	67.80	.60	1.28	.16	.81	76.99	1.05	2.19	.10	.60	65X	+	L706
L738	67.11	-.09	-.19	.20	1.03	76.26	.32	.67	.12	.72	65X	+	L738
L743	69.41	2.21	4.75	.15	.74	77.90	1.96	4.10	.05	.32	65X	+	L743

TOTAL NUMBER OF LABORATORIES REPORTING = 56

Best values: J34 67.0 ± 0.9 percent  
J38 76.0 ± 0.8 percent



DIRECTIONAL BLUE REFLECTANCE IN PERCENT  
TAPPI STANDARD T452 6S-77, 'BRIGHTNESS'; MARTIN SWEETS (ACBT & GE) IS STANDARD FOR THIS ANALYSIS


LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		JJ4	J38	MAJOR	MINOR	R <sub>0</sub> SDR	VAR			
L456	+	65.50	74.65	-2.11	.33	1.03	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L636C	*	66.01	75.86	-.88	.80	1.89	65M	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (GE), S-1
L176A	0	66.31	74.80	-1.44	-.15	.97	65A	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (ACBT),S-2
L256	+	66.54	75.69	-.64	.30	1.02	65B	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER
L591	+	66.56	75.22	-.97	-.04	.66	65B	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER
L105	+	66.64	76.14	-.25	.54	.84	65T	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER D25D2M
L636A	0	66.72	75.72	-.49	.19	.94	65M	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (GE), S-1
L442	+	66.75	75.35	-.74	-.08	1.11	65T	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER D25D2M
L636B	0	66.85	75.94	-.25	.25	.99	65M	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (GE), S-1
L259	+	66.86	75.77	-.36	.13	1.01	65B	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER
L673R	0	66.94	75.32	-.63	-.24	.71	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L317	0	66.95	75.14	-.75	-.38	1.01	65M	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (GE), S-1
L243	0	66.97	76.25	.06	.38	1.07	65A	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (ACBT),S-2
L288	0	67.05	75.94	-.11	.11	2.37	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L260	+	67.07	77.06	.72	.87	.46	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L213	+	67.07	76.10	.03	.20	.46	65T	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER D25D2M
L684	+	67.09	67.69	-6.03	-5.64	1.67	65B	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER
L738	+	67.11	76.26	.17	.29	.88	65X	BLUE	REFLECTANCE:GIVE INSTR.( )DIFFUSE,( )DIRECTNL,TRAF?,BASE?	
L190C	0	67.11	76.11	.06	.18	1.07	65A	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (ACBT),S-2
L122	0	67.14	75.59	-.30	-.20	.90	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L108	0	67.15	75.79	-.15	-.07	.81	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L643	+	67.17	75.77	-.14	-.10	.62	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L275	0	67.25	75.65	-.18	-.24	1.19	65M	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (GE), S-1
L115	0	67.31	75.57	-.19	-.33	.64	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L692	0	67.32	76.31	.35	.17	.84	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L210M	0	67.32	76.22	.29	.11	1.03	65M	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (GE), S-1
L241	+	67.32	76.06	.17	-.01	.86	65I	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER D25D2A
L210N	0	67.35	76.51	.51	.29	.98	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L132	0	67.36	75.61	-.13	-.34	.90	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L158	0	67.41	76.42	.49	.18	1.08	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L308	0	67.42	76.14	.30	-.03	1.01	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L223	+	67.45	76.89	.85	.48	.74	65G	BLUE	REFLECTANCE (DIRECTIONAL),	GARDNER
L315	0	67.49	76.34	.48	.07	.99	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L225	0	67.52	76.27	.46	-.00	.85	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L224	+	67.56	76.57	.71	.18	.94	65B	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER
L698	+	67.71	76.60	.83	.09	.74	65I	BLUE	REFLECTANCE (DIRECTIONAL),	BUNTER D25D2A
L565	0	67.71	75.71	.19	-.53	.66	65A	BLUE	REFLECTANCE (DIRECTIONAL),	MARTIN SWEETS (ACBT),S-2
L706	+	67.80	76.99	1.17	.29	.71	65X	BLUE	REFLECTANCE:GIVE INSTR.( )DIFFUSE,( )DIRECTNL,TRAF?,BASE?	
L285	0	67.91	76.62	.98	-.04	1.17	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L249	+	67.97	76.95	1.26	.14	.90	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L277	+	68.12	74.69	-.27	-1.53	6.74	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L617	+	68.14	77.66	1.89	.52	1.85	65G	BLUE	REFLECTANCE (DIRECTIONAL),	GARDNER
L211	0	68.24	76.75	1.30	-.19	.82	65N	BLUE	REFLECTANCE (DIRECTIONAL),	TECBNIDYNE/DIANG/M0 S0, S-4
L219	+	68.25	78.12	2.30	.76	1.38	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L704	+	68.87	76.12	1.29	-1.08	1.83	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L321	+	69.00	79.00	3.45	.82	.00	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L312	+	69.00	78.00	2.73	.13	.00	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L743	+	69.41	77.90	2.94	-.24	.53	65X	BLUE	REFLECTANCE:GIVE INSTR.( )DIFFUSE,( )DIRECTNL,TRAF?,BASE?	
L626	+	69.44	77.56	2.72	-.49	.98	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L339	+	69.62	78.94	3.84	.33	1.43	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L702	+	70.00	78.44	3.74	-.29	.54	65X	BLUE	REFLECTANCE:GIVE INSTR.( )DIFFUSE,( )DIRECTNL,TRAF?,BASE?	
L564	+	70.12	78.37	3.78	-.42	2.47	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L328	+	70.16	77.45	3.14	-1.09	2.03	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L380	+	71.00	79.00	4.84	-.62	.00	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L278	+	72.31	81.00	7.19	-.18	1.51	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
L562	+	73.50	81.00	8.01	-1.04	.00	65P	BLUE	REFLECTANCE (DIRECTIONAL),	FB0T0V0LT
GMEANS:		67.20	75.94			1.00				
		95% ELLIPSE:		1.61	.78					WITH GAMMA = 46 DEGREES



# BLUE REFLECTANCE, DIRECTIONAL

SAMPLE J34 = 67.2 PERCENT

SAMPLE J38 = 75.9 PERCENT

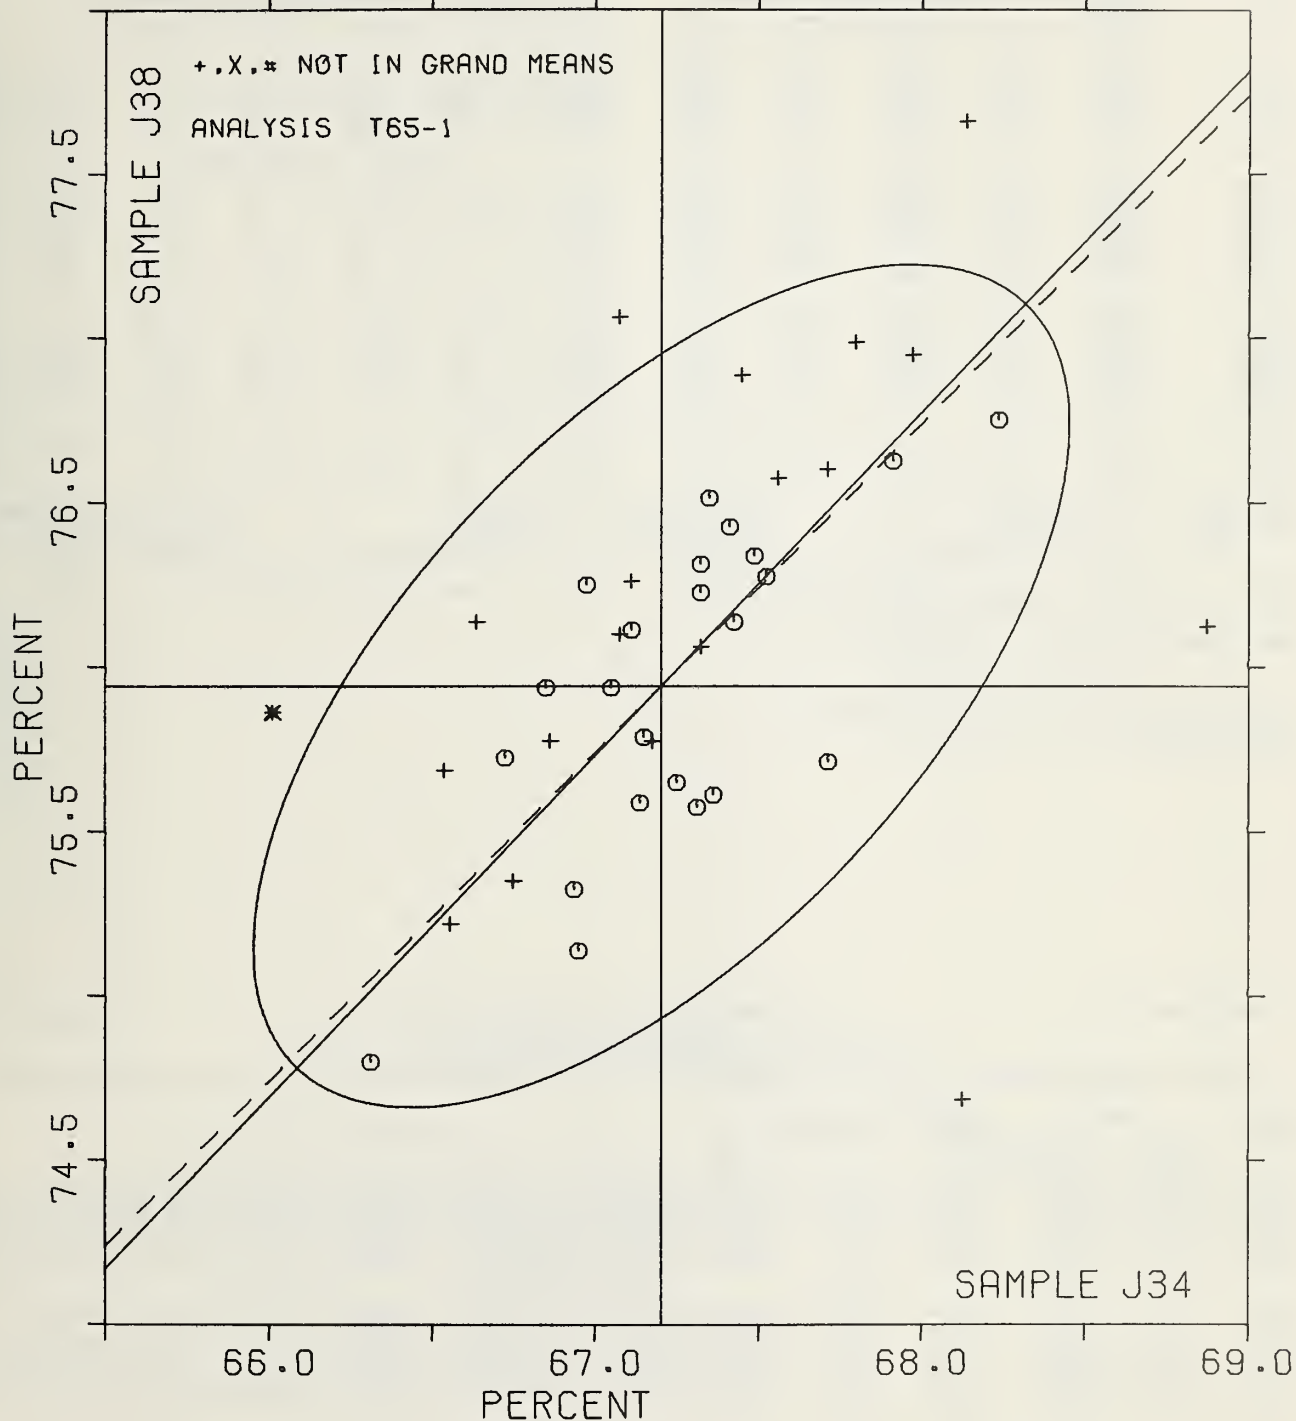




BLUE REFLECTANCE, DIFFUSE, WITH TRAP

SAMPLE J34 = 66.4 PERCENT

SAMPLE J38 = 74.9 PERCENT

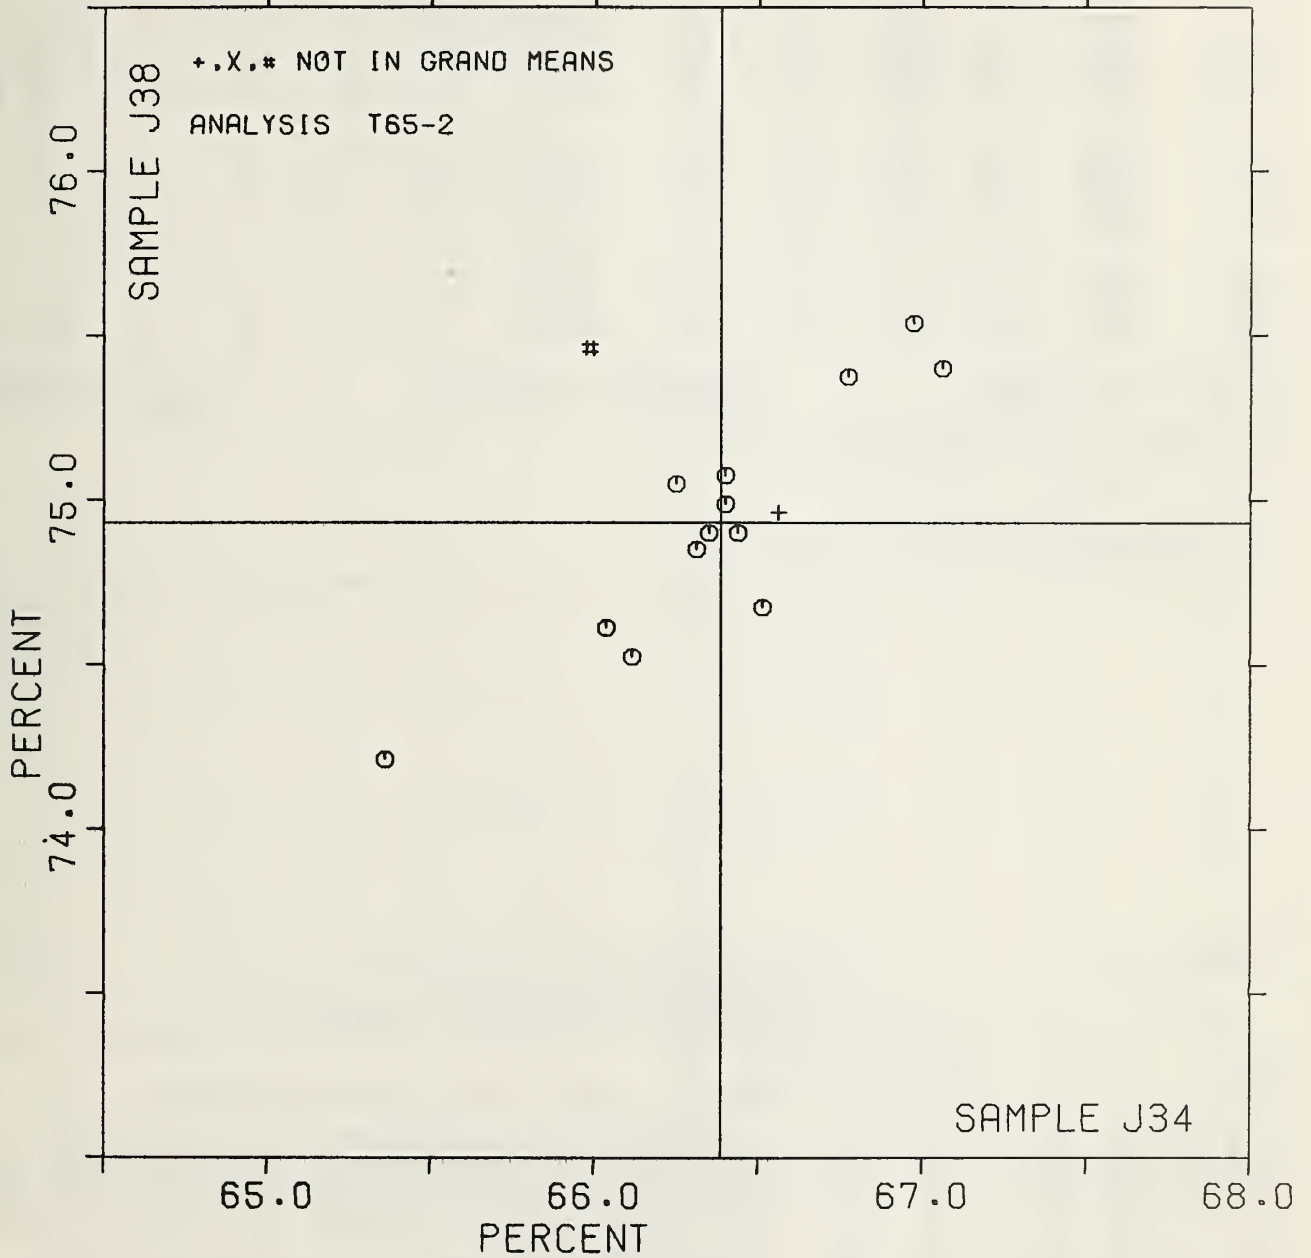

DIFFUSE BLUE REFLECTANCE IN PERCENT (NO GLOSS TRAP)

TAPPI SUGGESTED METHOD T525 SU-72, BRIGHTNESS OF PULP (DIFFUSE ILLUMINATION AND 0 DEG. OBSERVATION)

LAB CODE	SAMPLE J34 73 GRAMS PER SQUARE METER					SAMPLE J38 89 GRAMS PER SQUARE METER					TEST D <sub>0</sub> = 8		
	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L157	67.66	-0.21	-0.52	.27	2.18	77.11	.42	.72	.11	1.19	65E	0	L157
L161	76.72	0.85	21.73	.05	.37	67.96	-0.74	-14.91	.10	1.07	65E	#	L161
L173A	67.45	-0.42	-1.04	.05	.43	76.10	-0.59	-1.01	.08	.80	65E	0	L173A
L219	68.50	.63	1.54	.13	1.05	77.51	.82	1.40	.12	1.31	65E	0	L219
L238A	68.46	.59	1.45	.07	.60	77.01	.32	.55	.11	1.19	65E	0	L238A
L241	67.52	-0.35	-0.85	.13	1.03	75.81	-0.88	-1.50	.11	1.19	65E	0	L241
L251	68.05	.18	.43	.12	.96	77.27	.58	.99	.09	.94	65E	0	L251
L255	67.97	.10	.25	.07	.57	76.87	.18	.31	.07	.75	65D	0	L255
L309	66.57	-1.30	-3.19	.32	2.59	76.65	-0.04	-0.07	.17	1.78	65J	#	L309
L360	68.25	.38	.93	.09	.74	77.26	.57	.97	.11	1.12	65E	0	L360
L384	67.89	.01	.04	.11	.90	76.67	-0.02	-0.03	.05	.49	65S	0	L384
L565	67.77	-0.10	-0.24	.22	1.75	76.05	-0.64	-1.10	.14	1.49	65W	0	L565
L685	67.80	-0.07	-0.18	.11	.86	76.70	.01	.01	.08	.80	65E	0	L685
L734	67.14	-0.74	-1.81	.12	.95	75.92	-0.77	-1.31	.07	.75	65E	0	L734

GR. MEAN = 67.87 PERCENT  
SD MEANS = .41 PERCENT  
AVERAGE SDR = .12 PERCENT  
TOTAL NUMBER OF LABORATORIES REPORTING = 14

GRAND MEAN = 76.69 PERCENT  
SD OF MEANS = .59 PERCENT  
AVERAGE SDR = .09 PERCENT  
TEST DETERMINATIONS = 8  
12 LABS IN GRAND MEANS

Best values: J34 67.8 ± 0.6 percent  
J38 76.7 ± 0.8 percent

The following laboratories were omitted from the grand means because of extreme test results: 161, 309

DIFFUSE BLUE REFLECTANCE IN PERCENT (NO GLOSS TRAP)

TAPPI SUGGESTED METHOD T525 SU-72, BRIGHTNESS OF PULP (DIFFUSE ILLUMINATION AND 0 DEG. OBSERVATION)

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---CONDITIONS				
		J34	J38	MAJOR	MINOR	R <sub>0</sub> SDR	VAR					
L309	#	66.57	76.65	-0.74	1.07	2.19	65J	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, NBS ABSOLUTE				
L734	0	67.14	75.92	-1.04	.20	.85	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L173A	0	67.45	76.10	-0.73	.04	.61	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L241	0	67.52	75.81	-0.93	-0.18	1.11	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L157	0	67.66	77.11	.24	.40	1.68	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L565	0	67.77	76.05	-0.59	-0.26	1.62	65W	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, NBS MG0 BASE				
L685	0	67.80	76.70	-0.03	.07	.83	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L384	0	67.89	76.67	-0.01	-0.02	.69	65S	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, ABSOLUTE-UNKNOWN BASE				
L255	0	67.97	76.87	.21	.01	.66	65D	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, NRC-PTB ABSOLUTE				
L251	0	68.05	77.27	.59	.17	.95	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L360	0	68.25	77.26	.68	-0.01	.93	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L238A	0	68.46	77.01	.59	-0.32	.89	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L219	0	68.50	77.51	1.03	-0.08	1.18	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				
L161	#	76.72	67.96	-2.57	-12.17	.72	65E	DIFFUSE REFLECTANCE, ELREPH0, NO TRAP, MG0 (ZEISS) BASE				


GMEANS: 67.87 76.69  
95% ELLIPSE: 2.06 .61  
1.00  
WITH GAMMA = 57 DEGREES



BLUE REFLECTANCE, DIFFUSE, NO TRAP

SAMPLE J34 = 67.9 PERCENT

SAMPLE J38 = 76.7 PERCENT

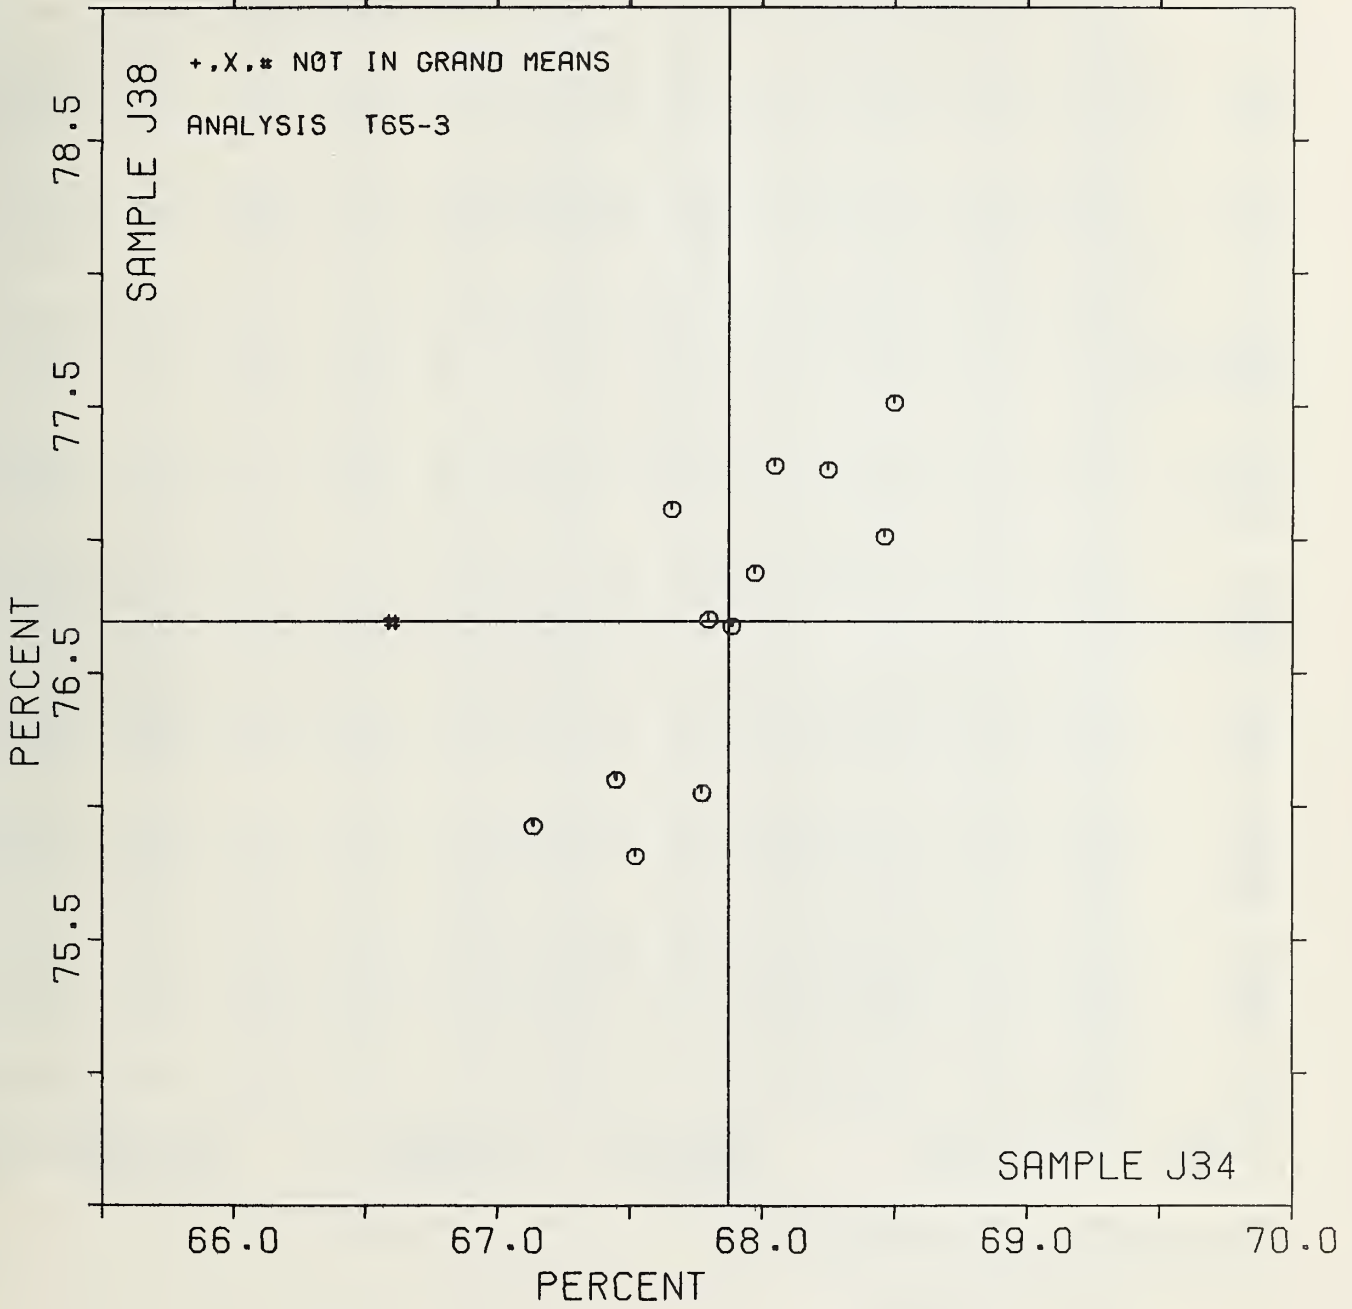

SPECULAR GLOSS AT 75 DEGREES, IN GLOSS UNITS - HIGH RANGE  
TAPPI OFFICIAL TEST METHOD T480 GS-78, SPECULAR GLOSS OF PAPER AND PAPERBOARD AT 75 DEGREES

LAB CODE	SAMPLE B80 COATED OFFSET BOOK 75 GRAMS PER SQUARE METER					SAMPLE E51 COATED BOOK 118 GRAMS PER SQUARE METER					TEST D <sub>0</sub> = 10		
	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L108	62.8	1.8	.91	2.3	1.35	69.0	1.1	.55	.7	.62	75B	Ø	L108
L121	62.1	1.2	.58	2.0	1.18	66.1	-1.9	-.97	.9	.77	75B	Ø	L121
L122	61.1	.1	.07	1.6	.96	68.0	-.0	-.00	1.3	1.14	75B	Ø	L122
L132	62.7	1.7	.66	1.9	1.12	71.3	3.3	1.72	1.0	.86	75G	Ø	L132
L189	60.3	-.6	-.29	1.1	.63	66.0	.1	.04	.9	.78	75F	Ø	L189
L190C	57.4	-3.5	-1.74	2.8	1.63	63.3	-4.7	-2.43	1.6	1.43	75G	Ø	L190C
L190R	63.6	2.7	1.32	1.7	.99	69.2	1.3	.66	1.2	1.01	75G	Ø	L190R
L206	62.6	1.6	.81	2.1	1.21	68.7	.8	.41	1.1	.94	75B	Ø	L206
L210	65.2	4.2	2.10	1.7	.97	72.0	4.1	2.12	1.1	.99	75B	Ø	L210
L211	58.7	-2.3	-1.11	1.7	1.01	66.6	-1.4	-.73	.9	.78	75B	Ø	L211
L230	60.9	-.0	-.02	1.0	.60	68.3	.3	.16	1.1	.93	75B	Ø	L230
L243	60.8	-.1	-.07	1.9	1.09	67.9	-.1	-.03	1.5	1.33	75B	Ø	L243
L251	56.8	-4.1	-2.02	2.1	1.23	66.7	-1.2	-.63	1.0	.90	75G	*	L251
L253P	62.3	1.3	.66	1.0	.57	68.1	.2	.09	1.0	.84	75G	Ø	L253P
L255	63.7	2.8	1.39	1.5	.85	70.7	2.7	1.42	1.3	1.13	75G	Ø	L255
L256	64.0	3.0	1.49	2.6	1.45	71.2	3.2	1.65	1.1	.95	75B	Ø	L256
L262	61.2	.3	.13	1.1	.66	70.6	2.6	1.37	1.3	1.11	75K	Ø	L262
L277A	61.1	.2	.08	2.6	1.54	69.5	1.5	.80	1.1	.94	75B	Ø	L277A
L277B	61.7	.8	.38	1.8	1.06	69.4	1.4	.75	1.1	.94	75B	Ø	L277B
L278	57.6	-3.3	-1.64	1.3	.73	66.9	-1.1	-.57	1.3	1.09	75G	Ø	L278
L279	61.8	.9	.43	2.4	1.39	66.6	-1.4	-.71	1.0	.84	75G	Ø	L279
L291	62.5	1.6	.78	1.9	1.12	69.3	1.4	.71	.6	.55	75B	Ø	L291
L317	61.5	.6	.28	.8	.49	68.5	.5	.28	.7	.62	75B	Ø	L317
L321	60.8	-.1	-.07	.6	.37	67.7	-.3	-.14	3.8	3.30	75G	Ø	L321
L323	56.2	-4.8	-2.35	2.2	1.27	64.6	-3.4	-1.75	1.1	.98	75B	Ø	L323
L339	55.2	-5.7	-2.83	3.9	2.27	59.8	-8.2	-4.25	4.3	3.80	75P	#	L339
L349	61.9	1.0	.50	1.7	1.00	68.6	.7	.35	.9	.75	75B	Ø	L349
L388	57.2	-3.7	-1.84	2.0	1.15	64.5	-3.5	-1.80	1.8	1.54	75P	Ø	L388
L483	61.9	1.0	.50	1.7	.99	67.5	-.4	-.22	.9	.75	75B	Ø	L483
L564	59.5	-1.4	-.71	.7	.41	67.9	-.1	-.03	1.1	.96	75P	Ø	L564
L573	60.1	-.8	-.41	1.4	.84	67.3	-.7	-.35	1.2	1.01	75G	Ø	L573
L574	60.7	-.2	-.12	1.6	.95	66.6	-1.4	-.71	.8	.74	75B	Ø	L574
L583	62.3	1.4	.68	1.5	.89	69.7	1.7	.89	1.2	1.04	75B	Ø	L583
L592	60.8	-.2	-.08	2.1	1.25	67.7	-.3	-.14	.8	.74	75B	Ø	L592
L598	58.2	-2.8	-1.37	1.4	.80	65.8	-2.1	-1.12	1.2	1.03	75B	Ø	L598
L643	60.2	-.7	-.34	2.0	1.15	66.6	-1.3	-.69	.9	.77	75B	Ø	L643
L654	63.0	2.1	1.04	1.7	.98	70.4	2.4	1.27	1.1	.98	75B	Ø	L654
L668	59.1	-1.8	-.88	1.3	.75	66.7	-1.2	-.65	1.4	1.24	75G	Ø	L668
L670	61.6	.7	.33	1.9	1.05	68.9	1.0	.51	1.4	1.26	75B	Ø	L670
L697	60.8	-.2	-.08	2.1	1.20	67.9	-.1	-.05	.8	.74	75B	Ø	L697
L704	60.6	-.3	-.14	1.5	.86	65.1	-2.8	-1.47	.7	.58	75P	Ø	L704
L738	60.8	-.1	-.06	2.4	1.40	66.8	-1.2	-.61	1.1	.95	75B	Ø	L738

GR<sub>0</sub> MEAN = 60.9 GLOSS UNITS      GRAND MEAN = 68.0 GLOSS UNITS      TEST DETERMINATIONS = 10  
SD MEANS = 2.0 GLOSS UNITS      SD OF MEANS = 1.9 GLOSS UNITS      41 LABS IN GRAND MEANS  
AVERAGE SDR = 1.7 GLOSS UNITS      AVERAGE SDR = 1.1 GLOSS UNITS

L250      60.4      -.5      -.26      2.2      1.26      66.8      -1.2      -.61      2.5      2.21      75G      \*      L250  
TOTAL NUMBER OF LABORATORIES REPORTING = 43

Best values: B80 61 ± 4 gloss units  
E51 68 ± 3 gloss units


The following laboratories were omitted from the grand means because of extreme test results: 339

SPECULAR GLOSS AT 75 DEGREES, IN GLOSS UNITS - HIGH RANGE  
TAPPI OFFICIAL TEST METHOD T480 CS-78, SPECULAR GLOSS CP PAPER AND PAPERBOARD AT 75 DEGREES

LAB CODE	F	MEANS		COORDINATES		AVG R <sub>s</sub> SDR VAR	PROPERTY---TEST INSTRUMENT---	CONDITIONS
		B80	E51	MAJOR	MINOR			
L339	#	55.2	59.8	-9.8	-2.0	3.03 75P	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, PHOTOVOLTI
L323	Ø	56.2	64.6	-5.8	.8	1.13 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L251	*	56.8	66.7	-3.8	1.9	1.07 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L388	Ø	57.2	64.5	-5.1	.0	1.37 75P	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, PHOTOVOLTI
L190C	Ø	57.4	63.3	-5.8	-1.0	1.53 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L278	Ø	57.6	66.9	-3.2	1.5	.91 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L598	Ø	58.2	65.8	-3.5	.3	.92 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L211	Ø	58.7	66.6	-2.6	.5	.89 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L668	Ø	59.1	66.7	-2.2	.3	.99 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L564	Ø	59.5	67.9	-1.1	.9	.69 75P	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, PHOTOVOLTI
L573	Ø	60.1	67.3	-1.1	.1	.93 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L643	Ø	60.2	66.6	-1.4	-.5	.96 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L189	Ø	60.3	68.0	-.4	.5	.71 75P	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, PHOTOVOLTI
L250	*	60.4	66.8	-1.2	-.5	1.74 75Q	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, PHOTOVOLTI, 20C, 65MRH
L704	Ø	60.6	65.1	-2.1	-1.9	.72 75P	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, PHOTOVOLTI
L574	Ø	60.7	66.6	-1.1	-.8	.84 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L592	Ø	60.8	67.7	-.3	-.1	.99 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L697	Ø	60.8	67.9	-.2	.0	.97 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L243	Ø	60.8	67.9	-.1	.0	1.21 75B	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, BAUSCH + LOMB
L321	Ø	60.8	67.7	-.3	-.1	1.83 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L738	Ø	60.8	66.8	-.9	-.8	1.17 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L230	Ø	60.9	68.3	.2	.2	.77 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L122	Ø	61.1	68.0	.1	-.1	1.05 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L277A	Ø	61.1	69.5	1.2	1.0	1.24 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L262	Ø	61.2	70.6	2.0	1.7	.88 75K	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GAERTNER (K-C TYPE)
L317	Ø	61.5	68.5	.8	.0	.56 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L670	Ø	61.6	68.9	1.2	.3	1.17 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L277B	Ø	61.7	69.4	1.5	.5	1.00 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L279	Ø	61.8	66.6	-.3	-1.6	1.12 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L349	Ø	61.9	68.6	1.2	-.2	.88 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L483	Ø	61.9	67.5	.5	-1.0	.87 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L121	Ø	62.1	66.1	-.4	-2.2	.97 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L253P	Ø	62.3	68.1	1.1	-.8	.70 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L583	Ø	62.3	69.7	2.2	.3	.96 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L291	Ø	62.5	69.3	2.1	-.1	.84 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L206	Ø	62.6	68.7	1.7	-.5	1.08 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L132	Ø	62.7	71.3	3.5	1.2	.99 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L108	Ø	62.8	69.0	2.1	-.5	.98 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L654	Ø	63.0	70.4	3.2	.3	.98 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L190R	Ø	63.6	69.2	2.8	-.9	1.00 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L255	Ø	63.7	70.7	3.9	.1	.99 75G	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, GARDNER
L256	Ø	64.0	71.2	4.4	.3	1.22 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
L210	Ø	65.2	72.0	5.9	.1	.98 75H	SPECULAR	GLOSS, 75 DEGREE, 50-95 UNITS, HUNTER
GMEANS:		60.9	68.0			1.00		
		95% ELLIPSE:		6.8	2.2	WITH GAMMA = 43 DEGREES		

# SPECULAR GLOSS, 75 DEGREE-HIGH RANGE

SAMPLE B80 = 60.9 GLOSS UNITS    SAMPLE E51 = 68.0 GLOSS UNITS

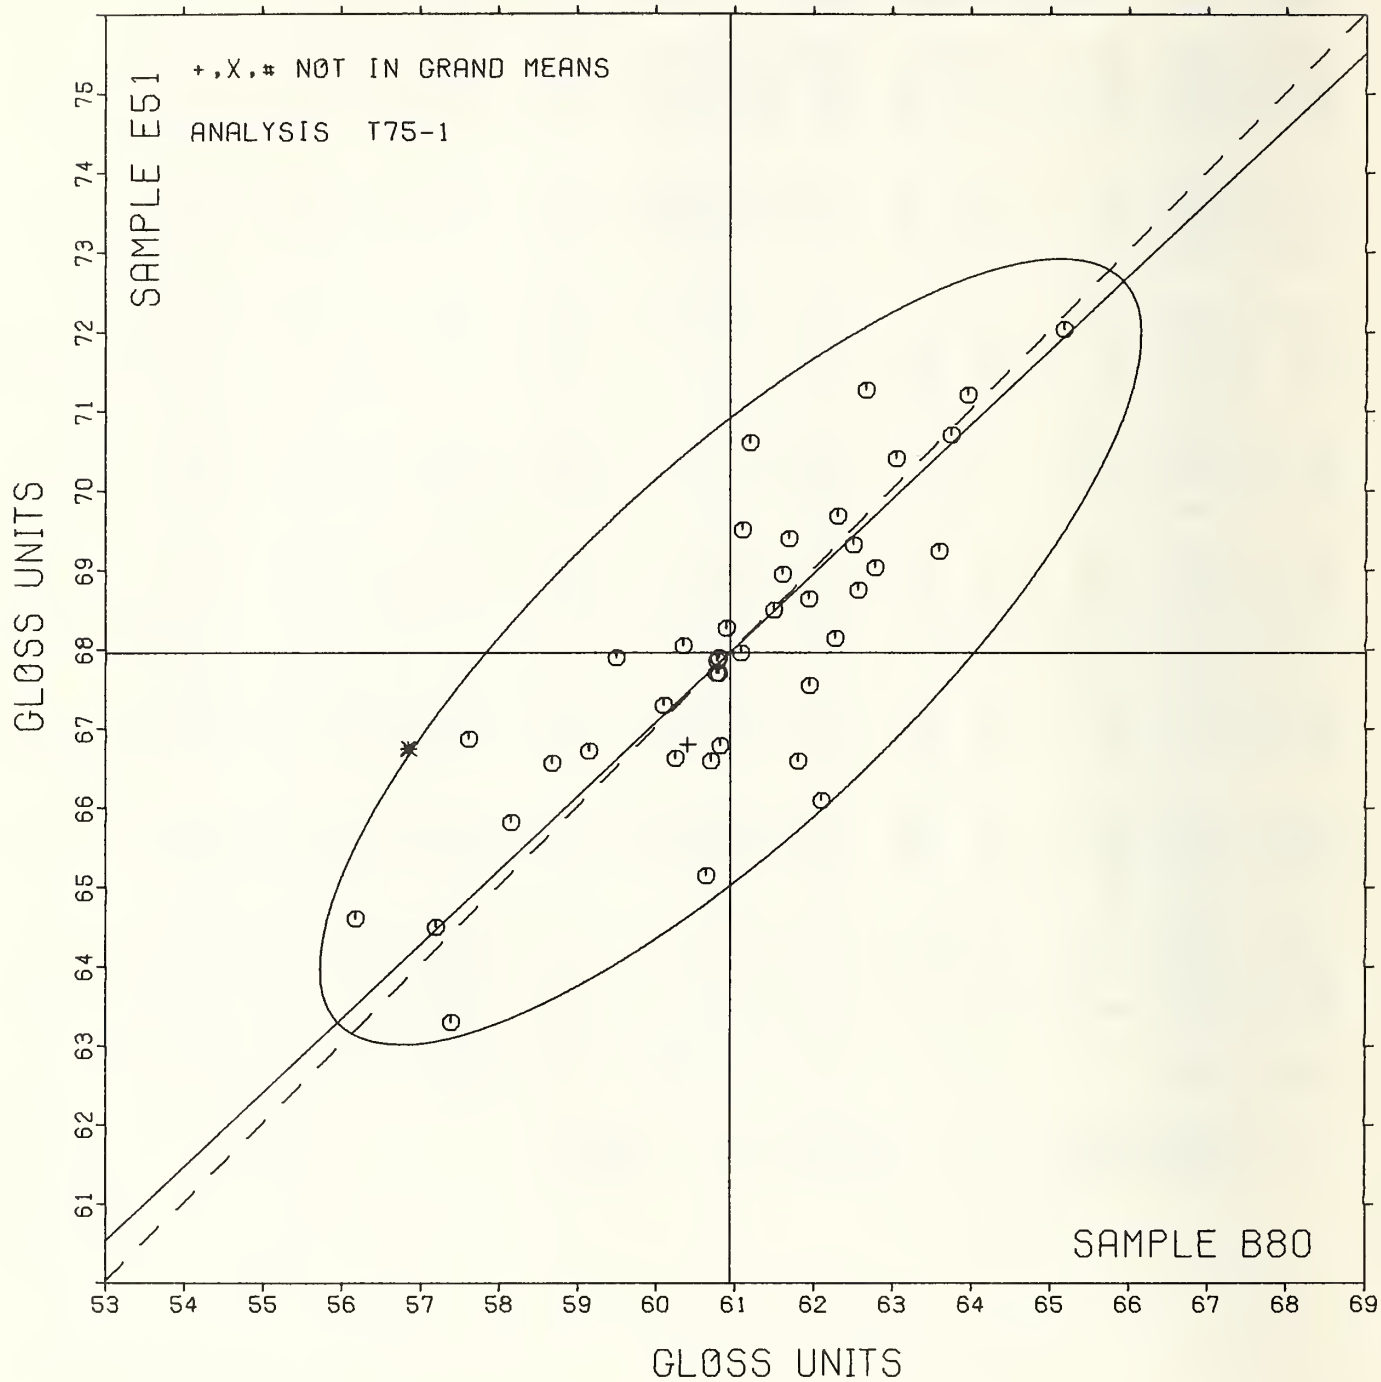






SPECULAR GLOSS, 75 DEGREE-LOW RANGE

SAMPLE G23 = 16.4 GLOSS UNITS      SAMPLE B47 = 47.8 GLOSS UNITS

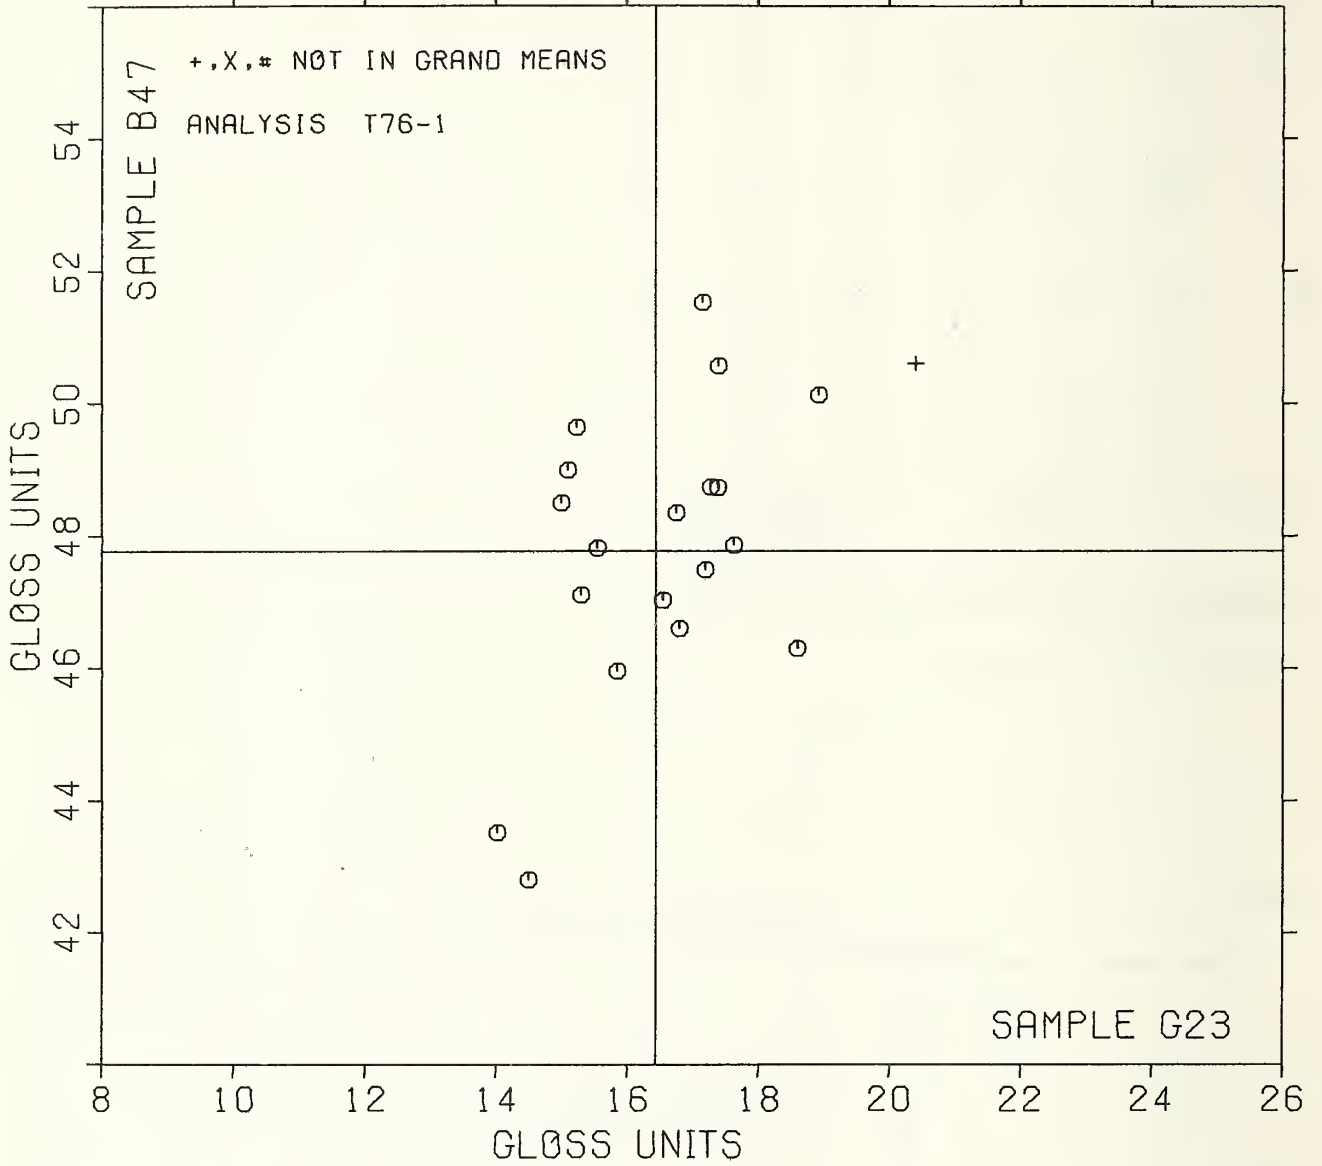

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS 190-1 TABLE 1  
THICKNESS (CALIPER), THOUSANDTHS OF AN INCH  
TAPPI OFFICIAL TEST METHOD T411 GS-76

LAB CODE	SAMPLE A88 MEAN	BLEACHED PAPER				SAMPLE G31 MEAN	KRAFT ENVELOPE				TEST D <sub>0</sub> = 10		
		82 GRAMS PER SQUARE METER	DEV	N <sub>0</sub> DEV	SDR		123 GRAMS PER SQUARE METER	DEV	N <sub>0</sub> DEV	SDR	VAR	F	LAB
L105	5.230	-.043	-.50	.026	.43	7.049	-.019	-.16	.043	.75	90Q	0	L105
L118	5.252	-.021	-.24	.053	.82	7.101	.033	.29	.047	.82	90Q	0	L118
L122	5.321	.048	.56	.079	1.31	7.238	.170	1.48	.060	1.05	90V	0	L122
L123F	5.495	.222	2.57	.069	1.14	7.355	.287	2.49	.060	1.05	90F	*	L123F
L125	5.200	-.073	-.84	.067	1.11	6.880	-.188	-1.63	.063	1.10	90T	0	L125
L128	5.328	.055	.64	.052	.86	7.052	-.016	-.14	.043	.76	90T	0	L128
L141	5.275	.002	.02	.063	1.06	7.085	.017	.15	.041	.72	90T	0	L141
L153	5.247	-.026	-.30	.065	1.09	6.983	-.085	-.74	.065	1.14	90T	0	L153
L158	5.270	-.003	-.03	.067	1.12	7.070	.002	.02	.082	1.44	90T	0	L158
L159	5.265	-.008	-.09	.071	1.18	7.200	.132	1.15	.082	1.43	90T	0	L159
L162	5.360	.087	1.01	.065	1.09	7.220	.152	1.32	.058	1.01	90V	0	L162
L166	5.311	.036	.44	.029	.48	7.095	.027	.24	.048	.84	90T	0	L166
L173B	5.270	-.003	-.03	.048	.80	7.070	.002	.02	.048	.84	90F	0	L173B
L174	5.280	.007	.08	.063	1.05	7.160	.092	.80	.070	1.22	90T	0	L174
L182	5.315	.042	.49	.071	1.18	7.080	.012	.11	.042	.73	90L	0	L182
L183	5.286	.013	.15	.056	.93	7.053	-.015	-.13	.057	1.00	90T	0	L183
L190C	5.120	-.153	-1.77	.063	1.05	6.830	-.238	-2.06	.082	1.44	90T	0	L190C
L212	5.332	.055	.68	.064	1.07	7.115	.047	.41	.048	.84	90T	0	L212
L213	5.270	-.003	-.03	.048	.80	7.080	.012	.11	.042	.74	90T	0	L213
L223	5.248	-.025	-.29	.075	1.25	7.064	-.004	-.03	.021	.36	90V	0	L223
L228	5.342	.069	.80	.040	.67	7.126	.058	.50	.057	1.00	90T	0	L228
L233	5.326	.053	.61	.049	.82	7.131	.063	.55	.052	.91	90Q	0	L233
L238A	5.314	.041	.47	.058	.97	7.043	-.025	-.22	.068	1.19	90T	0	L238A
L241	5.220	-.053	-.61	.048	.80	6.980	-.088	-.76	.109	1.85	90T	0	L241
L242B	5.256	-.017	-.20	.070	1.17	7.001	-.066	-.58	.059	1.03	90E	0	L242B
L242P	5.201	-.072	-.83	.059	.98	7.033	-.035	-.30	.033	.58	90P	0	L242P
L249	5.249	-.024	-.28	.081	1.36	7.007	-.061	-.53	.060	1.04	90T	0	L249
L259	5.383	.110	1.27	.090	1.49	7.194	.126	1.09	.046	.79	90Q	0	L259
L260	5.117	-.156	-1.80	.058	.97	6.977	-.091	-.79	.041	.71	90T	0	L260
L261	5.341	.068	.75	.050	.84	7.137	.069	.60	.065	1.13	90T	0	L261
L262	5.300	.027	.31	.033	.56	6.940	-.128	-1.11	.061	1.07	90T	0	L262
L285	5.443	.170	1.57	.035	.58	7.146	.078	.68	.047	.82	90T	*	L285
L291	5.222	-.051	-.55	.051	.85	6.956	-.112	-.97	.044	.77	90T	0	L291
L305	5.260	-.013	-.15	.052	.86	7.090	.022	.15	.032	.55	90T	0	L305
L309	5.280	.007	.08	.079	1.31	7.060	-.008	-.07	.052	.90	90T	0	L309
L315	5.345	.072	.83	.117	1.94	7.255	.187	1.62	.109	1.91	90T	0	L315
L318	5.139	-.134	-1.55	.074	1.24	7.066	-.002	-.02	.040	.69	90T	*	L318
L320	5.365	.092	1.06	.058	.97	7.135	.067	.58	.063	1.09	90T	0	L320
L323	5.330	.057	.66	.048	.80	7.230	.162	1.41	.067	1.18	90T	0	L323
L324	5.200	-.073	-.84	.047	.79	6.970	-.098	-.85	.067	1.18	90T	0	L324
L326	5.335	.062	.72	.078	1.31	7.115	.047	.41	.047	.83	90T	0	L326
L328	5.240	-.033	-.38	.047	.79	7.059	-.009	-.08	.049	.86	90T	0	L328
L333	5.143	-.130	-1.50	.036	.60	6.969	-.099	-.86	.052	.91	90V	0	L333
L339	5.143	-.130	-1.50	.057	.94	6.916	-.152	-1.31	.045	.79	90T	0	L339
L341	5.365	.092	1.06	.041	.68	7.168	.100	.87	.030	.52	90T	0	L341
L352	5.175	-.098	-1.13	.108	1.80	6.957	-.111	-.96	.110	1.92	90Q	0	L352
L356	1.324	-3.949	-45.64	.018	.30	1.765	-5.303	-46.00	.013	.22	90T	#	L356
L358	5.191	-.082	-.95	.045	.76	6.952	-.116	-1.01	.042	.73	90T	0	L358
L376	5.170	-.103	-1.19	.125	2.09	6.860	-.208	-1.80	.070	1.22	90T	0	L376
L380	5.310	.037	.43	.057	.95	7.000	-.068	-.55	.000	.00	90T	0	L380
L382	5.280	.007	.08	.042	.70	7.135	.067	.58	.082	1.43	90T	0	L382
L442	5.515	.242	2.80	.059	.98	7.365	.297	2.58	.054	.94	90V	*	L442
L554	5.270	-.003	-.03	.026	.43	7.030	-.038	-.33	.035	.61	90D	0	L554
L556	5.275	.002	.02	.057	.96	7.099	.031	.27	.053	.92	90T	0	L556
L567	5.198	-.075	-.87	.104	1.73	7.069	.001	.01	.143	2.50	90V	0	L567
L571	5.270	-.003	-.03	.082	1.37	7.150	.082	.71	.118	2.06	90V	0	L571
L574	5.140	-.133	-1.54	.055	.92	6.866	-.202	-1.75	.044	.77	90V	0	L574
L575	5.333	.060	.69	.051	.86	7.092	.024	.21	.042	.74	90T	0	L575
L576	5.299	.026	.30	.077	1.29	7.167	.095	.86	.052	.90	90T	0	L576
L581	5.330	.057	.66	.059	.98	7.145	.077	.67	.037	.64	90T	0	L581
L626	5.058	-.215	-2.48	.068	1.14	6.818	-.250	-2.17	.030	.52	90T	0	L626
L693	5.195	-.078	-.50	.049	.81	6.956	-.112	-.97	.050	.87	90T	0	L693
L704	5.205	-.068	-.79	.037	.61	6.890	-.178	-1.54	.074	1.29	90T	0	L704
L713	5.382	.105	1.26	.038	.64	7.218	.150	1.30	.053	.92	90T	0	L713
L737	5.340	.067	.77	.046	.77	7.090	.022	.15	.052	.90	90T	0	L737

GP. MEAN = 5.273 MILS  
SD MEANS = .087 MILS

GRAND MEAN = 7.068 MILS  
SD OF MEANS = .115 MILS

TEST DETERMINATIONS = 10  
64 LABS IN GRAND MEANS

AVERAGE SDR = .060 MILS  
GR. MEAN = 133.93 MICROMETER

AVERAGE SDR = .057 MILS  
GRAND MEAN = 179.52 MICROMETER



TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T90-1 TABLE 1  
THICKNESS (CALIPER), THOUSANDTHS OF AN INCH  
TAPPI OFFICIAL TEST METHOD T411 GS-76

LAB CODE	SAMPLE A88	BLEACHED BAG 82 GRAMS PER SQUARE METER				SAMPLE G31	KRAFT ENVELOPE 123 GRAMS PER SQUARE METER				TEST D <sub>0</sub> = 10		
	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	MEAN	DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L100	5.370	.097	1.12	.068	1.14	7.206	.138	1.20	.055	.96	90B	*	L100
L106	5.060	-.212	-2.46	.052	.86	6.990	-.078	-.68	.032	.55	90C	*	L106
L108	5.170	-.103	-1.19	.048	.80	7.000	-.068	-.59	.062	1.43	90C	*	L108
L134	5.369	.096	1.11	.059	.98	7.094	.026	.23	.030	.53	90X	*	L134
L185	5.360	.087	1.01	.052	.86	7.260	.192	1.67	.084	1.47	90Z	*	L185
L243	5.416	.143	1.65	.055	.91	7.088	.020	.17	.047	.83	90S	*	L243
L251	5.299	.026	.30	.038	.64	7.088	.020	.18	.063	1.10	90W	*	L251
L342	5.200	-.073	-.84	.051	.85	6.927	-.141	-1.22	.026	.45	90U	*	L342
L484	4.898	-.375	-4.34	.046	.77	6.744	-.324	-2.81	.032	.57	90E	*	L484
L563	5.400	.127	1.47	.082	1.36	7.200	.132	1.15	.094	1.65	90T	*	L563
L616	5.070	-.203	-2.35	.082	1.37	7.010	-.058	-.50	.032	.55	90C	*	L616
L684	5.300	.027	.31	.000	.00	7.050	-.018	-.16	.053	.92	90U	*	L684
L702	5.090	-.183	-2.11	.032	.53	7.030	-.038	-.33	.067	1.18	90X	*	L702
L706	5.290	.017	.20	.074	1.23	7.070	.002	.02	.067	1.18	90X	*	L706
L731	5.327	.054	.62	.071	1.19	7.080	.012	.11	.019	.33	90A	*	L731
TOTAL NUMBER OF LABORATORIES REPORTING = 80													

Best values: A88 5.27 ± 0.14 mils  
G31 7.07 ± 0.20 mils

Data from the following laboratories appear to be off by a multiplicative factor: 356



TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS 190-1 TABLE 2  
THICKNESS (CALIPER), THOUSANTHS OF AN INCH  
TAPPI OFFICIAL TEST METHOD 1411 GS-76

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		A88	G31	MAJOR	MINOR	R <sub>0</sub>	SDR VAR			
L356	#	1.324	1.765	-6.610	.147	.26	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L484	*	4.898	6.744	-.481	.118	.67	90E	THICKNESS (CALIPER),	SCHOPPER,	HAND DRIVEN
L626	Ø	5.058	6.818	-.328	.030	.83	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L106	*	5.060	6.990	-.187	.128	.71	90C	THICKNESS (CALIPER),	CADY,	HAND DRIVEN
L616	*	5.070	7.010	-.165	.132	.96	90C	THICKNESS (CALIPER),	CADY,	HAND DRIVEN
L702	*	5.090	7.030	-.137	.127	.85	90X	THICKNESS (CALIPER):	GIVE INSTR. MAKE+MODEL.(	MOTOR,( )HAND
L260	Ø	5.117	6.977	-.164	.074	.84	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L190C	Ø	5.120	6.830	-.283	-.013	1.25	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L316	*	5.139	7.066	-.079	.108	.97	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L574	Ø	5.140	6.866	-.242	-.009	.84	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN,DIGITIZED
L339	Ø	5.143	6.916	-.199	.016	.87	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L333	Ø	5.143	6.969	-.156	.049	.76	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN,DIGITIZED
L108	*	5.170	7.000	-.115	.045	1.12	90C	THICKNESS (CALIPER),	CADY,	HAND DRIVEN
L376	Ø	5.170	6.860	-.229	-.036	1.65	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L352	Ø	5.175	6.957	-.147	.016	1.86	90Q	THICKNESS (CALIPER),	EMVECO,	MOTOR DRIVEN
L358	Ø	5.191	6.952	-.142	-.000	.74	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L693	Ø	5.195	6.956	-.136	-.001	.84	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L567	Ø	5.198	7.069	-.043	.062	2.11	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN,DIGITIZED
L125	Ø	5.200	6.880	-.195	-.049	1.11	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L342	*	5.200	6.927	-.157	-.022	.65	90U	THICKNESS (CALIPER),	TMI,	HAND DRIVEN
L324	Ø	5.200	6.970	-.122	.003	.98	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L242P	Ø	5.201	7.033	-.070	.039	.78	90P	THICKNESS (CALIPER),	MESSMER,	MOTOR DRIVEN, ISO R534
L704	Ø	5.205	6.890	-.184	-.048	.95	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L241	Ø	5.220	6.980	-.102	-.008	1.35	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L291	Ø	5.222	6.956	-.121	-.023	.81	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L105	Ø	5.230	7.049	-.040	.024	.59	90Q	THICKNESS (CALIPER),	EMVECO,	MOTOR DRIVEN
L328	Ø	5.240	7.059	-.026	.022	.82	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L153	Ø	5.247	6.983	-.084	-.028	1.11	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L223	Ø	5.248	7.064	-.018	.018	.80	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN,DIGITIZED
L249	Ø	5.249	7.007	-.064	-.016	1.20	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L118	Ø	5.252	7.101	.015	.036	.85	90Q	THICKNESS (CALIPER),	EMVECO,	MOTOR DRIVEN
L242Ø	Ø	5.256	7.001	-.064	-.025	1.10	90Ø	THICKNESS (CALIPER),	MESSMER,	MOTOR DRIVEN, HS3963
L305	Ø	5.260	7.090	.011	.023	.71	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L159	Ø	5.265	7.200	.103	.083	1.30	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L213	Ø	5.270	7.080	.008	.009	.77	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L173B	Ø	5.270	7.070	.000	.004	.82	90F	THICKNESS (CALIPER),	FEDERAL,	MOTOR DRIVEN
L571	Ø	5.270	7.150	.065	.050	1.71	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN,DIGITIZED
L158	Ø	5.270	7.070	.000	.004	1.28	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L554	Ø	5.270	7.030	-.033	-.020	.52	90D	THICKNESS (CALIPER),	CADY,	MOTOR DRIVEN
L141	Ø	5.275	7.085	.015	.008	.89	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L556	Ø	5.275	7.099	.027	.016	.64	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L382	Ø	5.280	7.135	.059	.033	1.07	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L174	Ø	5.280	7.160	.079	.048	1.14	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L309	Ø	5.280	7.060	-.002	-.010	1.11	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L183	Ø	5.286	7.053	-.005	-.019	.97	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L706	*	5.290	7.070	.012	-.013	1.20	90X	THICKNESS (CALIPER):	GIVE INSTR. MAKE+MODEL.(	MOTOR,( )HAND
L576	Ø	5.299	7.167	.096	.036	1.10	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L251	*	5.299	7.088	.032	-.010	.87	90W	THICKNESS (CALIPER),	L + W,	MOTOR DRIVEN, 20 C, 65% RB
L262	Ø	5.300	6.940	-.089	-.096	.81	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L684	*	5.300	7.050	.001	-.032	.46	90U	THICKNESS (CALIPER),	TMI,	HAND DRIVEN
L380	Ø	5.310	7.000	-.034	-.070	.47	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L166	Ø	5.311	7.095	.044	-.015	.66	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L238A	Ø	5.314	7.043	.003	-.048	1.08	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L182	Ø	5.315	7.080	.034	-.027	.95	90I	THICKNESS (CALIPER),	L + W,	MOTOR DRIVEN
L122	Ø	5.321	7.238	.167	.059	1.18	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN,DIGITIZED
L233	Ø	5.326	7.131	.082	-.007	.86	90Q	THICKNESS (CALIPER),	EMVECO,	MOTOR DRIVEN
L1731	*	5.327	7.080	.041	-.037	.76	90A	THICKNESS (CALIPER),	L + W,	HAND DRIVEN
L128	Ø	5.328	7.052	.019	-.054	.81	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L323	Ø	5.330	7.230	.165	.047	.99	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L581	Ø	5.330	7.145	.096	-.002	.81	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L212	Ø	5.332	7.115	.073	-.021	.96	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L575	Ø	5.333	7.052	.054	-.035	.80	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L326	Ø	5.335	7.115	.074	-.023	1.07	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L737	Ø	5.340	7.090	.057	-.042	.83	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L261	Ø	5.341	7.137	.096	-.015	.98	90I	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS 190-1 TABLE 2  
THICKNESS (CALIPER), THOUSANDTHS OF AN INCH  
TAPPI OFFICIAL TEST METHOD T411 GS-7C

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---	TEST INSTRUMENT---	CONDITIONS
		A88	G31	MAJOR	MINOR	R <sub>s</sub>	SDR VAR			
L228	Ø	5.342	7.126	.087	-.023	.84	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L315	Ø	5.345	7.255	.194	.050	1.92	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L162	Ø	5.360	7.220	.174	.017	1.05	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN, DIGITIZED
L185	*	5.360	7.260	.207	.040	1.17	90B	THICKNESS (CALIPER),	AMTHER,	HAND DRIVEN
L320	Ø	5.365	7.135	.108	-.036	1.03	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L341	Ø	5.365	7.168	.135	-.017	.60	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L134	*	5.369	7.094	.077	-.063	.75	90X	THICKNESS (CALIPER):	GIVE INSTR. MAKE+MODEL.	(MOTOR, (HAND
L100	*	5.370	7.206	.169	.001	1.05	90B	THICKNESS (CALIPER),	AMTHER,	HAND DRIVEN
L713	Ø	5.382	7.218	.186	-.002	.78	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L259	Ø	5.383	7.194	.167	-.017	1.14	90Q	THICKNESS (CALIPER),	EMVECO,	MOTOR DRIVEN
L563	*	5.400	7.200	.181	-.027	1.50	90U	THICKNESS (CALIPER),	TMI,	HAND DRIVEN
L243	*	5.416	7.086	.099	-.105	.87	90S	THICKNESS (CALIPER),	SCROPPER,	HAND DRIVEN
L285	*	5.443	7.146	.162	-.053	.70	90T	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN
L123F	*	5.495	7.355	.363	-.015	1.09	90F	THICKNESS (CALIPER),	FEDERAL,	MOTOR DRIVEN
L442	*	5.515	7.365	.382	-.025	.96	90V	THICKNESS (CALIPER),	TMI,	MOTOR DRIVEN, DIGITIZED
GMEANS:		5.273	7.068			1.00				
		95% ELLIPSE:		.350	.100	WITH GAMMA = 54 DEGREES				


# THICKNESS (CALIPER)

SAMPLE A88 = 5.27 MILS

SAMPLE G31 = 7.07 MILS

SAMPLE A88 = 133.9 MICRØMETER

SAMPLE G31 = 179.5 MICRØMETER

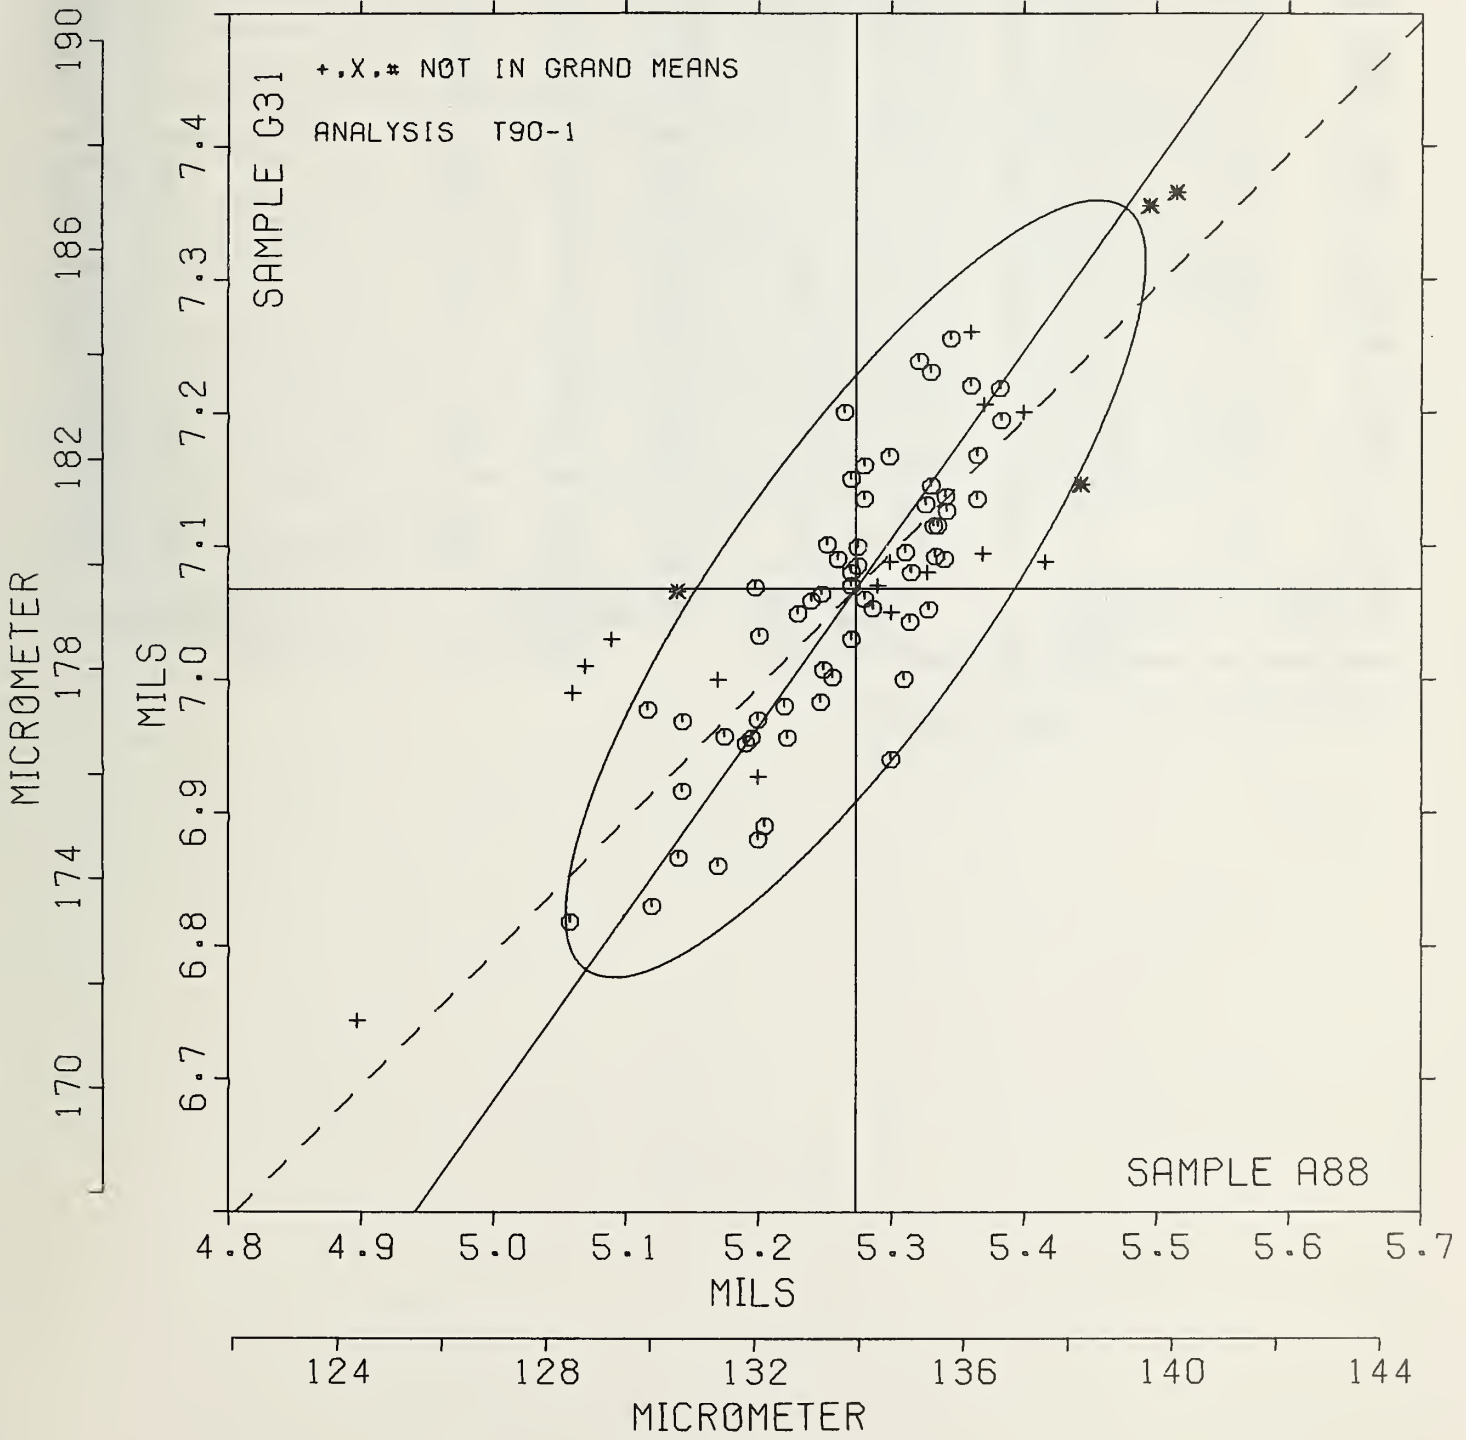

TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS T95-1 TABLE 1  
GRAMMAGE (MASS PER UNIT AREA)  
TAPPI OFFICIAL TEST METHOD T410 OS-79

LAB CODE	SAMPLE D37 MEAN	BUFF MANILA ENVELOPE 112 GRAMS PER SQUARE METER				SAMPLE D38 MEAN	KRAFT 124 GRAMS PER SQUARE METER				TEST D <sub>0</sub> = 10		
		DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR		DEV	N <sub>0</sub> DEV	SDR	R <sub>0</sub> SDR	VAR	F	LAB
L100	117.0	-0.3	-0.28	2.5	1.64	124.5	.4	.34	1.2	1.16	95C	Ø	L100
L121	116.8	-0.5	-0.51	1.7	1.09	123.2	-1.0	-0.89	1.1	1.09	95B	Ø	L121
L162	117.0	-0.3	-0.28	.7	.47	123.6	-0.5	-0.48	.5	.54	95K	Ø	L162
L213	117.4	.2	.18	1.2	.78	124.4	.3	.29	1.0	1.01	95F	Ø	L213
L233	117.8	.6	.58	1.4	.93	123.8	-0.3	-0.27	2.1	2.06	95T	Ø	L233
L244	117.3	-0.0	-0.01	1.1	.72	123.5	-0.6	-0.56	.6	.60	95T	Ø	L244
L249	118.0	.7	.73	2.0	1.29	124.5	.4	.39	.9	.84	95I	Ø	L249
L280	117.8	.5	.56	2.0	1.31	124.9	.8	.71	.6	.56	95T	Ø	L280
L285	115.1	-2.1	-2.24	.6	.38	122.4	-1.7	-1.58	.5	.49	95T	Ø	L285
L305	117.4	.1	.15	.9	.59	125.2	1.6	1.50	.5	.48	95T	Ø	L305
L339	115.9	-1.3	-1.39	.6	.39	122.5	-1.6	-1.44	.0	.00	95T	Ø	L339
L442	117.7	.4	.42	1.3	.84	124.7	.5	.49	.3	.28	95K	Ø	L442
L484	118.0	.7	.77	2.2	1.46	124.6	.5	.43	1.1	1.05	95B	Ø	L484
L564	116.5	-0.2	-0.81	2.0	1.29	125.2	1.1	.98	.9	.90	95E	Ø	L564
L567	116.9	-0.3	-0.35	1.8	1.21	123.0	-1.2	-1.06	.9	.92	95E	Ø	L567
L571	118.1	.2	.27	2.6	1.74	123.6	-0.5	-0.48	1.6	1.62	95P	Ø	L571
L574	116.7	-0.6	-0.60	2.0	1.34	124.6	.5	.41	1.1	1.03	95D	Ø	L574
L604	115.3	-2.0	-2.11	1.5	1.02	122.6	-1.5	-1.42	.8	.77	95T	Ø	L604
L616	117.9	.7	.72	1.5	.98	125.0	.9	.84	.9	.85	95T	Ø	L616
L626	117.6	.3	.35	1.3	.87	124.1	-0.0	-0.04	.7	.70	95E	Ø	L626
L693	119.4	2.1	2.24	.5	.36	127.0	2.9	2.63	1.4	1.39	95G	Ø	L693
L704	117.5	.2	.24	1.8	1.20	123.9	-0.2	-0.22	3.3	3.19	95T	Ø	L704
L731	118.0	.7	.77	1.7	1.12	123.5	-0.6	-0.57	1.5	1.48	95X	Ø	L731

GR<sub>C</sub> MEAN = 117.3 G/SQ.METER                      GRAND MEAN = 124.1 G/SQ.METER                      TEST DETERMINATIONS = 10  
SD MEANS = 1.0 G/SQ.METER                      SD OF MEANS = 1.1 G/SQ.METER                      23 LABS IN GRAND MEANS  
AVERAGE SDR = 1.5 G/SQ.METER                      AVERAGE SDR = 1.0 G/SQ.METER  
TOTAL NUMBER OF LABORATORIES REPORTING = 23

Best values: D37 117.3 ± 2.0 grams per square meter  
D38 124.1 ± 1.7 grams per square meter



TAPPI COLLABORATIVE REFERENCE PROGRAM  
ANALYSIS 195-1 TABLE 2  
GRAMMAGE (MASS PER UNIT AREA)  
TAPPI OFFICIAL TEST METHOD T410 G8-79

LAB CODE	F	MEANS		COORDINATES		AVG		PROPERTY---TEST INSTRUMENT---CONDITIONS
		D37	D38	MAJCE	MINCR	R, SDR	VAR	
L285	Ø	115.1	122.4	-2.7	.6	.44	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L604	Ø	115.3	122.6	-2.5	.6	.89	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L339	Ø	115.9	122.5	-2.1	.0	.20	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L564	Ø	116.5	125.2	.3	1.3	1.10	95E	BASIS WEIGHT (GRAMMAGE), GUILLIOTINE TYPE CUTTER
L574	Ø	116.7	124.6	-0.0	.7	1.19	95D	BASIS WEIGHT (GRAMMAGE), DIE CUT
L121	Ø	116.8	123.2	-1.1	-0.2	1.09	95B	BASIS WEIGHT (GRAMMAGE), CENCEFA CUTTER
L567	Ø	116.9	123.0	-1.1	-0.5	1.06	95E	BASIS WEIGHT (GRAMMAGE), GUILLIOTINE TYPE CUTTER
L162	Ø	117.0	123.6	-0.6	-0.1	.50	95K	BASIS WEIGHT (GRAMMAGE), WEIGHED AS RECEIVED
L100	Ø	117.0	124.5	.1	.4	1.40	95C	BASIS WEIGHT (GRAMMAGE), CUTTING BOARD
L244	Ø	117.3	123.5	-0.5	-0.4	.66	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L305	Ø	117.4	125.8	1.4	.9	.53	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L213	Ø	117.4	124.4	.4	.1	.89	95F	BASIS WEIGHT (GRAMMAGE), FOUR-SQUARE CUTTER
L704	Ø	117.5	123.9	-0.0	-0.3	2.20	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L626	Ø	117.6	124.1	.2	-0.3	.79	95E	BASIS WEIGHT (GRAMMAGE), GUILLIOTINE TYPE CUTTER
L442	Ø	117.7	124.7	.7	.0	.56	95K	BASIS WEIGHT (GRAMMAGE), WEIGHED AS RECEIVED
L280	Ø	117.8	124.9	.9	.1	.93	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L233	Ø	117.8	123.8	.1	-0.6	1.49	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L616	Ø	117.9	125.0	1.1	.1	.92	95T	BASIS WEIGHT (GRAMMAGE), TEMPLATE CUT
L249	Ø	118.0	124.5	.8	-0.3	1.07	95I	BASIS WEIGHT (GRAMMAGE), INGENTIC PAPER CUTTER
L731	Ø	118.0	123.5	-0.0	-1.0	1.30	95X	BASIS WEIGHT (GRAMMAGE): SHEET CUT BY WHAT DEVICE?
L484	Ø	118.0	124.6	.8	-0.3	1.25	95B	BASIS WEIGHT (GRAMMAGE), SQUARE AND BLADE
L571	Ø	118.1	123.6	.1	-1.0	1.68	95P	BASIS WEIGHT (GRAMMAGE), PRODUCTION REAM CUTTER
L693	Ø	119.4	127.0	3.6	.2	.87	95G	BASIS WEIGHT (GRAMMAGE), PRECISION CUTTER
GMEANS:		117.3	124.1			1.00		
		95% ELLIPSE:		3.6	1.5	WITH GAMMA = 50 DEGREES		



## SUMMARY TABLE

TEST METHOD	SAMPLE CODE	GRAND MEAN	SD OF MEAN	AVER SDF	REPL CRP	LABS INCL	LABS PARTIC	REPL TAPPI	REPEAT	REFRCD
AIR RESISTANCE, GURLEY T40-1	B68	49.2	3.2	4.7	10	58	65	10	4.1	8.9
	Z08	95.8	7.9	8.9					7.8	21.8
AIR RESISTANCE, SHEFFIELD T40-2	B68	71.2	4.9	6.6	10	37	46	10	5.7	13.7
	Z08	36.2	3.1	3.0					2.6	8.5
AIR RESISTANCE, GURLEY BG FRICTION T41-1	E37	76.0	57.0	103.0	10	15	15	10	90.0	157.0
	B73	1284.0	253.0	534.0					467.0	701.0
SMOOTHNESS, PARKER PRINTSURF T44-1	A84	5.683	.248	.085	10	6	7	10	.074	.687
	A83	4.566	.196	.174					.152	.542
SMOOTHNESS, SHEFFIELD T45-1	A84	227.8	10.3	8.2	15	90	92	10	7.2	28.8
	A83	107.5	9.5	11.4					10.0	27.0
SMOOTHNESS, BEKK T45-2	A84	13.05	.92	.84	15	10	12	5	1.04	2.67
	A83	54.93	7.36	9.25					11.46	22.43
SMOOTHNESS, BENDTSEN T47-1	A84	34.0	27.0	25.0	10	11	11	10	22.0	76.0
	A83	112.0	21.0	15.0					13.0	59.0
MOISTURE T53-1	E66	6.08	.56	.14	10	11	14	2	.28	1.57
	G32	5.56	.43	.18					.35	1.24
K & N INK ABSORPTION T56-1	E44	29.6	4.1	.6	4	10	10	2	1.3	11.4
	G03	57.5	6.2	.6					1.2	17.2
OPACITY, B&L, 89% BACKING, FINE P. T60-1	G22	85.70	.73	.97	10	62	78	5	1.20	2.20
	G26	88.25	.73	.96					1.19	2.19
OPACITY, EIREPHO, PAPER BACKING, FINE P. T60-2	G22	86.93	.43	.91	10	15	20	5	1.12	1.44
	G26	90.23	.44	.74					.92	1.38
OPACITY, B&L, 89% BACKING, NEWS T61-1	B01	75.15	.90	.70	10	21	28	5	.86	2.56
	A56	78.84	1.10	.92					1.14	3.14
BLUE REFLECTANCE, DIRECTIONAL T65-1	J34	67.20	.47	.20	8	24	56	5	.24	1.30
	J38	75.94	.48	.17					.20	1.33
BLUE REFLECTANCE, DIFFUSE, WITH TRAP T65-2	J34	66.38	.43	.16	8	13	18	5	.20	1.20
	J38	74.93	.37	.13					.16	1.04
BLUE REFLECTANCE, DIFFUSE, NO TRAP T65-3	J34	67.87	.41	.12	8	12	14	5	.15	1.13
	J38	76.69	.55	.09					.12	1.62
SPECULAR GLOSS, 75 DEGREE-HIGH RANGE T75-1	B80	60.9	2.0	1.7	10	41	43	5	2.1	5.8
	E51	68.0	1.9	1.1					1.4	5.4
SPECULAR GLOSS, 75 DEGREE-LOW RANGE T76-1	G23	16.4	1.4	1.6	10	19	20	5	1.9	4.0
	B47	47.8	2.2	1.8					2.3	6.3
THICKNESS (CALIPER) T90-1	A88	5.273	.087	.060	10	64	80	10	.053	.240
	G31	7.066	.115	.057					.050	.319
GPANNAGE (MASS PER UNIT AREA) T95-1	D37	117.3	1.0	1.5	10	23	23	3	2.4	3.3
	D38	124.1	1.1	1.0					1.6	3.3

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. TAPPI CRP 63G	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE Technical Association of the Pulp and Paper Industry COLLABORATIVE REFERENCE PROGRAM FOR PAPER Report #63G		5. Publication Date June 13, 1980	
7. AUTHOR(S) R.G. Powell, J. Horlick		8. Performing Organ. Report No. NSSIR-80-1833	
9. PERFORMING ORGANIZATION NAME AND ADDRESS NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, DC 20234		10. Project/Task/Work Unit No.	
12. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS (Street, City, State, ZIP) Collaborative Testing Services, Inc. 8343-A Greensboro Dirve, McLean, VA 22102 and Technical Association of the Pulp and Paper Industry		13. Type of Report & Period Covered Final	
15. SUPPLEMENTARY NOTES  <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.		14. Sponsoring Agency Code	
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.)  Collaborative Reference Programs provide participating laboratories with the means for checking periodically the level and uniformity of their testing in comparison with that of other participating laboratories. An important by-product of the programs is the provision of realistic pictures of the state of the testing art. This is one of the periodic reports showing averages for each participant, within and between laboratory variability, and other information for participants and standards committees.			
17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons) Collaborative reference program; Laboratory evaluation; Paper; Precision; Reference samples; Testing calibration			
18. AVAILABILITY <input type="checkbox"/> Unlimited <input checked="" type="checkbox"/> For Official Distribution. Do Not Release to NTIS  <input type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office, Washington, DC 20402, SD Stock No. SN003-003-  <input type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA, 22161		19. SECURITY CLASS (THIS REPORT) UNCLASSIFIED	21. NO. OF PRINTED PAGES 61
		20. SECURITY CLASS (THIS PAGE) UNCLASSIFIED	22. Price





