

NATIONAL BUREAU OF STANDARDS REPORT

3064

OPTICAL SPECTROSCOPIC DETERMINATION OF HYDROGEN ISOTOPES IN AQUEOUS MIXTURES

by

H.P.Broida, H.J.Morowitz and M.Selgin

Progress Report
to
Veterans Administration
and
Atomic Energy Commission



**U. S. DEPARTMENT OF COMMERCE
NATIONAL BUREAU OF STANDARDS**

U. S. DEPARTMENT OF COMMERCE

Sinclair Weeks, Secretary

NATIONAL BUREAU OF STANDARDS

A. V. Astin, Director



THE NATIONAL BUREAU OF STANDARDS

The scope of activities of the National Bureau of Standards is suggested in the following listing of the divisions and sections engaged in technical work. In general, each section is engaged in specialized research, development, and engineering in the field indicated by its title. A brief description of the activities, and of the resultant reports and publications, appears on the inside of the back cover of this report.

Electricity. Resistance Measurements. Inductance and Capacitance. Electrical Instruments. Magnetic Measurements. Applied Electricity. Electrochemistry.

Optics and Metrology. Photometry and Colorimetry. Optical Instruments. Photographic Technology. Length. Gage.

Heat and Power. Temperature Measurements. Thermodynamics. Cryogenics. Engines and Lubrication. Engine Fuels. Cryogenic Engineering.

Atomic and Radiation Physics. Spectroscopy. Radiometry. Mass Spectrometry. Solid State Physics. Electron Physics. Atomic Physics. Neutron Measurements. Infrared Spectroscopy. Nuclear Physics. Radioactivity. X-Rays. Betatron. Nucleonic Instrumentation. Radio-logical Equipment. Atomic Energy Commission Instruments Branch.

Chemistry. Organic Coatings. Surface Chemistry. Organic Chemistry. Analytical Chemistry. Inorganic Chemistry. Electrodeposition. Gas Chemistry. Physical Chemistry. Thermochemistry. Spectrochemistry. Pure Substances.

Mechanics. Sound. Mechanical Instruments. Aerodynamics. Engineering Mechanics. Hydraulics. Mass. Capacity, Density, and Fluid Meters.

Organic and Fibrous Materials. Rubber. Textiles. Paper. Leather. Testing and Specifications. Polymer Structure. Organic Plastics. Dental Research.

Metallurgy. Thermal Metallurgy. Chemical Metallurgy. Mechanical Metallurgy. Corrosion.

Mineral Products. Porcelain and Pottery. Glass. Refractories. Enameled Metals. Concrete Materials. Constitution and Microstructure. Chemistry of Mineral Products.

Building Technology. Structural Engineering. Fire Protection. Heating and Air Conditioning. Floor, Roof, and Wall Coverings. Codes and Specifications.

Applied Mathematics. Numerical Analysis. Computation. Statistical Engineering. Machine Development.

Electronics. Engineering Electronics. Electron Tubes. Electronic Computers. Electronic Instrumentation.

Radio Propagation. Upper Atmosphere Research. Ionospheric Research. Regular Propagation Services. Frequency Utilization Research. Tropospheric Propagation Research. High Frequency Standards. Microwave Standards.

Ordnance Development. These three divisions are engaged in a broad program of research and development in advanced ordnance. Activities include basic and applied research, engineering, pilot production, field testing, and evaluation of a wide variety of ordnance matériel. Special skills and facilities of other NBS divisions also contribute to this program. The activity is sponsored by the Department of Defense.

Electromechanical Ordnance. and development in advanced ordnance. Activities include basic and applied research, engineering, pilot production, field testing, and evaluation of a wide variety of ordnance matériel. Special skills and facilities of other NBS divisions also contribute to this program. The activity is sponsored by the Department of Defense.

● Office of Basic Instrumentation

● Office of Weights and Measures.

FOREWORD

The present report covers the completion of phases of the projects involving studies of the accuracy and limitations of the general optical spectroscopic method of determining hydrogen isotope ratios in aqueous solutions. It also contains a summary of some of the results of the use of this method for measurements with blood. Although part of this work was supported by the Veterans Administration and part by The Atomic Energy Commission, the results are interrelated and thus a joint report has been issued. Later, it is intended to publish this report in the Journal of Research, National Bureau of Standards.

A. V. Astin
Director


F. G. Brickwedde, Chief
Heat and Power Division

OPTICAL SPECTROSCOPIC DETERMINATION OF HYDROGEN ISOTOPES IN AQUEOUS MIXTURES

by

H. P. Broida, H.J.Morowitz* and M.Selgin

ABSTRACT

Extension of the optical spectroscopic method for isotope analysis of gaseous mixtures of hydrogen and deuterium to mixtures of water and heavy water provides a direct method for determining total water content of materials. A determination can be made on a sample of less than 0.1 ml in less than 10 minutes to an accuracy of a few percent. Using a sample of at least 1 ml, an accuracy of the order of 0.1 percent is obtained in an hour or less. This paper describes the system and the investigation of optimum operating conditions and effect of variations in operating conditions on precision and accuracy of measurement as well as limitations of the technique. A sample of blood or serum can be measured directly almost as easily as one of distilled water. The optical spectroscopic method can be used to determine water content of most materials whether in the solid, liquid or gas phase.

1. INTRODUCTION

Following initial work on an optical spectroscopic analysis of gaseous mixtures of hydrogen and deuterium [1,2]¹ a similar technique was tried with mixtures of water and heavy water. A preliminary study [3] indicated that it was possible to carry out such analyses to an accuracy of better than 3 percent. The work discussed in this paper represents a detailed extension of the preliminary study in an effort to extend both the precision and the range and to determine present limitations of the analysis. A detailed study was made to determine the influence of operating variables on precision and accuracy of measurement in order to find the optimum operating conditions. In these studies the

¹Figures in brackets indicate the literature references at the end of this report.

*Present address - National Heart Institute, National Institutes of Health, Bethesda, Maryland.

following accuracy was obtained: (a) .1 percent of the intensity ratio, in the isotope ratio range .01 to 1.0; (b) 1 percent, in the range .00015 to .01 (see table 5).

In addition the rather practical problems of developing the method into a routine analytical technique were taken into consideration. For this reason efforts were made to achieve a rapid analysis, and operating conditions were viewed with the possibility of constructing a simple flow system and optical system for routine use. Several types of routine measurements were made concurrently with the study of the technique.

The technique used is as follows. The vapor from an aqueous sample containing a mixture of H_2O and D_2O is pumped through a tube where a high frequency electrodeless discharge is maintained. The light emitted from the discharge tube contains lines of the Balmer series of hydrogen and deuterium with a very small amount of background radiation. The emitted light is dispersed by a monochromator and the relative intensities of the β lines of the Balmer series of hydrogen and deuterium are recorded and measured. The ratio of the intensities of the two lines is a monotonic function of the relative concentration of the isotopes and to a high degree of accuracy is equal to the ratio of the isotope concentrations. For precise work the measurement is a relative rather than an absolute one in that the relationship between intensity ratio and concentration ratio is obtained from calibration curves taken on standard samples whose compositions are determined by independent measurements.

The statistical terms [4, 5] used in this report are defined as follows. Precision refers to the variation encountered during readings taken in close succession under identical conditions. Reproducibility refers to the variation among readings when they are spread over a considerable time period. It is not a fixed quantity but depends somewhat on the time interval and the history of the apparatus in that interval. Accuracy refers to the variation of the measured concentration from the true value and is determined from the precision and reproducibility of the measurements and from the accuracy of the calibrated samples. The relationship between reproducibility and time determines how frequently it is necessary to take calibration points. These factors are all dependent on the stability of operating conditions.

The above variations are expressed either as standard deviation or as the coefficient of variation. These terms apply either for single measurements or for averages. Since the standard deviation of the average is dependent on the number of readings taken,

this value is most useful when compared to other sets of the same number of readings. For the purposes of this study, all standard deviations of the average refer to sets of 10 readings.

Stability of this system may be viewed in the following manner. Consider the measured ratio of intensities of the D_i Balmer line to the H_i Balmer line at 4860.0 Å and 4861.3 Å, respectively, and represent this ratio by D_i/H_i . This ratio is a function of a large number of variables such as the actual concentration ratio D/H in the sample, the temperature, the pressure, the flow rate, etc., and may be represented in the following fashion:

$$D_i/H_i = D/H f(D/H, X_1, X_2 \dots X_M)$$

where X_i are independent variables. In practice, operating conditions are found such that f is very nearly unity.


A completely stable set of operating conditions is one in which D_i/H_i is a function of D/H only and unaffected by small changes of $X_1, X_2 \dots X_M$. From a practical point of view the conditions of stability are that changes of D_i/H_i due to variations of the X_i are small compared with changes due to variations of D/H . Many of the experimental curves shown in the following sections are graphs of the ratio D_i/H_i as a function of one of the independent variables with all other variables kept as constant as possible.

The samples employed in these experiments are in all cases aqueous solutions or suspensions in which the solvent is a mixture of hydrogen oxide H_2O and deuterium oxide D_2O . The number used to describe concentrations is, unless otherwise specified, the atom ratio of deuterium to hydrogen, D/H . This figure depends only upon the number of atoms of hydrogen and deuterium in the sample and is independent of the equilibrium between H_2O , HDO and D_2O .

In taking measurements of isotope ratios the vapor is pumped from the liquid through the discharge tube. This procedure raises two questions; what is the relationship between D/H in the liquid and the vapor and what fractionation (isotope separation) occurs in the flow process? The first question is purely academic with respect to the analysis of water. A given ratio of D to H in the liquid will always give rise to a reproducible ratio in the vapor and since all measurements are taken relative to calibration samples the measurement taken is in all cases referred back to the liquid.

Owing to the difference in vapor pressure between H₂O, HDO and D₂O the process of evaporating liquid from samples involves some degree of fractional distillation. This has been investigated experimentally to study the overall effect and will be discussed in a later section.

The processes occurring in the breakdown of water vapor in the radio frequency field are imperfectly understood and will be discussed only briefly. The discharge through the water vapor in the tube causes excitation, ionization and dissociation giving rise to the following atoms and molecules from a mixture of normal and heavy water:



as well as other groupings, most of which may exist as normal, excited, or ionized molecules. The emission spectrum from the discharge contains lines and bands from many of these components. The Balmer lines of hydrogen and deuterium are prominent in this spectrum.

The β line of the Balmer series was chosen because the largest output signal was obtained for this line. This is a result of the product of the actual intensity and the phototube sensitivity being a maximum in the region of the β Balmer line of the hydrogen spectrum. The α lines at 6561.0 Å and 6562.8 Å for D and H, respectively, also can be used; this pair has the advantage of a somewhat larger separation than the β pair (1.8 Å compared to 1.3 Å).

2. EQUIPMENT

2.1 Glass Flow System

A glass flow system was employed to provide a steady flow of sample vapor through the discharge tube. A flow system decreases problems of contamination by previous samples and simplifies the preparation of the sample for analysis. The system, shown photographically in figure 1 and schematically in figure 2, consists of the following components:

(1) Sample bottles.- The sample bottles are equipped with an inverted standard taper ground glass joint so that rapid change of samples can be made.

(2) Sample connectors.- The connectors are standard taper ground glass joints corresponding to those on the bottles. A special vacuum line (figure 2) provides a means of evacuating the air from the sample chamber before admitting sample into the main flow system.

(3) Pressure regulator.- In order to vary and control pressure in the discharge tube a parallel network is provided consisting of a capillary and a continuously variable metal leak valve. In most of the studies described in this paper, the variable metal leak valve was used because fine pressure control and frequent adjustments were necessary. However, for routine measurements a fixed non-metallic orifice is preferable.

(4) Pressure gauge.- To measure pressure in the system, a pressure line connects through stopcocks to various critical locations. Pressure measurement is made by means of a commercial ionization gauge, which utilizes alpha particles from a radium source to provide ionization. The gauge can be used from pressures of 1 micron to 1 centimeter.

(5) Discharge tube.- The discharge tube consists of a glass inner cylinder surrounded by a glass water jacket. Water flows through the jacket at a constant rate controlled by a regulator at the tap. Air bubbles in the water, which might affect intensity measurements, are eliminated by an extractor shown at point G in figure 1.

(6) Pumps.- The two main vacuum lines shown in figure 2 connect with independent pumping systems. The left hand line goes to a trap, single stage oil diffusion pump and forepump while the right hand line goes only to a trap and mechanical pump. The diffusion pump was used in these investigations because a wide variation in conditions was to be studied.

2.2 High Frequency Source

The energy necessary to excite the spectrum of the sample was provided by a commercial 150 megacycle 150 watt oscillator. The energy is carried through a radio frequency cable which terminates in a tunable quarter-wavelength tank circuit with antennae held near the discharge tube. This terminal circuit is shown diagrammatically in figure 2. A radio frequency shield (point J in figure 1) cuts down stray radiation which might affect other electronic equipment.

2.3 Monochromator

The apparatus used to analyze the spectrum consists of a high resolution grating monochromator with a photomultiplier detector and associated amplifier and recorder². A detailed discussion of the original monochromator is given by Fastie [6].

The plane diffraction grating used in the monochromator is 3 by 3 inches and is ruled with 30,000 lines per inch; the instrument has a practical resolving power ($\lambda/\Delta\lambda$) of 55,000. This resolution is sufficient to observe some of the fine structure splitting of H_{α} and D_{α} lines. The choice of optimum resolving power is governed by two considerations: it must be sufficient to resolve the lines to be analyzed and at the same time be low enough to allow for the integrated intensity of a line to be approximated by the peak height of that line. The resolving power was varied by varying the width of the entrance and exit slits until the β line of deuterium could be resolved in a normal water discharge ($D/H = .00015$) [7]. Figure 3 shows the H, D, and H ghost lines resolved and indicates, on the basis of the half width of the line, a resolving power of 20,000. This resolving power proved suitable for subsequent studies.

The first Rowland ghost of the β line of hydrogen was spaced about 2.0 Å from the line and was approximately 1/500 as intense. The β line of deuterium appears between the H line and its first ghost. The ratio of ghost intensity to line intensity is a function of the optics of the system only, and under conditions of fixed optics may be taken as a constant. For low deuterium concentrations the ratio between the deuterium line and the H ghost is a fixed multiple of the ratio between the D and H lines. This fact proves useful in allowing comparison to be made between signals taken at the same scale of amplification, the calibration in this range being independent of the ratio of amplification for different scales.

2.4 Power Supply, Amplifier and Recorder

A chopper before the entrance slit of the monochromator converts the input signal to 60 cps. This signal is fed into a narrow band-pass synchronous amplifier, the output of which is recorded by

²This equipment was on field trial loan to the National Bureau of Standards from the Research Division of the Leeds and Northrup Company.

a pen on ten-inch chart paper. The recorder has a response time of one second. The power supply for the photomultiplier is continuously variable from 500 to 1300 volts. By using the photomultiplier with a sensitive linear a-c amplifier which has an accurate amplification factor ranging from 2 to 800, very small signals can be observed.

3. EXPERIMENTAL RESULTS

The primary purpose of this study was to determine the effects of numerous interrelated variables on the speed, accuracy and sensitivity of the method. The variables include pressure in the flow system, flow rate, sample size, solute composition of the sample, temperature, and oscillator characteristics. These variables will be considered in detail. The percent change in ratio per unit change in variable was computed for each operating curve and can be used to determine how closely each variable must be controlled to achieve a desired precision (see table 7).

The methods of measuring intensity ratios for the 0-1 percent D_2O range and the 1-99 percent D_2O range are shown in figure 3. As previously discussed the deuterium to ghost ratio is used instead of the deuterium to hydrogen ratio in the 0-1 percent range. In the 1-99 percent range the D and H lines were measured directly at a lower amplification. In both concentration ranges the baseline, or background, is somewhat arbitrary and is taken at a fixed distance from the deuterium peak. This causes no error in the final measurement since the calibration is made in the same manner as the measurement.

3.1 Memory

The speed with which a measurement can be taken is largely dependent on the memory of the system: i.e. the time required to clean the system of one sample and saturate it with another so that a constant ratio is obtained. Metal parts are troublesome, but the metal leak valve usually was employed to gain fine pressure control in spite of its memory effect.

Figure 4 shows a series of experiments under extreme conditions in which a pure water sample was run and then switched to commercial heavy water. Curve a shows the effect, under the slowest conditions, of using the metal leak valve with no intermediate pumping or flushing. Curve b shows the effect of using a glass capillary tube and a glass stopcock for pressure control with no intermediate pumping or flushing. For routine measurement the capillary tube and stopcock were used under the following

conditions. The system was pumped with and without sample between extreme pressures in the ratio of at least 15 to 1. These changes were made rapidly for approximately 2 minutes and then the pressure was stabilized to 400 microns. The memory effect was thereby reduced to that shown in curve c.

These curves show that an all glass system with intermediate flushing produces the greatest reduction of the memory effect. Even with an extreme change in concentration, equilibrium is reached to within 1 percent in less than 3 minutes and complete equilibrium in approximately 1 hour. The flow system shown in figure 2 was designed for maximum variability, but for routine use a much simpler system is advantageous. Also the elimination of side projections should reduce the memory time.

3.2 Pressure

The operating pressure in the discharge tube has an effect on the intensity ratio, especially in the 0-1 percent D_2O range (see figure 5). Flow rate was not held constant so actually the traces show ratio vs a combination of pressure and flow rate at constant pumping speed as determined by settings of the metal leak valve and the speed of the pump. The flow rate in milligrams per minute decreased from 0.011 at a pressure of 900 microns to 0.0023 at 400 microns and 0.001 at 200 microns. The pressure gauge used had the disadvantage of large metal surfaces and considerable memory effect. Such memory is undesirable for measurements where the concentration is being changed frequently. Therefore the gauge was isolated from the system after initial pressure setting and during the course of most intensity ratio measurements. The disadvantage of not taking continuous pressure readings was overcome by utilizing the fact that the length of the discharge is a sensitive function of the pressure, it provided a good check on the constancy and reproducibility of pressure and flow conditions.

Intensity as a function of pressure was investigated at various concentrations and the results are shown in figure 6. The curves are quite similar at all concentrations. An operating pressure of approximately 400 microns was chosen for routine use because it makes use of maximum intensity and the flattest portion of the intensity vs pressure curve. It also occurs at regions of the ratio vs pressure curves that are reasonably flat. The percent change of ratio per unit change in pressure at 400 microns as computed from figure 5 is .020 percent per micron. This means that the pressure must be held to ± 5 microns to achieve a precision of ± 1 percent.

3.3 Fractionation

At 20°C there is a difference of 2.3 mm of mercury between the vapor pressure of H₂O and D₂O with HDO having an intermediate pressure [7]. Thus a sample which is being evaporated will begin to concentrate deuterium. To check on the error to be expected from this effect, a 0.5 ml sample was run continuously to dryness with frequent checks made on the D/H ratio. The results at an operating pressure of 200 microns are shown in figure 7. From this curve the minimum sample size can be computed for a given flow rate and allowable error. This is shown in detail in Section 5, Discussion.

3.4 Temperature

The ratio of the vapor pressure of H₂O, D₂O and HDO changes with temperature so that some error might be expected from variation of sample temperature. To study this effect sample bottles were immersed in a constant temperature bath during these determinations. Table 1 shows the results taken at temperatures ranging from 0.4° to 25.8°C. From this table the percent change in ratio per unit change in sample temperature was computed to be .15 percent per degree Centigrade.

TABLE 1. Intensity Ratio vs Sample Temperature

Sample No.	Temperature °C	Ratio D _i /H _i
S-4	4.0	0.3895
	25.8	.3965
S-9	0.4	0.0454
	3.0	.0452
	17.0	.0466
	22.0	.0470

Pressure = 500 microns

3.5 Flow-Rate

Flow rate affects the D/H ratio, the rate of fractionation, and the size of the smallest sample measurable. It is a function of pressure, the geometry of the flow system, and the speed of the pump. Table 2 gives data obtained for D_i/H_i ratio as a function of the flow rate at constant pressure. This table shows that D_i/H_i decreases with decreased flow-rate and indicates that at least part of the effect of change of pressure (figure 5) is caused by the reduced flow rate at lower pressures. The percent change of ratio per unit change of flowrate computed from table 2 is 0.5 percent per g/min.

TABLE 2. Intensity Ratio vs Flow-Rate

Flow (grams/min)	Ratio D_i/H_i
0.01125	0.899
.00983	.894
.00331	.857

Pressure = 400 microns

Flow-rate obtained by weighing sample before and after flow.

3.6 Oscillator and Discharge Characteristics

The discharge characteristics can be varied by changes in oscillator plate current, antenna tuning, position of electrodes with respect to the tube, and the temperature of the cooling stream in the jacket of the discharge tube. Plate current is variable between 100 ma and 200 ma and the tuning is adjusted by the tuning capacitor in figure 2 as well as by the position of the radio frequency shield and electrodes. The radio frequency

shield and electrodes were placed to obtain maximum intensity and the tuning capacitor varied to give a range of discharge lengths. Ratio of D_i/H_i as a function of discharge length is shown in table 3. The effect on D_i/H_i of changing the oscillator plate current is shown in table 4. It is seen that there is no appreciable effect of the discharge length or plate current on the measured ratio. The temperature of the cooling stream was varied by changing the water flow rate through the discharge tube jacket. D_i/H_i varied less than 1 percent over the extreme range of temperature from a stream of the coldest water available from the tap (approximately 18°C) to no cooling (greater than 200°C).

TABLE 3. Intensity Ratio vs Percent Maximum Discharge Length

Sample No.	Percent of Maximum Discharge Length	Ratio D_i/H_i
S-9	100	4.71
	88.6	4.78
	73.8	4.85
	49.4	4.48
S-12	100	49.74
	98	49.5
	91.8	49.71
	82.7	49.79
	75.1	49.97
	64.7	50.17
	52.0	50.04
	49.0	49.79

Pressure = 500 microns

TABLE 4. Intensity Ratio vs Oscillator Plate Current

Sample No.	Plate Current (ma)	Ratio D_i/H_i
S-9	100	0.0503
	122	.0499
	140	.0491
	175	.0491
	190	.0490
S-12	100	1.015
	125	1.016
	130	1.013
	150	1.015
	185	1.012
	200	1.012
	210	1.012

Pressure = 500 microns

3.7 Solute Composition

Since this method of analysis may be extended for use with many aqueous solutions, preliminary investigation was made of the variation of D_i/H_i ratio with the amount of solids dissolved in the sample. This test was made with NaCl. With concentrations of 0 percent, 1 percent, 10 percent and a saturated solution, no variation of D_i/H_i was found within the experimental error.

4. CALIBRATION CURVES, PRECISION AND REPRODUCIBILITY

Calibration curves were necessary to achieve the highest accuracy. Figure 8 shows the 0-1 percent D_2O range and figure 9 the 1-80 percent D_2O ³ range. Samples were made by mixing portions of distilled water and commercial D_2O (99.8%) which had been weighed to an accuracy of 0.1 mg.

³Calibration curves were taken on samples up to 99.8 percent D_2O (commercially available), but no extensive measurements were made in the high concentration range. The analysis in this range differs from that in the low range only in the method of preparing standard samples.

Table 5 gives examples of the isotope content expressed, for comparison, in ratio and in percent, and shows precisions obtained under optimum conditions.

TABLE 5. Comparison of Ratio Method and Percent Concentration Method of Expressing Isotope Content

Ratio (D/H)	Standard Deviation of Average of Ratio ¹	Coefficient of Variation of Average ²	Deuterium Concentration Expressed in Percent (D/D+H x 100)	Standard Deviation of Average of Concentration ¹	Coefficient of Variation of Average ²
500	5.0	1.0	99.8	0.002	0.002
100	0.1	0.1	99.0	.001	.001
10	.01	.1	90.9	.01	.01
1	.001	.1	50.0	.25	.05
.1	.0001	.1	9.09	.01	.01
.01	.00001	.1	0.99	.001	.1
.001	.000007	.7	.100	.0007	.7
.0001	.000002	2.0	.01	.0002	2.0

¹Based on a set of 10 readings.

²Standard deviation of average expressed in percent

Reproducibility was measured on a 21 percent D₂O sample and a 0.2 percent D₂O sample. Measurements were taken at varying time intervals and in some cases with major changes taking place during the interval, both in the apparatus and in the concentration ratios. Results are shown in figure 10 for four portions of the 21 percent sample. Each point shows the average of 10 readings with the precision depicted as vertical spread. The grand average is a solid

horizontal line and the standard deviation computed directly from all 21 averages is shown by dotted lines on either side of the grand average. Thus the relation between precision and reproducibility at this stage of development can be seen at a glance. The results obtained for the 0.2 percent sample were similar. Data for it are listed in table 6.

TABLE 6. Reproducibility of Intensity Ratio for a 0.2% D₂O Sample Over One Month. Each Ratio is the Average of 10 Readings.

Date	D _i /G _i *
April 28, 1953	0.760
May 1	.737
May 2	.736
May 4	.733
May 7	.729
May 7	.724
May 7	.744
May 8	.751
May 8	.743
May 11	.753
May 15	.740
May 18	.769
May 18	.754
May 19	.765
May 20	<u>.753</u>
Average	0.746

Pressure = 200 microns

* G_i is the measured intensity of the ghost of the H line

5. DISCUSSION

The great number of variables which influence the measurement of D/H ratios makes it impossible to be certain that the final operating conditions are in fact the optimum ones. Indeed, it is not necessary to assume that there is a unique set of optimum conditions for this analysis. The operating conditions chosen therefore are the "best set" based upon data available and the nature of the measurements to be performed. Some of the final data used to evaluate operating conditions are shown in table 7. This table illustrates that there is no extreme problem in keeping the operating conditions constant enough so that the measurement can be made within the desired accuracy.

TABLE 7. Operating Variables

Condition Varied	Percent change of ratio per unit change of variable	Routine Operating Conditions
Sample temperature	.15% per °C	room temperature
Pressure	.020% per micron	400 microns
Salt concentration	0% per mole/liter	any
Flow-rate	0.5 per g/min	depending on sample size and desired speed of measurement
Tuning	0% per % change in discharge length	maximum discharge length
Osc. Plate Current	0% per mA	175 mA
Discharge Tube Temp.	.005% per °C	room temperature

Accessory factors enter into the choice of best conditions. The fractionation curve (figure 7) can be represented as $RS^k = K$ where R is the isotope ratio, S is the sample size and k and K are experimental constants. In differential form the fractionation curve can be represented as

$$\frac{dR}{R} = -\frac{k}{S} dS$$

where the left hand side represents the percent change of ratio due to fractionation. Setting dR/R equal to e the maximum tolerable fractionation error and realizing that $dS = -f\Delta t$, the flow-rate times the time increment, we arrive at the following expression for minimum sample size:

$$S = \frac{.068 f\Delta t}{e}$$

The value of k, 0.068, was obtained from the data shown in figure 7. As has been mentioned previously, flow-rate depends on operating pressure, flow-geometry and pumping speed, while time of measurement depends on memory and time necessary for pressure equilibrium, so that sample size is some complex function of the major operating variables. Under normal conditions at 400 microns operating pressure the flow-rate was .0023 ml/min and the time per determination was 20 minutes. The minimum sample size is therefore $.00313/e$ or .3 ml for a 1 percent error. The absolute minimum sample size under present conditions involves an operating pressure of 200 microns and a maximum error of 3 percent. Under these conditions, a seven-minute measurement is possible and the minimum sample size is .02 ml.

The operating conditions which were found to be most suitable with the equipment described in this paper are shown in table 6.

This study is not exhaustive inasmuch as there are many combinations of variables which were not tried. In addition no attempt was made to vary systematically such things as the oscillator frequency or discharge tube geometry. A few preliminary experiments with a 2240 mc oscillator indicate that a stable set of operating conditions can be set up at that frequency.

As pointed out in the beginning of this paper, the chief object of these studies was to determine how to minimize error, sample size, and time of determination. Of course it is impossible to minimize all three factors at once. Highest precision requires many determinations per sample, hence a long time and large sample size. The minimum values attainable at the present stage of development and the maximum values obtained while minimizing the others are given as follows:

	<u>Minimum</u>	<u>Maximum</u>
Precision (coefficient of variation of the average)	.1 - 2%	3%
Sample Size	.02 ml	1 ml
Time per Sample	7 minutes	60 minutes

With respect to precision and time per determination the optical spectroscopic case compares favorably with other methods. It finds particular application where the water samples contain impurities. Whereas other methods require one or two stages of purification, the sample vapor can be analyzed directly by this method. This method appears to be considerably more rapid and, for similar accuracy, less expensive than other methods.

While it is not the function of this paper to discuss, in detail, applications of hydrogen-deuterium analysis, we shall review briefly in the following paragraphs some of the most important uses to which the optical spectroscopic method has been placed. The dilution technique for determining the total water content of materials involved in these uses is described in reference [3]. Essentially it consists of dissolving or suspending a known amount of the material to be analyzed in a mixture of D₂O and H₂O and then determining spectroscopically the resulting change in the ratio of D₂O to H₂O.

(1) Determination of D₂O content of blood. In this application the blood, serum or plasma is placed in the sample bottle and the vapor analyzed in the usual manner. No prior preparation of the blood is necessary and high precision is obtainable. This technique finds application in the determination of total body water by D₂O dilution and in the study of water exchange in capillary beds. Over 150 blood samples have been run and no difficulty has been encountered in adapting the techniques to routine analysis.

(2) Determination of water of hydration or water of crystallization. The crystal to be analyzed is dissolved in D_2O , and the final intensity ratio gives a measure of the H_2O originally present in the crystal. Several hydrates have been tried and results agree with other methods.

(3) Determination of labile hydrogen. A weighed quantity of dry material containing labile hydrogens is dissolved in D_2O and the resultant ratio measured. From the number of exchangeable hydrogen atoms per molecule, information about structure of the molecule is obtained.

The most extensive work has been done with blood for which a brief description of the routine application follows.

Army Medical Service gave injections of 100 gms of commercially pure D_2O to several hemorrhagic fever patients and sampled blood at various time intervals. The serum samples were analyzed at the National Bureau of Standards to determine the total body water content of the patients. 73 samples in the concentration range .029 percent to .425 percent gave precisions of the order of 0.7 percent coefficient of variation of the average. Ten readings were taken per sample using the metal leak valve for pressure control. Time per sample ranged between 25 and 55 minutes depending on stability of operating conditions.

Reference [8] gives details of a study of transcapillary exchange rates of D_2O and thiocyanate in the forearm of man. A study has since been made of the exchange rates from the artery of one arm to the vein of the other. In this case only 5 readings were taken per sample and metal parts were eliminated, thus cutting the total time per sample down to 15 minutes plus data calculation time. The precision of measurement was of the order of 1.5 percent coefficient of variation of the average for 17 samples in the concentration range .015 percent to 2.000 percent D_2O .

6. REFERENCES

- [1] H.P.Broida and J.W.Moyer, Spectroscopic analysis of deuterium in hydrogen-deuterium mixtures, JOSA 42, 37(1952).
- [2] H.P.Broida and G.H.Morgan, Optical spectrophotometric analysis of hydrogen-deuterium mixtures in presence of air, Anal. Chem. 24, 799(1952).
- [3] H.J.Morowitz and H.P.Broida, Rapid spectroscopic determination of total water content, Anal. Chem. 24, 1657 (1952).
- [4] W.J.Youden, Statistical method for chemists, (John Wiley and Sons, 1951).
- [5] A.S.T.M. Manual on Quality Control of Materials, A.S.T.M., Phila., Pa., Jan. 1951.
- [6] William G. Fastie, A small plane grating monochromator, JOSA 42, 641(1952).
- [7] I. Kirshenbaum, Physical properties and analysis of heavy water, p. 396 (McGraw-Hill 1951).
- [8] Edward D. Freis, Thomas F. Higgins and Harold J. Morowitz, Transcapillary exchange rates of deuterium oxide and thiocyanate in the forearm of man, J. Applied Physiology 5, 526 (1953).

7. LEGENDS FOR FIGURES

- Fig. 1. Flow System for H-D Analysis. Points indicated are:
A, Sample bottles. B, Sample connectors. C, Metal leak valve. D, Glass capillary. E, Pressure gauge.
F, Discharge tube. G, Bubble extractor. H, Trap.
J, Shield for high frequency source. K, Lens. L, Chopper.
M, Photomultiplier tube.
- Fig. 2. Schematic Diagram of Flow System.
- Fig. 3. Method of Measuring Intensities (H_i , D_i , G_i). Height of H line (H_i) is approximately 500 times that of H ghost line (G_i). The zero line is arbitrarily taken 6.6 A from the H line and intensities are measured as distances above the zero line. From left to right, traces are of 0.4 percent and 10 percent D_2O samples, respectively.
- Fig. 4. Memory Effect. Pressure = 400 microns.
a, Metal leak valve with no intermediate pumping or flushing between samples.
b, Glass stopcock with no intermediate pumping or flushing.
c, Glass stopcock with intermediate pumping and flushing.
- Fig. 5. Intensity Ratio vs Pressure. Seven samples at various concentrations. The calibrated concentration of each sample by weighing is given at end of each trace.
- Fig. 6. Total $H_{\beta} + D_{\beta}$ Intensity vs Pressure at various concentrations.
- Fig. 7. Fractionation Effect. Flow was continuous at .063 ml/hr. D_i/G_i scale is greatly expanded.
- Fig. 8. Calibration Curve for 0-1% D_2O Concentration Range. Samples were made up by weighing.
- Fig. 9. Calibration Curve for 1-80% D_2O Concentration Range. 80-99 percent portion of the curve is omitted because of the extended scale. Samples were made up by weighing.
- Fig. 10. Precision and Reporducibility for 21% D_2O samples. Readings were taken on 4 identical samples over 3 months. Times of taking data are, from left to right, as follows:

<u>Sample Number</u>	<u>Date</u>
S-28	Dec. 9, 1952
	Dec. 9, 1952
	Dec. 23, 1952
S-29	Dec. 1, 1952
	Dec. 1, 1952
	Dec. 2, 1952
	Dec. 2, 1952
	Dec. 3, 1952
	Dec. 3, 1952
	Dec. 4, 1952
	Dec. 5, 1952
	Dec. 22, 1952
	Feb. 25, 1953
S-30	Dec. 4, 1952
	Dec. 4, 1952
	Dec. 23, 1952
S-31	Dec. 19, 1952
	Dec. 19, 1952

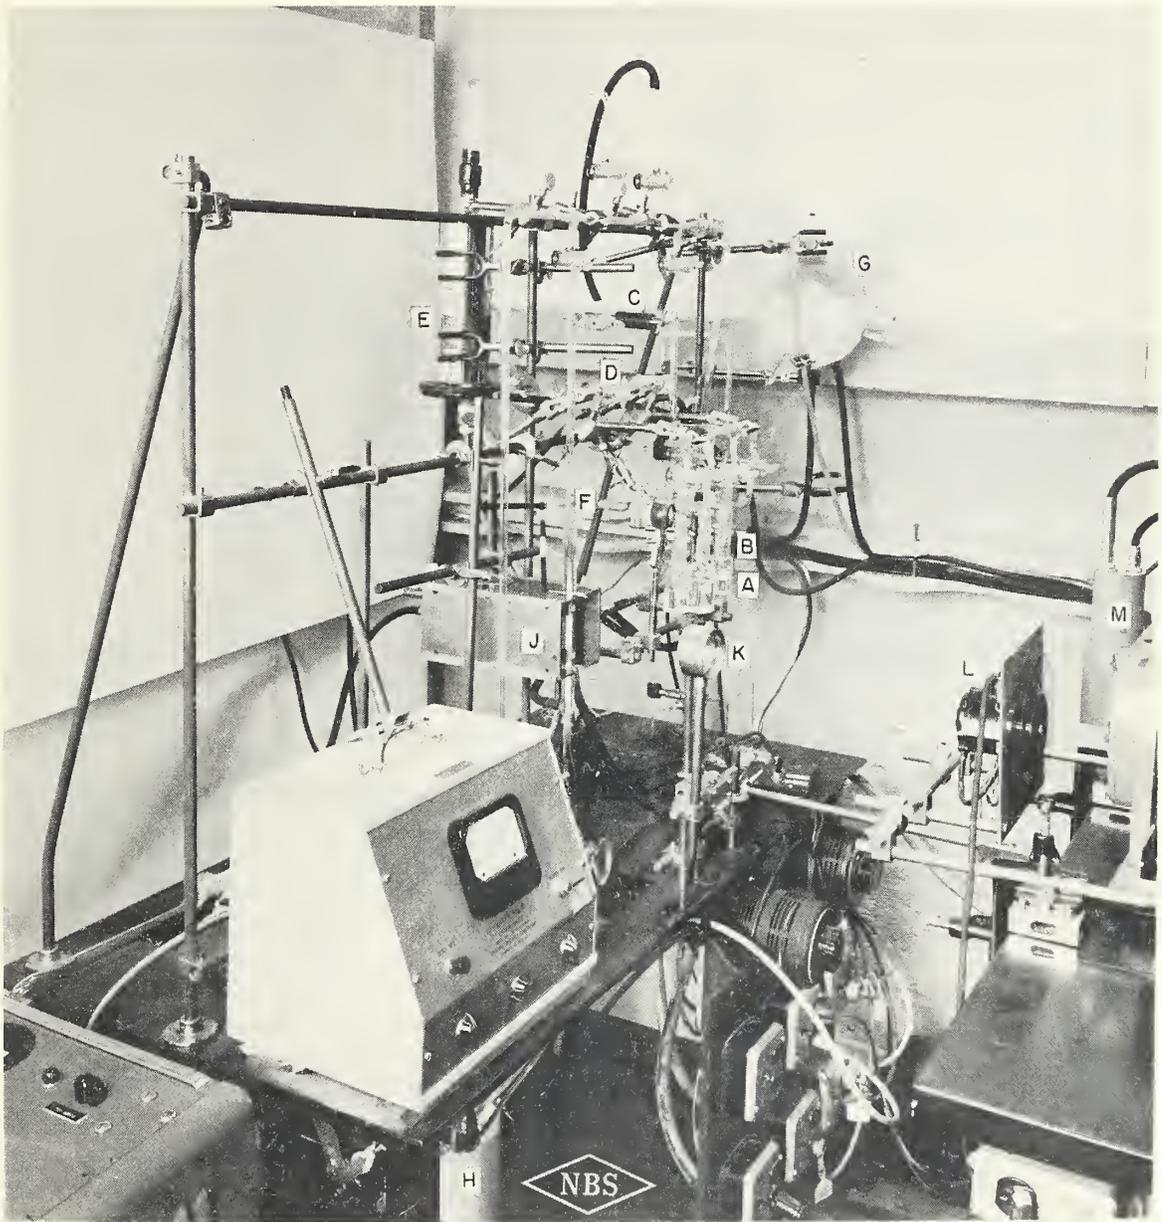


FIGURE 1.



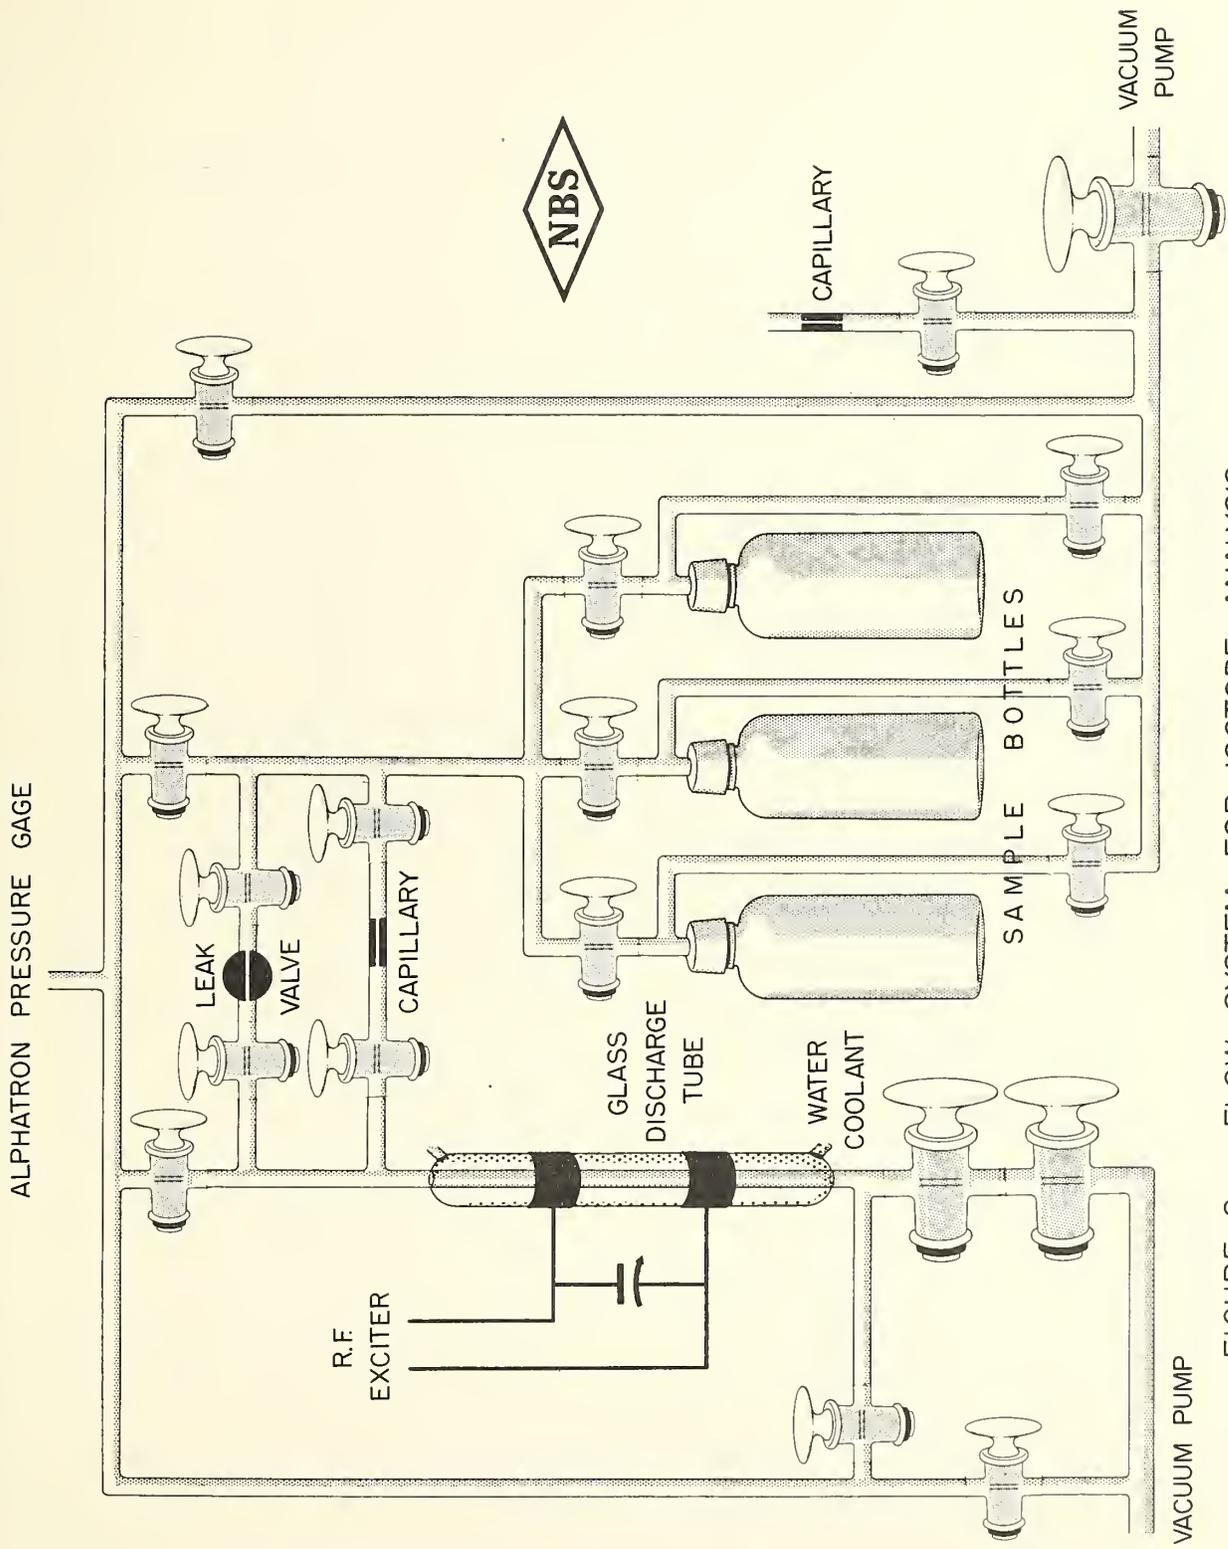


FIGURE 2. FLOW SYSTEM FOR ISOTOPE ANALYSIS

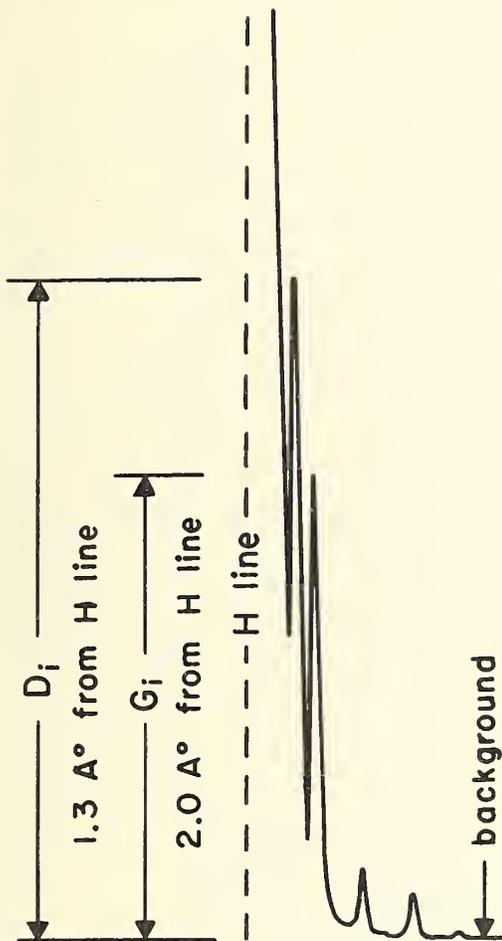

0 - 1% D_2O RANGE

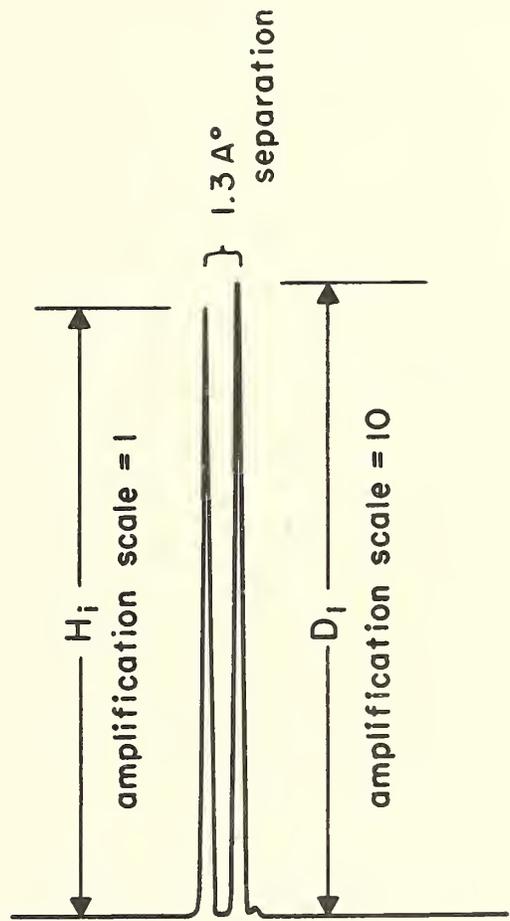

1 - 99% D_2O RANGE



FIGURE 3.

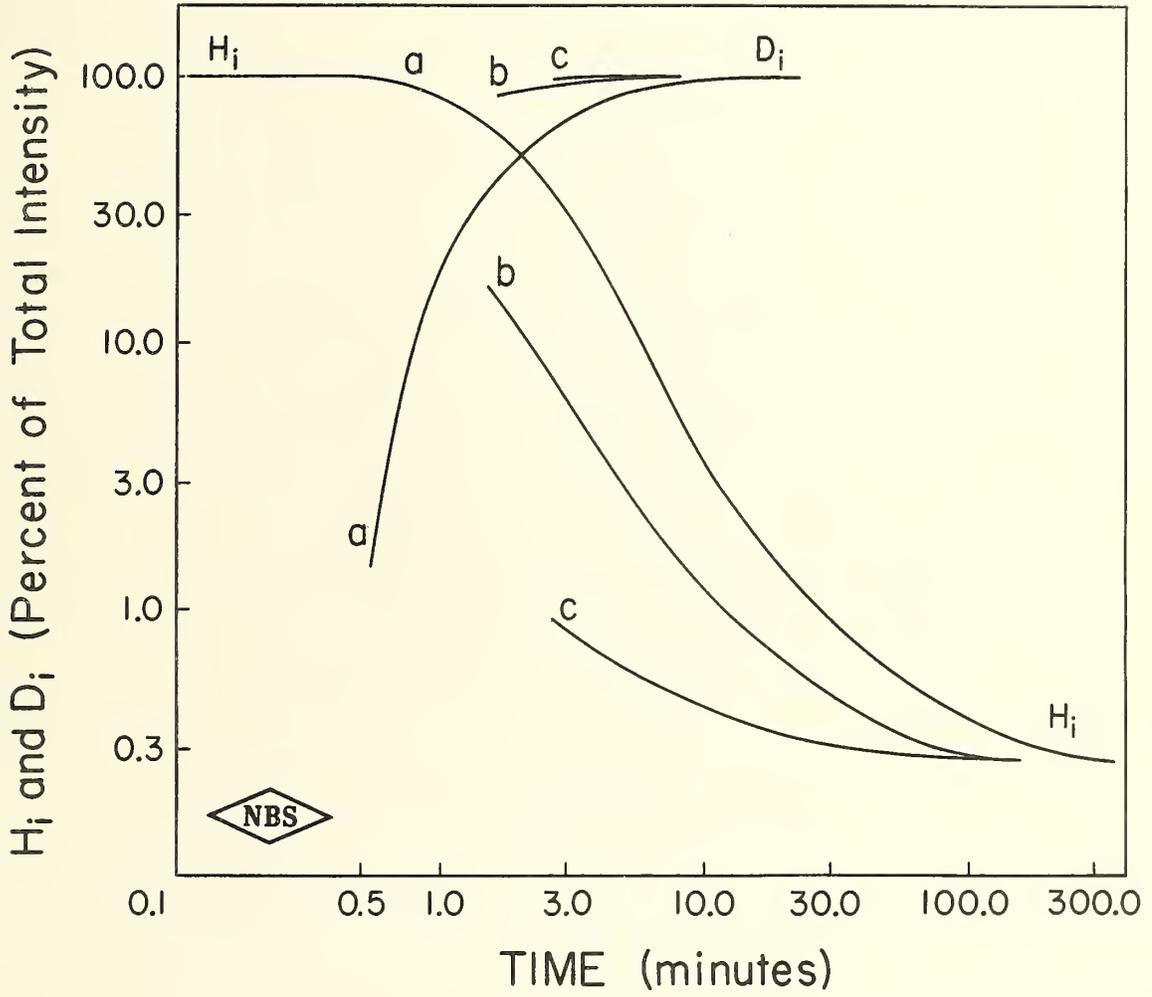


FIGURE 4.

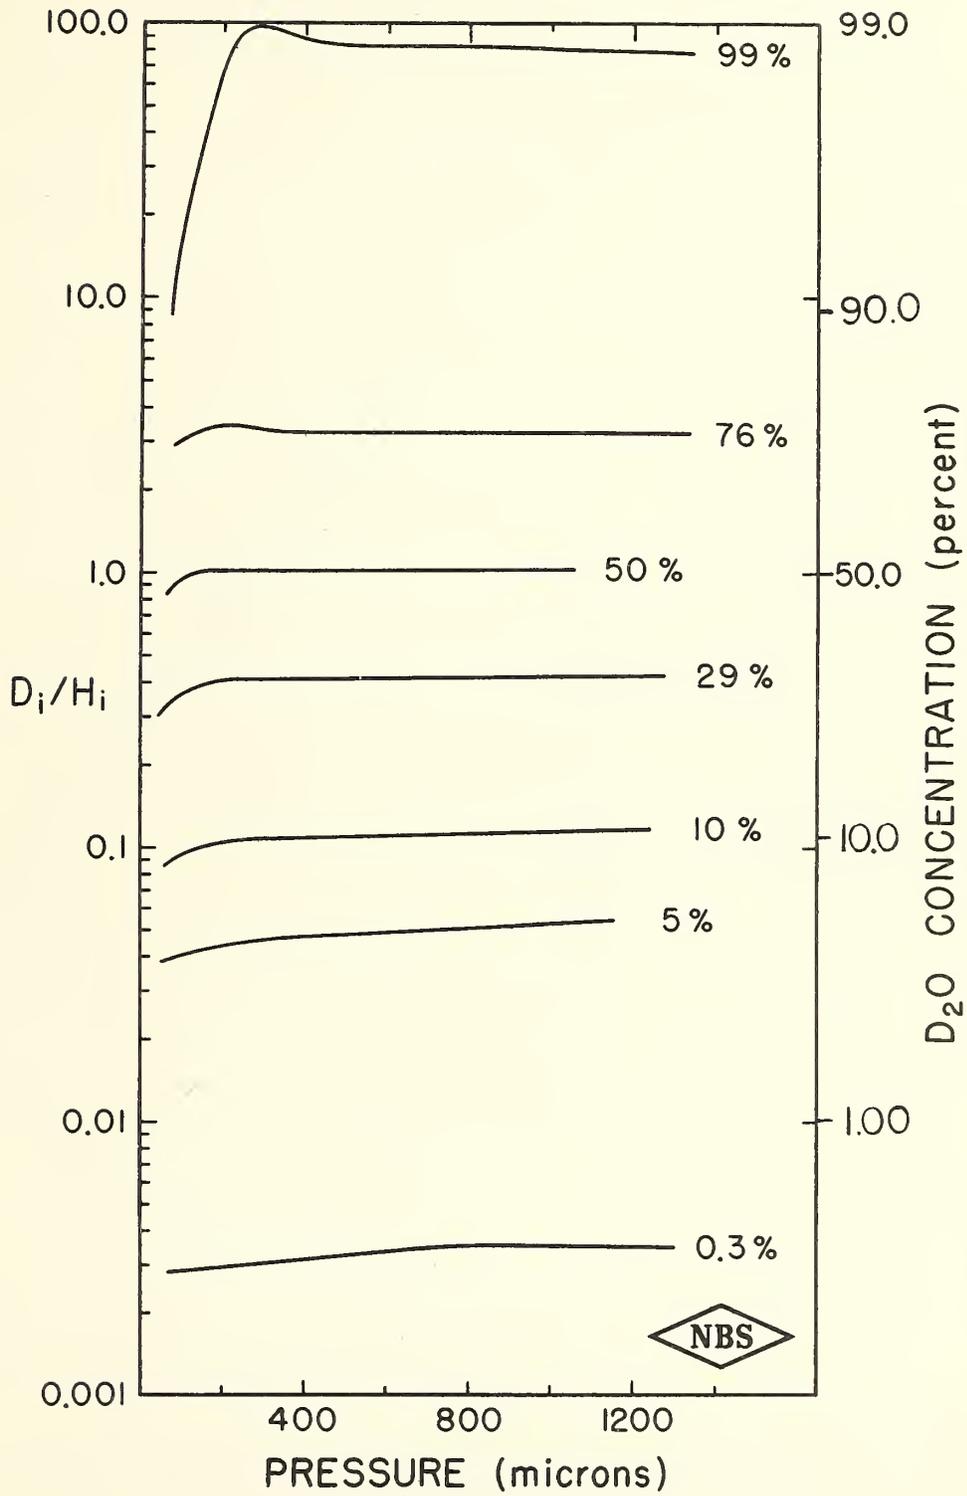


FIGURE 5.

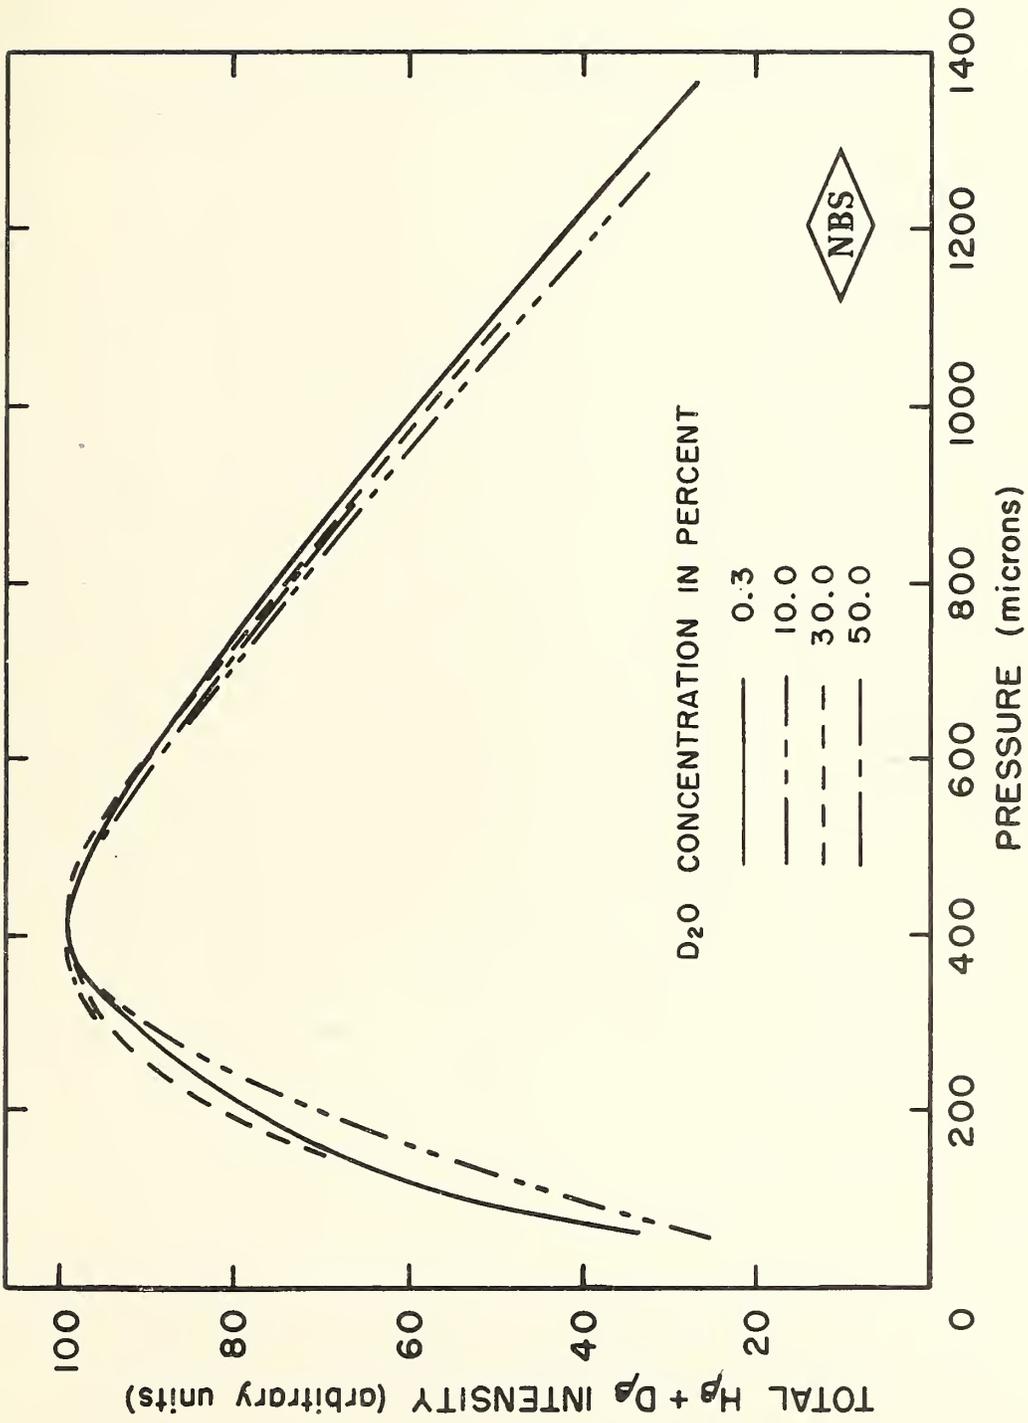


FIGURE 6.

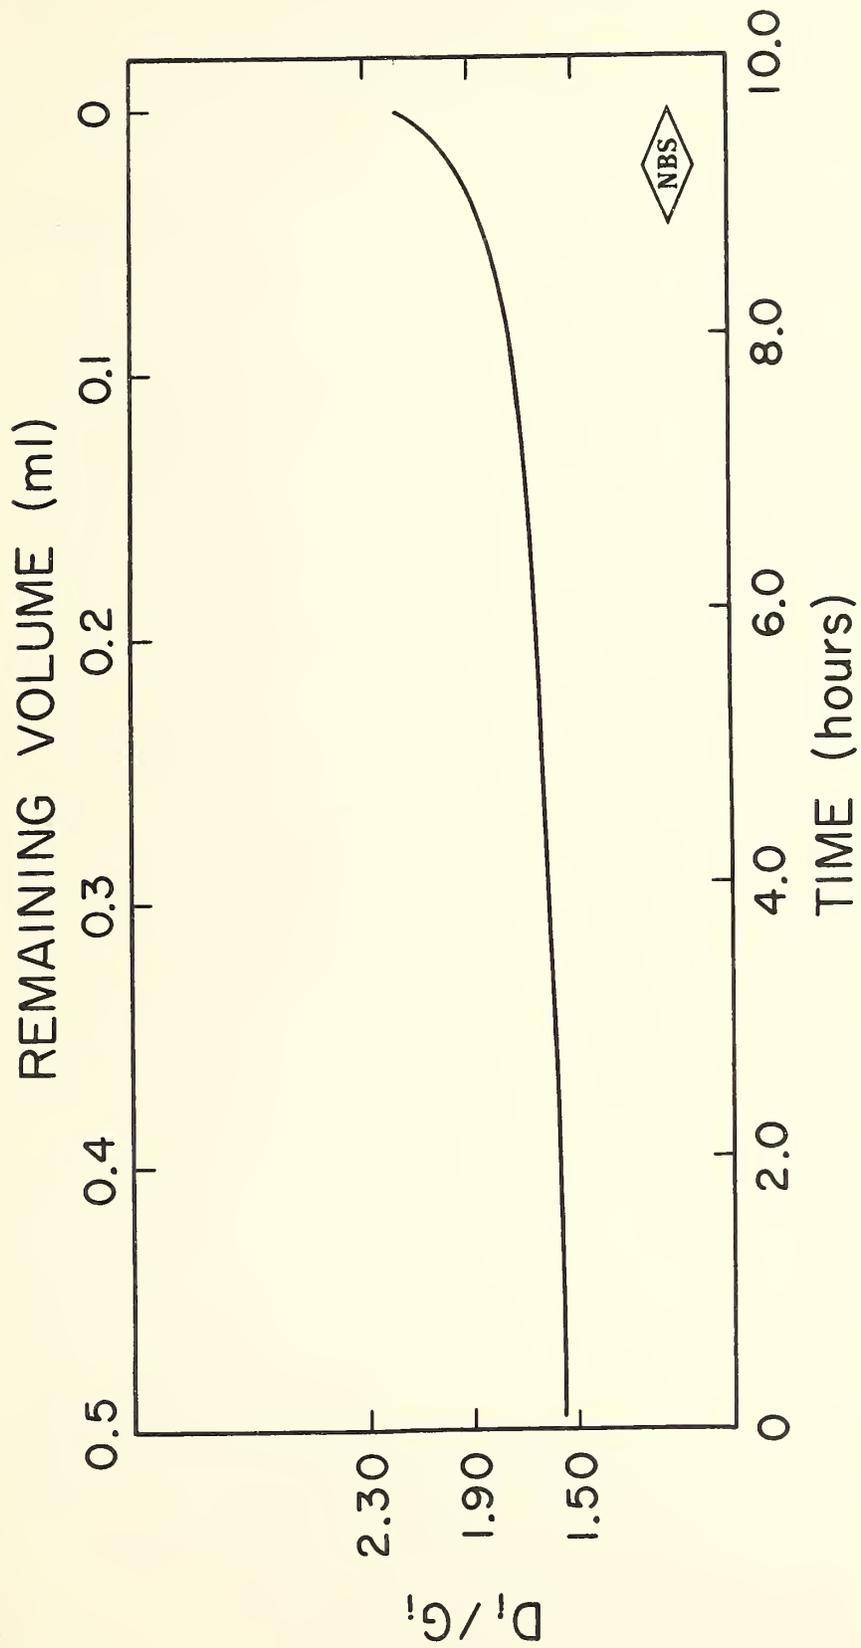


FIGURE 7

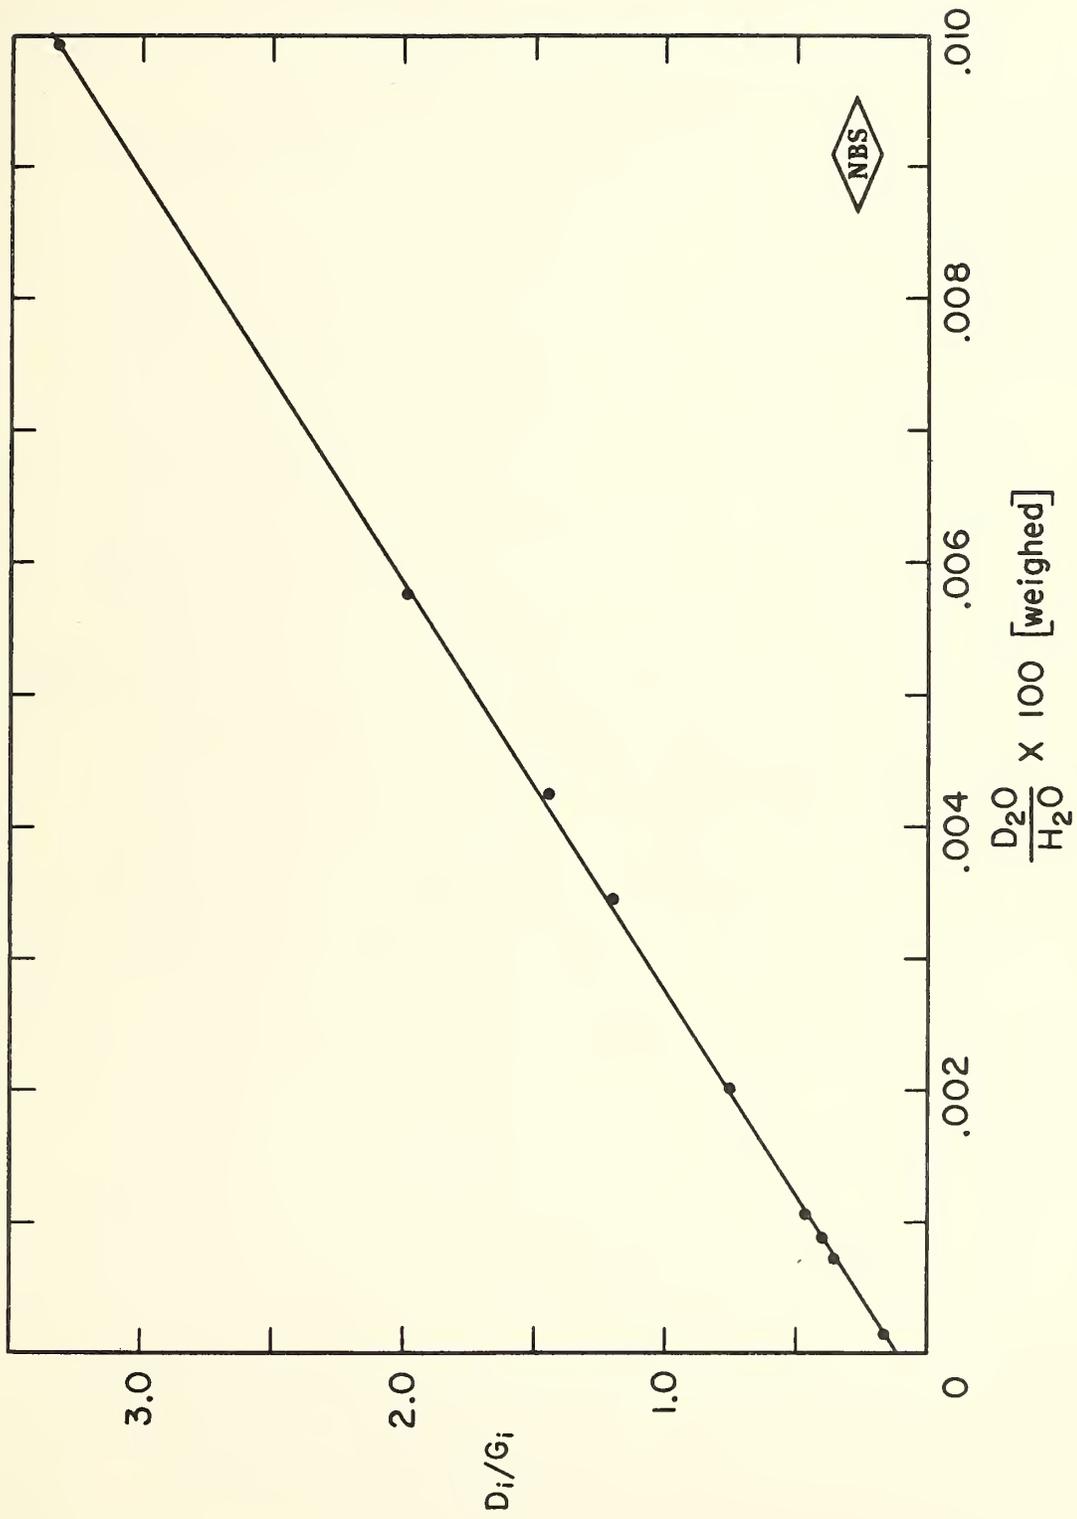


FIGURE 8.

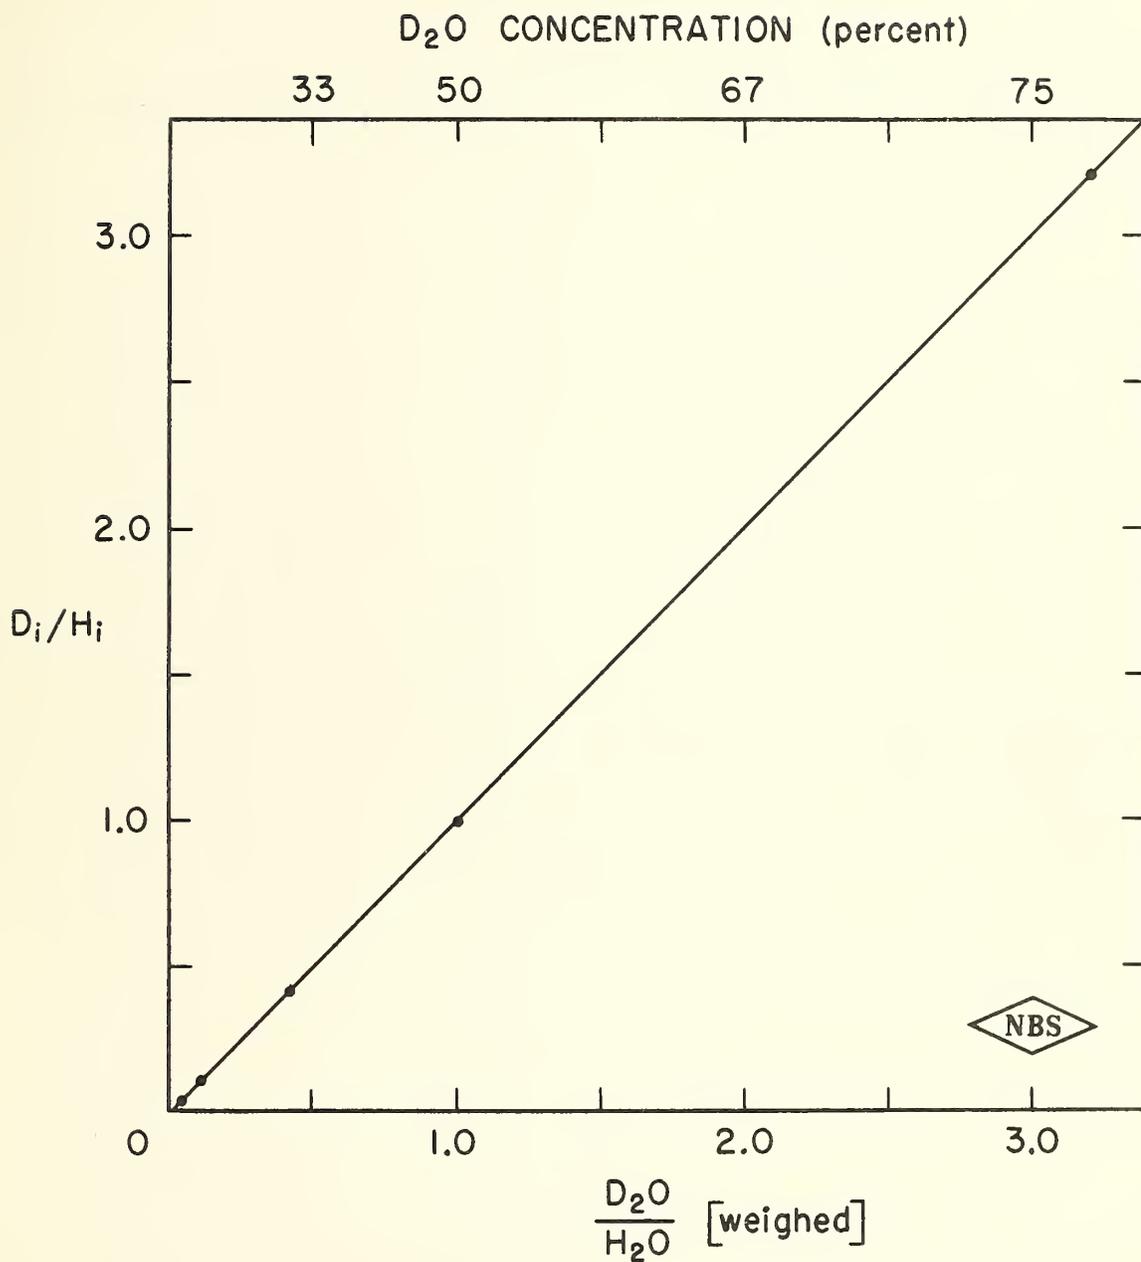


FIGURE 9.

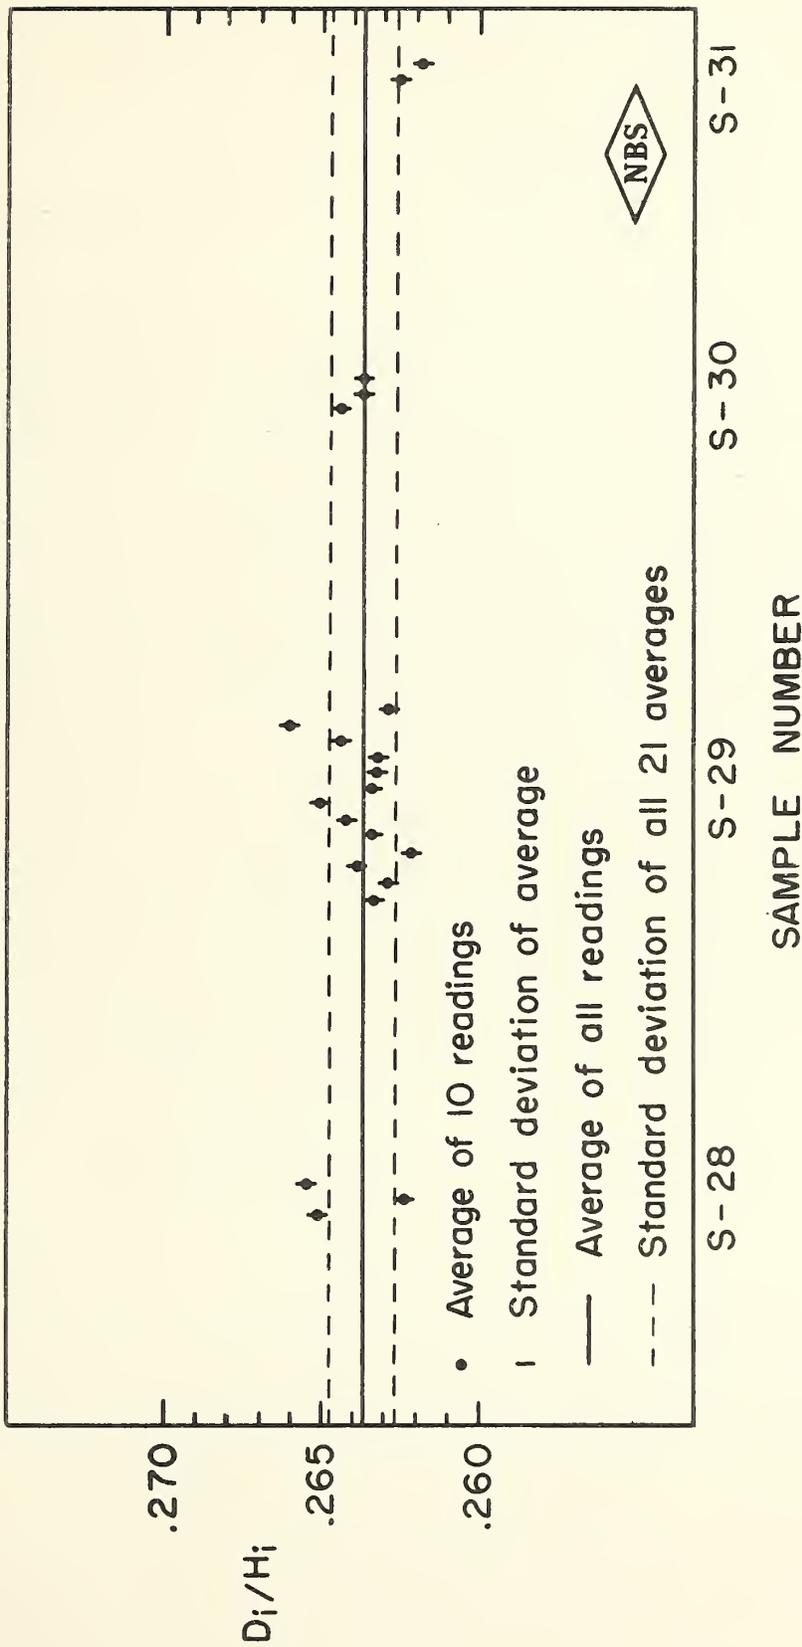


FIGURE 10.

THE NATIONAL BUREAU OF STANDARDS

Functions and Activities

The functions of the National Bureau of Standards are set forth in the Act of Congress, March 3, 1901, as amended by Congress in Public Law 619, 1950. These include the development and maintenance of the national standards of measurement and the provision of means and methods for making measurements consistent with these standards; the determination of physical constants and properties of materials; the development of methods and instruments for testing materials, devices, and structures; advisory services to Government Agencies on scientific and technical problems; invention and development of devices to serve special needs of the Government; and the development of standard practices, codes, and specifications. The work includes basic and applied research, development, engineering, instrumentation, testing, evaluation, calibration services, and various consultation and information services. A major portion of the Bureau's work is performed for other Government Agencies, particularly the Department of Defense and the Atomic Energy Commission. The scope of activities is suggested by the listing of divisions and sections on the inside of the front cover.

Reports and Publications

The results of the Bureau's work take the form of either actual equipment and devices or published papers and reports. Reports are issued to the sponsoring agency of a particular project or program. Published papers appear either in the Bureau's own series of publications or in the journals of professional and scientific societies. The Bureau itself publishes three monthly periodicals, available from the Government Printing Office: The Journal of Research, which presents complete papers reporting technical investigations; the Technical News Bulletin, which presents summary and preliminary reports on work in progress; and Basic Radio Propagation Predictions, which provides data for determining the best frequencies to use for radio communications throughout the world. There are also five series of nonperiodical publications: The Applied Mathematics Series, Circulars, Handbooks, Building Materials and Structures Reports, and Miscellaneous Publications.

Information on the Bureau's publications can be found in NBS Circular 460, Publications of the National Bureau of Standards (\$1.00). Information on calibration services and fees can be found in NBS Circular 483, Testing by the National Bureau of Standards (25 cents). Both are available from the Government Printing Office. Inquiries regarding the Bureau's reports and publications should be addressed to the Office of Scientific Publications, National Bureau of Standards, Washington 25, D. C.

