

A11103 085910



NBS SPECIAL PUBLICATION **260-67**

U.S. DEPARTMENT OF COMMERCE / National Bureau of Standards

Standard Reference Materials:

A REFERENCE METHOD FOR THE DETERMINATION OF CHLORIDE IN SERUM

QC

100

U57

10.260-67

1979

C-2

NATIONAL BUREAU OF STANDARDS

The National Bureau of Standards¹ was established by an act of Congress on March 3, 1901. The Bureau's overall goal is to strengthen and advance the Nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research and provides: (1) a basis for the Nation's physical measurement system, (2) scientific and technological services for industry and government, (3) a technical basis for equity in trade, and (4) technical services to promote public safety. The Bureau's technical work is performed by the National Measurement Laboratory, the National Engineering Laboratory, and the Institute for Computer Sciences and Technology.

THE NATIONAL MEASUREMENT LABORATORY provides the national system of physical and chemical and materials measurement; coordinates the system with measurement systems of other nations and furnishes essential services leading to accurate and uniform physical and chemical measurement throughout the Nation's scientific community, industry, and commerce; conducts materials research leading to improved methods of measurement, standards, and data on the properties of materials needed by industry, commerce, educational institutions, and Government; provides advisory and research services to other Government agencies; develops, produces, and distributes Standard Reference Materials; and provides calibration services. The Laboratory consists of the following centers:

Absolute Physical Quantities² — Radiation Research — Thermodynamics and Molecular Science — Analytical Chemistry — Materials Science.

THE NATIONAL ENGINEERING LABORATORY provides technology and technical services to the public and private sectors to address national needs and to solve national problems; conducts research in engineering and applied science in support of these efforts; builds and maintains competence in the necessary disciplines required to carry out this research and technical service; develops engineering data and measurement capabilities; provides engineering measurement traceability services; develops test methods and proposes engineering standards and code changes; develops and proposes new engineering practices; and develops and improves mechanisms to transfer results of its research to the ultimate user. The Laboratory consists of the following centers:

Applied Mathematics — Electronics and Electrical Engineering² — Mechanical Engineering and Process Technology² — Building Technology — Fire Research — Consumer Product Technology — Field Methods.

THE INSTITUTE FOR COMPUTER SCIENCES AND TECHNOLOGY conducts research and provides scientific and technical services to aid Federal agencies in the selection, acquisition, application, and use of computer technology to improve effectiveness and economy in Government operations in accordance with Public Law 89-306 (40 U.S.C. 759), relevant Executive Orders, and other directives; carries out this mission by managing the Federal Information Processing Standards Program, developing Federal ADP standards guidelines, and managing Federal participation in ADP voluntary standardization activities; provides scientific and technological advisory services and assistance to Federal agencies; and provides the technical foundation for computer-related policies of the Federal Government. The Institute consists of the following centers:

Programming Science and Technology — Computer Systems Engineering.

¹Headquarters and Laboratories at Gaithersburg, MD, unless otherwise noted; mailing address Washington, DC 20234.

²Some divisions within the center are located at Boulder, CO 80303.

NOV 30 1979
not Rec. File
02100
US7
no. 260-6
1979
c.2

Standard Reference Materials:

**A REFERENCE METHOD FOR THE DETERMINATION OF
CHLORIDE IN SERUM**

Rance A. Velapoldi, Robert C. Paule,
Robert Schaffer, John Mandel,
Thomas J. Murphy, and
John W. Gramlich

National Measurement Laboratory
National Bureau of Standards
Washington, D.C. 20234

With the cooperation of a Committee of Experts:

George N. Bowers, Jr.,¹ Bradley E. Copeland,²
Denis O. Rodgerson,³ and James M. White⁴

¹Hartford Hospital, Hartford, Connecticut

²New England Deaconess Hospital, Boston, Massachusetts

³Department of Pathology, University of California,
Los Angeles, California

⁴Center for Disease Control, Atlanta, Georgia



U.S. DEPARTMENT OF COMMERCE

Luther H. Hodges, Jr., Under Secretary

Jordan J. Baruch, Assistant Secretary for Science and Technology

NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Director

Issued November 1979

Library of Congress Catalog Card Number: 79-600174

National Bureau of Standards Special Publication 260-67

Nat. Bur. Stand. (U.S.), Spec. Publ. 260-67, 97 pages (Nov. 1979)

CODEN: XNBSAV

U.S. GOVERNMENT PRINTING OFFICE

WASHINGTON: 1979

For sale by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402

Stock No. 003-003-02136-9 Price \$3.75

(Add 25 percent additional for other than U.S. mailing).

PREFACE

Standard Reference Materials (SRM's) as defined by the National Bureau of Standards are well-characterized materials, produced in quantity and certified for one or more physical or chemical properties. They are used to assure the accuracy and compatibility of measurements throughout the nation. SRM's are widely used as primary standards in many diverse fields in science, industry, and technology, both within the United States and throughout the world. They are also used extensively in the fields of environmental and clinical analysis. In many applications, traceability of quality control and measurement processes to the national measurement system are carried out through the mechanism and use of SRM's. For many of the nation's scientists and technologists it is therefore of more than passing interest to know the details of the measurements made at NBS in arriving at the certified values of the SRM's produced. An NBS series of papers, of which this publication is a member, called the NBS Special Publication - 260 Series is reserved for this purpose.

This 260 Series is dedicated to the dissemination of information on different phases of the preparation, measurement, certification and use of NBS-SRM's. In general, much more detail will be found in these papers than is generally allowed, or desirable, in scientific journal articles. This enables the user to assess the validity and accuracy of the measurement processes employed, to judge the statistical analysis, and to learn details of techniques and methods utilized for work entailing the greatest care and accuracy. These papers also should provide sufficient additional information not found on the certificate so that new applications in diverse fields not foreseen at the time the SRM was originally issued will be sought and found.

Inquiries concerning the technical content of this paper should be directed to the author(s). Other questions concerned with the availability, delivery, price, and so forth will receive prompt attention from:

Office of Standard Reference Materials
National Bureau of Standards
Washington, D.C. 20234

George A. Uriano, Chief
Office of Standard Reference Materials

FOREWORD

A fundamental requirement for assuring adequate patient care is the need for the accurate analysis of constituents in body fluids. Two major functions of the National Bureau of Standards (NBS) are to provide certified Standard Reference Materials for the calibration of measurement systems and to develop new or improved analytical methods. The results presented in this NBS Special Publication provide a methodology of known accuracy for the determination of chloride in serum. The evaluation of a reference method by comparison to a definitive method, used for the first time at NBS in the development of reference methods for calcium, sodium, and potassium in serum, also was applied to this work. This hierarchy of analytical procedures has been accepted as a valid format for developing reference methods by the clinical community at a recent Conference on an Understanding for a National Reference System in Clinical Chemistry.

In an undertaking of this magnitude, extensive collaboration with a committee of experts, the Center for Disease Control, the Food and Drug Administration, and a wide spectrum of participating analytical laboratories that included Federal, state, hospital, industrial, and academic laboratories was essential to establish a widely accepted reference method. It is hoped that this work will provide an additional basis for the development of future clinical reference methods through continued collaboration and the concerted efforts of the individual participants.

Philip D. LaFleur, Director
Center for Analytical Chemistry

NOTE

Because of concern for the usability of this chloride reference method, the Center for Disease Control (CDC) management has declined to endorse the method described in this report. NBS supports the evolution of analytical methods and desires to participate in interlaboratory exercises that are aimed toward establishing the transferability of proposed reference procedures. NBS believes it important that the principles of analytical practice delineated in this present report be circulated in a timely manner. Since the method outlined in this report has been shown to satisfy the generally accepted criteria of a reference method, it should function as such until the efficacy of a subsequent method has been demonstrated. NBS will maintain its primary role in supplying SRM's and definitive methods.

OTHER NBS PUBLICATIONS IN THIS SERIES

- Catalog of NBS Standard Reference Materials (1979-80 edition), R. W. Seward, ed., NBS Spec. Publ. 260 (April 1979) \$3.00* SN003-003-02048-6
- Michaelis, R. E., and Wyman, L. L., Standard Reference Materials: Preparation of White Cast Iron Spectrochemical Standards, NBS Misc. Publ. 260-1 (June 1964). COM74-11061**
- Michaelis, R. E., Wyman, L. L., and Flitsch, R., Standard Reference Materials: Preparation of NBS Copper-Base Spectrochemical Standards, NBS Misc. Publ. 260-2 (October 1964). COM74-11063**
- Michaelis, R. E., Yakowitz, H., and Moore, G. A., Standard Reference Materials: Metallographic Characterization of an NBS Spectrometric Low-Alloy Steel Standard, NBS Misc. Publ. 260-3 (October 1964). COM74-11060**
- Hague, J. L., Mears, T. W., and Michaelis, R. E., Standard Reference Materials: Sources of Information, NBS Misc. Publ. 260-4 (February 1965). COM74-11059
- Alvarez, R., and Flitsch, R., Standard Reference Materials: Accuracy of Solution X-Ray Spectrometric Analysis of Copper-Base Alloys, NBS Misc. Publ. 260-5 (March 1965). PB168068**
- Shultz, J. I., Standard Reference Materials: Methods for the Chemical Analysis of White Cast Iron Standards, NBS Misc. Publ. 260-6 (July 1975). COM74-11068**
- Bell, R. K., Standard Reference Materials: Methods for the Chemical Analysis of NBS Copper-Base Spectrochemical Standards, NBS Misc. Publ. 260-7 (October 1965). COM74-11067**
- Richmond, M. S., Standard Reference Materials: Analysis of Uranium Concentrates at the National Bureau of Standards, NBS Misc. Publ. 260-8 (December 1965). COM74-11066**
- Anspach, S. C., Cavallo, L. M., Garfinkel, S. B., Hutchinson, J. M. R., and Smith, C. N., Standard Reference Materials: Half Lives of Materials Used in the Preparation of Standard Reference Materials of Nineteen Radioactive Nuclides Issued by the National Bureau of Standards, NBS Misc. Publ. 260-9 (November 1965). COM74-11065**
- Yakowitz, H., Vieth, D. L., Heinrich, K. F. J., and Michaelis, R. E., Standard Reference Materials: Homogeneity Characterization on NBS Spectrometric Standards II: Cartridge Brass and Low-Alloy Steel, NBS Misc. Publ. 260-10 (December 1965). COM74-11064**
- Napolitano, A., and Hawkins, E. G., Standard Reference Materials: Viscosity of Standard Lead-Silica Glass, NBS Misc. Publ. 260-11 (November 1966). NBS Misc. Publ. 260-11**
- Yakowitz, H., Vieth, D. L., and Michaelis, R. E., Standard Reference Materials: Homogeneity Characterization of NBS Spectrometric Standards III: White Cast Iron and Stainless Steel Powder Compact, NBS Misc. Publ. 260-12 (September 1966). NBS Misc. Publ. 260-12**
- Spijkerman, J. L., Snediker, D. K., Ruegg, F. C., and DeVoe, J. R., Standard Reference Materials: Mossbauer Spectroscopy Standard for the Chemical Shift of Iron Compounds, NBS Misc. Publ. 260-13 (July 1967). NBS Misc. Publ. 260-13**
- Menis, O., and Sterling, J. T., Standard Reference Materials: Determination of Oxygen in Ferrous Materials - SRM 1090, 1091, and 1092, NBS Misc. Publ. 260-14 (September 1966). NBS Misc. Publ. 260-14**
- Passaglia, E., and Shouse, P. J. Standard Reference Materials: Recommended Method of Use of Standard Light-Sensitive Paper for Calibrating Carbon Arcs Used in Testing Textiles for Colorfastness to Light, NBS Misc. Publ. 260-15 (June 1967). (Replaced by NBS Spec. Publ. 260-41.)
- Yakowitz, H., Michaelis, R. E., and Vieth, D. L., Standard Reference Materials: Homogeneity Characterization of NBS Spectrometric Standards IV: Preparation and Microprobe Characterization of W-20% MO Alloy Fabricated by Powder Metallurgical Methods, NBS Spec. Publ. 260-16 (January 1969). COM74-11062**
- Catanzaro, E. J., Champion, C. E., Garner, E. L., Marinenko, G., Sappenfield, K. M., and Shields, W. R. Standard Reference Materials: Boric Acid; Isotopic and Assay Standard Reference Materials, NBS Spec. Publ. 260-17 (February 1970). Out of Print

- Geller, S. B., Mantek, P.A., and Cleveland, N. G., Standard Reference Materials: Calibration of NBS Secondary Standard Magnetic Tape (Computer Amplitude Reference) Using the Reference Tape Amplitude Measurement "Process A," NBS Spec. Publ. 260-18 (November 1969). (See NBS Spec. Publ. 260-29.)
- Paule, R. C., and Mandel, J., Standard Reference Materials: Analysis of Interlaboratory Measurements on the Vapor Pressure of Gold (Certification of Standard Reference Material 745). NBS Spec. Publ. 260-19 (January 1970). PB190071**
- Paule, R. C., and Mandel, J., Standard Reference Materials: Analysis of Interlaboratory Measurements on the Vapor Pressures of Cadmium and Silver, NBS Spec. Publ. 260-21 (January 1971). COM74-11359**
- Yakowitz, H., Fiori, C. E., and Michaelis, R. E., Standard Reference Materials: Homogeneity Characterization of Fe-3 Si Alloy, NBS Spec. Publ. 260-22 (February 1971). COM74-11357**
- Napolitano, A., and Hawkins, E. G., Standard Reference Materials: Viscosity of a Standard Borosilicate Glass, NBS Spec. Publ. 260-23 (December 1970). COM71-00157**
- Sappenfield, K. M., Marineko, G., and Hague, J. L., Standard Reference Materials: Comparison of Redox Standards, NBS Spec. Publ. 260-24 (January 1972). COM72-50058**
- Hicho, G. E., Yakowitz, H., Rasberry, S. D., and Michaelis, R. E., Standard Reference Materials: A Standard Reference Material Containing Nominally Four Percent Austenite, NBS Spec. Publ. 260-25 (February 1971). COM74-11356**
- Martin, J. F., Standard Reference Materials: National Bureau of Standards-US Steel Corporation Joint Program for Determining Oxygen and Nitrogen in Steel, NBS Spec. Publ. 260-26 (February 1971). 85 cents* SN003-003-00786-2
- Garner, E. L., Machlan, L. A., and Shields, W. R., Standard Reference Materials: Uranium Isotopic Standard Reference materials, NBS Spec. Publ. 260-27 (April 1971). COM74-11358**
- Heinrich, K. F. J., Myklebust, R. L., Rasberry, S. D., and Michaelis, R. E., Standard Reference Materials: Preparation and Evaluation of SRM's 481 and 482 Gold-Silver and Gold-Copper Alloys for Microanalysis, NBS Spec. Publ. 260-28 (August 1971). COM71-50365**
- Geller, S. B., Standard Reference Materials: Calibration of NBS Secondary Standard Magnetic Tape (Computer Amplitude Reference) Using the Reference Tape Amplitude Measurement "Process A-Model 2," NBS Spec. Publ. 260-29 (June 1971). COM71-50282
- Gorozhanina, R. S., Freedman, A. Y., and Shaievitch, A. B. (translated by M. C. Selby), Standard Reference Materials: Standard Samples Issued in the USSR (A Translation from the Russian). NBS Spec. Publ. 260-30 (June 1971). COM71-50283**
- Hust, J. G., and Sparks, L. L., Standard Reference Materials: Thermal Conductivity of Electrolytic Iron SRM 734 from 4 to 300 K, NBS Spec. Publ. 260-31 (November 1971). COM71-50563**
- Mavrodineanu, R., and Lazar, J. W., Standard Reference Materials: Standard Quartz Cuvettes, for High Accuracy Spectrophotometry, NBS Spec. Publ. 260-32 (December 1973). 55 cents* SN003-003-01213-1
- Wagner, H. L., Standard Reference Materials: Comparison of Original and Supplemental SRM 705, Narrow Molecular Weight Distribution Polystyrene, NBS Spec. Publ. 260-33 (May 1972). COM72-50526**
- Sparks, L. L., and Hust, J. G., Standard Reference Materials: Thermoelectric Voltage, NBS Spec. Publ. 260-34, (April 1972). COM72-50371**
- Sparks, L. L., and Hust, J. G., Standard Reference Materials: Thermal Conductivity of Austenitic Stainless Steel, SRM 735 from 5 to 280 K, NBS Spec. Publ. 260-35 (April 1972.) 35 cents* COM72-50368**
- Cali, J. P., Mandel, J., Moore, L. J., and Young, D. S., Standard Reference Materials: A Referee Method for the Determination of Calcium in Serum, NBS SRM 915, NBS Spec. Publ. 260-36 (May 1972). COM72-50527**
- Shultz, J. I. Bell., R. K. Rains, T. C., and Menis, O., Standard Reference Materials: Methods of Analysis of NBS Clay Standards, NBS Spec. Publ. 260-37 (June 1972). COM72-50692**
- Richmond, J. C., and Hsia, J. J., Standard Reference Materials: Preparation and Calibration of Standards of Spectral Specular Reflectance, NBS Spec. Publ. 260-38 (May 1972). COM72-50528**
- Clark, A. F., Denson, V.A., Hust, J. G., and Powell, R. L., Standard Reference Materials The Eddy Current Decay Method for Resistivity Characterization of High-Purity Metals, NBS Spec. Publ. 260-39 (May 1972). COM72-50529**

- McAdie, H. G., Garn, P.D., and Menis, O., Standard Reference Materials: Selection of Thermal Analysis Temperature Standards Through a Cooperative Study (SRM 758, 759, 760), NBS Spec. Publ. 260-40 (August 1972). COM72-50776**
- Wood, L. A., and Shouse, P. J., Standard Reference Materials: Use of Standard Light-Sensitive Paper for Calibrating Carbon Arcs Used in Testing Textiles for Colorfastness to Light, NBS Spec. Publ. 260-41 (August 1972) COM72-50775**
- Wagner, H. L. and Verdier, P. H., eds., Standard Reference Materials: The Characterization of Linear Polyethylene, SRM 1475, NBS Spec. Publ. 260-42 (September 1972). COM72-50944**
- Yakowitz, H., Ruff, A. W., and Michaelis, R. E., Standard Reference Materials: Preparation and Homogeneity Characterization of an Austenitic Iron-Chromium-Nickel Alloy, NBS Spec. Publ. 260-43 (November 1972). COM73-50760**
- Schooley, J. F., Soulen, R. J., Jr., and Evans, G. A., Jr., Standard Reference Materials: Preparation and Use of Superconductive Fixed Point Devices, SRM 767, NBS Spec. Publ. 260-44 (December 1972). COM73-50037**
- Greifer, B., Maienthal, E. J. Rains, T. C., and Rasberry, S. D., Standard Reference Materials: Powdered Lead-Based Paint, SRM 1579, NBS Spec. Publ. 260-45 (March 1973). COM73-50226**
- Hust, J. G., and Giarratano, P. J., Standard Reference Materials: Thermal Conductivity and Electrical Resistivity Standard Reference Materials: Austenitic Stainless Steel, SRM's 735 and 798, from 4 to 1200 K, NBS Spec. Publ. 260-46 (March 1975). SN003-003-01278-5
- Hust, J. G., Standard Reference Materials: Electrical Resistivity of Electrolytic Iron, SRM 797, and Austenitic Stainless Steel, SRM 798, from 5 to 280 K, NBS Spec. Publ. 260-47 (February 1974). COM74-50176**
- Mangum, B. W., and Wise, J. A., Standard Reference Materials: Description and Use of Precision Thermometers for the Clinical Laboratory, SRM 933 and SRM 934, NBS Spec. Publ. 260-48 (May 1974). 60 cents* SN003-003-01278-5
- Carpenter, B. S., and Reimer, G. M., Standard Reference Materials Calibrated Glass Standards for Fission Track Use, NBS Spec. Publ. 260-49 (November 1974). SN003-003-01344-7
- Hust, J. G., and Giarratano, P. J., Standard Reference Materials: Thermal Conductivity and Electrical Resistivity Standard Reference Materials: Electrolytic Iron, SRM's 734 and 797 from 4 to 1000 K, NBS Spec. Publ. 260-50 (June 1975). \$1.00* SN003-003-01425-7
- Mavrodineanu, R., and Baldwin, J. R., Standard Reference Materials: Glass Filters As a Standard Reference Material for Spectrophotometry; Selection; Preparation; Certification; Use-SRM 930, NBS Spec. Publ. 260-51 (November 1975). \$1.90* SN003-003-01481-8
- Hust, J. G., and Giarratano, P. J., Standard Reference Materials: Thermal Conductivity and Electrical Resistivity Standard Reference Materials 730 and 799, from 4 to 3000 K, NBS Spec. Publ. 260-52 (September 1975). \$1.05* SN003-003-01464-8
- Durst, R. A., Standard Reference Materials: Standardization of pH Measurements, NBS Spec. Publ. 260-53 (Under Revision).
- Burke, R. W., and Mavrodineanu, R. Standard Reference Materials: Certification and Use of Acidic Potassium Dichromate Solutions as an Ultraviolet Absorbance Standard, NBS Spec. Publ. 260-54 (August 1977). \$3.00* SN003-003-01828-7
- Ditmars, D. A., Cezairliyan, A., Ishihara, S., and Douglas, T. B., Standard Reference Materials: Enthalpy and Heat Capacity; Molybdenum SRM 781, from 273 to 2800 K, NBS Spec. Publ. 260-55 (September 1977). \$2.20* SN003-003-01836-8
- Powell, R. L., Sparks, L. L., and Hust, J. G., Standard Reference Materials: Standard Thermocouple Materials, Pt.67: SRM 1967, NBS Spec. Publ. 260-56 (February 1978). \$2.20* SN003-003-018864
- Cali, J. P. and Plebanski, T., Guide to United States Reference Materials, NBS Spec. Publ. 260-57 (February 1978). \$2.20* SN003-003-01883-0
- Barnes, J. D., and Martin, G. M., Standard Reference Materials: Polyester Film for Oxygen Gas Transmission Measurements SRM 1470, NBS Spec. Publ. 260-58 (June 1979) \$2.00* SN003-003-02077
- Chang, T., and Kahn, A. H., Standard Reference Materials: Electron Paramagnetic Resonance Intensity Standard: SRM 2601, NBS Spec. Publ. 260-59 (August 1978) \$2.30* SN003-003-01975-5

- Velapoldi, R. A., Paule, R. C., Schaffer, R., Mandel, J., and Moody, J. R., Standard Reference Materials: A Reference Method for the Determination of Sodium in Serum, NBS Spec. Publ. 260-60 (August 1978). \$3.00* SN003-003-01978-0
- Verdier, P. H., and Wagner, H. L., Standard Reference Materials: The Characterization of Linear Polyethylene (SRM 1482, 1483, 1484), NBS Spec. Publ. 260-61 (December 1978). \$1.70* SN003-003-02006-1
- Soulen, R. J., and Dove, R. B., Standard Reference Materials: Temperature Reference Standard for Use Below 0.5 K (SRM 768), NBS Spec. Publ. 260-62 (April 1979). \$2.30* SN003-003-02047-8
- Velapoldi, R. A., Paule, R. C., Schaffer, R., Mandel, J., Machlan, J. L., and Gramlich, J. W., Standard Reference Materials: A Reference Method for the Determination of Potassium in Serum, NBS Spec. Publ. 260-63 (May 1979). \$3.75* SN003-003-02068
- Velapoldi, R. A., and Mielenz, K. D., Standard Reference Materials: A Fluorescence Standard Reference Material Quinine Sulfate Dihydrate (SRM 936), NBS Spec. Publ. 260-64 (in press).
- Marinenko, R. B., Heinrich, K. F. J., and Ruegg, F. C., Standard Reference Materials: Micro-Homogeneity Studies of NBS Standard Reference Materials, NBS Research Materials, and Other Related Samples, NBS Spec. Publ. 260-65 (September 1979). \$3.50* SN-003-003-02114-1
- Venable, W. H., Jr. and Eckerle, K. L., Standard Reference Materials: Didymium Glass Filters for Calibrating the Wavelength Scale of Spectrophotometers (SRM 2009, 2010, 2013), NBS Spec. Publ. 260-66 (in press).
- Velapoldi, R. A., Paule, R. C., Schaffer, R., Mandel, J., Murphy, T. J., and Gramlich, J. W., Standard Reference Materials: A Reference Method for the Determination of Chloride in Serum, NBS Spec. Publ. 260-67 (in press).

* Send order with remittance to: Superintendent of Documents, US Government Printing Office, Washington, DC 20402. Remittance from foreign countries should include an additional one-fourth of the purchase price for postage.

** May be ordered from: National Technical Information Services (NTIS), Springfield, Virginia 22151.

TABLE OF CONTENTS

	PAGE
I. INTRODUCTION.	2
II. DEVELOPMENT OF THE SERUM CHLORIDE REFERENCE METHOD.	4
A. Organization.	4
B. Participating Laboratories, Standards, Serum Samples, and Definitive Method.	7
C. Functions of the Various Groups	10
D. Plan for Testing the Candidate Reference Method.	12
III. REFERENCE METHOD PROTOCOL FOR THE DETERMINATION OF SERUM CHLORIDE	14
A. General	14
B. Protocol Synopsis	14
C. Detailed Protocol	15
IV. RESULTS AND STATISTICAL ANALYSIS.	29
A. Interlaboratory Exercise Results.	29
V. DISCUSSION.	56
A. Candidate Protocol.	56
VI. CONCLUSIONS	60
VII. REFERENCES.	62
APPENDIX A.	65
APPENDIX B.	66
APPENDIX C.	68
APPENDIX D.	78

LIST OF TABLES

TABLE NO.	PAGE
1. Preliminary results from NBS comparing the coulometric-amperometric (C-A) and IDMS techniques for the determination of serum chloride.	6
2. Chloride concentrations for the seven serum pools as determined by IDMS, the definitive method. .	10
3. Sodium chloride standard solutions.	18
4. Serum chloride concentrations reported by the participating laboratories for the Preliminary Interlaboratory Exercise.	31
5. Concentration of serum chloride reported by the participating laboratories for Interlaboratory Exercise I, micro- and macropipetting protocols.	34 & 35
6. Concentration of serum chloride reported by the participating laboratories for Interlaboratory Exercise II, micropipetting protocol.	38 & 39
7. Concentration of serum chloride reported by the participating laboratories for Interlaboratory Exercise II, macropipetting protocol.	40
8. Percent deviations from averages for chloride in serum from Interlaboratory Exercise II, micropipetting protocol	43
9. Percent deviations from averages for chloride in serum from Interlaboratory Exercise II, macropipetting protocol	44
10. Ratios of standard deviations to average standard deviation for chloride in serum from Interlaboratory Exercise II, micropipetting protocol . .	45
11. Ratios of standard deviations to average standard deviation for chloride in serum from Interlaboratory Exercise II, macropipetting protocol . .	46
12. Components of standard deviation in mmol/L for all Interlaboratory Exercise II chloride ion levels (79-117 mmol/L)	48

LIST OF TABLES (continued)

TABLE NO.		PAGE
13.	Summary of imprecision and bias results in mmol/L for chloride ion in serum, Interlaboratory Exercise II	50
14.	Summary of chloride ion in serum values ± 2 standard errors	51
15.	Calibration curve data for chloride in serum, Interlaboratory Exercise II, micropipetting protocol.	53
16.	Calibration curve data for chloride in serum, Interlaboratory Exercise II, macropipetting protocol.	54
17.	Calibration curve results for chloride in serum as standard deviation of fit (s_{fit}) in mmol/L .	55
18.	Instruments, pipets, and various protocol parameters used by the participating laboratories in Interlaboratory Exercise I and Interlaboratory Exercise II	58

LIST OF FIGURES

<u>FIGURE NO.</u>	PAGE
1. Interrelationships and functions of the various groups in the development of a clinical reference method for the determination of serum chloride.	11
2. Typical calibration curve for the determination of serum chloride by a coulometric-amperometric technique	25
3. Percent deviation of individual results from the collective average of the measurements obtained in the Preliminary Interlaboratory Exercise . .	32
4. Percent deviations of the Interlaboratory Exercise I measurements using micro- and macropipetting from the definitive method values.	36
5. Percent deviations of the Interlaboratory Exercise II measurements using micro- and macropipetting from the definitive method values.	41

ABSTRACT

Guided by a committee of experts in clinical chemistry, a reference method was established for the determination of serum chloride based on a coulometric titration-amperometric end-point determination (C-A). Its accuracy was evaluated by comparing the values obtained by use of the method in 14 laboratories against the results obtained by a definitive analytical method based on isotope dilution-mass spectrometry (IDMS). Seven serum pools with chloride concentrations in the range 79.2 to 116.8 mmol/L were analyzed. Micro- and macropipetting alternatives were tested using sample sizes of 0.010-0.100 and 5.0 mL, respectively.

The laboratories used several different C-A instruments. The results showed that the standard error for a single laboratory's performance of the procedure was approximately 1.0 mmol/L with a maximum bias of 0.5 mmol/L over the range of concentrations studied. These values are within the accuracy and precision goals that had been set by the committee. The results from the micro- and macropipetting techniques were similar. The calibration curve data showed excellent linearity over the total concentration range, with 12 of 14 curves having standard deviations of fit of less than 0.80 mmol/L.

With appropriate experimental design, the reference method may be used to establish the accuracy of field methods as well as to determine reference chloride values for pooled sera.

Key Words: Amperometry; chloride analysis; clinical analysis; clinical chemistry; coulometry; definitive method; electrolytes; reference method; serum chloride analysis.

I. INTRODUCTION

Chloride, an electrolyte commonly analyzed in serum, plays an integral role in the assessment of acid-base imbalance, in calculating the anion gap, and acts as a secondary indication of changes in other electrolyte concentrations [1]⁵. An excess concentration of chloride in perspiration is indicative of the disease cystic fibrosis [2].

Serum chloride has been determined by a wide range of analytical methods; these include gravimetry, photometry, iodometry, titrimetry, electrometry, conductometry, and polarography as well as isotope dilution, indirect flame emission photometry, and atomic absorption [3]. In general, all these procedures suffer from interference from the presence of bromide ion, and care must be taken in interpreting analytical results for patients who may have elevated levels of serum bromide [4].

Three analytical techniques have been suggested as standard procedures. They are: a mercurimetric determination using diphenyl carbazone as an indicator [5]; an argentimetric determination using dichlorofluorescein as an indicator [6]; and a procedure developed by Cotlove based on established principles of coulometric generation of titrant (Ag^+) and amperometric indication of the end point [7]. Whether any of these methods should be considered by clinical laboratories as the clinical reference method for serum chloride has not been proven; the accuracy of none of these methods is known.

Two approaches may be used for establishing the accuracy of analytical methods. In the first, the results obtained from the methods in use for that analyte are compared using typical samples and selected samples containing known interferences for the analyses. Statistical correlations are used

⁵The bracketed numerals refer to the references listed at the end of this paper.

to express the interrelationships of the methods. A technique is then considered to be accurate to the degree established by knowledge of the sources of error and the agreement of results. In the second, a single candidate method is selected (possibly the 'best' of the methods recognized by the first approach) and studied in detail. Each step of the candidate method is optimized and examined so that the systematic and the random errors can be quantitatively expressed.

Studies have been organized using a combination of these approaches to establish the accuracies of clinical chemistry methods for total calcium, sodium, and potassium in serum [8,9,10]. For calcium, the analytical procedure was based on the flame atomic absorption spectrometric method of Pybus, Feldman, and Bowers [11], while for sodium and potassium the method was based on flame atomic emission spectrometry. The accuracies of these methods were assessed by using them on several human serum pools for calcium and bovine serum pools for sodium and potassium in selected clinical laboratories and comparing the results obtained against those obtained for the same pools by isotope dilution-mass spectrometry (IDMS) methods for calcium and potassium and an ion-exchange - gravimetry method for sodium. These analyses were performed at the National Bureau of Standards (NBS) where the high accuracy of those methods⁶ were established by determining their systematic and random errors [12].

These studies, carried out with the guidance of clinical laboratory experts, used (a) Standard Reference Materials [13] as the pure, primary reference material to prepare standard solutions of calcium, sodium, and potassium for all the analyses; (b) serum pools prepared at the Hartford Hospital (Hartford) and/or the Center for Disease Control (CDC,

⁶Such methods are referred to as definitive methods because of their high accuracy and utility for evaluating the accuracy of a candidate reference method.

Atlanta); (c) definitive method analyses for calcium, sodium, or potassium at NBS; (d) statistical analysis of the data at NBS; and (e) accuracy and precision goals as performance standards that the methods would have to meet to be recommended as the clinical reference method for total calcium [14], sodium, or potassium [15] in serum.

This same approach was adopted to develop clinical reference methods for a number of other serum electrolytes including chloride, lithium, and magnesium. The work was begun with the cooperation of individuals from the Standards Committees of the American Association for Clinical Chemistry (AACC) and the College of American Pathologists (CAP), the CDC and the NBS. The Food and Drug Administration (FDA) provided major support for the NBS work. The progress of this program was reported regularly to the AACC Standards Committee. We present in this report the development of a clinical reference method for serum chloride.

A proposed reference method for both sodium and potassium in serum using similar methodologies but without interlaboratory exercises has been reported recently [16].

II. DEVELOPMENT OF THE SERUM CHLORIDE REFERENCE METHOD

A. Organization

A panel of experts in clinical chemistry was invited to meet at NBS in March 1974 to consider the development of reference methods for five serum electrolytes, namely, chloride, potassium, sodium, lithium, and magnesium. The overall program for the development of these reference methods was organized by Dr. Robert Schaffer (NBS) and Dr. Rance A. Velapoldi (NBS). The invited experts were Dr. George N. Bowers, Jr. (Hartford Hospital), Dr. Bradley E. Copeland (New England Deaconess Hospital),

Dr. Denis O. Rodgerson (Center for Health Sciences, University of California in Los Angeles), and Dr. James M. White⁷ (CDC).

Prior to the meeting, several bovine serum pools prepared at the CDC had been analyzed for chloride by a coulometric-amperometric technique and by IDMS. The results, summarized in Table 1, were presented at the meeting as follows:

coulometric-amperometric (C-A)⁸ as obtained at NBS using commercial instrumentation by Dr. R. A. Durst; and IDMS as obtained at NBS by Mr. T. J. Murphy. On consideration of 1) the quite similar analytical results in Table 1, 2) alternative clinical laboratory procedures, and 3) instrumentation available in most clinical laboratories, it was concluded that the coulometric-amperometric technique using commercial instrumentation for the determination of serum chloride was the appropriate candidate methodology to evaluate as the reference method and that its evaluation should be made using IDMS as the definitive method.

⁷Dr. James White died after this program was well underway. He was recommended for membership on this Experts Committee on electrolytes by Dr. Joseph H. Boutwell (CDC). Dr. White made significant contributions to the development of the reference methods. His knowledge, advice, and cooperation in all phases of this work contributed greatly to the success of the program.

⁸The end point may be determined potentiometrically; however, for simplicity, the procedure will be represented by the letters C-A.

Table 1. Preliminary results from NBS comparing the coulometric-amperometric (C-A) and IDMS techniques for the determination of serum chloride.

<u>Pool</u>	Cl in Serum, mmol/L	
	<u>IDMS^a</u>	<u>C-A^b</u>
1	79.2	79.8
4	101.8	100.8
7	116.8	115.3

^aData from T. J. Murphy (NBS).

^bData from R. A. Durst (NBS).

The experts agreed to serve as the Committee to oversee the development of the reference method for chloride (as well as for the other electrolytes discussed at the meeting). The Committee chose Dr. Bowers as chairman. Dr. Copeland agreed to serve as the Committee's representative to work with those at NBS who would be involved in writing the protocol for the chloride reference method. The Committee agreed that the coulometric method should use a concentration bracketing technique rather than calibration curves for determining chloride concentrations. However, calibration curve data should be obtained as a general check on the measurement system and to determine which of the primary standard solutions would be used to bracket the chloride levels in the samples being analyzed.

As goals for the candidate reference method, the maximum bias of the method and its one-standard deviation imprecision limit were set by the Committee at 2.0 and 1.5 mmol/L, respectively, for serum chloride at the 100.0 mmol/L level. These goals were to be achieved by controlled, interlaboratory

tests involving a selected group of clinical chemistry laboratories which would perform the analyses by the C-A method according to the written protocol. NBS would provide chloride values by the definitive method.

B. Participating Laboratories, Standards, Serum Samples, and Definitive Method

The laboratories that were asked to participate in the interlaboratory study were chosen to represent a wide spectrum of clinical chemistry interests and included government (federal and state) and hospital laboratories, and laboratories associated with suppliers of instruments and of test and control materials. Two hospitals were located outside the United States. The principal investigators at these laboratories are named in the list below. Other scientists in each of the laboratories who contributed to this study are acknowledged by name in Appendix A. The list includes three laboratories that participated only in the concluding interlaboratory work. They were added to maintain a minimum number of laboratories when some of the original laboratories were unable to continue their participation. In alphabetical order of the principal investigator, the laboratories that participated in the interlaboratory studies are:

Dr. George N. Bowers, Jr.

Dr. Robert W. Burnett

Hartford Hospital

Hartford, CT 06115

Dr. Bradley E. Copeland

New England Deaconess Hospital

Boston, MA 02215

Dr. Richard A. Durst
National Bureau of Standards
Washington, D. C. 20234

Dr. Gordon Edwards
Dade Division
American Hospital Supply Co.
Miami, FL 33152

Dr. Lorentz Eldjarn
Dr. Johan Kofstad
Rikshospitalet, University of Oslo
Oslo, Norway

Dr. Nathan Gochman
Veterans Administration Hospital
San Diego, CA 92161

Mr. Cecil Hassig
American Instrument Co.
Silver Spring, MD 20910

Dr. Denis O. Rodgerson
Center for Health Sciences, University of California
Los Angeles, CA 90025

Mr. William Ryan
Beckman Instruments
Fullerton, CA 92634

Mr. Leonard Sideman
Department of Health
Philadelphia, PA 19130

Dr. Barbara Tejeda
Food and Drug Administration
Washington, D. C. 20250

Dr. Thomas Tracey
Technicon, Inc.
Tarrytown, NY 10591

Dr. James M. White
Dr. Richard Carter
Center for Disease Control
Atlanta, GA 30333

Dr. Charles E. Willis
College of American Pathologists, Cleveland Clinic
Cleveland, OH 44106

NBS Standard Reference Material Sodium Chloride (SRM 919, see Appendix B) was to be used as the pure, primary reference material for all analyses [13]. Seven pools of homogeneous, sterile, bovine serum having different concentrations of chloride, were prepared at the CDC by Dr. David Bayse and Ms. Sue Lewis. Samples of each pool were supplied in approximately 7-mL volumes in sealed vials that were labeled with computer-generated random numbers. The samples, packed in dry ice, were shipped to NBS by air and within 24 h of packing were placed in freezers kept at -50 °C [17]. The pools were numbered in code from 1 to 7 according to increasing chloride concentration.

A definitive method based on IDMS was developed at NBS and is given in Appendix C. The chloride concentrations for the seven serum pools were determined by this procedure and the results obtained are summarized in Table 2.

Table 2. Chloride concentrations for the seven serum pools as determined by IDMS, the definitive method.

<u>Pool</u>	<u>[Cl⁻], mmol/L</u>
1	79.2 ± 0.4 ^a
2	84.5 ± 0.4
3	94.0 ± 0.5
4	101.8 ± 0.5
5	107.2 ± 0.5
6	112.9 ± 0.6
7	116.8 ± 0.6

^aEstimated maximum error of 0.5 percent of the value as reported by NBS Analytical Mass Spectrometry Section. This estimated maximum error includes both imprecision and an estimated upper bound for possible systematic errors. The estimated maximum error is believed to be equal to or greater than the true error for the 95 percent confidence limits.

C. Functions of the Various Groups

The interrelationships and functions of the various groups involved in developing C-A as a reference method for serum chloride are represented in figure 1. The Committee, CDC, and NBS provided guidance and technical support for the program and also served as participating laboratories. The Experts Committee selected the candidate reference method, set maximum bias and imprecision goals for an acceptable reference method, assisted NBS in selecting other participating laboratories, and reviewed all analytical results. The CDC provided the serum pools. The participating laboratories provided the interlaboratory test data and critiques of the candidate reference method protocol.

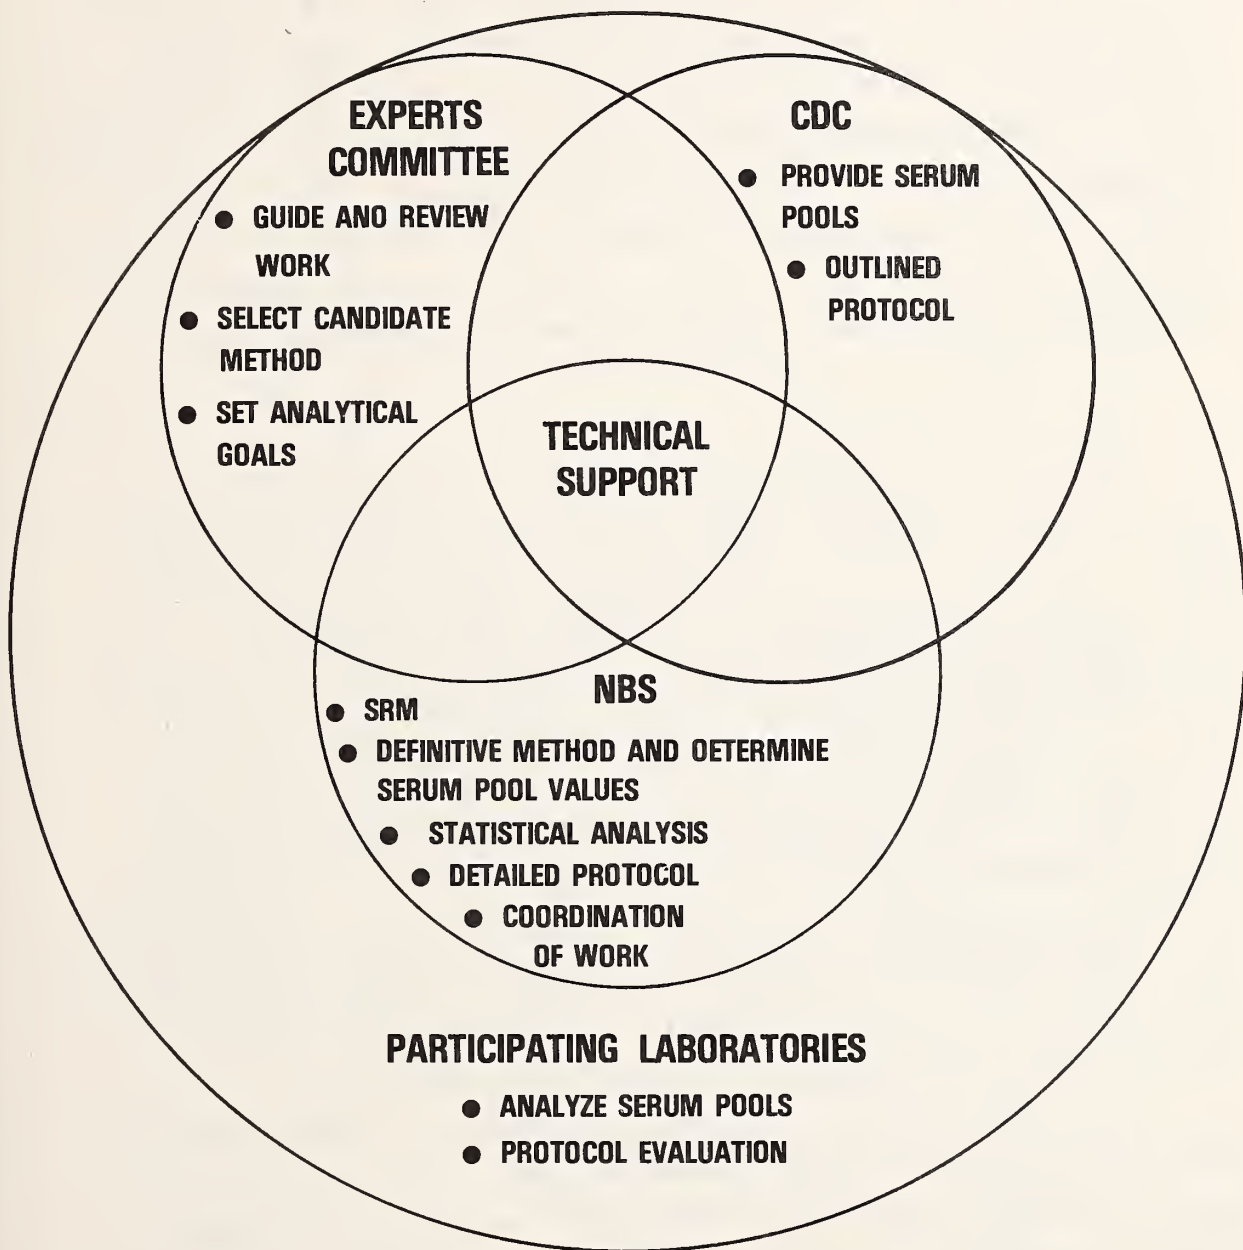


Figure 1. Interrelationships and functions of the various groups in the development of a clinical reference method for the determination of serum chloride.

At NBS, Dr. R. Schaffer served as the Reference Method Program Manager and Dr. R. A. Velapoldi served as the coordinator. The format of the interlaboratory exercises (IE)⁹ was established within the constraints imposed by protocol requirements and sample availability by Drs. John Mandel, Robert Paule, and Rance Velapoldi. Dr. Velapoldi wrote the protocol for the candidate reference method from the outline provided by Drs. B. Copeland and D. Grisley. Drs. Mandel and Paule performed the statistical evaluation of the results from the interlaboratory tests. The definitive method was performed by Mr. Thomas Murphy and Dr. John Gramlich.

D. Plan for Testing the Candidate Reference Method

The general plan was to evaluate the candidate reference method by performing a series of interlaboratory exercises, which would consist of a preliminary test (IE-P) followed by successive interlaboratory exercises until the goals for the reference method were reached. A main objective of the IE-P was to allow participating laboratories to become familiar with and comment on the protocol. Since an evaluation of the bias was not sought in the IE-P testing phase, normal bovine serum samples [18] not having definitive method analyses were to be used. However, interlaboratory imprecision was to be measured. If the imprecision of the results in the IE-P was found to be small, IE testing would begin on samples having definitive method chloride values.

In an IE, each participating laboratory would perform the same analyses on two separate days: i.e., analyze a pair of samples from each serum pool on each of two days where a minimum of one day or a maximum of seven days were to elapse between the two series of analyses. The bias and

⁹In previous reports, the Interlaboratory Exercises were called Round Robin Tests.

imprecision values obtained by statistical analysis would then be compared to the goals set by the Committee for the reference method. If the goals were not met, additional IE's using samples from other pools would be conducted by following the protocol or a modified form of it until the bias and imprecision goals were reached. Revisions and modifications to the protocol could be made after an inter-laboratory exercise had been completed but would not be made after the final IE.

Three kinds of information were to be supplied by each participating laboratory after finishing an interlaboratory exercise:

1. General Data — a list of the instrumental parameters used and comments on the protocol including problems encountered during the analysis;
2. Calibration Curve Data — a list of the 'instrumentally' measured mmol/L values¹⁰ versus the actual chloride concentrations of the standards calculated from the NaCl used; and
3. Valid Measurement Data — a list of the sets of data that constituted the three measurements on a single sample.

Examples of the data sheets on which the information was collected are shown in Appendix D, Note 8.

¹⁰These measured values also could have the units of time for coulometric production of the titrant.

III. REFERENCE METHOD PROTOCOL FOR THE DETERMINATION OF SERUM CHLORIDE

A. General

This protocol provides for the analysis of serum chloride by a coulometric-amperometric procedure using a micropipet to introduce the serum samples directly into the titration cup. A macropipetting and diluting procedure is also included as an alternative; however, the same instrumentation is used for the determination. Both procedures are to conform to the requirements of the instrumentation used.

B. Protocol Synopsis

The protocol must be followed exactly. The reference method is used to analyze four samples of a serum or pool: two on one day and the other two on a subsequent day. Approximately 2 mL of sample is required to carry out the micropipetting procedure while 25-40 mL is needed to carry out the macropipetting procedure.

1. Use an analytical balance to weigh the SRM NaCl in the appropriate quantity to prepare a stock standard chloride solution;
2. Use single or multiple micropipets or a single macropipet to transfer aliquots of the sample to the C-A titration cup or to dilute the aliquots to the levels used as working solutions of a) the serum, b) the stock standard chloride solutions, and c) the solution used as a blank;
3. Obtain calibration curve data on the working blank and standards;

4. Measure the C-A values on the working solutions of the serum sample; select the pair of working standards whose C-A values most closely bracket the value for each sample;
5. For each sample to be analyzed, obtain three valid measurement sets by measuring the C-A values obtained from repeated sequential measurements of the working solutions of the low bracketing standard, the aliquot of that sample, and the high bracketing standard;
6. Calculate the chloride concentration of the aliquot for each set by mathematical interpolation;
7. Average the three calculated values to obtain a 'single measurement' of that sample; (in the statistical analysis, each such average is designated a 'single measurement');
8. Perform steps (4) through (7) for each sample to be analyzed on the first day;
9. Repeat steps (1) through (8) on the subsequent day to obtain the second pair of measurements needed for each sample;
10. Average the four values obtained by the replicate determinations to obtain the chloride concentration for each serum pool.

C. Detailed Protocol

The selection of the specific alternatives of the protocol to be used dictates the glassware and diluent volumes needed. These needs are summarized in the protocol or in Appendix D notes. Stock solutions and working solutions are to be prepared at and maintained at a room temperature that is constant within ± 2 °C (see Appendix D, Note 1).

1. Reagent Specifications

- a. Water: At the time of preparation, the distilled and/or deionized water used should exhibit a specific resistance of at least $10 \text{ k}\Omega\cdot\text{m}$ at $23 \pm 2 \text{ }^\circ\text{C}$. At the time of use, titration of this water should show a C-A value that is less than 0.1 percent of full scale at the instrumental settings used for the analysis. A large quantity of this water (more than 10 L) must be available for use as diluent and for the final rinsings of all glassware and other apparatus that come in contact with the solutions involved. Unless specified otherwise, the water referred to in this protocol is this tested water.
- b. Chloride Standard Solutions: Use Standard Reference Material Sodium Chloride (originally issued as SRM 919, Certificate reproduced in Appendix B) [13] certified by the National Bureau of Standards. The SRM NaCl should be dried at $110 \text{ }^\circ\text{C}$ for four hours in a loosely capped container and then stored in a desiccator containing CaSO_4 or an equivalent desiccant.
- c. The supporting electrolyte constituents used are specified in the instruction manual for the particular instrument used.
- d. Nitric acid, chloroform, methanol and 95-percent ethanol conforming to ACS [19] (or equivalent) specifications are to be used.

2. Glassware Specifications

- a. Volumetric glassware (Appendix D, Note 2) should be of borosilicate material and meet NBS Class A [20] or equivalent specifications.

- b. The micropipets should have the following accuracy tolerances:

<u>Volume (μL)</u>	<u>± 3 S.D. (μL)</u>
20	0.24
100	1.4

(Examples of appropriate micropipets are: Clay-Adams, Parsippany, New Jersey 07054, Number 4625 for the 100 μL pipet and Number 4618 for the 20 μL , see footnote 11, p. 57.)

All glass or plastic surfaces that come into contact with reagents, water, diluent, sample, or supporting electrolyte must be clean (Appendix D, Note 3).

3. Preparation of Reagents

- a. Chloride Standard Stock Solutions: Prepare standard solutions with nominal chloride concentrations of 75-, 90-, 100-, 110-, and 125-mmol/L. Weigh accurately (to 0.1 mg) approximately 1.09, 1.32, 1.46, 1.61, and 1.83 g of dried SRM NaCl (MW = 58.44277, Appendix D, Note 4) and transfer each quantitatively into separate, appropriately labelled, 250-mL volumetric flasks. Dissolve the NaCl using approximately 100 mL of water. Fill flasks to the calibrated volume with water, stopper, and mix by inverting the flask and shaking ten times. Repeat flask inversion and shaking ten times. Calculate the concentration of the NaCl solutions in mmol/L to two decimal places according to the exact weights of sodium chloride used, and record these values on the data sheets; an example of this step is given in Table 3.

Table 3. Sodium chloride standard solutions.

<u>Solution</u>	<u>(NaCl)^a, mmol/L</u>	<u>NaCl, g</u>
1	75.00	1.0958
2	90.07	1.3150
3	100.12	1.4628
4	110.09	1.6085
5	125.10	1.8278

^aThe NaCl concentrations were calculated using atomic weights from the literature reference cited in Appendix D, Note 4.

- b. Supporting Electrolyte Solution Follow the instrument manufacturer's instructions for the preparation of the supporting electrolyte.
- c. Dilute Nitric Acid (0.77 mol/L): Prepare by making a twenty-fold dilution of concentrated nitric acid (15.4 mol/L) with water.

4. Pipetting and Dilution Procedures

- a. For Instruments in Which Microvolumes of Sample are Added Directly to the Titration Cell
- (1) Micropipetting of Solutions, General: Several types of micropipets may be used including those in which the solutions are drawn up by capillary action or suction (aspirator or plunger). Micropipets are to be used with a wash-out technique. If all micropipets meet the accuracy specifications given in Section IIIC-2, then different micropipets may be used for solutions of blank, standard, and sample; if they do not meet these specifications, a single micropipet must be used throughout. In

the latter case, the micropipet must be cleaned as described in Appendix D, Note 3, or if this micropipet employs a plunger with a positive displacement that ejects all of the aliquot, the pipet must be rinsed with the solution by filling and expelling three times with some of the solution transferred for this purpose to a separate container.

- (2) Micropipetting Technique: Fill the micropipet by immersing the tip just below the surface of the solution and tilting the micropipet so that the solution is drawn up the bore. Stop filling the capillary at the calibrated mark. Withdraw the pipet from the solution. Wipe the exterior wall of the micropipet with clean absorbent paper taking care to avoid contact with the delivery tip. Deliver the aliquot to the sample cell by immersing the tip of the micropipet just below the surface of the supporting electrolyte and gently expel all of the sample from the micropipet by blowing. Alternatively, the solution is carefully ejected by use of the plunger. Check to see that the plunger has ejected all of the solution. Before raising the micropipet tip from the electrolyte solution in the cell, the micropipet is rinsed with the supporting electrolyte-sample mixture by drawing the mixture into the micropipet to the calibrated mark and expelling back into the sample cell. (NOTE: Do not immerse the micropipet deep into the supporting electrolyte-sample mixture and do not wipe off the exterior wall of the micropipet as previously done.) Repeat this rinse operation twice more.

- b. For Instruments Which Require Samples that are Prediluted with Supporting Electrolyte: The solution used for measurement must contain a silver chloride dispersant for smooth titration performance. Directions for the preparation and addition of the dispersant are found in the manufacturer's instruction book for the instrument.
- (1) Macropipetting and Diluting, General: To prepare working solutions, the blank, stock standard, and serum solutions are diluted fifty-fold with supporting electrolyte solution (Section IIIC-3b) using a 5-mL pipet with a wash-out technique ("to contain" mode). Only one volumetric pipet is used and the wash-out technique is employed throughout to avoid errors that may arise due to differences in pipet volumes and delivery times.
- (2) Macropipetting and Diluting Using the Wash-Out Technique: Transfer approximately 200 mL of the supporting electrolyte solution to a 250-mL volumetric flask. Then add 5 mL of the appropriate solution by the following procedure. Fill the 5-mL pipet to approximately 1 cm above its calibration mark, withdraw the pipet from the container, and wipe the delivery tip with clean, absorbent paper. Contact the tip of the pipet to the side of a clean waste container, and allow excess solution to drain until the meniscus is at the calibrated mark on the pipet. Remove the pipet from contact with the container and direct the delivery tip of the pipet into the receiver. Deliver the sample by contact of the pipet tip with the wall inside the volumetric flask and allow the solution to drain fully. After drainage stops, gently expel the residual liquid. Rinse the pipet by lowering the pipet tip into the

solution within the flask and refill the pipet with solution to approximately 1 cm above the mark. Allow the solution to drain fully and gently expel residual liquid. Repeat the pipet rinsing two more times. Finally wash the pipet tip with approximately 4 mL of fresh supporting electrolyte solution using a wash bottle or a clean, disposable Pasteur pipet. (NOTE: New, disposable pipets should be cleaned before use.) Fill the flask to the calibrated volume with the electrolyte solution. Mix thoroughly by inverting the flask and shaking ten times. Repeat the inversion and shaking procedure ten times.

(3) Preparation of Working Solutions:

(a) Working Blank Solution and Working Standard Solutions: Prepare the working solutions of the blank solution and the working 75.0-, 90.0-, 100.0-, 110.0-, and 125.0- mmol/L chloride standard solutions by making dilutions in appropriately labeled volumetric flasks in the order cited. Condition the 5-mL pipet by filling it with the solution to be diluted. Discard this pipetful and repeat filling and discarding twice more. Then refill the pipet with the solution, adjust to the calibrated volume, and deliver into the volumetric flask to be used for the dilution. Rinse the pipet by filling it three times with the supporting electrolyte solution, each time delivering the rinse solution into the volumetric flask. Fill the flask to the calibrated volume with the electrolyte solution. Wash out the pipet three times with water (see Appendix D, Note 5) and expel the residual liquid.

(b) Working Sample Solutions: If at least 10 mL of serum sample is available, condition the 5-mL pipet with some of the sample to be diluted in the

following way: (1) Draw 1-2 mL of the sample into the pipet, (2) withdraw the pipet from the container, (3) wipe off the tip with a clean, absorbent paper, (4) tilt the pipet to a horizontal position, (5) allow a small volume of air to leak in and rotate the pipet so that the conditioning liquid wets all the internal surface to approximately 0.5 cm above the calibration mark, (6) discard this conditioning solution, and (7) repeat steps (1-6). Then prepare the working solutions as described in sections IIIC-4b-(2), fill the 5-mL pipet with the sample, adjust volume to the mark, deliver, rinse three times into the volumetric flask with supporting electrolyte, dilute to the calibrated volume, and mix. Finally, wash out the pipet three times with water (Appendix D, Note 5). For each of the next sample solutions to be diluted, repeat step IIIC-4b-(3)(b).

If between 5 and 10 mL of each sample is available, a dry, 5-mL pipet must be used for each sample since this volume of serum is insufficient for the pipet-conditioning technique described above. In this case, fill the clean, dry, 5-mL pipet with the serum sample, adjust to volume, deliver and rinse into the receiver, and dilute. Clean the pipet for the next sample by washing the pipet with dilute HNO_3 , rinse with a minimum of four portions of water and finally rinse twice with 95 percent ethanol. Allow the pipet to drain. Apply minimum suction to the top end of the pipet for one minute to remove any remaining ethanol. The pipet is then ready for use with the next serum sample. (NOTE: If the dilute HNO_3 washings do not drain cleanly from the pipet, wash the pipet as described in Appendix D,

Note 5. Then follow with the ethanol wash as above.) Prepare the working solutions as above.

- (4) Solution Transfer to Sample Cell; Macropipetting in the 'To Deliver' Mode, General: Different 4-mL pipets may be used for the transfer of the working low standard, the working sample, and the working high standard solutions to the sample titration cell. Condition the pipet as described in IIIC-4b-(3). Fill the pipet by the procedure described in IIIC-4b-(2). Deliver the solution into the clean sample titration cell by allowing the pipet to drain with the tip against the side of the sample cell. (NOTE: As a minimum, allow the pipet to drain for the delivery time inscribed on the pipet.) After drainage is complete, remove the pipet and proceed with the titration. This pipet may be used for further transfers of the same solution after rinsing once with the solution to be transferred. Keep each of the three pipets used for the transfer of the working low standard, working sample, and the working high standard separate to prevent cross-contamination of solutions. After each titration, clean the sample cell and electrodes by rinsing them three times with water.

5. Coulometric-Amperometric Titration Procedure

It is not possible to provide detailed instructions for each type of instrument to assure necessary instrument stability, linearity, titration conditions, etc. The operator must be familiar with the instrument used. The instrument should meet all the manufacturer's specifications. In general, the accuracy of the method cannot be attained unless the instrument is in optimum operating condition.

a. Determination of Standard Curve for Instruments with Direct Concentration Readout

- (1) Calibrate the system with the 100 mmol/L chloride standard according to the instructions for the particular instrument.
- (2) Titrate ten samples of the 100 mmol/L standard. Calculate the mean and standard deviation of the values. The mean value should be within 0.5 mmol/L of the value calculated from the amount weighed. If this value is exceeded, recalibrate. The standard deviation should not exceed 1 mmol/L.
- (3) Titrate five samples of each of the approximately 75-, 90-, 110-, and 125-mmol/L standards in the same manner as in step (2) above. The range of values for the 75- and 90-mmol/L solutions should not exceed 2 mmol/L and for the 110- and 125-mmol/L standard should not exceed 4 mmol/L. If these ranges are exceeded, recalibrate and repeat (2) above. The mean values for all the standards should be within 0.5 mmol/L of the calculated value. On the data sheet provided, record the standard solution concentrations in mmol/L to 2 decimal places and the experimentally obtained values to at least one decimal place.
- (4) A typical calibration curve is shown in figure 2.

b. Calibration for Time Readout Instruments Which Measure Samples Prediluted with Supporting Electrolyte:

- (1) Titrate reagent blanks in triplicate and calculate the average time of titration (\bar{B}).
- (2) Titrate ten samples of the approximately 100 mmol/L working standard. Calculate the gross mean standard

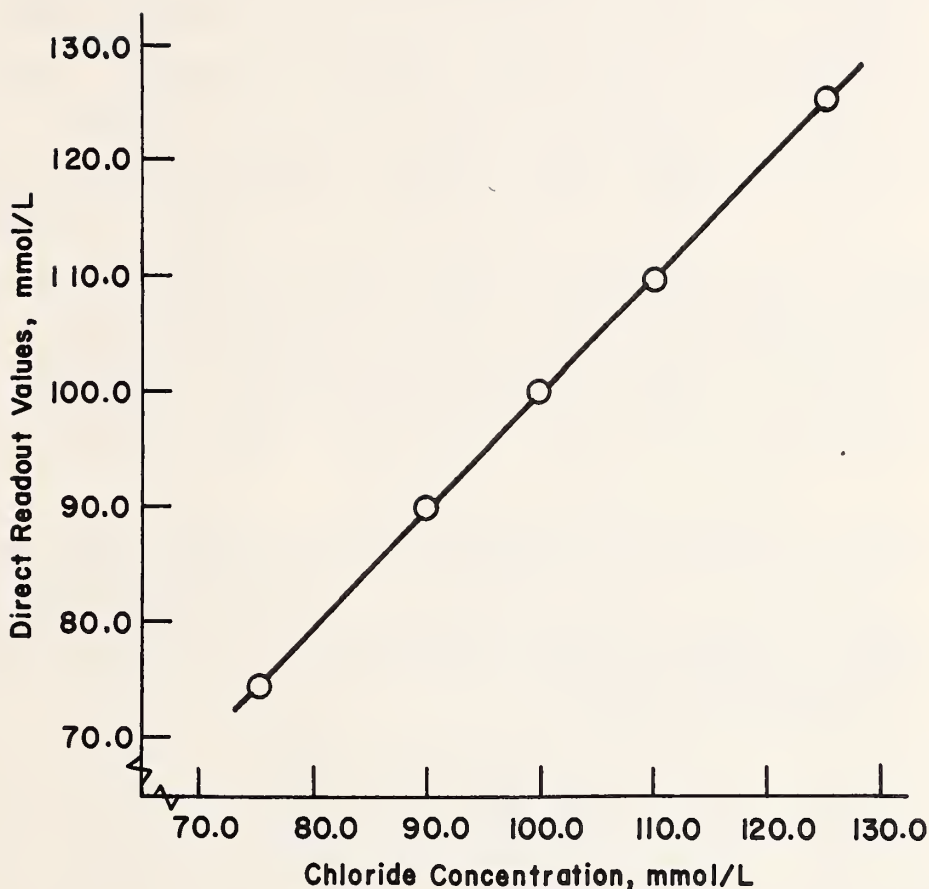


Figure 2. Typical calibration curve for the determination of serum chloride by a coulometric-amperometric technique.

time (\overline{GS}_{100}) and standard deviation of the time of titration. The standard deviation should be within 0.4 second.

- (3) Calculate the net mean standard time (\overline{NS}) by:

$$\overline{NS}_{100} = \overline{GS}_{100} - \overline{B} \quad (1)$$

- (4) Titrate five samples of the approximately 75-, 90-, 110-, and 125-mmol/L standards. Calculate the gross mean standard times. For \overline{GS}_{75} , \overline{GS}_{90} , \overline{GS}_{110} , and \overline{GS}_{125} , the values for the standard deviations should not exceed 0.5 seconds. If this limit is exceeded, trouble-shoot the system. Calculate \overline{NS}_{75} , \overline{NS}_{90} , \overline{NS}_{110} , and \overline{NS}_{125} as in (3) above and record the data on the sheet provided.
- (5) Plot on rectilinear graph paper the \overline{NS} values as ordinate versus the corresponding calculated standard concentrations expressed in mmol/L of chloride. The plot should be linear passing through the origin ± 1 second.
- c. The standard deviation of fit for both types of readouts can be calculated from the deviations, d_i , of the N points from the least squares fitted calibration line:

$$s_{\text{fit}} = \sqrt{\sum_{i=1}^N (d_i^2) / (N-2)}. \quad (2)$$

If on visual inspection, one point of the plot exhibits a large residual from a smooth curve drawn through the remaining points, remeasure that standard solution. If the remeasured value for the solution continues to exhibit the large deviation, prepare that standard solution again, remeasure it, and compare the values obtained.

d. Sample Measurements

(1) Transfer the working sample to the sample titration cell by the appropriate pipetting technique. Titrate the working sample solution and select the two working standard solutions whose direct readout values or titration times most closely bracket that of the sample.

(2) Titrate the lower working standard, the working sample, and the higher working standard in that order and record each reading in the set.

(3) Repeat step d(2) until 3 'sets' of data are obtained.

(4) Repeat steps d(1), (2), and (3) for all of the samples.

(5) If one chloride value (working standard or working sample) in the measurement format is wrong due to a known error in technique, it may be disregarded and a repeat titration for that particular solution should be run immediately. However, if one chloride value appears to be in error and cannot be excluded due to known faulty technique, report that set of values. A repeat of the measurement format should be run for that particular working sample and both formats are to be reported with appropriate explanation.

e. Data Recording and Calculations

(1) On the data sheet, record the concentrations of the standard solutions in mmol/L of chloride to two decimal figures and the corresponding instrument readings to as many decimal places as possible.

(2) Calculate the concentration \hat{C} of chloride present in the sample in mmol/L by mathematical interpolation as follows:

$$\hat{C} = C_1 + \frac{(C_2 - C_1)(Y - X_1)}{(X_2 - X_1)} \quad (3)$$

where

\hat{C} is the sample concentration of chloride in mmol/L,

C_1 is the low standard concentration of chloride in mmol/L,

C_2 is the high standard concentration of chloride in mmol/L,

Y is the chloride concentration in mmol/L or the titration time for the working sample minus the blank,

X_1 is the chloride concentration in mmol/L or the titration time for the low working standard minus the blank, and

X_2 is the chloride concentration in mmol/L or the titration time for the high working standard minus the blank.

(3) Record the \hat{C} calculated values to a minimum of two decimal places in the column provided on the data sheet.

(4) Average the results for the three aliquots of the serum analyzed to obtain the 'single measurement' value. (See Section IV.)

(5) Average the four single measurement values to obtain a chloride value for the serum pool analyzed.

IV. RESULTS AND STATISTICAL ANALYSIS

The main objective of the statistical analyses of the round robin data is to derive measures of precision and accuracy for the micro- and macropipetting versions of the reference method. Precision is characterized by the variability of the protocol measurements within a single laboratory, $\hat{\sigma}_{\text{within}}$, and by the total variability of a laboratory's protocol measurements, $\hat{\sigma}_{\text{total}}$. This latter uncertainty includes the variability of 'between laboratory' measurements. Accuracy relates to the comparison between reference method and definitive method values and is related to the magnitude of the bias.

Each reported data point (test result) is the end product of three sets of data, the number of sets specified by the protocol. For simplicity of discussion, each reported data point is referred to as a single measurement, meaning that each is the product of a single run-through of the protocol. When "replication" is mentioned, replication of the entire protocol process is meant, and "replication error" thus refers to the variability among the end results of repeated run-throughs of the protocol. Each interlaboratory exercise is discussed separately; the final, detailed statistical analysis is reported for the results from IE-II.

A. Interlaboratory Exercise Results

1. Preliminary Interlaboratory Exercise (Dates Run: April-August 1975).
 - a. Objectives: To allow the participating laboratories to become familiar with and comment on the protocol and to determine interlaboratory precision.

- b. Samples: Three vials, each containing a sample from the same serum pool. Each participating laboratory was to analyze a single portion of each sample within one day.
- c. Procedure: The micro- or macropipetting protocol was used.
- d. Data: The three data points reported by the individual laboratories are summarized in Table 4. The data are presented graphically in figure 3 as the percent difference from the collective average of the reported values. Essentially all reported values are within three percent of the collective average of 103.9 mmol/L with a relative standard deviation (CV) of less than two percent.
- e. Comments and Protocol Deviations: The following laboratory comments or protocol deviations were received:
 - (1) Lab 3: Schales-Schales titration procedure used rather than C-A procedure.
 - (2) Lab 4: Instrument designed for 1:40 dilution rather than 1:50 specified in protocol.
 - (3) Lab 8: The three samples were turbid. (Growth of microorganisms?)
 - (4) Lab 11: Stock standard solutions prepared in 500 mL quantities. Glassware cleaning done with detergents.
 - (5) Lab 13: Instrument designed for 1:100 dilution rather than 1:50 specified in the protocol.

- f. Direction: On examining these results with the statisticians and the Experts Committee, it was concluded that an interlaboratory exercise should be undertaken using samples with chloride concentration values determined by the definitive method.

Table 4. Serum chloride concentrations reported by the participating laboratories for the Preliminary Interlaboratory Exercise.

- - - - - [Cl], mmol/L ^a - - - - -				
<u>Laboratory</u>	<u>Vial 1</u>	<u>Vial 2</u>	<u>Vial 3</u>	<u>Laboratory Average</u>
1	105.0	104.7	105.3	105.0
2	102.0	100.3	100.7	101.0
3	105.0	103.7	105.0	104.6 ^b
4 ^c	104.5	104.7	104.9	104.7
5	101.1	103.3	104.5	103.0
6 ^c	103.5	103.7	104.6	103.9
7	105.6	105.6	104.2	105.1
8	103.2	104.1	103.5	103.6
9	104.5	104.3	104.2	104.3
10	102.0	104.0	103.7	103.2
11	101.7	102.0	102.7	102.1
12	104.7	105.7	105.0	105.1
13 ^c	104.4	104.6	105.3	104.8

^aEach value represents a single measurement on a sample.

^bSchales-Schales titration procedure was used. Value was not used to determine collective laboratory average.

^cMacropipetting procedure.

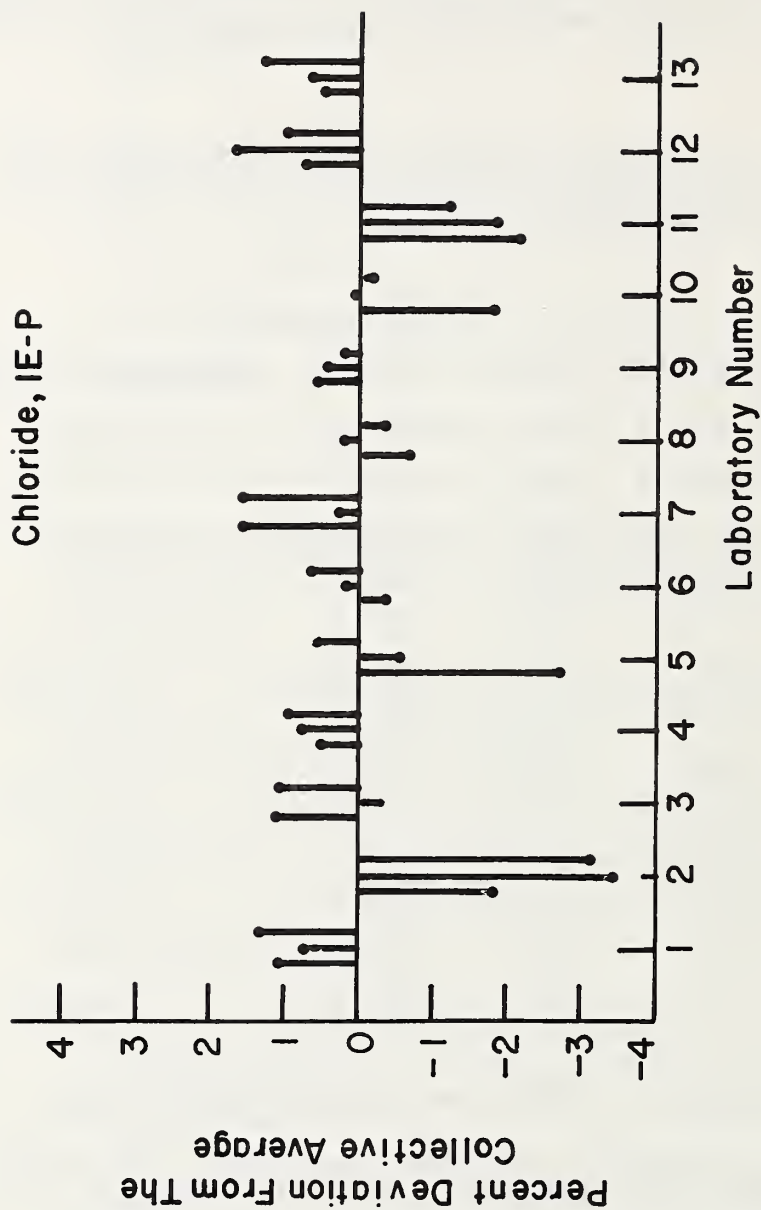


Figure 3. Percent deviation of individual results from the collective average of the measurements obtained in the Preliminary Interlaboratory Exercise.

2. Interlaboratory Exercise I (IE-I) (Dates Run: October-December 1975.)
 - a. Objectives: To test the micro- and macropipetting procedures on serum samples having a wider range of chloride values and to determine the imprecision and bias of the test results.
 - b. Samples: IE-I was a test series run on 12 samples — four vials (samples) of each of three different concentrations (Pools 2, 4, and 6). Each laboratory was to analyze two vials of each pool on one day and the remaining pairs of samples on a subsequent day with the requirement that a minimum of one day and a maximum of seven days should elapse between analyses.
 - c. Protocol: The micro- and macropipetting protocols were used.
 - d. Comments and Protocol Deviations: The following laboratory comments or protocol deviations were received:
 - (1) Lab 3: Schales-Schales titration procedure used.
 - (2) Lab 4: Used 1:40 dilution (instrument required) rather than 1:50 dilution.
 - e. Data: The single-measurement data reported by the laboratories for both pipetting alternatives are summarized in Table 5. The data are presented graphically in figure 4 as percent deviation of each one-day 'single measurement' average from the definitive method value. In general, the data reported by most laboratories were within three percent of the definitive method values. Most of the laboratories reported results that bracketed

Table 5. Concentrations of serum chloride reported by the participating laboratories for Interlaboratory Exercise I, micro- and macropipetting protocols.

- - - - - [Cl], mmol/L ^a - - - - -						
Laboratory	Pool 2		Pool 4		Pool 6	
	Day 1	Day 2	Day 1	Day 2	Day 1	Day 2
1	84.71	88.60	102.49	100.69	114.52	110.19
	89.40	79.89	101.53	99.26	120.04	109.84
2	82.67	81.00	100.00	100.33	110.00	109.67
	83.00	82.33	100.33	100.33	110.00	109.33
3 ^b	89.67	90.98	108.67	107.33	108.75	117.33
	89.37	89.67	105.86	108.28	116.67	117.12
4 ^c	84.35	84.55	101.43	101.62	112.15	113.53
	84.32	84.49	101.62	102.61	112.62	113.25
5 ^c	85.44	84.55	100.74	100.56	112.52	112.02
	84.52	83.44	100.52	101.26	113.28	110.97
6 ^c	83.91	85.52	102.56	101.86	112.81	114.55
	84.61	85.17	101.24	102.68	113.95	115.32
7	84.60	84.45	101.49	101.82	112.72	113.35
	84.68	84.90	101.63	102.82	114.47	113.63
8	85.66	83.96	102.27	101.61	113.30	113.24
	84.28	84.71	102.43	102.18	112.69	113.03
9	84.27	84.57	102.23	102.20	112.17	112.27
	84.57	84.93	99.80	101.87	112.63	112.03
10	84.83	84.67	102.80	102.17	113.17	113.67
	84.83	84.67	102.00	102.67	112.17	114.17
11 ^c	84.73	83.46	101.86	102.03	113.83	113.86
	84.78	83.46	103.62	102.24	116.29	112.78
12	85.37	84.53	102.40	102.10	114.27	112.33
	84.47	84.37	102.40	102.27	114.40	111.43
13	85.00	85.67	102.33	102.67	113.00	114.67
	85.33	85.67	102.33	103.00	113.33	114.67

continued


Table 5 (continued)

- - - - - [C1], mmol/L ^a - - - - -						
<u>Laboratory</u>	<u>Pool 2</u>		<u>Pool 4</u>		<u>Pool 6</u>	
	<u>Day 1</u>	<u>Day 2</u>	<u>Day 1</u>	<u>Day 2</u>	<u>Day 1</u>	<u>Day 2</u>
14	85.33	85.33	104.77	102.40	114.37	114.80
	85.37	84.73	104.37	102.77	116.43	113.77
15	84.61	84.77	102.29	102.13	113.28	113.19
	84.67	84.70	102.05	102.09	113.36	113.21
15 ^c	84.29	85.01	102.16	101.97	113.63	113.32
	84.63	85.19	102.14	101.95	113.41	113.21
Definitive						
Method Values	84.5		101.8		112.9	

^aEach value is the single measurement average of three C-A readings made on a single sample.

^bSchales-Schales titration method, data for comparison only.

^cMacropipetting protocol.

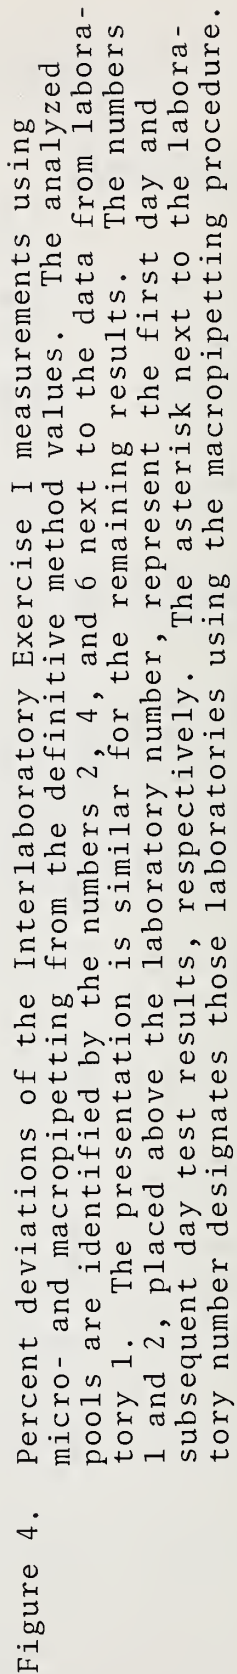

or were quite close to the definitive method values.

- f. Direction: A second Interlaboratory Exercise (IE-II) was to be run using both the micro- and macropipetting protocols. Test samples would cover the full range of chloride concentrations.
3. Interlaboratory Exercise II: (IE-II. Dates Run: February-April 1976.)
 - a. Objective: To test both the micro- and macro-pipetting alternatives of the protocol on samples with chloride concentrations over the nominal range of 79.2 to 116.8 mmol/L.
 - b. Samples: IE-II was a test series run on a total of 20 samples – four vials of each of five different chloride concentrations (Pools 1, 3, 4, 5, and 7). Each laboratory was to analyze two vials of each concentration on the first day and the remaining pairs of samples after the elapse of a minimum of one day and a maximum of seven days.
 - c. Protocol: The micro- and macropipetting versions of the protocol were used.
 - d. Data Statistical Analysis: Results from IE-II are given in Tables 6-7 and illustrated in figure 5.
 - e. Statistical Analysis: The data are presented as two-way tables in which the rows represent the different participating laboratories and the columns represent the different sample pools. The sample pool concentrations ranged from 79.2 to 116.8 millimoles of chloride ion per liter of serum. The results for the micropipetting procedure and for the macropipetting procedure are listed separately, and all single measurements reported

Table 6. Concentration of serum chloride reported by the participating laboratories for Interlaboratory Exercise II, micropipetting protocol.

- - - - - [Cl], mmol/L - - - - -					
<u>Laboratory^a</u>	<u>Pool 1</u>	<u>Pool 3</u>	<u>Pool 4</u>	<u>Pool 5</u>	<u>Pool 7</u>
1-1	79.53 80.05	94.70 94.77	102.38 102.65	108.57 108.47	117.21 117.74
1-2	80.32 80.14	93.57 95.45	103.20 102.31	107.91 108.16	117.28 117.64
2-1	77.00 76.75	91.60 90.70	99.60 101.70	106.62 104.90	116.10 113.90
2-2	76.36 77.94	92.10 92.66	99.95 99.95	104.52 106.10	114.20 115.00
4-1	79.37 79.95	94.88 94.28	101.90 101.82	108.00 107.64	117.71 117.80
4-2	79.49 79.67	95.37 94.73	102.70 101.88	108.26 107.65	118.45 118.44
7-1	78.76 79.20	94.47 95.31	101.96 100.00	107.01 107.20	117.49 117.68
7-2	79.45 80.36	95.40 93.57	101.77 102.05	107.59 107.29	118.12 115.49
8-1	78.05 79.10	94.33 94.96	102.01 101.31	106.92 106.68	116.64 117.17
8-2	79.43 78.60	94.40 94.00	102.07 101.30	107.21 107.26	115.79 116.16
9-1	80.20 79.50	94.83 94.10	101.13 100.87	106.53 107.23	114.53 113.50
9-2	80.43 78.53	94.17 93.70	100.97 100.17	106.30 106.07	116.73 116.30
10-1	78.35 78.53	94.50 94.03	100.40 99.80	105.20 106.90	115.60 114.00
10-2	80.10 77.80	93.10 93.63	99.41 102.50	107.29 106.14	116.95 116.99

continued

Table 6 (continued)

	- - - - - [Cl], mmol/L - - - - -				
<u>Laboratory^a</u>	<u>Pool 1</u>	<u>Pool 3</u>	<u>Pool 4</u>	<u>Pool 5</u>	<u>Pool 7</u>
13-1	80.00 79.70	94.67 95.00	102.70 102.00	107.30 107.00	117.20 116.50
13-2	79.80 79.50	95.00 95.00	102.00 101.90	106.33 107.20	117.20 117.00
14-1	81.50 80.20	96.60 96.50	103.30 106.60	109.60 109.90	118.90 117.30
14-2	80.40 79.30	95.10 94.30	101.40 102.70	107.00 107.80	117.30 116.50
15-1	79.46 79.54	94.59 94.76	101.93 101.99	107.47 107.52	116.92 116.89
15-2	79.51 79.39	94.81 94.68	102.01 101.97	107.40 107.23	116.99 116.86
Definitive Method Values	79.2	94.0	101.8	107.2	116.8

^aThe laboratory designation consists of two parts: the initial digit(s) represents the assigned laboratory number and the last digit represents either the first or second day's results.

Table 7. Concentration of serum chloride reported by the participating laboratories for Interlaboratory Exercise II, macropipetting protocol.

- - - - - [Cl], mmol/L - - - - -					
<u>Laboratory^a</u>	<u>Pool 1</u>	<u>Pool 3</u>	<u>Pool 4</u>	<u>Pool 5</u>	<u>Pool 7</u>
5-1	79.87	94.74	100.85	106.51	116.45
	78.33	94.14	100.49	106.81	115.27
5-2	79.45	93.44	101.58	105.68	116.70
	78.68	94.17	102.04	107.14	116.64
6-1	78.24	94.73	101.88	106.43	117.08
	78.63	95.01	101.12	106.24	117.00
6-2	78.56	93.48	101.34	106.01	115.95
	78.30	93.61	101.63	106.68	116.52
11-1	79.58	93.53	101.26	107.12	115.22
	79.14	95.09	103.43	107.03	115.11
11-2	80.11	94.48	101.98	108.01	116.74
	79.60	94.87	102.00	107.63	116.84
Definitive Method Values	79.2	94.0	101.8	107.2	116.8

^aThe laboratory designation consists of two parts: the initial digit(s) represent the assigned laboratory number and the last digit represents either the first or second day's results.

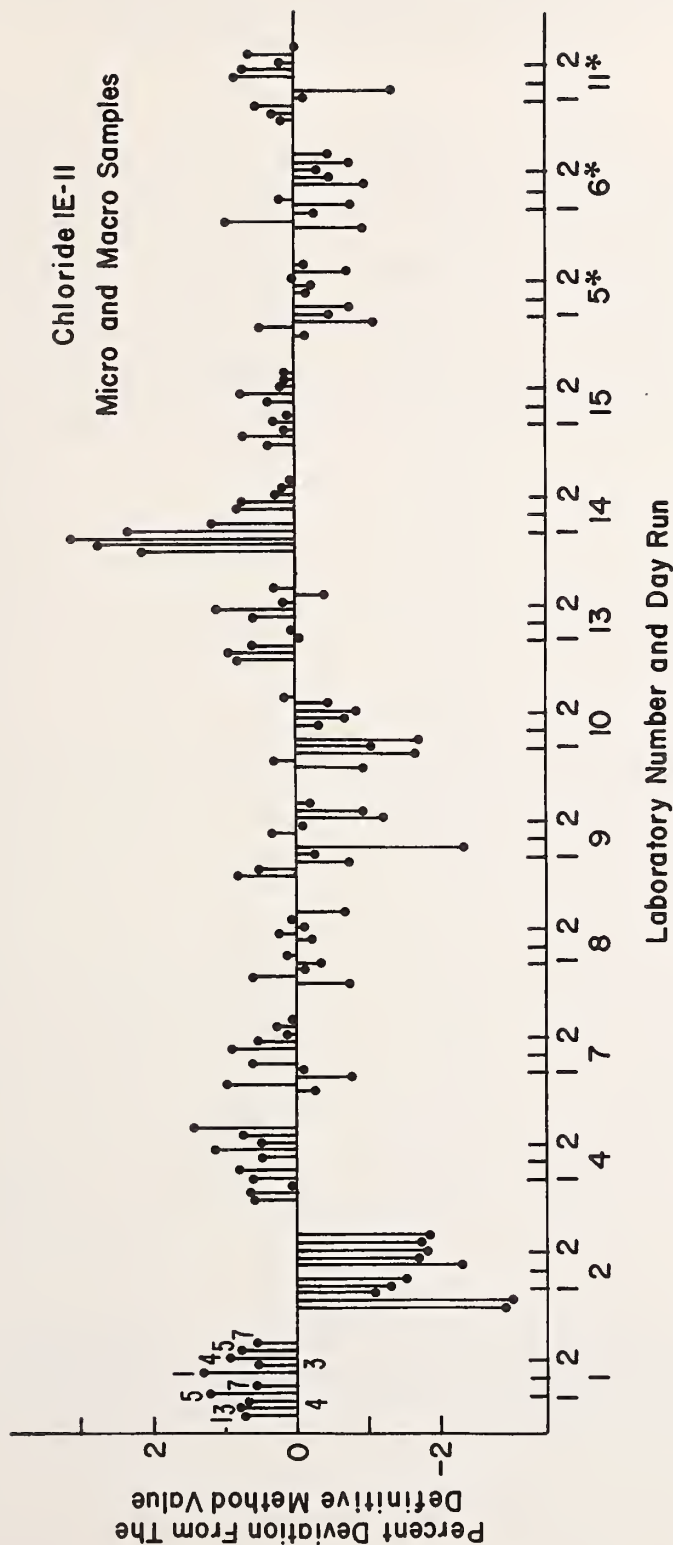


Figure 5. Percent deviations of the Interlaboratory Exercise II measurements using micro- and macropipetting from the definitive method values. The analyzed pools are identified by the numbers 1, 3, 4, 5, and 7 next to the data from laboratory 1. The presentation is similar for the remaining results. The numbers 1 and 2, placed directly above the laboratory number, designate the first day and subsequent day test results, respectively. The asterisk next to the laboratory number designates those laboratories using the macro-pipetting procedure.

are included in the tables. The definitive method values for the chloride concentrations in the sample pools are listed at the bottom of Tables 6-7.

The following statistical analysis was made. First the data were inspected by calculating the percent deviation of each day's results for each pool from an overall average for that sample pool. These percent deviation values for all laboratories using the two pipetting procedures are listed in Tables 8-9.

Table 8. Percent deviations from averages for chloride in serum from Interlaboratory Exercise II, micro-pipetting protocol.

<u>Laboratory^a</u>	<u>Pool 1</u>	<u>Pool 3</u>	<u>Pool 4</u>	<u>Pool 5</u>	<u>Pool 7</u>
1-1	0.64	0.40	0.79	1.25	0.70
1-2	1.20	.16	1.03	.79	.69
2-1	-3.04	-3.40	-1.04	-1.33	-1.42
2-2	-2.69	-2.10	-1.73	-1.75	-1.76
4-1	.48	.24	.15	.59	.94
4-2	.38	.73	.57	.72	1.54
7-1	-.38	.56	-.71	-.07	.80
7-2	.79	.13	.20	.24	.13
8-1	-.89	.30	-.05	-.36	.21
8-2	-.34	-.17	-.02	.05	-.58
9-1	.72	.11	-.69	-.28	-2.26
9-2	.25	-.45	-1.12	-.93	-.12
10-1	-1.06	-.10	-1.58	-1.06	-1.59
10-2	-.42	-1.05	-.74	-.44	.27
13-1	.72	.51	.63	-.03	.17
13-2	.46	.68	.24	-.39	.38
14-1	1.98	2.32	3.19	2.39	1.24
14-2	.72	.36	.34	.20	.21
15-1	.28	.34	.25	.29	.21
15-2	.21	.41	.28	.12	.23
Average used in calculations, mmol/L	79.28	94.36	101.71	107.18	116.65

^aThe laboratory designation consists of two parts: the initial digit(s) represent the assigned laboratory number and the last digit represents either the first or second day's results.

Table 9. Percent deviations from averages for chloride in serum from Interlaboratory Exercise II, macro-pipetting protocol.

<u>Laboratory^a</u>	<u>Pool 1</u>	<u>Pool 3</u>	<u>Pool 4</u>	<u>Pool 5</u>	<u>Pool 7</u>
5-1	0.07	0.18	-0.95	-0.11	-0.37
5-2	.03	-.50	.17	-.34	.32
6-1	-.77	.63	-.13	-.41	.64
6-2	-.77	-.77	-.15	-.40	-.05
11-1	.40	.04	.70	.28	-.97
11-2	1.03	.43	.35	.98	.43
Average used in calculations, mmol/L	79.04	94.27	101.63	106.77	116.29

^aThe laboratory designation consists of two parts: the initial digit(s) represent the assigned laboratory number and the last digit represents either the first or second day's results.

A comparison was next made of the ability of each laboratory to replicate its values relative to that of the average replication ability of all laboratories. This was done by comparing the standard deviation for each day's measurements for each pool against the average standard deviation for all laboratories for that pool (see Tables 10-11). If all of the participating laboratories were of the same population in regard to replication error, the standard deviation ratios reported in Tables 10-11 would be larger than 2.44 and 2.14, respectively, only about one percent of the time. In practice, it is not too uncommon to encounter

Table 10. Ratios of standard deviations to average standard deviation for chloride in serum from Inter-laboratory Exercise II, micropipetting protocol.

<u>Laboratory^a</u>	<u>Pool 1</u>	<u>Pool 3</u>	<u>Pool 4</u>	<u>Pool 5</u>	<u>Pool 7</u>
1-1	0.70	0.12	0.30	0.17	0.74
1-2	.24	3.11	.98	.43	.50
2-1	.34	1.49	2.32	2.95	3.08
2-2	2.14	.93	.00	2.71	1.12
4-1	.78	.99	.09	.62	.13
4-2	.24	1.06	.91	1.05	.01
7-1	.59	1.39	2.16	.33	.27
7-2	1.23	3.03	.31	.51	3.69
8-1	1.42	1.04	.77	.41	.74
8-2	1.12	.66	.85	.09	.52
9-1	.95	1.21	.29	1.20	1.44
9-2	2.57	.78	.88	.39	.60
10-1	.24	.78	.66	2.91	2.24
10-2	3.11	.88	3.41	1.97	.06
13-1	.41	.55	.77	.51	.98
13-2	.41	.00	.11	1.49	.28
14-1	1.76	.17	3.64	.51	2.24
14-2	1.49	1.32	1.43	1.37	1.12
15-1	.11	.28	.07	.09	.04
15-2	.16	.22	.04	.29	.18
Average standard deviation, mmol/L	0.523	0.427	0.641	0.413	0.505

^aThe laboratory designation consists of two parts: the initial digit(s) represents the assigned laboratory number and the last digit represents either the first or second day's results.

Table 11. Ratios of standard deviations to average standard deviation for chloride in serum from Inter-laboratory Exercise II, macropipetting protocol.

<u>Laboratory^a</u>	<u>Pool 1</u>	<u>Pool 3</u>	<u>Pool 4</u>	<u>Pool 5</u>	<u>Pool 7</u>
5-1	2.36	0.98	0.53	0.58	3.37
5-2	1.18	1.19	.68	2.83	.17
6-1	.60	.46	1.12	.37	.23
6-2	.40	.21	.43	1.30	1.63
11-1	.68	2.54	3.21	.17	.31
11-2	.78	.63	.03	.74	.29
Average standard deviation, mmol/L	0.461	0.435	0.478	0.364	0.247

^aThe laboratory designation consists of two parts: the initial digit(s) represents the assigned laboratory number and the last digit represents either the first or second day's results.

ratios that are somewhat larger, as this is a reflection of some heterogeneity of the laboratory population in regard to replication error. (As long as the standard deviation ratios are not too large, this is normally not used as a reason for rejection of a laboratory. However, laboratories with large standard deviation ratios are advised to reexamine their procedures for possible sources of excessive replication error.)

The calculations on IE-II data were made on the data in Tables 6 and 7 using a weighted least squares fit to the following model [21]:

$$Y_{ijk} = \mu_i + \beta_i (X_j - \bar{X}) + \lambda_{ij} + \epsilon_{ijk} \quad (4)$$

where:

Y_{ijk} = the sample concentration reported by the i^{th} laboratory, for the j^{th} sample, and for the k^{th} replicate measurement,

μ_i = a constant factor associated with the average bias for laboratory i ,

β_i = a slope factor for laboratory i , expressing the relation of bias to concentration,

X_j = the observed average concentration for sample pool j (this average is taken over all laboratories),

\bar{X} = the weighted average concentration for all samples (this average is taken over all laboratories and over all sample pools),

λ_{ij} = a random sample interference factor (matrix effect) for laboratory i and sample pool j , and

ϵ_{ijk} = a random replication error.

The above model is quite general, and extensive experience has shown that it is well suited to describe a number of measurement factors in inter-laboratory tests [22].

Weighted analyses of variance were made on the data in the two-way tables using the fits to the above model. (A modified version of the weighting procedure reported in reference 23 was used.) From the analyses it is possible to derive the following estimates for three components of variability, each characterized by its standard deviation:

$\hat{\sigma}_{\epsilon} = \hat{\sigma}_{\epsilon(\text{Repl})}$ = the uncertainty observed for replicate measurements in a given, laboratory on a given day,
 $\hat{\sigma}_{\text{D}} = \hat{\sigma}_{\text{Day}}$ = the additional uncertainty that is observed when measurements are made on different days within the same laboratory, and
 $\hat{\sigma}_{\text{L}} = \hat{\sigma}_{\text{Lab}}$ = the additional uncertainty that is observed when measurements are made by different laboratories.

From the analyses, it was observed that the ranges of values for the $\hat{\sigma}_{\epsilon}$, $\hat{\sigma}_{\text{D}}$, and $\hat{\sigma}_{\text{L}}$ components of standard deviation were small, and that the values did not depend significantly on the chloride ion concentration. Because of this, only average $\hat{\sigma}_{\epsilon}$, $\hat{\sigma}_{\text{D}}$, and $\hat{\sigma}_{\text{L}}$ values are reported. These components of standard deviation are given in Table 12.

Table 12. Components of standard deviation in mmol/L for all IE-II chloride ion levels (79-117 mmol/L).

	$\hat{\sigma}_{\epsilon(\text{Repl})}$	$\hat{\sigma}_{\text{Day}}$	$\hat{\sigma}_{\text{Lab}}$
Micropipetting Protocol (Pooled results from 10 labs)	.69	.42	.90
Macropipetting Protocol (Pooled results from 3 labs)	.53	.37	.36

Because of the relatively small size of the chloride ion IE tests, the individual components of standard deviation are considered to be only advisory in nature. Nevertheless, they do seem to indicate that the three components ($\hat{\sigma}_{\epsilon}$, $\hat{\sigma}_{\text{D}}$, and $\hat{\sigma}_{\text{L}}$) are all of about the same order of magnitude. The final,

statements of uncertainty are made through the recombination of these components.

One such final statement is $\hat{\sigma}_{\text{within}}$, the expected uncertainty within a single laboratory from running the complete protocol (2 replicates/day for 2 days). The $\hat{\sigma}_{\text{within}}$ results are reported in columns three and seven in the top section of Table 13, and are calculated as follows:

$$\hat{\sigma}_{\text{within}} = \sqrt{\frac{\hat{\sigma}_{\epsilon}^2}{4} + \frac{\hat{\sigma}_D^2}{2}} \quad (5)$$

These are the expected uncertainties that a single average laboratory could see by repeating the complete protocol a number of times and observing the variability of its results. This $\hat{\sigma}_{\text{within}}$ is not the total uncertainty since there is also a "between laboratory" component, $\hat{\sigma}_{\text{Lab}}$.

The standard deviation of the total uncertainty expected as a result of a single laboratory running the complete protocol is calculated as follows:

$$\sigma_{\text{Total}} = \sqrt{\frac{\hat{\sigma}_{\epsilon}^2}{4} + \frac{\hat{\sigma}_D^2}{2} + \hat{\sigma}_L^2} \quad (6)$$

Columns four and six in the top section of Table 13 list such standard deviations for the micro- and macropipetting protocol data from IE-II. The precision goal for the reference method is listed in column five. Comparison of the tabulated standard deviations and the goal shows that the precision goals have been met.

Table 13. Summary of imprecision and bias results in mmol/L for chloride ion in serum, IE-II.

----- 1σ Precision -----							
Cl Level mmol/L	<u>Micropipetting Protocol</u>			<u>Goal</u>	<u>Macropipetting Protocol</u>		
	$\hat{\sigma}_{comp}$	$\hat{\sigma}_{within}$	$\hat{\sigma}_{total}$		$\hat{\sigma}_{total}$	$\hat{\sigma}_{within}$	$\hat{\sigma}_{comp}$
79-117	.32	.46	1.01	1.5	.52	.37	.30
----- Accuracy -----							
Cl Level mmol/L	<u>Micropipetting Protocol</u>			<u>Goal</u>	<u>Macropipetting Protocol</u>		
	Round Robin Composite Bias ($X_{obs} - X_{DM}$)				Round Robin Composite Bias ($X_{obs} - X_{DM}$)		
79	.1			±2.0	-.2		
94	.4			±2.0	.3		
102	-.1			±2.0	-.2		
107	0			±2.0	-.4		
117	-.1			±2.0	-.5		

The standard errors of the IE-II composite values are given in columns two and eight of the top section of Table 13. These standard errors are calculated from the components of standard deviation as follows:

$$\hat{\sigma}_{Comp} = \sqrt{\left(\frac{1}{N}\right) \left[\frac{\hat{\sigma}_E^2}{4} + \frac{\hat{\sigma}_D^2}{2} + \hat{\sigma}_L^2 \right]} \quad (7)$$

where N represents the 10 or 3 laboratories participating in the micro- or macropipetting procedures, respectively. The bottom section of Table 13 lists the observed biases between the reference method

interlaboratory composite values and the definitive method values. The observed biases are within the goals for the reference method.

The composite IE-II sample averages \pm twice the standard error for the micro- and the macropipetting versions, and for the corresponding definitive method values are listed in Table 14.

The accuracy of the IE-II results is within the recommended goal of the reference method.

Table 14. Summary of chloride ion in serum values ± 2 standard errors.

IE-II - Composite Values (mmol/L)		Definitive Method Values (mmol/L)
<u>Micro</u>	<u>Macro</u>	
79.3 \pm .64	79.0 \pm .60	79.2 \pm .4 ^a
94.4 \pm .64	94.3 \pm .60	94.0 \pm .5
101.7 \pm .64	101.6 \pm .60	101.8 \pm .5
107.2 \pm .64	106.8 \pm .60	107.2 \pm .5
116.7 \pm .64	116.3 \pm .60	116.8 \pm .6

^aEstimated maximum error of 0.5 percent of the value as reported by NBS Analytical Mass Spectrometry Section. This estimated maximum error includes both imprecision and an estimated upper bound for possible systematic errors. The estimated maximum error is believed to be equal to or greater than the true error for the 95 percent confidence limits.

Auxiliary Statistical Analysis

The protocol requires a check on the automated titrimeter by running a calibration curve each day using freshly prepared standard solutions. The necessity of these curves also provides a check on the correct preparation of the standard solutions. The data reported here on the calibration curve check are advisory in nature since in the actual analytical procedure only the pair of calibrating solutions nearest to the unknown concentration is used. The calibration curve data for the micro- and macropipetting procedures were reported and are given in Tables 15 and 16. Straight line least square fits were made to these data and the resultant standard deviations of fit are given in Table 17. These standard deviations of fit are expressed in units of chloride ion concentration (mmol/L). The calibration curve data show excellent linearity with all curves having standard deviation of fit of 1.23 mmol/L or less, and 12 of the 14 curves having s_{fit} of 0.79 mmol/L or less. This analysis indicates that if in the calibration step it is found that any calibration point deviates from the calibration curve by more than 1.3 mmol/L, then the standard solutions and the instrument should be checked for sources of excessive error before proceeding further into the analysis.

Table 15. Calibration curve data for chloride in serum, Interlaboratory Exercise II, micropipetting protocol.

<u>Lab. No.</u> ^a		<u>Std. 1</u>	<u>Std. 2</u>	<u>Std. 3</u>	<u>Std. 4</u>	<u>Std. 5</u>
1-1	X ^b	75.0	90.0	100.0	110.0	125.0
	Y ^c	75.16	90.02	100.28	110.08	124.74
1-2	X	75.0	90.0	100.0	110.0	125.0
	Y	75.00	90.70	99.95	109.80	125.30
4-1	X	75.02	90.01	100.00	110.00	125.00
	Y	75.31	89.73	100.36	110.38	125.47
4-2	X	75.02	90.01	100.00	110.00	125.00
	Y	74.62	89.86	99.81	109.72	124.82
8-1	X	75.00	90.00	100.00	110.00	125.00
	Y	75.0	89.8	99.8	110.2	124.8
9-1	X	75.01	90.00	100.00	110.03	125.01
	Y	74.4	89.4	99.9	109.4	124.8
13-1	X	75.00	90.00	100.00	110.00	125.00
	Y	75.0	90.0	100.0	110.0	125.0
14-1	X	75.0	90.0	100.0	110.0	125.0
	Y	76.0	90.0	99.0	109.0	124.0
14-2	X	75.0	90.0	100.0	110.0	125.0
	Y	75.0	90.0	100.0	111.0	124.0
15-1	X	75.00	90.00	100.00	110.00	125.00
	Y	47.14	56.14	62.16	68.23	77.23

^aThe laboratory designation consists of two parts: the initial digit(s) represent the assigned laboratory number and the last digit represents either the first or second day's results.

^bX = standard solution values in mmol/L.

^cY = instrument readings.

Table 16. Calibration curve data for chloride in serum, Interlaboratory Exercise II, macropipetting protocol.

<u>Lab. No.^a</u>		<u>Std. 1</u>	<u>Std. 2</u>	<u>Std. 3</u>	<u>Std. 4</u>	<u>Std. 5</u>
5-1	X ^b	75.01	90.01	100.01	110.00	125.00
	Y ^c	23.2	27.9	31.0	34.2	39.0
5-2	X	75.01	90.01	100.01	110.00	125.00
	Y	23.1	27.8	31.0	34.2	38.8
6-1	X	75.00	89.96	99.93	110.27	124.87
	Y	79.06	94.40	104.85	115.58	130.36
11-1	X	74.99	90.03	100.04	110.08	124.98
	Y	26.62	30.34	33.5	36.72	41.42
11-2	X	74.99	90.03	100.04	110.08	124.98
	Y	25.74	30.9	33.94	38.22	42.84

^aThe laboratory designation consists of two parts: the initial digit(s) represent the assigned laboratory number and the last digit represents either the first or second day's results.

^bX = standard solution values in mmol/L.

^cY = instrument readings.

Table 17. Calibration curve results for chloride in serum as standard deviation of fit (s_{fit}) in mmol/L.

- - - - - Micro - - - - -		- - - - - Macro - - - - -	
<u>Laboratory Number^a</u>	<u>s_{fit}</u>	<u>Laboratory Number^a</u>	<u>s_{fit}</u>
1-1	0.18	5-1	0.16
1-2	.41	5-2	.18
4-1	.30	6-1	.13
4-2	.10	11-1	1.23
8-1	.20	11-2	.98
9-1	.28		
13-1	(0)		
14-1	.79		
14-2	.51		
15-1	.04		

^aThe laboratory designation consists of two parts: the initial digit(s) represent the assigned laboratory number and the last digit represents either the first or the second day's results.

V. DISCUSSION

A. Candidate Protocol:

1. Preliminary Tests

Generally, in the development of a reference method where the state of analytical knowledge leaves an uncertainty in the choice of a candidate reference method, it is essential that investigations be undertaken to assure optimized analytical conditions, minimized interferences, and freedom from other sources of bias. Such preparation helps avoid initiating the interlaboratory testing process with inappropriate procedures. However, in the case of chloride, the similarity of test results obtained by use of the C-A method and the highly specific IDMS method, led the Committee to decide to proceed directly to the interlaboratory exercise phase with the C-A method, without further preliminary studies.

2. Specifications

In light of prior experience [8,9,10,14,15,24], the written protocol is explicit as to reagent and glassware specifications, pipetting, and directions for dilution of standard and sample. Thus, Class A or equivalent glassware, reagent grade or equivalent chemicals, 'tested' water, analytical balances with a ± 0.1 mg weighing capability, and micro-pipets with specified accuracy and precision are used. In addition, the reference method provides for the use of analytical techniques that should reduce the combined error due to weighing, pipetting, and dilution to below one percent of the measured values.

3. Coulometric-Amperometric Instrumentation

Coulometric-amperometric instrumentation has been used extensively for the determination of serum chloride in the clinical laboratory. In the Committee's judgment, it was felt that these instruments might provide the necessary

accuracy and precision in a clinical reference method, and that instructions for the use of specific instruments should not be given in the protocol. Instead, it should be left to the investigator to use the manufacturer's instructions for the specific instrument he employs, since different readouts, electrolytes, dispersants, micropipets, and sample volumes might be used. Thus specifications were not presented other than a requirement for stable instrument operating conditions. As in sample preparation and handling, the human element in achieving accuracy and precision is critical. It is essential that operators be thoroughly familiar with their instruments and alert to the onset of instrumental difficulties. Instrument linearity requirements are not included in the protocol since the bracketing method for obtaining valid measurements is used to ensure minimal error attributable to instrumental variation.

Instruments produced by five different manufacturers¹¹ were used in the interlaboratory exercise. All gave excellent results and are listed in Table 18. On examination of the data reported for calibration curves, excellent linearity was found over the range of chloride concentrations from 75 to 125 mmol/L. More than 92 percent of the calibration curves showed standard deviations of fit of 1.00 mmol/L or less. A standard deviation of fit larger than 1.30 mmol/L would clearly warrant a laboratory's examination of its operation of the procedure and/or preparation of the standard solutions.

¹¹To describe instruments, it was necessary to identify commercial products by the manufacturer's name. In no instance does such identification imply endorsement by the National Bureau of Standards, nor does it imply that the particular product is necessarily the best available for that purpose.

Table 18. Instruments, pipets, and various protocol parameters used by the participating laboratories in Interlaboratory Exercise I and Interlaboratory Exercise II^a.

Lab.	Instrument	Readout		Electrolyte	Dispersant	Micropipet	Protocol	
		Direct Time					Micro Macro	Sample Volume (μL)
1	Buchler	X		NR ^b	NR ^b	Clay Adams 4625	X	—
2	Corning 920M	X		Corning Acid Buffer	NR ^b	Dade Micropipettes	X	100
4	Buchler 4-2500	X		Acetic/Nitric	Gelatin Reagent	Micromedic	X	100
5	AMINCO Co.	X		NR ^b	Gelatin Reagent	—	X	—
6	Buchler 4-2088	X		Acetic/Nitric	Polyvinyl Alcohol	—	X	—
8	Corning-HEEL 920	X		Acetic/Nitric	Gelatin Reagent	—	X	—
9	Radiometer CMT-10	X		Radiometer LS 101	(Premixed)	NR ^b	X	20
10	AMINCO J4-4411	X		Acetic/Nitric	Gelatin Reagent	Automatic	X	40
11	AMINCO 4-4433	X		Acetic/Nitric	Gelatin Reagent	—	X	—
13	Radiometer CMT-10	X		Acetic/Nitric	Polyvinyl Alcohol	SMI Micro/Pettor	X	20
14	Beckman C1/CO ₂	X		.12 N H ₂ SO ₄	Polyvinyl Alcohol	Beckman	X	10
15	AMINCO J4-4415	X		Acetic/Nitric	Gelatin Reagent	—	X	—
15	AMINCO J4-4415	X		Acetic/Nitric	Gelatin Reagent	Micromedic	X	100

^aLaboratory 3 information not included since the Schales-Schaes titration procedure was used.

^bNot reported.

4. Statistical Analysis

The results discussed here are based on the analysis of four replicate samples analyzed as pairs on two separate days. Adherence to this pattern of replicate analysis facilitated analysis of the performance of the reference method.

The imprecision and bias goals of 1.5 and 2.0 mmol/L, respectively set at the 100 mmol/L level, were in fact reached over the total concentration range by the laboratories using either the micro- or macropipetting protocols. We believe there are no differences in the imprecision or bias values obtained by the two pipetting alternatives. In Table 13, the $\hat{\sigma}_{\text{total}}$ value for the macropipetting procedure was observed to be approximately one-half that for the micropipetting procedure. Because of the limited three-laboratory sample in the macropipetting procedure, the $\hat{\sigma}_{\text{total}}$ has a lower reliability than that for the micropipetting procedure which involved 10 laboratories. Comparison of results from IE-I with those from IE-II suggests that the imprecisions and biases for both pipetting procedures are essentially equal (see, for example, figures 4 and 5). The micropipetting procedure results may be considered indicative of the imprecisions and biases for both pipetting procedures.

Considering the uncertainties in the definitive method values, the results from the micro- and macropipetting procedures show no significant bias from the definitive method values, Table 14.

In summary, for laboratories in the population typical of those participating in this study (i.e., clinical laboratories that have practiced the reference method and are in good quality control) have imprecisions ($\hat{\sigma}_{\text{total}}$) within 1.0 mmol/L and biases within 0.5 mmol/L can be expected in the performance of this reference method.

Auxiliary statistical analysis on the calibration curve data showed excellent linearity with all curves having standard deviations of fit of 1.23 mmol/L or less and 12 of the 14 curves having s_{fit} of 0.79 mmol/L or less.

VI. CONCLUSIONS

A candidate reference method, specified by a written protocol for the determination of serum chloride employing commercial coulometric-amperometric instrumentation, was evaluated by comparing the results of analyses run on serum and aqueous samples in a selected group of laboratories that used the method against definitive method values for the same samples. The results for samples having chloride concentrations in the 79 to 117 mmol/L range, showed a total imprecision ($\hat{\sigma}_{\text{total}}$) of approximately 1.0 mmol/L and a maximum bias of 0.5 mmol/L. In IE-I and IE-II, similar imprecisions and biases were found whether macropipetting or micropipetting was used in the C-A procedure.

Statistical analysis of the results shows that the C-A method can be carried out with the accuracy and precision expected of a reference method for serum chloride. Hence, the candidate method is considered to be the reference method. This reference method may be used to establish the accuracy of field methods for chloride by comparative testing. It may also be used to determine reference material values for serum chloride. Each of these uses would require an appropriate experimental design to ensure its achievement of accuracy and precision equal to those demonstrated here.

We would like to especially thank the principal investigators and other scientists in the participating laboratories (listed in Appendix A), who, through their efforts, made this work meaningful and possible. We thank Dr. David Bayse and Ms. Sue Lewis, CDC, for providing excellent, homogeneous serum pools used in the interlaboratory testing process.

The work at NBS was carried out in the Institute for Materials Research. We thank Dr. Philip D. LaFleur, Director, Center for Analytical Chemistry, and Mr. J. Paul Cali, Chief, Office of Standard Reference Materials, for their support and encouragement throughout this program. Special thanks go to Dr. Richard Durst for discussions and suggestions in the area of electrochemistry. Acknowledgement is also made to Mr. John Matwey for help in sample handling. Special thanks are due to Mrs. Joy Shoemaker of the Text Editing Facility for her efforts in manuscript production which included formatting, editing, and typing.

The Bureau of Medical Devices of The Food and Drug Administration is acknowledged for their financial support of this project.

VII. REFERENCES

- [1] Weissberg, H. F., in "Water, Electrolyte, and Acid-Base Balance," 2nd Edition, Williams and Wilkins Co., Baltimore, MD 1962, p. 81.
- [2] di Sant'Agnese, P. A., Darling, R. C., Perera, G. A., and Shea, E., Am. J. Med., 15, 777 (1953).
- [3] Weissman, N. and Pileggi, V. J., in "Clinical Chemistry: Principles and Technics." Henry, R. J., Cannon, D. C., and Winkelman, J. W., Eds. 2nd Edition, Harper and Row, New York, NY 1974, p. 712; Tietz, N. W., in "Fundamentals of Clinical Chemistry, W. B. Saunders Co., Publisher, Philadelphia, PA 1970, p. 621
- [4] Driscoll, J. L. and Martin, H. F., Clin. Chem., 12, 314 (1966).
- [5] Schales, O., in "Standard Methods of Clinical Chemistry," Vol. I., M. Reiner, Ed., Academic Press, New York, NY 1953, p. 37.
- [6] Klein, G., in "Standard Methods of Clinical Chemistry," Vol. II, D. Seligson, Ed., Academic Press, New York, NY 1958, p. 22.
- [7] Cotlove, E., in "Standard Methods of Clinical Chemistry," Vol. III, D. Seligson, Ed., Academic Press, New York, NY 1961, p. 81; Cotlove, E., Trantham, H. V., and Bowman, R. L., J. Lab. Clin. Med., 51, 461 (1968); Ibbott, F. A., in "Standard Methods of Clinical Chemistry," Vol. V, S. Meites, Ed., Academic Press, New York, NY 1965, p. 101.
- [8] Cali, J. P., Mandel, J., Moore, L. J., and Young, D. S., "A Referee Method for the Determination of Calcium in Serum" Nat. Bur. Stand. (U.S.) Special Publication 260-36 (1972). For sale by: Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402 SD Cat. No. C13.10:260-36.

- [9] Velapoldi, R. A., Paule, R. C., Schaffer, R., Mandel, J., and Moody, J. R., "A Reference Method for the Determination of Sodium in Serum", Nat. Bur. Stand. (U.S.) Special Publication, 260-60 (1978). For sale by: Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402 SD Cat. No. C13.10:260-60.
- [10] Velapoldi, R. A., Paule, R. C., Schaffer, R., Mandel, J., Machlan, L. A., and Gramlich, J. W., "A Reference Method for the Determination of Potassium in Serum," Nat. Bur. Stand. (U.S.) Special Publication, 260-63 (1979). For sale by: Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402 SN 003-003-02068.
- [11] Pybus, J., Feldman, F. J., and Bowers, G. N. Jr., Clin. Chem., 16, 998 (1970).
- [12] See specific references in the Sections on Definitive Methods in references 8-10.
- [13] Available from: Office of Standard Reference Materials, National Bureau of Standards, Washington, D. C. 20234.
- [14] Cali, J. P., Bowers, G. N., and Young, D. S., Clin. Chem., 19 (10), 1208 (1973).
- [15] Velapoldi, R. A., Paule, R. C., Schaffer, R., Mandel, J., and Moody, J. R., and Velapoldi, R. A., Paule, R. C., Schaffer, R., Mandel, J., Machlan, L. A., and Gramlich, J. W., To be Submitted.
- [16] Carter, R. J., Mather, A., Dawson, C. D., Turner, W. E., Neese, J. W., and Bayse, D. D., "The Development of a CDC Reference Method for Sodium and Potassium in Serum," Draft Copy, Center for Disease Control, Atlanta, GA 30333.
- [17] Serum samples have been stored frozen for several years at temperatures below -20 °C with no apparent affect on electrolyte concentration. White, J. CDC, Private Communication.

- [18] Thawed serum samples were mailed to the participating laboratories. In previous experiences at CDC, thawed samples mailed to the west coast and returned after two weeks showed no change in serum electrolyte concentration. White, J., CDC, Private Communication.
- [19] Reagent Chemicals, American Chemical Society Specifications ACS Publications, Washington, D.C. (1968).
- [20] Hughes, J. C., "Testing of Glass Volumetric Apparatus," NBS Circular 602, 1959. For sale by: The Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20025.
- [21] Mandel, J., "Models, Transformations of Scale, and Weighting", Journal of Quality Technology, Vol. 8, No. 2, 86-97 (1976).
- [22] Mandel, J., "The Interlaboratory Evaluation of Testing Methods", ASTM Bulletin 239, 53-61 and 133 (1959).
- [23] Mandel, J., "Estimation of Weighting Factors in Linear Regression and Analysis of Variance", Technometrics, 6, 1-25 (1964).
- [24] Clinical reference methods are also being developed at NBS for lithium and magnesium.

APPENDIX A

Scientists not previously acknowledged who contributed to this study are:

Mrs. Harriet Bailey
Dr. Daniel Grisley
New England Deaconess Hospital

Ms. Leyda Ortega
Mr. G. S. King
American Hospital Supply

Ms. J. Schmitz
Veterans Administration Hospital

Ms. K. Koch
Beckman Instruments

Miss C. Wong
Mrs. Shirley Wertlake
University of California

Mr. Frank Doherty
Pennsylvania Department of Health

Ms. R. Stauffenberg
Food and Drug Administration

National Bureau of Standards Certificate of Analysis

Standard Reference Material 919

Sodium Chloride (Clinical Standard)

This Standard Reference Material is certified for use in the calibration and standardization of procedures employed in the determination of sodium and chloride ions in clinical analyses. The sample consists of highly purified sodium chloride. Chemical assay as well as analyses for specific impurities indicate that the material may be considered essentially pure, except for occluded moisture.

Purity 99.9 \pm 0.0 percent

The above value for the purity of the material is based on a sample dried over magnesium perchlorate for 24 hours. At room temperature sodium chloride is hygroscopic above 60 percent relative humidity. The sorbed water can be removed, however, by desiccation over freshly exposed P_2O_5 or $Mg(ClO_4)_2$ for 24 hours. Chloride was determined using the coulometric method of Marinenko and Taylor [J. Res. NBS, 67A, 31 (1963)].

Based on 8 independent measurements of chloride content, the sample is considered homogeneous.

When the material is crushed and dried at 200 °C for 18 hours, the loss of moisture is about 0.08 percent. Coulometric determinations of chloride on the dried material indicate 99.995 ± 0.004 percent purity.

The sodium chloride used for this Standard Reference Material was obtained from the J. T. Baker Chemical Company, of Phillipsburg, New Jersey. Analyses were performed by G. Marinenko, J. R. Baldwin, M. Darr, and T. C. Rains.

The overall direction and coordination of technical measurements leading to the certification were under the chairmanship of R. A. Durst.

The technical and support aspects concerning the preparation, certification, and issuance of this Standard Reference Material were coordinated through the Office of Standard Reference Materials by T. W. Mears.

Washington, D. C. 20234
August 6, 1973

J. Paul Cali, Chief
Office of Standard Reference Materials

(over)

This material was examined for compliance with the specifications for reagent grade sodium chloride as given in Reagent Chemicals, 4th edition, published by the American Chemical Society. The material meets or exceeds the minimum requirements in every respect.

Sodium was assayed using a gravimetric procedure in which the sodium chloride was converted to sodium sulfate. Approximately 250 mg of sodium chloride (dried at 500 °C for 4 hours in a platinum crucible) was dissolved in ultrapure sulfuric acid solution (1:1) and evaporated to dryness. Ammonium carbonate was added and the crucible slowly heated to 600 °C, then 900 °. This treatment was repeated until the weight of sodium sulfate remained constant. Based on 6 determinations, the sodium assay is 39.3₂ weight percent or 99.9₆ percent of the amount computed for perfectly pure, stoichiometric NaCl.

A semiquantitative survey for trace elements by emission spectroscopy indicated less than 10 µg/g calcium, copper, iron, and magnesium. A value of less than 3 µg/g magnesium was obtained by atomic absorption spectrometry. Flame emission spectrometry indicated the presence of the following elements: potassium, 11 µg/g; calcium and cesium, less than 2 µg/g; and rubidium and lithium less than 0.5 µg/g.

This Standard Reference Material is intended for "in vitro" diagnostic use only.

This material is intended for use as a standard for the determination of sodium and chloride ions in clinical chemistry.

Sodium is most frequently determined by flame emission photometry. The operative details of this methodology vary from instrument to instrument and are discussed at length in their respective operating manuals. A standard solution of 100 mmol of sodium chloride per liter (suitable for both sodium and chloride determinations) may be prepared by placing 5.85 g of SRM 919 (dried at 110 °C) in a 1-liter volumetric flask and adding 3 ml of concentrated nitric acid (ACS Reagent Grade) and 100 ml of deionized water. After the NaCl is dissolved, dilute to the mark with deionized water. The concentration required for analysis may be prepared by accurate dilutions with distilled water.

This Standard Reference Material should be stored in the well-closed original bottle under normal laboratory conditions. It is recommended that weighing and other manipulations not be made when the relative humidity exceeds 60 percent.

Solutions of SRM 919 are stable indefinitely when stored in a well-stoppered, all-glass container. All such solutions should be clear and display no turbidity.

References:

- [1] N. W. Tietz, Fundamentals of Clinical Chemistry, pp. 616-618; 621-625, W. B. Saunders Co., Philadelphia, Pa. (1970).
- [2] R. D. Henry, Clinical Chemistry, Principles and Practice, pp. 345-350; 402-409, Hoeber Medical Division, Harper & Row, New York, N. Y. (1967).

This Standard Reference Material has been measured and certified at the laboratories of the National Bureau of Standards, Gaithersburg, Maryland. All inquiries should be addressed to:

Office of Standard Reference Materials
Room B311, Chemistry Building
National Bureau of Standards
Washington, D. C. 20234

The date of issuance and certification of this Standard Reference Material was August 6, 1973.

APPENDIX C

DEFINITIVE METHOD

Thermal Ionization Isotope Dilution Mass Spectrometry

Isotope dilution mass spectrometry (IDMS), because of its innate accuracy, has been used extensively at NBS to accurately determine the concentration of elements in Standard Reference Materials and other reference materials. An accurate measurement may be defined as one that is both precise and free of unevaluated systematic errors. The concentration determined by this procedure represents the "true value" within the stated uncertainty limits.

At NBS the most accurate methods available to measure a given chemical property are known as definitive methods. A definitive method can be defined as one which has a valid and well described theoretical foundation, has been experimentally evaluated so that reported results have negligible systematic errors, and has high levels of precision. Thermal ionization isotope dilution is regarded at NBS as a definitive method.

In isotope dilution mass spectrometry the quantity of an element present is estimated from the change produced in its isotope composition by the addition of a known quantity of an isotope of the element which alters the analyte's isotopic composition. This alteration is measured by mass spectrometry and the initial amount of the element present in the sample is calculated.

The method, as we use it, consists essentially of the following steps:

- 1) The addition to a weighed sample of a known amount of a separated isotope of the element to be determined. We prefer to make this addition as a weighed portion of a solution of known concentration.

2) Dissolution of the sample by appropriate means, and thorough mixing of the resulting solution to ensure equilibration of the isotopes from the spike and the sample. This may necessitate chemical treatment to convert the separated isotope and natural element to the same oxidation state.

3) Chemical extraction of the isotopically altered element in a form suitable for mass spectrographic analysis. A major advantage of IDMS is the fact that since we are only concerned with the ratio of isotopes, recoveries need not be quantitative after equilibration.

4) Measurement of the altered isotopic ratio by thermal ionization mass spectrometry. The instruments used are solid sample, single stage instruments, designed and built at NBS. Essential detailed descriptions of these instruments have been published [1,2].

5) Calculation of the amount of element present in the sample from the isotope ratio measurement. The calculation for an element with isotopes a and b is shown by equation (1).

$$\mu\text{g/g} = \frac{W_{\text{sp}} C[A_{\text{sp}} - RB_{\text{sp}}]}{BR - A} \cdot \frac{M}{W_s} \quad (1)$$

where

- R = measured isotopic ratio
- W_{sp} = weight spike solution, g
- A_{sp} = mole fraction a in spike
- B_{sp} = mole fraction b in spike
- A = mole fraction a in natural element
- B = mole fraction b in natural element
- M = atomic weight natural element
- W_s = weight of sample, g

(This calculated concentration must be corrected for blank.)

An analysis of the possible errors in IDMS shows that errors could result from the following sources:

a) Error in the calibration of the concentration of the spike isotope. The accuracy of a determination depends on the "spike calibration". The spike solution is calibrated against at least two different solutions of the pure natural element by what has been called reverse isotope dilution. Whenever possible, SRMs are used as the natural material. The error from the spike calibration will be the same as for the element determination and is due to the imprecision of the ratio measurement.

b) Chemical errors. These could be caused by:

1) Incomplete dissolution of the sample. This is a problem common to all wet analytical methods, and the analyst must devise a system that ensures complete sample solution or decomposition. 2) Loss of the element from sample or spike due to volatility or adsorption during dissolution. This can usually be detected by spiking some samples before dissolution and some samples after dissolution. 3) Incomplete mixing or equilibration of spike and natural isotopes. This can be caused by differences of oxidation state or by the occurrence of the natural element in a complex or chelated form. This source of error can be eliminated by proper chemical treatment, for example, oxidation or reduction and wet-ashing. 4) Isotopic fractionation in the chemical treatment if the separation is not quantitative. This is usually not a problem but may occur with some techniques, such as in the separation of lithium by ion exchange chromatography. This can be detected by isotopic analysis of small fractions of the natural material that have been put through the partial separation.

In regard to the total chemical error, no undetected errors should arise from this source in a well designed analysis.

c) Contamination or blank. Contamination or blank may arise from reagents, apparatus, or dust from the laboratory environment. It can be minimized by carrying out the chemical operations in a carefully controlled atmosphere and by using special high purity reagents. The total blank may be estimated by carrying a number of "blanks" through all the steps of the analysis. The average blank value can be treated as a systematic error and used as a correction. The uncertainty of this correction is equal to the randomness of its measurement. For concentrations where the blank represents a significant fraction of the element determined, the blank may become the largest source of error.

d) Interferences. Interferences mainly occur between elements with isobars, that is different elements that have isotopes of equal mass. This problem may be avoided by basing the analysis on those isotopes of the element that are not isobaric, or by chemically separating the interfering element. Fortunately, most of the elements with isobars are in different groups of the periodic table, so separations are not difficult. No concealed systematic error should arise from this source.

For example, ^{40}K is isobaric with ^{40}Ca , but K can be easily separated from Ca by ion exchange chromatography. To be sure that the ^{40}K level is insignificant, the analyst can monitor ^{39}K which is four orders of magnitude more abundant than ^{40}K in natural potassium.

e) Instrumental errors. Instrumental errors may be caused by mass discrimination or fractionation, but are usually cancelled since the same percentage error would be present in the ratio measurement for the spike calibration. With some elements, impurities in a sample can cause a different fractionation pattern from pure material. These effects are usually small (less than 0.1%) and can usually be corrected by repurifying the sample.

This analysis of the possible sources of systematic error shows that these errors can be eliminated or corrected as in the case of the blank. We are left then with the random errors. Random errors are present in the isotope ratio measurements for both the determination and the spike calibration and the blank correction. If the blank correction is insignificant, then the total error in a careful determination reduces to the combined random error for the spike calibration and the determination. This error is reflected in the precision of the isotopic measurements which for many elements is of the order of 0.05 to 0.25 percent. Therefore, absolute accuracies of 0.1 to 0.5 percent are possible even for very low concentrations in complex materials.

When the blank correction is significant then the uncertainty from this source must be added to the uncertainties from the ratio measurements.

Determination of Chloride

Introduction

Some years ago, the absolute $^{35}\text{Cl}/^{37}\text{Cl}$ ratio was measured at NBS during a redetermination of the atomic weight of chlorine [3]. The absolute $^{35}\text{Cl}/^{37}\text{Cl}$ ratio was determined to be 3.127 ± 0.008 . A study of chlorine minerals had shown this ratio to be invariant in natural samples within the measurement uncertainty.

With the exception of sample size, the same mass spectrographic method in which chloride was analyzed using an ammonical solution of silver chloride, seemed to be applicable to the determination of chloride in blood serum by isotope dilution. However, preliminary experiments with serum revealed that silver nitrate solution precipitated not only silver chloride, but also some other material, probably protein, so attempts were made to first remove the protein.

The Folin-Wu method [4] in which protein is precipitated by sodium tungstate from an acidified serum solution, produced a clear "protein-free" filtrate. Unfortunately, the blank for chloride was too high due principally to the chloride content of the sodium tungstate. A modification of this method using ammonium molybdate, which also precipitates protein, and nitric acid instead of sulfuric acid reduced the chloride blank to about 1 μg Cl or less than 0.1 percent of the chloride contained in 1 g of serum.

During actual IDMS determination of Cl in serum, it was found that further purification from organic matter was necessary. Some samples became dark on drying on a filament and gave a different fractionation pattern from the reference during mass spectrometric analysis. When these samples were further purified by allowing ammonia gas to escape and AgCl to crystallize slowly from ammonical solution, the problem disappeared.

Procedure

Four randomly selected vials (5 for lot 1) from each of the seven pools of bovine blood serum were used for the determination of chloride ion concentrations. The frozen samples were allowed to thaw and equilibrate to room temperature. One-gram sub-samples were taken from each of the vials and a duplicate sample was taken from one of the vials from each lot. Each sub-sample was then treated as follows:

The 1-g sub-sample was spiked with ^{37}Cl (sufficient to give a 35/37 ratio of approximately one), 8 mL of 0.1 mol/L HNO_3 was added, and the solution was thoroughly mixed and heated for two hours to equilibrate natural chloride with the spike chloride. Protein was then precipitated with ammonium molybdate solution and removed by filtration.

The chloride in the "protein-free" filtrate was precipitated as silver chloride which was allowed to settle from the solution. The supernatant solution was removed by decantation and the AgCl was dissolved with a minimum of ammonium hydroxide solution. AgCl was reprecipitated by the addition of nitric acid, separated by centrifugation and redissolved in concentrated ammonium hydroxide. Further purification was accomplished by allowing ammonia gas to escape and AgCl to slowly crystallize. The supernatant liquid was withdrawn and AgCl was again recrystallized from ammonium hydroxide solution. Finally, the recrystallized AgCl was dissolved in concentrated ammonium hydroxide to give a chloride concentration of 3 mg/mL.

Two different mass spectrometers were used for chlorine isotopic ratio measurements. One instrument was dedicated to blanks and separated isotope samples and the other to spiked samples and the natural isotopic standard. The mass spectrometric technique is described in NBS Technical Note 277 [5]. Major modifications in the procedure were the use of degassed filaments and reduction of the sample size per analyses to approximately 60 μg .

Results

The results of these determinations are shown in Table 1. The blank correction based on six blank determinations was 0.7 μg or less than 0.03 percent of the amount of chloride present in any sample. The results are reported both on a weight and a volume basis using an average density of 1.0312 g/mL at 23 °C for all lots of serum. The indicated uncertainty is an estimated limit of error, and is larger than the 95 percent confidence limits for a single determination ($t\sigma$) calculated from the concentration data. The additional allowance is made for possible error contributions

from spike calibrations and background signals. The estimated accuracy is 0.5 percent and includes allowance for all known sources of systematic error.

References

- [1] Shields, W. R., Ed., Analytical Mass Spectrometry Section: Summary of Activities, July 1966 to June 1967, U. S. National Bureau of Standards Technical Note 426, 1-53, U. S. Government Printing Office, Washington, D. C. 20402 (1967).
- [2] Garner, E. L., Machlan, L. A., and Shields, W. R., Standard Reference Materials: Uranium Isotopic Standard Reference Materials, U. S. National Bureau of Standards Special publication 260-27, 1-150, U. S. Government Printing Office, Washington, D. C. 20402 (1971).
- [3] Shields, W. R., Garner, E. L., and Dibeler, V. H., J. Res. Nat. Bur. Stand. (U.S.), 66A (Phys. and Chem.), No. 1, 1-3 (Jan.-Feb. 1962).
- [4] Folin, O. and Wu, H., J. Biol. Chem. 38, 81 (1919).
- [5] Shields, W. R., Editor, NBS Technical Note 277, 99 pages, U. S. Government Printing Office, Washington, D. C. 20234 (1966).

Table 1. Chloride in CDC Serum.

<u>Pool</u>	<u>Sub-Sample</u>	<u>Chloride Concentration</u>	
		<u>mmol/kg</u>	<u>mmol/L</u>
P1	1-1	76.95	79.35
	2-1	76.91	79.31
	3-1	76.63	79.02
	4-1	76.92	79.32
	5-1	76.85	79.25
	5-2	76.92	79.32
	Average	76.9 \pm 0.4	79.2 \pm 0.4 ^a
P2	1-1	81.83	84.38
	2-1	82.06	84.62
	3-1	81.90	84.46
	4-1	81.94	84.50
	4-2	81.95	84.40
	Average	81.9 \pm 0.4	84.5 \pm 0.4 ^a
P3	1-1	91.18	94.02
	2-1	91.12	93.96
	3-1	91.24	94.09
	4-1	91.14	93.98
	4-2	91.22	94.06
	Average	91.2 \pm 0.5	94.0 \pm 0.5 ^a
P4	1-1	98.62	101.69
	2-1	98.76	101.85
	3-1	98.68	101.76
	4-1	98.70	101.78
	4-2	98.66	101.74
	Average	98.7 \pm 0.5	101.8 \pm 0.5 ^a
P5	1-1	103.77	107.00
	2-1	104.00	107.25
	3-1	103.95	107.20
	4-1	103.86	107.10
	4-2	103.98	107.22
	Average	103.9 \pm 0.5	107.2 \pm 0.5 ^a

continued

Table 1 (continued)

<u>Pool</u>	<u>Sub-Sample</u>	<u>Chloride Concentration</u>			
		<u>mmol/kg</u>		<u>mmol/L</u>	
P6	1-1	109.45		112.86	
	2-1	109.51		112.93	
	3-1	109.56		112.98	
	4-1	109.50		112.92	
	4-2	109.53		112.95	
	Average	109.5	0.5	112.9	0.6 ^a
P7	1-1	113.15		116.68	
	2-1	113.15		116.68	
	3-1	113.34		116.87	
	4-1	113.38		116.92	
	4-2	113.14		116.67	
	Average	113.2	0.6	116.8	0.6 ^a

^aEstimated maximum error of 0.5 percent of the value as reported by NBS Analytical Mass Spectrometry Section. This estimated maximum error includes both imprecision and an estimated upper bound for possible systematic errors. The estimated maximum error is believed to be equal to or greater than the true error for the 95 percent confidence limits.

APPENDIX D

Note 1:

A temperature range of ± 2 °C is designated as the operating temperature. In this temperature range the maximum difference in aqueous solution volumes due to thermal expansion of the liquid is 0.102 percent and the difference in volume due to the volumetric glassware is very small since the coefficient of expansion for borosilicate glass is 0.00001 per °C. (J. Lembeck, "Calibration of Small Volumetric Laboratory Glassware", NBSIR Report 74-461, 1974, Institute for Basic Standards, National Bureau of Standards, Washington, D. C. 20234). We judge these errors to be acceptable for this reference method. Larger temperature variations may necessitate appropriate correction.

Note 2:

Glassware Required:

a) Micropipetting alternative:

Volumetric Flasks: Five 250-mL.

Pipets: Micropipets as required for instrument with the accuracy requirement specified in Section IIIC-2.

b. Macropipetting alternative:

Volumetric Flasks: Ten 250-mL plus as many additional 250-mL volumetric flasks as there are samples to be analyzed.

Pipets: One 5-mL; five 4-mL plus as many additional 4-mL pipets as there are samples to be analyzed.

Note 3:

Cleaning of Glassware:

a) Clean the glassware in the following manner:

- (1) soak glassware for 60 min in 0.77 mol/L HNO_3 .
- (2) Rinse six times with a volume of water equal to at least 10 percent of the container volume.
- (3) Use immediately or air dry (inverted in a dust-free environment) for later use.

Note 4:

The atomic weights used in this report are those reported in : Pure and Applied Chemistry, 47, 75 (1976).

Note 5:

If the wash solution does not drain cleanly from the pipet, wash with 0.77 mol/L HNO_3 , H_2O , MeOH, 70:30 v/v CHCl_3 :MeOH, MeOH, and H_2O in that order. Then repeat the water wash and check that the pipet does drain properly.

Note 6:

The three following pages are examples of the data sheets returned from each laboratory after each round robin test.

ELECTROLYTES IN SERUM -- CLINICAL REFERENCE METHOD

CHLORIDE ION

LABORATORY 5 ANALYST XY INTERLABORATORY EXERCISE II
DATE SAMPLES RECEIVED 2-18-76 DATES ANALYZED (1) 2-24 (2) 2-26
American Aminco-Cotlove
INSTRUMENT MANUFACTURER Instrument Co. MODEL Chloride Titrator
METHOD: MICRO _____ MACRO X DIRECT READING _____ TIME X
VOLUME TRANSFERRED TO TITRATION CELL 4.0 (ML)
TYPE MICROPIPET USED _____
6.4 mL conc. Nitric Acid +
ELECTROLYTE USED 100 mL Glacial Acetic QS to 1 liter
DISPERSANT USED Gelatin Reagent (6.2 g to 1 liter of hot water)

	Weight ratio
Composed of: Knox Gelatin #1	60
Thymol Blue	1
Thymol	1

COMMENTS: Due to time involved in performing the macro
procedure on 10 samples, the dilutions of the serum samples
were made on the day before the titrations were performed.
They were allowed to set overnight at room temperature and
were shaken vigorously to ensure thorough mixing before
the analyses. This change was discussed with and approved
by NBS personnel.

DATA SHEET: STANDARD CURVE

LAB 5 DAY 2/24/76

PROTOCOL USED; MANUAL X SEMI-AUTOMATED

<u>STANDARD</u>	<u>CALCULATED ION CONCENTRATION, MMOL/L</u>	<u>DIRECT READ-OUT OR TIME</u>
1	<u>75.01</u>	<u>23.2</u>
2	<u>90.01</u>	<u>27.9</u>
3	<u>100.01</u>	<u>31.0</u>
4	<u>110.00</u>	<u>34.2</u>
5	<u>125.00</u>	<u>39.0</u>
6	<u> </u>	<u> </u>
DILUENT BLANK		<u>1.7</u>

DATA REPORTING SHEET FOR VALID MEASUREMENTS

PROTOCOL USED: MACRO X MICRO _____
 LAB 5 ION Cl⁻ INTERLABORATORY EXERCISE II
 DATE ANALYZED 2/24 OPERATOR XY

SAMPLE # <u>536603</u>		TIME OR DIRECT READOUT			
STANDARD CONCENTRATIONS MMOL/L (CALCULATED)	VALID SET	LO STD (C ₁)	SAMPLE (Y)	HI STD (C ₂)	\hat{C}
LO <u>110.00</u> (C ₁)	1.	<u>35.6</u>	<u>37.9</u>	<u>40.5</u>	<u>117.04</u>
	2.	<u>35.8</u>	<u>37.9</u>	<u>40.6</u>	<u>116.56</u>
HI <u>125.00</u> (C ₂)	3.	<u>35.8</u>	<u>37.6</u>	<u>40.5</u>	<u>115.74</u>


SAMPLE # <u>496322</u>		TIME OR DIRECT READOUT			
STANDARD CONCENTRATIONS MMOL/L (CALCULATED)	VALID SET	LO STD (C ₁)	SAMPLE (Y)	HI STD (C ₂)	\hat{C}
LO <u>75.01</u> (C ₁)	1.	<u>24.8</u>	<u>26.0</u>	<u>29.4</u>	<u>78.92</u>
	2.	<u>24.9</u>	<u>25.9</u>	<u>29.4</u>	<u>78.34</u>
HI <u>90.01</u> (CH ₂)	3.	<u>24.8</u>	<u>26.1</u>	<u>29.3</u>	<u>79.34</u>

SAMPLE # <u>453700</u>		TIME OR DIRECT READOUT			
STANDARD CONCENTRATIONS MMOL/L (CALCULATED)	VALID SET	LO STD (C ₁)	SAMPLE (Y)	HI STD (C ₂)	\hat{C}
LO <u>100.01</u> (C ₁)	1.	<u>32.7</u>	<u>34.9</u>	<u>35.9</u>	<u>106.88</u>
	2.	<u>32.6</u>	<u>34.8</u>	<u>36.1</u>	<u>106.29</u>
HI <u>110.00</u> (C ₁)	3.	<u>32.7</u>	<u>34.8</u>	<u>36.0</u>	<u>106.37</u>

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. NBS SP-260-67	2. Gov't. Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE A REFERENCE METHOD FOR THE DETERMINATION OF CHLORIDE IN SERUM		5. Publication Date November 1979	
		6. Performing Organization Code	
7. AUTHOR(S) Rance A. Velapoldi, Robert C. Paule, Robert Schaffer, John Mandel, Thomas J. Murphy, and John W. Gramlich		8. Performing Organ. Report No.	
9. PERFORMING ORGANIZATION NAME AND ADDRESS NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, DC 20234		10. Project/Task/Work Unit No.	
		11. Contract/Grant No.	
12. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS (Street, City, State, ZIP) Same as above		13. Type of Report & Period Covered Final	
		14. Sponsoring Agency Code	
15. SUPPLEMENTARY NOTES Library of Congress Catalog Card Number: 79-600174 <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.			
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.) Guided by a committee of experts in clinical chemistry, a reference method was established for the determination of serum chloride based on a coulometric titration- amperometric end-point determination (C-A). Its accuracy was evaluated by comparing the values obtained by use of the method in 14 laboratories against the results obtained by a definitive analytical method based on isotope dilution-mass spectrometry (IDMS). Seven serum pools with chloride concentrations in the range 79.2 to 116.8 mmol/L were analyzed. Micro- and macropipetting alternatives were tested using sample sizes of 0.010-0.100 and 5.0 mL, respectively. The laboratories used several different C-A instruments. The results showed that the standard error for a single laboratory's performance of the procedure was approx- imately 1.0 mmol/L with a maximum bias of 0.5 mmol/L over the range of concentrations studied. These values are within the accuracy and precision goals that had been set by the committee. The results from the micro- and macropipetting techniques were similar. The calibration curve data showed excellent linearity over the total concentration range, with 12 of 14 curves having standard deviation of fit of less than 0.80 mmol/L. With appropriate experimental design, the reference method may be used to establish the accuracy of field methods as well as to determine reference chloride values for pooled sera.			
17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons) Amperometry; chloride analysis; clinical analysis; clinical chemistry; coulometry; definitive method; electrolytes; reference method; serum chloride analysis.			
18. AVAILABILITY <input checked="" type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input checked="" type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office, Washington, DC 20402, SD Stock No. SN003-003- 02136-9 <input type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA. 22161		19. SECURITY CLASS (THIS REPORT) UNCLASSIFIED	21. NO. OF PRINTED PAGES 97
		20. SECURITY CLASS (THIS PAGE) UNCLASSIFIED	22. Price \$3.75



U.S. DEPARTMENT OF COMMERCE

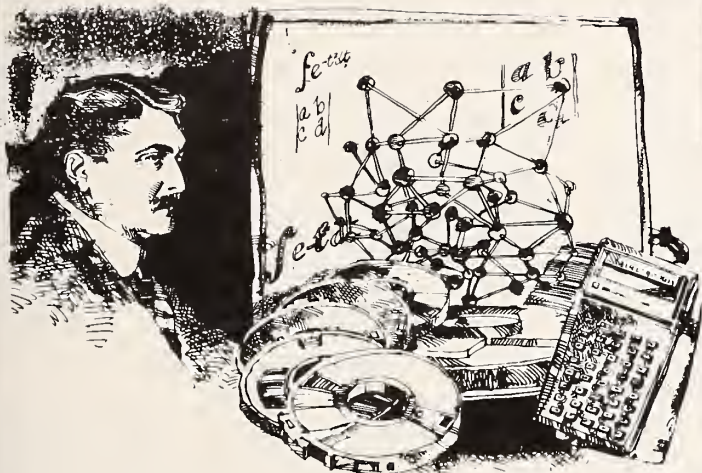

Subscribe now— The new National Bureau of Standards Journal

The expanded Journal of Research of the National Bureau of Standards reports NBS research and development in those disciplines of the physical and engineering sciences in which the Bureau is active. These include physics, chemistry, engineering, mathematics, and computer sciences. Papers cover a broad range of subjects, with major emphasis on measurement methodology, and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Bureau's technical and scientific programs. As a special service to subscribers each issue contains complete citations to all recent NBS publications in NBS and non-NBS media. Issued six times a year. Annual subscriptions: domestic \$17.00; foreign \$21.25. Single copy. \$3.00 domestic; \$3.75 foreign.

- **Note:** The Journal was formerly published in two sections: Section A "Physics and Chemistry" and Section B "Mathematical Sciences."

NBS Board of Editors
Churchill Eisenhart,
Executive Editor (Mathematics)
John W. Cooper (Physics)
Donald D. Wagman (Chemistry)
Andrew J. Fowell (Engineering)
Joseph O. Harrison (Computer Science)
Howard J. M. Hanley (Boulder Labs.)

Subscription Order Form

Enter my subscription to NBS Journal of Research
at \$17.00. Add \$4.25 for foreign mailing. No additional postage is
required for mailing within the United States or its possessions.
(SJRA—File Code 2N)

Send Subscription to:

Name-First, Last		
Company Name or Additional Address Line		
Street Address		
City	State	Zip Code
(or) COUNTRY		

PLEASE PRINT

Credit Card Orders Only

Total charges \$ _____ **Fill in the boxes below.**

Credit
Card No.[illegible]

Master Charge

Interbank No.

--	--	--	--	--

Expiration Date

Month/Year

--	--	--	--

- ☐ Remittance Enclosed. Domestic:
Check or money order. Foreign:
International money order,
draft on an American or Canadian
Bank, or by UNESCO coupons,
Made payable to the
Superintendent of Documents.
- ☐ Charge to my Deposit
Account No.

MAIL ORDER FORM TO:
Superintendent of Documents
Government Printing Office
Washington, D.C. 20402

NBS TECHNICAL PUBLICATIONS

PERIODICALS

JOURNAL OF RESEARCH—The Journal of Research of the National Bureau of Standards reports NBS research and development in those disciplines of the physical and engineering sciences in which the Bureau is active. These include physics, chemistry, engineering, mathematics, and computer sciences. Papers cover a broad range of subjects, with major emphasis on measurement methodology and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Bureau's technical and scientific programs. As a special service to subscribers each issue contains complete citations to all recent Bureau publications in both NBS and non-NBS media. Issued six times a year. Annual subscription: domestic \$17; foreign \$21.25. Single copy, \$3 domestic; \$3.75 foreign.

NOTE: The Journal was formerly published in two sections: Section A "Physics and Chemistry" and Section B "Mathematical Sciences."

DIMENSIONS/NBS—This monthly magazine is published to inform scientists, engineers, business and industry leaders, teachers, students, and consumers of the latest advances in science and technology, with primary emphasis on work at NBS. The magazine highlights and reviews such issues as energy research, fire protection, building technology, metric conversion, pollution abatement, health and safety, and consumer product performance. In addition, it reports the results of Bureau programs in measurement standards and techniques, properties of matter and materials, engineering standards and services, instrumentation, and automatic data processing. Annual subscription: domestic \$11; foreign \$13.75.

NONPERIODICALS

Monographs—Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

Handbooks—Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

Special Publications—Include proceedings of conferences sponsored by NBS, NBS annual reports, and other special publications appropriate to this grouping such as wall charts, pocket cards, and bibliographies.

Applied Mathematics Series—Mathematical tables, manuals, and studies of special interest to physicists, engineers, chemists, biologists, mathematicians, computer programmers, and others engaged in scientific and technical work.

National Standard Reference Data Series—Provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated. Developed under a worldwide program coordinated by NBS under the authority of the National Standard Data Act (Public Law 90-396).

NOTE: The principal publication outlet for the foregoing data is the Journal of Physical and Chemical Reference Data (JPCRD) published quarterly for NBS by the American Chemical Society (ACS) and the American Institute of Physics (AIP). Subscriptions, reprints, and supplements available from ACS, 1155 Sixteenth St., NW, Washington, DC 20056.

Building Science Series—Disseminates technical information developed at the Bureau on building materials, components, systems, and whole structures. The series presents research results, test methods, and performance criteria related to the structural and environmental functions and the durability and safety characteristics of building elements and systems.

Technical Notes—Studies or reports which are complete in themselves but restrictive in their treatment of a subject. Analogous to monographs but not so comprehensive in scope or definitive in treatment of the subject area. Often serve as a vehicle for final reports of work performed at NBS under the sponsorship of other government agencies.

Voluntary Product Standards—Developed under procedures published by the Department of Commerce in Part 10, Title 15, of the Code of Federal Regulations. The standards establish nationally recognized requirements for products, and provide all concerned interests with a basis for common understanding of the characteristics of the products. NBS administers this program as a supplement to the activities of the private sector standardizing organizations.

Consumer Information Series—Practical information, based on NBS research and experience, covering areas of interest to the consumer. Easily understandable language and illustrations provide useful background knowledge for shopping in today's technological marketplace.

Order the above NBS publications from: Superintendent of Documents, Government Printing Office, Washington, DC 20402.

Order the following NBS publications—FIPS and NBSIR's—from the National Technical Information Services, Springfield, VA 22161.

Federal Information Processing Standards Publications (FIPS PUB)—Publications in this series collectively constitute the Federal Information Processing Standards Register. The Register serves as the official source of information in the Federal Government regarding standards issued by NBS pursuant to the Federal Property and Administrative Services Act of 1949 as amended, Public Law 89-306 (79 Stat. 1127), and as implemented by Executive Order 11717 (38 FR 12315, dated May 11, 1973) and Part 6 of Title 15 CFR (Code of Federal Regulations).

NBS Interagency Reports (NBSIR)—A special series of interim or final reports on work performed by NBS for outside sponsors (both government and non-government). In general, initial distribution is handled by the sponsor; public distribution is by the National Technical Information Services, Springfield, VA 22161, in paper copy or microfiche form.

BIBLIOGRAPHIC SUBSCRIPTION SERVICES

The following current-awareness and literature-survey bibliographies are issued periodically by the Bureau:

Cryogenic Data Center Current Awareness Service. A literature survey issued biweekly. Annual subscription: domestic \$25; foreign \$30.

Liquefied Natural Gas. A literature survey issued quarterly. Annual subscription: \$20.

Superconducting Devices and Materials. A literature survey issued quarterly. Annual subscription: \$30. Please send subscription orders and remittances for the preceding bibliographic services to the National Bureau of Standards, Cryogenic Data Center (736) Boulder, CO 80303.

U.S. DEPARTMENT OF COMMERCE
National Bureau of Standards
Washington, D.C. 20234

OFFICIAL BUSINESS

Penalty for Private Use, \$300

POSTAGE AND FEES PAID
U.S. DEPARTMENT OF COMMERCE
COM-215



SPECIAL FOURTH-CLASS RATE
BOOK
