


NIST Measurement Services:

Gas Flowmeter Calibrations with the 34 L and 677 L *PVT*t Standards

NIST Special Publication 250-63

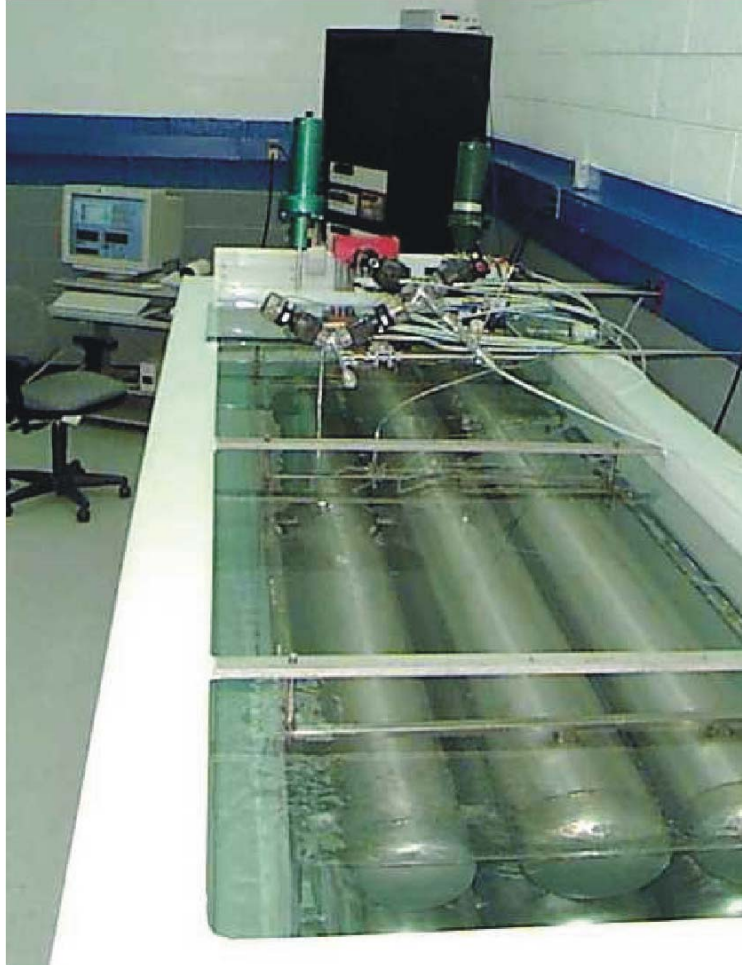

John D. Wright, Aaron N. Johnson, Michael R. Moldover, and Gina M. Kline

U. S. Department of Commerce
Technology Administration
National Institute of Standards and Technology

Table of Contents

Gas Flowmeter Calibrations with the 34 L and 677 L <i>PVTt</i> Standards	
Abstract.....	1
1 Introduction.....	2
2 Description of Measurement Services	4
3 Procedures for Submitting a Flowmeter for Calibration.....	7
4 Pressure, Volume, Temperature, and time (<i>PVTt</i>) Standards	7
5 Design and Operation of the <i>PVTt</i> Standard.....	11
5.1 Average Temperature of the Collected Gas	11
5.2 Mass Change in the Inventory Volume	16
5.3 Measurement of the Tank and Inventory Volumes	24
6 Uncertainty Analysis of the 34 L and 677 L <i>PVTt</i> Flow Standards.....	27
6.1 Techniques for Uncertainty Analysis	28
6.2 Mass Flow Uncertainty	31
6.3 Pressure	33
6.4 Temperature.....	36
6.5 Compressibility, Molecular Weight, and Gas Constant	39
6.6 Density.....	42
6.7 Collection Time	43
6.8 Volume of the 677 Liter Collection Tank (Gravimetric Method).....	44
6.9 Volume of the 34 Liter Collection Tank (Volume Expansion Method)	48
6.10 Inventory Volume.....	50
7 Experimental Verification of the Uncertainty of the 34 L and 677 L <i>PVTt</i> Gas Flow Standards.....	55
7.1 Comparison of the 34 L and 677 L Flow Standards.....	56
7.2 Multiple Diversions in the 677 L Flow Standard	59
8 Summary	60
9 References.....	62
Appendix: Sample Calibration Report	

Abstract

This document provides a description of the 34 L and 677 L pressure, volume, temperature, and time (*PVTt*) primary gas flow standards operated by the National Institute of Standards and Technology (NIST) Fluid Flow Group. These facilities are used to provide gas flowmeter calibration services as reported in NIST Special Publication 250 [Marshall 1998] for Test Numbers 18010C and 18050C. The *PVTt* standard uses two collection tanks and two diverter valve systems to perform gas flowmeter calibrations between 1 L/min and 2000 L/min (the reference temperature and pressure conditions are 293.15 K and 101.325 kPa). The standard measures flow by collecting gas in a tank of known volume during a measured time interval. The uncertainty of the flow measurement is between 0.02 % and 0.05 % ($k = 2$ or approximately 95 % confidence level), depending on the gas used and where in the flow range the facilities are being used.

We provide an overview of the gas flow calibration service and the procedures for customers to submit their flowmeters to NIST for calibration. We describe the significant and novel features of the standard and analyze its uncertainty. The gas collection tanks have a small diameter and are immersed in a uniform, stable, thermostatted water bath. The collected gas achieves thermal equilibrium rapidly, and the uncertainty of the average gas temperature is only 7 mK ($22 \times 10^{-6} T$). A novel operating method leads to essentially zero mass change in and very low uncertainty contributions from the inventory volume.

Gravimetric and volume expansion techniques were used to determine the tank and the inventory volumes. Gravimetric determinations of collection tank volume made with nitrogen and argon agree with a standard deviation of $16 \times 10^{-6} V_T$. The largest source of uncertainty in the flow measurement is drift of the pressure sensor over time, which contributes a relative standard uncertainty of 60×10^{-6} to the determinations of the volumes of the collection tanks and to the flow measurements. Throughout the range 3 L/min to 110 L/min, flows were measured independently using the 34 L and the 677 L collection systems, and the two systems agreed within a relative difference of 150×10^{-6} .

Double diversions were used to evaluate the 677 L system over a range of 300 L/min to 1600 L/min, and the relative differences between single and double diversions were less than 75×10^{-6} .

Key words: calibration, correlated uncertainty, flow, flowmeter, gas flow standard, inventory volume, *PVTt* standard, mass cancellation, meter, sensor response, uncertainty.

1 Introduction

Calibrations of gas flowmeters are performed with primary standards [ISO 1993] that are based on measurements of more fundamental quantities, such as length, mass, and time. Primary flow calibrations are accomplished by collecting a measured mass or volume of the flowing fluid over a measured time interval under approximately steady state conditions of flow, pressure, and temperature at the meter under test. The flow measured by the primary standard is computed along with the average of the flow indicated by the meter under test during the collection interval. All of the quantities measured in connection with the calibration standard (i.e., temperature, pressure, time, etc.) are traceable to established national standards. A gas calibration facility consists of a fluid source (e.g., an air compressor or compressed gas cylinders), a test section that provides stable thermodynamic conditions and a fully developed flow profile, and a system for diverting and timing the collection of a quantity of the fluid.

NIST offers calibrations of gas flowmeters in order to provide traceability to flowmeter manufacturers, secondary flow calibration laboratories, and flowmeter users. For a calibration fee, NIST calibrates a customer's flowmeter and delivers a calibration report that documents the calibration procedure, the calibration results, and their uncertainty. The flowmeter and its calibration results may be used in different ways by the customer. The flowmeter is often used as a transfer standard to perform a comparison of the customer's primary standards to the NIST primary standards so that the customer can establish traceability, validate their uncertainty analysis, and demonstrate proficiency.

Customers with no primary standards use their NIST calibrated flowmeters as working standards or reference standards in their laboratory to calibrate other flowmeters.

The Fluid Flow Group of the Process Measurements Division (part of the Chemical Science and Technology Laboratory) at NIST provides gas flow calibration services over a range of 1 L/min to 77600 L/min.* Table 1 presents the flow ranges covered by the primary gas flow standards in the Fluid Flow Group. Flows from 900 L/min to 77600 L/min can be measured with a 26 m³ *PVTt* standard that was built in the late 1960's and has been upgraded several times [Olsen and Baumgarten 1971, Johnson et al. 2003]. Flows of 1 L/min or less can be calibrated by the NIST Pressure and Vacuum Group.

Table 1. Primary gas flow calibration capabilities within the NIST Fluid Flow Group.

Flow Standard	Flow Range (L/min)	Gas	Pressure Range (kPa)	Uncertainty (<i>k</i> = 2) (%)
34 L <i>PVTt</i>	1 - 100	N ₂	100 – 7000	0.03 – 0.04
	1 - 100	Air	100 - 1700	0.05
	1 - 100	CO ₂	100 - 4000	0.05
	1 - 100	Ar	100 - 7000	0.05
	1 - 100	He	100 - 7000	0.05
677 L <i>PVTt</i>	10 - 150	N ₂	100 - 800	0.02 – 0.03
	10 - 2000	Air	100 - 1700	0.05
26 m ³ <i>PVTt</i>	860 - 77600	Air	100 - 800	0.13

This document describes the theory, methods of operation, and uncertainty of the 34 L and 677 L *PVTt* primary standards that cover the 1 L/min to 2000 L/min flow range. From the late 1960's to 2002, this flow range was covered by a set of three mercury-sealed piston provers and two bell provers [Wright and Mattingly 1998]. The 34 L and 677 L *PVTt* standards were completed in 2002, and for a period of one year we used both

* Reference conditions of 293.15 K and 101.325 kPa are used throughout this document for volumetric flows.

the old and the new primary standards for customer calibrations. In 2003, the new primary standards and their uncertainty statements were sufficiently validated [Wright 2003A], and we began using the new standards alone to calibrate customers' flowmeters.

The *PVTt* standard is ideally suited for the calibration of critical flow venturis (CFV's) since they provide pressure isolation and provide a well defined boundary for the inventory volume. A set of NIST CFV's, calibrated by the *PVTt* standards are used as working standards in another calibration facility called the Working Gas Flow Standard (WGFS). The WGFS provides calibrations, particularly for laminar flowmeters, in which the reference flow is measured with uncertainty of 0.1% or less. The methods and uncertainty analysis for the WGFS are covered in a separate document.

2 Description of Measurement Services

Customers should consult the web address www.nist.gov/fluid_flow to find the most current information regarding our calibration services, calibration fees, technical contacts, and flowmeter submittal procedures.

NIST uses the *PVTt* primary standards described herein to provide gas flowmeter calibrations for flows between 1 L/min and 2000 L/min. The facility has been used at flows as low as 0.025 L/min, but calibrations below 1 L/min should be discussed with the technical contacts before a flowmeter is submitted for such low flows.

The gases available for calibrations in the 34 L *PVTt* standard are dry air, nitrogen, carbon dioxide, argon, and helium. The source of air, at pressures up to 1700 kPa, is an oil-free reciprocating compressor and a refrigeration drier. The dew point temperature of the dried air is 250 K so the mole fraction of water in the air is 0.08 %. Nitrogen (at pressures up to 800 kPa and purity of 99.998%) is supplied by liquid nitrogen dewars. Higher pressures of nitrogen as well as argon, carbon dioxide, and helium gas can be supplied from compressed gas cylinders. Other non-toxic, non-corrosive gases can be accommodated upon customer request. While other gases are certainly feasible in the 677

L *PVTt* standard, gases are practically limited to air from the compressor and nitrogen from dewars since a very large number of gas cylinders would be necessary to provide gas at 2000 L/min. The gas temperatures are nominally room temperature.

Readily available fittings for the installation of flowmeters in the 34 L and 677 L *PVTt* standards are Swagelok* (1/8" to 1"), A/N 37 degree flare (1/4" to 1"), national pipe thread or NPT (1/8" to 3"), VCR (1/4" and 1/2"), and VCO (1/2" and 1").

Meters can be tested if the flow range, gas, and piping connections are suitable, and if the system to be tested has precision appropriate for calibration with the NIST flow measurement uncertainty. The vast majority of flowmeters calibrated in the gas flow calibration service are either critical flow venturis (critical nozzles) or laminar flowmeters since these are presently regarded as the best candidates for transfer and working standards by the gas flow metrology community [Wright 2003B]. Other meter types that we have tested include positive displacement meters, roots meters, rotary gas meters, thermal mass flowmeters, and turbine meters. Meter types with calibration instability significantly larger than the primary standard uncertainty should not be calibrated with the NIST standards for economic reasons. For example, a rotameter for which the float position is read by the operator's eye normally cannot be read with precision any better than 1 %. It is not practical to pay thousands of dollars to obtain 0.05 % or less uncertainty flow data from NIST for such a flowmeter when 0.5% data is perfectly adequate and available from other laboratories at significantly lower cost.

A normal flow calibration performed by the NIST Fluid Flow Group consists of five flows spread over the range of the flowmeter. For a CFV, typical calibration set points are at 200 kPa, 300 kPa, 400 kPa, 500 kPa, and 600 kPa. A laminar flowmeter is normally calibrated at 10 %, 25 %, 50 %, 75 %, and 100 % of the meter full scale. At each of these flow set points, three (or more) flow measurements are made with the *PVTt*

* Certain commercial equipment, instruments, or materials are identified in this paper to foster understanding. Such identification does not imply recommendation or endorsement by the National Institute of Standards and Technology, nor does it imply that the materials or equipment identified are necessarily the best available for the purpose.

standard. The same set point flows are tested on a second occasion, but the flows are tested in decreasing order instead of the increasing order of the first set. Therefore, the final data set consists of six (or more) primary flow measurements made at five flow set points, i.e., 30 individual flow measurements. The sets of three measurements can be used to assess repeatability, while the sets of six can be used to assess reproducibility. For further explanation, see the sample calibration report that is included in this document as an appendix. Variations on the number of flow set points, spacing of the set points, and the number of repeated measurements can be discussed with the NIST technical contacts. However, for data quality assurance reasons, we rarely will conduct calibrations involving fewer than three flow set points and two sets of three flow measurements at each set point.

The Fluid Flow Group prefers to present flowmeter calibration results in a dimensionless format that takes into account the physical model for the flowmeter type [Wright 1998]. The dimensionless approach facilitates accurate flow measurements by the flowmeter user even when the conditions of usage (gas type, temperature, pressure) differ from the conditions during calibration. Hence for a CFV calibration, the calibration report will present Reynolds number and discharge coefficient and for a laminar flowmeter, a report presents the viscosity coefficient and the flow coefficient. In order to calculate the uncertainty of these flowmeter calibration factors, we must know the uncertainty of the standard flow measurement as well as the uncertainty of the instrumentation associated with the meter under test (normally absolute pressure, differential pressure, and temperature instrumentation). We prefer to connect our own instrumentation (temperature, pressure, etc.) to the meter under test since they have established uncertainty values based on calibration records that we would not have for the customer's instrumentation. In some cases, it is impractical to install our own instrumentation on the meter under test and the meter under test outputs flow. In these cases, we provide a table of flow indicated by the meter under test, flow measured by the NIST standard, and the uncertainty of the NIST flow value.

3 Procedures for Submitting a Flowmeter for Calibration

The Fluid Flow Group follows the policies and procedures described in Chapters 1, 2, and 3 of the NIST Calibration Services Users Guide [Marshall 1998]. These chapters can be found on the internet at the following addresses:

<http://ts.nist.gov/ts/htdocs/230/233/calibrations/Policies/policy.htm>,

<http://ts.nist.gov/ts/htdocs/230/233/calibrations/Policies/domestic.htm>, and

<http://ts.nist.gov/ts/htdocs/230/233/calibrations/Policies/foreign.htm>.

Chapter 2 gives instructions for ordering a calibration for domestic customers and has the sub-headings: A.) Customer Inquiries, B.) Pre-arrangements and Scheduling, C.) Purchase Orders, D.) Shipping, Insurance, and Risk of Loss, E.) Turnaround Time, and F.) Customer Checklist. Chapter 3 gives special instructions for foreign customers. The web address www.nist.gov/fluid_flow has information more specific to the gas flow calibration service, including the technical contacts in the Fluid Flow Group, fee estimates, and turnaround times.

4 Pressure, Volume, Temperature, and time (*PVTt*) Standards

PVTt systems have been used as primary gas flow standards by NIST and other laboratories for more than 30 years [Olsen and Baumgarten 1971, Kegel 1995, Ishibashi et al. 1985, Wright 2001]. The *PVTt* systems at NIST consist of a flow source, valves for diverting the flow, a collection tank, a vacuum pump, pressure and temperature sensors, and a critical flow venturi (CFV) which isolates the meter under test from the pressure variations in the downstream piping and tank (see Fig. 1).

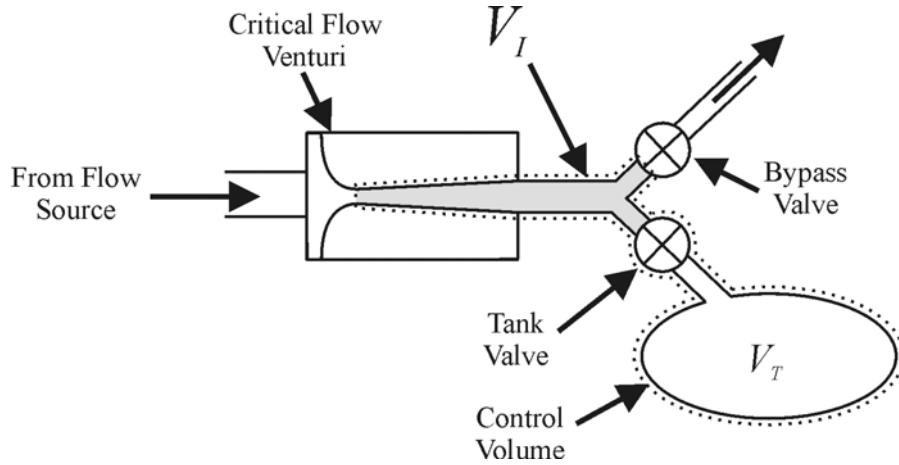


Figure 1. Arrangement of equipment in a *PVTt* system.

The process of making a *PVTt* flow measurement normally entails the following steps:

1. Close the tank valve, open the bypass valve, and establish a stable flow through the CFV.
2. Evacuate the collection tank volume (V_T) with the vacuum pump.
3. Wait for pressure and temperature conditions in the tank to stabilize and then acquire initial values for the tank (P_T^i and T_T^i). These values will be used to calculate the initial density and the initial mass of gas in the tank (m_T^i).
4. Close the bypass valve and, during the “dead-end time” when both the bypass and tank valves are fully closed, choose a start time (t^i). At the same time, acquire the initial pressure and temperature in the inventory volume (P_I^i and T_I^i). These values will be used along with the equation of state for the gas and the inventory volume (V_I) to obtain an initial mass in the inventory volume (m_I^i). Shortly after the bypass valve is fully closed, open the tank valve.
5. Wait for the tank to fill to a prescribed upper pressure and then close the tank valve and choose the stop time (t^f) during the dead-end time. At the same time, acquire the pressure and temperature in the inventory volume (P_I^f and T_I^f) and hence the final mass in the inventory. Open the bypass valve.

6. Wait for stability and then acquire P_T^f and T_T^f and hence m_T^f .

By writing a mass balance for the control volume composed of the inventory and tank volumes (see the volume defined by the dashed line in Fig. 1), one can derive an equation for the average mass flow during the collection time:

$$\dot{m} = \frac{(m_T^f - m_T^i) + (m_I^f - m_I^i)}{t^f - t^i}, \quad (1)$$

or, neglecting the volume changes between the initial and final conditions:

$$\dot{m} = \frac{V_T(\rho_T^f - \rho_T^i) + V_I(\rho_I^f - \rho_I^i)}{t^f - t^i}, \quad (2)$$

where ρ is the gas density determined via a real gas equation of state, $\rho = (PM)/ZRT$, where M is the gas molecular weight, R is the universal gas constant, and Z is the compressibility factor.

The start and stop times can be chosen at any point during the dead-end time as long as the inventory conditions are measured coincidentally. Why is this true? Implicit in the $PVTt$ basis equation (Eq. 2) are two requirements: 1) the measurement of the initial and final densities must be coincident with the measurement of the start and stop times and 2) there must not be any other sources or sinks of mass flow to the control volume. The second condition is met for the entire time that the bypass valve is fully closed, including the start and stop dead-end times. It is not necessary that the initial and final determinations of the mass in the collection tank be done coincidentally with the start and stop times because the tank is free of leaks and it is advantageous to measure these mass values when the tank conditions have reached equilibrium. The freedom to choose the start and stop times from within the dead-end time intervals allows one to choose times where the initial and final inventory densities match, giving essentially zero mass change

in the inventory volume (Δm_I) and extremely good cancellation of certain correlated inventory uncertainties.

The *PVTt* measurement process can be performed in a “blow down” mode also, where initial and final values of the mass in a tank that is the *source* of flow instead of the collector of flow are utilized. Such a system has the advantage that a small compressor can be used to charge a large pressure vessel over a long period of time allowing one to achieve very large flows relatively inexpensively. The blow down method has the disadvantage that it is more difficult to maintain stable pressure and temperature conditions at the meter under test since the high-side pressure of the flow control throttling process is changing continuously as the tank discharges.

The bypass and tank valves can be operated with valve overlap, i.e. where one valve begins to open before the other is fully closed, or with zero overlap, where one is completely closed before the other begins to open (as described above) [Harris 1980]. With zero overlap, there is no question about lost or extra mass occurring during the diversion. For instance, if the tank is at an initial pressure less than atmospheric, when both valves are partially open, flow can enter the tank from the room instead of through the meter under test. Zero overlap avoids this possibility. For a zero overlap system it is important that any valve design be fast acting. There is a short period of time during the actuation of the diverter valves during which both valves are closed (the “dead end” time) and the mass of gas that passed through the critical venturi accumulates in the inventory volume. The mass accumulation leads to a pressure rise in the inventory volume that will depend on the mass flow, the size of the inventory volume, and the dead end time of the diverter valves. The pressure in the inventory must not be permitted to reach a high enough level that the flow at the venturi is no longer critical, lest pressure perturbations reach the meter under test and disrupt the steady state flow conditions at the meter.

5 Design and Operation of the *PVTt* Standard

Experience with a previous, 26 m³ *PVTt* flow standard at NIST indicated that improvements in temperature and pressure instrumentation as well as in the design and operation of the new system would be necessary in order to achieve an uncertainty of 0.05 % or better [Johnson et al. 2003]. In the following three sections we will describe aspects of the design and operation of the new flow standard that are important to achieve this low uncertainty. The first of these sections describes the measurement of the average temperature of the collected gas. A subsequent section describes the procedures that minimize the uncertainty of the mass change in the inventory volume, and the last section describes the determination of the tank and inventory volumes.

5.1 Average Temperature of the Collected Gas

One of the most important sources of uncertainty in a *PVTt* flow standard is the measurement of the average temperature of the gas in the collection tank, particularly after filling. The evacuation and filling processes lead to cooling and heating of the gas within the volume due to flow work and kinetic energy phenomena [Wright and Johnson 2000]. The magnitude of the effect depends on the flow; however, the temperature rise in an adiabatic tank can be 10 K or more. Hence, immediately after filling and evacuation, significant thermal gradients exist within the collected gas. For a large tank, the equilibration time for the gas temperature can be many hours. If the exterior of the tank has non-isothermal or time varying temperature conditions, stratification and non-uniform gas temperatures will persist even after many hours [Johnson et al. 2003].

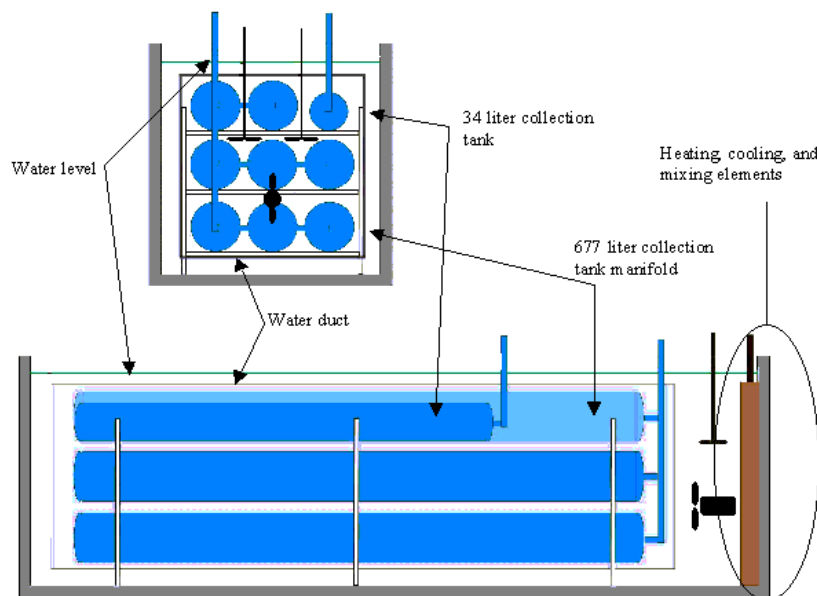


Figure 2. A schematic of the *PVTt* collection tanks, water bath, duct, and temperature control elements.

In this work, we avoided long equilibration times and the difficult problem of measuring the average temperature of a non-uniform gas by designing the collection tanks for rapid equilibration of the collected gas and by immersing the tanks in a well-mixed, thermostatted, water bath (see Fig. 2 and Fig. 3). There are two control volumes, a 34 L collection tank and a 677 L collection tank. Because the equilibration of the 677 L tank is slower, we consider it here. The 677 L tank is composed of eight, cylindrical, 2.5 m long, stainless steel shells connected in parallel by a manifold. Each shell has a wall thickness of $l = 0.6$ cm and an internal radius of $a = 10$ cm. Because all of the collected gas is within 10 cm of a nearly isothermal shell, the gas temperature quickly equilibrates with that of the bath. After the collected gas equilibrates with the bath, the gas temperature is determined by comparatively simple measurements of the temperature of the recirculating water. Remarkably, the water temperature measurements made with 14 sensors had a standard deviation of only 0.4 mK during a typical, 20-minute-long, equilibration interval. In the next section, we describe the bath; in the section after that, we discuss the equilibration of the collected gas.

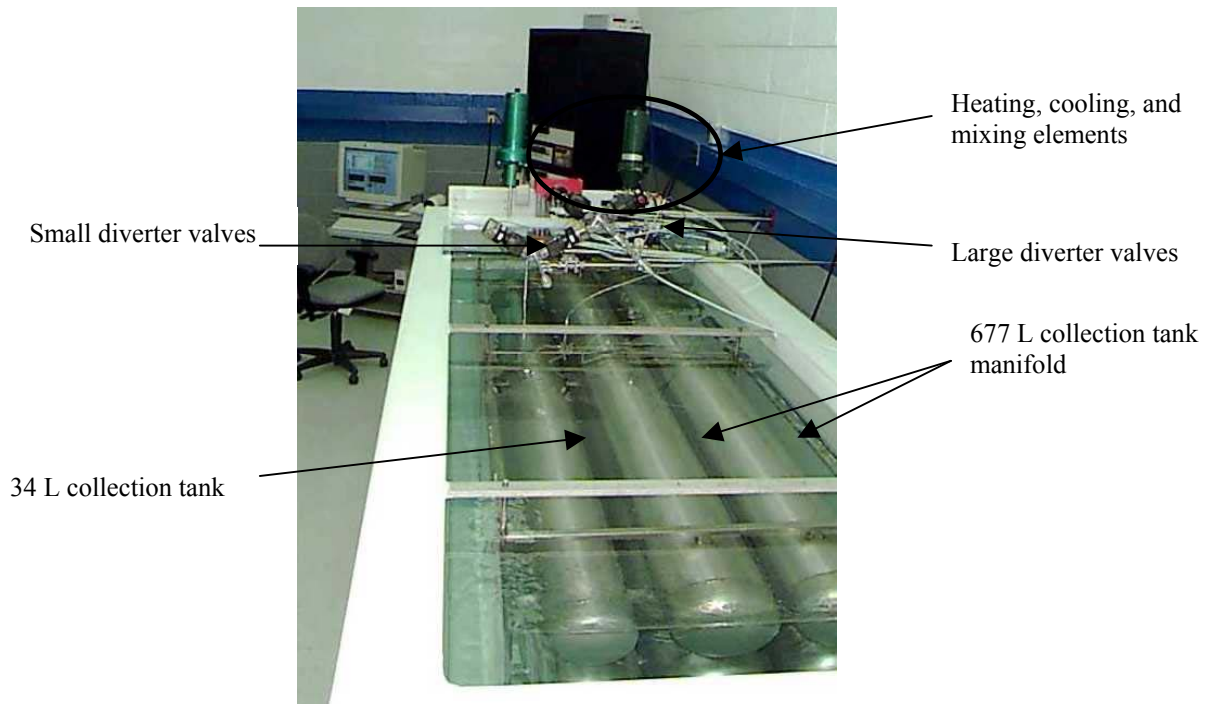


Figure 3. A photograph of the two *PVTt* collection tanks submerged in the temperature controlled water bath.

5.1.1 The Water Bath

The water bath is a rectangular trough 3.3 m long, 1 m wide, and 1 m high. Metal frames immersed in the tank support all the cylindrical shells and a long duct formed by four polycarbonate sheets. The duct surrounds the top, bottom, and sides of the shells: however, both ends of the duct are unobstructed. At the upstream end of the bath, the water is vigorously stirred and its temperature is controlled near the temperature of the room (296.5 K) using controlled electrical heaters and tubing cooled by externally refrigerated, circulated water. A propeller pushes the vigorously stirred water through the duct along the collection tanks. When the flowing water reaches the downstream (unstirred) end of the trough, it flows to the outsides of the duct and returns to the stirred

volume through the unobstructed, 10 cm thick, water-filled spaces between the duct and the sides, the top, and the bottom of the rectangular tank.

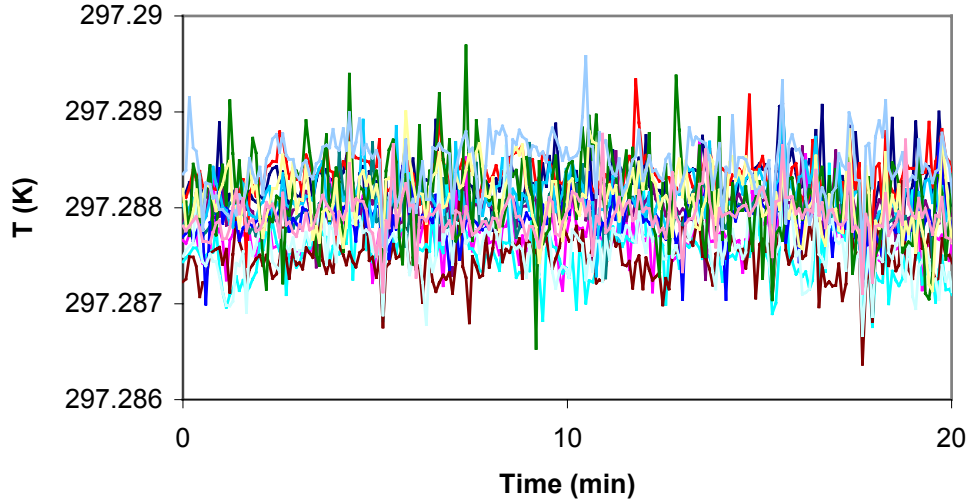


Figure 4. Temperature data for 14 thermistors distributed in the water bath.

The uniformity and stability of the water temperature was studied using 14 thermistors. The thermistors were bundled together and zeroed at one location in the water bath. Then, they were distributed throughout the water bath. Figure 4 plots data recorded at 5 s intervals from these 14 thermistors. Nearly all of the data in Fig. 4 is within ± 1 mK of their mean and the standard deviation of the data from their mean is only 0.4 mK. The largest temperature transients occur where the mixed water enters the duct, indicating incomplete mixing. The tank walls attenuate these thermal transients before reaching the collected gas. Thus, after equilibration, the non-uniformity of the water bath and the fluctuations of the average gas temperature are less than ± 1 mK ($3 \times 10^{-6} T$).

5.1.2 Equilibration of the Collected Gas

For design purposes, we estimated the time constant (τ_{gas}) that characterizes the equilibration of the gas within the collection tank after the filling process. The estimate considers heat conduction in an infinitely long, isotropic, “solid” cylinder of radius a [Carslaw and Jaeger 1946]. For the slowest, radially symmetric heat mode,

$\tau_{gas} = (a/2.405)^2/D_T$, where D_T is the thermal diffusivity of the gas. This estimate gives $\tau_{gas} = 80$ s for nitrogen in the 677 L tank. This estimate for τ_{gas} is too large insofar as it neglects convection, conduction through the ends of the tanks, and the faster thermal modes, all of which hasten equilibration. The time constants for heat to flow from the gas through the tank walls and the time constant for a hot or cold spot within a wall to decay have been calculated and found to be less than a second. Therefore, we expect the collected gas to equilibrate with a time constant of 80 s or less.

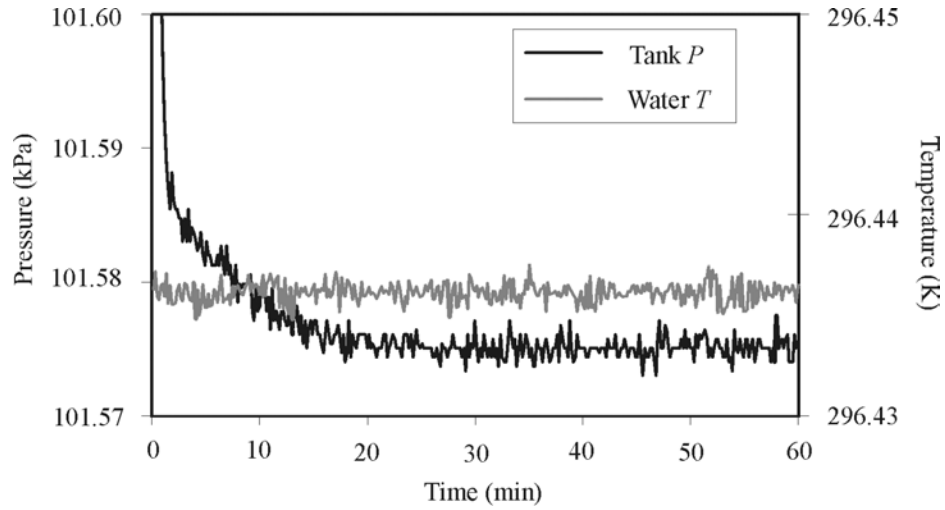


Figure 5. The equilibration of pressure and temperature immediately following a filling of the 34 L tank at 25 L/min.

The equilibration of the collected gas was observed by using the tank as a constant-volume gas thermometer. After the tank valve was closed, the pressure of the collected gas was monitored, as shown in Fig. 5. Our analysis of data such as those in Fig. 5 leads to the experimental values τ_{gas} of less than 60 s for both the 677 L and 34 L tanks, in reasonable agreement with the estimates. The measured time constant and Fig. 5 show that a wait of 20 minutes guarantees that the collected gas is in equilibrium with the bath, within the resolution of the measurements.

The manifold linking the 8 cylindrical shells is completely immersed in the water bath. Thus, the gas in the manifold quickly equilibrates to the bath temperature as well. However, each collection system has small, unthermostatted, gas filled volumes in the tubes that lead from the collection tanks to the diverter valves, the pressure transducers, etc. In Section 6.4.1, we show the possible temperature variations of these small, unthermostatted volumes make very small contributions to the uncertainty of the gas temperature and the flow measurements.

5.2 Mass Change in the Inventory Volume

5.2.1 Overview and Strategy

As outlined in Section 4, the start time t^i and the stop time t^f used in Eqs. 1 and 2 are chosen to occur during the brief “dead-end times” (< 100 ms) when both the tank valve and the bypass valve are closed, i.e., we use a “zero overlap” diversion [Harris and Johnson 1990]. This choice has the advantage of clear mass balance accountability for all the gas flowing through the critical flow venturi during both diversions and the tank filling. Unfortunately, it is difficult to determine either m_I^f or m_I^i and hence the change in mass within the inventory volume accurately (especially at high flows) because both the pressure and the temperature in the inventory volume rise rapidly as the flow through the critical venturi accumulates in the inventory volume (see Fig. 6).

Our strategy for dealing with the inventory mass change has two elements. First, by design, the inventory volume V_I is much smaller than the collection tank volume V_T . (For the 34 L system, $V_T/V_I = 500$; for the 677 L system, $V_T/V_I = 700$.) Thus, the uncertainty of mass flow is relatively insensitive to uncertainty in m_I^f and m_I^i since both are small compared with the total mass of collected gas. Second, we choose t^i near the end of the dead-end time and we chose t^f such that $P(t^i) = P(t^f)$. These choices define a “mass cancellation” method: since the initial and final inventory densities are essentially equal, Δm_I is nearly zero. In fact, we will assume that Δm_I is zero and consider the quantity only in terms of flow measurement uncertainty, not as part of the flow calculation. Symmetry

of the inventory transients (see Fig. 7) and the mass cancellation method also give uncertainty benefits due to high correlation in the uncertainties of pressure and temperature measurements for Δm_I .

We tested our strategy for choosing t^i and t^f for both the 34 L and the 677 L flow standards. (See Section 7 for details of these tests.) To test the 34 L system, we collected identical flows spanning the range $3 \text{ L/min} < \dot{m} < 100 \text{ L/min}$ in both the small and the large tanks, using the large tank as a reference for the small tank since its inventory uncertainties are quite small in this flow range. To test the 677 L collection system, we collected identical flows in the 677 L tank following two different protocols. In the first protocol, the inventory volume was dead-ended at the beginning and end of the collection interval in the usual manner. In the second protocol the collection interval was divided into two subintervals, which doubled Δm_I and allowed assessment of its uncertainty contribution.

These tests indicate uncertainties due to the inventory volume that are proportional to flow as would be expected based on a thermodynamic model of the inventory pressure and temperature transients. If the inventory uncertainties are considered to arise from uncertainty in the collection time, the inventory mass change uncertainty found experimentally for the 34 L system was $u_{\Delta m_I} = 4 \text{ ms} \times \dot{m}$ ($200 \times 10^{-6} \dot{m}$ for its maximum flow). For the 677 L system, single and double diversions changed the flow measurement by $75 \times 10^{-6} \dot{m}$ or less.

In the remainder of this section, we describe conditions within the inventory volume during the dead-end times using both a model and measurements. The measurements show that $T(t)$ and $P(t)$ are nearly the same during the start and stop dead-end times. Finally, we show that Δm_I is insensitive to the exact choice of t^i , provided that the condition $P(t^i) = P(t^f)$ is applied near the end of the dead-end time.

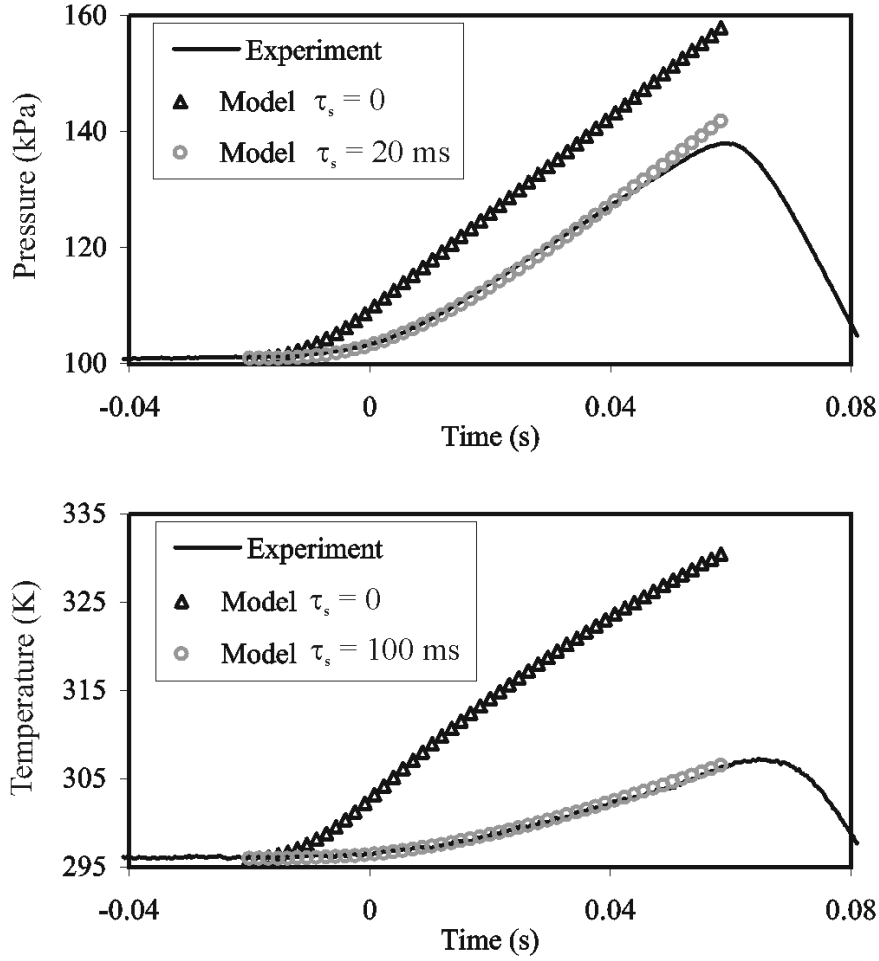


Figure 6. Experimentally measured data (25 L/min in the 34 L tank) and thermodynamic model predictions for zero and non-zero sensor time constants. The model outputs demonstrate that neglect of sensor response causes significant error in the measurement of inventory conditions.

5.2.2 Conditions within the Inventory Volume

Figure 6 displays the time dependent temperature $T(t)$ and pressure $P(t)$ in the inventory volume of the smaller collection system at a typical collection rate ($\dot{m} = 25$ L/min; collection time = 82 s). The time $t = 0$ in Fig. 6 is defined by the signal indicating that the valve is fully closed. The triangles ($\tau = 0$) in Fig. 6 were calculated from the lumped-parameter, thermodynamic model developed by Wright and Johnson [2000]. The model assumes a constant mass flow \dot{m} at the entrance to the inventory volume. The model

neglects heat transport from the gas to the surrounding structure and non-uniform conditions, such as the jet entering the volume. For Fig. 6, $T(t)$ and $P(t)$ were calculated on the assumption that the diverter valve reduced the flow linearly (in time) to zero during the interval $-0.02 \text{ s} < t < 0$. Experimentally measured values of $T(t)$ and $P(t)$ recorded at 3000 Hz (smooth curves) are also shown in Fig. 6. Most of the differences between the measured curve and the ($\tau = 0$) calculated triangles result from the time constants of the sensors used to measure $T(t)$ and $P(t)$. This is demonstrated by the agreement between the experimental curve and the model results when time constants are incorporated (circles).

In Fig. 6, the calculated curves do not display features that mark either the onset or the completion of the diverter valve closing. Thus, even $T(t)$ and $P(t)$ data from perfect sensors cannot be used to mark these events. For this reason, the times t^i and t^f were chosen at times that were clearly within the dead-end time intervals.

Figure 6 shows that the measured values of $T(t)$ and $P(t)$ are consistent with the Wright-Johnson model for the inventory volume after allowance is made for the response times of the sensors. The consistency shows that the behavior of the inventory volume is understood semi-quantitatively. However, this is not sufficient to accurately calculate the density $\rho(t)$ from measurements of $T(t)$ and $P(t)$ because the fraction of the flow collected as the valves are closing cannot be deduced from the measurements. Instead, we relied on the pressure sensor to choose t^i . The pressure sensor is preferred to the temperature sensor because it responds more quickly and also because it responds to the average conditions throughout the inventory volume rather than the conditions at only one location. We choose t^i near the end of the dead-end time, where the $P(t)$ measurements are nearly parallel to the $\tau = 0$ model. In this regime, the derivative dP/dt is large and its dependence on precisely how the valve closed is small. Because the dependence on how the valve closed has decayed, we expect that $P(t)$ will be the same during the start and the stop dead-end times, improving the mass cancellation as well as the correlation of initial and final inventory density uncertainties.

5.2.3 Near Symmetry of Start and Stop Behavior of $P(t)$

Figure 7 shows records of $T(t)$ and $P(t)$ taken during the dead-end time intervals at the start and the stop of a single flow measurement. As before, the data were recorded at 3000 Hz for 500 ms and the plots were displaced along the horizontal axis until they nearly overlapped. The pressure and the temperature at the beginning of the start dead-end time were slightly lower than those at the stop dead end time; however, the two records match closely during the dead-end time. This implies that the time-dependent densities $\rho(t)$ also nearly match.

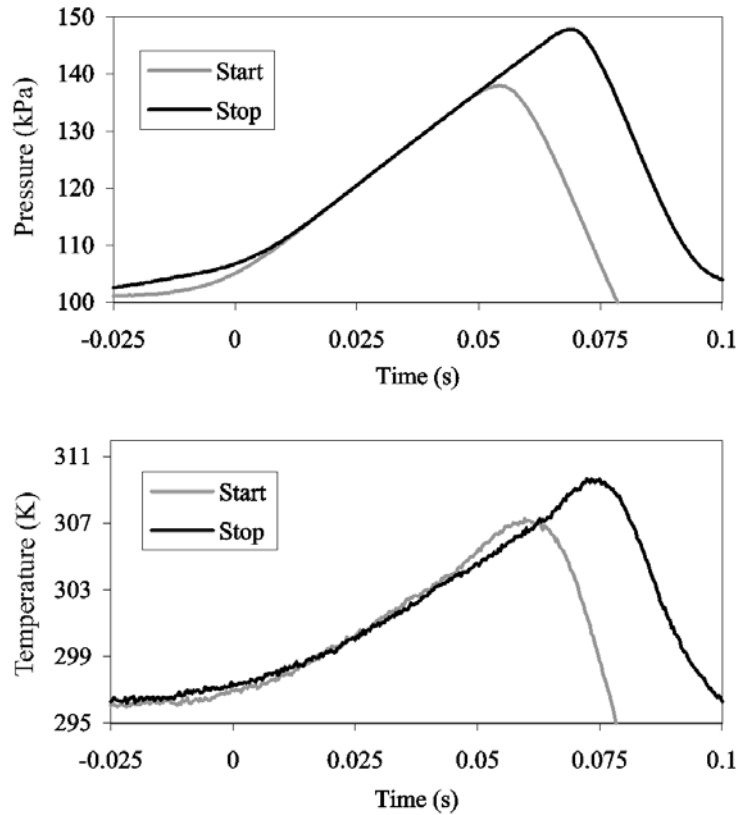


Figure 7. Superimposed inventory data traces for a start diversion and a stop diversion in the 34 L tank at 25 L/min demonstrating “symmetric” diverter valve behavior. The stop dead-end time was approximately 15 ms longer.

At both diversions shown in Fig. 7, valve trigger signals were gathered along with the temperature and pressure measurements using a commercially manufactured data

acquisition card (see Fig. 8). The trigger signals originate from an LED/photodiode pair and a flag on the valve actuator positioned so that the circuit output rises to a positive voltage when the valve is closed. These valve signals are used to trigger timers that give the approximate collection time.

As represented in Fig. 8, the inventory record is post-processed by the controlling program to obtain both the initial and final measurements of pressure and temperature in the inventory volume as well as the final collection time. A “match pressure” $P(t^i)$ is chosen that falls late within the start dead-end interval. The stop time is then found in the stop dead-end interval by choosing $P(t^f) = P(t^i)$. Time corrections between the match pressure measurement and the start and stop trigger signals (Δt^i and Δt^f) are determined from the data record. The appropriate time corrections are added to the approximate collection time from the timers. Thus, by adjusting the collection time using the inventory data records, the initial and final inventory pressures and temperatures are nearly matched, leading to nearly equal initial and final inventory densities and inventory mass cancellation.

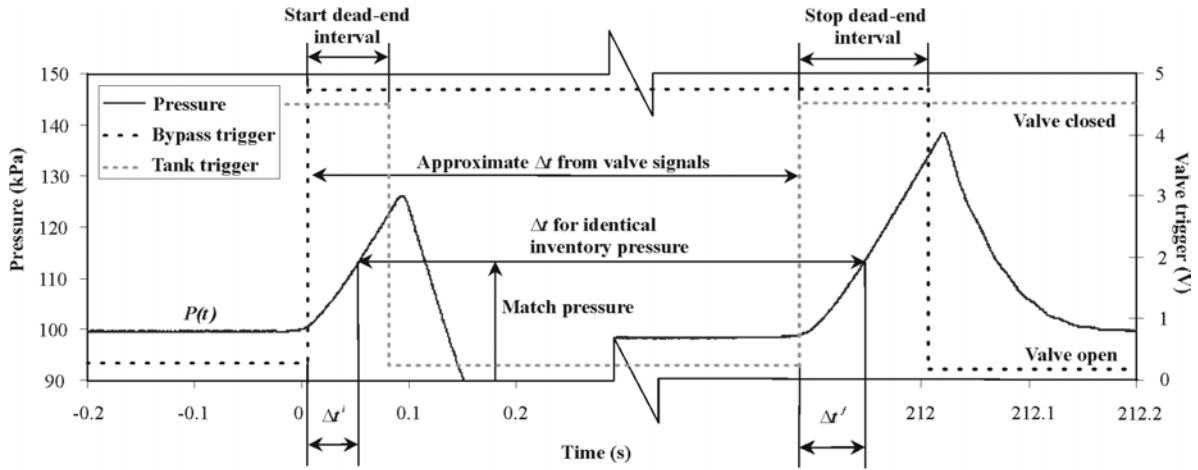


Figure 8. Data records of inventory sensors and valve trigger signals are used to adjust the collection time and improve cancellation of the initial and final inventory mass as well as inventory uncertainties.

5.2.4 Insensitivity of Δm_I to the Match Pressure

Figure 9 shows the total correction time as a function of the match pressure for two flows in the 34 L system. The 100 L/min flow is very high for the 34 L tank, having only an 18 s collection time. Match pressure is shown as a percentage of the range of pressures measured during the diversion transient. For a perfectly fast system (valves and sensors), these plots would be horizontal lines, i.e. any chosen match pressure would result in the same time correction. However, for the real system with its inevitable limitations, the match pressure does matter. Exploring the possible reasons for this is valuable for improving the system and for obtaining an accurate uncertainty analysis.

First recall that the inventory sensors have non-zero time constants and therefore the measurements they provide are damped versions of the real conditions and further, the values they report at any given instant are subject to the recent history of the pressure or temperature value. Second, realize that perfect symmetry of conditions before and during diversion is unobtainable and that these imperfections and the significance of the sensor damping increase with the flow. For example, at high flows, the rate of change of pressure during the tank filling process is large and it becomes more difficult to make the pressure at which the stop diversion begins closely match the pressure at which the start diversion began (due to sensor response and valve control delays). This “trigger pressure difference” will be considered again in Section 7. As another example, the bypass and tank valves may not close at the same speed.

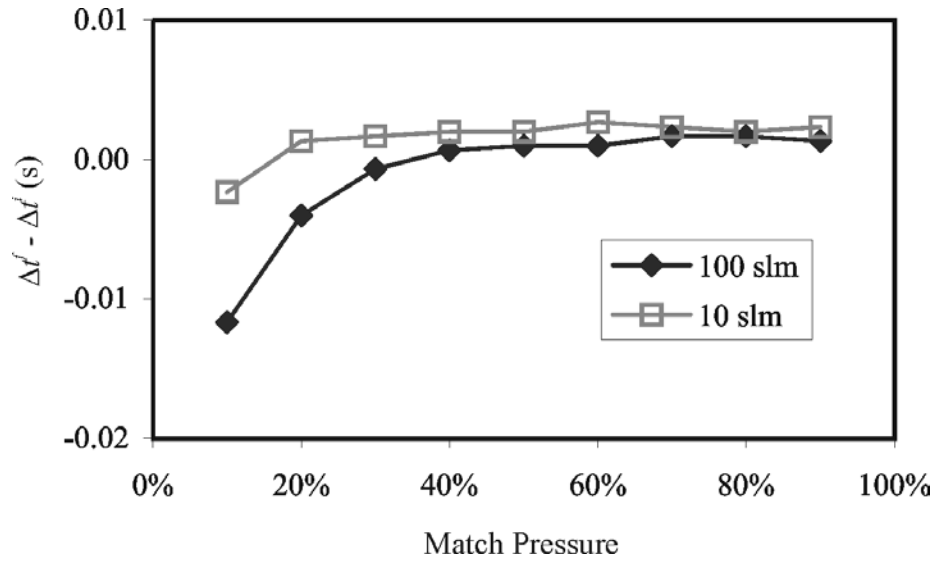


Figure 9. The collection time correction versus the match pressure used in the inventory mass cancellation algorithm.

Analysis of the thermodynamic model of the inventory and its sensors shows that times later in the dead-end time give better mass cancellation under these circumstances since the sensor output enters a period with nearly constant slope that is equal to the real pressure slope. The experimental results given in Fig. 9 support this assertion: match pressures between 50 % and 90 % result in nearly constant correction times, while low match pressures (early in the dead-end time) give much larger corrections. Based on this analysis, a match pressure of 80 % has been selected for use in the flow standard. Figure 9 demonstrates the insensitivity of Δm_I to a wide range of match pressure values.

Figure 9 also illustrates the concept that uncertainties related to the inventory volume can be treated not only as mass measurement uncertainties, but as time measurement uncertainties as well. One can consider the uncertainty in the measurement of time between conditions of perfect mass cancellation, or one can consider the uncertainty in the measurement of inventory mass differences between the start and stop times. Both perspectives offer insight and verification of the uncertainties of the inventory volume and flow diversion process.

5.3 Measurement of the Tank and Inventory Volumes

5.3.1 Gas Gravimetric Method

The volume of the 677 L tank was determined by the gas gravimetric method. In this method, the mass of an aluminum high pressure cylinder was measured before and after discharging its gas into the evacuated collection tank. The change in mass of the high-pressure cylinder and the change in density of the gas in the collection tank were used to calculate the collection tank volume. Nominally,

$$V_{grav} = \frac{m_c^i - m_c^f}{\rho_T^f - \rho_T^i} - V_{extra} , \quad (3)$$

where the m_c indicates the mass of the high-pressure cylinder and V_{extra} represents the extra volume temporarily connected to the tank for the purpose of introducing the gas from the cylinder to the tank (usually a small volume of tubing and a valve body). The extra volume is calculated from dimensional measurements or measured by liquid volume transfer methods.

In practice, a more complex formula than Eq. 3 was used to account for a small amount of gas that enters the control volume from the room when the cylinder is disconnected from the collection tank since the final tank pressure was less than atmospheric. For the volume determinations performed for the 677 L tank, the effect amounts to only $5 \times 10^{-6} V_T$.

The volume determination was conducted with both nitrogen and argon gas. In both cases high purity gas was used (99.999 %) and care was taken to evacuate and purge the system to minimize composition uncertainties. When nitrogen was used, the aluminum cylinder weighed approximately 4200 g when filled at 12.5 MPa, and approximately 3800 g after it was emptied to 55 kPa. When argon was used, the initial and final masses were 4440 g

and 3820 g respectively. The standard deviation of the six volume measurements (4 with nitrogen, 2 with argon) was $16 \times 10^{-6} V_T$.

The initial and final masses of the gas cylinder were measured using a substitution process with reference masses and a mass comparator enclosed in a wind screening box. The comparator has a full scale of 10 kg and a resolution of 1 mg. The cylinder and a set of reference masses of nearly the same weight were alternated on the scale 5 times. The zero corrected scale readings were then calibrated to the reference masses and buoyancy corrected via the following formula:

$$m_c = \frac{S_c}{S_{ref}} m_{ref} \left(1 - \frac{\rho_{air}}{\rho_{ref}} \right) + \rho_{air} V_{ext} , \quad (4)$$

where S represents the scale reading, ref indicates the reference masses, ρ_{air} is the ambient air density where the measurements were conducted, and V_{ext} is the external volume of the high pressure cylinder and its valve and fittings. The density of the ambient air was calculated from the barometric pressure, the temperature and humidity inside the wind screen, and an air density formula that includes humidity [Jaeger and Davis 1984].

The external volume of the high-pressure cylinder appears in Eq. 4 due to air buoyancy corrections. The external volume of the cylinder was measured by Archimedes principle, i.e. by measuring the change in apparent mass of the object in two media with differing and known densities. One of the media was distilled water, and the cylinder apparent mass in the water was measured as follows. Liquid was added to the cylinder interior until it was nearly neutrally buoyant in the tank of distilled water. The addition of liquid inside the cylinder has no effect on its external volume. The temperature of the distilled water was raised or lowered (thereby changing the density of the distilled water) until the cylinder was essentially neutrally buoyant. At this point, the apparent mass in the distilled water is zero. The temperature of the distilled water was recorded and its density was calculated via an equation from the literature [Patterson and Morris 1994]. Hence, the temperature of the distilled water was used in place of a weigh scale to measure the

apparent mass in water. The apparent mass of the cylinder in air (with the liquid still inside) was measured using the comparator described above. The density of air with humidity was calculated as previously described. The external volume of the cylinder was calculated for the nominal room temperature (T_{ref}) of 296.5 K with the following formula:

$$V_{ext}(T_{ref}) = \frac{m_{air}^A - m_{water}^A}{\rho_{water} [1 + 3\alpha(T_{water} - T_{ref})] - \rho_{air} [1 + 3\alpha(T_{air} - T_{ref})]}, \quad (5)$$

where the superscript A indicates apparent mass and α is the coefficient of linear thermal expansion for the aluminum tank. The terms containing α correct for changes in the cylinder volume due to differences between the water temperature, the air temperature, and the reference temperature. However, for this particular case, these thermal expansion issues could have been neglected since both the water temperature and air temperature never differed from T_{ref} by more than 1.5 K. The thermal expansion corrections to the external volume were less than 0.5 cm^3 or $100 \times 10^{-6} V_{ext}$ and the external volume has a small sensitivity coefficient in the collection tank volume determination process.

The expansion of the external cylinder volume as a function of its internal pressure was not negligible. The Archimedes principle measurements showed a volume increase from 4697.5 cm^3 to 4709 cm^3 between the 100 kPa and 12.5 Mpa pressures. This change agreed well with predictions based on material properties, and the appropriate experimental values for external volume were used in the cylinder mass calculations (Eq. 4), depending on whether the cylinder was empty or full. If this issue were neglected, it would lead to relative errors in the mass change measurements of about 35×10^{-6} .

5.3.2 Volume Expansion Method

The 34 L collection tank volume, the inventory volume for the large collection tank, and the small inventory volume were all determined with a volume expansion method. In this method, a known volume is pressurized, the unknown volume is evacuated, a valve is opened between the two volumes, and the density changes within the two volumes are used to calculate the unknown volume. Applying conservation of mass to the system of the two tanks yields:

$$V_2 = \frac{(\rho_1^f - \rho_1^i)V_1}{(\rho_2^i - \rho_2^f)} - V_{extra}, \quad (6)$$

where the subscripts 1 and 2 refer to the known and unknown volumes respectively. As before, the density values are based on pressure and temperature measurements of the gas within the volumes and gas purity issues must be considered. Note that in many cases the final densities can be considered the same in both volumes 1 and 2, but for the determination of the 34 L tank volume, elevation differences between the two tanks required a head correction to the pressure measurements and therefore the two densities were not strictly equal. The difference in elevation resulted in a relative difference in gas density of 20×10^{-6} even though the two tanks were connected.

6 Uncertainty Analysis of the 34 L and 677 L *PVTt* Flow Standards

In this section, we will analyze the uncertainty of the 34 L and 677 L *PVTt* standards. We will begin by giving an overview of the subject of uncertainty analysis including the issue of correlated uncertainties. Next we will give the results of the uncertainty analysis for mass flow. In following sections, we will give uncertainties of the sub-components that were combined to obtain the mass flow uncertainty. The largest source of uncertainty in the flow measurement is drift of the pressure sensor over time, which contributes a

relative standard uncertainty of 60×10^{-6} to the determinations of the volumes of the collection tanks and to the flow measurements.

6.1 Techniques for Uncertainty Analysis

The uncertainty of a mass flow measurement made with the *PVTt* standard use the propagation of uncertainties techniques described in the ISO Guide to the Expression of Uncertainty in Measurement [ISO 1996]. The process identifies the equations involved in the flow measurement so that the sensitivity of the final result to uncertainties in the input quantities can be evaluated. The uncertainty of each of the input quantities is determined, weighted by its sensitivity, and combined with the other uncertainty components to arrive at a combined uncertainty.

As described in the references [ISO 1996, Coleman and Steele 1999], consider a process that has an output, y , based on N input quantities, x_i . For the generic basis equation:

$$y = y(x_1, x_2, \dots, x_N), \quad (7)$$

if all the uncertainty components are uncorrelated, the standard uncertainties are combined by root-sum-square (RSS):

$$u_c(y) = \sqrt{\sum_{i=1}^N \left(\frac{\partial y}{\partial x_i} \right)^2 u^2(x_i)}, \quad (8)$$

where $u(x_i)$ is the standard uncertainty for each of the inputs, and $u_c(y)$ is the combined standard uncertainty of the measurand. The partial derivatives in Eq. 8 represent the sensitivity of the measurand to the uncertainty of each input quantity.

In cases where correlated uncertainties are significant (as in the following analysis), the following expression should be used instead of Eq. 8:

$$u_c(y) = \sqrt{\sum_{i=1}^N \left(\frac{\partial y}{\partial x_i} \right)^2 u^2(x_i) + 2 \sum_{i=1}^{N-1} \sum_{j=i+1}^N \frac{\partial y}{\partial x_i} \frac{\partial y}{\partial x_j} u(x_i) u(x_j) r(x_i, x_j)} \quad , \quad (9)$$

where $r(x_i, x_j)$ is the correlation coefficient, ranging from -1 to 1 , and equaling zero if the two components are uncorrelated. As will be seen in the following analysis, some uncertainty components in the present system are correlated and this leads to a significant improvement in the uncertainty of the measurand.

A simple example of a correlated uncertainty is illustrative. Suppose that a thermometer was used to measure a temperature difference. Also suppose that the only uncertainty in the thermometer measurement was an unknown offset in its calibration. When the difference between two temperatures was calculated from measurements made with this thermometer, the offset would cancel and would not contribute to the uncertainty of the temperature difference. In this case, the subtraction process used to calculate the difference leads to sensitivity coefficients of opposite sign for the two temperature measurements. Since the sensor always has the same offset, the uncertainties are perfectly correlated ($r(x_i, x_j) = 1$). When this hypothetical scenario is processed through Eq. 9, the uncertainty of the temperature difference is zero. Of course in a real case, there would be other, uncorrelated uncertainties that would make the uncertainty of the temperature difference non-zero. Nonetheless, the example demonstrates that under certain circumstances, correlated uncertainties will reduce the uncertainty of a measured quantity.

In the following uncertainty analysis, correlated and uncorrelated uncertainties will be treated as separate components, even if they are related to the same physical quantity. For instance, there will be a correlated as well as an uncorrelated inventory pressure component. In this manner, the correlated components can be considered as having a correlation coefficient of 1, while uncorrelated components have correlation coefficients of 0. This approach simplifies the process to deciding which uncertainty sources are correlated versus uncorrelated and checking that the assumption of perfect correlation is reasonable.

Most of the equations utilized to calculate flow, mass, volume, and other necessary intermediate quantities for the *PVTt* standard have been discussed in prior sections. In Fig. 10 the information is summarized in a diagram that shows the measurement chain used to calculate flow. At the top of the diagram is the output, mass flow. At the second level are the inputs to Eq. 2, the quantities needed to calculate mass flow: density, volumes, and collection time. To calculate density, the inputs to the equation of state are necessary: pressure, temperature, compressibility, the universal gas constant, and molecular weight. The other necessary quantities and their basis equations are shown as well. Figure 10 will serve as a guide for the *PVTt* uncertainty analysis.

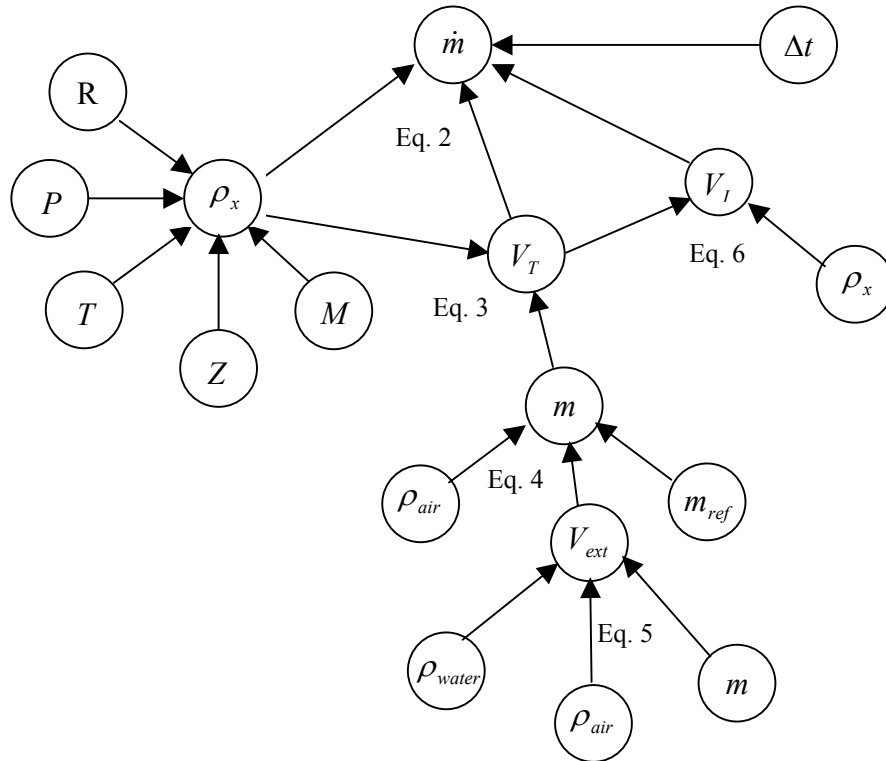


Figure 10. The chain of measurements and equations used for the *PVTt* flow standard.

The discharge coefficient resulting from a flowmeter calibration will have additional uncertainties not considered herein due to measurements associated with the meter under test. For instance, if the meter under test is a critical flow venturi, uncertainties related to the temperature and pressure measurements at the meter must be included in the uncertainty of the discharge coefficient.

The uncertainties tabulated herein are $k = 1$, standard, or 68 % confidence level uncertainties. At the conclusion of the uncertainty analysis, a coverage factor of 2 will be applied to give an expanded uncertainty for mass flow measurements with an approximate 95 % confidence level. In the remainder of this section, we will give the uncertainty of mass flow for both the 34 L and 677 L *PVTt* systems, and then the uncertainty components that contribute to the *PVTt* mass flow measurement will be traced to their fundamental sources.

6.2 Mass Flow Uncertainty

Table 2. Uncertainty of nitrogen flow measurement with the 677 L standard.

<i>Uncertainty Category</i>	Standard Uncertainty ($k = 1$)		Contrib	Comments
<i>Flow (677 L, N₂)</i>	Relative ($\times 10^6$)		(%)	
Tank volume	71	48.44 cm ³	50 to 23	see Table 15
Tank initial density	10	2.27×10^{-12} g/cm ³	1 to 0	
Tank final density	68	7.77×10^{-8} g/cm ³	45 to 21	see Table 9
Inventory mass change	0 to 109	0.084 g	0 to 53	see Table 21
Collection time	15	0.287 ms	0 to 1	see Table 11
Std deviation of repeated meas.	20	0.001 g/sec	4 to 2	
RSS (combined uncertainty)	102 to 150			
Expanded uncertainty ($k = 2$)	204 to 300			

The uncertainty for flows between 20 L/min and 2000 L/min of nitrogen or argon in the 677 L tank is given in Table 2. The standard uncertainty of each sub-component is given

in both relative ($\times 10^{-6}$) and dimensional forms. The units of the dimensional values are given in the third column. The relative contribution of each sub-component to the combined uncertainty is listed in the fourth column. This contribution is the percentage of the squared individual component relative to the sum of the squares of all sub-components. The uncertainty from the inventory volume, the combined uncertainty, the expanded uncertainty, and the uncertainty contributions are given as a range covering the minimum to maximum flow. To calculate their relative uncertainty in Table 2, the tank initial density was normalized by the tank final density and the inventory mass change was normalized by the total mass collected.

At the highest flow, uncertainty contributions are principally divided between the tank volume, the final gas density, and the inventory uncertainty. The $k = 2$ uncertainty falls to $204 \times 10^{-6} \dot{m}$ for the smallest flows as the uncertainty contributions of the inventory volume become negligible. For an air flow measurement, the uncertainty of the 677 L system is less than $500 \times 10^{-6} \dot{m}$ over the entire flow range and the uncertainty is driven by the tank final density measurement (80 % contributor).

Table 3. Uncertainty of nitrogen flow measurement with the 34 L standard.

<i>Uncertainty Category</i>	Standard Uncertainty ($k = 1$)		Contrib (%)	Comments
	Relative ($\times 10^6$)			
Flow (34 L, N₂)				
Tank volume	116	3.955 cm ³	72 to 28	see Table 16
Tank initial density	10	2.27×10^{-12} g/cm ³	1 to 0	
Tank final density	68	7.77×10^{-8} g/cm ³	25 to 10	see Table 9
Inventory mass change	0 to 170	0.007 g	0 to 61	see Table 22
Collection time	15	0.287 ms	0 to 0	see Table 11
Std deviation of repeated meas.	20	4×10^{-5} g/sec	2 to 1	
RSS (combined uncertainty)	137 to 219			
Expanded uncertainty ($k = 2$)	274 to 438			

Table 3 presents the uncertainty of flow measurements from the 34 L system for flows between 1 L/min and 100 L/min. The expanded uncertainty varies between $270 \times 10^{-6} \dot{m}$ and $440 \times 10^{-6} \dot{m}$. At high flows, the significant uncertainty sources are the tank volume, the tank final density, and the uncorrelated inventory uncertainties. For low flows, the major contributors are tank volume and final gas density. For air flow measurements, the 34 L system has a nearly constant uncertainty over its entire flow range of about $500 \times 10^{-6} \dot{m}$ and it is driven by the uncertainty of the final gas density.

6.3 Pressure

A Ruska Model 2465-754 gas lubricated piston pressure gauge is used as the primary pressure standard to calibrate pressure transducers within the Fluid Flow Group. The uncertainties in a single pressure measurement made with this device are listed in Table 4. Uncertainties in the pressure standard can be traced to the effective area of the piston, piston thermal expansion, the masses, local gravity, and the measurement of the pressure under the bell jar covering the piston and masses (necessary for absolute pressure measurements). The uncertainty shown in Table 4 is for a pressure value of 100 kPa. No buoyancy corrections are made to the masses since the reference pressure, and hence the density under the bell, are small enough that the buoyancy corrections (and uncertainties) are negligible ($\ll 1 \times 10^{-6} P$). The uncertainty of the piston pressure gauge is $17 \times 10^{-6} P$ at 100 kPa.

Table 4. Uncertainties for a 100 kPa pressure measurement made with the piston pressure gage used as the standard for pressure calibrations.

Uncertainty Category	Standard Uncertainty ($k = 1$)		Contrib	Comments
	Relative ($\times 10^6$)	(kPa)		
<i>Piston Pressure Gage</i>				
<i>Pressure value</i>		100		
piston effective area	12	0.0012	59	from NIST Pressure and Vacuum Group cal.
thermal expansion	6	0.0006	15	assume T unc of 0.2K
masses	1	0.0001	0	Mass Group calibration
local gravity	0.2	0.00002	0	9.801011+/- 0.000002
air density for buoyancy	0	0	0	neg. air density relative to mass density
ref. P for absolute	10	0.001	41	based on calibration data of the vac gauge
RSS	17	0.0017		

6.3.1 Collection Tank Pressure

Measurements of the collection tank initial pressure are made with a pair of thermocouple vacuum gauges (Varian Convectorr P-type) that have been calibrated by comparison to a reference standard in the NIST Pressure and Vacuum Group. The manufacturer's uncertainty specification for this gauge is 10 % of reading. Based on the NIST calibration results, the consistent agreement between the redundant sensors, and the repeatable readings of the gauges at the vacuum pump ultimate pressure, a standard uncertainty of 5 % of reading will be used. As will be seen when the components are combined to give the flow measurement uncertainty, this large value has little impact due to the low initial pressure in the collection tank (20 Pa).

Pressure measurements of the full collection tank are made with a Paroscientific Model 740 with a full scale of 200 kPa. The manufacturer's uncertainty specification for this transducer is 0.01 % of full scale, but under the conditions of the present usage, the uncertainty is less. The uncertainties in the collection tank pressure measurement are

listed in Table 5. They include the uncertainties from the piston pressure gage, the long term drift of the Paroscientific transducer which has been quantified by periodic recalibrations, as well as the residuals from the best fit calibration equation (including hysteresis), and thermal effects. Uncertainties due to spatial non-uniformity of pressure within the tank and time response of the sensor are negligible since the calibration procedure is to wait as much as 20 minutes for equilibration before the measurements are made.

Figure 11 is a control chart that shows the changes in pressure calibration versus time at a pressure of 100 kPa for one of the pressure transducers used to measure collection tank pressure. Also shown are the $k = 1$ uncertainty tolerance bounds ($64 \times 10^{-6} P$ from Table 5) and error bars that represent the $k = 1$ uncertainty of the piston pressure gage used to calibrate the sensor ($17 \times 10^{-6} P$ from Table 4).

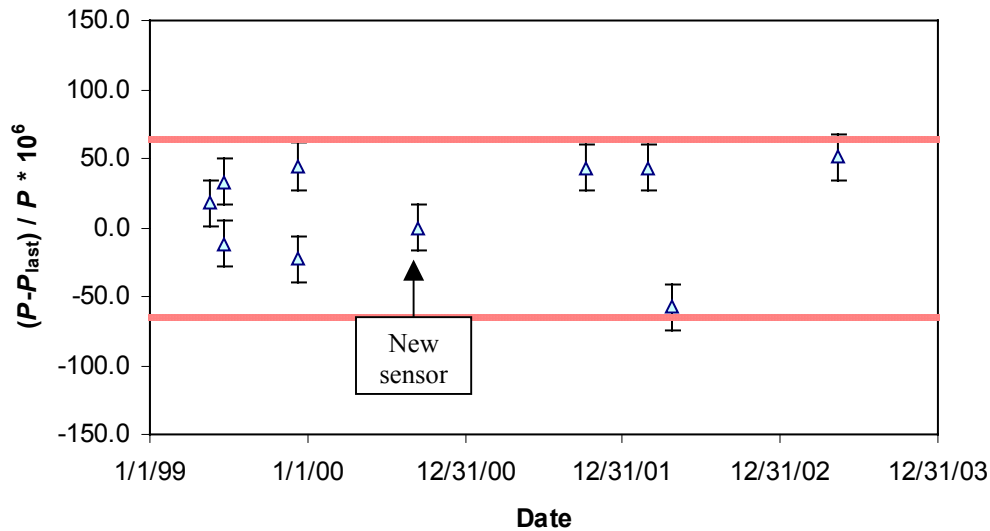


Figure 11. A calibration control chart for a 200 kPa pressure transducer used to measure the collection tank pressure.

Temperature effects as large as $40 \times 10^{-6} P$ have been observed in the tank pressure sensor, and care was taken to minimize their influence. When the tank is quickly filled from a pressurized cylinder during the volume determination process, cold gas enters the sensor, cooling it. The pressure readings asymptotically approach a final value as the

sensor returns to room temperature (with a time constant of approximately 1 hr). The temperature dependence of the sensor was confirmed by testing with an environmental chamber. Temperature effects also result in a hysteresis loop for the sensor calibration data that enlarges the calibration fit residuals. The calibration process entails increasing and decreasing the pressure in steps. The pressure steps result in heating and cooling of the pressure sensing elements and a hysteresis loop. Therefore the residuals of the pressure calibration fit include contributions due to thermal effects. We noticed that the thermal effects due to pressure changes in the transducers can be larger than the values given in Table 5. During volume determinations, we allowed sufficient time for the sensor to return to room temperature so that the remaining temperature effects were much smaller than the allowance for calibration drift.

Table 5. Uncertainties in the collection tank pressure measurement at 100 kPa.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib (%)	Comments
	Relative ($\times 10^6$)	(kPa)		
<i>Pressure Measurement</i>				
<i>Pressure value</i>		100		
piston pressure gage	17	0.0017	7	from Table 4
drift	60	0.0060	88	< 0.01 % in 6 mos, assume rect.
residuals, hysteresis, thermal effects	14	0.0014	5	from cal. records, experiments
RSS	64	0.0064		

6.4 Temperature

The temperature sensors used in the flow standard are traceable to the NIST Thermometry Group through calibrations made with a four-wire thermister transfer standard (Thermometrics Model TS8901) and a recirculating water constant temperature bath. The uncertainty of the transfer standard thermister is 1.2 mK (see Table 6). The drift of the transfer standard is considered negligible based on 7 annual calibrations that have always differed from each other by less than the calibration uncertainty.

Table 6. Uncertainties for the Fluid Flow Group temperature transfer standard.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib (%)	Comments
	Relative ($\times 10^6$)	(mK)		
<i>Temperature Transfer Standard</i>				
<i>Temperature value</i>		3×10^5		
Thermometry Group cal	4	1.2	94	unc. for 274 K to 368 K
fit residuals	1	0.3	6	some years, 1/6 this size
drift	0	0	0	less than discernable given cal unc.
radiation, self-heating, etc.	0	0	0	deeply immersed in water bath
RSS	4	1.2		

6.4.1 Collection Tank Temperature

The measurement of the temperature of the gas in the collection tank has additional uncertainties that are listed and quantified in Table 7. Temperature is measured with YSI Model 46000 thermistors in 3 mm diameter stainless steel sheaths, a Keithley model 224 current source, a Keithley model 7001 switch system, and a Keithley model 2002 multimeter. Uncertainty sources include the temperature transfer standard covered by Table 6, the uniformity and stability of the water bath used to calibrate the thermistors, and the residuals of the best-fit equation to the calibration data. The largest uncertainty component is the calibration drift between periodic calibrations. Radiation and stem conduction are negligible since the thermistors are immersed at least 15 cm in room temperature water. Tests were conducted to measure the significance of self-heating by varying the thermistor current while the sensor was held in a stable water bath and watching the resulting change in sensor reading. Based on this experiment, the current through the 5000 ohm thermistors was set to 10 μ A which leads to self-heating of less than 1 mK. The *PVTt* bath stability and uniformity (1 mK) were discussed earlier, as was the issue of thermal equilibrium between the water bath and the gas in the collection tank. The sensors are calibrated over their entire range of usage, so there is no uncertainty

related to extrapolation of their calibration data. Uncertainty related to the time response of the thermistors is negligible since the time constant for the sensor is on the order of 10 s and the wait for thermal equilibrium is 30 or more times longer.

Small portions of the gas collection tank are not immersed in the water bath. They include the tubing connecting the outlet of the diverter valve to the collection tank, the tubing that connects the tank to pressure and vacuum transducers, and the internal volume of these transducers. Because we assumed that the bath temperature represents the gas temperature, and the room temperature may differ from that of the bath, the small portion of the tank not immersed leads to a gas temperature uncertainty. The room temperature is maintained at $23.5 \pm 1^\circ\text{C}$. The fractional error in mass contained in the collection tank due to a 1 K difference between the room and the water bath is:

$$\frac{\delta m}{m} \approx \frac{V_{out}}{V_T} \frac{\delta T}{T}, \quad (10)$$

where V_{out} is the volume of the portion of the tank that is at room temperature and δT is the difference between the room and water bath temperatures. For the large tank, V_{out} is 200 cm^3 and the total tank volume is 677 L. For δT of 1 K, the relative mass uncertainty is 1×10^{-6} . This uncertainty will be treated as an uncertainty in the average gas temperature of $1 \times 10^{-6} T$ or 0.3 mK in the following analysis. For the small tank this temperature uncertainty is 1.2 mK or $4 \times 10^{-6} T$.

By RSS of the components listed in Table 7, the combined uncertainty for the average temperature of the gas in the collection tank is 7 mK when using the thermistors dedicated to the flow standard.

Table 7. Uncertainty of average gas temperature in the collection tank with the dedicated temperature sensors.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
	Relative ($\times 10^6$)	(mK)	(%)	
<i>Tank Gas Average Temperature</i>				
<i>Temperature value</i>		297000		
temperature transfer standard	4	1.2	4	from Table 7
cal. bath uniformity and stability	3	1	2	based on notes made during cal
fit residuals	7	2	9	
drift (I, R, DMM, thermistors)	20	5.8	77	YSI spec is <10mK/10 mo., assume rect.
radiation, stem cond., self-heating	3	1	2	expt. varied current, 5 mK, assume rect.
<i>PVTt</i> bath uniformity and stability	3	1	2	based on experimental measurements
diff. between water and room T's	4	1.2	3	see Eq. 10
extrapolation	0	0	0	cal covers whole operating range
sensor time constant	0	0	0	wait time is $>10 \times$ sensor time constant
RSS	22	7		

6.5 Compressibility, Molecular Weight, and Gas Constant

The remaining contributors to gas density uncertainty are the compressibility, the molecular weight, and the gas constant. Four gas cases will be considered. Tank volume determinations were conducted with ultra high purity nitrogen (99.999 %) and ultra high purity argon (99.999 %). During normal calibrations, industrial liquid nitrogen vaporized from dewars (99.998 %) and compressed, dried air are used.

6.5.1 Gas Constant

The universal gas constant is known with relative standard uncertainty better than 2×10^{-6} [Moldover et al. 1988].

6.5.2 Compressibility

The compressibility factor can be calculated from the following expression:

$$Z = 1 + B\rho_n + C\rho_n^2, \quad (11)$$

where ρ_n is the molar density (mol/ cm³) and B and C are the second and third virial coefficients respectively. For nitrogen, the virial coefficients can be calculated from the correlations:

$$B_{N_2} = -131.21 + 0.65125 T + -7.636 \times 10^{-4} T^2, \quad (12)$$

$$C_{N_2} = 3454.2 - 11.35 T + 0.015 T^2, \quad (13)$$

where temperature is in K and B and C are in cm³/mol and cm⁶/mol² respectively and the units of the constants have been suppressed. For dry air the correlations for the virial coefficients are:

$$B_{Air} = -137.06 + 0.66785 T + -7.833 \times 10^{-4} T^2, \quad (14)$$

$$C_{Air} = 3528.9 - 12.40 T + 0.016 T^2. \quad (15)$$

These expressions are the result of least squares best fitting to outputs from a database of the property measurements by numerous experimenters [Lemmon et al. 2002]. Equations 12 through 15 were fitted to data over the range of 270 K to 330 K. This range allows application of the correlations at the conditions found in the test section of the flow standard. However, it should be noted that the conditions in the collection tank are much narrower, with pressures ranging from 0 kPa to 101 kPa at a nearly constant temperature of 296.5 K. For these narrower conditions, the third virial coefficient could be ignored with negligible impact on the density uncertainty.

Uncertainty estimates for experimental studies of compressibility are often unavailable, especially for older publications. Comparison of previously compiled compressibility values obtained by various researchers [Dymond and Smith 1980, Hilsenrath et al. 1955, Span et al. 2000, Lemmon et al. 2000] shows agreement to within 10×10^{-6} in the 270 K to 330 K temperature range at 100 kPa. Perhaps more valuable is that this level of agreement is achieved between compressibility measurements made by the traditional *PVT* method and by the more recent speed of sound techniques [Trusler et al. 1997]. Based on this information, a relative standard uncertainty of 10×10^{-6} will be used for the experimental measurements of compressibility. This uncertainty is for a pressure of 100 kPa and it scales with density. The residuals of the equation fitting process to the experimental data are negligibly small ($<1 \times 10^{-6}$ Z). The uncertainty components of the compressibility factor are listed in Table 8.

Table 8. Uncertainty of the compressibility for nitrogen, argon, and dry air.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
	Relative ($\times 10^6$)	(-)	(%)	
Compressibility (Z)				
<i>Compressibility value</i>		1		
experimental data	10	1×10^{-5}	99	based on analysis of literature
impurity effects on Z	1	1×10^{-6}	1	
residuals of best fit	0	0	0	$<1 \times 10^{-6}$
RSS	10	1×10^{-5}		

The source of the dry air used in the flow standard is a Joy oil-free two stage reciprocating compressor and a Zurn refrigeration dryer. The mole fraction of water in this air source is 0.0010 ± 0.0005 . This uncertainty in composition leads to uncertainty in the compressibility of only 1×10^{-6} Z. The uncertainty in compressibility due to impurities is smaller for the other gases.

6.5.3 Molecular Weight

The departure of the molecular weight of ultra high purity nitrogen, industrial liquid nitrogen, and ultra high purity argon from the molecular weight of the pure substance was examined using the impurity specifications of the gas manufacturer. This analysis results in molecular weight relative standard uncertainties less than 1×10^{-6} , but 1×10^{-6} will be assumed for the molecular weight of nitrogen (28.01348 g/mol) and argon (39.94800 g/mole). For the dry air described above, the molecular weight is 28.9532 g/mol and its relative standard uncertainty is 190×10^{-6} due to the variability of water content.

6.6 Density

Now that the sub-components have been quantified, the uncertainty of density measurements made in the collection tank with nitrogen and argon (for volume determinations and for flow measurements) and with dry air (for flow measurements) can be calculated and they are presented in Tables 9 and 10. For the pure gases, the relative standard uncertainty is 68×10^{-6} and the primary contributor is the pressure measurement. For air, the relative standard uncertainty is 208×10^{-6} and the largest contribution is due to water content variations. The uncertainties of the density of ambient air (needed for buoyancy corrections) and of distilled water are considered in the section pertaining to tank volume determinations.

Table 9. The uncertainty of collection tank gas density for nitrogen and argon.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
Collection Tank Density (N_2 & Ar)	Relative ($\times 10^6$)		(%)	
pressure	64	6.45×10^{-3} kPa	88	from Table 5
temperature	22	6.47 mK	10	from Table 7
compressibility	10	1×10^{-5}	2	from Table 8
molecular weight (purity)	1	2.80×10^{-5} g/mol	0	
gas constant	2	1.41×10^{-2} (cm ²)/(s ² K)	0	
RSS	68	7.82×10^{-8} g/cm³		

Table 10. The uncertainty of collection tank gas density for dry air from the NIST Fluid Flow Group small compressor and dryer system.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
Collection Tank Density (Air)	Relative ($\times 10^6$)		(%)	
pressure	64	6.45×10^{-3} kPa	9	from Table 5
temperature	22	6.47 mK	1	from Table 7
compressibility	10	1×10^{-5}	0	from Table 8
molecular weight (purity)	190	5.5×10^{-3} g/mol	89	
gas constant	2	1.41×10^{-2} (cm ²)/(s ² K)	0	
RSS	208	2.38×10^{-7} g/cm³		

6.7 Collection Time

As explained in section 5.2.3, the collection time is an approximate time measured by timers that is then corrected via analysis of records of the inventory pressure data and trigger voltages to minimize inventory mass and improve uncertainty cancellation. The base time is measured redundantly with two Hewlett-Packard Model 53131A counters. The counter calibration and usage leads to less than 0.01 ms uncertainty. Due to the 3000 Hz recording frequency of the inventory pressure and trigger data, the actual rise of

the trigger voltage can be any time within a 0.33 ms window. Assuming a rectangular distribution, the post-processing corrections will have a standard uncertainty of 0.19 ms. This uncertainty applies to both the start and stop times. The time uncertainties of the two pressure measurements used in the mass cancellation procedure are negligible since the times are found by interpolation of the data records and are much smaller than 0.33 ms. The combined collection time uncertainty is 0.3 ms (see Table 11).

Table 11. Collection time uncertainties.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib (%)	Comments
	Relative ($\times 10^6$)	(ms)		
Collection Time				
<i>Time value</i>		100000		
timer cal and usage	0	0.01	0	base time uncertainty
inventory correction (start)	2	0.19	50	3000 Hz, rectangular distribution
inventory correction (stop)	2	0.19	50	3000 Hz, rectangular distribution
RSS	3	0.3		

6.8 Volume of the 677 Liter Collection Tank (Gravimetric Method)

The uncertainty of the determination of the collection tank volume by the previously described gravimetric method (section 5.3.1) is traceable to the uncertainty of the mass and density measurements made during the process, which are in turn dependent on the quantities shown in Fig. 10. The uncertainty of the density measurements for the pure nitrogen and argon gases used for the volume measurements was given in Table 9. The scale used was a Mettler-Toledo model PR10003, which has a 10 kg capacity. The uncertainty of the mass measurements of the high-pressure cylinder before and after discharge is dependent on the buoyancy corrections (ambient air density and cylinder external volume), the reference masses used with the mass comparator, and the performance of the mass comparator. The measurement of the external volume of the high-pressure cylinder via the Archimedes principle was described in an earlier section.

The uncertainty of this measurement is traceable to the density of distilled water, ambient air, reference masses, and the performance of the mass measuring systems.

The uncertainty of the density of ambient air during the course of the various weighing procedures is given in Table 12. The pressure, temperature, and relative humidity uncertainties account for instrument calibration uncertainties as well as variations in the room conditions during the time needed to make a mass measurement. The relative combined uncertainty of the ambient air density is about 500×10^{-6} , with the largest contribution being from temperature.

Table 12. Uncertainty of the density of ambient air.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
Ambient air density	Relative ($\times 10^6$)		(%)	
pressure	129	0.013 kPa	6	cals and change during meas
temperature	336	100 mK	45	cals and change during meas
relative humidity	189394	2.5 %	15	cals and change during meas
equation of state (Z, M, R)	200	0.0002	33	based on literature references
RSS	513	$6.02 \times 10^{-7} \text{ g/cm}^3$		

Table 13. Uncertainty of the external volume of the high-pressure cylinder.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
External tank volume	Relative ($\times 10^6$)		(%)	
apparent mass in air	1	$4.61 \times 10^{-3} \text{ g}$	0	
apparent mass in water	-	0.14 g	34	based on water T uncertainties
density of air	513	$6.01 \times 10^{-7} \text{ g/cm}^3$	0	correlation and meas unc
density of water	20	$2 \times 10^{-5} \text{ g/cm}^3$	15	correlation and meas unc
expansion	20	$9.38 \times 10^{-2} \text{ cm}^3$	15	T and P effects
std deviation of repeated meas.	30	0.14 cm^3	35	
RSS	51	0.24 cm^3		

The uncertainties related to the determination of the external volume of the high-pressure cylinder are listed in Table 13. The 1×10^{-6} relative standard uncertainty for the apparent mass in air is based on uncertainty calculations for the true mass of the weighed cylinder (discussed later). The uncertainty of the apparent mass in water is based on the recorded temperatures of water that made the cylinder barely sink or barely float. Uncertainty of the water temperature for neutral buoyancy of 0.2 K leads to a value for the uncertainty of the apparent mass in water. This uncertainty is not reported in a relative form since the apparent mass in water is zero and the relative uncertainty is therefore undefined. The RSS is calculated using the results in the third column and their sensitivity coefficient. The water density uncertainty includes thermometer uncertainties, estimates of non-uniformity of the water temperature, and uncertainty of the water density correlation obtained from the literature. As previously stated, different values of external volume were used for the full and empty cylinder due to pressure dilation, but an uncertainty related to pressure and temperature effects is included here. The collection tank volume is not very sensitive to this external tank volume, hence larger uncertainty values than $51 \times 10^{-6} V_{ext}$ could certainly be tolerated.

Table 14. Uncertainty of the high-pressure cylinder mass measurement.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
<i>Final mass of high P cylinder</i>	Relative ($\times 10^6$)		(%)	
reference masses	0.5	$1.91 \times 10^{-3} \text{ g}$	26	from NIST Mass Group cal report
room air density	513	$6.01 \times 10^{-7} \text{ g/cm}^3$	45	
reference mass density	0	0 g/cm^3	0	same value for cal. and usage
external cylinder volume	51	0.24 cm^3	1	from unc. of Archimedes method
std deviation of repeated meas.	1	0.002 g	28	
RSS	1	0.00376 g		

The relative standard uncertainties of the cylinder mass measurement (Table 14) are quite small (1×10^{-6}) with the major components being the reference masses, the room air density (for buoyancy corrections) and the performance of the comparator (repeatability of the 5 measurements made with the comparator, a type A uncertainty). The complete mass measurement process was repeated several times for the full and empty cylinder conditions to assess the repeatability of the process, and these repeated mass values never differed by more than $1 \times 10^{-6} m_c$. This repetition was undertaken since a previously used cylinder showed changes over time, probably due to absorption of water from room humidity variations. The uncertainty of the density of the reference masses (7.8 g/cm^3) is negligible since the sensitivity of mass measurements to this component is extremely small. While some of the mass measurement uncertainties for the full and empty cylinder are correlated and this could be used to reduce the uncertainty of the mass delivered to the collection tank, this benefit was not utilized since the improvement was not significant. A table of uncertainty components of the empty cylinder mass measurement is not presented because it is so similar to Table 14.

Finally, the uncertainty of the collection tank volume is presented in Table 15. The relative value of the initial collection tank density uncertainty is quite large, but the sensitivity of the result to this quantity is very small. Recall that uncertainty due to the effects of room temperature variations on the portion of the collection tank not submerged has already been incorporated as a temperature uncertainty. The effects of pressure changes from vacuum to 100 kPa on the tank volume have been considered analytically and found to be negligible. A small volume (1 cm^3) of connecting tubing and valve was necessary to introduce gas from the pressurized cylinder to the collection tank. This volume was measured with alcohol and a graduated syringe and the uncertainty of this volume correction was estimated to be 0.5 cm^3 . By far the largest contribution is from the final gas density, and this in turn is nearly completely traceable to the pressure measurement.

Table 15. Uncertainty of the 677 liter collection tank volume.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
	Relative ($\times 10^6$)		(%)	
Collection tank volume				
Initial mass of high P cylinder	1	0.00385 g	2	see Table 14
Final mass of high P cylinder	1	0.00376 g	2	see Table 14
initial collection tank gas density	100000	$1.14 \times 10^{-9} \text{ g/cm}^3$	0	
final collection tank gas density	68	$4.25 \times 10^{-8} \text{ g/cm}^3$	92	see Table 9
expansion due to P and T	0	0 cm^3	0	< 1 ppm
extra volume uncertainty	1	0.50 cm^3	0	related to liq transfer meas.
std deviation of repeated meas.	16	10.85 cm^3	5	6 measurements, 2 gases
RSS	71	48.44 cm^3		

Each gravimetric volume determination required one day to complete due to the time required to achieve ultimate vacuum in the tank (1 Pa), the time for the pressure transducer to reach thermal equilibrium after filling, and the time to take multiple cylinder mass measurements separated by an hour each time. The volume measurements were done 6 times, 4 times with nitrogen and twice with argon. The standard deviation of these six determinations was $16 \times 10^{-6} V_T$, quite good when one considers that two different gases were used and the uncertainty of their equations of state. The combined uncertainty of the 677 L collection tank volume is $71 \times 10^{-6} V_T$. The 677 L volume was used as a reference to determine the remaining three unknown volumes via the volume expansion method.

6.9 Volume of the 34 Liter Collection Tank (Volume Expansion Method)

As explained in section 5.3.2, the volume expansion method is performed by pressurizing a known volume with pure gas and opening a valve to expand the gas into a previously evacuated unknown volume. The density changes and known volume are used to calculate the unknown volume via Eq. 6. In this case the 677 L volume was used to determine the large inventory volume and the 34 L collection tank volume. Subsequently, the 34 L collection tank volume was used to determine the small inventory volume.

Significant uncertainties of the volume expansion method are related to density and the measurement of pressure. Many components of the previously given pressure uncertainty are correlated for a pressure change measurement made with the same pressure transducer over a short time period (about 1 h). Uncertainties of the piston pressure gauge and the sensor drift can be considered correlated for the short time period and small pressure changes involved (5 kPa to 8 kPa out of 200 kPa full scale).

The uncorrelated uncertainties in the measurement of pressure change are due to sensor non-linearity, resolution, hysteresis, and thermal effects. In order to quantify these uncertainties for the volume expansion method, the piston pressure gauge was used to repeatedly provide a reference step change of 6 kPa to the pressure transducer. The pressure change measured by the pressure transducer was compared to the pressure change calculated from the pressure standard. Based on these experiments, the uncertainty of the pressure difference measurement during the 34 L tank volume determination is 0.3 Pa

Table 16. Uncertainty of the 34 L tank volume determined by the volume expansion method.

Uncertainty Category	Standard Uncertainty (<i>k</i> =1)		Contrib	Comments
	Relative ($\times 10^6$)		(%)	
<i>Collection tank volume</i>				
677 L volume	71	48.4 cm ³	38	from gravimetric determination
large inventory volume	1788	1.298 cm ³	0	from volume expansion method
677 L density change	40	3.53×10^{-9} g/cm ³	12	dominated by pressure
34 L density change	65	-1.12×10^{-7} g/cm ³	32	dominated by pressure
extra volume uncertainty	15	0.5 cm ³	2	measured by liq transfer
std deviation of repeated meas.	46	1.58 cm ³	16	13 volume determinations
RSS	116	4.0 cm³		

The 34 L tank volume uncertainty is summarized in Table 16. The largest uncertainty contributions are from the 677 L volume uncertainty, the density change in the 34 L volume, and the standard deviation of the repeated volume measurements. The uncertainty of the density change in the 677 L volume is dominated by uncertainty in the measurement of the pressure change.

6.10 Inventory Volume

The mass change in the inventory volume is negligible since we used the mass cancellation procedure. However, since there are imperfections in the procedure, uncertainty components related to the inventory mass change cannot be neglected. Fortunately, the most significant of these uncertainty components (due to sensor time constants) are correlated between the start and stop diversions for the methods of operation used in this flow standard. Other correlated inventory volume uncertainties include the pressure and temperature sensor calibrations and the differences between sensed and stagnation values of pressure and temperature. For instance, the inventory temperature is measured incorrectly low by the same amount at both the start and stop conditions due to slow sensor response time, so cancellation of temperature uncertainty occurs. More precisely, the uncertainty of the mass change within the inventory volume caused by the *correlated* pressure and temperature uncertainties can be expressed as:

$$u(\Delta m_I) = \frac{V_I M}{ZR} \left[\left(\frac{1}{T_I^f} u(P_I^f) - \frac{1}{T_I^i} u(P_I^i) \right)^2 + \left(\frac{P_I^f}{(T_I^f)^2} u(T_I^f) - \frac{P_I^i}{(T_I^i)^2} u(T_I^i) \right)^2 \right]^{1/2} \quad (16)$$

where in this equation, $u(P_I)$, $u(T_I)$, and $u(\Delta m_I)$ are the uncertainties of the inventory pressure, the inventory temperature, and the inventory mass change during the collection, respectively. Note that if the uncertainties and the initial and final conditions are equal (i.e. $u(T_I^i) = u(T_I^f)$, $u(P_I^i) = u(P_I^f)$, $T_I^i = T_I^f$, and $P_I^i = P_I^f$), then the terms within parentheses cancel, and the flow uncertainty related to the inventory volume is zero. Equation 16 demonstrates the benefit of matching the initial and final inventory conditions to optimize the cancellation of correlated uncertainties.

Not all of the measurement uncertainties of the inventory volume are correlated. For perfect inventory mass cancellation, the pressure and temperature measured at specific locations in the inventory volume must exhibit perfect correlation with the pressures and temperatures throughout the inventory volume. In this way, the sensor readings “represent” the conditions throughout the volume and when the readings at the specific locations match, the conditions throughout the inventory volume are matched. Unfortunately, this representative relationship may not exist and there may be inconsistencies between the pressure and temperature fields between the start and stop diversions. These inconsistencies may originate from a change in the inventory wall temperature or from differences in the flow paths between the start and stop diversions. The spatial inconsistencies are uncorrelated and their magnitude is likely a function of the mass flow.

Another source of inventory uncertainty, alluded to previously, is due to imperfection in matching the stop diversion pressure to the start diversion pressure. Recall that the inventory pressure is recorded while the bypass valve is open (nominally the barometric pressure), and that the tank filling is stopped when the inventory pressure regains this same pressure. In this way, the pressure at the beginning of the dead-end time transients is nearly equal for both diversions and the symmetry of the transients is improved. At high flows, it becomes more difficult to match these initial pressures in the high speed data records and a “trigger pressure difference” that increases with increasing flow occurs. The size of the trigger pressure difference can be reduced by using faster sensors and a fast data acquisition and diverter valve control system. An example of the trigger pressure difference can be seen in Fig. 7, where at times less than zero, the pressure traces differ by about 1.6 kPa. The trigger pressure difference, coupled with the “historical” nature of the inventory pressure measurements due to the sensor time constant, is another reason that matching of the pressure sensor readings does not necessarily lead to matching of the actual conditions in the inventory volume. Hence the trigger pressure difference is another source of inventory uncertainty that scales with the flow.

It is difficult to assess the magnitude of the uncorrelated uncertainties of pressure and temperature between the start and stop diversions in the inventory volume. Our strategy is to estimate the uncorrelated inventory uncertainties and then perform experiments (see Section 7) to confirm that the estimates are reasonable. We assumed that the uncorrelated inventory uncertainties scale with the flow and are essentially zero at the minimum flow of each tank. We will assume values of 3 kPa and 9 K (about 3 % of the nominal values) for the maximum flow of each tank.

Uncertainties related to the fast measurement of pressure with a 700 kPa full scale Heise Model HPO sensor in the inventory volume are listed in Table 17, separated into correlated and uncorrelated components.

Table 17. Uncertainties in the inventory pressure measurement, correlated and uncorrelated, for maximum flow conditions.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib (%)	Comments
	Relative ($\times 10^6$)	(kPa)		
<i>Inventory Pressure Measurement</i>				
<i>Pressure value</i>		100		
sensor calibration	3000	0.30	0	
sensor time response	1350000	135	100	from inv. model at max flow
sensed vs. stagnation	710	0.071	0	for max flow
RSS (correlated)	1350004	135		
sensor repeatability	3.00E+02	0.03	0	from calibration data
spatial inconsistency	3.00E+04	3	100	estimated
RSS (uncorrelated)	30001	3.0		

Table 18. Inventory temperature uncertainties, correlated and uncorrelated, for the maximum flow for each tank.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
	Relative ($\times 10^6$)	(mK)		
Inventory Thermocouple				
<i>Temperature value</i>		297000		
sensor calibration	337	100	0	
sensor time response	168350	50000	97	from inventory model
sensed vs. stagnation	50	15	0	for max flow
RSS (correlated)	168351	50000		
sensor repeatability	286	85	0	from calibration data
spatial inconsistency	30303	9000	100	estimated
RSS (uncorrelated)	30304	9000		

The uncertainties of the measurement of temperature in the inventory volume are listed in Table 18, again divided into correlated and uncorrelated components. The uncertainties include calibration, time response, sensed versus stagnation issues, sensor repeatability, and spatial non-uniformity or inconsistency between start and stop diversions.

Table 19. Uncertainty of the 1000 cm³ (large) inventory volume.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
	Relative ($\times 10^6$)			
Collection tank volume			(%)	
677 L volume	71	48.4 cm ³	0	
677 L density change	1039	3.41×10^{-9} g/cm ³	54	
inv. vol. density change	120	2.81×10^{-7} g/cm ³	1	
extra volume uncertainty	526	0.5 cm ³	14	
std. deviation of repeated meas.	799	0.76 cm ³	32	
RSS	1419	1.35 cm³		

The uncertainties for the large and small inventory volumes determined by the volume expansion method are presented in Tables 19 and 20. Although the relative uncertainties

of these volumes are large, the sensitivity of the flow measurement to these volumes is small due to the inventory mass cancellation scheme and the relatively small size of V_L . For the very small pressure changes used for the inventory volume determinations, the ability of the pressure transducers to measure the pressure change becomes a large uncertainty issue. The standard deviation of repeated measurements is large for these volume determinations due to the uncertainty of the small pressure change measurements. The ratio of the known tank volume to the unknown inventory volume is about 500 to 1, hence the pressure change is only about 0.3 kPa for an initial pressure of 150 kPa. The uncertainty of the pressure change measurement (0.3 Pa) is based on the previously described experiments using the pressure standard. The instrument resolution (1.3 Pa) is also a concern for such small pressure changes measured with a 200 kPa full-scale transducer. Although the noise in the pressure data is greater than 1.3 Pa, averaging the pressure measurements over 30 seconds reduces the resolution to an acceptable level. For the inventory volumes, the “extra volume” includes tubing and valves used to introduce gas to the system and volume changes caused by the actuation of the diverter valves. The extra volume corrections are based on liquid transfer into or out of the volume by pipette, and /or by dimensional calculations.

Table 20. Uncertainty of the 75 cm³ (small) inventory volume.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
<i>Collection tank volume</i>	Relative ($\times 10^6$)		(%)	
34 L volume	116	4.0 cm ³	0	
34 L density change	811	3.41×10^{-9} g/cm ³	24	
inv. vol. density change	120	2.31×10^{-7} g/cm ³	1	
extra volume uncertainty	1346	0.1 cm ³	66	
std. deviation of repeated meas.	511	0.038 cm ³	9	
RSS	1661	0.12 cm³		

Tables 21 and 22 show the uncertainty in the mass change in the inventory volume for the largest flows in the 34 L and 677 L systems. The relative inventory uncertainty is

extremely large since the mass change is nearly zero. The mass change was calculated using the same 3 kPa and 9 K uncorrelated uncertainty values previously discussed.

Table 21. Uncertainty of the inventory mass change for the 677 L system.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
<i>Inventory mass change</i>	Relative ($\times 10^6$)		(%)	
initial density	42643	$6.29 \times 10^{-5} \text{ g/cm}^3$	50	3 kPa and 9 K uncorr. inv. unc.
final density	42643	$6.24 \times 10^{-5} \text{ g/cm}^3$	50	3 kPa and 9 K uncorr. inv. unc.
volume	1419	1.35 cm^3	0	see Table 19
RSS	-	$8.42 \times 10^{-2} \text{ g}$		

Table 22. Uncertainty of the inventory mass change for the 34 L system.

Uncertainty Category	Standard Uncertainty ($k=1$)		Contrib	Comments
<i>Inventory mass change</i>	Relative ($\times 10^6$)		(%)	
initial density	42643	$6.29 \times 10^{-5} \text{ g/cm}^3$	50	3 kPa and 9 K uncorr. inv. unc.
final density	42643	$6.24 \times 10^{-5} \text{ g/cm}^3$	50	3 kPa and 9 K uncorr. inv. unc.
volume	1661	0.123 cm^3	0	see Table 20
RSS	-	$6.58 \times 10^{-3} \text{ g}$		

The sub-component uncertainties of gas density, volume, collection time, and inventory mass change above have been combined in Section 6.2 to give the uncertainty in mass flow.

7 Experimental Verification of the Uncertainty of the 34 L and 677 L *PVTt* Gas Flow Standards

Throughout the range 3 L/min to 110 L/min, flows were measured independently using the 34 L and the 677 L collection systems, using a set of critical flow venturis (CFV) as transfer standards, and the two systems agreed within a relative difference of 150×10^{-6} . Double diversions were used to evaluate the 677 L system over a range of 300 L/min to 1600 L/min, and the relative differences between single and double diversions were less than 75×10^{-6} . These differences are within our expectations based on the uncertainty analysis presented in Section 6.

7.1 Comparison of the 34 L and 677 L Flow Standards

To test both systems, we performed comparisons between the two flow standards over the range of flows where they could both be used: $3 \text{ L/min} < \dot{m} < 110 \text{ L/min}$ (3.6 g/min to 138 g/min of nitrogen). The collections ranged from as short as 18 s to more than 4 h.

Figure 11 shows the difference in the discharge coefficients of several critical flow venturis as measured by both the 34 L and 677 L systems, plotted versus flow. The agreement between the two flow standards is $150 \times 10^{-6} \dot{m}$ over the entire range tested. The throat diameters of the venturis used for the comparisons ranged between 0.2921 mm and 1.7 mm. The comparisons were done with the same pressure and temperature sensors associated with the venturi during the testing on both flow standards in order to reduce some possible sources of discharge coefficient differences. Numerous collections were made for each tank at each flow to confirm stability of the conditions at the meter under test.

How well should the two systems agree? The difference between the discharge coefficients measured by the two *PVTt* systems should be less than the root sum square (RSS) of the uncertainties of the two standards, especially when one considers that the uncertainties due to pressure and temperature measurements are correlated between the two standards. For the lowest flows of the comparison range, the uncertainties originating from the inventory volume are quite small for both systems and the observed differences between them are dominated by tank volume uncertainties. From Fig. 11 it can be seen

that the two systems differ by about $100 \times 10^{-6} \text{ m}$ for flows less than 20 L/min. The RSS of the two relative standard volume uncertainties is 137×10^{-6} ($k = 1$).

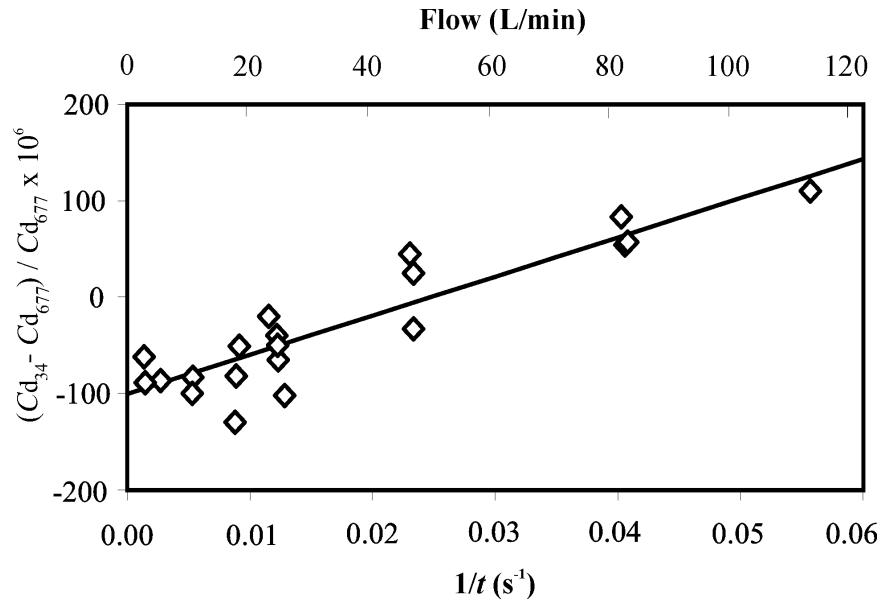


Figure 11. Difference in the discharge coefficient of critical flow venturis calibrated on both the 34 L and 677 L flow standards versus flow and the inverse of the collection time for the 34 L tank. Also plotted is a linear best fit of the data.

At the higher flows of the comparison range, the uncertainties associated with the transient conditions in the inventory volume should be negligible in the 677 L system, but growing with increasing flow for the 34 L system. Because the collection times were $1/20^{\text{th}}$ as long when using the smaller tank, any timing error (or, equivalently any imperfection of the mass cancellation technique) was 20 times more important when using the smaller tank. Figure 11 suggests that the inventory uncertainties cause the flow standard to read too high as the flow is increased, changing the difference by about $200 \times 10^{-6} \text{ m}$ over the range of flows compared. This value is comparable to the relative uncertainty of 135×10^{-6} ($k = 1$) contributed by the inventory volume at the highest flows in the 34 L system (61% of 219×10^{-6} from Table 3). Therefore, the differences observed in the comparison are in reasonable accordance with the uncertainty analysis.

Figure 11 also shows the tank comparison results from the perspective of time measurement uncertainty rather than the mass. We interpreted the comparison results using the simplified model $\dot{m} = m/t$, where m is the mass collected and t is the collection time using the 34 L tank. Making the assumption that there exists a constant error in the mass measurement, δm , for all flows (say due to a tank volume error) and a constant error in time measurement, δt , for all flows (say due to the time constant of the inventory pressure sensor), we can derive a simple linear model for the error in mass flow measurement, i.e.,

$$\frac{\delta \dot{m}}{\dot{m}} = \frac{\delta m}{m} - \frac{\delta t}{t}. \quad (17)$$

Since the mass collected and the mass error are both essentially constant, this model suggests that a linear function of the inverse of the collection time should fit the tank comparison data. Such a linear function fits reasonably well, as shown in Fig. 11, and its slope implies a constant timing error of 4 ms. A timing error of this order is not surprising because the timing is based on a pressure sensor with a time constant of approximately 20 ms. The standard deviation of a measurement from the best fit line is $24 \times 10^{-6} \dot{m}$.

The comparison results could be the basis for corrections to the 34 L system. The intercept of Fig. 11 could be used to change the volume of the 34 L tank and improve the agreement between the two systems at low flows. The slope could be used to improve agreement at higher flows. This approach offers the possibility of reducing the comparison differences to zero with a standard deviation of $24 \times 10^{-6} \dot{m}$. However, these corrections have not been made at the present time for several reasons. The comparison results are consistent with the uncertainty analysis. Also, despite the success of Eq. 17, we feel that the inventory uncertainties are more related to pressure and temperature than time, so it is more appropriate to make improvements in those measurements to reduce the slope in the comparison data. The volume (or offset) differences can be improved by repeating and refining the volume expansion process used to determine the 34 L tank

size. This approach adheres to the definition of primary standard for both systems since neither one has been calibrated by a flow measurement against some other flow standard.

During some of the comparison flows, we noticed that the pressure downstream of the critical flow venturi was significantly higher in the 34 L system than in the 677 L system (108 kPa vs. 100 kPa) due to the smaller tube size and resultant higher pressure drop. For some of our venturis (with relatively short diffusers) this pressure difference caused slight changes in the upstream pressure (and the discharge coefficient), even at conditions well above the critical pressure ratio. Therefore, our assumption that for the same throat Reynolds number, the discharge coefficient of the venturi is independent of the downstream pressure may not be perfectly valid. We suspect that some of the differences observed between the tanks in Fig. 11 are due to the venturis (even though long diffusers were used).

In one series of experiments, the trigger pressure difference was purposely varied over a range from -2 kPa to 27 kPa at a constant flow of 82 L/min in the 34 L system. The purpose of the test was to measure the dependence of the venturi discharge coefficient on the trigger pressure difference and hence assess its influence on the inventory volume uncertainties. The tests showed a relative change of 10×10^{-6} in discharge coefficient for each 1 kPa change in the trigger pressure difference. Since the largest trigger pressure difference is less than 3 kPa in the present system, this effect is expected to contribute only $30 \times 10^{-6} \dot{m}$ to the flow uncertainty. Therefore the major contributor to the inventory uncertainty appears to be spatial inconsistency of the pressure and temperature fields between the start and stop diversions or some other, unknown flow dependent uncertainty source.

7.2 Multiple Diversions in the 677 L Flow Standard

To confirm that the uncertainty analysis for the inventory volume of the 677 L collection system was reasonable, we performed CFV calibrations at identical flows following two different protocols. In the first protocol, the inventory volume was dead-ended at the

beginning and end of the collection interval in the usual manner. In the second protocol, the collection interval was divided into two subintervals, i.e. each flow measurement had *two* start and stop diversions. The intermediate dead-end times were set up so that the pressure transients in the inventory volume still permitted the mass cancellation procedure. Breaking the collection into two subintervals has the effect of doubling the uncertainty contribution from the inventory volume. The CFV discharge coefficients from the two protocols were compared to assess the magnitude of the uncertainties introduced by the inventory volume and the flow diversion process. Three flows between 300 L/min and 1600 L/min were tested and the differences in discharge coefficient were all less than $75 \times 10^{-6} \dot{m}$ as shown in Table 23.

Table 23. Differences in CFV discharge coefficients (C_d) for two and one diversion in the 677 L flow standard.

Flow (L/min)	$[C_d(2 \text{ diversions}) - C_d]/C_d \times 10^6$
300	53 ± 25
700	-27 ± 31
1600	75 ± 122

8 Summary

We have given a description of the gas flowmeter calibration services that use the 34 L and 677 L *PVTt* primary standards within the NIST Fluid Flow Group. These *PVTt* standards were designed to calibrate flowmeters between 1 L/min to 2000 L/min, with uncertainties between 0.02 % and 0.05 %. See Table 1 for more details about the test capabilities of the calibration service such as available gases and pressure at the test section. The 34 L *PVTt* standard has been used at flows as low as 0.025 L/min.

The intended audience for this document is potential flowmeter calibration customers, hence we have attempted to address their likely questions. We have described the method of operation of the primary standard and have given the uncertainty analysis for a mass flow measurement (see Tables 2 and 3). We have given a description of the standard gas

flow calibration, including a sample calibration report, as well as sources for instructions for submitting a flowmeter for calibration.

The 34 L and 677 L *PVTt* flow standards have several novel features. The collection tanks are immersed in a water bath that matches the nominal room temperature and is stable and uniform to 1 mK. The collection tanks are divided into sections of small enough diameter that the gas inside them achieves thermal equilibrium with the surrounding water bath in 20 minutes or less. This reduces the contribution of temperature to the flow measurement uncertainty to a low level.

Uncertainties related to the inventory volume and the diversion of gas into the collection tank at the start and stop of a flow measurement have been studied in great detail. A thermodynamic model of the inventory volume during diversion has been utilized to understand the large pressure and temperature transients and the importance of sensor time constants on the flow measurement uncertainty. The flow standard is operated to achieve “mass cancellation” in the inventory volume, thereby taking advantage of correlated sensor uncertainties to minimize uncertainty contributions from the inventory volume. The uncertainty contributions of the inventory volume have been considered from both the time and mass perspectives.

The volumes of the collection tanks were measured by two methods, a gas gravimetric method and a volume expansion method. Six gravimetric determinations of the 677 L collection tank volume made with nitrogen and argon agree with a standard deviation of $16 \times 10^{-6} V_T$.

A detailed uncertainty analysis for the gas flow standard has been presented. The analysis started with the basis equation utilized to calculate flow in a *PVTt* system and followed the propagation of uncertainties method suggested by international standards. The uncertainties of the sub-components have been examined at a fundamental level.

The uncertainty analysis shows that the 677 L system measures mass flow with an uncertainty between $200 \times 10^{-6} \dot{m}$ and $300 \times 10^{-6} \dot{m}$ for a pure gas like nitrogen or argon. The higher uncertainty applies to higher flows as the inventory transients and the related uncertainties grow larger. For the 34 L tank and pure gases, the uncertainties range from $440 \times 10^{-6} \dot{m}$ to $270 \times 10^{-6} \dot{m}$. The uncertainties are larger for the 34 L tank because the tank volume uncertainty is relatively greater and the inventory volume is relatively larger for the small system. For pure gas measurements, the largest sources of uncertainty can be traced to pressure measurement (about $70 \times 10^{-6} P$) which is the major contributor to gas density and tank volume uncertainties. For air flow measurements using gas from the existing compressor and drier, mass flow uncertainties are about $500 \times 10^{-6} \dot{m}$ for both standards and the major contribution is the uncertainty in the moisture content of the air.

Comparisons between the 34 L and 677 L standards from 3 L/min to 100 L/min show agreement within $150 \times 10^{-6} \dot{m}$ or better. Experiments using single diversions (normal operation) and double diversions to the collection tank were used to validate the uncertainty estimates of the 677 L inventory volume and the differences between these two methods were less than $75 \times 10^{-6} \dot{m}$. The evaluation results along with comparisons to previously existing gas flow standards support the uncertainty statements for the new standards.

9 References

Carslaw, H. S. and Jaeger, J. C., *Conduction of Heat in Solids*, 2nd Edition, Clarendon Press, Oxford, pp 198-201, 1946.

Coleman, H. W. and W. G. Steele, *Experimentation and Uncertainty Analysis for Engineers*, John Wiley and Sons, 2nd edition, 1999.

Dymond, J. H. and Smith, E. B., *The Virial Coefficients of Pure Gases and Mixtures: A Critical Compilation*, Clarendon Press, Oxford, 1980.

Harris, R. E. and Johnson, J. E., *Primary Calibration of Gas Flows with a Weight / Time Method*, Proceedings 2nd International Symposium on Fluid Flow Measurement, Calgary, Canada, pp. 347–358, June, 1990.

Hilsenrath, J., Beckett, C. W., Benedict, W. S., Fano, L., Hoge, H. J., Masi, J. F., Nuttall, R. L., Touloukian, Y. S., and Woolley, H. W., *Tables of Thermal Properties of Gases*, NBS Circular 564, 1955.

International Organization for Standardization, *International Vocabulary of Basic and General Terms in Metrology*, 2nd edition, 1993.

International Organization for Standardization, *Guide to the Expression of Uncertainty in Measurement*, Switzerland, 1996.

Ishibashi, M., Takamoto, M., and Watanabe, N., *New System for the Pressurized Gas Flow Standard in Japan*, Proceedings of International Symposium on Fluid Flow Measurements, AGA, 1985.

Jaeger, J. B. and Davis, R. S., *A Primer for Mass Metrology*, NBS Special Publication 700-1, National Bureau of Standards, Gaithersburg, Maryland, Eq. 20a, pp. 22, 1984.

Johnson, A. N., Wright, J. D., Moldover, M. R., and Espina, P. I., *Temperature Characterization in the Collection Tank of the NIST 26 m³ PVT Gas Flow Standard*, Metrologia, 40, 211–216, 2003.

Kegel, T., *Uncertainty Analysis of a Volumetric Primary Standard for Compressible Flow Measurement*, 3rd International Symposium of Fluid Flow Measurement, San Antonio, TX, USA, 1995.

Lemmon, E. W., Jacobsen, R. T., Penoncello, S. G., and Friend, D. G., *Thermodynamic Properties of Air and Mixtures of Nitrogen, Argon, and Oxygen from 60 to 2000 K at Pressures to 2000 MPa*, J. Phys. Chem. Ref. Data, 29, (3), 331-362, 2000.

Lemmon, E. W., McLinden, M. O., and Huber, M. L., Refprop 23: Reference Fluid Thermodynamic and Transport Properties, NIST Standard Reference Database 23, Version 7, National Institute of Standards and Technology, Boulder, Colorado, 2002.

Marshall, J. L., *NIST Calibration Services Users Guide 1998*, NIST Special Publication 250, January, 1998.

Moldover, M. R., Trusler, J. P. M., Edwards, T. J., Mehl, J. B., and Davis, R. S., *Measurement of the Universal Gas Constant R Using a Spherical Acoustic Resonator*, NIST J. of Res., 93, (2), 85–143, 1988.

Olsen, L. and Baumgarten, G., *Gas Flow Measurement by Collection Time and Density in a Constant Volume*, Flow: Its Measurement and Control in Science and Industry, Instrument Society of America, Pittsburgh, PA, USA, pp. 1287–1295, 1971.

Patterson, J. B. and Morris, E. C., *Measurement of Absolute Water Density, 1° C to 40° C*, Metrologia, 31, pp. 277-288, 1994.

Trusler, J. P. M., Wakeham, W. A., and Zarari, M. P., *Model Intermolecular Potentials and Virial Coefficients Determined from the Speed of Sound*, Molecular Physics, 90, (5), pp. 695–703, 1997.

Wright, J. D., *The Long Term Calibration Stability of Critical Flow Nozzles and Laminar Flowmeters*, National Conference of Standards Laboratories Conference Proceedings, Albuquerque, NM, USA, pp. 443-462, 1998.

Wright, J. D. and Mattingly, G. E., *NIST Calibration Services for Gas Flow Meters: Piston Prover and Bell Prover Gas Flow Facilities*, NIST Special Publication 250-49, National Institute of Standards and Technology, Gaithersburg, Maryland, August, 1998.

Wright, J. D., *Gas Flow Measurements and Standards: Development and Validation of a PVTt Primary Gas Flow Standard*, Doctoral thesis to Kogakuin University, Tokyo, Japan, September, 2003A.

Wright, J. D., *What Is the “Best” Transfer Standard for Gas Flow?*”, FLOMEKO, Groningen, the Netherlands, May, 2003B.

Appendix: Sample Calibration Report

REPORT OF CALIBRATION

FOR

A CRITICAL FLOW NOZZLE

July 7, 2003

Mfg.: Meter Builders, Inc.
Serial No: 1234
Throat Diameter: 0.125 in (0.3175 cm)

submitted by

Flowmasters, Inc.
Metertown, MD

Purchase Order No. A123 dated June 23, 2003

The flow meter identified above was calibrated by flowing filtered dry air at a constant rate through the flow meter and then into a volumetric prover (the NIST 677 L *PVTt* standard). The *PVTt* standard determines mass flow, \dot{m} , by measuring the change in density of gas diverted into a known volume for a measured period of time.¹ The flow meter was tested at five flows and at each flow, three (or more) measurements were gathered on two different occasions and used to produce averages at each of these flows. As a result, the tabulated data for this test are averages of six or more individual calibration measurements.

The nozzle was installed in an assembly that meets the ISO Standard for critical nozzles² and a photograph of the installation is shown in Figure 1. The nozzle temperature (T_1) and pressure (P_1) were measured with NIST sensors, (Keithley SN 687848, thermistor #3, and Paroscientific SN 75971). Stagnation temperature, T_0 was calculated from the measured temperature via the following equation, using a recovery factor, r , of 0.75:

$$T_0 = T_1 \cdot \left[1 + \frac{\gamma - 1}{2} \cdot M^2 \cdot (1 - r) \right] \quad (1)$$

¹ Wright, J. D., Johnson, A. N., and Moldover, M. R., *Design and Uncertainty Analysis for a PVTt Gas Flow Standard*, J. Res. Natl. Inst. Stand. Technol., 108, 21-47, 2003.

² *Measurement of Gas Flow by Means of Critical Flow Venturi Nozzles*, ISO 9300: 1990 (E), International Organization for Standardization, Geneva, Switzerland, 1990.

and the stagnation pressure, P_0 , was calculated via the equation:

$$P_0 = P_1 \cdot \left[1 + \frac{\gamma - 1}{2} \cdot M^2 \right]^{\frac{\gamma}{\gamma - 1}} \quad (2)$$

where γ is the specific heat ratio and M is the Mach number in the approach pipe, both based on P_1 and T_1 . The largest of these corrections is 0.0067% for pressure.

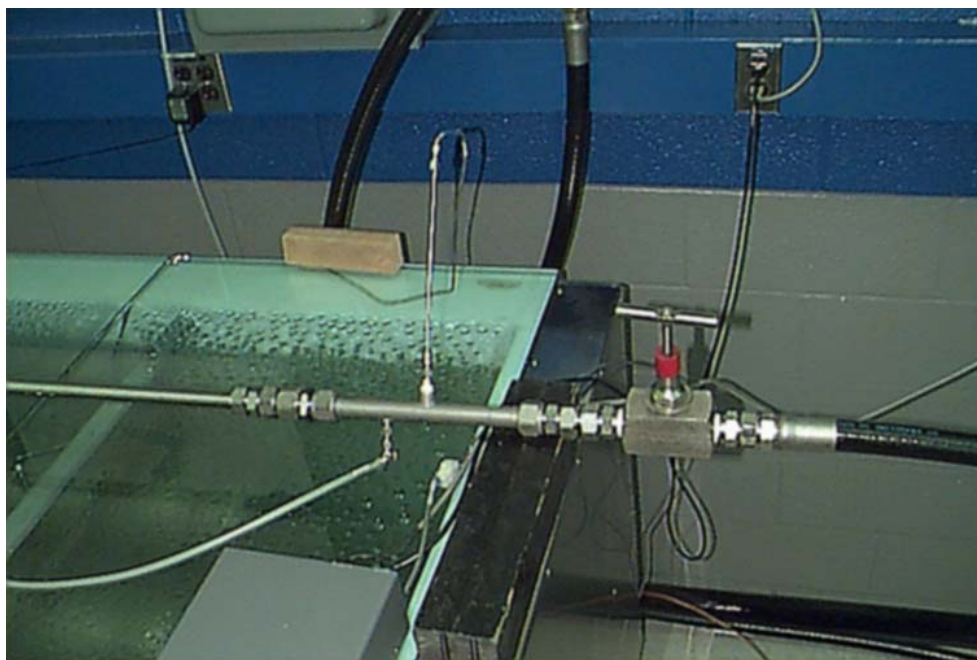


Figure 1. A photograph of the flow meter installation.

The Reynolds number is included in the tabulated data and it was calculated using the following expression:

$$Re = \frac{4 \cdot \dot{m}}{\pi \cdot d \cdot \mu} \quad (3)$$

where \dot{m} is the mass flow of gas, d is the nominal nozzle throat diameter, and μ is the gas viscosity, all in consistent units so that Re is dimensionless. The viscosity of the gas was calculated using best-fit equations which are based on the NIST gas properties database³:

$$\mu = a_0 + a_1 T_0 + a_2 T_0^2 + a_3 T_0^3 \quad (4)$$

³ Lemmon, E. W., McLinden, M. O., and Huber, M. L., *Refprop 23: Reference Fluid Thermodynamic and Transport Properties*, NIST Standard Reference Database 23, Version 7, National Institute of Standards and Technology, Boulder, Colorado, 2002.

where μ has units g / (cm s), and T_0 is in K. The polynomial coefficients, a_i are in turn polynomial functions of pressure

$$a_i = b_0^i + b_1^i P_0 + b_2^i P_0^2 + b_3^i P_0^3 \quad (5)$$

where P_0 is in kPa and the coefficients b_j^i for dry air are:

$$b_j^i(\mu) = \begin{matrix} & -1.48711900\text{E-}06 & 2.36550580\text{E-}08 & -4.74728350\text{E-}11 & 3.80951780\text{E-}14 \\ & 8.03433280\text{E-}07 & -2.06447690\text{E-}10 & 4.86819380\text{E-}13 & -3.87442880\text{E-}16 \\ -7.32108840\text{E-}10 & 6.60598760\text{E-}13 & -1.65670740\text{E-}15 & 1.31012510\text{E-}18 & \\ 4.44444440\text{E-}13 & -7.23905720\text{E-}16 & 1.87289560\text{E-}18 & -1.47306400\text{E-}21 & \end{matrix} \quad (6)$$

where i = row number and j = column number.

The discharge coefficient C_d was calculated from the expression:

$$C_d = \frac{4 \cdot \dot{m} \cdot \sqrt{R \cdot T_0}}{\pi \cdot d^2 \cdot P_0 \cdot C^*} \quad (7)$$

where R is the gas constant (the universal gas constant, 8.314471 J / (mol K), divided by the gas molecular weight, 28.9646431 g/mol). The critical flow factor, C^* , was calculated from the expression:

$$C^* = \sqrt{\gamma \frac{2}{\gamma+1} \frac{\gamma+1}{\gamma-1}} \quad (8)$$

where γ is the specific heat ratio, calculated using the same system of polynomials described above with the following coefficients:

$$b_j^i(\gamma) = \begin{matrix} & 1.40035540\text{E+}00 & 2.31594790\text{E-}04 & 2.32361020\text{E-}08 & 3.48369500\text{E-}13 \\ & -2.51273630\text{E-}06 & -1.63018610\text{E-}06 & -2.01773710\text{E-}10 & -4.02631530\text{E-}15 \\ 9.40776360\text{E-}08 & 4.19213690\text{E-}09 & 5.90056690\text{E-}13 & 1.42526470\text{E-}17 & \\ -3.01845240\text{E-}10 & -3.79086500\text{E-}12 & -5.81559640\text{E-}16 & -1.61335590\text{E-}20 & \end{matrix} \quad (9)$$

The calibration results are presented in the following table and figure.

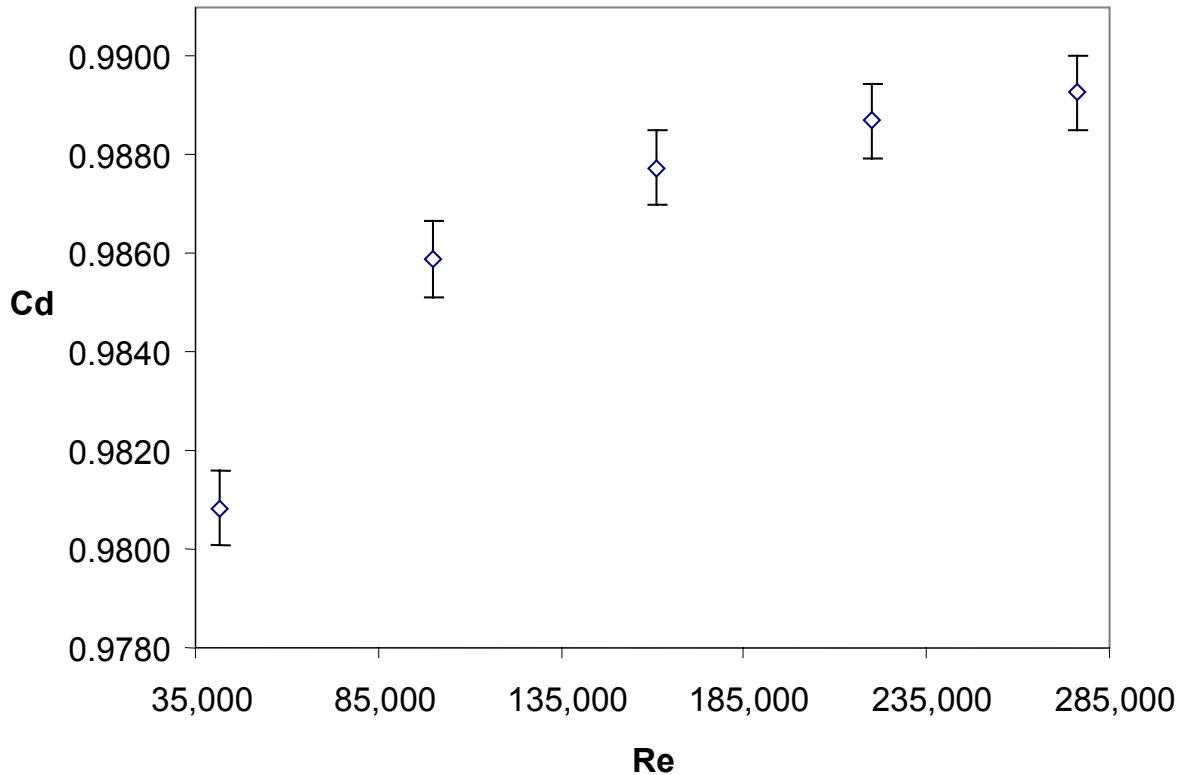


Figure 2. Calibration results for 0.125 in (0.3175 cm), SN 1234 nozzle

Table 1. Calibration results for 0.125 in (0.3175 cm), SN 1234 nozzle from the 677 L PVTt standard.

P_0 [kPa]	T_0 [K]	\dot{m} [lb _m /s]	C^* []	Re []	C_d []	U_r [%]
104.07	295.73	0.004189	0.68505	41471.1	0.9808	0.08
249.69	295.26	0.010117	0.68550	100147.9	0.9859	0.08
399.90	294.87	0.016256	0.68597	160854.2	0.9877	0.08
546.52	294.63	0.022261	0.68643	220116.4	0.9887	0.08
685.88	294.49	0.027979	0.68686	276392.8	0.9893	0.08

An analysis was performed to assess the uncertainty of the results obtained for the meter under test.^{4,5,6} The process involves identifying the equations used in calculating the

⁴ International Organization for Standardization, *Guide to the Expression of Uncertainty in Measurement*, Switzerland, 1996 edition.

⁵ Taylor, B. N. and Kuyatt, C. E., *Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results*, NIST TN 1297, 1994 edition.

calibration result (measurand) so that the sensitivity of the result to uncertainties in the input quantities can be evaluated. The 67% confidence level uncertainty of each of the input quantities is determined, weighted by its sensitivity, and combined with the other uncertainty components by root-sum-square to arrive at a combined uncertainty (U_c).

The combined uncertainty is multiplied by a coverage factor of 2.0 to arrive at an expanded uncertainty (U_e) of the measurand with approximately 95% confidence level.

As described in the references, if one considers a generic basis equation for the measurement process, which has an output, y , based on N input quantities, x_i ,

$$y = y(x_1, x_2, \dots, x_N) \quad (10)$$

and all uncertainty components are uncorrelated, the normalized expanded uncertainty is given by,

$$\frac{U_e(y)}{y} = k \frac{U_c(y)}{y} = k \sqrt{\sum_{i=1}^N s_i^2 \left(\frac{u(x_i)}{x_i} \right)^2} \quad (11)$$

In the normalized expanded uncertainty equation, the $u(x_i)$'s are the standard uncertainties of each input, and s_i 's are their associated sensitivity coefficients, given by,

$$s_i = \frac{\partial y}{\partial x_i} \frac{x_i}{y} \quad (12)$$

The normalized expanded uncertainty equation is convenient since it permits the usage of relative uncertainties (in fractional or percentage forms) and of dimensionless sensitivity coefficients. The dimensionless sensitivity coefficients can often be obtained by inspection since for a linear function they have a magnitude of unity.

For this calibration, the uncertainty of the discharge coefficient has components due to the measurement of the mass flow by the primary standard, $u(\dot{m}) = 0.025\%$,⁷ as well as the pressure, $u(P) = 0.02\%$, and temperature, $u(T) = 0.03\%$, measurements at the meters under test. The sensitivity coefficients for mass flow and pressure are 1, and the sensitivity coefficient for temperature is $\frac{1}{2}$. This uncertainty analysis assumes that the user will use the same values for the throat diameter and the critical flow factor given herein and that the uncertainties in these quantities are correlated and cancel.

To measure the reproducibility⁸ of the test, the standard deviation of the discharge

⁶ Coleman, H. W. and Steele, W. G., *Experimentation and Uncertainty Analysis for Engineers*, John Wiley and Sons, 2nd ed., 1999.

⁷ Wright, J. D., Johnson, A. N., and Moldover, M. R., *Design and Uncertainty Analysis for a PVTt Gas Flow Standard*, J. Res. Natl. Inst. Stand. Technol., 108, 21-47, 2003.

⁸ Reproducibility is herein defined as the closeness of agreement between measurements with the flow changed and then returned to the same nominal value.

coefficient at each of the nominal flows was used to calculate the relative standard uncertainty (the standard deviation divided by the mean and expressed as a percentage). The reproducibility was root-sum-squared along with the other uncertainty components to calculate the combined uncertainty. Using the values given above results in the expanded uncertainties listed in the data table and shown as error bars in the figure.

For the Director,
National Institute of Standards and Technology

Dr. Pedro I. Espina
Leader, Fluid Flow Group
Process Measurements Division
Chemical Science and Technology Laboratories