



A11105 974018



NBS TECHNICAL NOTE 1154

U.S. DEPARTMENT OF COMMERCE / National Bureau of Standards

A Programmable Sample Dryer for Thermal Ionization Mass Spectrometry

QC
100
.U5753
No. 1154
1982

NATIONAL BUREAU OF STANDARDS

The National Bureau of Standards¹ was established by an act of Congress on March 3, 1901. The Bureau's overall goal is to strengthen and advance the Nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research and provides: (1) a basis for the Nation's physical measurement system, (2) scientific and technological services for industry and government, (3) a technical basis for equity in trade, and (4) technical services to promote public safety. The Bureau's technical work is performed by the National Measurement Laboratory, the National Engineering Laboratory, and the Institute for Computer Sciences and Technology.

THE NATIONAL MEASUREMENT LABORATORY provides the national system of physical and chemical and materials measurement; coordinates the system with measurement systems of other nations and furnishes essential services leading to accurate and uniform physical and chemical measurement throughout the Nation's scientific community, industry, and commerce; conducts materials research leading to improved methods of measurement, standards, and data on the properties of materials needed by industry, commerce, educational institutions, and Government; provides advisory and research services to other Government agencies; develops, produces, and distributes Standard Reference Materials; and provides calibration services. The Laboratory consists of the following centers:

Absolute Physical Quantities² — Radiation Research — Thermodynamics and Molecular Science — Analytical Chemistry — Materials Science.

THE NATIONAL ENGINEERING LABORATORY provides technology and technical services to the public and private sectors to address national needs and to solve national problems; conducts research in engineering and applied science in support of these efforts; builds and maintains competence in the necessary disciplines required to carry out this research and technical service; develops engineering data and measurement capabilities; provides engineering measurement traceability services; develops test methods and proposes engineering standards and code changes; develops and proposes new engineering practices; and develops and improves mechanisms to transfer results of its research to the ultimate user. The Laboratory consists of the following centers:

Applied Mathematics — Electronics and Electrical Engineering² — Mechanical Engineering and Process Technology² — Building Technology — Fire Research — Consumer Product Technology — Field Methods.

THE INSTITUTE FOR COMPUTER SCIENCES AND TECHNOLOGY conducts research and provides scientific and technical services to aid Federal agencies in the selection, acquisition, application, and use of computer technology to improve effectiveness and economy in Government operations in accordance with Public Law 89-306 (40 U.S.C. 759), relevant Executive Orders, and other directives; carries out this mission by managing the Federal Information Processing Standards Program, developing Federal ADP standards guidelines, and managing Federal participation in ADP voluntary standardization activities; provides scientific and technological advisory services and assistance to Federal agencies; and provides the technical foundation for computer-related policies of the Federal Government. The Institute consists of the following centers:

Programming Science and Technology — Computer Systems Engineering.


¹Headquarters and Laboratories at Gaithersburg, MD, unless otherwise noted; mailing address Washington, DC 20234.

²Some divisions within the center are located at Boulder, CO 80303.

A Programmable Sample Dryer for Thermal Ionization Mass Spectrometry

John W. Gramlich and Ronald W. Shideler

Center for Analytical Chemistry
National Measurement Laboratory
National Bureau of Standards
Washington, DC 20234



U.S. DEPARTMENT OF COMMERCE, Malcolm Baldrige, Secretary
NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Director

Issued January 1982

National Bureau of Standards Technical Note 1154

Nat. Bur. Stand. (U.S.), Tech. Note 1154, 19 pages (Jan. 1982)

CODEN: NBTNAE

U.S. GOVERNMENT PRINTING OFFICE
WASHINGTON: 1982

TABLE OF CONTENTS

	<u>PAGE</u>
1. Introduction	1
2. Electronic Circuit Operation	2
3. Construction	7
4. Calibration and Operation.	7
5. References	13

LIST OF FIGURES

<u>FIGURE NO.</u>	<u>PAGE</u>
1. Digital programming section schematic.	3
2. Analogue constant current section schematic.	4
3. Personality card PC layout	5
4. Schematic, layout, and parts list for alarm.	6
5. PC board for alarm	7
6. Chassis layout and parts list.	8
7. Main PC board (front).	9
8. Main PC board (back)	10
9. Main circuit board layout and parts list	11
10. Sample dryer	12
11. Time <u>vs.</u> resistance calibration plot	14
12. Current <u>vs.</u> resistance calibration plot.	15

John W. Gramlich and Ronald W. Shideler

Center for Analytical Chemistry
National Measurement Laboratory
National Bureau of Standards
Washington, DC 20234

A sample dryer has been designed which allows reproducible and automatic filament current and timing adjustments for up to five separate steps. Designed around inexpensive TTL logic, the dryer may be programmed by resistors on a plug-in card to provide the proper drying conditions, be programmed to stop and signal the operator after any step, or be allowed to continue uninterrupted through the entire drying sequence. A programmable 110 volt output is provided for controlling a heat lamp or other accessory.

Key words: isotopic analysis; isotopic fractionation; sample dryer; thermal ionization mass spectrometry.

1. Introduction

Samples for isotope ratio measurements by thermal ionization mass spectrometry are usually dried on a filament from a solution of a soluble salt before insertion into the mass spectrometer. Frequently, the drying procedure entails a sequence of drying times and temperatures. As in the case of the analysis of lead, zinc, and cadmium by the silica gel method [1,2], it may be necessary to add additional reagents to the filament at preset intervals during the drying procedure.

The process of thermally ionizing an element from a hot filament causes a mass dependent fractionation of the isotopic ratios. The rate and magnitude of the isotopic fractionation is dependent, at least in part, upon the chemical species present on the filament, and in the case of a multiple filament ion source, the molecular species resulting from vaporization of the sample from the filament. The theoretical and empirical aspects of the isotopic fractionation problem have been covered in some detail by Moore et al., [3]. The chemical species formed by drying a sample on a filament can be quite complex. For example, it has been shown that calcium nitrate, in a dilute nitric acid solution, produces a mixture of calcium rhenates when dried on a rhenium filament [3]. These species include Ca_2ReO_4 , $\text{Ca}_3\text{Re}_2\text{O}_9$, $\text{Ca}_6\text{Re}_2\text{O}_{11}$, and $\text{Ca}_5\text{Re}_2\text{O}_{12}$.

Obtaining precise and accurate mass spectrometric isotope ratio measurements requires that all samples (standards and unknowns) show the same rate and degree of isotopic fractionation during the analysis. Only if this condition is met, can unknown samples be compared with the standards and corrected to absolute isotopic ratios, in those cases where standards of known absolute isotopic composition are available. This condition of comparable isotopic

fractionation can be met only if the standards and unknowns are in the same chemical form on the filament.

It has been generally accepted for some time that variations in the drying procedure between sample loadings can decrease the accuracy of mass spectrometric isotope ratio measurements, and most laboratories engaged in this type of analysis make some attempt to reproduce the sample loading procedure. However, the magnitude of the errors that can result from sample loading variations is not fully appreciated. Uranium isotopic ratios, for example, can be shifted by as much as 0.25 percent by small filament temperature differences during the sample loading. Errors of this magnitude are unacceptable for use in the accountability and safeguarding of nuclear materials. Recent work in this laboratory [4,5] has indicated that "state-of-the-art" isotope ratio measurements (i.e., 0.01 percent or less uncertainty) for some elements require extremely close tolerances on sample drying parameters. Such reproducibility is difficult, if not impossible, to achieve manually.

The potential for errors attributable to sample loading variations is especially great in high volume laboratories where several analysts, often working in shifts, may each analyze parts of a suite of samples. The inter-analyst data may show systematic biases, in addition to the random and intra-analyst variations. Automated sample drying can substantially reduce these systematic biases, as well as minimize the variations inherent in manual control of current settings and drying times.

The sample dryer, described herein, has been in operation on a daily basis in the mass spectrometry laboratory, Inorganic Analytical Research Division, for the past 4 years. Five such units are currently in operation and have proven to be extremely trouble free and reproducible. They have contributed, not only to improved accuracy and precision, but also to increased sample analysis output.

2. Electronic Circuit Operation

The electronic circuitry is comprised of a digital programming section (figure 1) and an analogue constant filament power supply (figure 2). The digital programmer selects the proper current circuit, as well as the duration of the time interval for each current selected.

The digital programmer is made up of a single BCD counter (U6) with its output state indicated by a seven segment LED. The output is also decoded by a one-of-ten decoder (U5) which selects one of the five timed, current active states or one of the four halt states. Programming is accomplished by means of a personality card (22 pin PC card, figure 3) with jumpers, timing resistors, and current control resistors selected, to provide parameters tailored to the particular element being dried on the sample filament. The state selected is routed by the personality card to produce the desired functions. A halt state can be jumpered to allow continuation to the next current active state, or when left open, sound an alarm and interrupt the filament current. Resumption of operation, at the next current active state, occurs when the operator presses the start-continue button. When a current active state is selected, one resistor is used to establish the filament

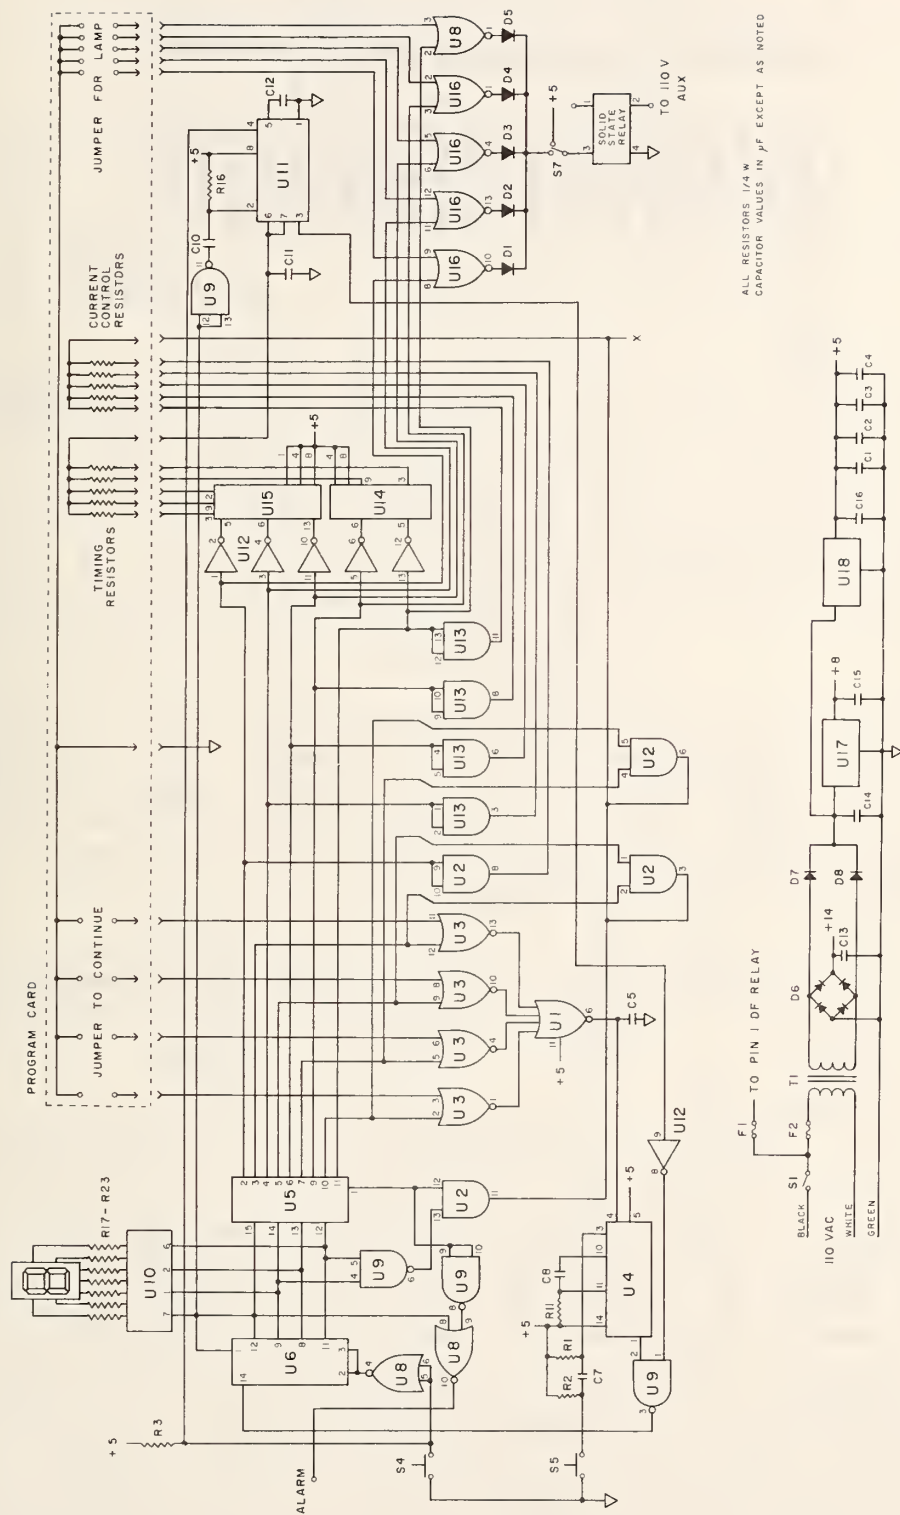


Figure 1. Digital programming section schematic.

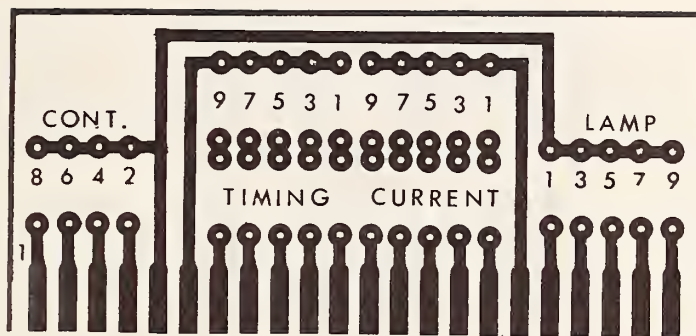


Figure 3. Personality Card PC layout.

current, while another resistor determines the time interval. The timing resistors are individually connected to a +5 V source through an analogue switch (U15, U16) to become the pull-up resistor of the 555 one-shot circuit (U11). The output of the one shot returns to the state counter, advancing the state at the one-shot's time out. During the time interval defined for a given state, the filament current is set by the current control resistor selected. Each current control resistor is connected as one element of a voltage divider and is selected by means of one of five open collector TTL gates (U13, U2) when the selected output goes active low. The voltage level established determines the filament set current.


Halt states are provided between each active state and are bypassed by appropriate jumpers. When the halt state is entered, the signal is logically enabled by the presence of a jumper through one of the four gates (U3). The output is collected through an or-gate (U1) and used to trigger the start-continue one shot (U4), which immediately advances the state counter. This one shot is also activated by the start-continue push button.

The final aspect of the digital circuitry provides an auxiliary 110-Vac output activated at any active state desired and selected by a jumper. One or more jumpers enable the gates (U8, U16), which operate the solid state relay when the selected state signal is present.

The analogue section of this device supplies a programmed constant current to the filament being dried. The current that is supplied is proportional to the voltage determined by the resistor on the personality card. This voltage is applied to the non-inverting input of the operational amplifier (U7). The output of the operational amplifier drives transistor Q1, whose output, in turn, drives transistors Q2 and Q3 as a double emitter follower or "Darlington circuit". The emitter outputs of Q2 and Q3 supply current to the filament which is connected to ground through the current metering resistors R24 and R25. The voltage developed across the metering resistors is returned to the inverting input of the operational amplifier to complete the negative feedback loop. In this configuration, the operational amplifier maintains its output voltage at the level necessary to drive the output transistors to source a current through the sample filament and metering resistors, providing a feedback voltage developed across the metering resistors that exactly matches the programmed input voltage. Components R12, R5, and C9 are used to insure stability of the circuit under various load and voltage conditions.

Power is supplied to this system by a transformer input and diode bridge rectifier circuit. Unregulated power is used for the filament source current. A regulated +5 volt source (U18) supplies power to the TTL logic, and a regulated +8 volts (U17) is used to drive the operational amplifier.

The alarm signal output from the main circuit board provides a continuous high output from the U8 gate. This can be fed into an alarm circuit (figure 4) to provide a one shot signal of a fixed duration. The length of the audible signal can be adjusted by varying the value of R33 or C21. The RC time constant of R30 and C18 is sufficient to prevent triggering of the 555 one shot (U11) when the unit advances automatically to the next active state. The alarm circuit board (figure 5) is designed to mount directly on the terminals of the signal device.

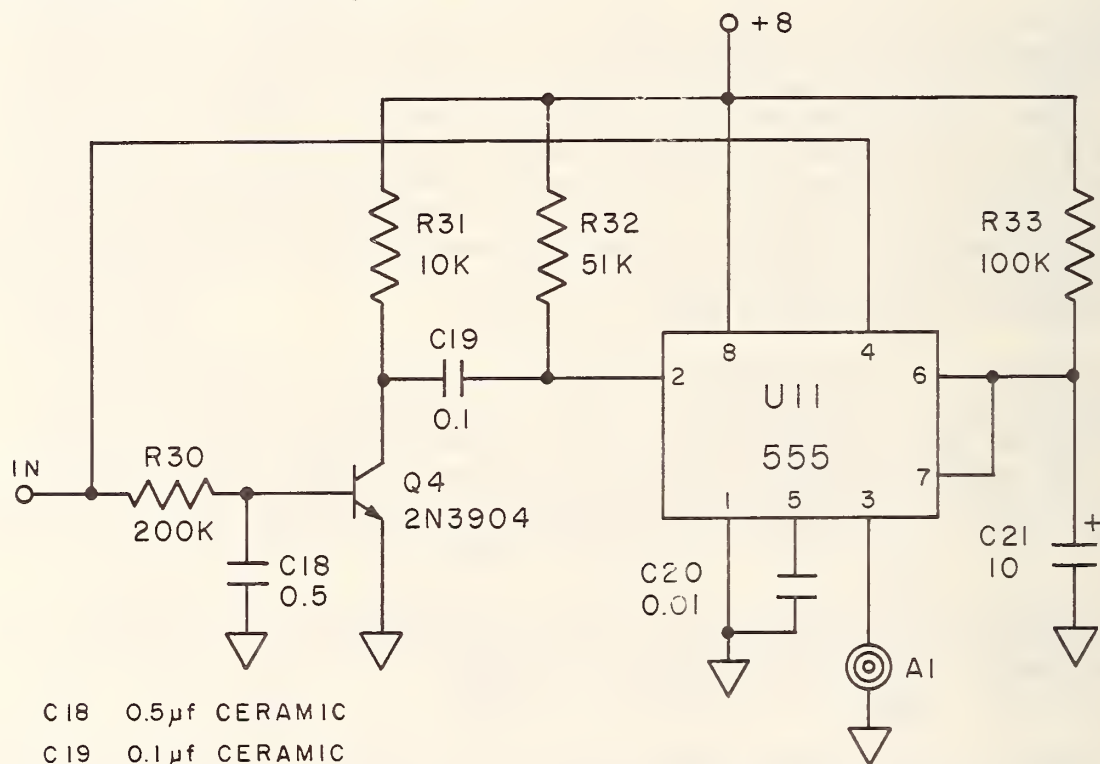

- C18 0.5µf CERAMIC
- C19 0.1µf CERAMIC
- C20 0.01µf CERAMIC
- C21 10µf ELECTROLYTIC
- R30 200 K
- R31 10 K
- R32 51 K
- R33 100 K
- Q4 2N3904
- U11 555 TIMER
- A1 ELECTRONIC SIGNAL DEVICE, 2900 Hz

ALL RESISTORS 1/4W TIN OXIDE

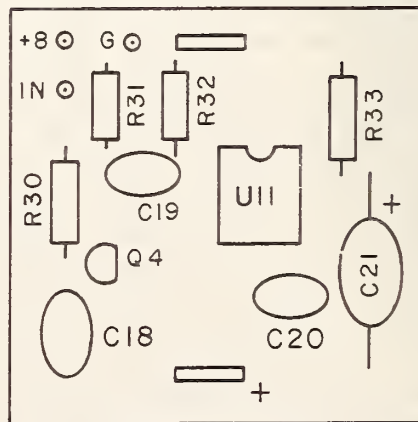


Figure 4. Schematic, layout, and parts list for alarm.

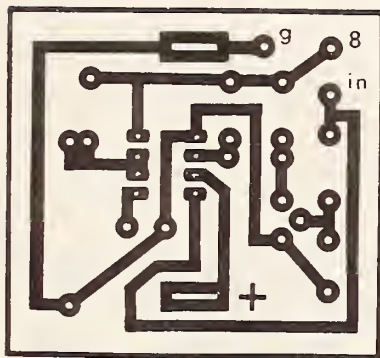


Figure 5. PC board for alarm.


3. Construction

The sample dryer can be contained in an inverted 12" x 7" x 3" aluminum chassis box. The power supplies, controls, and high current components are mounted on the chassis box (figure 6), while the remainder of the circuitry is mounted on the main PC board (figures 7, and 8). The component layout for the main circuit board is given in figure 9. The main circuit board is mounted on the side and near the top of the chassis, and is attached by means of a 22-contact edge card receptacle soldered to the board. Connections between the main circuit board and the chassis-mounted components are provided through a 16-pin DIP socket, allowing for easy removal of the board. Ground and +5 volt supply voltage to the TTL logic are provided through screw terminals on the board. The manual current control (R28), filament sockets, and heat lamp assembly are attached to a 12" x 7" x 1/8" aluminum plate mounted on the chassis with 1/2" standoffs. Figure 10 shows the positioning of these components. The standoffs provide for air circulation under the plate to minimize the heating of the electronics by the lamp. The chassis-mounted phone jack allows monitoring of the voltage across R24-R25, which is numerically equal to one-half of the current through the filaments. Switch S7, mounted on the back of the chassis, allows operation of the 110-Vac auxiliary output without entering one of the current active states.

4. Calibration and Operation

Offset voltage nulling of the operational amplifier (U7) is accomplished with a 100 K Ω variable resistance (R13-R15), connected across terminals 1 and 5, with the potentiometer slider arm connected to ground. The offset voltage should be set to produce zero current at the filament when the dryer is in a halt state.

If more than one sample dryer is in operation in a laboratory, it may be desirable to have interchangeability of the personality cards among the units. Potentiometer R6 can be used to adjust the voltage divider output to the noninverting input of the operational amplifier to compensate for small differences in the output voltage of the +5 volt regulators (U18) in the different units. Through adjustment of R6, the five sample dryers in this laboratory produce the same current (over the range of 0-2 A) to within 0.2

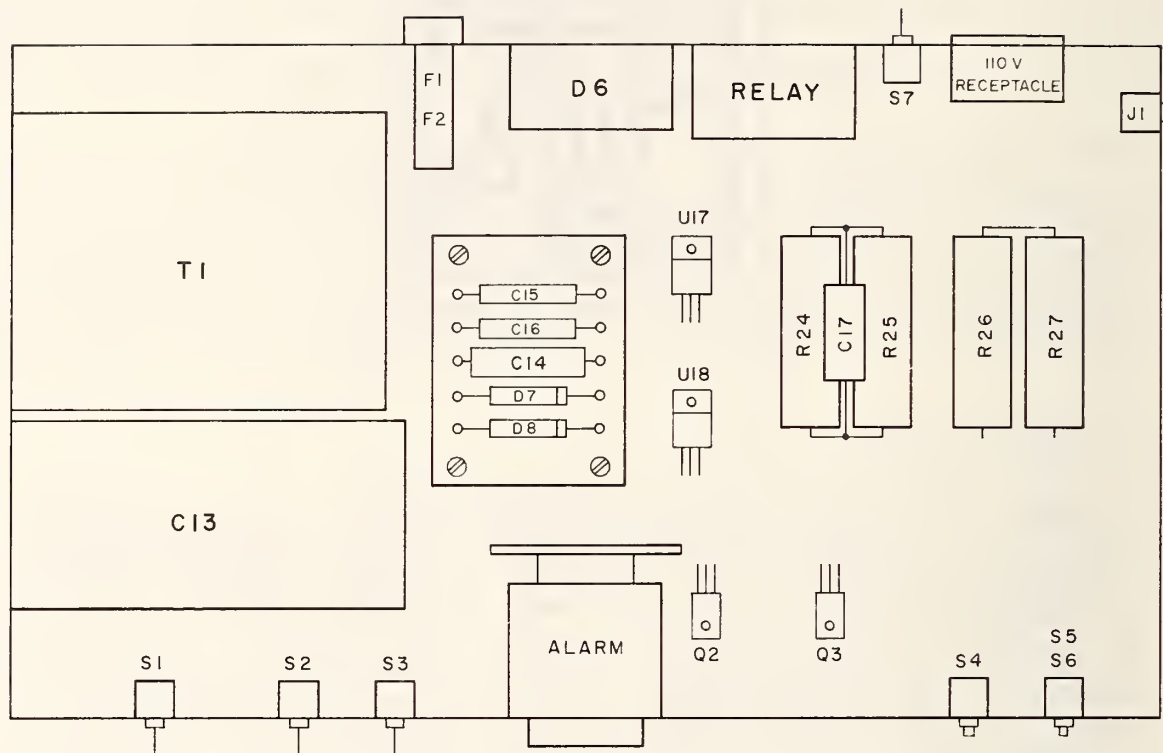

ACTIVE COMPONENTS

U17	7808
U18	7805
Q2, Q3	2N5191
D6	10A BRIDGE RECTIFIER
D7, D8	1N 4001
RELAY	PHOTO ISOLATED SOLID STATE RELAY, 110 VAC 10 A 3-32 VDC CONTROL SIGNAL

PASSIVE COMPONENTS

C13	14000 μ F ELECTROLYTIC
C14	2000 μ F ELECTROLYTIC
C15, C16	0.5 μ F
C17	100 μ F
R24-R27	1 Ω 25W
S1-S3, S6	DPDT 5A MIN. TOGGLE
S7	SPDT 5A MIN. TOGGLE
S4, S5	SPST PUSHBUTTON, N.O.
T1	TRANSFORMER, 10V 8A
J1	MIN. PHONE JACK, N.O.
F1	2.5A SLO-BLO FUSE
F2	1A FUSE
110V REC.	3 WIRE FEMALE POWER LINE CONNECTOR

Figure 6. Chassis layout and parts list.

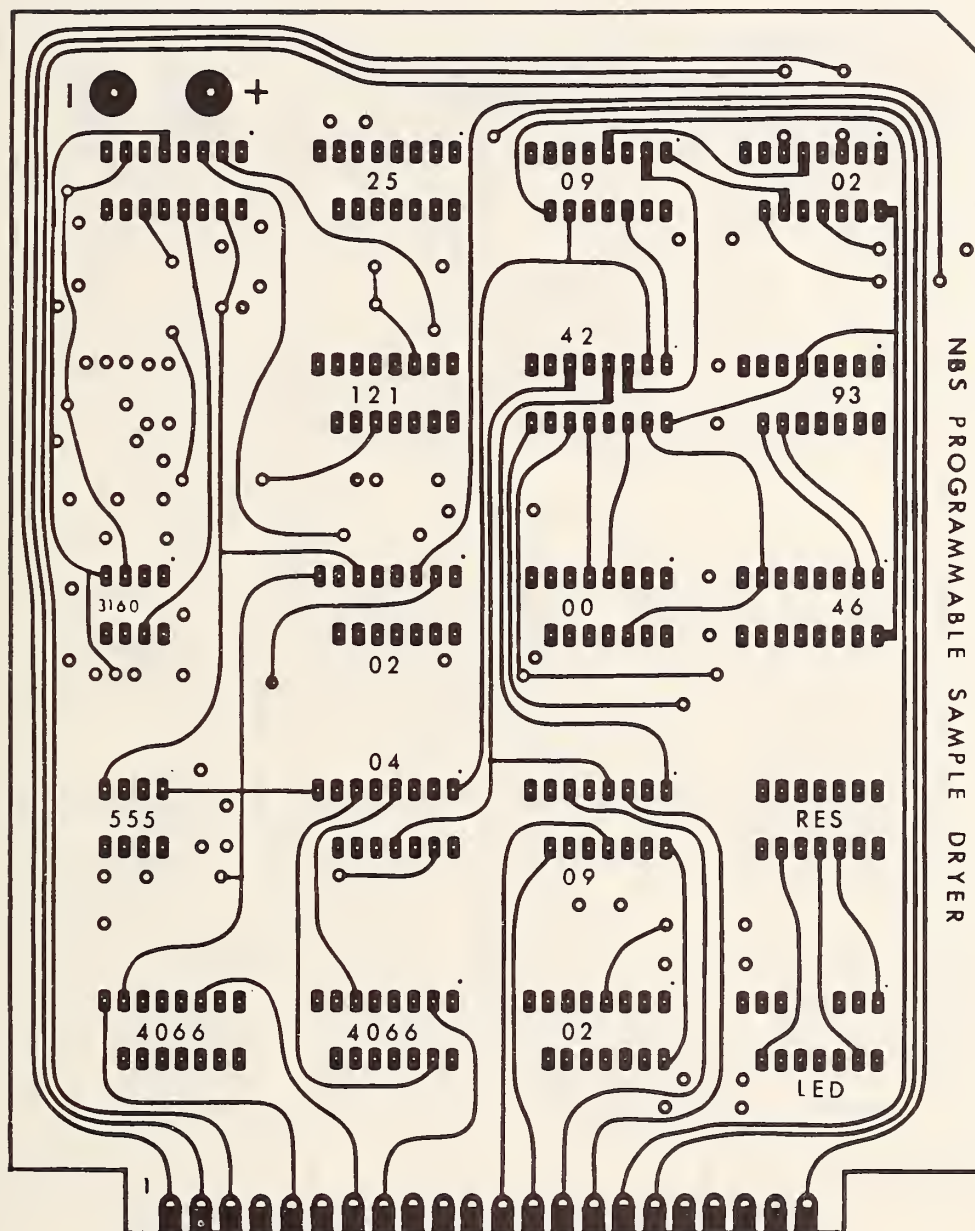


Figure 7. Main PC board (front).


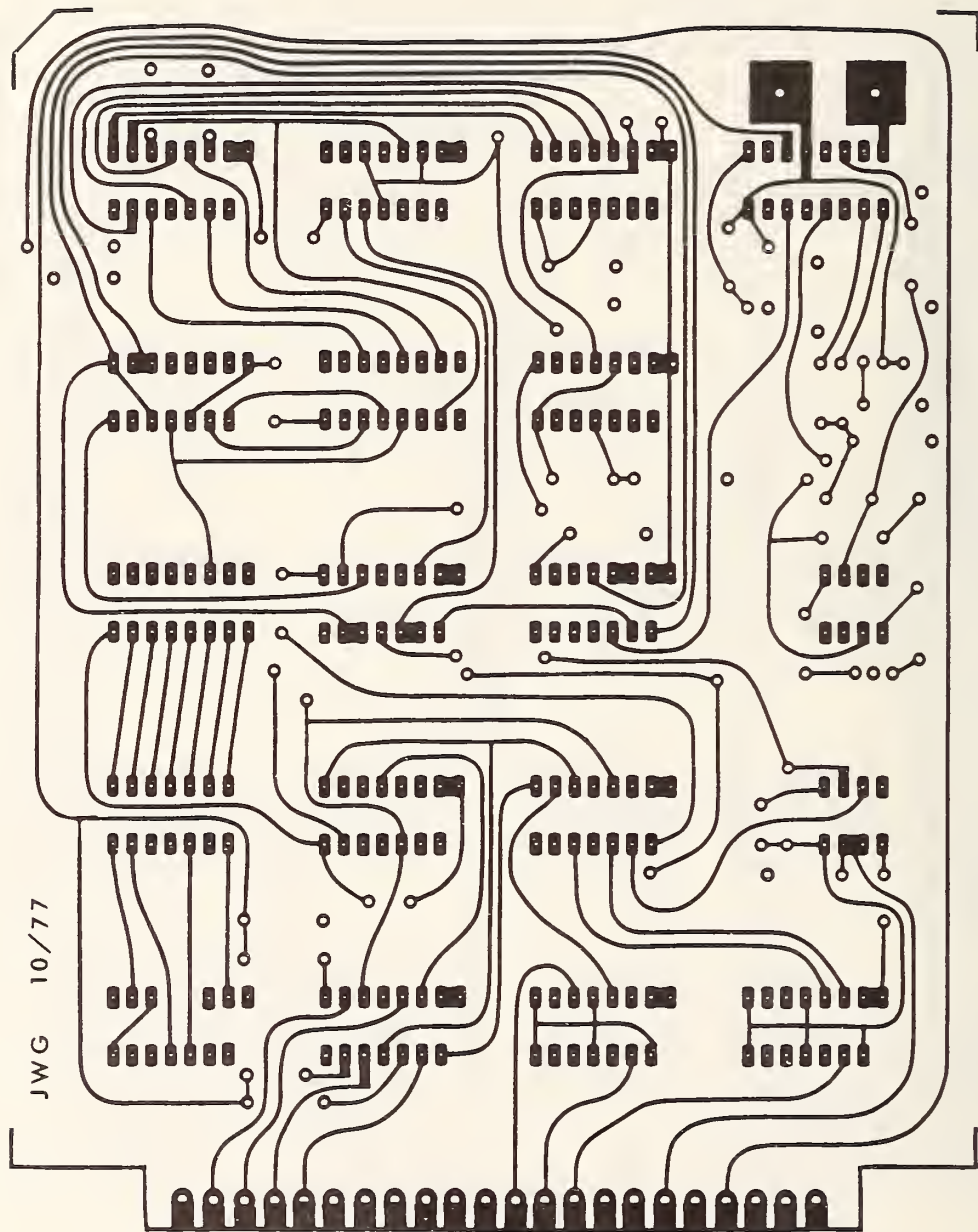


Figure 8. Main PC board (back).

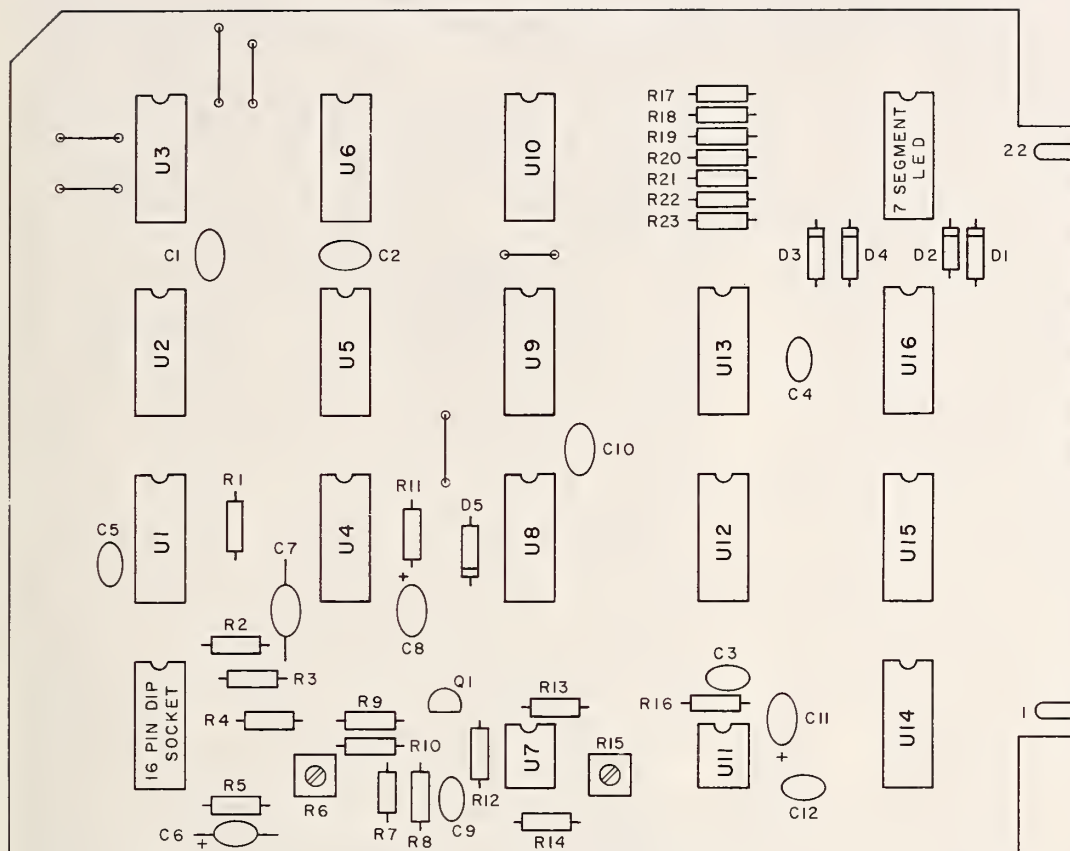

ACTIVE COMPONENTS

U1	7425
U2,U13	7409
U3,U8,U16	7402
U4	74121
U5	7442
U6	7493
U7	CA3160
U9	7400
U10	7447
U11	555
U12	7447
U14,U15	CD4066
D1-D5	1N270
Q1	2N2222

PASSIVE COMPONENTS

C1-C4,C9	0.1 μ F CERAMIC
C5	50 pF CERAMIC
C6,C8	1 μ F TANTALUM
C7	0.05 μ F
C10	1000 pF SILVER MICA
C11	100 μ F TANTALUM
C12	0.01 μ F CERAMIC
R1,R3,R5,R16	10 K
R2	500 K
R4,R8,R12	1 K
R6,R15	2 K SINGLE TURN
R7	9.1 K
R9,R10	30
R11	39 K
R13+R14	98 K TOTAL
R17-R23	270

ALL RESISTORS 1/4 W TIN OXIDE

Figure 9. Main circuit board layout and parts list.

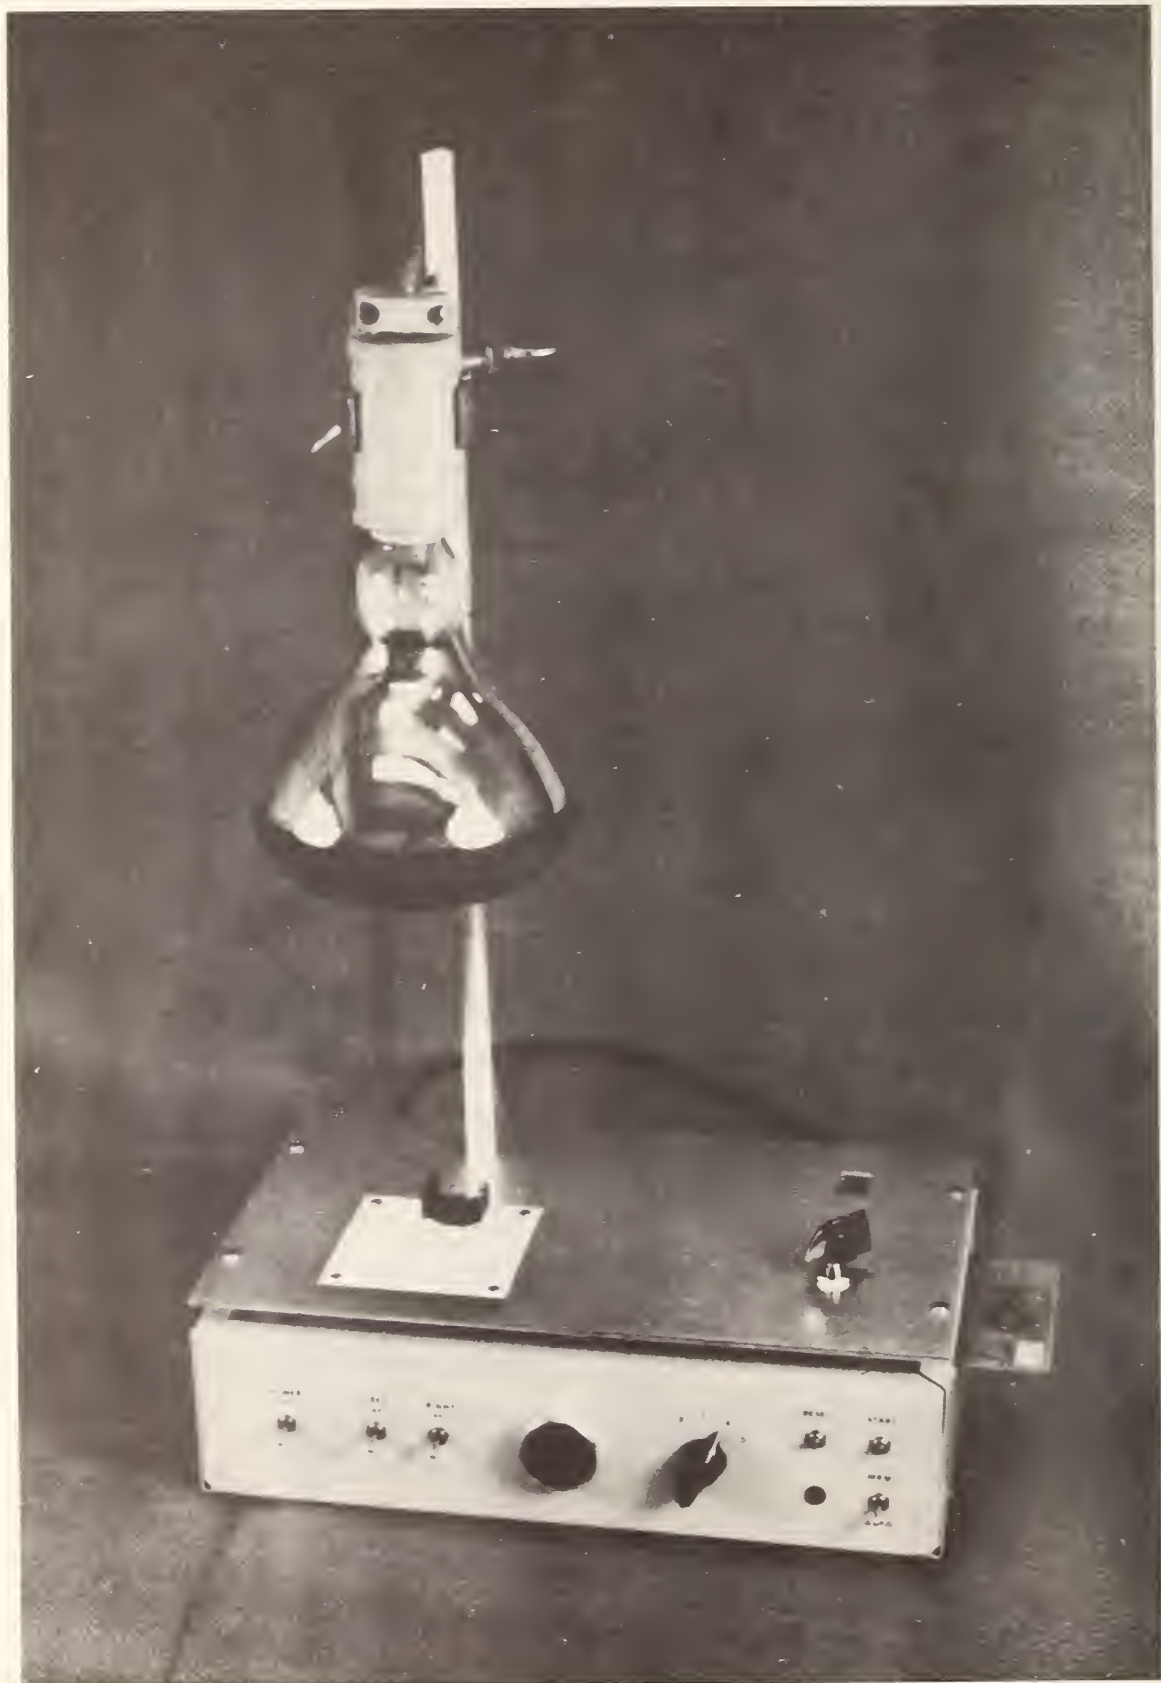


Figure 10. Sample dryer.

percent from the same personality card. For multiple units, it is also necessary to match the timing capacitor (C11) of the 555 one shot to achieve personality card interchangeability.

The relationship between the values of the timing resistors and the time of the current active states is given in figure 11. The similar relationship between the values of the current control resistors and the filament currents is given in figure 12. For the most accurate settings, the dryer should be calibrated with resistors of known value, rather than relying on figures 11 and 12.

Although the 110-Vac programmable output is most frequently used to control a heat lamp used to aid the drying process, it can also be used to control external temperature sensing instrumentation. One unit in this laboratory is interfaced to a digital remote sensing infrared thermometer, capable of monitoring the filament temperature in the range of 400 °C to 1650 °C. For filament drying temperatures above 400 °C, the programmed 110-Vac output allows the infrared thermometer to control the filament current by means of an output control signal, proportional to the difference between the filament temperature and a preset temperature. Timing of the high temperature drying is still controlled by the personality card timing resistor for the particular current active state.

5. References

- [1] Barnes, I. L.; Murphy, T. J.; Gramlich, J. W.; Shields, W. R. Lead Separation by Anodic Deposition and Isotope Ratio Mass Spectrometry of Microgram and Smaller Samples. *Anal. Chem.* 45: 1881-1884; 1973.
- [2] Gramlich, J. W.; Machlan, L. A.; Murphy, T. J.; Moore, L. J. The Determination of Zinc, Cadmium, and Lead in Biological and Environmental Materials by Isotope Dilution Mass Spectrometry, in Trace Substances in Environmental Health-XI, D. D. Hemphill, ed. University of Missouri, Columbia; 1977. 376-380.
- [3] Moore, L. J.; Heald, E. F.; Filliben, J. J. An Isotopic Fractionation Model for the Multiple Filament Thermal Ion Source. *Advances in Mass Spectrometry* 7: 448-474; 1978.
- [4] Dunstan, L. P.; Gramlich, J. W.; Barnes, I. L.; Purdy, W. C. Absolute Isotopic Abundance and the Atomic Weight of a Reference Sample of Thallium. *J. Res. Nat. Bur. Stand. (U.S.)*. 85: 1-10; 1980.
- [5] Powell, L. J.; Murphy, T. J.; Gramlich, J. W. The Absolute Isotopic Abundance and Atomic Weight of a Reference Sample of Silver. *J. Res. Nat. Bur. Stand. (U.S.)*. Jan.-Feb. 1982.

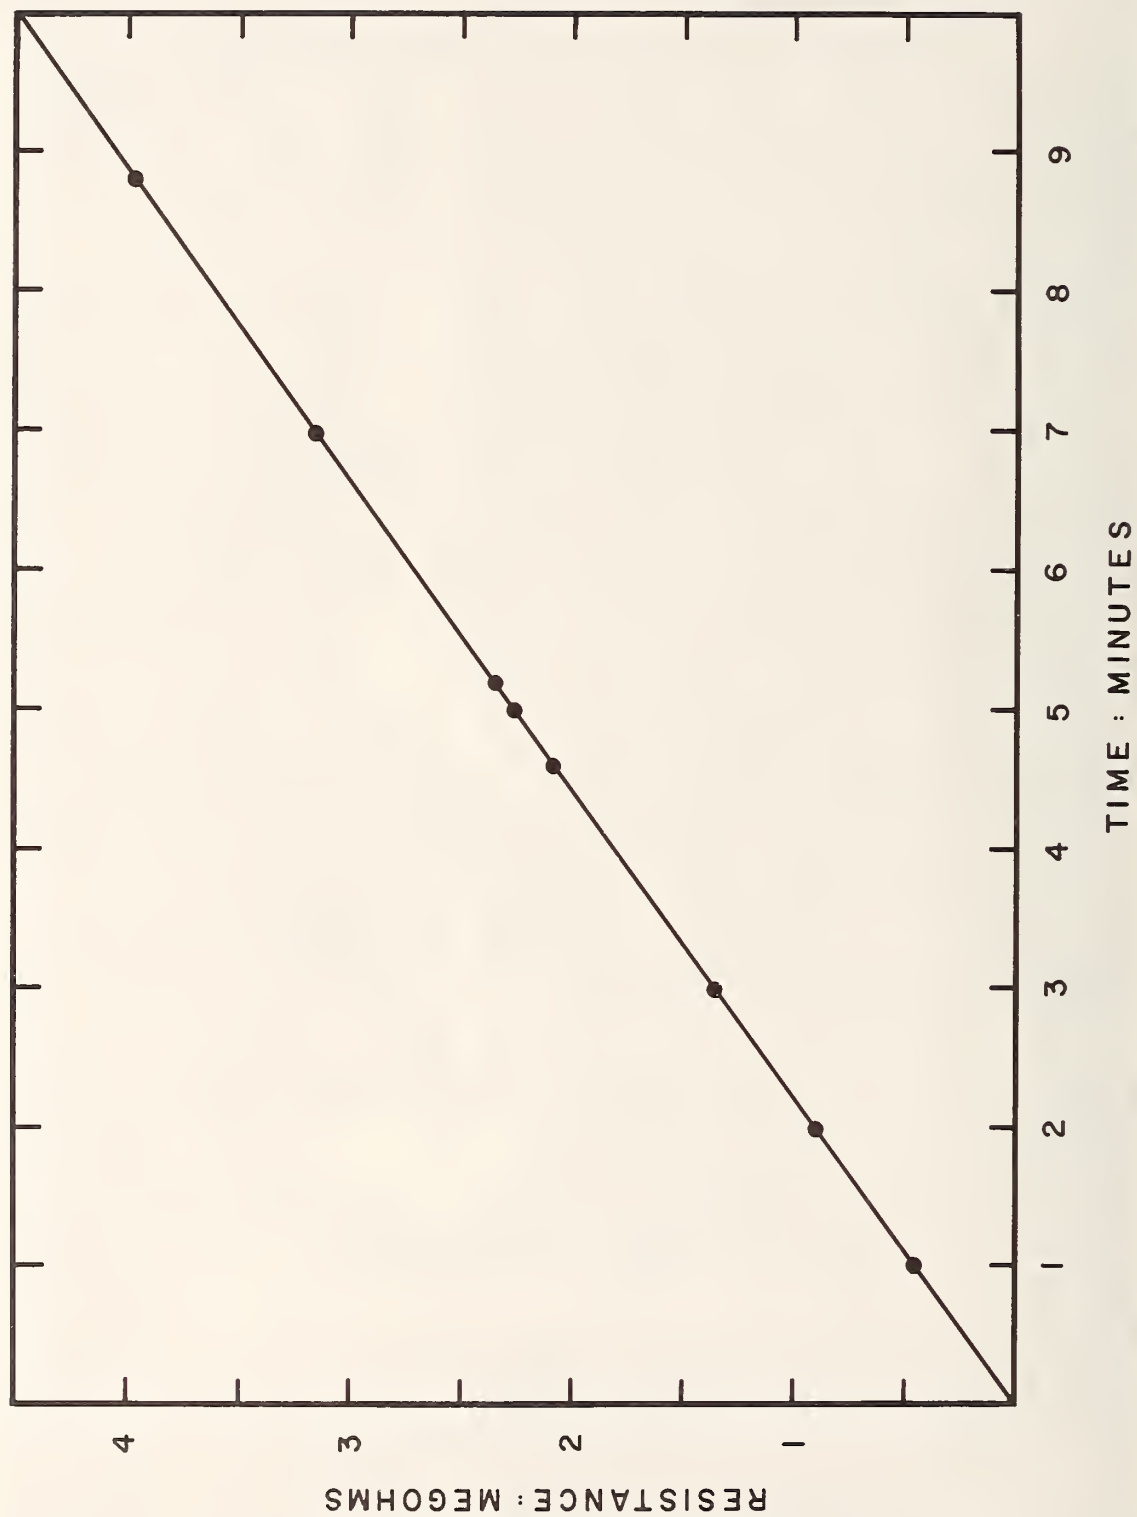


Figure 11. Time vs. resistance calibration plot.

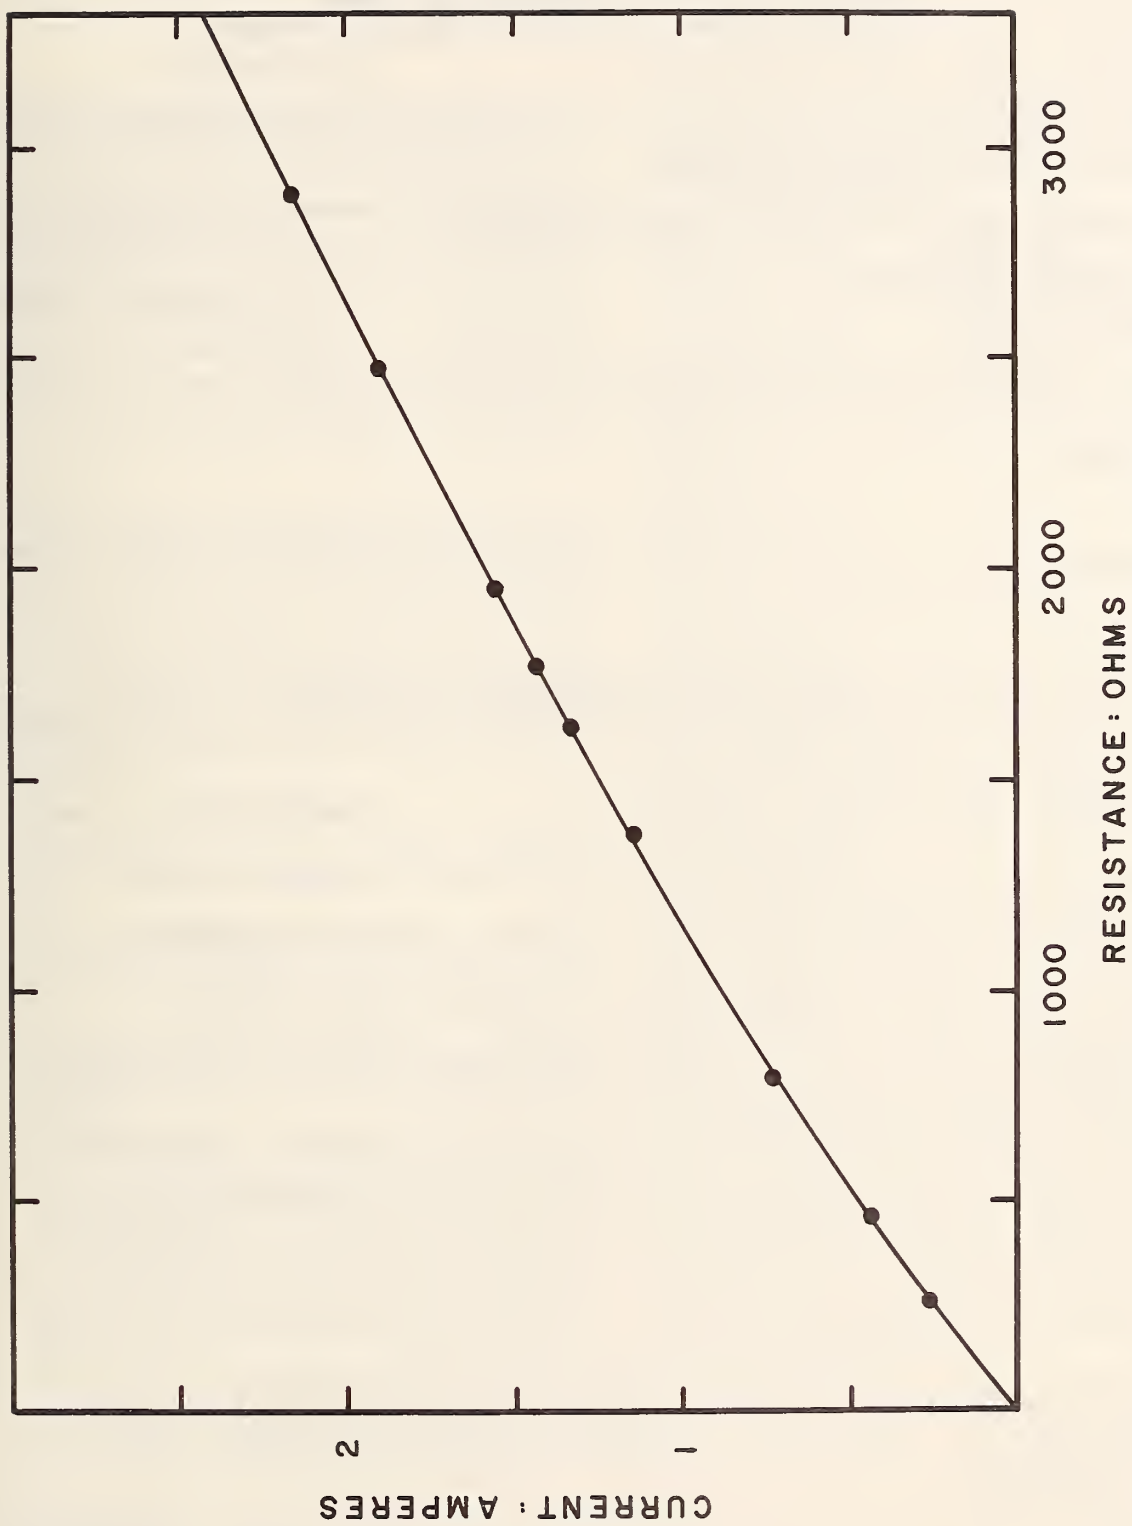


Figure 12. Current vs. resistance calibration plot.

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET <i>(See instructions)</i>	1. PUBLICATION OR REPORT NO. NBS TN 1154	2. Performing Organ. Report No.	3. Publication Date January 1982
4. TITLE AND SUBTITLE A Programmable Sample Dryer for Thermal Ionization Mass Spectrometry			
5. AUTHOR(S) John W. Gramlich and Ronald W. Shideler			
6. PERFORMING ORGANIZATION <i>(If joint or other than NBS, see instructions)</i> NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		7. Contract/Grant No.	8. Type of Report & Period Covered Final
9. SPONSORING ORGANIZATION NAME AND COMPLETE ADDRESS <i>(Street, City, State, ZIP)</i> Same as above.			
10. SUPPLEMENTARY NOTES <input type="checkbox"/> Document describes a computer program; SF-185, FIPS Software Summary, is attached.			
11. ABSTRACT <i>(A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here)</i> A sample dryer has been designed which allows reproducible and automatic filament current and timing adjustments for up to five separate steps. Designed around inexpensive TTL logic, the dryer may be programmed by resistors on a plug-in card to provide the proper drying conditions, be programmed to stop and signal the operator after any step, or be allowed to continue uninterrupted through the entire drying sequence. A programmable 110 volt output is provided for controlling a heat lamp or other accessory.			
12. KEY WORDS <i>(Six to twelve entries; alphabetical order; capitalize only proper names; and separate key words by semicolons)</i> isotopic analysis; isotopic fractionation; sample dryer; thermal ionization mass spectrometry.			
13. AVAILABILITY <input checked="" type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input type="checkbox"/> Order From Superintendent of Documents, U.S. Government Printing Office, Washington, D C 20402. <input checked="" type="checkbox"/> Order From National Technical Information Service (NTIS), Springfield, VA 22161			14. NO. OF PRINTED PAGES 19 15. Price

NBS TECHNICAL PUBLICATIONS

PERIODICALS

JOURNAL OF RESEARCH—The Journal of Research of the National Bureau of Standards reports NBS research and development in those disciplines of the physical and engineering sciences in which the Bureau is active. (These include physics, chemistry, engineering, mathematics, and computer sciences. Papers cover a broad range of subjects, with major emphasis on measurement methodology and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Bureau's technical and scientific programs. As a special service to subscribers each issue contains complete citations to all recent Bureau publications in both NBS and non-NBS media. Issued six times a year. Annual subscription: domestic \$18; foreign \$22.50. Single copy \$4.25 domestic; \$5.35 foreign.

NOTE: The Journal was formerly published in two sections: Section A "Physics and Chemistry" and Section B "Mathematical Sciences."

DIMENSIONS/NBS—This monthly magazine is published to inform scientists, engineers, business and industry leaders, teachers, students, and consumers of the latest advances in science and technology, with primary emphasis on work at NBS. The magazine highlights and reviews such issues as energy research, fire protection, building technology, metric conversion, pollution abatement, health and safety, and consumer product performance. In addition, it reports the results of Bureau programs in measurement standards and techniques, properties of matter and materials, engineering standards and services, instrumentation, and automatic data processing. Annual subscription: domestic \$11; foreign \$13.75.

NONPERIODICALS

Monographs—Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

Handbooks—Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

Special Publications—Include proceedings of conferences sponsored by NBS, NBS annual reports, and other special publications appropriate to this grouping such as wall charts, pocket cards, and bibliographies.

Applied Mathematics Series—Mathematical tables, manuals, and studies of special interest to physicists, engineers, chemists, biologists, mathematicians, computer programmers, and others engaged in scientific and technical work.

National Standard Reference Data Series—Provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated. Developed under a worldwide program coordinated by NBS under the authority of the National Standard Data Act (Public Law 90-396).

NOTE: The principal publication outlet for the foregoing data is the Journal of Physical and Chemical Reference Data (JPCRD) published quarterly for NBS by the American Chemical Society (ACS) and the American Institute of Physics (AIP). Subscriptions, reprints, and supplements available from ACS, 1155 Sixteenth St., NW, Washington, DC 20056.

Building Science Series—Disseminates technical information developed at the Bureau on building materials, components, systems, and whole structures. The series presents research results, test methods, and performance criteria related to the structural and environmental functions and the durability and safety characteristics of building elements and systems.

Technical Notes—Studies or reports which are complete in themselves but restrictive in their treatment of a subject. Analogous to monographs but not so comprehensive in scope or definitive in treatment of the subject area. Often serve as a vehicle for final reports of work performed at NBS under the sponsorship of other government agencies.

Voluntary Product Standards—Developed under procedures published by the Department of Commerce in Part 10, Title 15, of the Code of Federal Regulations. The standards establish nationally recognized requirements for products, and provide all concerned interests with a basis for common understanding of the characteristics of the products. NBS administers this program as a supplement to the activities of the private sector standardizing organizations.

Consumer Information Series—Practical information, based on NBS research and experience, covering areas of interest to the consumer. Easily understandable language and illustrations provide useful background knowledge for shopping in today's technological marketplace.

Order the above NBS publications from: Superintendent of Documents, Government Printing Office, Washington, DC 20402.

Order the following NBS publications—FIPS and NBSIR's—from the National Technical Information Services, Springfield, VA 22161.

Federal Information Processing Standards Publications (FIPS PUB)—Publications in this series collectively constitute the Federal Information Processing Standards Register. The Register serves as the official source of information in the Federal Government regarding standards issued by NBS pursuant to the Federal Property and Administrative Services Act of 1949 as amended, Public Law 89-306 (79 Stat. 1127), and as implemented by Executive Order 11717 (38 FR 12315, dated May 11, 1973) and Part 6 of Title 15 CFR (Code of Federal Regulations).

NBS Interagency Reports (NBSIR)—A special series of interim or final reports on work performed by NBS for outside sponsors (both government and non-government). In general, initial distribution is handled by the sponsor; public distribution is by the National Technical Information Services, Springfield, VA 22161, in paper copy or microfiche form.

U.S. DEPARTMENT OF COMMERCE
National Bureau of Standards
Washington, DC 20234

POSTAGE AND FEES PAID
U.S. DEPARTMENT OF COMMERCE
COM-215



OFFICIAL BUSINESS

Penalty for Private Use, \$300

FIRST CLASS
