

E-01 Admin. Bldg.  
UL 3 0 1969



# TECHNICAL NOTE


NATIONAL BUREAU  
OF STANDARDS  
LIBRARY

MAR 6 1973

711702

373

## Radio-Frequency Measurements in the NBS Institute for Basic Standards



U.S. DEPARTMENT OF COMMERCE  
National Bureau of Standards

## NATIONAL BUREAU OF STANDARDS

The National Bureau of Standards<sup>1</sup> was established by an act of Congress March 3, 1901. Today, in addition to serving as the Nation's central measurement laboratory, the Bureau is a principal focal point in the Federal Government for assuring maximum application of the physical and engineering sciences to the advancement of technology in industry and commerce. To this end the Bureau conducts research and provides central national services in four broad program areas. These are: (1) basic measurements and standards, (2) materials measurements and standards, (3) technological measurements and standards, and (4) transfer of technology.

The Bureau comprises the Institute for Basic Standards, the Institute for Materials Research, the Institute for Applied Technology, the Center for Radiation Research, the Center for Computer Sciences and Technology, and the Office for Information Programs.

**THE INSTITUTE FOR BASIC STANDARDS** provides the central basis within the United States of a complete and consistent system of physical measurement; coordinates that system with measurement systems of other nations; and furnishes essential services leading to accurate and uniform physical measurements throughout the Nation's scientific community, industry, and commerce. The Institute consists of an Office of Measurement Services and the following technical divisions:

Applied Mathematics—Electricity—Metrology—Mechanics—Heat—Atomic and Molecular Physics—Radio Physics<sup>2</sup>—Radio Engineering<sup>2</sup>—Time and Frequency<sup>2</sup>—Astrophysics<sup>2</sup>—Cryogenics.<sup>2</sup>

**THE INSTITUTE FOR MATERIALS RESEARCH** conducts materials research leading to improved methods of measurement standards, and data on the properties of well-characterized materials needed by industry, commerce, educational institutions, and Government; develops, produces, and distributes standard reference materials; relates the physical and chemical properties of materials to their behavior and their interaction with their environments; and provides advisory and research services to other Government agencies. The Institute consists of an Office of Standard Reference Materials and the following divisions:

Analytical Chemistry—Polymers—Metallurgy—Inorganic Materials—Physical Chemistry.

**THE INSTITUTE FOR APPLIED TECHNOLOGY** provides technical services to promote the use of available technology and to facilitate technological innovation in industry and Government; cooperates with public and private organizations in the development of technological standards, and test methodologies; and provides advisory and research services for Federal, state, and local government agencies. The Institute consists of the following technical divisions and offices:

Engineering Standards—Weights and Measures—Invention and Innovation—Vehicle Systems Research—Product Evaluation—Building Research—Instrument Shops—Measurement Engineering—Electronic Technology—Technical Analysis.

**THE CENTER FOR RADIATION RESEARCH** engages in research, measurement, and application of radiation to the solution of Bureau mission problems and the problems of other agencies and institutions. The Center consists of the following divisions:

Reactor Radiation—Linac Radiation—Nuclear Radiation—Applied Radiation.

**THE CENTER FOR COMPUTER SCIENCES AND TECHNOLOGY** conducts research and provides technical services designed to aid Government agencies in the selection, acquisition, and effective use of automatic data processing equipment; and serves as the principal focus for the development of Federal standards for automatic data processing equipment, techniques, and computer languages. The Center consists of the following offices and divisions:

Information Processing Standards—Computer Information—Computer Services—Systems Development—Information Processing Technology.

**THE OFFICE FOR INFORMATION PROGRAMS** promotes optimum dissemination and accessibility of scientific information generated within NBS and other agencies of the Federal government; promotes the development of the National Standard Reference Data System and a system of information analysis centers dealing with the broader aspects of the National Measurement System, and provides appropriate services to ensure that the NBS staff has optimum accessibility to the scientific information of the world. The Office consists of the following organizational units:

Office of Standard Reference Data—Clearinghouse for Federal Scientific and Technical Information—Office of Technical Information and Publications—Library—Office of Public Information—Office of International Relations.

<sup>1</sup> Headquarters and Laboratories at Gaithersburg, Maryland, unless otherwise noted; mailing address Washington, D.C. 20234.

<sup>2</sup> Located at Boulder, Colorado 80302.

<sup>3</sup> Located at 5255 Port Royal Road, Springfield, Virginia 22151.

UNITED STATES DEPARTMENT OF COMMERCE  
Maurice H. Stans, Secretary  
NATIONAL BUREAU OF STANDARDS • A. V. Astin, Director



# TECHNICAL NOTE 373

ISSUED JUNE 1969

Nat. Bur. Stand. (U.S.), Tech. Note 373, 116 pages (June 1969)  
CODEN: NBTNA

## RADIO-FREQUENCY MEASUREMENTS IN THE NBS INSTITUTE FOR BASIC STANDARDS

EDITED BY ROBERT S. POWERS  
AND WILBERT F. SNYDER

Institute for Basic Standards  
National Bureau of Standards  
Boulder, Colorado 80302

NBS Technical Notes are designed to supplement the Bureau's regular publications program. They provide a means for making available scientific data that are of transient or limited interest. Technical Notes may be listed or referred to in the open literature.



## TABLE OF CONTENTS

Abstract .....	iv
Introduction .....	1
Measurement Representation .....	5
Time and Frequency Standards .....	6
Time and Frequency Dissemination .....	7, 8, 9, 10
Cavity Wavemeters .....	11
Stability of Stable Oscillators and Other Signal Sources .....	12
RF Power in Coaxial Systems: .....	13, 14
Dry Load Calorimetric Measurement and Coaxial Bolometer Units .....	13
Flow Calorimetric Measurement .....	14
Microwave Power: .....	15, 16, 17
Coaxial Bolometer Units, Adapter Method .....	15
Waveguide Bolometer Units: .....	16, 17
Microcalorimetric Measurement .....	16
Impedance Measurement .....	17
RF Peak-Pulse Power in Coaxial Systems .....	18
Noise Temperature: .....	19, 20
Noise Temperature, Coaxial Systems .....	19
Effective Noise Temperature, Waveguide Systems .....	20
RF Voltage, Coaxial Systems .....	21
RF Microvoltage .....	22
Pulse Voltage .....	23
Field Strength .....	24
Field Strength Meters, Antennas .....	25
Attenuation: .....	26, 27
Coaxial Systems .....	26
Waveguide Systems .....	27
Phase Shift: .....	28, 29
Coaxial Phase Shifters .....	28
Waveguide Phase Shifters .....	29
Reflection Coefficient Magnitude of Waveguide Devices .....	30
Distributed Parameters in Coaxial Systems .....	31
High Frequency Immittance .....	32
Large Complex Relative Dielectric Permittivity .....	33
High Frequency Relative Dielectric Permittivity .....	34
High Frequency Dielectric Loss .....	35
Microwave Complex Relative Dielectric Permittivity: .....	36, 37
Dielectric Loaded Transmission Lines .....	36
Transmission Cavities .....	37

## ABSTRACT

This volume is a collection of diagrams, tables, and text material, which has been assembled to show the inter-relationships between various radio frequency measurements made by the Institute for Basic Standards (IBS). In particular, the measurements are those which lead to services provided to the public or to other government agencies. These services include not only calibrations made for fees, but the broadcast services of the four NBS radio stations. Measurements made as part of the IBS research and development program are not included.

The information included is designed to give the users and potential users of the radio frequency services a clearer understanding of the origins of the measurement output of IBS in this field.

Key words: accuracy; calibration services; measurements; measurement techniques; radio frequency; uncertainties of measurement.

# RADIO-FREQUENCY MEASUREMENTS IN THE NBS INSTITUTE FOR BASIC STANDARDS

Edited by Robert S. Powers  
and Wilbert F. Snyder

## INTRODUCTION

This volume is being published to give users of the National Bureau of Standards calibration services at radio frequencies a collection of information about the uncertainties given in Report of Calibration. It is a collection of diagrams, tables, and text material which shows the interrelationships among various radio frequency measurements made by the Institute for Basic Standards (IBS). In particular, the measurements are those which lead to services provided to the public or to other government agencies. These services include not only calibrations made for fees, but also the broadcast services of the four NBS radio stations. Measurements made as part of the IBS research and development program are not included.

It is hoped that this information will give the users and potential users of the radio-frequency services a clearer understanding of the origins of the measurement output of IBS in this field.

Generally, the sequence of measurements which leads to an output calibration or other service is shown by measurement flow charts. The notations of these charts are explained on page 5.

Each measurement may have errors arising from many sources. Typical values of these errors are given in one of two ways. In most cases, known or suspected sources of bias error are listed along with typical values of the random errors (or imprecision). In addition, in many instances, Error Flow Diagrams have been included to show more explicitly the way the various sources of uncertainty enter the measurement chain.

The study that led to these charts and tables was initiated to provide the management of the Institute and its divisions with a fairly detailed analysis of how the elements of the NBS part of the national system of radio measurements relate to each other. This was to help identify those parts of the "NBS subsystem of radio measurement" which could make the greatest contributions to improving the output of

the subsystem as a whole, if given the limited funds that are available. The principal suggestion arising from the study was that significant gains in the overall performance of the IBS system could result from improvement in the treatment and reporting of the known error sources. At this time, a program to improve the reporting of uncertainties is under way.

This information is current as of approximately January, 1969. It serves to update, and present in a different form, some of the information in NBS Technical Note 262.\*

The term "error" means the difference between the value actually measured and some "true value" which would have been obtained from a hypothetical "perfect" experiment.\*\* The term "uncertainty" refers to the range within which the metrologist believes the actual error, as defined above, does fall. Thus, an error does have a particular value, although the metrologist does not know that value; the uncertainty is a range of values specified by the metrologist to indicate his best knowledge about the likely value of the error.

The phrase "bias uncertainties" has been used rather than the more commonly used "systematic errors" to express the uncertainty about the sources of error listed. If the error itself could be evaluated, a correction would be made. The phrase "random error" is used to represent observed deviations of measurements from the mean of a set of measurements.

In perusing these pages, the reader will observe that the values for errors are sometimes shown with plus and minus signs ( $\pm$ ) and sometimes without the signs. There is no significant difference between the two designations, it being mostly a matter of personal choice. Prepared material for this volume came from a number of sources, and no particular effort was made to bring the use of plus and minus signs into uniformity. To do so would have required extensive redrafting and re-typing.

---

\* NBS Technical Note 262, Accuracy in measurements and calibrations, 1965, edited by W. A. Wildhack, R. C. Powell, and H. L. Mason, issued June 15, 1965.

\*\* The concept of "true value" is discussed in some detail by Churchill Eisenhart in his paper, Realistic evaluation of the precision and accuracy of instrument calibrating systems, J. Res. NBS 67C, 161 (1963).



### Bias Uncertainties:

The uncertainties shown in these tables are typical values and in general may vary somewhat, depending on the range of frequency, the magnitude of the measurand (the quantity being measured), or the nature of the particular device being calibrated. Sometimes the magnitude is given as a single typical value and sometimes as a range of values. More details can be obtained from the person(s) listed under Personnel.

Where error flow diagrams were available, they were used in place of tables.

### Random Errors:

In general, the number given for the random error represents approximately three times the estimated standard deviation ( $3\sigma$ ) for a representative set of measurements.

### Total Uncertainty:

The total uncertainty figure represents the sum of the estimated bias uncertainties and the  $3\sigma$  random errors. Note that in a rather large number of the radio frequency measurements the random errors are quite negligible with respect to the bias uncertainties. The terms "limits of uncertainty" and "limits of error" are often used interchangeably with "total uncertainty."

### Uncertainty quoted customer:

The uncertainty quoted to the customer is not always equal to the total uncertainty as described above. It is sometimes larger due to round-off, and sometimes larger to include an additional margin of safety in the estimate of possible error. Reporting practice is tending more and more toward quoting the actual number obtained as above, rather than the larger figures.

### Notes:

The notes include information and comments which are intended to clarify the diagrams and charts or otherwise help the reader to understand some aspect of the measurement.

## References:

The lists of references are not intended to be complete, but rather to supply the reader with at least one source of published information concerning the measurement, as made by NBS. Sometimes no such sources are available. Where references are given, they often include extensive bibliographies on the subject measurement. Unpublished information can often be obtained from the personnel whose names are listed.

## Personnel:

The name of the person(s) responsible for each measurement is given. Anyone requiring more detailed information about any of the measurements is invited to write to the appropriate person at

National Bureau of Standards  
Institute for Basic Standards  
Boulder, Colorado 80302


or telephone (303) 447-1000 and ask for the person named.

These names are also listed to give credit to those who helped to prepare the charts and other information on the various measurements.


# MEASUREMENT REPRESENTATION

The Symbol :


Represents :



A measurement technique or device




The output of one measurement and input to other measurements; e.g., a calibrated meter having uncertainty  $u$ . The uncertainty is expressed either as a percentage, as a fraction, or as a quantity with dimensions; e.g. "5%", " $3 \times 10^{-7}$ ", or " $10 \mu\text{sec}$ ". These outputs are usually available to NBS customers.



A measurement output available to NBS customers.

# TIME AND FREQUENCY STANDARDS

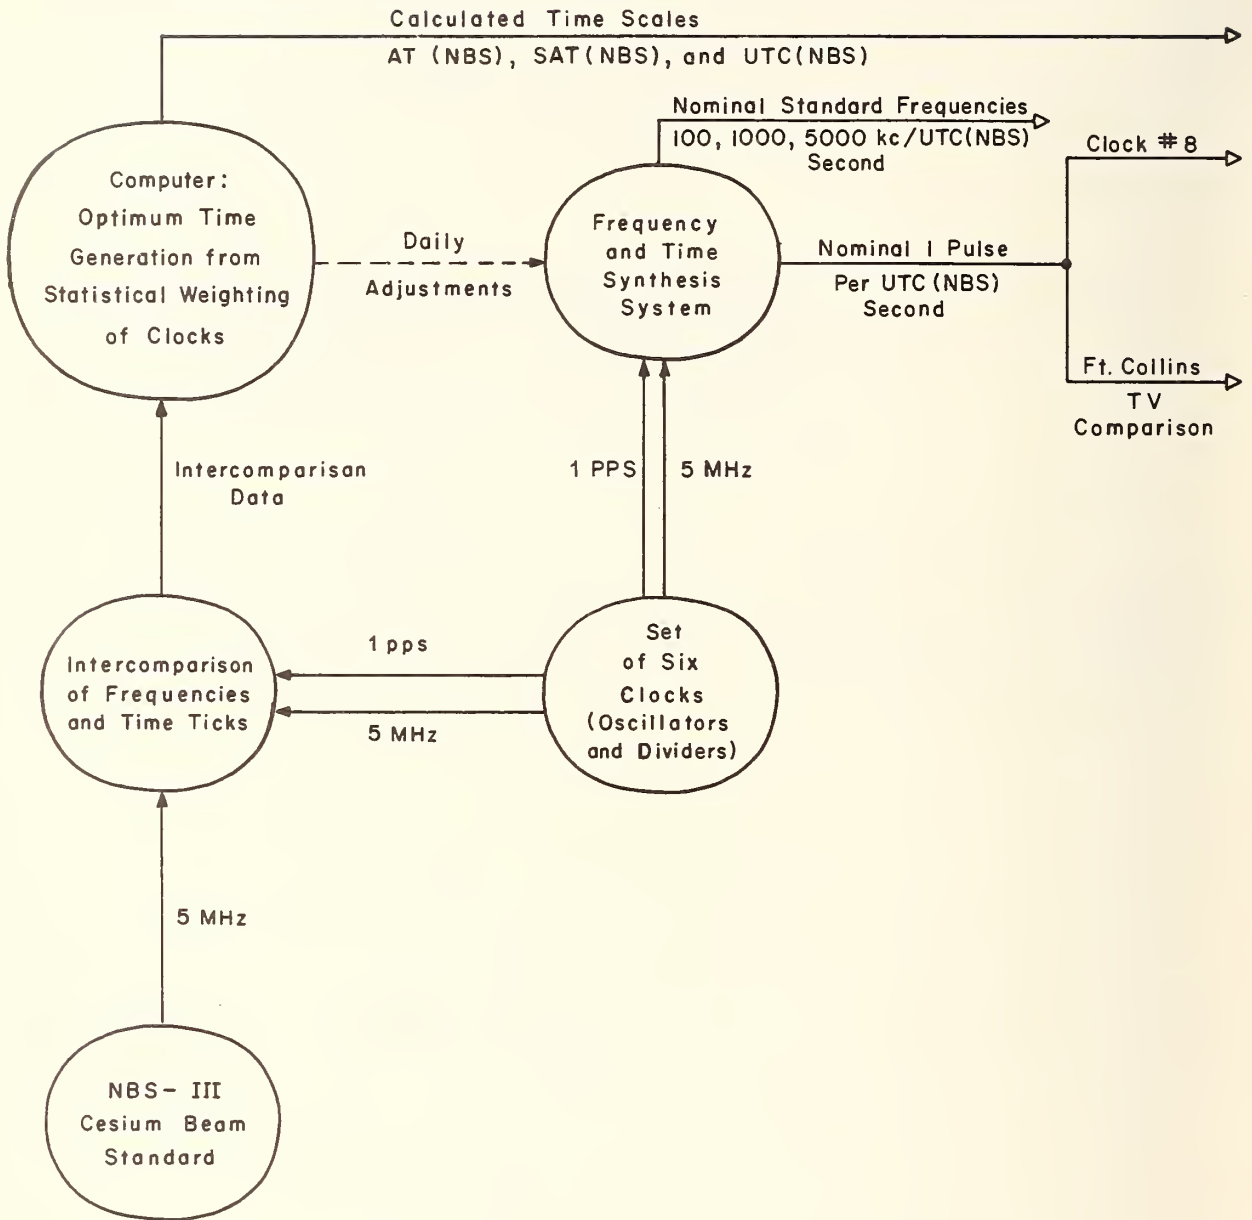

## Time and Frequency Standards

### Bias Uncertainties:

Source of Uncertainty	Fractional Uncertainty	
Magnitude of $\overline{H(x)}$ ( $3\sigma$ limits)	0.3	(parts in $10^{12}$ )
Overlap of neighboring transitions	1.0	
Use of $H(x)^2$ for $H^2(x)$	0.1	
Distortion arising from C-field nonuniformity	0.5	
Cavity mistuning	0.1	
Uncertainty in magnitude of cavity phase shift	3.0	
Doppler shifts	1.0	
Microwave power level	1.0	
Spectral purity of excitation	2.0	
Second harmonic distortion of servo modulation	0.5	
Miscellaneous servo system effects	2.0	
Multiplier chain transient phase shifts	1.0	
<u>Random Errors</u> (one hour averaging, $3\sigma$ ):	0.5	
<hr style="width: 20%; margin: 10px auto;"/>		
<u>Total Uncertainty</u> (square root of sum of squares):	4.7	(parts in $10^{12}$ )

Notes: Error sources listed here contribute to the uncertainty in determining the frequency of a particular atomic state separation of the free cesium atom. The fractional uncertainty is given as  $3\sigma$  limits for statistically determined quantities and by estimated extreme limits for other quantities.

The random error given above refers to the random variations between successive frequency comparisons (with one hour averaging time) between the NBS-III cesium beam machine and another highly stable oscillator. The contribution of NBS-III to the relative fluctuation between the pair of signals generated can be identified (approximately) because the stability of the second signal generator is known from comparisons with still other oscillators.

NBS-III cannot be operated continuously -- the NBS time scale is actually computed from the data obtained by daily intercomparisons between NBS-III and the signals from five sources (two crystal and three cesium) which do operate continuously. Data obtained from these intercomparisons may be

used to adjust the frequencies of the five working sources, when necessary, as shown on page 6.

The standard signals used to control the NBS broadcast stations are generated from one of the working oscillators. The AT (NBS) time scale is derived directly from the frequency of the cesium atom, as realized by NBS-III. The UTC (NBS) scale is generated from a signal having a frequency offset which has been promulgated by the Bureau International de l'Heure to make the time scale correspond approximately to the UT2 time scale.

### USNO and NBS Time Coordination

On 1 October 1968 the epochs of the UTC (NBS) and the UTC (USNO) time scales were within one microsecond of each other. Since there was a slight rate difference between the master clocks at these two institutions, this time coincidence would not have continued. Hence, the USNO and the NBS agreed to each change their rates by nominally half the difference on 1 October 1968, and from thenceforth coordinate the rates so that the master clock at the USNO and the master clock at the NBS would remain near synchronous. It was initially felt and agreed upon that the time difference could be kept less than  $5 \mu s$ .


In the figure (page 6), the abbreviation "pps" means "pulses per second."

Reference: R. E. Beehler and D. J. Glaze, The performance and capability of cesium beam frequency standards at the National Bureau of Standards, IEEE Trans. Instr. Meas., IM-15, 48 (1966).


Personnel: D. Halford  
D. W. Allan

**TIME AND FREQUENCY  
DISSEMINATION - WWVL**  
19.9 or 20.5 and 20.0 kc/(sec-UTC)  
UTC (NBS) Time Scale

AT BOULDER :

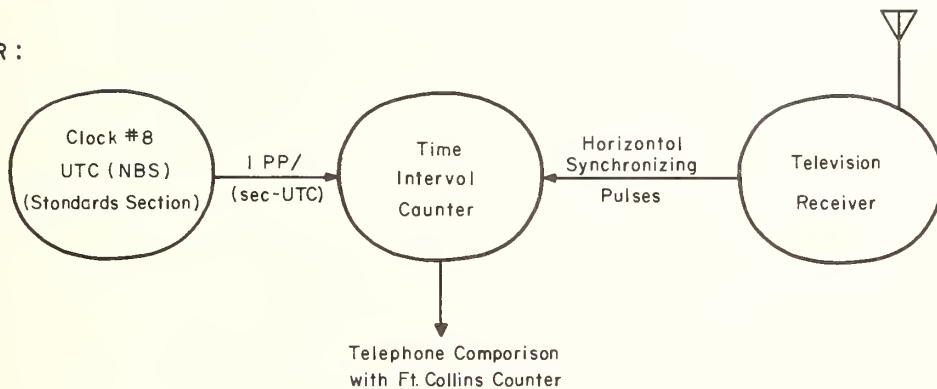


AT FT. COLLINS :

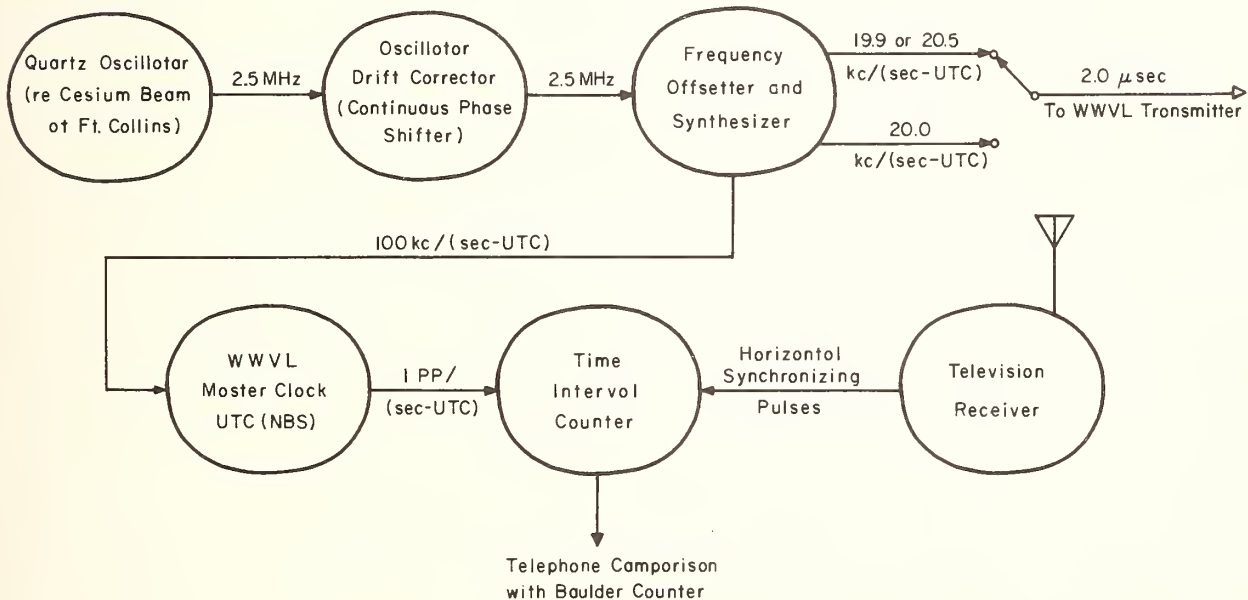


TIME AND FREQUENCY  
DISSEMINATION - WWVB  
60 kHz SAT (NBS) Time Scale

AT FT. COLLINS:

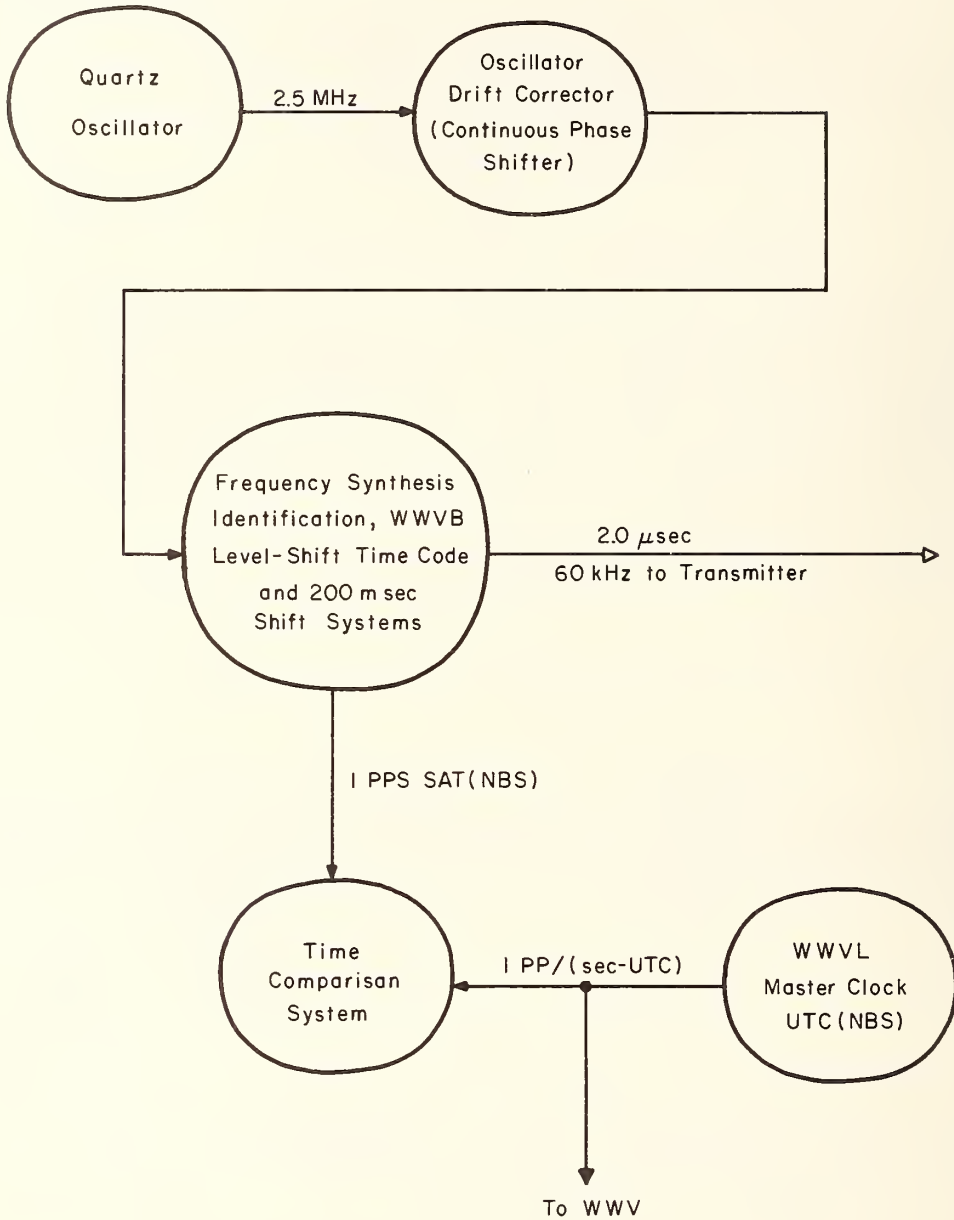




**TIME AND FREQUENCY  
DISSEMINATION - WWV**  
2.5, 5, 10, 15, 20 & 25 Mc/(sec-UTC)  
UTC (NBS) Time Scale

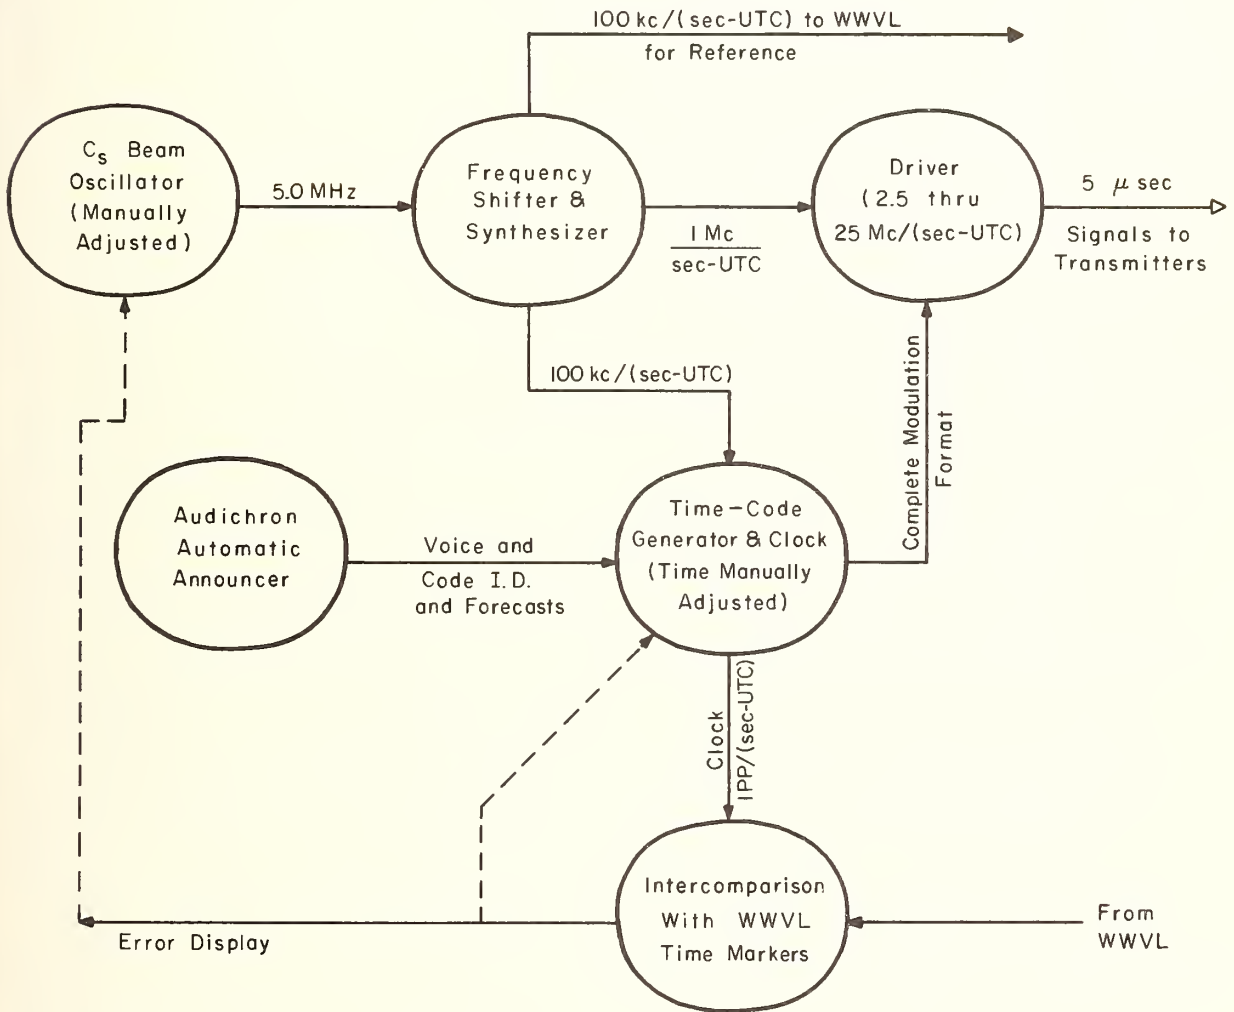

# TIME AND FREQUENCY DISSEMINATION - WWVH

2.5, 5, 10 & 15 Mc/(sec-UTC)  
UTC (NBS) Time Scale

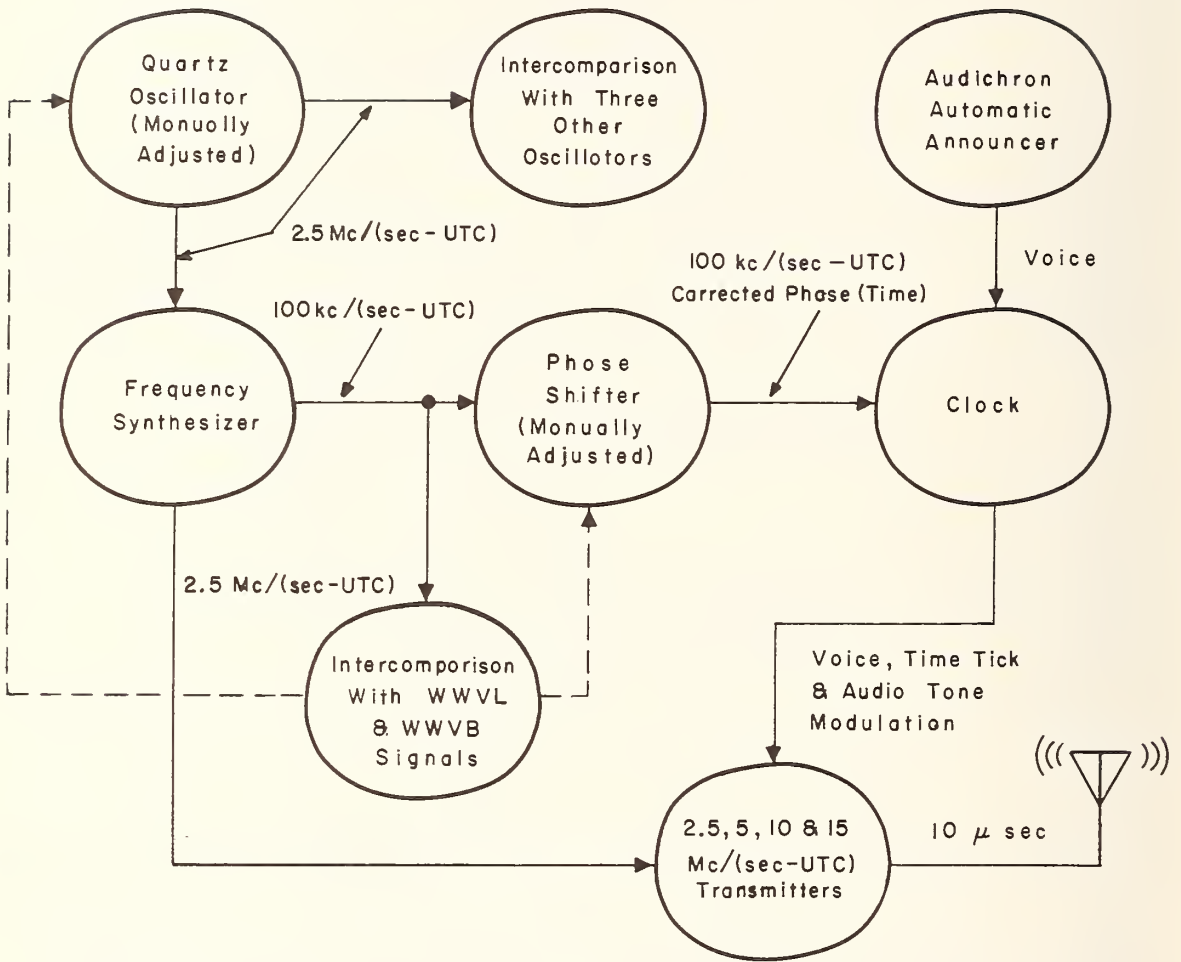

## Time and Frequency Dissemination

### WWVL, WWVB, WWV, and WWVH:

Bias Uncertainties: Since the signals from all the stations are controlled by the standards in Boulder, as shown on pages 7-10 , there is no significant long-term bias in the phase of the broadcast signals relative to the NBS time scales.

Random Errors: The phase (time) uncertainties given below are random fluctuations due to weather-caused changes in antenna impedance and to operator and equipment limitations.

Station	Maximum Phase Error [re SAT(NBS) or UTC(NBS)] (microseconds)
WWVL	2.0
WWVB	2.0
WWV	5.0
WWVH	10.0

Total Uncertainty: Same as Random Errors

Notes: Standard time and frequency signals are broadcast from four radio stations operated by the National Bureau of Standards. WWVL, WWVB, and WWV are located near Ft. Collins, Colorado; WWVH is on the island of Maui, Hawaii. For detailed description of the information available on each signal, see the reference below.

The unit of frequency, Hz, is used to denote one cycle per second, where the second is that defined internationally in terms of a transition in cesium. The unit, c/(sec -UTC), denotes one cycle per second where the second is derived from the UTC(NBS) time scale.

The frequency offset from the internationally defined atomic frequency required to generate the UTC(NBS) time scale is determined annually by the Bureau International de l'Heure (BIH) in Paris. At present the offset is -300 parts in  $10^{10}$ .

SAT(NBS) is a Stepped Atomic Time scale based on the atomic frequency with periodic retardations to approximate UT-2.

Time synchronization between the NBS coordinated time scale UTC(NBS) and the clocks at the Ft. Collins transmitter sites is checked daily.

Reference: NBS Standard Frequency and Time Services, Special Pub. 236  
(1968). (Revised annually).

Personnel: P. Vierzbicke

## DIRECT COMPARISON:

In addition to obtaining time information from the broadcast signals, one can also make direct comparisons between the NBS clocks at Boulder and a portable clock.

Bias Uncertainties: See Notes

Random Errors: See Notes

Total Uncertainty: See Notes

Uncertainty quoted customer: See Notes


Notes: Comparison between AT(NBS) and the customer clock can be made with a precision of about 1 n sec. and an accuracy of about 100 n sec.

Reference: D. W. Allan, R. L. Fey, H. E. Machlan, J. A. Barnes, An ultraprecise time synchronization system designed by computer simulation, Frequency 6, #1, 11 (1968).

Personnel: D. W. Allan

# CAVITY WAVEMETERS

100 MHz - 90 GHz

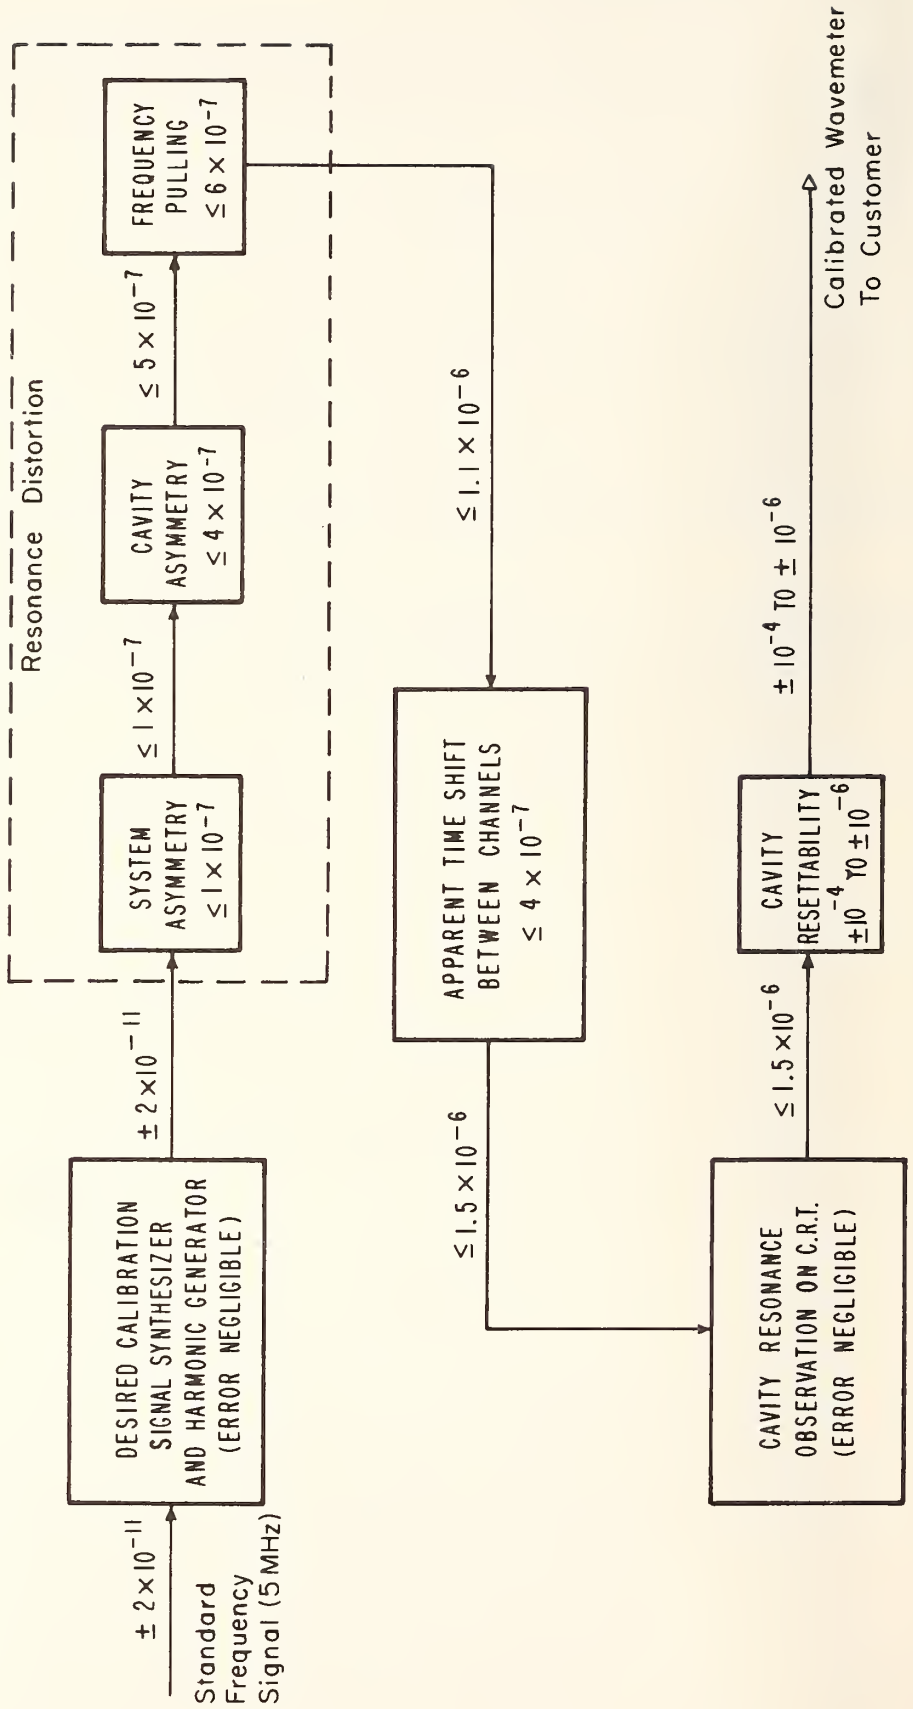

Cavity Wavemeters

100 MHz - 90 GHz

Bias Uncertainties:

Random Errors:

Total Uncertainty:

Uncertainty quoted customer:

} See Error Flow Diagram, page 11


Notes: None

Reference: C. G. Montgomery, Techniques of microwave measurements, Radiation Laboratory Series, No. 11, pp. 291-293 (1947).

Personnel: R. E. Larson  
C. K. S. Miller

STABILITY OF STABLE OSCILLATORS AND OTHER  
SIGNAL SOURCES: FREQUENCY, PHASE, TIME, AND AMPLITUDE STABILITY

Carrier Frequency : 0 Hz - 12.4 GHz  
Frequency Domain :  $10^{-6}$  Hz -  $10^6$  Hz Fourier Frequency  
Time Domain :  $10^{-6}$  s -  $10^6$  s Time Interval

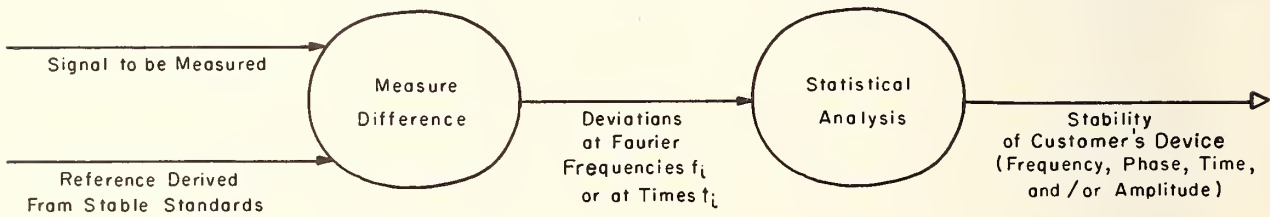



Stability of Stable Oscillators and Other  
Signal Sources: Frequency, Phase, Time,  
and Amplitude Stability

Carrier Frequency: 0 Hz - 12.4 GHz  
Frequency Domain:  $10^{-6}$  Hz -  $10^6$  Hz Fourier Frequency  
Time Domain:  $10^{-6}$  s -  $10^6$  s Time Interval

Bias Uncertainties: Less than 3dB typical, to as low as 0.1dB

Random Errors: Less than 3 dB typical, to as low as 0.1dB

Total Uncertainty: Less than 5 dB typical, to as low as 0.2 dB

Uncertainty quoted customer: Same as Total Uncertainty.

Notes: These calibrations can be performed on quartz crystal oscillators, atomic frequency standards, signal generators, frequency synthesizers, frequency multiplier chains, frequency dividers, amplifiers, buffers, phase shifters, and in general any device which generates or processes a frequency, phase, or time signal. Spectrum analysis can be done directly at Fourier frequencies  $f$  greater than 1 hertz, with an analyzer bandwidth as narrow as 1 hertz. The entire range of frequency domain stability can be obtained by Fourier transformation of time domain data.


References: D. W. Allan, Statistics of atomic frequency standards, Proc. IEEE, 54, 221 (1966), and L. S. Cutler and C. L. Searle, Some aspects of the theory and measurement of frequency fluctuations in frequency standards, Proc. IEEE, 54, 136 (1966).

Personnel: J. H. Shoaf  
D. Halford

## RF POWER IN COAXIAL SYSTEMS

10 - 4000 MHz  
1 - 10 mW Power Level

### BOLOMETER CALIBRATION FROM DRY LOAD CALORIMETRIC MEASUREMENT

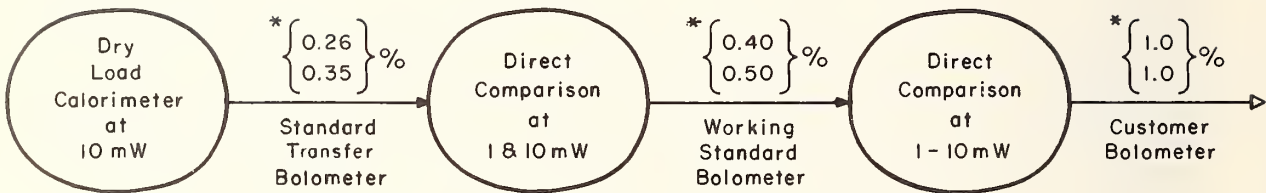

\*  $\left\{ \begin{matrix} 10 \text{ to } 1000 \text{ MHz} \\ 1000 \text{ to } 4000 \text{ MHz} \end{matrix} \right\}$

## RF Power in Coaxial Systems

### DRY LOAD CALORIMETRIC MEASUREMENT:

10 - 4000 MHz  
50 mW - 5W

#### Bias Uncertainties:

	<u>10 - 1000 MHz</u>	<u>1000 - 4000 MHz</u>
Calorimeter efficiency	0.04%	0.08%
VSWR mismatch	negligible	negligible
RF - dc substitution	0.05	0.10
dc power	0.02	0.02
Feedback loop error	0.15	0.15
<u>Random Errors:</u>	negligible	negligible
<u>Total Uncertainty:</u>	0.26%	0.35%

Uncertainty quoted customer: See Notes

Notes: Ordinarily this measurement is not offered to the public as a service, but is used for international comparisons and to calibrate standard transfer bolometers which are in turn used to calibrate working standard bolometers for the NBS Electronic Calibration Center.

Reference: M. L. Crawford, A new RF - dc substitution calorimeter with automatically controlled reference power, IEEE Trans. Instr. Meas. IM-17, 378 (Dec. 1968).

Personnel: P. A. Hudson

## RF Power in Coaxial Systems

### TRANSFER BOLOMETER CALIBRATION BY DIRECT COMPARISON:

At 10 mW power level

#### Bias Uncertainties:

The bias uncertainties are taken to be equal to the total error estimated for the calibration of the standard transfer bolometer by the dry load calorimeter. See page 13-1.

Random Errors: Random errors are less than 0.1%.

#### Total Uncertainty:

10 - 1000 MHz: 0.40%  
1000 - 4000 MHz: 0.50%

Uncertainty quoted customer: See Notes

Notes: Ordinarily this measurement is not offered to the public as a service, but is used to calibrate working standard bolometer units for use in the NBS Electronic Calibration Center.

Reference: None

Personnel: P. A. Hudson

## RF Power in Coaxial Systems

### BOLOMETER CALIBRATION BY DIRECT COMPARISON:

At 1, 3, 10 mW power levels

#### Bias Uncertainties:

Bias uncertainties are taken to be the total estimated error in the calibration of the working standard bolometer. See page 13-2.

Random Errors: Random errors in calibration of customer units by direct comparison are less than 0.15%.

#### Total Uncertainty:

10 - 300 MHz: 0.50%  
300 - 1000 MHz: 0.65%  
1000 - 4000 MHz: 0.85%

#### Uncertainty quoted customer:

10 - 300 MHz: 1%  
300 - 1000 MHz: 1%  
1000 - 4000 MHz: 1%

References: P. A. Hudson, A precision RF power transfer standard, IRE Trans. Instr. I-9, 280 (1960).


R. F. Desch and R. E. Larson, Bolometric microwave power calibration techniques at the National Bureau of Standards, IEEE Trans. Instr. Meas. IM-12, 29 (1963).

Personnel: F. X. Ries

## RF POWER IN COAXIAL SYSTEMS

dc - 4000 MHz  
2 - 100 W Power Level

### FLOW CALORIMETER MEASUREMENT

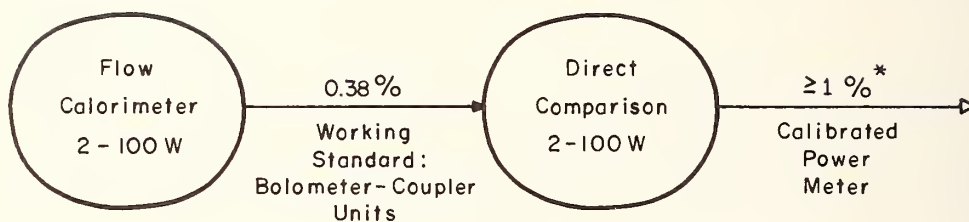

\* Error Limits Are Often Quoted As Greater Than 1%,  
Since Many Meters Calibrated Are Inherently Less  
Accurate Than 1%.

RF Power in Coaxial Systems  
dc - 4000 MHz  
2 - 100 W Power Level

FLOW CALORIMETRIC MEASUREMENT:

2 - 100 watts

Bias Uncertainties:

dc power	0.02%
RF - dc substitution	0.10
Calorimeter efficiency	0.05
Thermal drift and flow rate variations	0.15

Random Errors: See Notes 0.06

Total Uncertainty: 0.38%

Uncertainty quoted customer: See Notes

Notes: Ordinarily this measurement is not offered to the public as a service, but is used only for international comparisons and to calibrate working standard bolometer-coupler units for use in the NBS Electronic Calibration Center.

The random error given here is the maximum observed variation.

Reference: None

Personnel: P. A. Hudson

RF Power in Coaxial Systems

FLOW CALORIMETRIC MEASUREMENT, DIRECT COMPARISON:

2 - 100 watts

Bias Uncertainties:

Uncertainty of working standard	0.5%
VSWR mismatch and errors in meter to be calibrated	0.3

Random Errors: 0.2

Total Uncertainty: 1.0%

Uncertainty quoted customer: 1%

Notes: Errors inherent in the meter to be calibrated can be more than the allowance made here, that is 0.3%. Thus, occasionally the uncertainty quoted the customer is greater than 1%.

Reference: None


Personnel: F. X. Ries



## MICROWAVE POWER: COAXIAL BOLOMETER UNITS

Type N Connector, Male : 4 - 10 GHz  
Precision Connector (GPC - 14) : 4 - 8.5 GHz  
1 - 10 mW Power Level

### ADAPTER METHOD OF MEASUREMENT

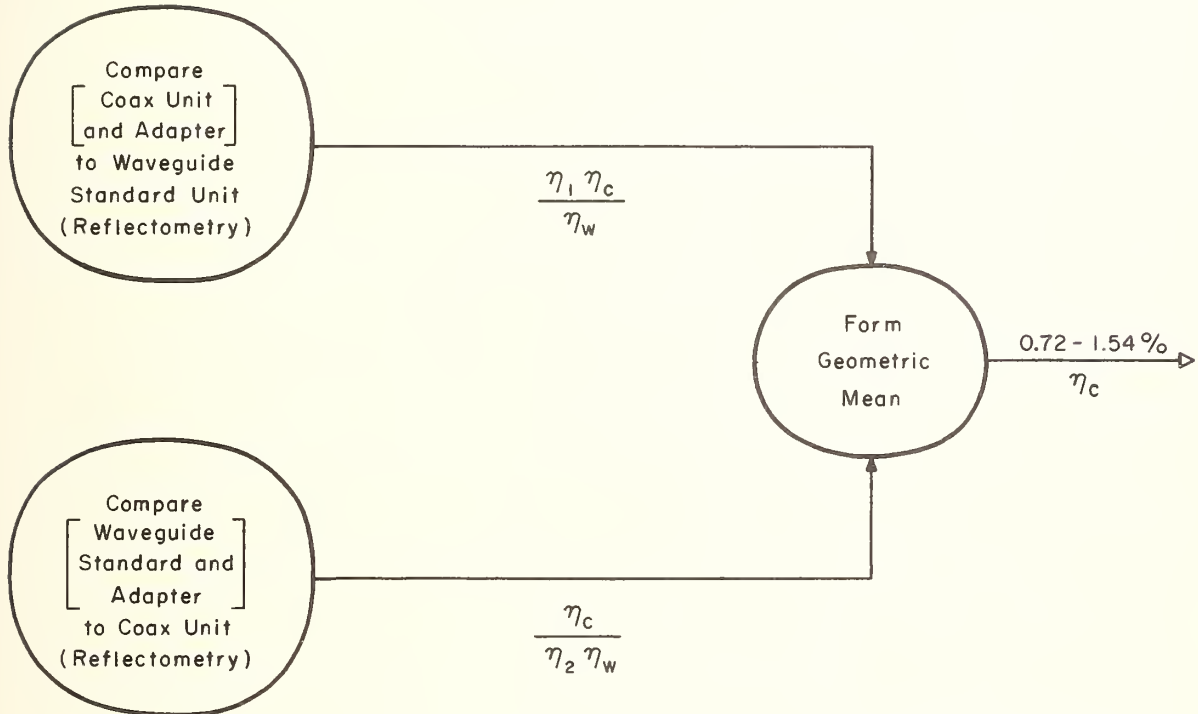

$\eta_c$ : Effective Efficiency of Coaxial Unit

$\eta_w$ : Effective Efficiency of Waveguide Standard Unit

$\eta_{1/2}$ : Efficiency of Adapter as Used In Step ( $\frac{1}{2}$ )

Microwave Power: Coaxial Bolometer Units  
Type N Connector, Male: 4 - 10 GHz  
Precision Connector (GPC-14): 4 - 8.5 GHz  
1 - 10 mW Power Level

ADAPTOR METHOD OF MEASUREMENT:

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagrams, pages 15-2 and 15-3

Uncertainty quoted customer: 0.8% to 1.8%


Notes: This measurement permits the comparison of a coaxial bolometer unit directly with a waveguide standard bolometer unit. Thus, it is not necessary to develop a calorimetric technique for calibrating working standard coaxial bolometer units in this frequency range. See reference. The uncertainty in the waveguide standard in the frequency range 4 to 7.05 GHz (where the impedance method of measurement is used) is 0.75%. In the frequency range 7.05 to 10 GHz (where the calorimetric method of measurement is used), the uncertainty in the waveguide standard is 0.2%.

Symbols appearing in the error flow diagrams are defined in the reference below.


Reference: G. F. Engen, Coaxial power meter calibration using a waveguide standard, J. Res. NBS 70C, 127, (1966).

Personnel: R. F. Desch

**MICROWAVE POWER: COAXIAL BOLOMETER UNITS  
ERROR FLOW DIAGRAM FOR CALIBRATION TRANSFER SYSTEM  
FOR TYPE N CONNECTORS  
ADAPTOR METHOD**

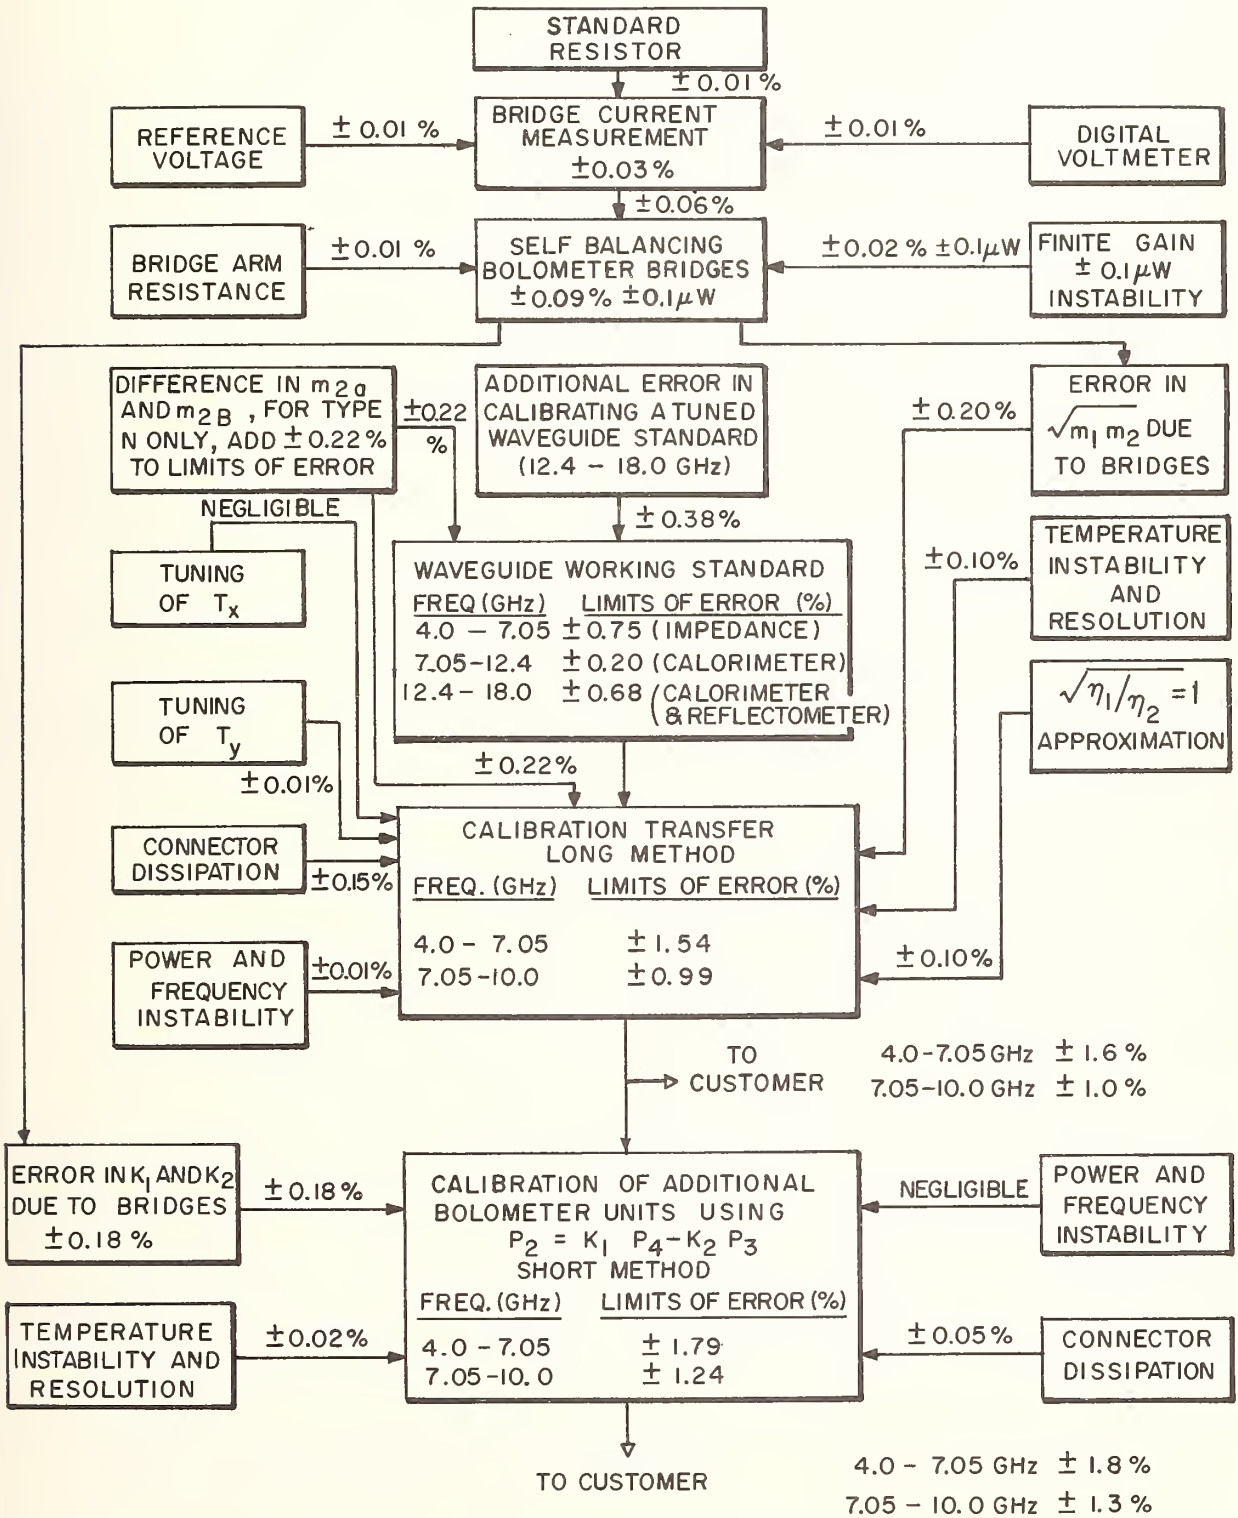

**MICROWAVE POWER: COAXIAL BOLOMETER UNITS**  
**ERROR FLOW DIAGRAM FOR CALIBRATION TRANSFER SYSTEM**  
**FOR PRECISION CONNECTORS (GPC-14 STOPS AT 8.5 GHz)**  
**ADAPTOR METHOD**

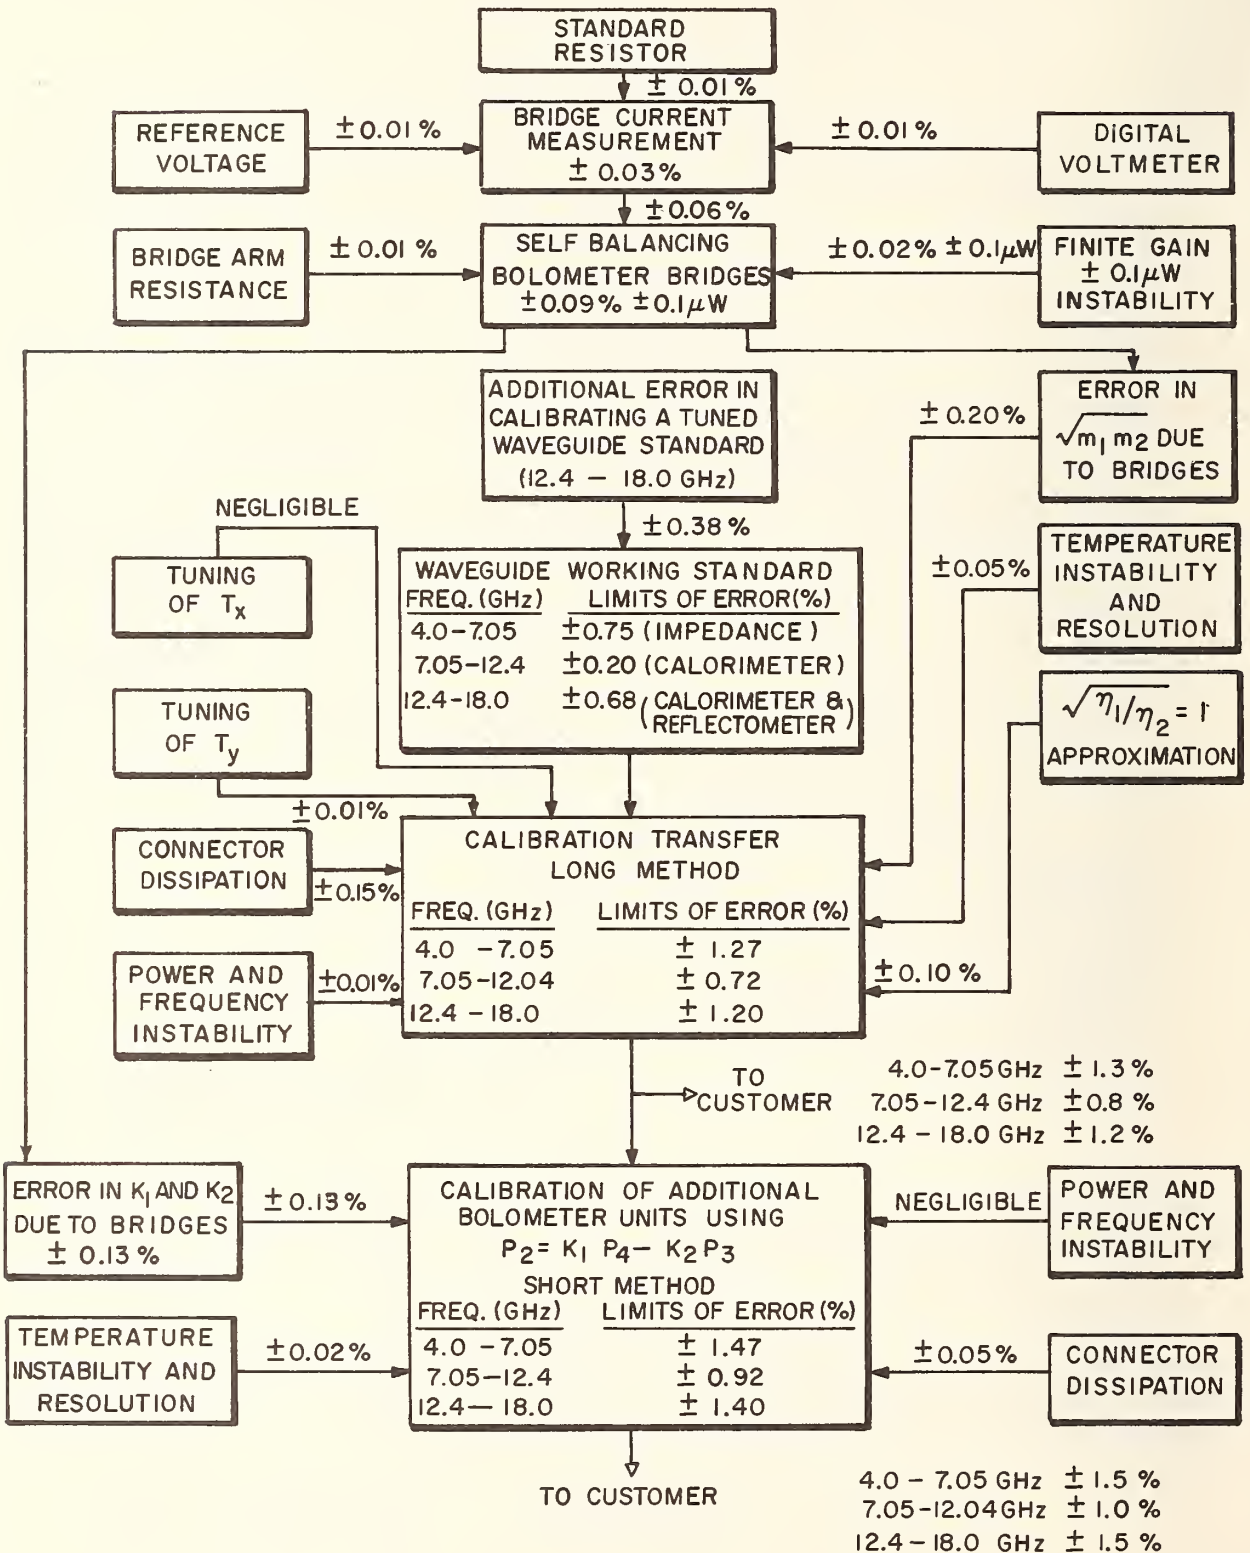

# MICROWAVE POWER : WAVEGUIDE BOLOMETER UNITS

WR 28 : 26.5 - 40.0 GHz

WR 42 : 18.0 - 26.5 GHz


WR 62 : 12.4 - 18.0 GHz

WR 90 : 8.2 - 12.4 GHz

WR 112 : 7.05 - 10.0 GHz

10 mW Power Level

## MICROCALORIMETRIC MEASUREMENT

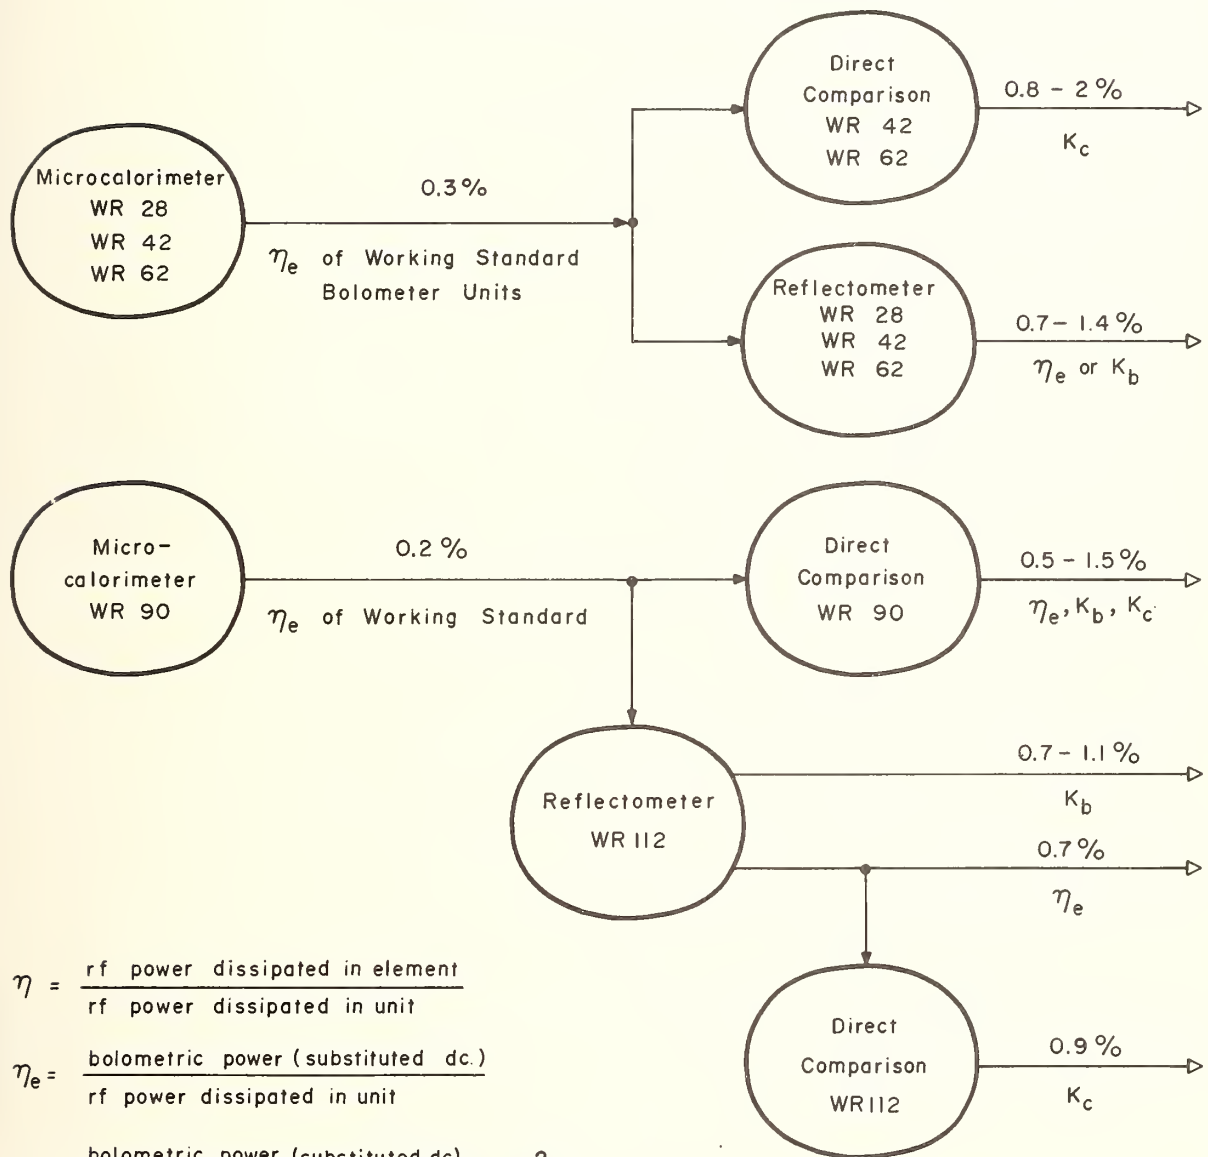

$$\eta = \frac{\text{rf power dissipated in element}}{\text{rf power dissipated in unit}}$$

$$\eta_e = \frac{\text{bolometric power (substituted dc)}}{\text{rf power dissipated in unit}}$$

$$K_b = \frac{\text{bolometric power (substituted dc)}}{\text{rf power incident on unit}} = (1 - |\Gamma|^2) \eta_e$$

$$K_c = \frac{\text{bolometric power in sidearm (substituted dc)}}{\text{rf power incident on non-reflecting main-arm load}}$$

Microwave Power

WR 28: 26.5 - 40 GHz

WR 42: 18.0 - 26.5 GHz

WR 62: 12.4 - 18.0 GHz

WR 90: 8.2 - 12.4 GHz

10 mW Power Level

MICROCALORIMETRIC MEASUREMENT:

Bias Uncertainties:

Random Errors:

Total Uncertainty:


} See Error Flow Diagram, p. 16-2

Uncertainty quoted customer: See Notes

Notes: Ordinarily this measurement is not offered to the public as a service, but is used only for international comparisons and to calibrate working standard bolometer units for use in the NBS Electronic Calibration Center.

Reference: G. F. Engen, A refined X-band microwave microcalorimeter, J. Res. NBS 63C, 77 (1959).

MICROWAVE POWER: WAVEGUIDE BOLOMETER UNITS  
 ERROR FLOW DIAGRAM FOR REFERENCE STANDARD  
 MICROCALORIMETRIC MEASUREMENT  
 WR90 AND WR62

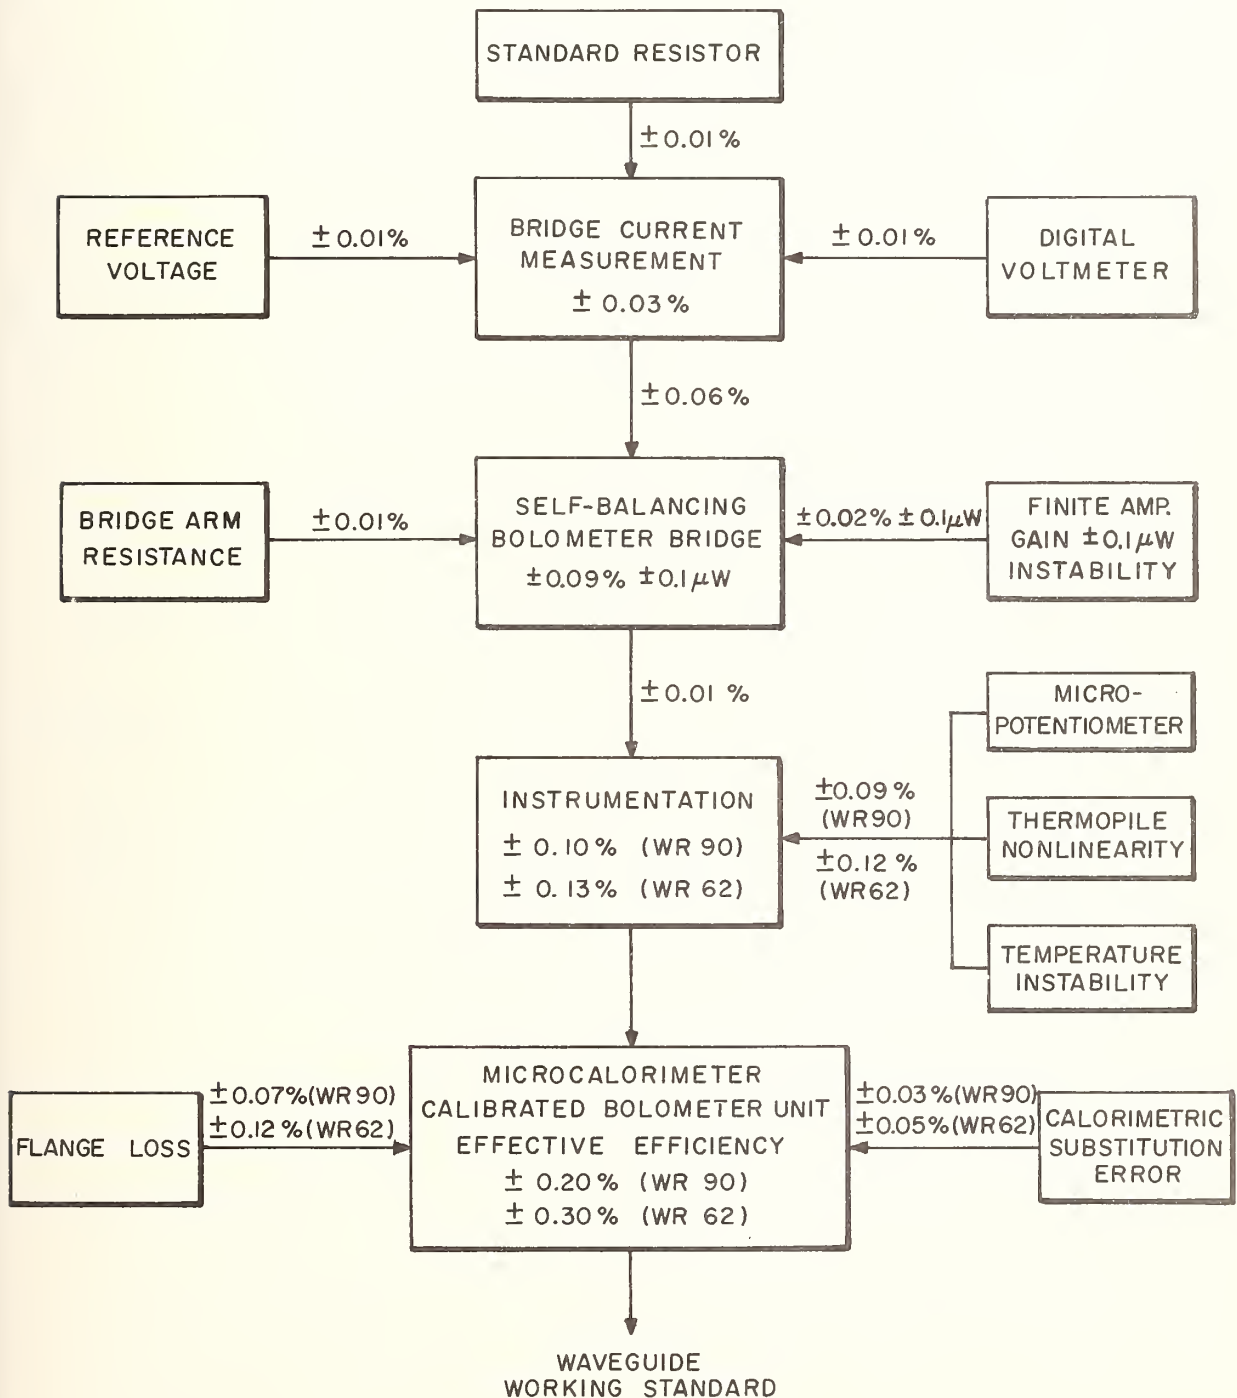

## Microwave Power

### MICROCALORIMETRIC MEASUREMENT, DIRECT COMPARISON METHOD:

#### Bias Uncertainties:

Calorimetric measurement of working standard	0.2 to 0.3%
RF power, temperature, and frequency stability	0.02
dc power	0.1
Flange dissipation and misalignment	0.05 to 0.1
VSWR mismatch (for $0.01 <  \Gamma  < 0.20$ )	0.03 to 1.23

Random Errors: Typical value 0.04

Total Uncertainty:(for  $0.01 < |\Gamma| < 0.20$ ) 0.40 to 1.75%

Uncertainty quoted customer: 0.5 to 1.8%

Notes: This measurement method is used for  $K_c$  only. (See definition below.)

$|\Gamma|$  is the absolute value of the complex reflection coefficient of the bolometer unit.

An error flow diagram for the measurement in the WR 90 waveguide size is given on page 16-5.

In this document the term "bolometer element" will refer to the thermo-element in which the RF power is detected. "Bolometer mount" will refer to the waveguide in which the element is mounted, and "bolometer unit" will refer to the combination. A "bolometer-coupler unit" is a bolometer unit mounted on an arm of a directional coupler.

The definitions of efficiency ( $\eta$ ), effective efficiency ( $\eta_e$ ), and calibration factor ( $K_b$ ) of bolometer units are as follows:

$$\eta = \frac{\text{RF power dissipated in bolometer element}}{\text{RF power dissipated in bolometer unit}}$$

$$\eta_e = \frac{\text{bolometer power (substituted dc in the bolometer unit)}}{\text{RF power dissipated in bolometer unit}}$$

$$K_b = \frac{\text{bolometer power (substituted dc)}}{\text{RF power incident on unit}} = (1 - |\Gamma|^2) \eta_e$$



The calibration factor ( $K_c$ ) for a bolometer-coupler unit is:

$$K_c = \frac{\text{bolometer power in the sidearm (substituted dc)}}{\text{RF power incident on a non-reflecting main-arm load}}$$

The nominal 10 mW power level is for direct incidence on the unit attached to the main arm.

Bolometer-coupler units are calibrated at the power level appropriate to the coupler.


Symbols appearing in the error flow diagram are defined in the reference below.

Reference: R. F. Desch and R. E. Larson, Bolometric microwave power calibration techniques at the National Bureau of Standards, IEEE Trans. Instr. Meas., IM-12, 29 (1963).

Personnel: R. F. Desch

MICROWAVE POWER: WAVEGUIDE BOLOMETER UNITS  
 ERROR FLOW DIAGRAM  
 MICROCALORIMETRIC MEASUREMENT,  
 DIRECT COMPARISON METHOD

WR 90 WAVEGUIDE

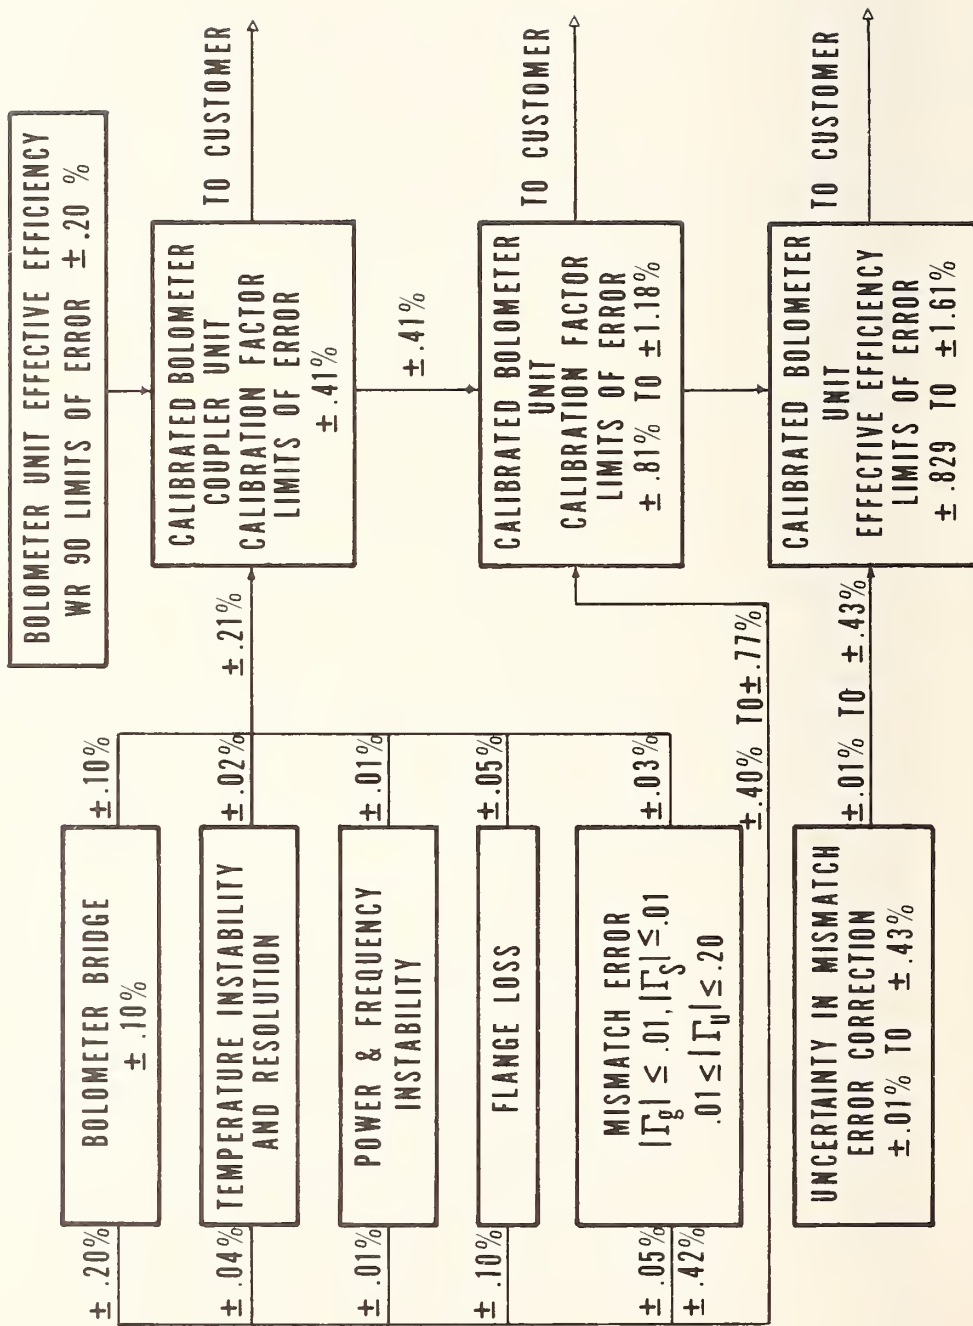

## Microwave Power

### MICROCALORIMETER MEASUREMENT, REFLECTOMETER METHOD:

Bias Uncertainties:

Random Errors:

Total Uncertainty:

Uncertainty quoted customer:

} See Error Flow Diagram,  
page 16-7

Notes: See notes for Direct Comparison method (see p. 16-3).

This measurement method is used for  $\eta_e$  and  $K_b$  only. (See definitions on p. 16-3.)

The estimated uncertainty in a measurement of  $K_b$  is actually about 0.1% higher than that for  $\eta_e$ , because reflection at the waveguide junction has an effect in that case. The uncertainty is still considerably less than 1%, however.

Symbols appearing in the Error Flow Diagram are defined in the reference below.


The self-balancing bolometer bridge (see p. 16-7) with an uncertainty at 0.10% contributes 0.20% to the total uncertainty because the bridge is used more than once in the power measurement.

Reference: G. F. Engen, A transfer instrument for the intercomparison of microwave power meters, IRE Trans. Instr., 1-9, 203 (1960).

Personnel: N. T. Larsen  
R. F. Desch

MICROWAVE POWER: WAVEGUIDE BOLOMETER UNITS  
 ERROR FLOW DIAGRAM  
 MICROCALORIMETRIC MEASUREMENT,  
 REFLECTOMETER METHOD

WR 284, WR 187, WR 137, WR 112, WR 90, WR 62, WR 42, WR 28

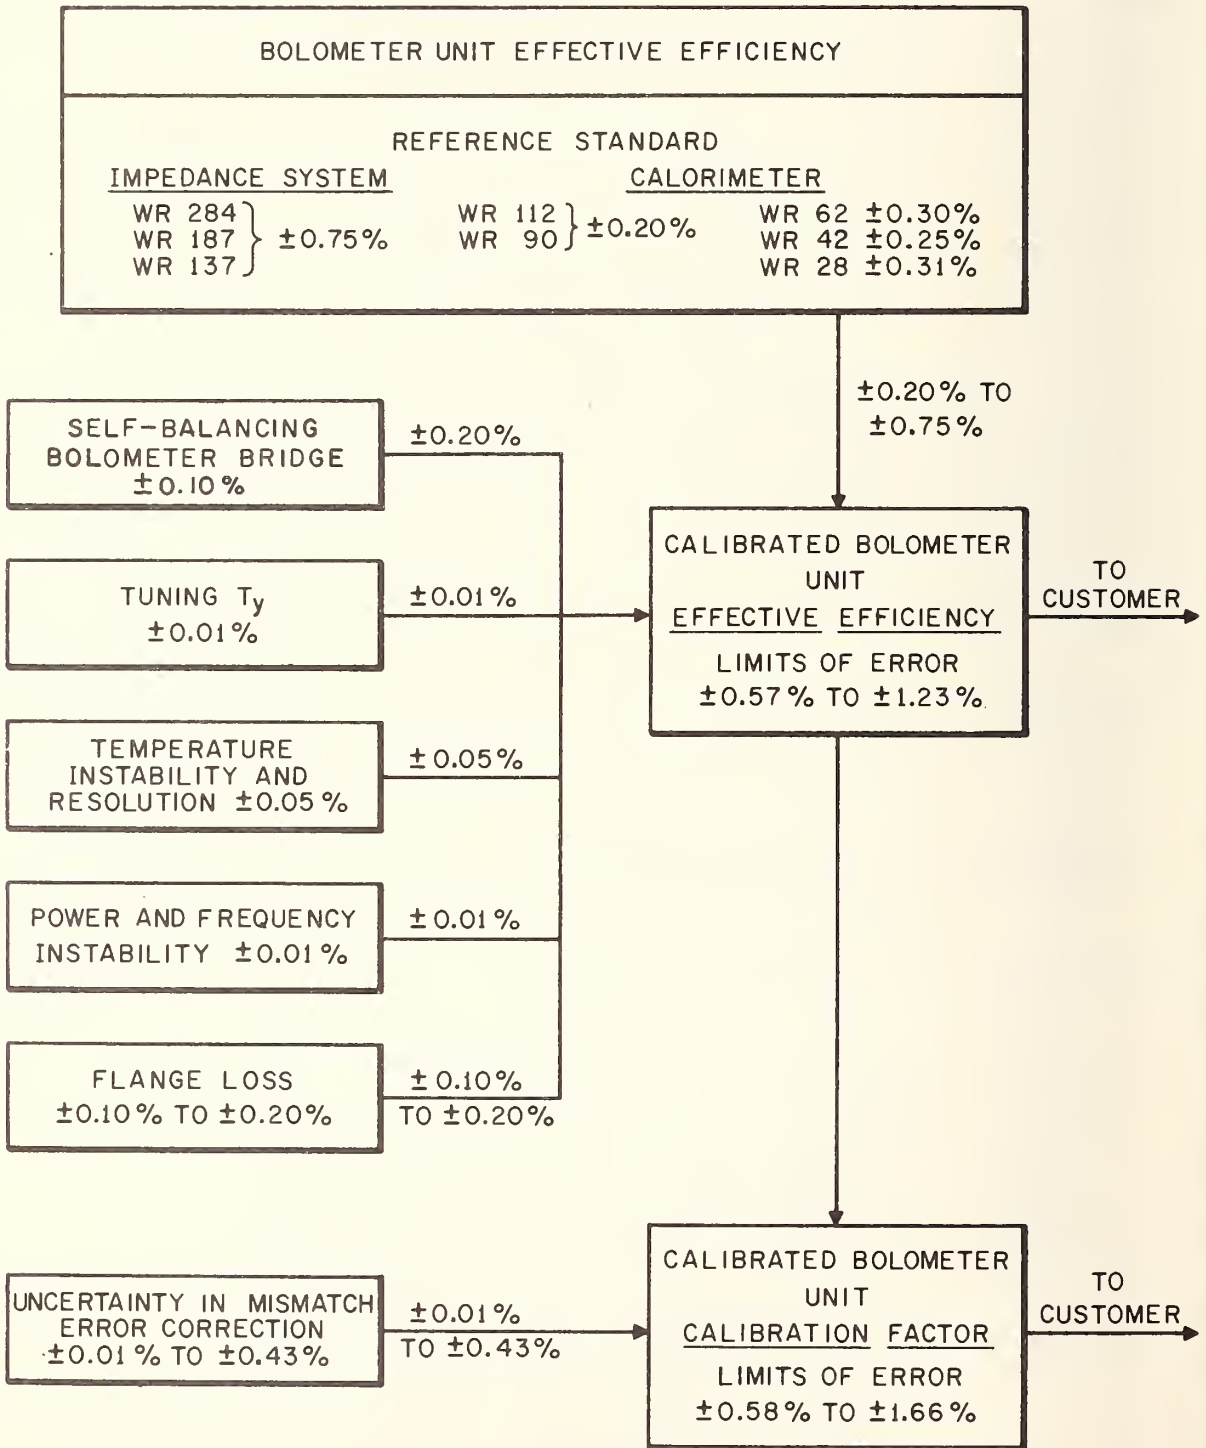

# MICROWAVE POWER : WAVEGUIDE BOLOMETER UNITS


WR 137 : 5.85 – 8.20 GHz

WR 187 : 3.95 – 5.85 GHz

WR 284 : 2.60 – 3.95 GHz

10mW Power Level

## IMPEDANCE METHOD OF MEASUREMENT

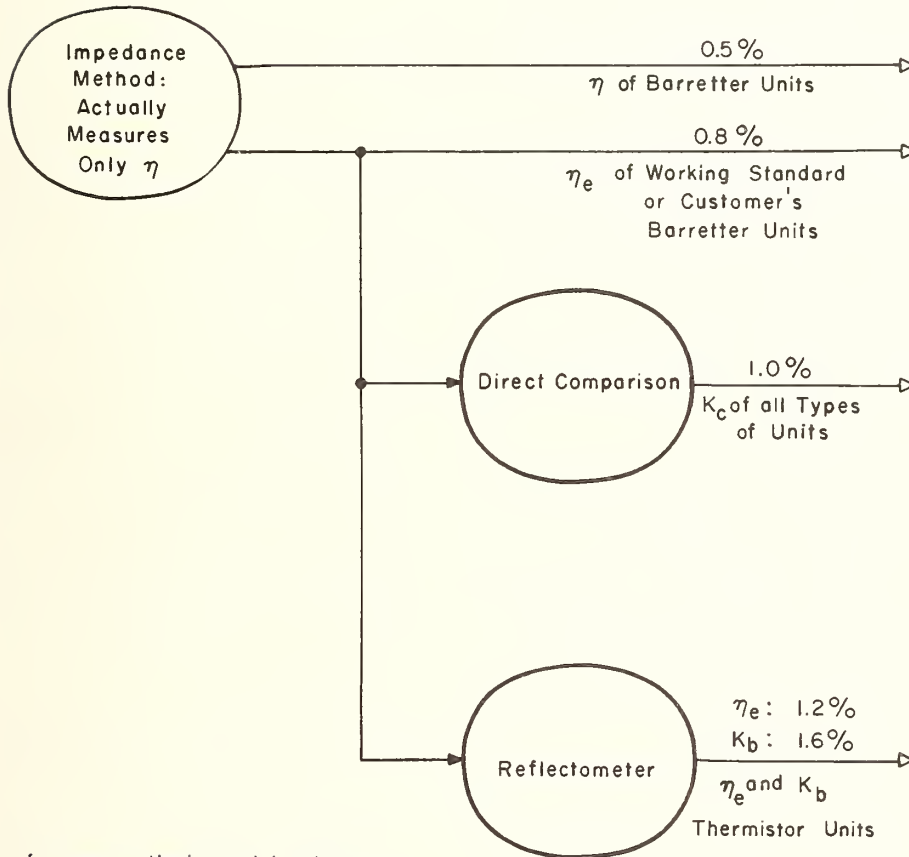

$$\eta = \frac{\text{rf power dissipated in element}}{\text{rf power dissipated in unit}}$$

$$\eta_e = \frac{\text{bolometric power (substituted dc)}}{\text{rf power dissipated in unit}}$$

$$K_b = \frac{\text{bolometric power (substituted dc)}}{\text{rf power incident on unit}} = (1 - |\Gamma|^2) \eta_e$$

$$K_c = \frac{\text{bolometric power in sidearm (substituted dc)}}{\text{rf power incident on non-reflecting main-arm load}}$$

Microwave Power

WR 137: 5.85 - 8.20 GHz

WR 187: 3.95 - 5.85 GHz

WR 284: 2.60 - 3.95 GHz

10 mW Power Level

IMPEDANCE METHOD OF MEASUREMENT:

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagram, page 17-2

Uncertainty quoted customer: 1%


Notes: The impedance method actually measures only  $\eta$ , the efficiency of a bolometer unit. The limits on the effective efficiency of the working standard are obtained from the measured efficiency,  $\eta$ , and an estimate of the RF-dc substitution error. The standard is then used, as shown on page 17, to calibrate the customer's units when  $\eta_e$ ,  $K_b$ , or  $K_c$  is desired.

Symbols appearing in the Error Flow Diagram are defined in reference below.

Reference: G. F. Engen, A bolometer mount efficiency measurement technique, J. Res., NBS, 65C, 113 (1961).

Personnel: R. F. Desch

**MICROWAVE POWER: WAVEGUIDE BOLOMETER UNITS  
 ERROR FLOW DIAGRAM FOR WORKING STANDARD  
 IMPEDANCE METHOD  
 WR284, WR187, WR137**

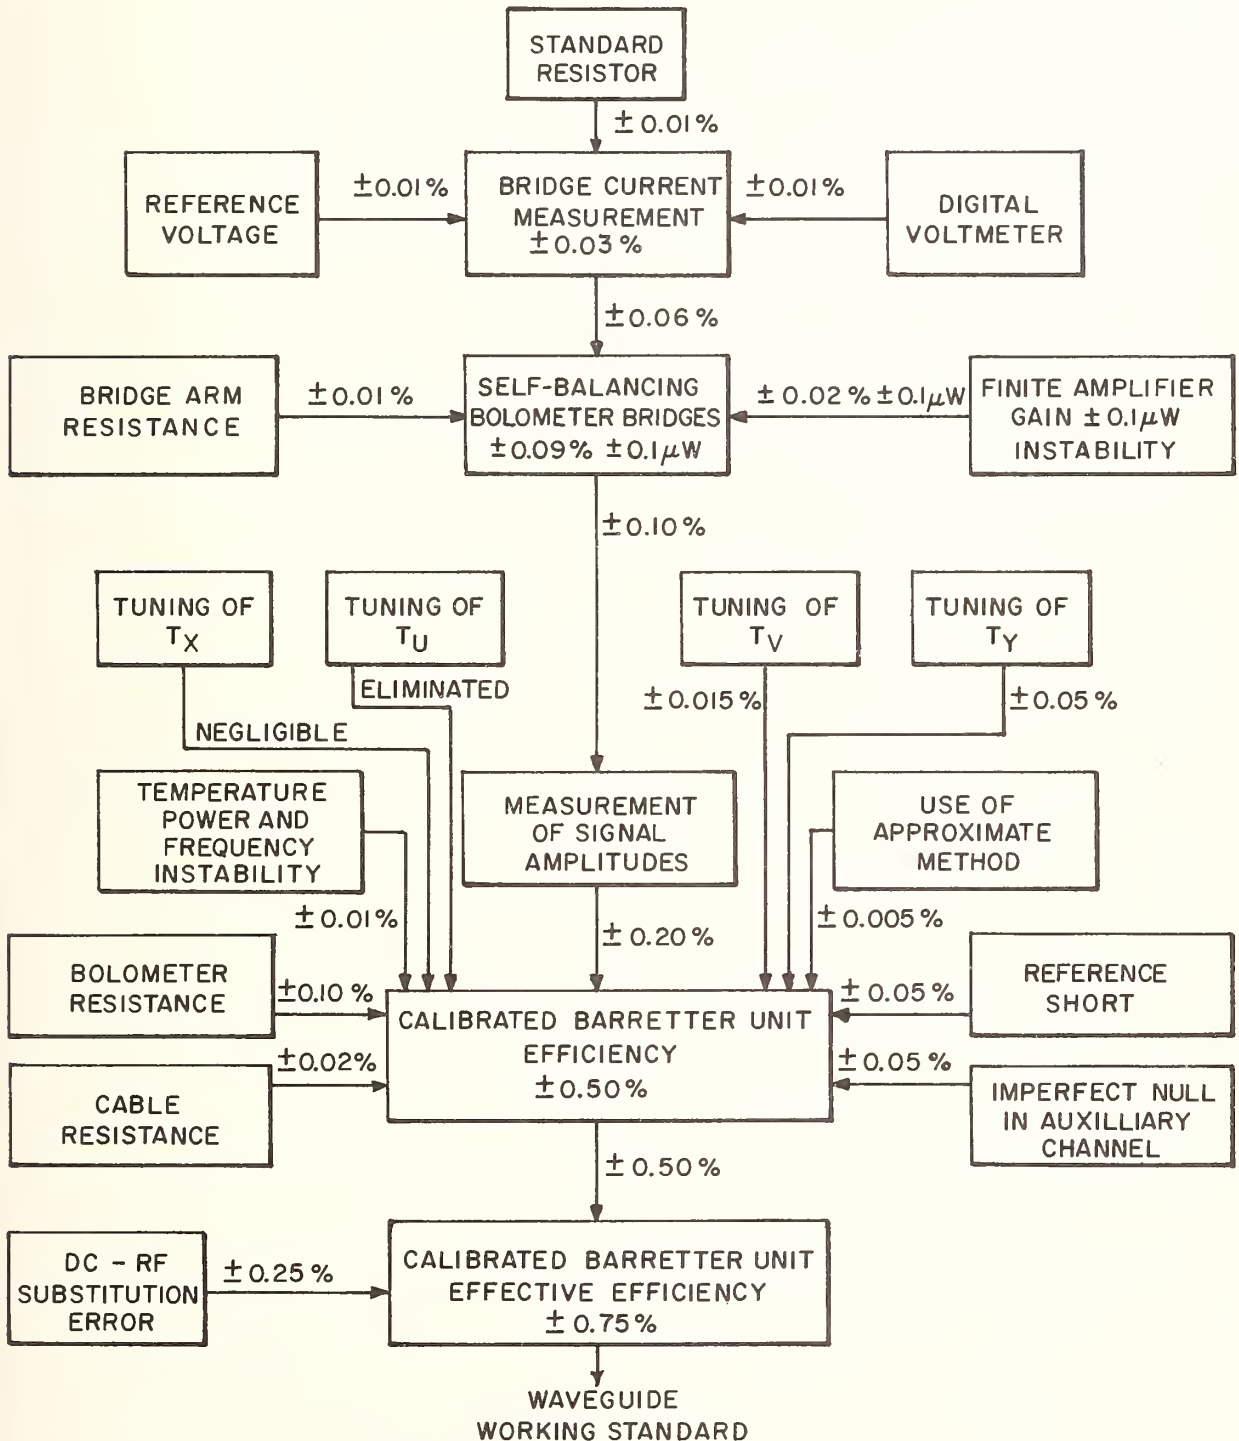

Microwave Power

IMPEDANCE METHOD OF MEASUREMENT,  
DIRECT COMPARISON METHOD:

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagram, page 16-5

Uncertainty quoted customer: 1.5%

Notes: This measurement is used to obtain  $K_c$  for bolometer-coupler units with any type of element.

Reference: None

Personnel: R. F. Desch



Microwave Power

IMPEDANCE METHOD OF MEASUREMENT,  
REFLECTOMETER METHOD:

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagram, page 16-7

Uncertainty quoted customer:  $\eta_e$  for  $|\Gamma| < 0.01$ : 1%  
 $K_b$  for  $|\Gamma| < 0.2$  : 1%

Notes: This measurement is used to obtain  $\eta_e$  and  $K_b$  for bolometer units with thermistor-type elements.

Reference: None

Personnel: R. F. Desch

# RF PEAK-PULSE POWER IN COAXIAL SYSTEMS

300 - 500 MHz


950 - 1200 MHz

Pulse Duration : 2 - 10  $\mu$ sec

Pulse Repetition Rate : 100-1600 pps

Maximum Duty Factor :  $33 \times 10^{-4}$

Peak - Pulse Power : 1.0 mW - 3.0 kW

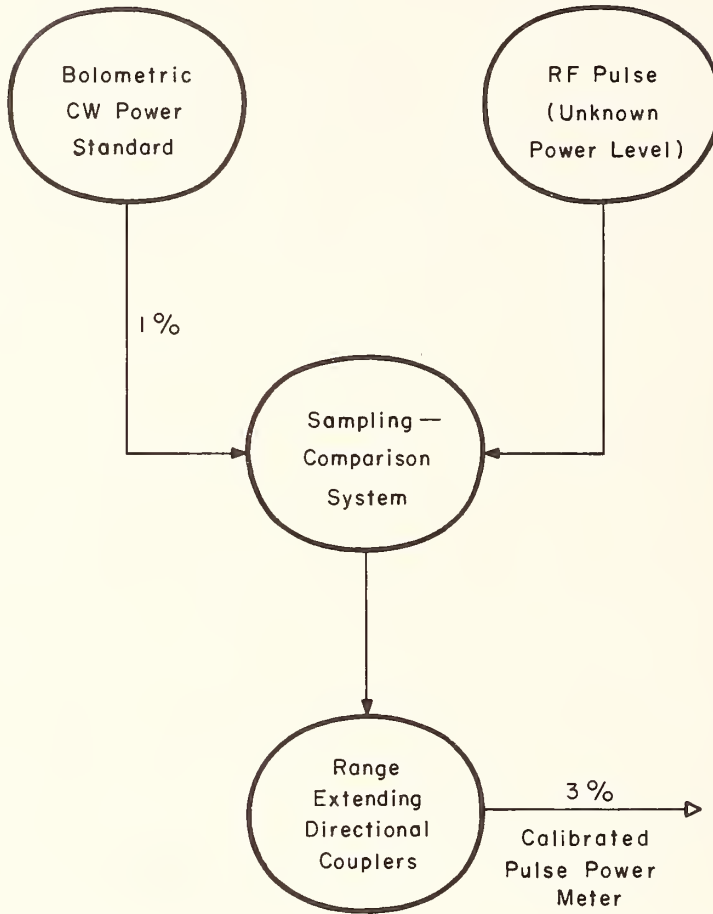

Peak-Pulse Power in Coaxial Systems

300 - 500 MHz

950 - 1200 MHz

Peak-Pulse Power: 1.0 mW - 3.0 kW

Bias Uncertainties:

RF power measurement

a. signal level (CW)	1%
b. direction coupler calibration	1
c. comparison system	1

Random Errors:

negligible

Total Uncertainty:

3%

Uncertainty quoted customer: 3%

Notes: This measurement can be made with the uncertainties stated only on the following conditions:

- (1) Pulse duration must be between 2 and 10 microseconds.
- (2) Pulse repetition rate range: 100 to 1600 pps.
- (3) The duty factor (duty cycle) must be less than  $33 \times 10^{-4}$ .
- (4) The peak-pulse power range must be between 1.0 mW and 3.0 kW.


References: P. A. Hudson, W. L. Ecklund and R. A. Ondrejka, Measurement of RF peak-pulse power by a sampling-comparison method, IRE Trans. Instr., 1-11, 280 (1962).

Peak-pulse power calibrations initiated, NBS, RSL, Engineering Division, IEEE Trans. Microwave Theory and Tech., MTT-14, 47 (1966).


Personnel: P. A. Hudson  
P. A. Simpson

# NOISE TEMPERATURE

Coaxial Noise Generator at 3MHz  
75K to 30,000K

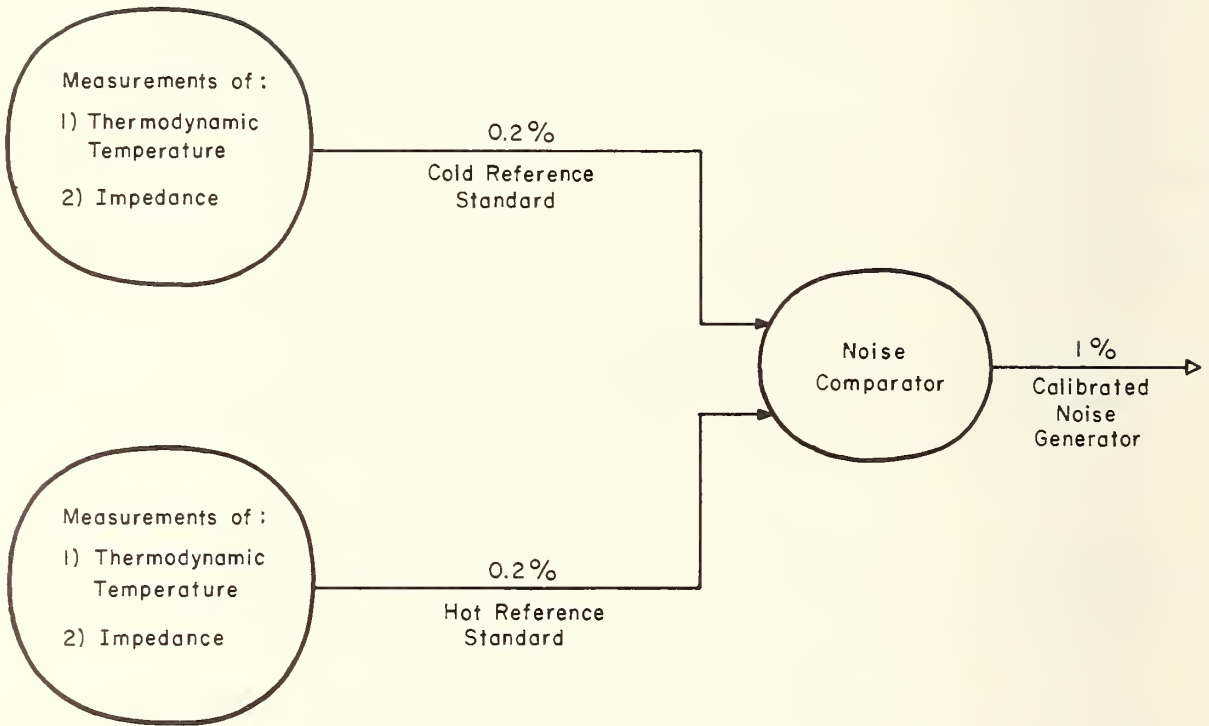

NOISE TEMPERATURE  
COAXIAL NOISE GENERATOR AT 3 MHz  
75 K TO 30,000 K

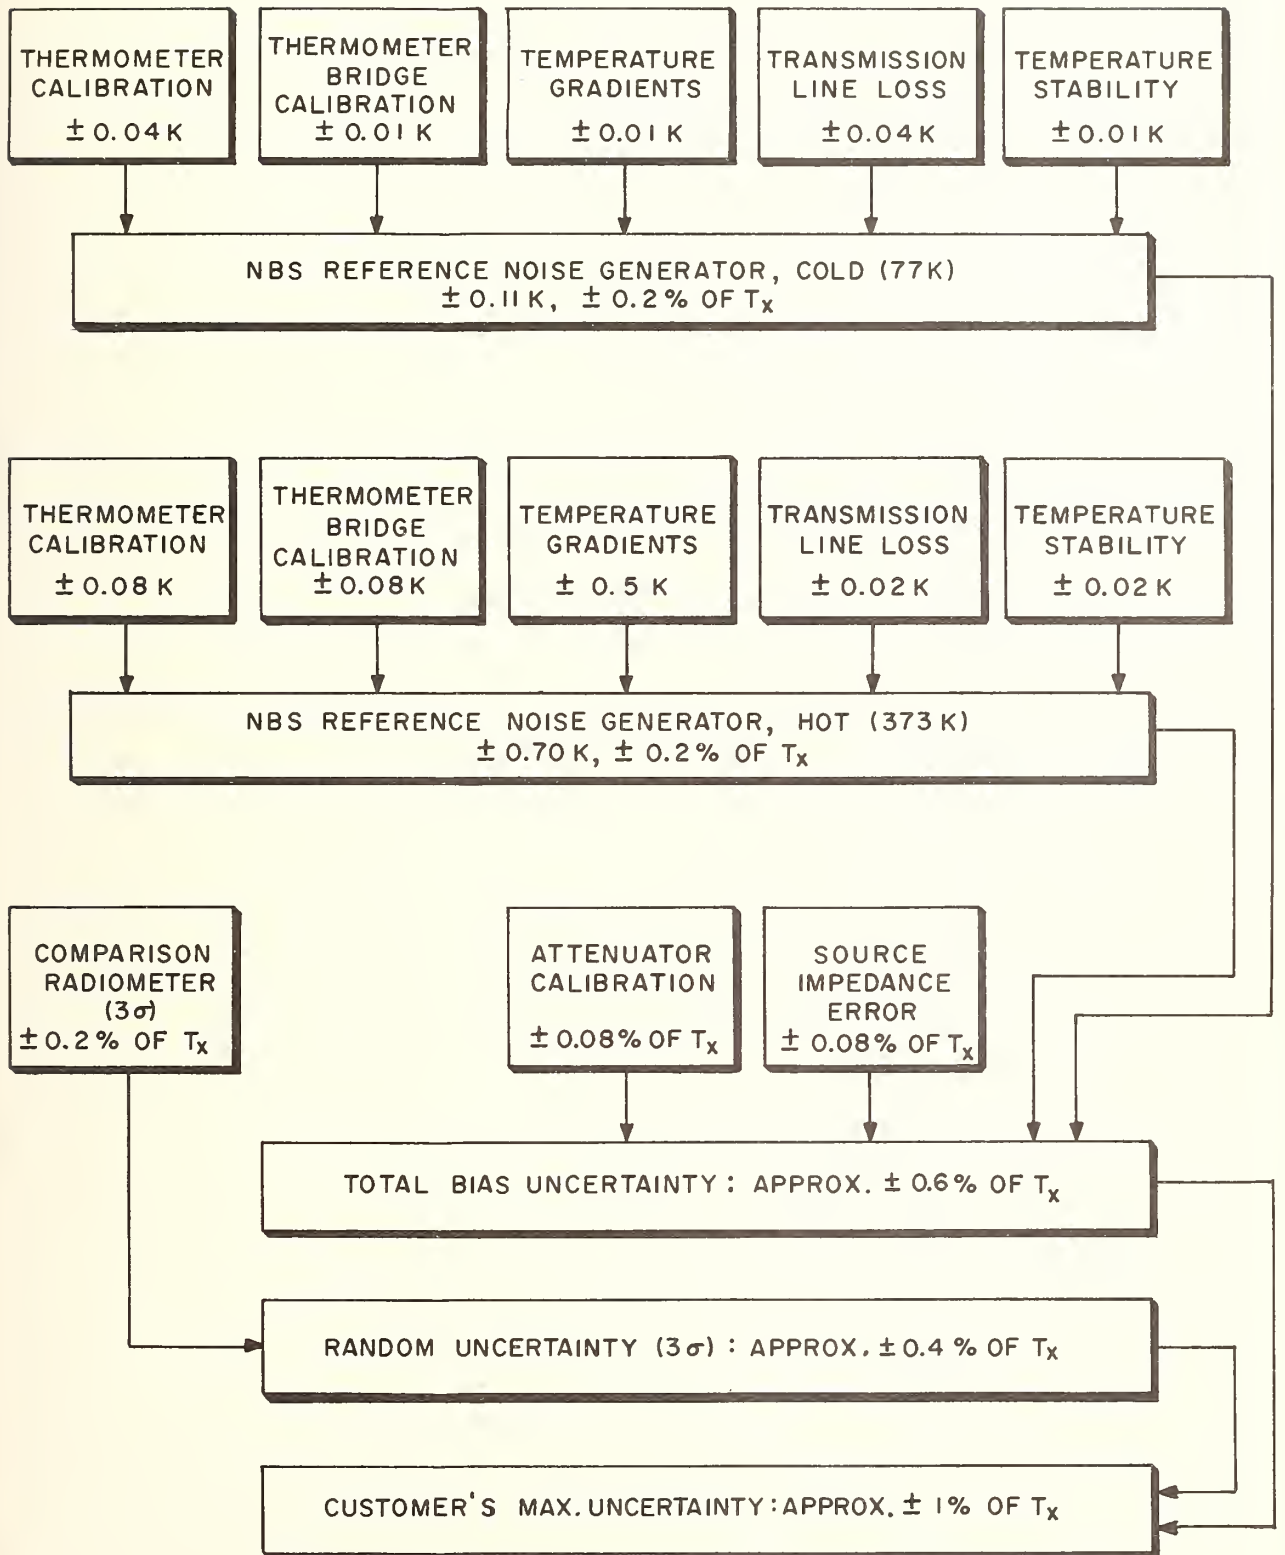

Noise Temperature  
Coaxial Noise Generator at 3 MHz  
75 K to 30,000 K

Bias Uncertainties: Approximately  $\pm 0.6\%$

Random Errors: Approximately  $\pm 0.4\%$

Total Uncertainty: Approximately  $\pm 1\%$


Uncertainty quoted customer: Actual total uncertainty as computed from the measurement data, using the error equation for the measurement process.

Notes: The uncertainties on the diagram (page 19-1) are typical values. Two values are given for each reference generator. The first is the actual uncertainty in the noise temperature of the reference generator; the second is the contribution by that reference generator to the total uncertainty in the measured value of the unknown noise temperature,  $T_x$ .


Reference: M. G. Arthur, C. M. Allred, and M. K. Cannon, A precision noise-power comparator, IEEE Trans. Instr. Meas., IM-13, 301 (1964).

Personnel: M. G. Arthur

EFFECTIVE NOISE TEMPERATURE  
WAVEGUIDE NOISE SOURCE AT 9 GHz  
11,000 K

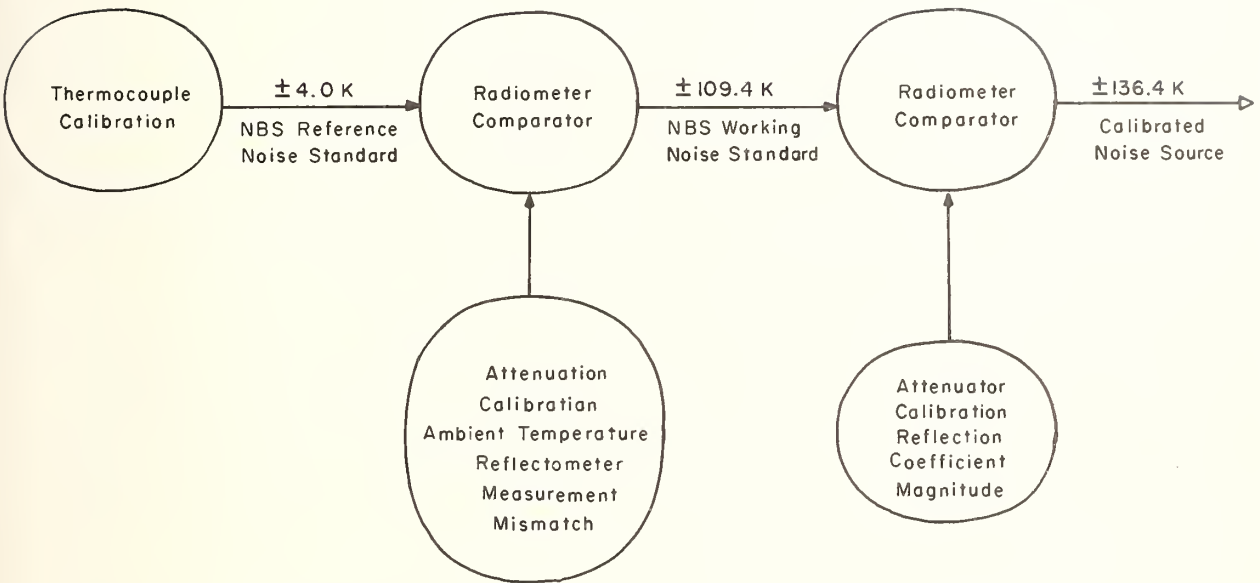

EFFECTIVE NOISE TEMPERATURE  
FOR ARGON NOISE SOURCE, OR  
WAVEGUIDE NOISE SOURCE AT 9GHz  
OPERATING AT 11,000 K

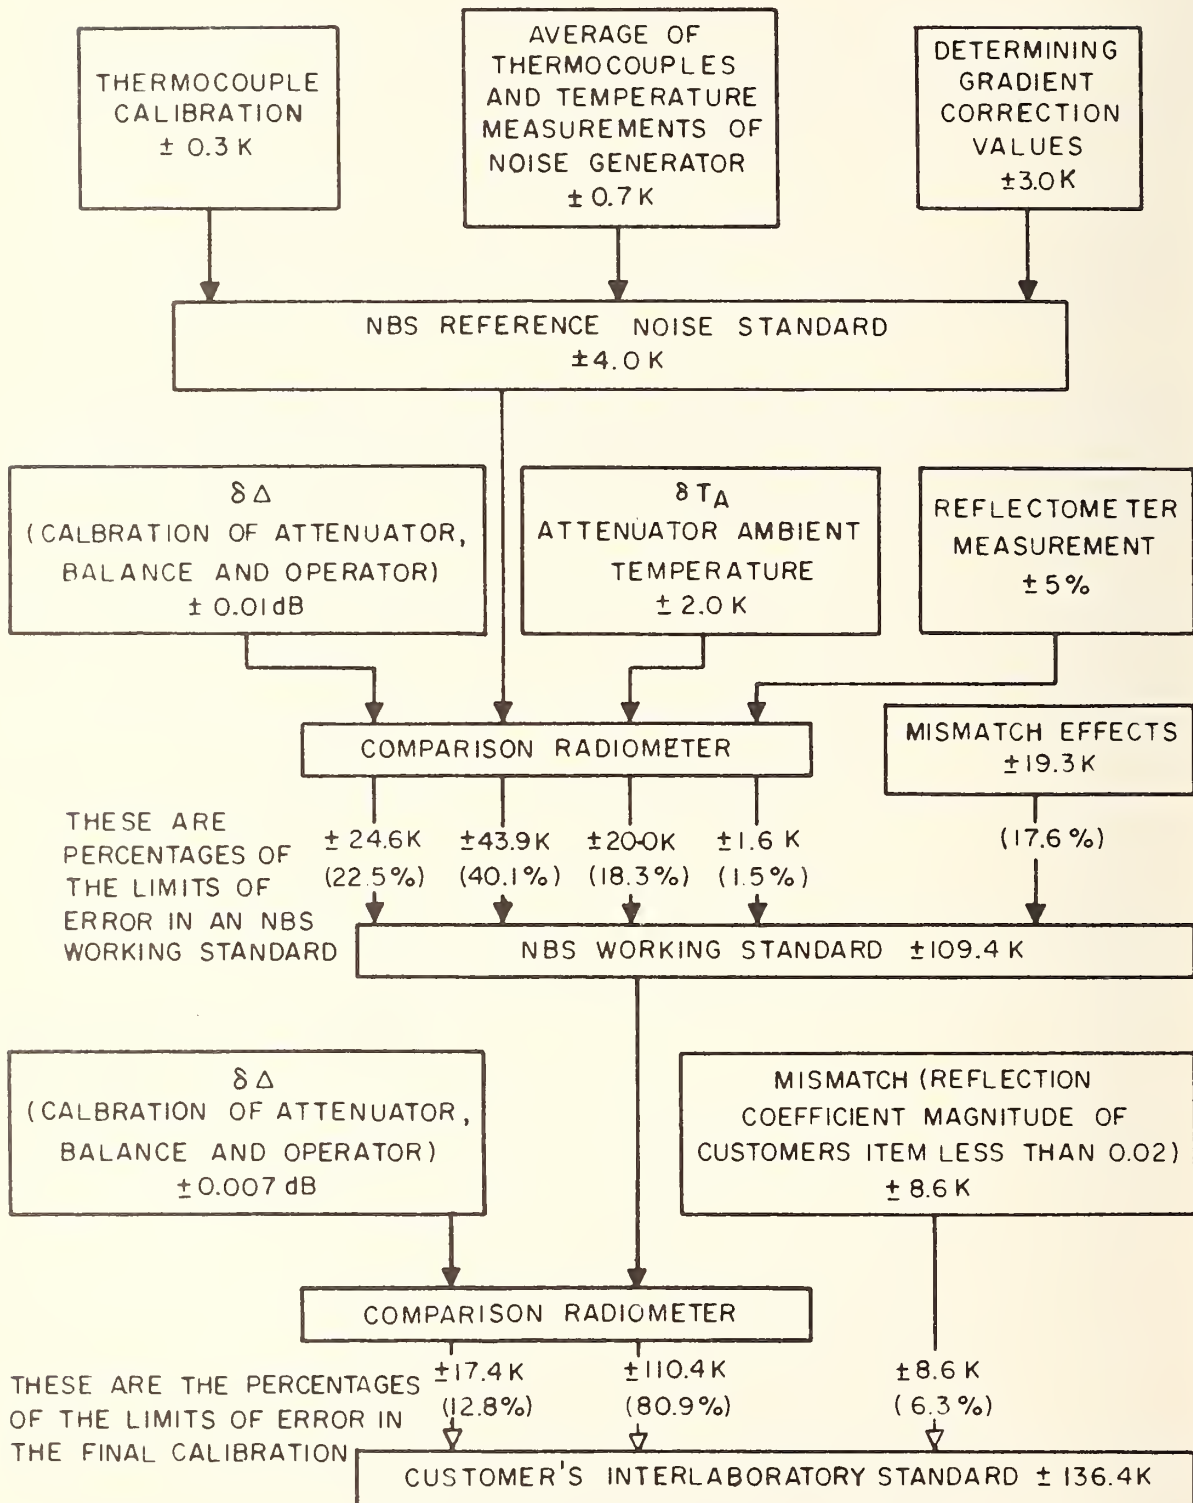



Effective Noise Temperature  
For Argon Noise Source, or  
Waveguide Noise Source at 9 GHz  
11,000 K

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See page 20-1

Uncertainty quoted customer: Same as Total Uncertainty.

Notes: The uncertainties on the diagram (page 20-1) are typical values of systematic error at 9.0 GHz. The error limits depend in a very complicated way on several parameters.


Reference: J. S. Wells, W. C. Daywitt and C. K. S. Miller, Measurement of effective temperatures of microwave noise sources, IEEE Trans. Instr. Meas., IM-13, 17 (1964).

Personnel: C. K. S. Miller

## RF VOLTAGE, COAXIAL SYSTEMS

30 kHz - 1000 MHz

0.1 - 300 Volts

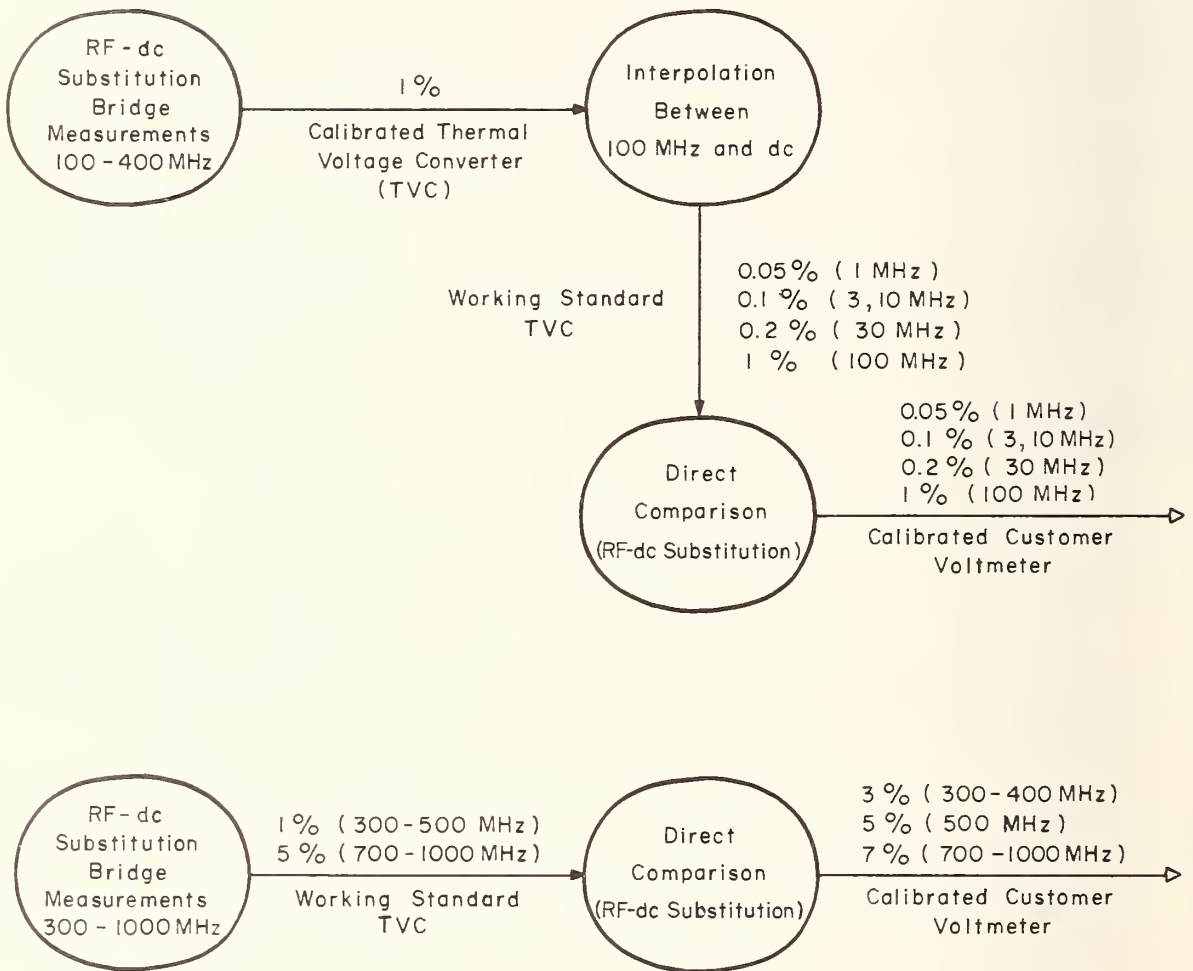

RF Voltage (cw) in Coaxial Systems  
 30 kHz - 1000 MHz  
 0.1 - 300 Volts

BOLOMETER BRIDGE MEASUREMENT:

A. Frequencies 30 kHz - 100 MHz

Bias Uncertainties:

dc voltages and resistances	0.061%
RF source drift	0.020
Galvanometer noise	0.050
Stability of interlaboratory standard resistor	0.010
Short time thermal effects on standard resistor	0.005

Random Errors (3 $\sigma$ ): 0.251

Total Uncertainty: 0.397%

B. Frequencies 100 - 1000 MHz

Analysis similar to the above yields the following estimated error limits:

<u>Frequency</u> (MHz)	<u>Total Uncertainty</u> (%)
100	1
300, 500	1
700, 1000	5

Uncertainty quoted customer: See Notes

Notes: Ordinarily this measurement is not offered to the public as a service, but is used only for international comparisons and to calibrate working standards for use in the NBS Electronic Calibration Center.

Reference: M. C. Selby and L. F. Behrent, A bolometer bridge for standardizing radio-frequency voltmeters, J. Res. NBS, 44, 15 (1950).

Personnel: M. C. Selby

## RF Voltage (cw) in Coaxial Systems

### THERMAL VOLTAGE CONVERTERS at frequencies 30 kHz - 100 MHz

At frequencies below 100 MHz the uncertainties involved in using thermal voltage converters (TVC's) to compare directly dc and ac voltage, without calibration of the converter on a bridge, have been shown by Hermach and Williams to be generally less than the bridge uncertainties (See p. 21). The most important error in this direct procedure is the ac-dc substitution error, which has been investigated theoretically by Hermach and Williams (see Reference p. 21-3). They checked their theoretical results by making measurements of the ac-dc difference on the bolometer bridge at frequencies up to 400 MHz, and found satisfactory agreement. In particular, the theory was verified at frequencies above 100 MHz, where the ac-dc substitution error is greatest and the bridge uncertainties are less than that error. On the basis of this verification of the theory, the converters are used as devices (working standards) to compare ac voltages to dc standards without the use of a bridge. The uncertainty in the TVC as a working standard is taken to be just the substitution error, as follows:

<u>Frequency</u> <u>(MHz)</u>	<u>Uncertainty</u> <u>(%)</u>
1	0.05
3, 10	0.1
30	0.2
100	1.0

## RF Voltage (cw) in Coaxial Systems

DIRECT COMPARISON of customer voltmeters with NBS working standard TVC's:

Bias Uncertainties: In addition to the substitution error considered on page 21-2, other possible sources of error in an actual comparison of ac voltage with dc are:

- Measurement of the dc voltage
- Mismatch
- Determination of the reference plane

It is felt that these errors are negligible with respect to the uncertainty of the working standard at frequencies up to 100 MHz, and that they add between two and four percent to the uncertainties of the working standard at frequencies between 300 and 1000 MHz.

Random Errors: Negligible

Total Uncertainty:

Frequency (MHz)	Uncertainty (%)
1	0.05
3, 10	0.1
30	0.2
100	1
300, 400	3
500	5
700, 1000	7

Uncertainty quoted customer: Same as Total Uncertainty above.

Notes: None

References: F. L. Hermach and E. S. Williams, Thermal voltage converters for accurate voltage measurements to 30 megacycles per second, Trans. AIEE, Communication and Electronics, No. 49, 200 (July 1960).


M. C. Selby and L. F. Behrent, A bolometer bridge for standardizing radio frequency voltmeters, J. Res. NBS, 44, 15 (1950).

M. C. Selby, Voltage measurement at high and microwave frequencies in coaxial systems, Proc. IEEE, 55, 877 (1967).

Personnel: M. C. Selby, F. X. Ries

## RF MICROVOLTAGE

1 - 100 Microvolts,    50 kHz - 500 MHz  
 100 - 100,000 Microvolts,    50 kHz - 900 MHz

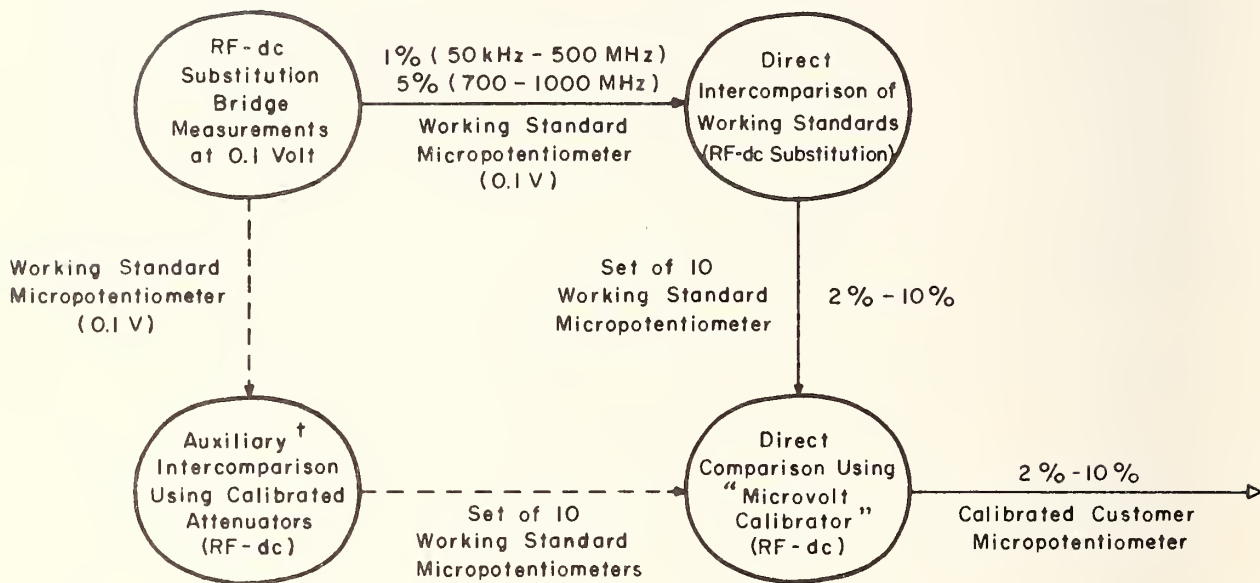

† Each Set of 10 Working Standards is Intercompared by Two Different Techniques as an Internal Check.

RF Microvoltage  
1 - 100 Microvolts; 50 kHz - 500 MHz  
100 - 100,000 Microvolts; 50 kHz - 900 MHz

MICROPOTENTIOMETER CALIBRATION:

Bias Uncertainties:

Uncertainty of the standard (thermal voltage converter)  
dc voltage measurement  
dc current measurement  
attenuation measurement  
RF leakage  
ground currents (dc)  
transfer instrument (RF receiver) sensitivity  
determination of voltage reference plane

The largest of these is the uncertainty of the thermal voltage converter.

Random Errors: Negligible

Total Uncertainty:

<u>Frequency</u> MHz	<u>Voltage Range</u> microvolts	<u>Uncertainty</u> %
0.05 - 300	1 - 100	5
300 - 500	1 - 100	10
0.05 - 10	100 - 100,000	2
10 - 300	100 - 100,000	3
300 - 900	100 - 100,000	5

Uncertainty quoted customer: Same as Total Uncertainty, above.

Notes: None


Reference: M. C. Selby, Accurate radio-frequency microvoltages,  
Trans. AIEE, Communication and Electronics, No. 6, 158-164  
(May 1953).

Personnel: M. C. Selby  
F. X. Ries

# PULSE VOLTAGE

5 - 1000 Volts

Pulse Length :  $\geq 10$  Nanoseconds

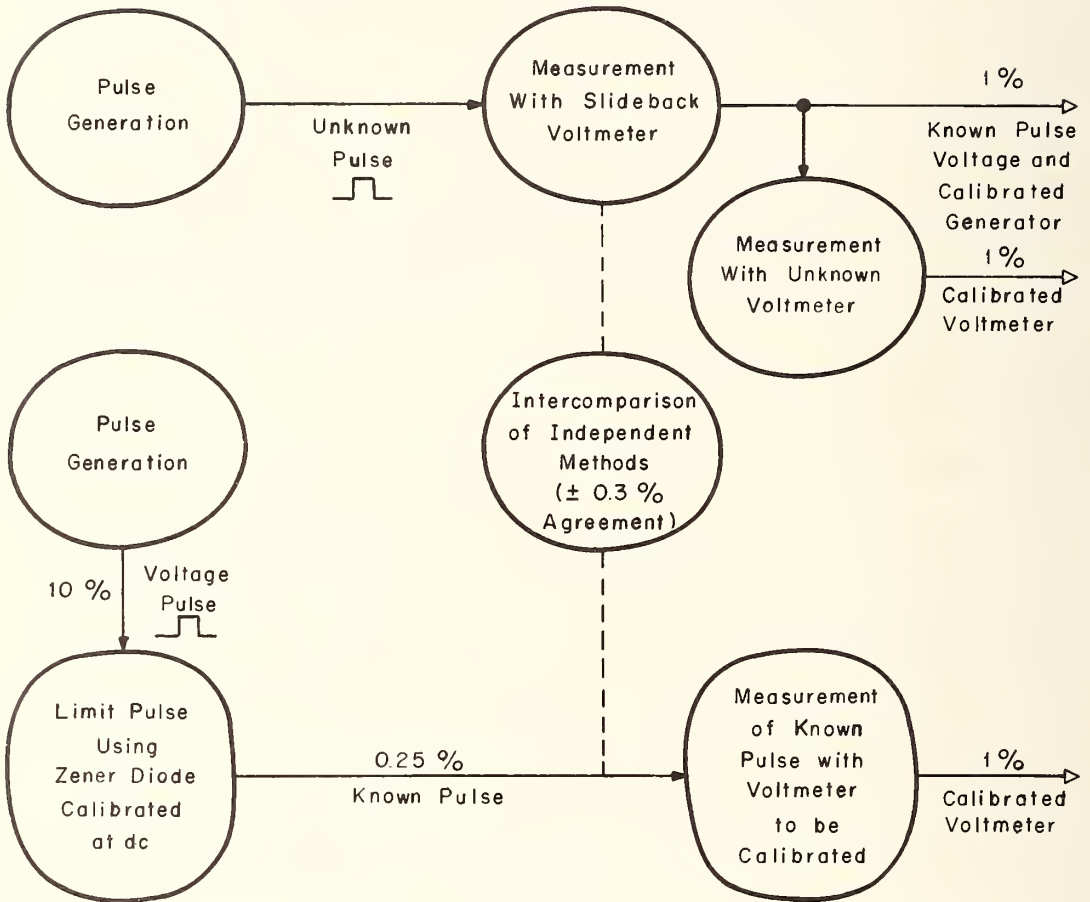



Pulse Voltage  
5 - 1000 Volts  
Pulse Duration:  $\leq 10$  Nanoseconds

SLIDEBACK VOLTMETER METHOD:

Bias Uncertainties:

Thermal effects	10 mV
Detector null sensitivity	10 mV
dc voltage	0.05 %

Random Errors: 0.1 %

Total Uncertainty: 0.15 %  $\pm$  20 mV

Uncertainty quoted customer: 1%

Notes: This measurement is made only for pulses longer than 10 nanoseconds.

Measurement agreement between this slideback voltmeter method and the standard pulse generator method is 0.3 %. See page 23-2.

Reference: A. R. Ondrejka and P. A. Hudson, Measurement standards for low and medium peak-pulse voltages, J. Res. NBS, 70C, 13 (1966).

Personnel: P. A. Hudson  
P. A. Simpson

## Pulse Voltage

### STANDARD PULSE GENERATOR (ZENER DIODE) SYSTEM:

#### Bias Uncertainties:

Thermal effects	0.1 %
10% uncertainty in input pulse voltage	0.1
dc voltage	0.05

#### Random Errors:

negligible

#### Total Uncertainty:

0.25%

Uncertainty quoted customer: 1%

Notes: This measurement is made only for pulses longer than 10 nanoseconds.

The 10% uncertainty in input pulse voltage can be either an amplitude variation of the flat top of an individual pulse or an amplitude modulation in a series of pulses, or a combination of both.

Measurement agreement between this standard pulse generator system and the slideback voltmeter system is 0.3%. See page 23-1.

Reference: A. R. Ondrejka and P. A. Hudson, Measurement standards for low and medium peak-pulse voltages, J. Res. NBS, 70C, 13 (1966).

Personnel: P. A. Hudson  
P. A. Simpson

## FIELD STRENGTH

30 Hz — 1 GHz  
20 — 400 mV/m

### MAGNETIC FIELDS - LOOP ANTENNAS

Measurement of  
Geometry and Input  
Current to  
Standard  
Transmitting  
Antenna

Field  
Calculations

3-5%

Known Field at Receiver  
20 — 200 mV/m  
30 Hz — 30 MHz

Standard Field Method  
Normally Used 30 Hz — 30 MHz

### ELECTRIC FIELDS - DIPOLE ANTENNAS

Measurement  
of Geometry  
and Voltage  
Output of  
Standard  
Receiving  
Antenna

Antenna  
Calculations

12%

Known Field at Receiver  
20 — 400 mV/m  
0.03 — 1 GHz

Standard Antenna Method  
Normally Used 30 MHz — 1 GHz

## Field Strength

### LOOP ANTENNAS, STANDARD FIELD METHOD:

30 Hz - 30 MHz  
20 - 200 mV/m

#### Bias Uncertainties:

Antenna dimensions  
Input current  
Output voltage (RF)  
Effect of earth and other objects  
Attenuation measurement

Random Errors: Not reported.

Total Uncertainty: 3% (See Notes)

Uncertainty quoted customer: 3%

Notes: The uncertainty of calibration is determined from two independent measurement methods: (1) the standard-field method, (2) the standard-antenna method. The standard-field method is used to calibrate loop antennas. The loop is calibrated in terms of a quasi-static magnetic field and converted to the equivalent electric field based on free space calibrations.

References: F. M. Greene, NBS field-strength standards and measurements (30 Hz to 1000 MHz), Proc. IEEE, 55, 970 (June 1967).

H. E. Taggart, Field-strengths and RFI standards at the National Bureau of Standards, 1968 IEEE Electromagnetic Compatibility Symposium Record, IEEE 68CIZ-EMC, 149-158.

Personnel: F. M. Greene  
H. E. Taggart

## Field Strength

### DIPOLE ANTENNAS, STANDARD ANTENNA METHOD:

30 - 1000 MHz  
20 - 400 mV/m

#### Bias Uncertainties:

Antenna dimensions  
Output voltage (dc or RF)  
Effect of earth and other objects  
Attenuation measurements

Random Errors: Not reported.

Total Uncertainty: 12% (See notes)

Uncertainty quoted customer: 12%

Notes: The uncertainty of calibration is determined from two independent measurement methods: (1) the standard-field method, (2) the standard-antenna method. The standard-antenna method is used to calibrate dipole antennas. The dipole antenna is calibrated by placing it in a known field at a specified height above ground.


References: F. M. Greene, NBS field-strength standards and measurements (30 Hz to 1000 MHz), Proc. IEEE, 55, 970 (June 1967).

H. E. Taggart, Field-strengths and RFI standards at the National Bureau of Standards, 1968 IEEE Electromagnetic Compatibility Symposium Record, IEEE 68CIZ-EMC, 149-158.

Personnel: F. M. Greene  
H. E. Taggart

# FIELD STRENGTH METER

30 Hz - 1 GHz  
(20 - 400 mV/m)

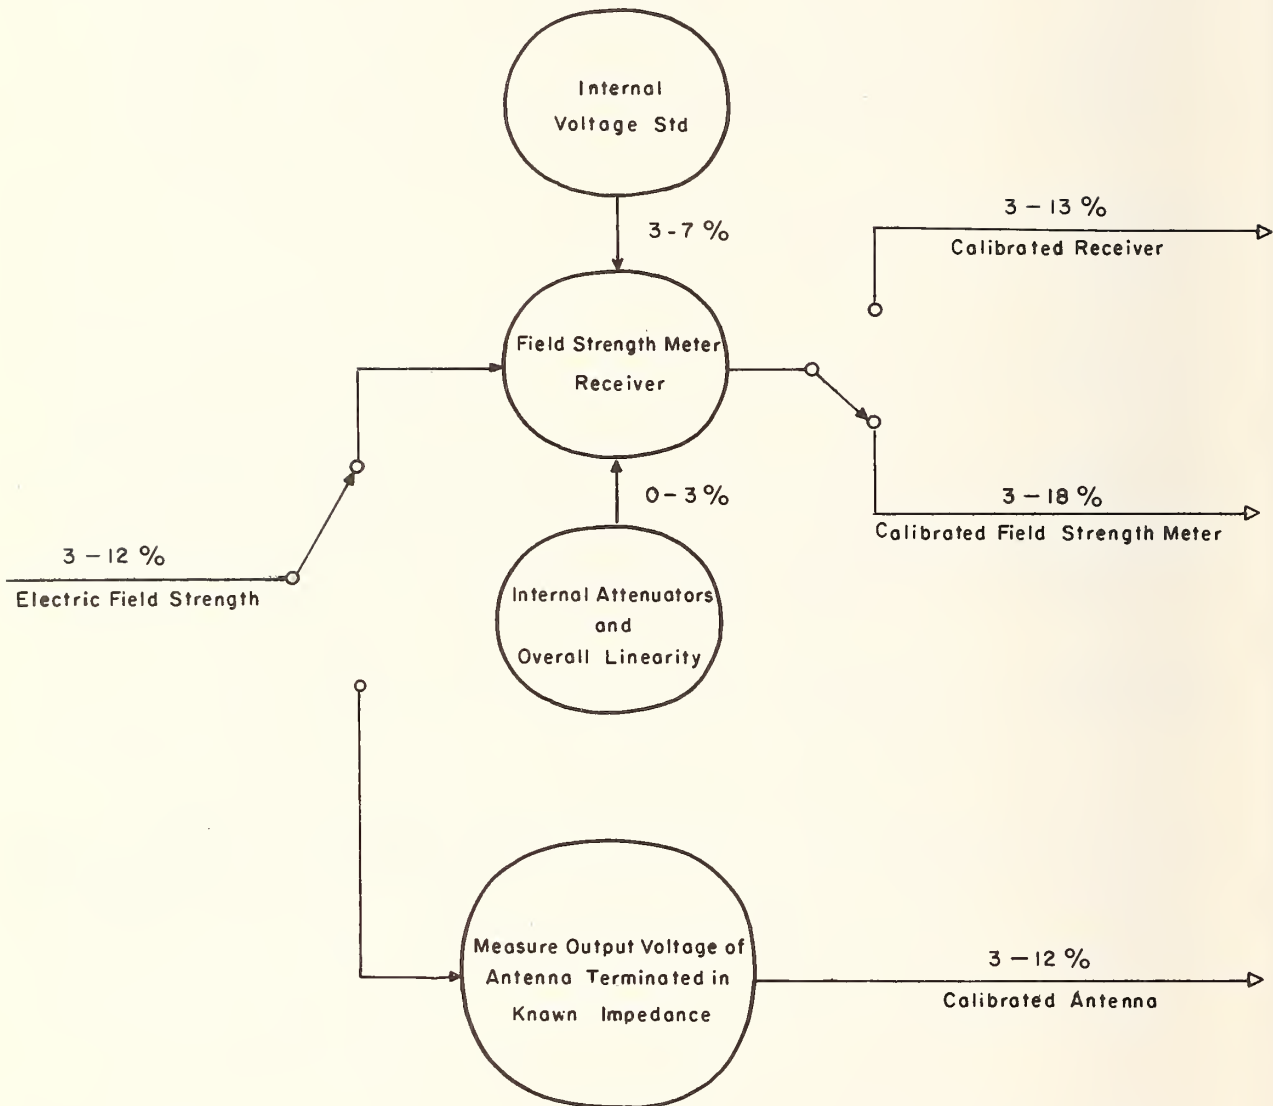

Field Strength Meter  
30 Hz - 1 GHz  
20 - 400 mV/m

RECEIVER CALIBRATION: (See Notes)

Bias Uncertainties:

Voltage measurement	30 Hz - 100 MHz	3%
	100 - 500 MHz	5%
	500 - 900 MHz	7%
Calibration of attenuators and overall linearity of receiver	30 Hz - 400 MHz	0.1dB+0.03dB/10dB
	400 - 1000 MHz	0.1dB+0.05dB/10dB

Random Errors: Not reported.

Total Uncertainty: 3% + 0.1dB + 0.03dB/10dB to  
7% + 0.1dB + 0.05dB/10dB

Uncertainty quoted customer:

30 Hz - 100 MHz	5%
100 - 500 MHz	7%
500 - 1000 MHz	10%

Notes: As shown on page 25, a field strength meter consisting of an antenna and a receiver (which itself consists of a detector, internal attenuators and a voltmeter) can be calibrated as a unit (the "switch" is shown in that position), or the receiver and the antenna can be calibrated separately (the other "switch" position). When calibrated as a unit, the uncertainties are those as given on pages 24-1 and 24-2. When calibrated separately, the uncertainties are as given on pages 25-1 and 25-2.

Reference: None

Personnel: F. M. Greene  
H. E. Taggart

## Antennas

### ANTENNA CALIBRATION:

Loop antennas: 30 Hz - 30 MHz

Dipole antennas: 30 - 1000 MHz

Bias Uncertainties: See Notes.

Random Errors: Not reported.

Total Uncertainty: Loop antennas, 3%; dipole antennas, 12%.

Uncertainty quoted customer: Loop antennas, 3%; dipole antennas, 12%.

Notes: As shown on page 25 the calibration of an antenna by itself is done by placing the antenna in a known field, terminating it in a known impedance, and measuring its output voltage. The total uncertainty is taken to be equal to that of the uncertainty in the field itself, which is obtained as on pages 24, 24-1, and 24-2.

References: F. M. Greene, NBS field-strength standards and measurements (30 Hz to 1000 MHz), Proc. IEEE, 55, 970 (June 1967).

H. E. Taggart, Field-strengths and RFI standards at the National Bureau of Standards, 1968 IEEE Electromagnetic Compatibility Symposium Record, IEEE 68CIZ-EMC, 149-158.


Personnel: F. M. Greene  
H. E. Taggart



## ATTENUATION: COAXIAL SYSTEMS

10 - 18,000 MHz

0 - 140 dB

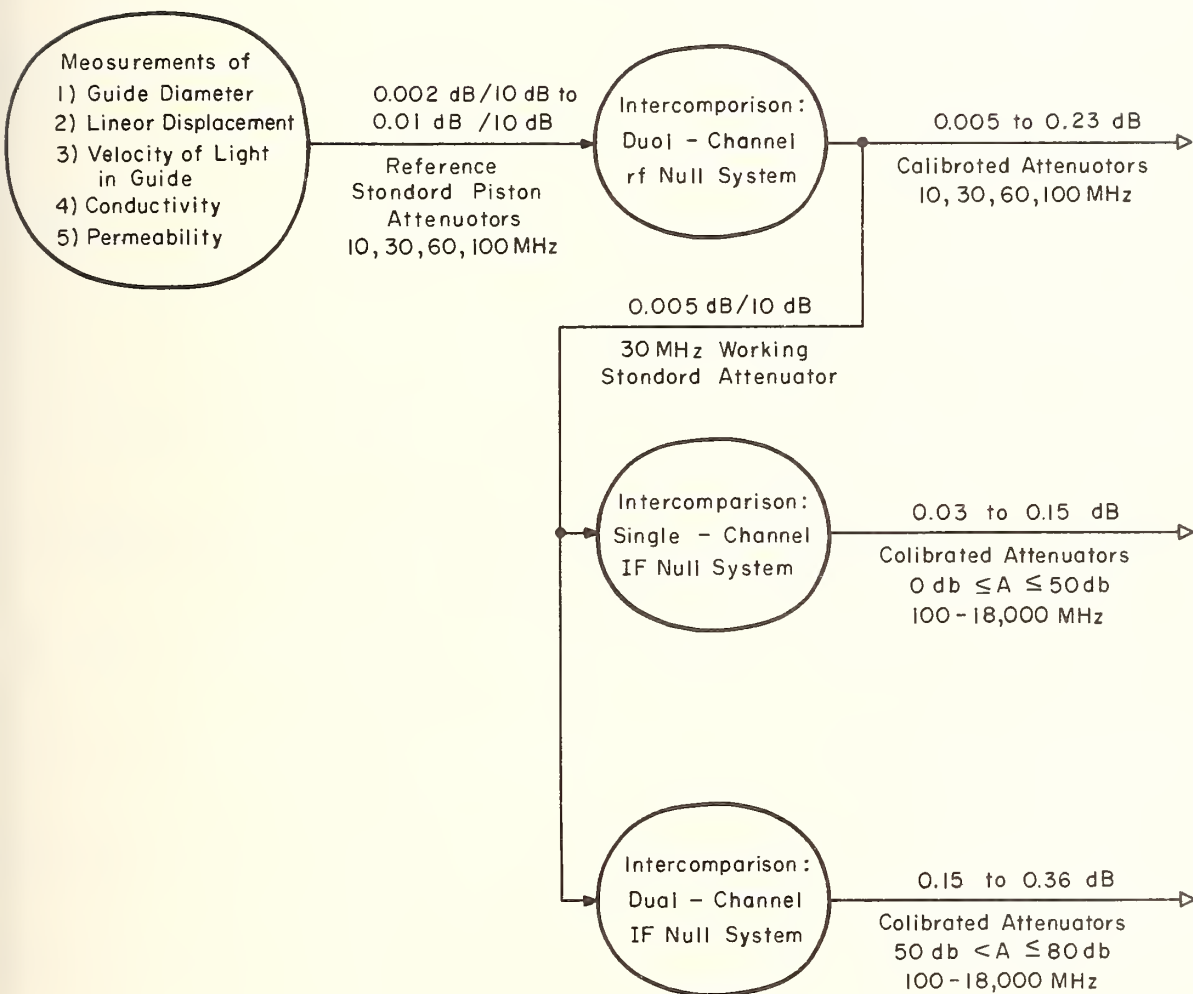

## Attenuation: Coaxial Systems

### PISTON ATTENUATION:

10, 30, 60, 100 MHz  
0 - 140 dB

### Bias Uncertainties:

Coaxial waveguide diameter	0.0003dB/10dB
Linear displacement of receiving coil	0.001dB/10dB-0.01dB/10dB
Velocity of electromagnetic waves in medium inside guide	negligible
RF conductivity of guide	0.00026dB/10dB
RF permeability of guide	negligible

Random Errors: negligible

Total Uncertainty: 0.002dB/10dB-0.01dB/10dB

Uncertainty quoted customer: See Notes.

Notes: Lower limits of these measurements are not available to customers, but are used only to establish the uncertainty in the National Bureau of Standards reference standard piston attenuators.

Reference: C. M. Allred and C. C. Cook, A precision RF attenuation calibration system, IRE Trans. Instr. I-9, 268 (1960).

Personnel: R. T. Adair

## Attenuation: Coaxial Systems

### DUAL-CHANNEL RF NULL SYSTEM:

10, 30, 60, 100 MHz  
0 - 140dB

### Bias Uncertainties:

Reference standard piston attenuator	0.002dB/10dB-0.01dB/10dB
Mismatch errors	0.001dB/10dB
Leakage	0.001dB/10dB

Random Errors: See Notes. 0.001 - 0.06dB

---

Total Uncertainty: 0.005 - 0.23dB

Uncertainty quoted customer: Uncertainty is estimated for each individual case and those estimates are reported directly to the customer.

Notes: The random errors are reported to the customer as 3 times the standard error, which is defined on the calibration report. Typical standard errors range from about 0.001dB at low attenuations up to about 0.06dB at high attenuations.

Explicit numbers for mismatch errors and leakage errors are estimated for each individual case.

The maximum range of the standard piston attenuators is 140dB at 30 MHz and 100dB at 10, 60, and 100 MHz.

The numbers quoted for bias uncertainties are typical values, and may not apply to a particular calibration.

Reference: C. M. Allred and C. C. Cook, A precision RF attenuation calibration system, IRE Trans. Instr., I-9, 269 (1960).

Personnel: R. T. Adair

Attenuation: Coaxial Systems

SINGLE-CHANNEL IF NULL SYSTEM:

100 - 18,000 MHz  
0 - 50dB

Bias Uncertainties:

Mismatch errors	0.01dB/10dB
Mixer non-linearity	0.005dB/10dB
Noise, as a systematic error	0.005dB/10dB
Leakage	0.005dB/10dB
Working standard piston attenuator uncertainty	0.005dB/10dB

Random Errors: See Notes.

Total Uncertainty: 0.03 - 0.15dB

Uncertainty quoted customer: Reported as estimated in each individual case.

Notes: The random errors include such effects as connector precision, generator and detector fluctuations, and noise or instability in the unknown attenuator. They are reported to the customer as 3 times the standard error, with a sample size usually 6, giving about a 96% confidence limit. These random errors are generally negligible.

Explicit numerical entries for the bias uncertainties are estimated in each individual case.

Reference: David H. Russell, An unmodulated twin-channel microwave measurement system, ISA Trans., 4, 162 (1965).

Personnel: R. T. Adair

## Attenuation: Coaxial Systems

### DUAL-CHANNEL IF NULL SYSTEM:

100 - 18,000 MHz  
50 - 80dB

### Bias Uncertainties:

Mismatch errors	0.01dB/10dB-0.02dB/10dB
Mixer non-linearity	0.005dB/10dB-0.01dB/10dB
Noise, as a systematic error	0.005dB/10dB
Leakage	0.005dB/10dB
Working standard piston attenuator	0.005dB/10dB

Random Errors: See Notes, page 26-3.

Total Uncertainty: 0.15 - 0.36dB

Uncertainty quoted customer: Reported as estimated in each individual case.

Notes: Explicit numerical entries for the bias uncertainties are estimated in each individual case.

References: D. Russell and W. Larson, RF attenuation, Proc. IEEE, 55, 942 (1967).

B. O. Weinschel, G. U. Sorger, and A. L. Hedrich, Relative voltmeter for VHF/UHF signal generator attenuator calibration, IRE Trans. Instr., I-8, 22 (1959).


A. L. Hedrich, B. O. Weinschel, G. U. Sorger, and S. J. Raff, Calibration of signal generator output voltage in the range of 100 to 1000 megacycles, IRE Trans. Instr., I-7, 275 (1958).

Personnel: R. T. Adair

## ATTENUATION : WAVEGUIDE SYSTEMS

1.7 - 40 GHz

0 - 50 dB

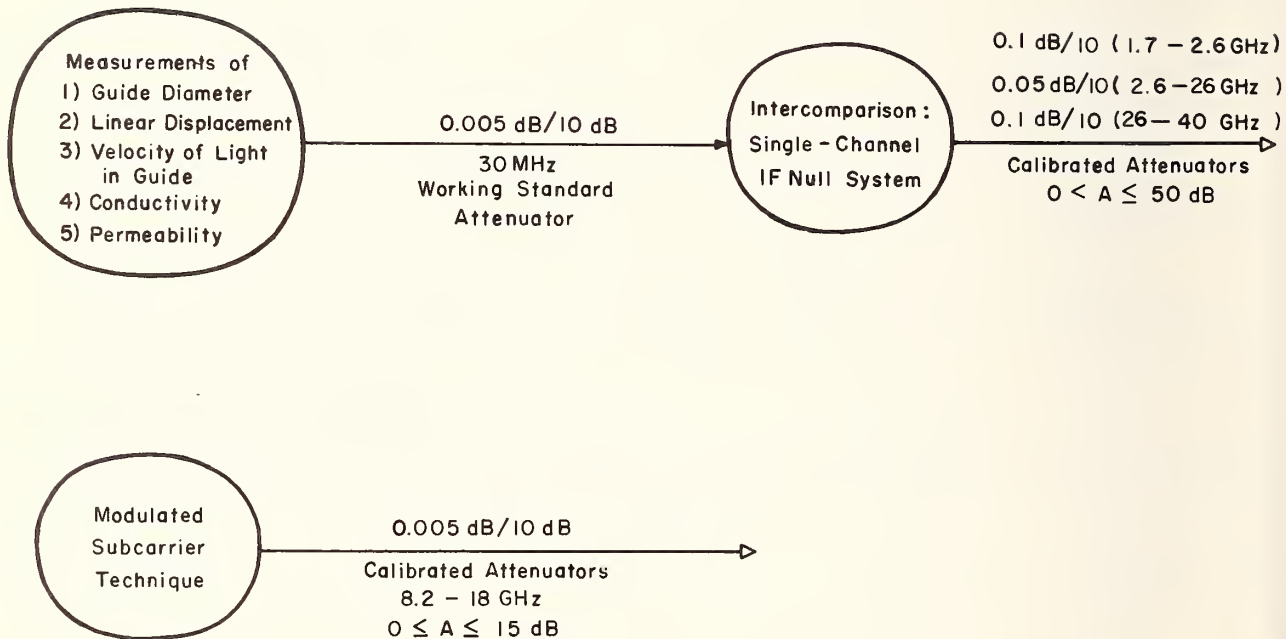

Attenuation: Waveguide Systems

1.7 - 40 GHz

0 - 50dB

PISTON ATTENUATOR: See page 26-1.

SINGLE-CHANNEL IF SYSTEM:

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagram, page 27-2

Uncertainty quoted customer:

0.1dB/10dB;            1.7 - 2.6 GHz

0.05dB/10dB;        2.6 - 26 GHz

0.1dB/10dB;        26 - 40 GHz

Notes: None


Reference: R. E. Larson, Microwave measurements in the NBS  
Electronic Calibration Center, Proc. IEE (London), 109, part B,  
suppl. 23, 644 (1962).

Personnel: W. Larson

# IF ATTENUATION CALIBRATION SYSTEM ERROR FLOW DIAGRAM

FREQUENCY 1.7 - 40 GHz

WR 430 ----- WR 28

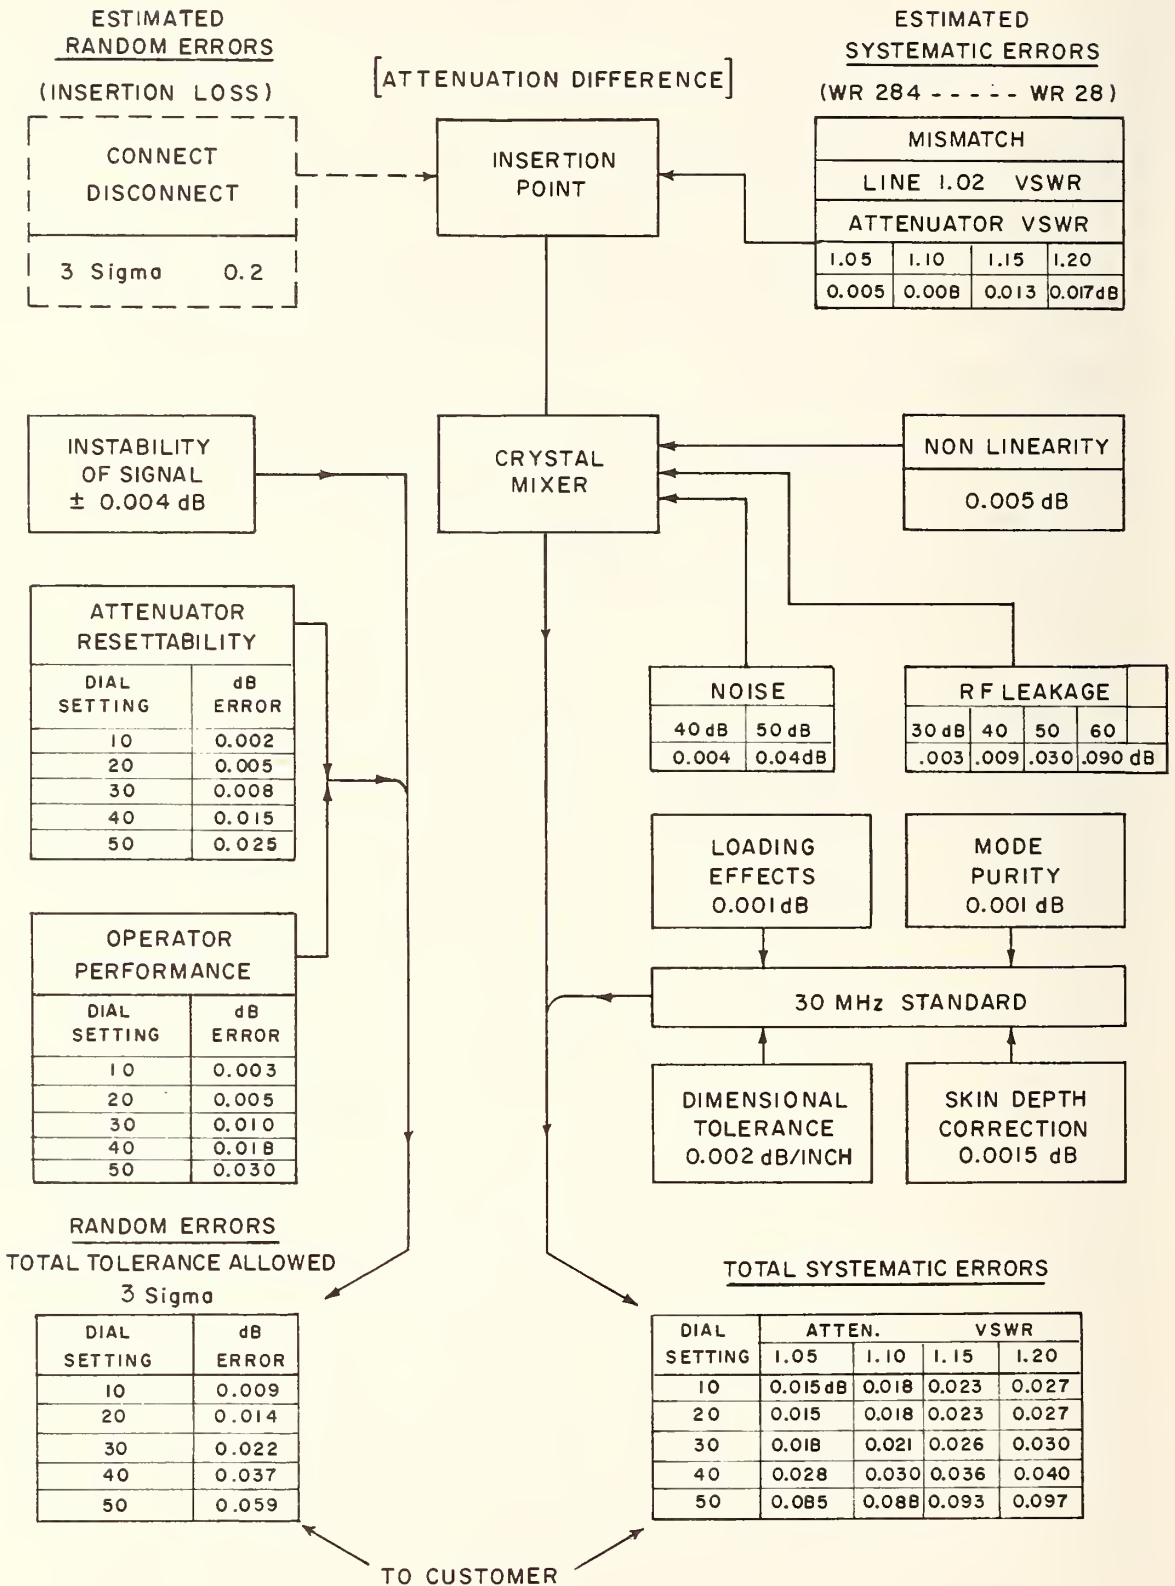



Attenuation: Waveguide Systems

MODULATED SUBCARRIER TECHNIQUE:

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagram, page 27-4

Uncertainty quoted customer: 0.005dB/10dB; 8.2 - 18.0GHz


Notes: none

Reference: G. E. Schafer and R. R. Bowman, A modulated subcarrier technique of measuring microwave attenuation, Proc. IEE (London), 109, part B, suppl. 23, 783 (1962).

Personnel: W. Larson

# ATTENUATION : WAVEGUIDE SYSTEMS


## ERROR FLOW CHART FOR MODULATED SUBCARRIER

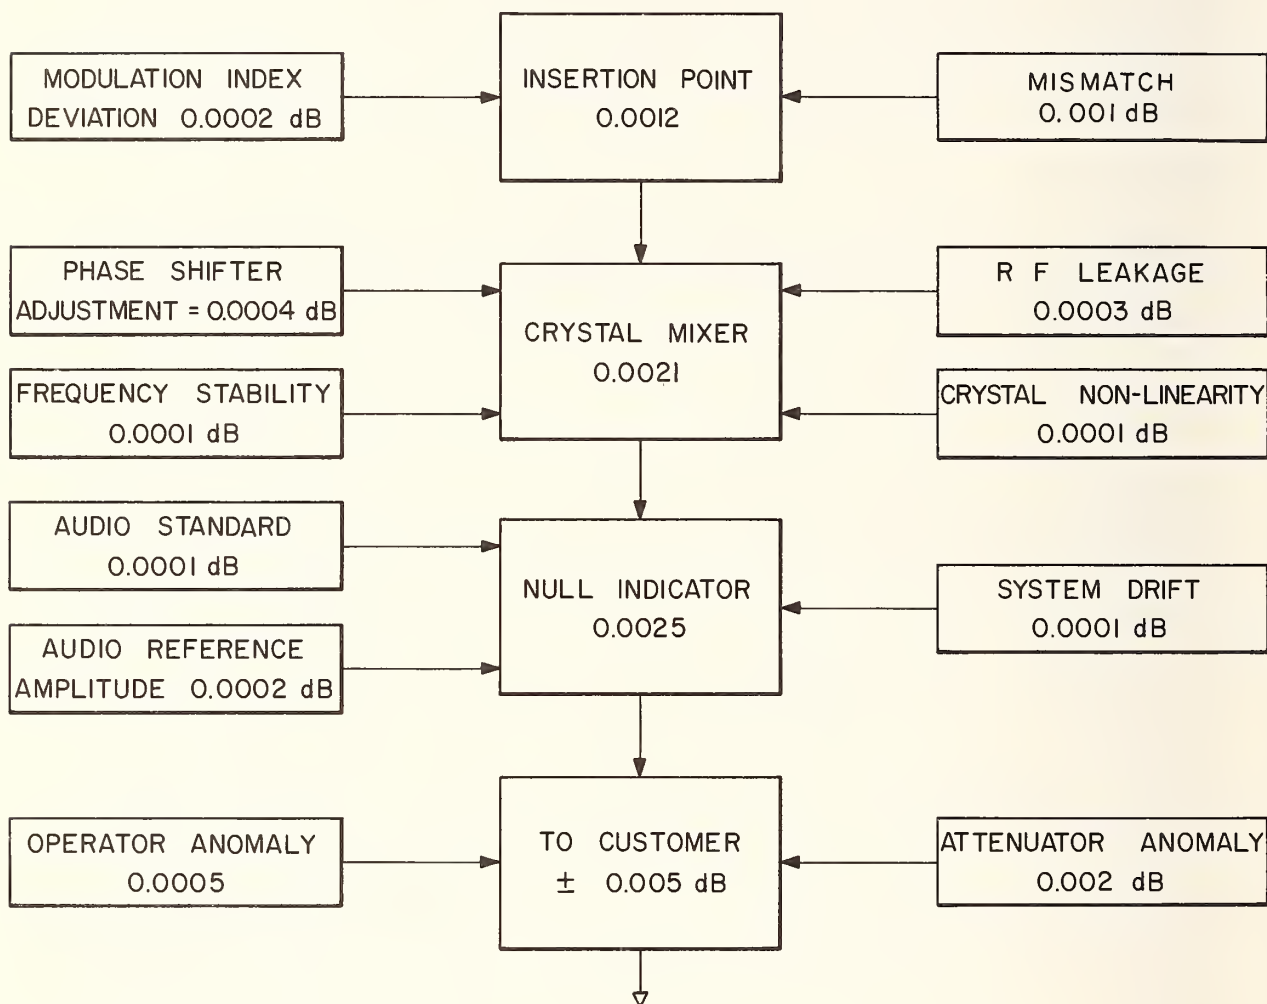

# PHASE SHIFT IN COAXIAL PHASE SHIFTERS

30 - 12,400 MHz

0 - 360 Degrees

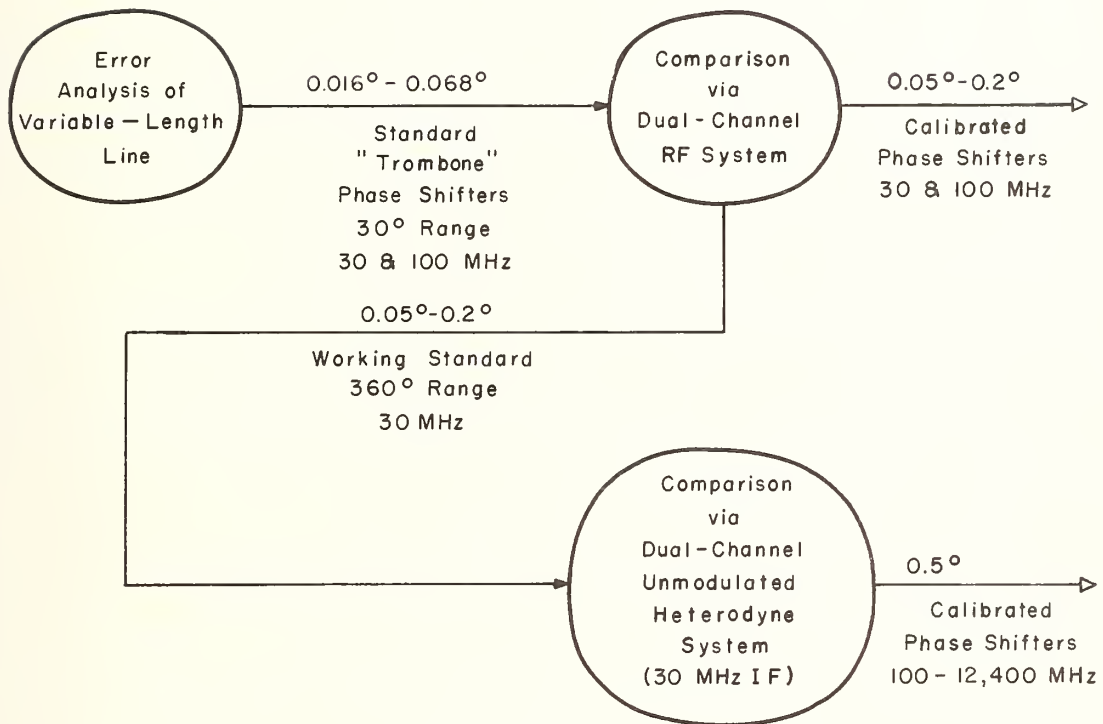

Phase Shift in Coaxial Two-Ports  
30 and 100 MHz  
0.05 - 360 Degrees

DUAL-CHANNEL RF COMPARISONS:

Bias Uncertainties:

Mechanical stability and length measurement in trombone phase shifter	0.004 - 0.048 degree (30 MHz) 0.012 - 0.144 (100 MHz)
Mismatch of trombone	0.012
Phase shift in standard attenuator	0.01
Resolution in auxiliary phase shifter	0.02 - 0.13

Random Errors:

negligible

Total Uncertainty:

0.046 - 0.2 degree (30 MHz)  
0.054 - 0.208 degree (100 MHz)

Uncertainty quoted customer: Reported as estimated for each individual case.

Notes: Where there is a range of uncertainty in the list above, the uncertainty is a function of the phase shift in the coaxial two-port.

Reference: David H. Russell, An unmodulated twin-channel microwave measurement system, ISA Trans., 4, 162 (1965).

Personnel: R. T. Adair

Phase Shift in Coaxial Phase Shifters  
30 - 12,400 MHz  
0 - 360 degrees

DUAL-CHANNEL RF COMPARISONS:

Bias Uncertainties:

Mechanical stability and length measurement in trombone phase shifter	0.004 - 0.048 degree (30 MHz) 0.012 - 0.144 (100 MHz)
Mismatch of trombone	0.012
Phase shift in standard attenuator	0.01
Resolution in auxiliary phase shifter	0.02 - 0.13

Random Errors: negligible

---

Total Uncertainty: 0.05 - 0.2 degree (30 MHz)  
0.05 - 0.21 degree (100 MHz)

Uncertainty quoted customer: Reported as estimated for each individual case.

Notes: Where there is a range of uncertainty in the list above, the uncertainty is a function of the phase shift in the coaxial phase shifter.

Reference: David H. Russell, An unmodulated twin-channel microwave measurement system, ISA Trans., 4, 162 (1965).

Personnel: R. T. Adair

## Phase Shift in Coaxial Phase Shifters

### DUAL-CHANNEL IF UNMODULATED COMPARISON SYSTEM:

100 - 18,000 MHz  
0 - 360 degrees

#### Bias Uncertainties:

30 MHz working standard (resolver)	0.2 degree
Mismatch of unknown phase shifter	0.05
Mixer non-linearity (See Notes)	
Resolution (null sensitivity)	0.1

Random Errors: negligible

Total Uncertainty: < 0.35 degree

Uncertainty quoted customer: 0.5 degree.

Notes: The mixer non-linearity error is determined separately for each calibration.

Reference: David H. Russell, An unmodulated twin-channel microwave measurement system, ISA Trans., 4, 162 (1965).

Personnel: R. T. Adair


PHASE SHIFT  
IN WAVEGUIDE PHASE SHIFTERS

WR 62 : 12.4 - 18.0 GHz


WR 90 : 8.20 - 12.4 GHz

WR 137 : 5.85 - 8.20 GHz

0 - 720 Degrees

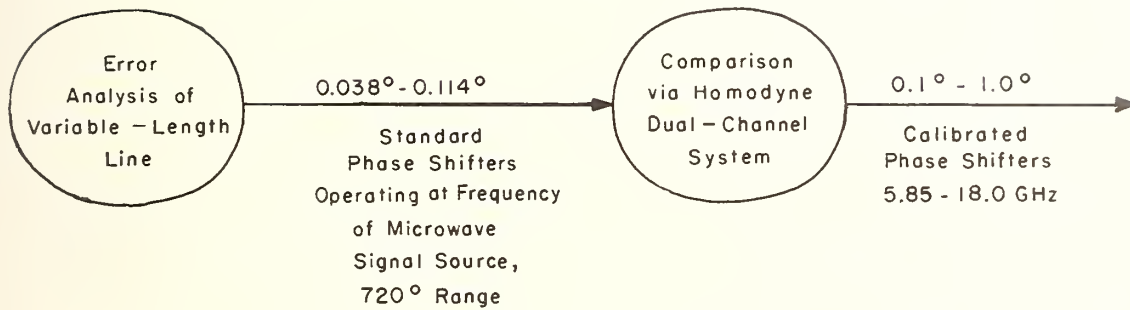

**PHASE SHIFT IN WAVEGUIDE PHASE SHIFTERS**  
**ERROR FLOW DIAGRAM**  
 FREQUENCY 5.85 - 18.0 GHz WR 62, WR 90 and WR 137

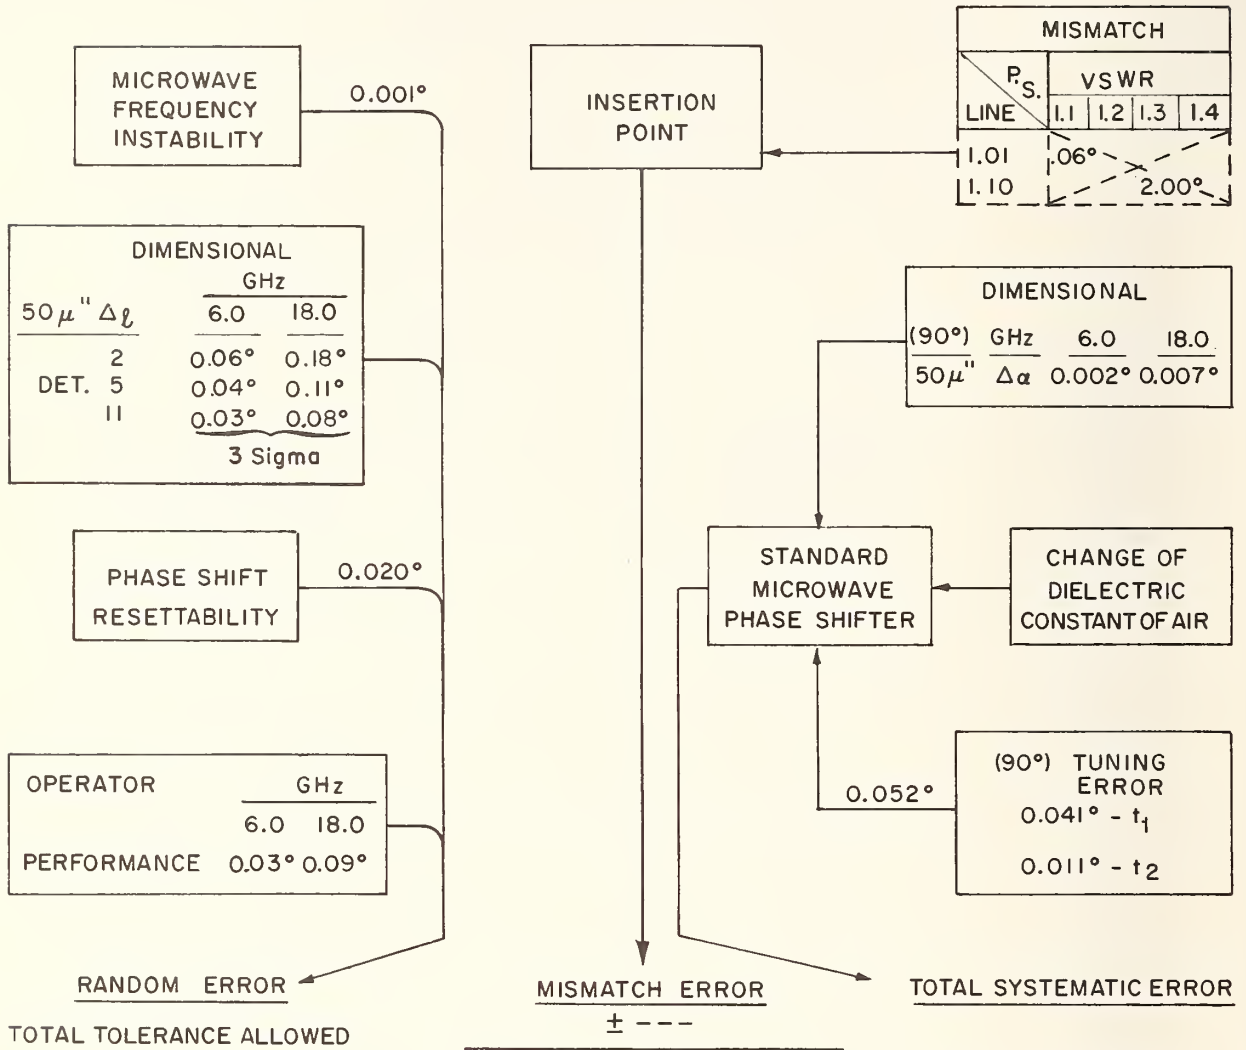

**3 Sigma**

Det.	GHz	
	6.0	18.0
2	0.11°	0.29°
5	0.09°	0.22°
11	0.08°	0.19°

P. S. LINE	VSWR			
	1.10	1.20	1.30	1.40
1.01	.060°	.110°	.150°	.195°
1.02	.120°	.210°	.300°	.400°
1.05	.320°	.560°	.810°	.960°
1.10	.780°	1.25°	1.60°	2.00°

φ	GHz	
	6.0	18.0
90°	0.055°	0.056°
180°	0.079°	0.081°
360°	0.011°	0.013°

TOTAL UNCERTAINTY IS ARITHMETICAL SUM (LIKE SIGNS) OF THE  
 RANDOM ERROR, AND TOTAL SYSTEMATIC ERROR

↓  
 TO CUSTOMER



Phase Shift in Waveguide Phase Shifters  
5.85 - 18 GHz  
0 - 720 degrees

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagram, page 28-1

Uncertainty quoted customer: Same as Total Uncertainty.

Notes: The VSWR of the phase shifter must be less than 1.5. Resolution of the phase shifter should be  $0.5^\circ$  or better.

Reference: D. A. Ellerbruch, Evaluation of a microwave phase measurement system, J. Res. NBS, 69C, 55 (1965).

Personnel: W. Larson  
E. D. Hall

## REFLECTION COEFFICIENT MAGNITUDE OF WAVEGUIDE DEVICES

WR 42 : 18.0 - 26.5 GHz

WR 62 : 12.4 - 18.0

WR 90 : 8.2 - 12.4

WR 112 : 7.05 - 10.0


WR 137 : 5.85 - 8.2

WR 187 : 3.95 - 5.85

WR 284 : 2.6 - 3.95

$$0.024 \leq |\Gamma| \leq 0.2$$

Power Level : 0.01 mW

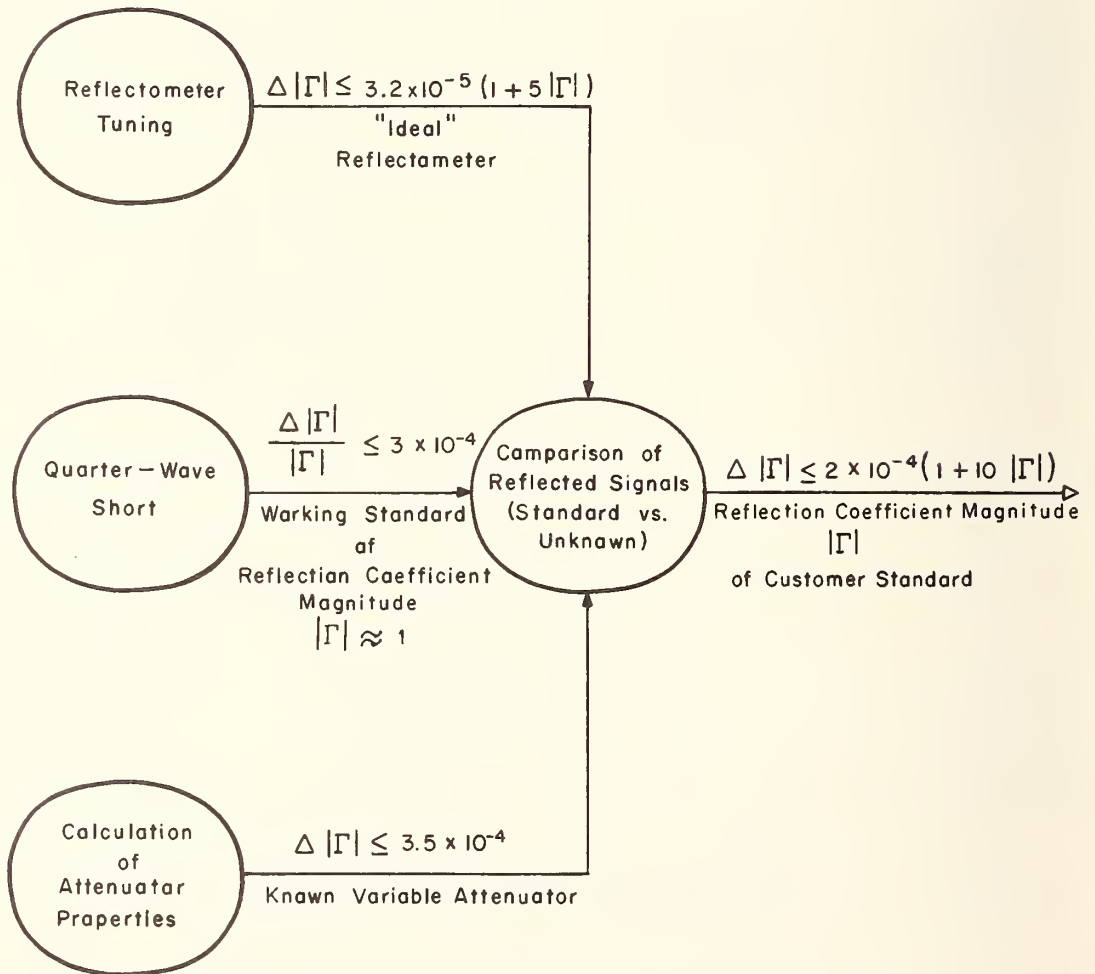

## Reflection Coefficient Magnitude of Waveguide Devices

WR 42:	18.0	-	26.5	GHz
WR 62:	12.4	-	18.0	
WR 90:	8.2	-	12.4	
WR 112:	7.05	-	10.0	
WR 137:	5.85	-	8.2	
WR 187:	3.95	-	5.85	
WR 284:	2.6	-	3.95	
Power Level:	0.01 - 4 mW			

Bias Uncertainties:

Random Errors:

Total Uncertainty:

} See Error Flow Diagrams, pages 30-2 and 30-3

Uncertainty (typical) quoted customer:

$$\begin{aligned}
 &|\Gamma| \geq 0.024, \\
 &\Delta |\Gamma| = 2 \times 10^{-4} (1 + 6|\Gamma|). \\
 &|\Gamma| < 0.024, \\
 &\Delta |\Gamma| = 2 \times 10^{-4} (1 + 10|\Gamma|).
 \end{aligned}$$

Notes: The uncertainties due to the precision waveguide section (see error flow diagrams, pages 30-2 and 30-3) are as follows:

<u>Waveguide</u>	<u>Uncertainty in <math> \Gamma </math></u>
WR 284	< 0.0001
WR 187	< 0.0001
WR 137	< 0.0001
WR 112	< 0.0001
WR 90	< 0.00015
WR 62	< 0.0001
WR 42 (square flange)	< 0.0004
WR 42 (round flange)	< 0.0003


Reference: Wilbur J. Anson, A guide to the use of the modified reflectometer technique of VSWR measurement, J. Res. NBS, 65C, 217 (1961).

Personnel: B. C. Yates

# ERROR FLOW DIAGRAM

## FOR REFLECTION COEFFICIENT MAGNITUDE OF WAVEGUIDE DEVICES

$$|\Gamma| < 0.024$$

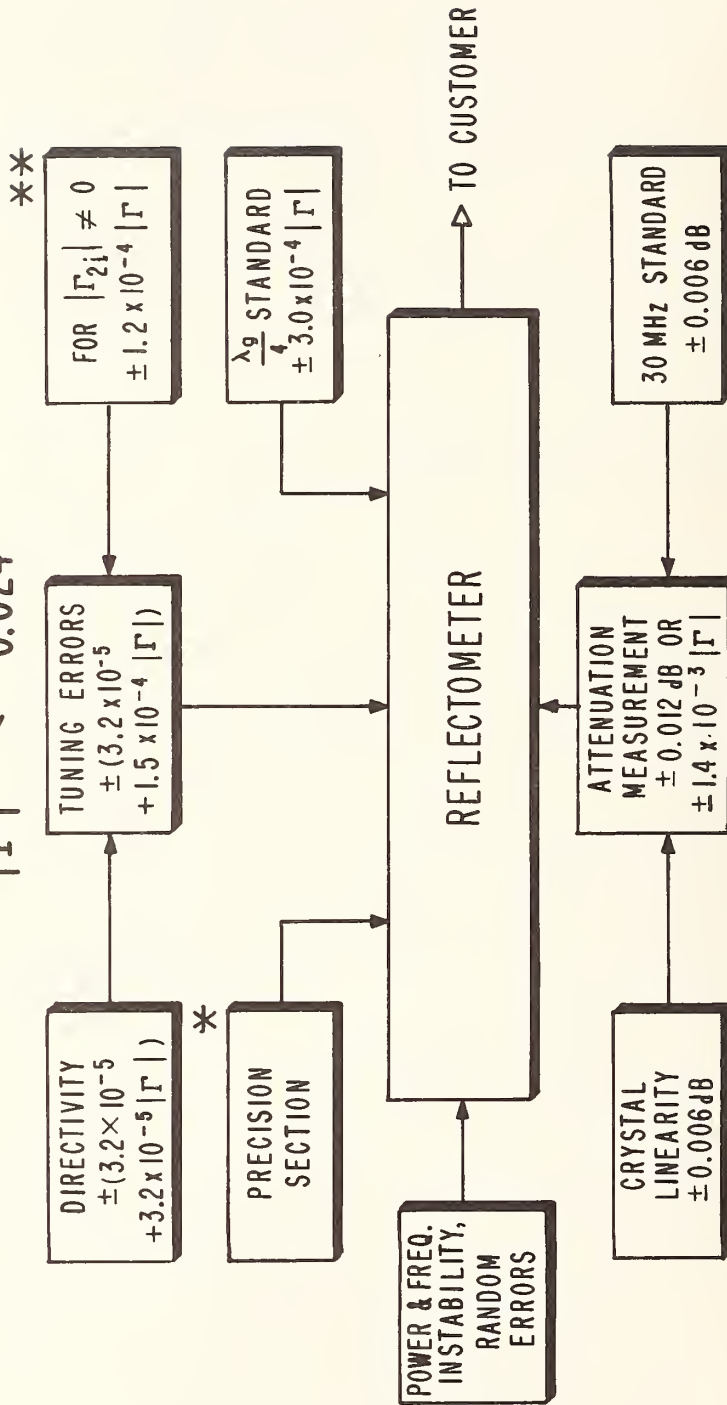


\* See Notes

\*\* See Reference

# ERROR FLOW DIAGRAM

## FOR REFLECTION COEFFICIENT MAGNITUDE OF WAVEGUIDE DEVICES

$$|\Gamma| \geq 0.024$$

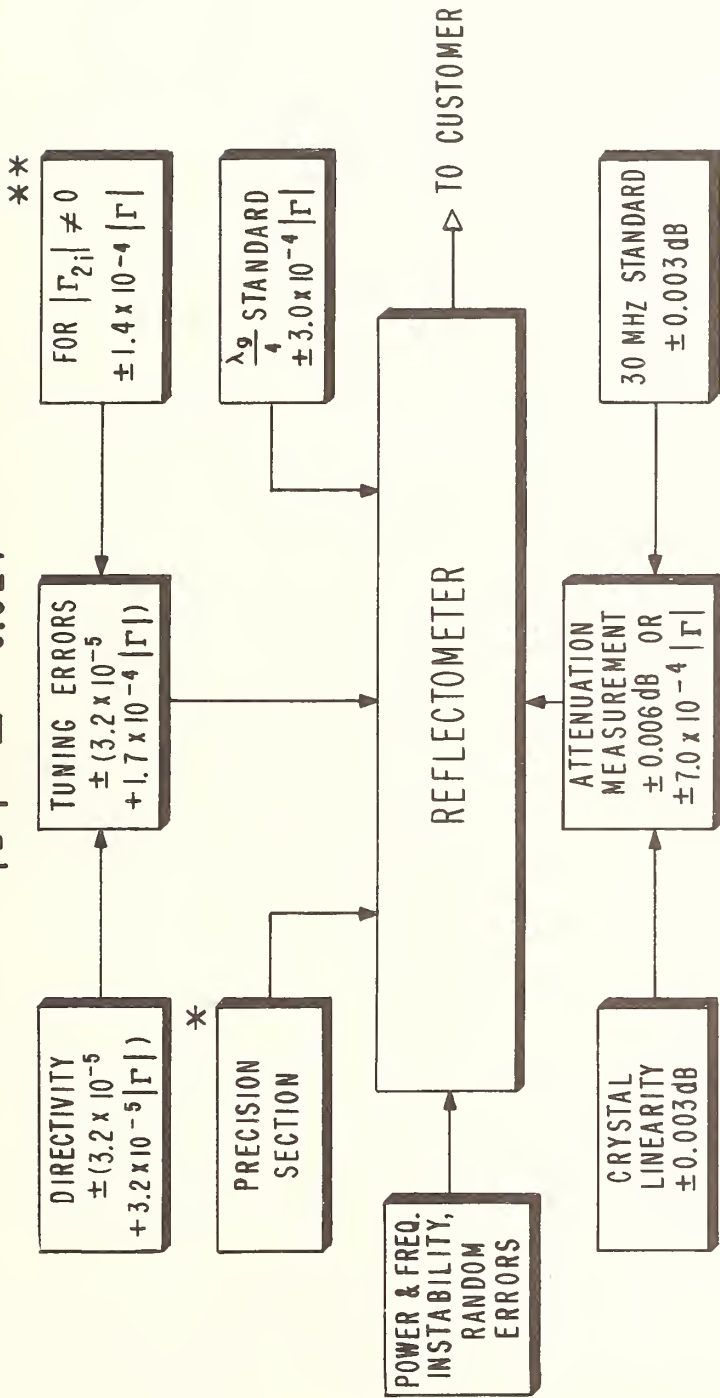


\* See Notes

\*\* See Reference

## DISTRIBUTED PARAMETERS IN COAXIAL SYSTEMS

0.5 - 8 GHz

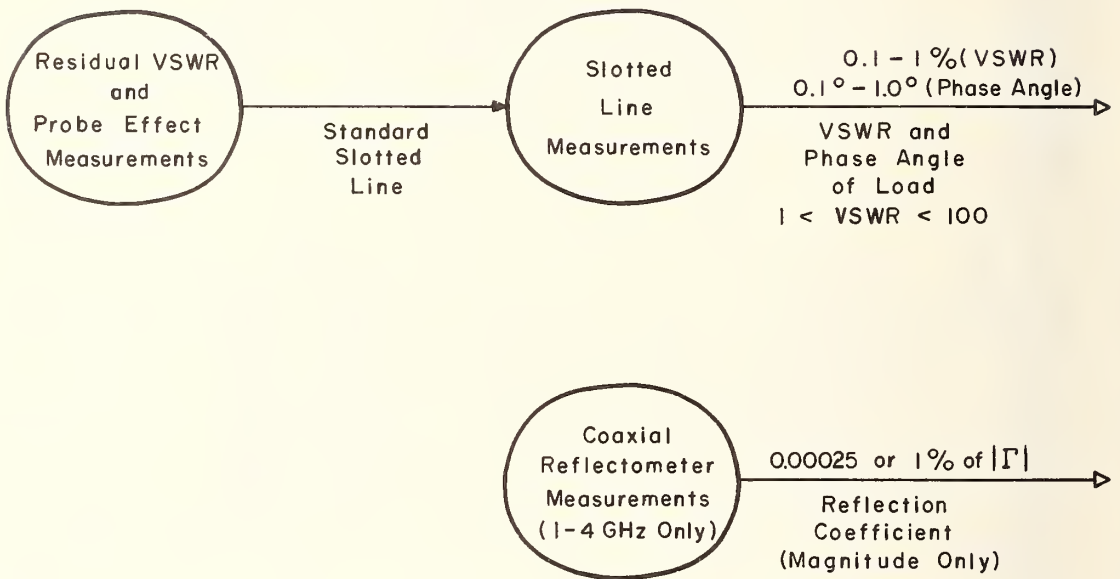

Distributed Parameters in Coaxial Systems  
0.5 - 8 GHz

SLOTTED LINE MEASUREMENTS:

500 MHz - 8 GHz  
 $1 \leq \text{VSWR} \leq 100$

Bias Uncertainties:

Residual VSWR

- (a) Imperfect transition from connector to slotted line
- (b) Variation in characteristic impedance
- (c) Slot effects

Probe Effects

- (a) Variation of probe coupling with probe position
- (b) Probe loading of the slotted line

Line losses

Detector nonlinearity

Determination of the position of a voltage minimum

Power and frequency instability

Random Errors: Negligible

Total Uncertainty:

0.1 - 1.0% for  $1 \leq (\text{VSWR}) \leq 4$   
0.1 - 1 degree (phase angle)

Uncertainty quoted customer: As above.


Notes: Page 31-2 gives some details of the error sources. Further details are available from R. L. Jesch (below).

Uncertainty figures assume precision 14mm coaxial connectors. Uncertainties for other connectors and larger VSWR's will, in most cases, be larger.

Reference: R. L. Jesch and R. M. Jickling, Impedance measurements in coaxial waveguide systems, Proc. IEEE, 55, 912 (June 1967).

Personnel: R. L. Jesch

**ERROR FLOW DIAGRAM FOR COAXIAL IMPEDANCE STANDARDS EQUIPPED WITH PRECISION 14mm COAXIAL CONNECTORS MEASURED WITH A 14 mm COAXIAL SLOTTED LINE EMPLOYING REGULAR MEASUREMENT TECHNIQUES UP TO 8 GHz**

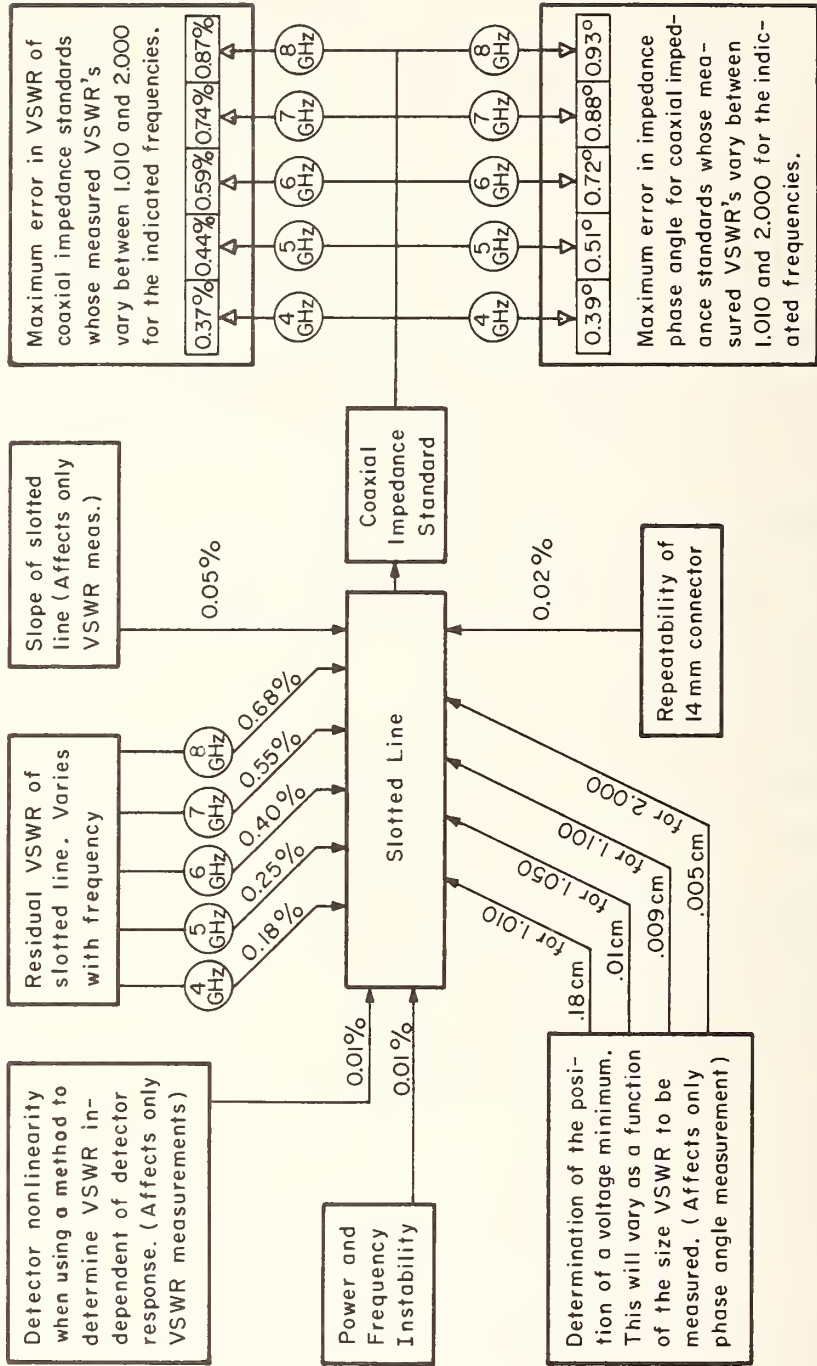



Distributed Parameters in Coaxial Systems  
1 - 4 GHz

COAXIAL REFLECTOMETER MEASUREMENTS:

$$1 - 4 \text{ GHz}$$
$$0 \leq |\Gamma| \leq 1$$

Bias Uncertainties:

Tuning errors  
Detector errors  
Precision air-line section  
Power and frequency instability

Random Errors: Negligible

Total Uncertainty:

$$\text{for } 0 \leq |\Gamma| \leq 0.025: \Delta |\Gamma| \leq 0.00025$$
$$\text{for } 0.025 \leq |\Gamma| \leq 1: \Delta |\Gamma| \leq 1\% |\Gamma|$$

Uncertainty quoted customer: As above

Notes: In other than exacting standards work, or unless specially requested, this measurement is rarely done for customers. Satisfactory results may be obtained at a much lower cost by the slotted-line technique.

Reference: W. E. Little and J. P. Wakefield, Measurement of Precision coaxial connectors using reflectometer techniques, IEEE International Conv. Rec., pt. 11, 89-97, March 1965.

Personnel: R. J. Jesch

# HIGH FREQUENCY IMMITTANCE


30 KHz - 300 MHz

C :  $10^{-12}$  -  $10^{-7}$  F

L :  $10^{-8}$  - 1 H

R : 0.1 -  $10^6 \Omega$

Effective Resonating Capacitance ( $C_e$ ) :  $35 \times 10^{-17}$  -  $450 \times 10^{-2}$  F  
 Effective Quality Factor ( $Q_e$ ) : 90 - 700

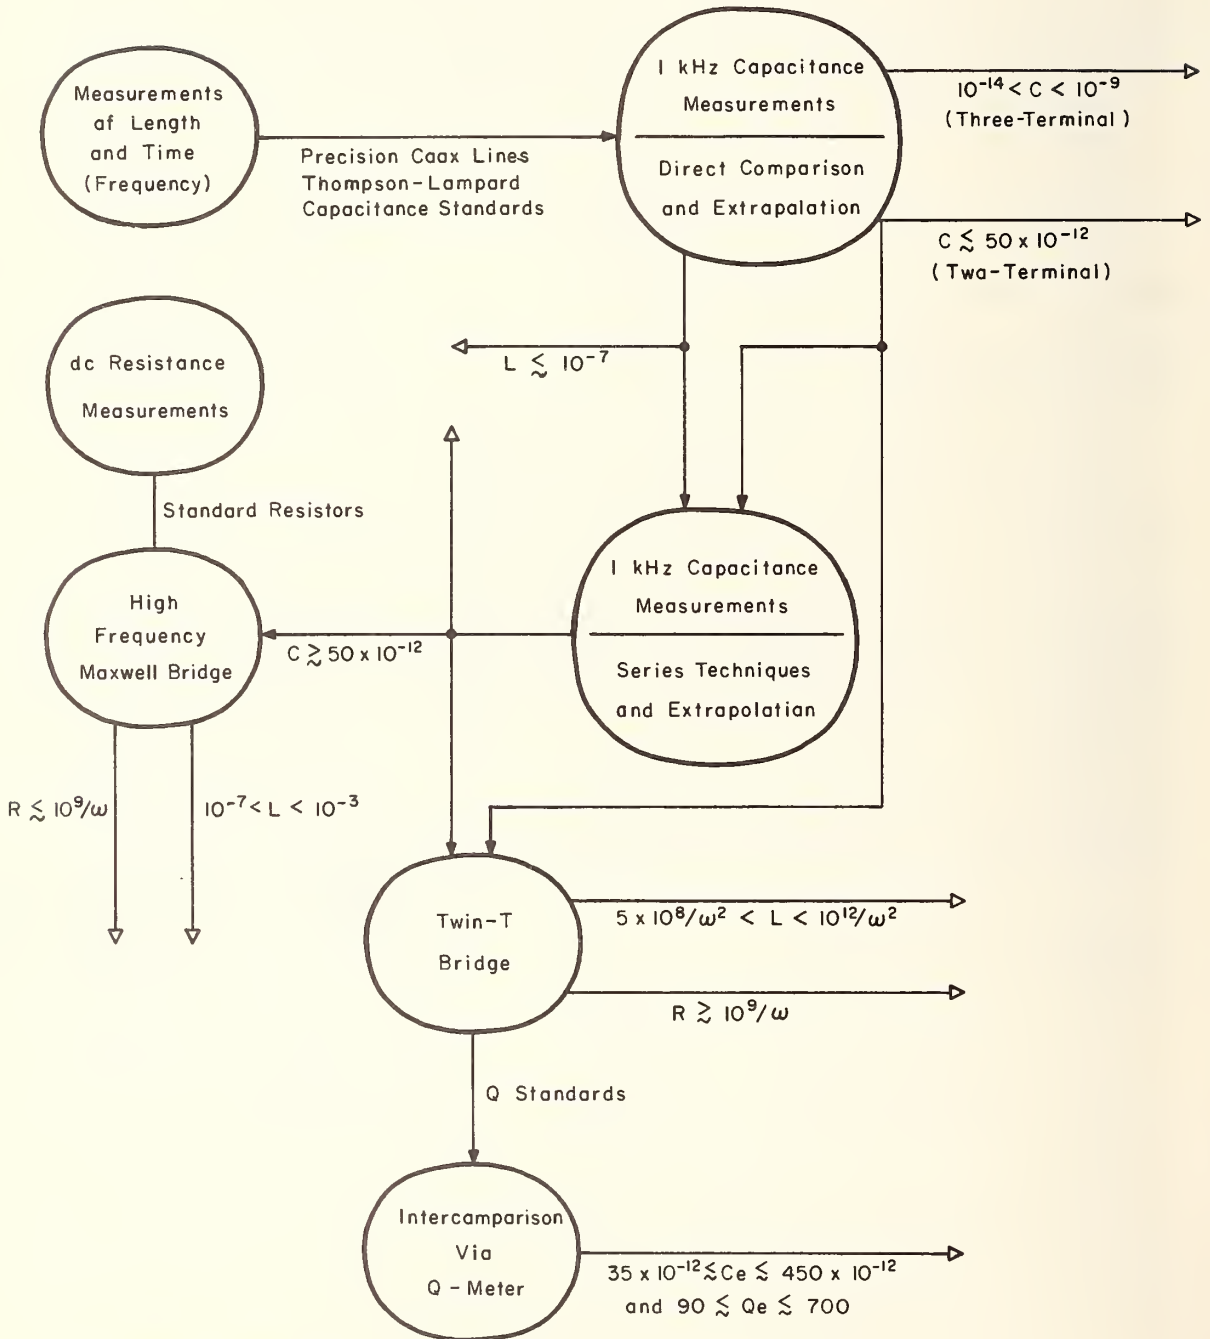

$\omega$  : Angular Frequency

## High Frequency Immittance

30 kHz - 300 MHz

Capacitance:  $10^{-12}$  -  $10^{-7}$  F  
Inductance:  $10^{-8}$  -  $10^{-6}$  H  
Resistance: 0.1 -  $10^6$   $\Omega$

### Bias Uncertainties:

Null detection  
Generator frequency stability  
Mechanical errors (e. g. , gears)  
Connectors

Random Errors: 0.01 to 0.05% (see Notes).

### Total Uncertainty:

Capacitance (2 terminal)	0.1 - 0.5%
Capacitance (3 terminal, see Notes)	0.01 - 2%
Inductance	0.1 - 20%
Resistance	0.1 - 10%

Uncertainty quoted customer: Quoted as estimated for each individual case.

Notes: The 3-terminal capacitance measurements are made only in the frequency range 100 kHz - 1 MHz, and in the capacitance range 0.01 - 1000 pF.

A more detailed listing of the uncertainties as a function of frequency and value of the immittance is available from R. N. Jones or R. E. Nelson (below).

The distribution of random errors depends strongly on the nature of the device being calibrated. In the field of immittance there is little uniformity in the transfer standards used throughout the industry. Thus, it is not generally possible for NBS to give information on random errors based on a large amount of experience with a particular type of transfer standard.

The uncertainties are stated on the basis of the use of precision connectors, which are not always used on devices NBS is asked to calibrate. Where precision connectors are not used the errors can be considerably larger than those quoted.

The uncertainties listed under bias uncertainties above apply to all bridge measurements shown on page 32.

The chart on page 32 shows the most commonly used sequence of measurements. The procedure varies somewhat for specific frequencies and magnitudes.

Reference: L. F. Huntley and R. N. Jones, Lumped parameter impedance measurements, Proc. IEEE 55, 900 (1967).

Personnel: R. N. Jones  
R. E. Nelson

Quality Factor and Effective Resonating Capacitance

50 kHz - 45 MHz

Ranges: Effective Quality Factor ( $Q$ ): 100 - 700

Effective Resonating Capacitance ( $C_e$ ): 30 - 500 pF

Bias Uncertainties:

Inductance and resistance measurements using NBS standards  
Connector errors

Random Errors: See Notes

Effective resonating capacitance ( $C_e$ )	0.15 - 0.5%
Effective quality factor ( $Q_e$ )	0.8 - 2.3%

Total Uncertainty: See Notes

Uncertainty quoted customer: Same as Random Errors. See Notes.

Notes: The  $Q$  standards calibrated by NBS are used largely to establish measurement agreement, with less concern with the absolute accuracy of the measurement of quality factor or effective resonating capacitance. The bias uncertainties are believed to be about the same as the random errors stated above, except for  $Q_e$  above 5 MHz, where difficulties due to connectors and measurement of  $C_e$  small resistances become more severe.

As in the immittance standards calibrated by NBS, the uncertainties associated with connectors other than precision connectors are serious.

A more detailed display of the uncertainties as a function of frequency and magnitude of the parameter being measured is available from R. N. Jones or R. E. Nelson (below).

Reference: R. N. Jones, Standards for the calibration of  $Q$ -meters, 50 kHz to 45 MHz, J. Res. NBS, 68C, 243 (1964).

Personnel: R. N. Jones  
R. E. Nelson


LARGE  
COMPLEX RELATIVE DIELECTRIC PERMITTIVITY

30 kHz - 100 MHz

Ranges :  $\epsilon'$  (Real Part) > 1

$10^{-2} < \tan \delta$  (Loss Tangent) <  $10^2$

Frequencies : 30 kHz - 100 MHz

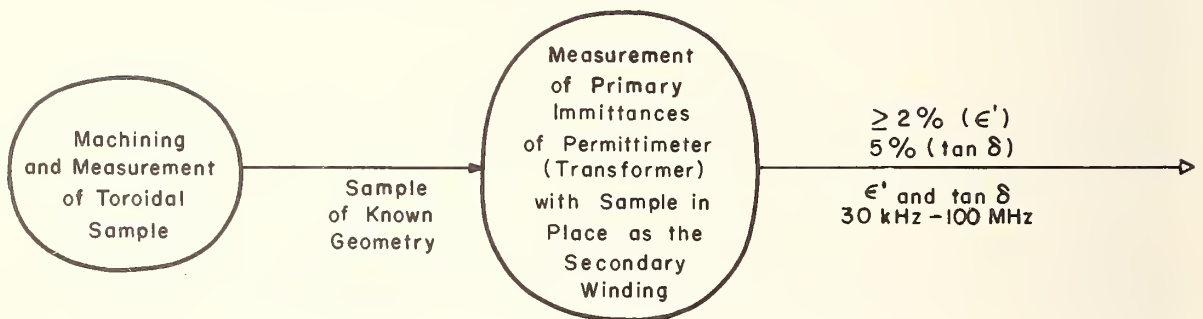

Large  
Complex Relative Dielectric Permittivity

PERMITTIMETER MEASUREMENT:

30 kHz - 100 MHz

$$\text{Range: } \epsilon' > 10^{14} / [f \text{ (Hz)}]^{1.5}$$

$$\sigma > 10^4 / [f \text{ (Hz)}]^{0.5}$$

$$10^{-2} < \tan \delta < 10^2 \text{ (see Notes)}$$

Bias Uncertainties:

Toroidal sample geometry

Reproducibility of making and breaking magnetic circuit

Immittance measurements on primary winding of permittimeter

Random Errors: Not reported.

Total Uncertainty:  $\epsilon'$  :  $\geq 2\%$

$\tan \delta$  :  $\geq 5\%$

Uncertainty quoted customer: Same as Total Uncertainty.


Notes: The range of  $\tan \delta$  is approximate. The specified rather large values of either  $\epsilon'$  or  $\delta$ , to give either displacement or real currents, is a fundamental requirement.

Reference: R. C. Powell and A. L. Rasmussen, A radio frequency permittimeter, IRE Trans. Instr., I-9, 179 (1960).

Personnel: H. E. Bussey

HIGH FREQUENCY  
RELATIVE DIELECTRIC PERMITTIVITY, REAL PART

30 kHz - 1 GHz  
Range:  $1 - 10^4$

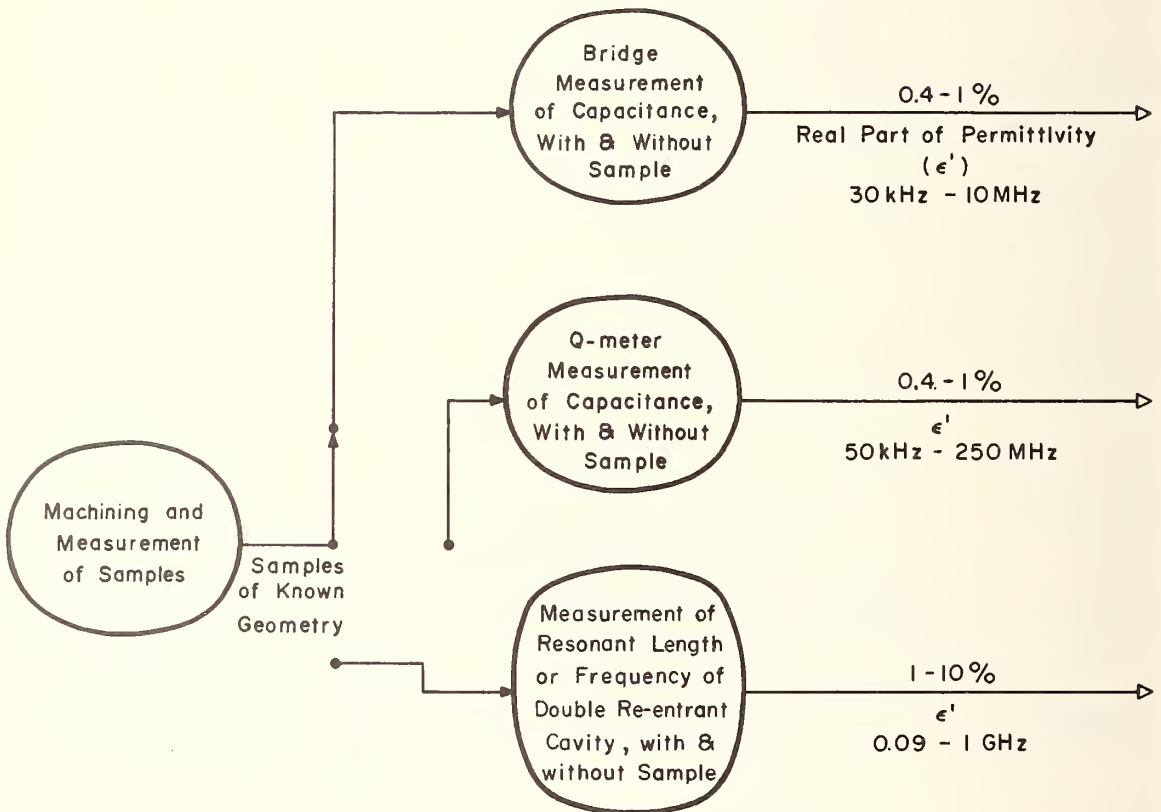



High Frequency Relative Dielectric Permittivity, Real Part,  $\epsilon'$

BRIDGE MEASUREMENT:

Capacitor-type sample holder  
30 kHz - 10 MHz,  $1 < \epsilon' < 10^4$

Bias Uncertainties:

Capacitance (see Notes)	0.05%
Lead inductance	negligible
Fringing capacitance	negligible
Sample geometry (see Notes)	$0.5 (10^{-2}/t)\%$
Sample stability including humidity effects	negligible
Interaction of real and imaginary parts	negligible

Random Errors:

not reported

Total Uncertainty:

$[0.05 + 0.5(10^{-2}/t)]\%$

Uncertainty quoted customer: 0.4 - 1%

Notes: The capacitance measurement is a change in capacitance, with and without the sample. The error depends upon the thickness of the sample and upon  $\epsilon'$ .

The sample geometry uncertainty depends upon the thickness of the sample,  $t$ , which is approximately 0.1 inch.

Reference: H. E. Bussey, Measurements of RF properties of materials, a survey, Proc. IEEE, 55, 1046 (June 1967).

Personnel: H. E. Bussey

High Frequency Relative Dielectric Permittivity, Real Part,  $\epsilon'$

Q-METER MEASUREMENT:

Capacitor-type sample holder  
50 kHz - 250 MHz,  $1 < \epsilon' < 10^4$

Bias Uncertainties:

Capacitance (see Notes)	0.05%
Lead inductance	negligible
Fringing capacitance	negligible
Sample geometry	$0.5 (10^{-2}/t)\%$
Sample stability	negligible
Indirection of real and imaginary parts	negligible

Random Errors:

not reported

Total Uncertainty:

$[0.05 + 0.5(10^{-2}/t)]\%$

Uncertainty quoted customer: 0.4 - 1%

Notes: The capacitance measurement is a change in capacitance, with and without the sample. The error depends upon the thickness of the sample and upon  $\epsilon'$ .

The sample geometry uncertainty depends upon the thickness of the sample,  $t$ , which is approximately 0.1 inch.

Reference: See page 34-1

Personnel: H. E. Bussey

High Frequency Relative Dielectric Permittivity, Real Part,  $\epsilon'$

RE-ENTRANT CAVITY MEASUREMENT:

Capacitive gap in coaxial transmission line  
0.09 - 1 GHz,  $1 < \epsilon' < 10^4$

Bias Uncertainties:

Capacitance	0.2 to 0.5%
Sample geometry, including foil contact	$2(10^{-2}/t)\%$
Fringing fields	0.2%

Random Errors: not quoted

Total Uncertainty:  $[0.4 \text{ to } 0.7 + 2(10^{-2}/t)]\%$

Uncertainty quoted customer: 1 - 10%

Notes: The sample thickness,  $t$ , is approximately 0.05 inch.


Reference: See page 34-1

Personnel: H. E. Bussey

# HIGH FREQUENCY DIELECTRIC LOSS

30 kHz - 1 GHz

Range :  $10^{-4}$  -  $10^3$  ( $\tan \delta$ )

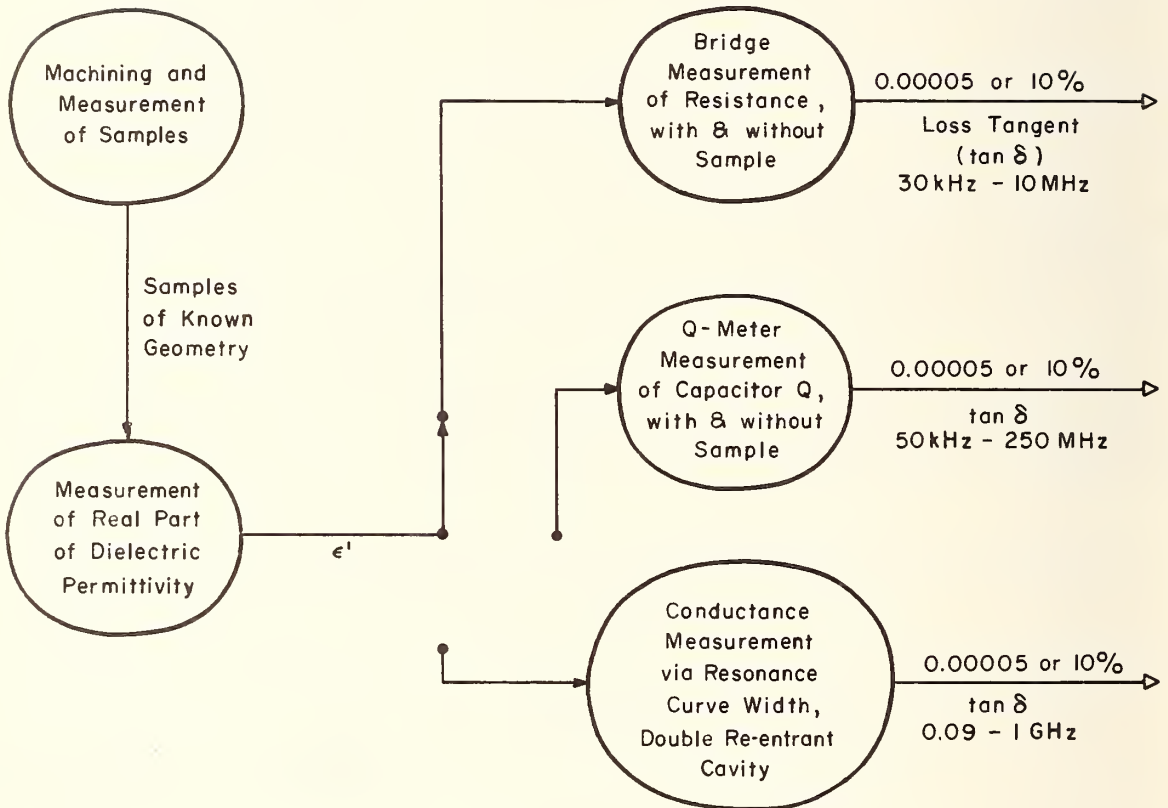

## High Frequency Dielectric Loss

### BRIDGE MEASUREMENTS:

Capacitor-type sample holder  
30 kHz - 10 MHz,  $10^{-4} < \tan \delta < 10$

### Bias Uncertainties:

Sample geometry	0.5 to 1%
Bridge measurement of conductance	2%

### Random Errors:

$5 \times 10^{-3} / \tan \delta$  %

### Total Uncertainty:

$[2.5 \text{ to } 3 + 5 \times 10^{-3} / \tan \delta]$  %

Uncertainty quoted customer: 0.00005 or 10%, whichever is larger.

Notes: None

Reference: See page 34-1

Personnel: H. E. Bussey

## High Frequency Dielectric Loss

### Q-METER MEASUREMENT:

Capacitor-type sample holder  
50 kHz - 250 MHz,  $10^{-4} < \tan \delta < 10$

### Bias Uncertainties:

Geometry of sample	0.5 to 1%
Q-meter measurement	5%

Random Errors:  $5 \times 10^{-3} / \tan \delta \%$

Total Uncertainty:  $[5.5 \text{ to } 6 + 5 \times 10^{-3} / \tan \delta] \%$

Uncertainty quoted customer: 0.00005 or 10%, whichever is larger.

Notes: By special request, loss tangents as low as 0.00001 are measured.

Reference: See page 34-1.

Personnel: H. E. Bussey

## High Frequency Dielectric Loss

### RE-ENTRANT CAVITY MEASUREMENT:

Capacitive gap in coaxial transmission line  
0.09 - 1 GHz,  $10^{-4} < \tan \delta < 1$

### Bias Uncertainties:

Attenuation measurement	0.3%
Sample geometry	1 to 2%
Q measurement, including attenuation errors	2 to 3%
Bias from unknown sources (see Notes)	$4 \times 10^{-2} / \tan \delta$ %

### Random Errors:

not quoted

### Total Uncertainty:

$[3 \text{ to } 5 + 4 \times 10^{-2} / \tan \delta]$  %

Uncertainty quoted customer: 0.00005 or 10%, whichever is larger.


Notes: There are some bias errors from sources which have not yet been identified. Their total magnitude is determined by calibration against samples having known loss tangents.

Reference: See page 34-1.

Personnel: H. E. Bussey

MICROWAVE  
COMPLEX RELATIVE DIELECTRIC PERMITTIVITY  
Dielectric Loaded Transmission Lines

0.3 - 8.6 GHz  
Range: 1 - 20 (Real Part)  
 $10^{-4}$  -  $10^{-1}$  (Loss Tangent)

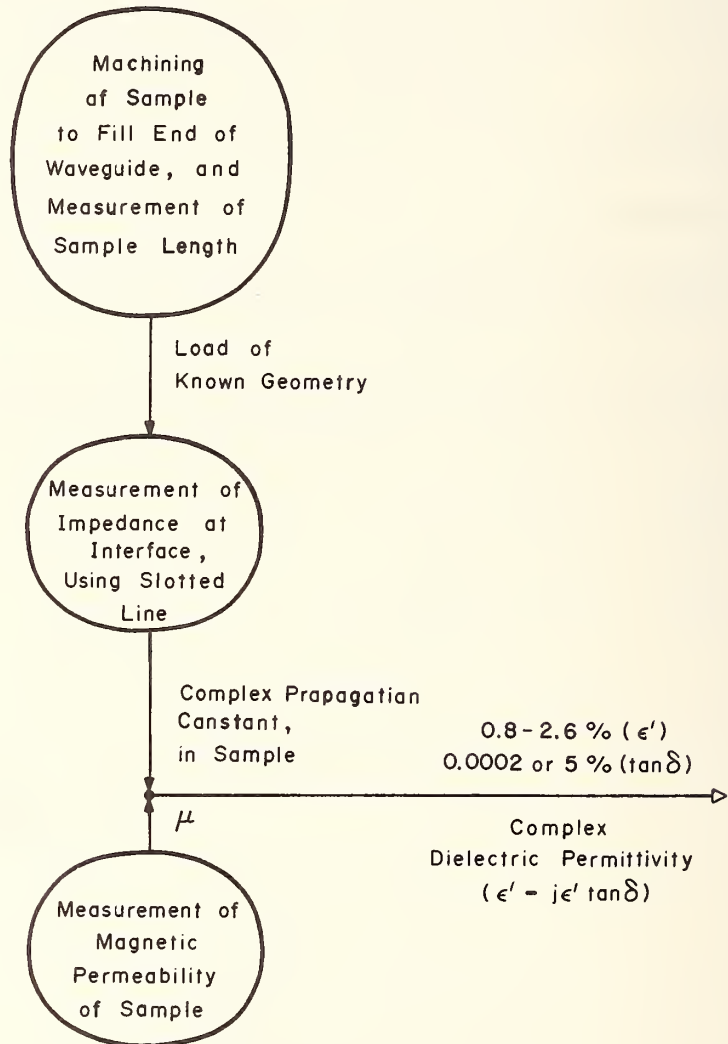



Microwave Complex Relative Dielectric Permittivity, Real Part,  $\epsilon'$

DIELECTRIC LOADED TRANSMISSION LINES:

Slotted line impedance measurements  
0.3 - 8.6 GHz

Bias Uncertainties

Sample dimensions	0.5%
Gap errors around sample	0.2 to 2%
Attenuation measurement	negligible
Probe position and wavelength measurements	0.1%

Random Errors: not reported

Total Uncertainty: 0.8 to 2.6%

Uncertainty quoted customer: 0.8 - 2.6%

Notes: The real and imaginary parts of the permittivity are determined together in this method, as shown by the diagram on page 36. However, the errors in the real and imaginary parts are not the same, and are therefore discussed separately on pages 36-1 and 36-2.

Reference: See page 34-1.

Personnel: H. E. Bussey

Microwave Complex Relative Dielectric Permittivity,  
Loss Tangent

DIELECTRIC LOADED TRANSMISSION LINES

Slotted line impedance measurement  
0.3 - 8.6 GHz

Bias Uncertainties:

Contribution of magnetic permeability	0 to 1%
Gap errors	0.2 to 2%
"Law" of crystal	2%
Environment (see Notes)	0.5%

Random Errors: not reported

Total Uncertainty: 3.5 to 5.5%

Uncertainty of  $\tan \delta$  quoted customer: 0.0002 or 5%, whichever is larger.

Notes: Errors due to environment include foreign surface conductivity, temperature effects, etc.

Reference: See page 34-1

Personnel: H. E. Bussey


# MICROWAVE COMPLEX RELATIVE DIELECTRIC PERMITTIVITY

## Transmission Cavities

0.5, 1, 3, 6, 9 and 30 GHz

Range : 1-100 (Real Part)

$10^{-4}$  -  $10^{-1}$  (Loss Tangent)

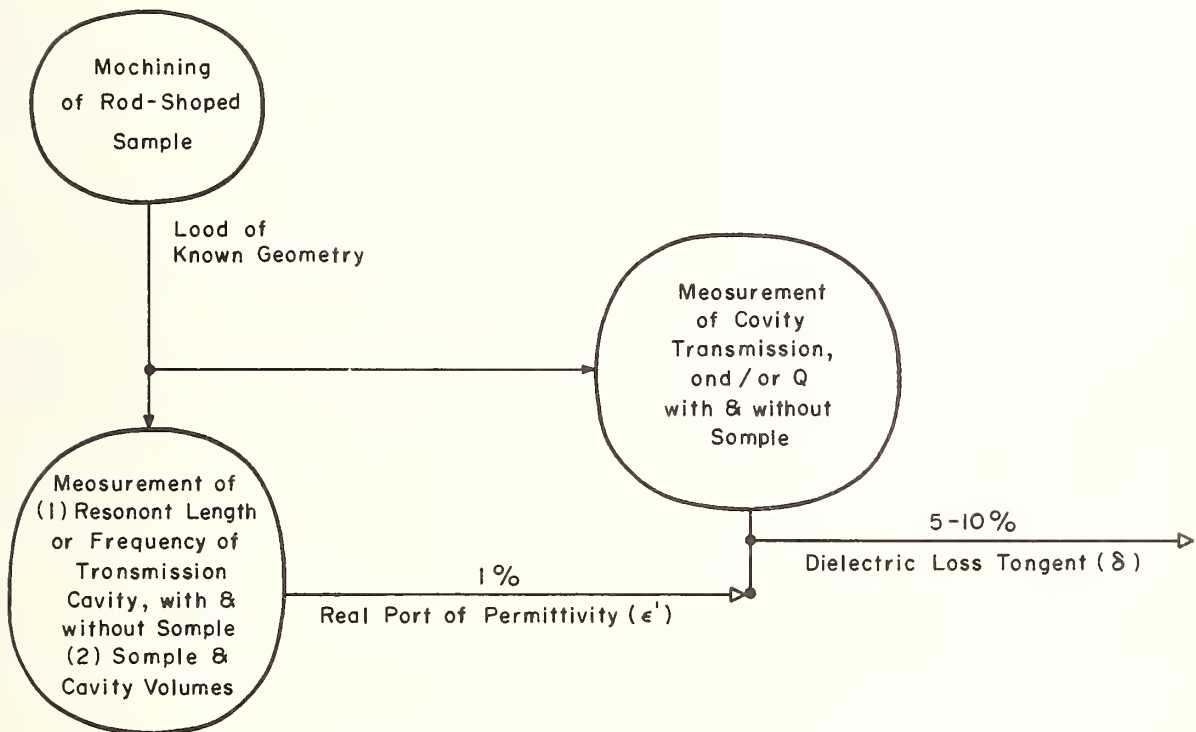

Microwave Complex Relative Dielectric Permittivity, Real Part,  $\epsilon'$

TRANSMISSION CAVITIES:

$1 < \epsilon' < 100$   
0.5, 1, 3, 6, 9, and 30 GHz

Bias Uncertainties:

Volume measurements (sample volume and cavity volume)	0.1 to 0.2%
Change in length or change in frequency	negligible
Misfit of sample in cavity	0.2 to 0.8%

Random Errors: not quoted

Total Uncertainty: 0.3 to 1%

Uncertainty quoted customer: 0.3 - 1%

Notes: A  $TE_{011}$  mode circular cavity resonator is used at 3, 9, and 30 GHz. Sample may be either a rod or a disk. At 0.5, 1, and 6 GHz other modes are used, and the accuracy is lower than for the  $TE_{011}$  modes. Results are based on exact solutions for a rod and disk. Either a complex propagation constant may be used when the loss is high, or the real and imaginary parts may be calculated separately.

Reference: See page 34-1

Personnel: H. E. Bussey

# Microwave Complex Relative Dielectric Permittivity, Loss Tangent

## TRANSMISSION CAVITIES:

$10^{-4} - 10^{-1}$

0.5, 1, 3, 6, 9 and 30 GHz

## Bias Uncertainties:

Attenuation	0.3%
Q measurement, including attenuation errors	1 to 2%
Gap errors	1%
Environment	see Notes
Bias from unknown sources	$[4 \times 10^{-3} / \tan \delta] \%$

## Random Errors:

not reported

## Total Uncertainty:

$[2.5 \text{ to } 3.5 + 4 \times 10^{-3} / \tan \delta] \%$

Uncertainty quoted customer: 5 - 10%

Notes: Environmental errors include foreign surface conductivity, temperature effects, etc. Their magnitudes are not well known.

There are some bias errors from sources which have not yet been identified. Their total magnitude is determined by calibration against samples having known loss tangents.

The transmission coefficient of the cavity is often used to obtain the loss; see reference below.

Also, see Notes on page 37-1.

Reference: H. E. Bussey, Cavity resonator dielectric measurements on rod samples, 1959 Annual Report, Conference on Electrical Insulation, National Academy of Sciences, Publication 756 of the National Research Council.

Personnel: H. E. Bussey



# NBS TECHNICAL PUBLICATIONS

## PERIODICALS

**JOURNAL OF RESEARCH** reports National Bureau of Standards research and development in physics, mathematics, chemistry, and engineering. Comprehensive scientific papers give complete details of the work, including laboratory data, experimental procedures, and theoretical and mathematical analyses. Illustrated with photographs, drawings, and charts.

*Published in three sections, available separately:*

### ● Physics and Chemistry

Papers of interest primarily to scientists working in these fields. This section covers a broad range of physical and chemical research, with major emphasis on standards of physical measurement, fundamental constants, and properties of matter. Issued six times a year. Annual subscription: Domestic, \$9.50; foreign, \$11.75\*.

### ● Mathematical Sciences

Studies and compilations designed mainly for the mathematician and theoretical physicist. Topics in mathematical statistics, theory of experiment design, numerical analysis, theoretical physics and chemistry, logical design and programming of computers and computer systems. Short numerical tables. Issued quarterly. Annual subscription: Domestic, \$5.00; foreign, \$6.25\*.

### ● Engineering and Instrumentation

Reporting results of interest chiefly to the engineer and the applied scientist. This section includes many of the new developments in instrumentation resulting from the Bureau's work in physical measurement, data processing, and development of test methods. It will also cover some of the work in acoustics, applied mechanics, building research, and cryogenic engineering. Issued quarterly. Annual subscription: Domestic, \$5.00; foreign, \$6.25\*.

## TECHNICAL NEWS BULLETIN

The best single source of information concerning the Bureau's research, developmental, cooperative and publication activities, this monthly publication is designed for the industry-oriented individual whose daily work involves intimate contact with science and technology—for engineers, chemists, physicists, research managers, product-development managers, and company executives. Annual subscription: Domestic, \$3.00; foreign, \$4.00\*.

\* Difference in price is due to extra cost of foreign mailing.

Order NBS publications from:

Superintendent of Documents  
Government Printing Office  
Washington, D.C. 20402

## NONPERIODICALS

**Applied Mathematics Series.** Mathematical tables, manuals, and studies.

**Building Science Series.** Research results, test methods, and performance criteria of building materials, components, systems, and structures.

**Handbooks.** Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

**Special Publications.** Proceedings of NBS conferences, bibliographies, annual reports, wall charts, pamphlets, etc.

**Monographs.** Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

**National Standard Reference Data Series.** NSRDS provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated.

**Product Standards.** Provide requirements for sizes, types, quality and methods for testing various industrial products. These standards are developed cooperatively with interested Government and industry groups and provide the basis for common understanding of product characteristics for both buyers and sellers. Their use is voluntary.

**Technical Notes.** This series consists of communications and reports (covering both other agency and NBS-sponsored work) of limited or transitory interest.

**Federal Information Processing Standards Publications.** This series is the official publication within the Federal Government for information on standards adopted and promulgated under the Public Law 89-306, and Bureau of the Budget Circular A-86 entitled, Standardization of Data Elements and Codes in Data Systems.

## CLEARINGHOUSE

The Clearinghouse for Federal Scientific and Technical Information, operated by NBS, supplies unclassified information related to Government-generated science and technology in defense, space, atomic energy, and other national programs. For further information on Clearinghouse services, write:

Clearinghouse  
U.S. Department of Commerce  
Springfield, Virginia 22151

U.S. DEPARTMENT OF COMMERCE  
WASHINGTON, D.C. 20230

OFFICIAL BUSINESS



POSTAGE AND FEES PAID  
U.S. DEPARTMENT OF COMMERCE

---