


NAT'L INST. OF STAND & TECH



A11106 209610

Ref



NBS
Publi-
cations

NBS TECHNICAL NOTE 691

U.S. DEPARTMENT OF COMMERCE / National Bureau of Standards

Clock Synchronization and Comparison: Problems, Techniques and Hardware

QC
100
.U5753
NO.691
1976

NATIONAL BUREAU OF STANDARDS

The National Bureau of Standards¹ was established by an act of Congress March 3, 1901. The Bureau's overall goal is to strengthen and advance the Nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research and provides: (1) a basis for the Nation's physical measurement system, (2) scientific and technological services for industry and government, (3) a technical basis for equity in trade, and (4) technical services to promote public safety. The Bureau consists of the Institute for Basic Standards, the Institute for Materials Research, the Institute for Applied Technology, the Institute for Computer Sciences and Technology, and the Office for Information Programs.

THE INSTITUTE FOR BASIC STANDARDS provides the central basis within the United States of a complete and consistent system of physical measurement; coordinates that system with measurement systems of other nations; and furnishes essential services leading to accurate and uniform physical measurements throughout the Nation's scientific community, industry, and commerce. The Institute consists of the Office of Measurement Services, the Office of Radiation Measurement and the following Center and divisions:

Applied Mathematics — Electricity — Mechanics — Heat — Optical Physics — Center for Radiation Research: Nuclear Sciences; Applied Radiation — Laboratory Astrophysics² — Cryogenics² — Electromagnetics² — Time and Frequency².

THE INSTITUTE FOR MATERIALS RESEARCH conducts materials research leading to improved methods of measurement, standards, and data on the properties of well-characterized materials needed by industry, commerce, educational institutions, and Government; provides advisory and research services to other Government agencies; and develops, produces, and distributes standard reference materials. The Institute consists of the Office of Standard Reference Materials, the Office of Air and Water Measurement, and the following divisions:

Analytical Chemistry — Polymers — Metallurgy — Inorganic Materials — Reactor Radiation — Physical Chemistry.

THE INSTITUTE FOR APPLIED TECHNOLOGY provides technical services to promote the use of available technology and to facilitate technological innovation in industry and Government; cooperates with public and private organizations leading to the development of technological standards (including mandatory safety standards), codes and methods of test; and provides technical advice and services to Government agencies upon request. The Institute consists of the following divisions and Centers:

Standards Application and Analysis — Electronic Technology — Center for Consumer Product Technology: Product Systems Analysis; Product Engineering — Center for Building Technology: Structures, Materials, and Life Safety; Building Environment; Technical Evaluation and Application — Center for Fire Research: Fire Science; Fire Safety Engineering.

THE INSTITUTE FOR COMPUTER SCIENCES AND TECHNOLOGY conducts research and provides technical services designed to aid Government agencies in improving cost effectiveness in the conduct of their programs through the selection, acquisition, and effective utilization of automatic data processing equipment; and serves as the principal focus within the executive branch for the development of Federal standards for automatic data processing equipment, techniques, and computer languages. The Institute consists of the following divisions:

Computer Services — Systems and Software — Computer Systems Engineering — Information Technology.

THE OFFICE FOR INFORMATION PROGRAMS promotes optimum dissemination and accessibility of scientific information generated within NBS and other agencies of the Federal Government; promotes the development of the National Standard Reference Data System and a system of information analysis centers dealing with the broader aspects of the National Measurement System; provides appropriate services to ensure that the NBS staff has optimum accessibility to the scientific information of the world. The Office consists of the following organizational units:

Office of Standard Reference Data — Office of Information Activities — Office of Technical Publications — Library — Office of International Relations — Office of International Standards.

¹ Headquarters and Laboratories at Gaithersburg, Maryland, unless otherwise noted; mailing address Washington, D.C. 20234.

² Located at Boulder, Colorado 80302.

Clock Synchronization and Comparison: Problems, Techniques and Hardware

Technical Information

James E. Gray

Time and Frequency Division
Institute for Basic Standards
National Bureau of Standards
Boulder, Colorado 80302



U.S. DEPARTMENT OF COMMERCE, Elliot L. Richardson, Secretary

Edward O. Vetter, Under Secretary

Dr. Betsy Ancker-Johnson, Assistant Secretary for Science and Technology

NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Acting Director

Issued November 1976

NATIONAL BUREAU OF STANDARDS TECHNICAL NOTE 691
Nat. Bur. Stand. (U.S.), Tech Note 691, 12 pages (November 1976)

CODEN: NBTNAE

U.S. GOVERNMENT PRINTING OFFICE
WASHINGTON: 1976

For sale by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402
(Order by SD Catalog No. C13.46:691). Price 35 cents (Add 25 percent additional for other than U.S. mailing).

CLOCK SYNCHRONIZATION AND COMPARISON:
PROBLEMS, TECHNIQUES AND HARDWARE
James E. Gray

This report summarizes a lecture-discussion of practical problems in measurement electronics as experienced in a laboratory for precise timekeeping. It includes environmental problems, instrumentation problems, procedural problems and ends with a description of a convenient automatic measuring instrument, the chronograph.

KEY WORDS: Chronograph; frequency-stability measurement; instrumentation; laboratory technique: time measurement.

INTRODUCTION

Experiments are planned, using idealized models of the hardware to be used, and one of the surprises of laboratory work is the occasional discovery that the behavior of some instrument is neither so simple nor so ideal as it was supposed to be. I shall be discussing this class of problems - problems which could have been foreseen and avoided, but which sometimes are not. The assortment of instruments used in a precise time laboratory presents an assortment of problems. I have grouped the ones I shall discuss in three categories: environmental problems, instrumentation problems and procedural problems. Finally, I shall describe a convenient automatic measuring instrument, the chronograph.

I. Environmental Problems

- A. Time is often kept by digitally counting the cycles of an oscillator to produce a tick once per second. Occasionally the digital divider will count some cycles which did not occur in the oscillator - the clock jumps. In this laboratory, I have most often found this to be due to electrical noise potentials existing between the "grounds" in different relay racks. Most of our signals are communicated over RG-55 cables, grounded at both ends. Although this system is convenient when using commercial instruments with grounded BNC jacks on their panels, it does have the disadvantage that ground noise potentials and their associated currents are in the signal circuits. Several remedies might be considered. For example, a bifilar choke, a length of coaxial cable wound on a transformer core, can be placed at the input of the divider. Depending upon the location of the noise source, this may cause the noise current to take some alternative route. In practice, I have found this method rather ineffective if used alone. In my experience, a heavy copper braid connected between racks has been most effective. Passing the oscillator signal through an isolation transformer should also help, though I have not yet tried it, because ground straps have been adequate.
- B. In a laboratory that uses the short-term stability of a cesium frequency standard, a surprising amount of isolation may be needed. Suppose that a 5 MHz sine wave signal is stable to a part in 10^{11} at one second. 10^{-11} seconds of phase shift is 314 micro-radians of phase shift. Thus an admixture of 8 parts in 10^6 of some other 5 MHz signal, will cause phase shifts in the desired signal which are comparable to the stability being utilized. That requires an isolation

between 5 MHz signals of 70 dB or better. Many laboratory devices do not meet that specification. Isolation amplifiers, dividers, and even cables laid parallel in cable races may provide more cross coupling than can be tolerated in some high-precision measurements.

- C. Temperature changes may alter the phase delay of a divider. We have some old dividers with slow rise-time circuits and ripple-carry design which move 20 nanoseconds from day to day. Some of our newer dividers have a temperature coefficient of about 0.05 nanosecond per degree, estimated from the circuit. There seems to be a variety of circuits on the market; look at the specifications before choosing one.

II. Instrumentation Problems

- A. Generation of Ticks. The commercial dividers that I have recently seen for generating precise one-second ticks generally use "window" or re-clocked circuits to avoid propagation delay through the dividers, but I still find one-shot multivibrators used to provide an adjustable delay. Such convenience is purchased at the cost of added jitter and temperature sensitivity. One popular clock is specified at 5 nanoseconds jitter. An alternative to using ticks, is to measure the time of zero crossing of the sine wave coming from the oscillator. A divider is still needed to identify the correct zero crossing, but measurements can be made on the sine wave directly. Typical errors in setting the trigger levels of the counter used to measure the time of zero crossing can introduce errors of the order of 1 nanosecond at 5 MHz, 7 nanoseconds at 1 MHz and 66 nanoseconds at 100 kHz. These estimates assume 1.5 volt peak sine wave amplitude and trigger level set using a $\pm 2.5\%$ meter on its 2.5 volt scale.
- B. Impedance Problems. The sine wave from an oscillator is often carried to the site of measurement by RG 55 cable. In addition to cross talk mentioned above, consider impedance matching of these cables. Any mismatch along such a cable will cause a reflection. The reflected sine wave adds to the original one to produce a resultant with altered phase. Although it is not necessary to maintain a perfect match along such cables, it is necessary to remember that any impedance change is capable of shifting the phase being measured. In addition to the effects of reflected waves on the cables, load impedance changes affect the phase of the output from some oscillators. This load sensitivity is large enough to be important in many applications. For example, I observed the following phase shifts when I connected an additional load in parallel with a 50 Ω resistive load on the 5 MHz output of a commercial cesium frequency standard:

<u>Additional Load</u>	<u>Phase Shift (nanoseconds)</u>
100 Ω	+ 2.6
47 Ω	+ 4.8
24 Ω	+ 7.8
330pf	-13.3
680pf	-21.2
1000pf	-27.6

Phase shift with load is not one of the specified characteristics of these frequency standards, so that the effect is probably different for other instruments, but these observations suggest the approximate magnitude of the problem. 47 Ω might represent an additional 50 Ω cable paralleled on the output of the oscillator; 680 pf might represent about 5 meters of 50 Ω cable terminating in a high impedance device.

Similar considerations apply to cables carrying pulses. For example, we observed erratic results when the arrival times of pulses were measured with a time-interval counter after they had travelled between buildings via underground cable. There appeared to be a discrete error. Sometimes the pulses were late; when they were, the delay was always the same. An oscilloscope paralleled with the counter showed the rising edge of the pulse as in figure 1. Slight errors in setting the trigger level of the counter resulted in some measurements being taken above the step, an error. Investigation showed that someone had run a few meters of cable from the source of each tick to an open jack on a nearby patch panel for trouble shooting use. This was in addition to the long, underground cable. The two cables presented an initial load of 25 Ω to the source which expected 50 Ω . Thus the pulse only rose part way. Later, when the pulse returned to its source after reflection from the open jack, the voltage at the source rose to its full height. The resulting stepped rise was causing an intermittent error equal to the round-trip transit time for the pulse on that few meters of open-ended cable to the patch panel (about 10 nanoseconds per meter of cable).

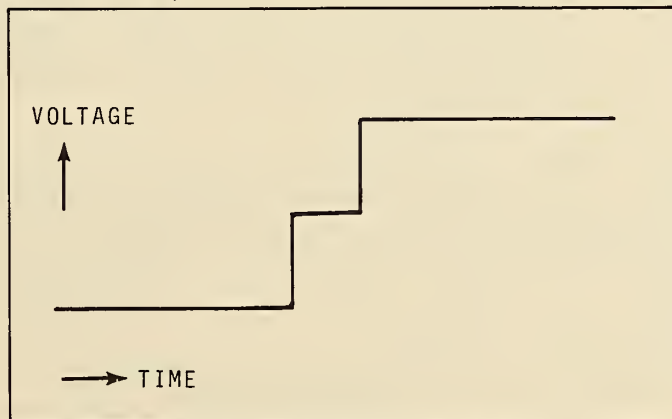


FIG. 1 Stepped rise due to cable reflections.

- C. Internal Errors of Instruments. The errors of time interval counters appear to be rather well described in the counter specifications. Resolution and trigger errors of the order of a nanosecond are available. Other errors that depend upon the length of the interval being measured, can also be of the order of a nanosecond for intervals of about one second. These errors include time-base accuracy and interpolator accuracy. In using such counters for precision measurements, one usually needs to use a matched load at the end of the cable to avoid ringing which can trouble the trigger circuits of the counter.

The chronograph is a less well-known method of time keeping which deserves to be mentioned because of its ability to measure the relative phases of the oscillators in an ensemble with high precision. The chronograph is an instrument which mixes the sine-wave signals from pairs of radio frequency oscillators and records the times of zero crossing of the resulting low-frequency beat. Although the chronograph was developed for other purposes, it can be used to take the data needed to construct a time scale with an ensemble of oscillators. For example, the following procedure might be used.

All the five-megahertz oscillators, except number one, are set low in frequency by one part in 10^8 so that each will have a 20 second beat period when mixed with number one. Oscillator number one is used to drive a 1/20 pps divider. The ticks of that divider are used to start a time interval counter. The zero crossing of the beat between oscillator one and oscillator i is used to stop the counter. Call the measured time interval B_i .

If all the oscillators started in phase with one another and were noiseless and on frequency, then all the zero crossings would coincide with the ticks of the 1/20 pps divider. In fact, they occur at other times as measured by B_i . Thus B_i represents the accumulated phase error between oscillator one and oscillator i . From another point of view, B_i represents the phase error of oscillator one as measured by oscillator i . From this data (the B_i 's), a time scale computation can be made which will give a value for the error of oscillator one as measured by the ensemble of oscillators. Oscillator one can also be used to drive conventional hours, minutes, seconds displays and put out 1 pps ticks if desired.

The random noise and frequency offsets of commercial cesium beam frequency standards in such an ensemble are small enough so that there would generally be a period of several days before the phase of an oscillator has changed by one cycle. Thus, daily measurement would be sufficient to keep track of all the oscillators even if only number one had a divider.

Suppose that the time-interval counter had a resolution of 0.1 microsecond so that the phase comparisons were made with a resolution of 0.1 microsecond out of 20 seconds or five parts in 10^9 . This is a resolution of one femto second in the phase at 5 MHz. Using commercial double-balanced mixers and operational amplifiers, the zero crossings are probably not detectable with this precision, but a resolution of one picosecond seems reasonable.

III. Procedural Problems

A. Redundancy. Useful protection can be achieved against the effects of human errors and equipment failures by redundant measurements. In a time-keeping laboratory it is useful to have the relative phase of each signal recorded at several different reference planes, each under fully specified conditions of measurement. At times of equipment failure and repair, the phase history of an oscillator after the equipment repair can be related to that before, because not all of the reference planes will be affected by the failure and repair work. For example, on a portable clock trip, if the divider fails or jumps, the data can still be obtained by measurement of the times of zero crossing of the sine-wave outputs of the clock, providing that tick-to-phase time intervals are known for that portable clock. The time of zero crossing of the 5 MHz output can be measured with a precision of about one nanosecond and the zero crossings of the 100 kHz output are far enough apart to make it reasonably easy to identify the correct cycle.

A second example: when we placed in service a new pulse cable from one laboratory to another, we calibrated its delay by carrying a portable quartz clock from one end to the other. But we made a redundant measurement by observing the return of the pulse, reflected from the open-circuited end of the cable. I paralleled an oscilloscope across the sending end of the cable and saw something like figure 2a, a completely unexpected result.

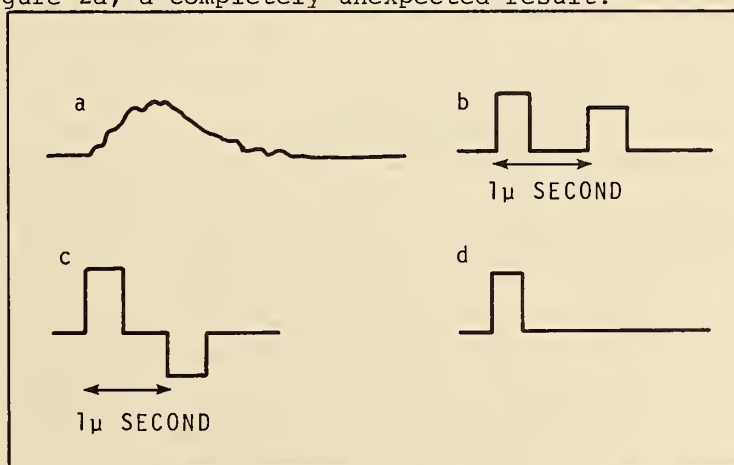


FIG. 2 Voltage at sending end of a pulse cable
a) faulty connector
b) open-circuit load
c) short-circuit load
d) matched load

Investigating the find the cause, we found a badly installed connector at the sending end, which did not contact the outer conductor. When we replaced the connector, the oscilloscope trace looked like figure 2b. A short circuit at the far end gave figure 2c, and a matched load gave figure 2d. 2b, 2c, and 2d are just what I would expect to observe. The redundant measurement not only gave us an independent measurement of the cable delay, but also permitted us to correct a fault before it caused trouble.

- B. Rate Effect. A time-interval counter is often thought of as a device that measures the instantaneous phase relationship between two oscillators. Actually it compares the phase of one oscillator at the instant it starts counting with the phase of the other oscillator at the instant it stops. Thus the measured value includes any phase change between the two oscillators during the measurement interval. That phase change is often negligible but in some circumstances it can cause trouble if overlooked. If the oscillators are offset 300 parts in 10^{10} , and the measurement interval is one second, the error will be 30 nanoseconds.
- C. Remeasurement error. In constructing our time scale, we measure the time of each clock daily, using a time-interval counter with a resolution of one nanosecond. If the counter makes an error of one-half nanosecond every day, by the end of the year, a few tenths of a microsecond error will have accumulated. This is an acceptable error in our application, but if we were to measure once every hour rather than once a day the remeasurement error would be 24 times as great and no longer acceptable.
- D. Portable clock trip. A portable clock is also a non-ideal device. Many of the imperfections of portable clocks are unpredictable and merely set limits to the precision of the time transfer. An interesting exception is a rubidium clock developed at NBS. Its frequency is a known function of barometric pressure. Even an approximate record of barometric pressure during the trip will permit adequate corrections to the time of such a clock. For example, this clock was recently taken from NBS Boulder to the United States Naval Observatory and gave a result within 0.1 microsecond of that obtained a few days later with a cesium clock. The approximate barometric record is shown in figure 3. At Boulder pressure and aircraft cabin pressure which happened to be the same, the clock went late 0.78 microseconds and at sea level pressure, it went late another 0.27 microseconds as calculated from the data shown in figure 3. This total correction of 1.05 microseconds was applied as a clock correction. Assuming a time of descent of pressure of one-half hour, the error due to the uncertainty in the shape of the curve during that period is of the order of one hundredth of a microsecond and can be neglected.

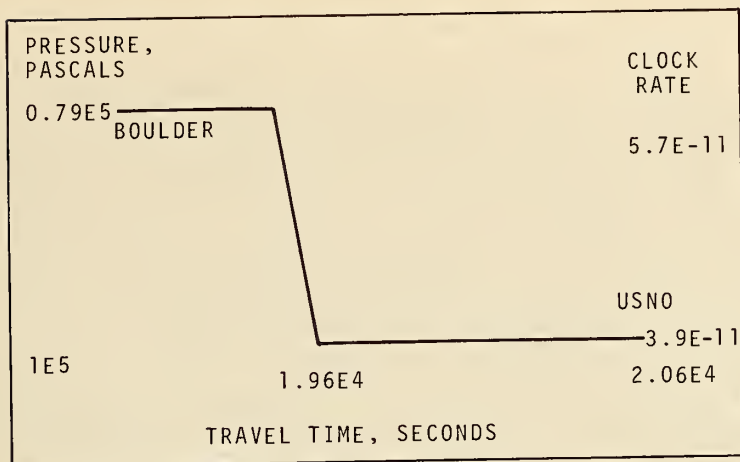


FIG. 3 Barometric record of portable clock trip.

IV. The Chronograph

A. Specifications

The chronograph is a versatile measuring instrument designed for time and frequency measurements. It mixes the sine-wave signals from pairs of radio frequency oscillators and records the times of zero crossing of the resulting low frequency beat. From the recorded data, relative frequencies and stabilities of oscillators can be computed for various sample times, τ , without dead time. I am building a new chronograph to the following performance estimates:

- 1) Ten channels to permit simultaneous measurements on ten pairs of oscillators.
- 2) Input 1 volt nominal, broadband from 1 MHz through 60 MHz.
- 3) Averaging times $\tau \geq$ one millisecond.
- 4) Scale factors $N = 1, 16, 256, 8192$.
(The chronograph will record every Nth zero crossing)
- 5) Measurement bandwidths 2 Hz, 20 Hz, 200 Hz, 1800 Hz.
- 6) Noise floor $\sigma_y(1 \text{ second}) \approx 1 \times 10^{-14}$.

B. General Configuration

Figure 4 shows the overall structure of the chronograph.

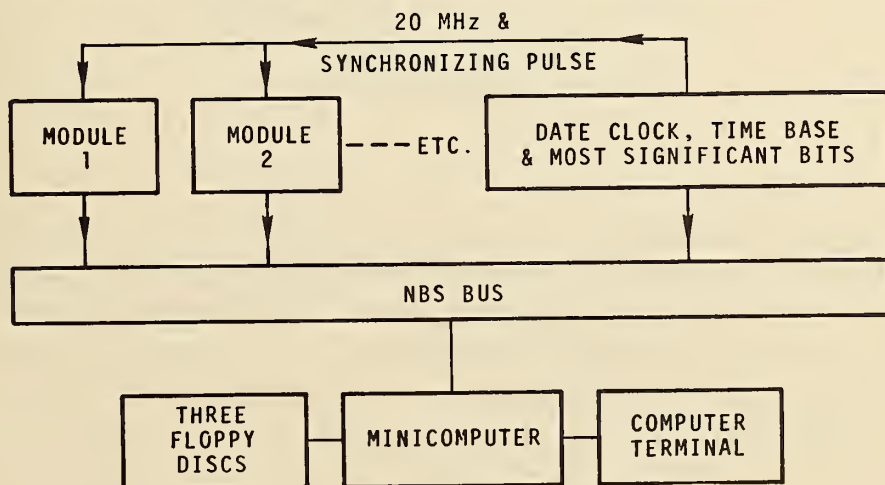


FIGURE 4. Chronograph Configuration

A group of independent modules plug into a computer-access bus. Each module accepts the signals from one pair of oscillators and feeds the time of phase-crossing to the computer. Completely independent modules facilitate maintenance and permit the use of special purpose modules for unusual experiments. The data is stored on three floppy discs, one to receive incoming data, one to permit examination of data taken in the past (without interrupting current measurements) and a third disc for overflow. The NBS bus is a computer interface for which many instrument interfaces are available. Consequently, temperature sensors, etc., can be connected to the bus to permit the measurement of the environmental sensitivity of oscillators.

The minicomputer supervises data acquisition and in its spare time, reduces the data to yield convenient measures such as Allan variances. It controls the modules, setting their bandwidth, scale factors, etc. This permits the experimenter to adjust his measurement parameters directly from the keyboard or indirectly under programmed control.

C. Module Operation

Figure 5 is a block diagram of a typical module.

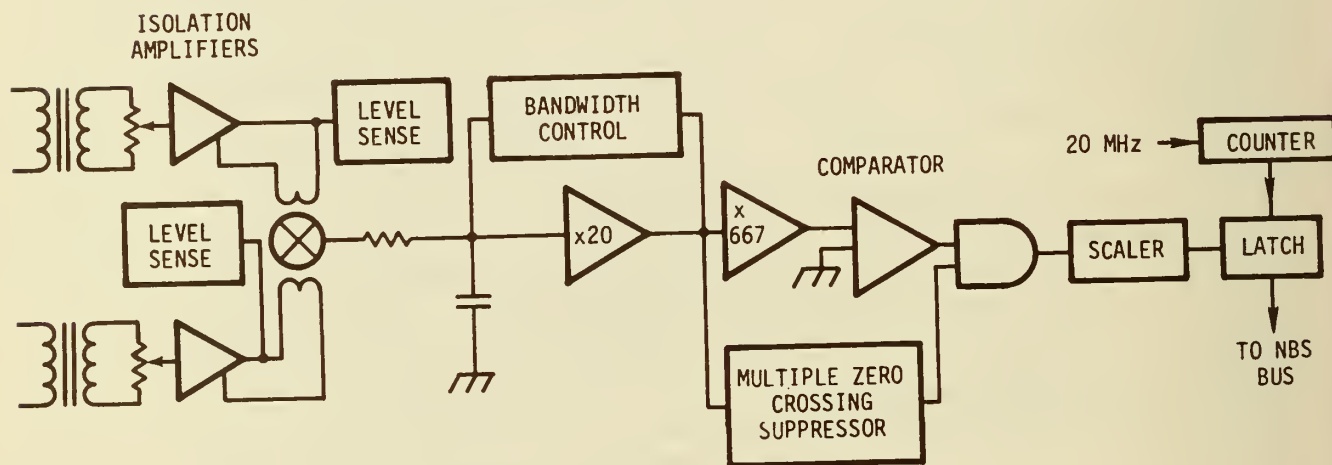


FIGURE 5. Chronograph Module

The two incoming signals are suitably isolated to protect them from contaminating each other by cross-modulation or ground loops and are mixed to produce the low-frequency beat. Zero-crossings of this beat are detected and counted by the scaler. On the Nth zero crossing, the reading of the time-base counter is strobed into the latch for transfer to the computer.

In addition to the standard mode of operation described above, there are two special modes. In the slave mode, the chronograph does not record every zero crossing but rather it records the time of the next zero crossing after it is armed by a command from the computer. It also records how many zero crossings have occurred since the last one that was recorded. This effectively compares the relative phases of the oscillators at a time chosen by the experimenter. In the double mixer mode, each of the two oscillators to be compared is fed to a different chronograph module, and the remaining two input ports are driven by a common oscillator. The computer then takes the difference between the times of phase-crossing in the two modules. This subtraction eliminates most of the noise introduced by the common oscillator. In this mode, oscillators can be compared even though they are on the same frequency and therefore cannot beat with one another directly.

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. NBS-TN-691	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE Clock Synchronization and Comparison: Problems, Techniques and Hardware			5. Publication Date November 1976
7. AUTHOR(S) James E. Gray			8. Performing Organ. Report No.
9. PERFORMING ORGANIZATION NAME AND ADDRESS NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE Boulder, Colorado 80302			10. Project/Task/Work Unit No. 2774246
			11. Contract/Grant No.
2. Sponsoring Organization Name and Complete Address (Street, City, State, ZIP) same as #9			13. Type of Report & Period Covered
5. SUPPLEMENTARY NOTES			14. Sponsoring Agency Code

6. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.)

This report summarizes a lecture-discussion of practical problems in measurement electronics as experienced in a laboratory for precise timekeeping. It includes environment problems, instrumentation problems, procedural problems, and ends with a description of a convenient automatic measuring instrument, the chronograph.

7. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons)
Chronograph; frequency-stability measurement; instrumentation; laboratory technique; time measurement.

8. AVAILABILITY <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input checked="" type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office Washington, D.C. 20402, SD Cat. No. C13.46:691 <input type="checkbox"/> Order From National Technical Information Service (NTIS) Springfield, Virginia 22151	19. SECURITY CLASS (THIS REPORT) UNCLASSIFIED 20. SECURITY CLASS (THIS PAGE) UNCLASSIFIED	21. NO. OF PAGES 12 22. Price \$0.35
---	--	---

NBS TECHNICAL PUBLICATIONS

PERIODICALS

JOURNAL OF RESEARCH reports National Bureau of Standards research and development in physics, mathematics, and chemistry. It is published in two sections, available separately:

• **Physics and Chemistry (Section A)**

Papers of interest primarily to scientists working in these fields. This section covers a broad range of physical and chemical research, with major emphasis on standards of physical measurement, fundamental constants, and properties of matter. Issued six times a year. Annual subscription: Domestic, \$17.00; Foreign, \$21.25.

• **Mathematical Sciences (Section B)**

Studies and compilations designed mainly for the mathematician and theoretical physicist. Topics in mathematical statistics, theory of experiment design, numerical analysis, theoretical physics and chemistry, logical design and programming of computers and computer systems. Short numerical tables. Issued quarterly. Annual subscription: Domestic, \$9.00; Foreign, \$11.25.

DIMENSIONS/NBS (formerly *Technical News Bulletin*)—This monthly magazine is published to inform scientists, engineers, businessmen, industry, teachers, students, and consumers of the latest advances in science and technology, with primary emphasis on the work at NBS. The magazine highlights and reviews such issues as energy research, fire protection, building technology, metric conversion, pollution abatement, health and safety, and consumer product performance. In addition, it reports the results of Bureau programs in measurement standards and techniques, properties of matter and materials, engineering standards and services, instrumentation, and automatic data processing.

Annual subscription: Domestic, \$9.45; Foreign, \$11.85.

NONPERIODICALS

Monographs—Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

Handbooks—Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

Special Publications—Include proceedings of conferences sponsored by NBS, NBS annual reports, and other special publications appropriate to this grouping such as wall charts, pocket cards, and bibliographies.

Applied Mathematics Series—Mathematical tables, manuals, and studies of special interest to physicists, engineers, chemists, biologists, mathematicians, computer programmers, and others engaged in scientific and technical work.

National Standard Reference Data Series—Provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated. Developed under a world-wide program coordinated by NBS. Program under authority of National Standard Data Act (Public Law 90-396).

BIBLIOGRAPHIC SUBSCRIPTION SERVICES

The following current-awareness and literature-survey bibliographies are issued periodically by the Bureau:

Cryogenic Data Center Current Awareness Service. A literature survey issued biweekly. Annual subscription: Domestic, \$20.00; Foreign, \$25.00.

Liquified Natural Gas. A literature survey issued quarterly. Annual subscription: \$20.00.

NOTE: At present the principal publication outlet for these data is the *Journal of Physical and Chemical Reference Data* (JPCRD) published quarterly for NBS by the American Chemical Society (ACS) and the American Institute of Physics (AIP). Subscriptions, reprints, and supplements available from ACS, 1155 Sixteenth St. N.W., Wash. D. C. 20056.

Building Science Series—Disseminates technical information developed at the Bureau on building materials, components, systems, and whole structures. The series presents research results, test methods, and performance criteria related to the structural and environmental functions and the durability and safety characteristics of building elements and systems.

Technical Notes—Studies or reports which are complete in themselves but restrictive in their treatment of a subject. Analogous to monographs but not so comprehensive in scope or definitive in treatment of the subject area. Often serve as a vehicle for final reports of work performed at NBS under the sponsorship of other government agencies.

Voluntary Product Standards—Developed under procedures published by the Department of Commerce in Part 10, Title 15, of the Code of Federal Regulations. The purpose of the standards is to establish nationally recognized requirements for products, and to provide all concerned interests with a basis for common understanding of the characteristics of the products. NBS administers this program as a supplement to the activities of the private sector standardizing organizations.

Consumer Information Series—Practical information, based on NBS research and experience, covering areas of interest to the consumer. Easily understandable language and illustrations provide useful background knowledge for shopping in today's technological marketplace.

Order above NBS publications from: Superintendent of Documents, Government Printing Office, Washington, D.C. 20402.

Order following NBS publications—NBSIR's and FIPS from the National Technical Information Services, Springfield, Va. 22161.

Federal Information Processing Standards Publications (FIPS PUBS)—Publications in this series collectively constitute the Federal Information Processing Standards Register. Register serves as the official source of information in the Federal Government regarding standards issued by NBS pursuant to the Federal Property and Administrative Services Act of 1949 as amended, Public Law 89-306 (79 Stat. 1127), and as implemented by Executive Order 11717 (38 FR 12315, dated May 11, 1973) and Part 6 of Title 15 CFR (Code of Federal Regulations).

NBS Interagency Reports (NBSIR)—A special series of interim or final reports on work performed by NBS for outside sponsors (both government and non-government). In general, initial distribution is handled by the sponsor; public distribution is by the National Technical Information Services (Springfield, Va. 22161) in paper copy or microfiche form.

Superconducting Devices and Materials. A literature survey issued quarterly. Annual subscription: \$20.00. Send subscription orders and remittances for the preceding bibliographic services to National Bureau of Standards, Cryogenic Data Center (275.02) Boulder, Colorado 80302.

U.S. DEPARTMENT OF COMMERCE
National Bureau of Standards
Washington, D.C. 20234

OFFICIAL BUSINESS

Penalty for Private Use, \$300

POSTAGE AND FEES PAID
U.S. DEPARTMENT OF COMMERCE
COM-215



Fourth Class Mail



75 YEARS
NBS
1901-1976